



SAMPLE RUN LOG-ICP-OES-02
Perkin Elmer OPTIMA 7500
Serial No. - 077C8121202

IEC Date: 6-24-10

Analysis Date: 8-6-10

Analyst: A

LR Date: 6-25-10

Page: 1 of 7

All corrections made by analyst unless otherwise noted.

48-6-10

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|------------|-------------|----------------------|------------|----------|----------------------|
| | | SMO | | | 2747-15 |
| | | 2 | | | -2 |
| | | 3 | | | -3 |
| | | 4 | | | -4 |
| | | 5 | | | -5 |
| 222 | | ICV 22222 | | | |
| | | SMO5 | | | |
| | | ICV | | | 2732-14 |
| | | ICB | | | |
| | | CR1 | | | |
| | | ICSA | | | |
| | | ICSA ₂ | | | |
| | | ICV1 | | | Ca Ad Ca 330 Si high |
| | | ICV1 | | | |
| | | SMO | | | 2747-15 |
| | | 2 | | | -2 |
| | | 3 | | | -3 |
| | | 4 | | | -4 |
| | | 5 | | | -5 |
| | | ICV | | | 2232-14 |
| | | ICM | | | |
| | | CR1 | | | |
| | | ICSA | | | |
| | | ICSA ₂ | | | |



IEC Date: _____

Analysis Date: 8-6-10

Analyst: AD

LR Date: _____

Page: 2 of 7

All corrections made by analyst unless otherwise noted.

#86-10

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|----------------|-------------|--------------------------------------|------------|----------|--|
| | | CCV1 | | | AD Na330 Si high |
| | | CCB1 | | | |
| | ✓ | RF71 MBI | SUC | Z | Work |
| | ✓ | RG11 MBI ↓ A | | | re 1/5 (Fe) |
| | | RF71 ADup A | | | CAF |
| | ✓ | Aspl AFpost | | | Sb 12% 0.016 mL St1000 0.08 mL ICP spl |
| ZZZ | ✓ | ADup | | | Sb |
| | ✓ | MBISpl | | | |
| | ✓ | RG11 MBISpl | | | |
| SUC | ✓ | MBISPD | | | |
| | | CCV2 | | | Al or Na33 Si high |
| | | CCB2 | | | |
| | | STD2 | | | |
| | | ↓ 5 | | | |
| | | CCV3 | | | |
| | | CCB3 | | | |
| | | RG30 MBI | TWC | | |
| | | F | | | |
| | | G | | | |
| | | H | | | |
| | | ADup | | | |
| | | ↓ A | | | |



IEC Date: _____ Analysis Date: 8-6-10 Analyst: JA
LR Date: _____ Page: 5 of 7

All corrections made by analyst unless otherwise noted. MS-6-10

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|------------|-------------|-----------------|------------|----------|---------------|
| | | RG 30 Aspik | TWE | | |
| | | MBispk | ↓ | | |
| | | CCV4 | | | Se high |
| | | CCB4 | | | |
| | | RF71 MBI | SWC | 2 | |
| | | RG11 MBI | | ↓ | |
| | | A | | 5 | |
| | | RF71 ADup | | 2 | |
| | | A | | | |
| | | Aspk | | | 56% R low CAR |
| 272 | | ASPK | | | not packed |
| | | h MBispk | | | |
| | | RG11 MBispk | | | |
| SWC | | h MBISPD | ↓ | ↓ | |
| | | CCV5 | | | |
| | | CCB5 | | | |
| | ✓ | RG84 D | SWC | 10 | Went |
| | | G | | ↓ | |
| | | H | | 2 | |
| | | I | | | |
| | | J | | | |
| | | K | | ↓ | |
| | | ADup | | 20 | |
| | | DIC | ↓ | | |



IEC Date: _____

Analysis Date: 8-6-10

Analyst: AT

LR Date: _____

Page: 1 of 7

All corrections made by analyst unless otherwise noted.

AKS-640

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|------------|-------------|---------------|------------|----------|---------------------------------------|
| | ✓ | RG84 A | SWC | 20 | |
| | ✓ | ↓ Aspl | ↓ | ↓ | |
| | | CCV6 | | | Al Ca Fe K Mg Na 300 Si Sr Ti Zn high |
| | | CCB6 | | | |
| | | RG823MB | LEN | 5 | Ba 0.009 A.N |
| | | ↓ ADup | ↓ | ↓ | |
| | | ↓ A | ↓ | ↓ | |
| | | ↓ Aspl | ↓ | ↓ | |
| | | RG54 K | SWC | 2 | |
| | | ↓ L | ↓ | ↓ | |
| | | CCV7 | | | Si high |
| | | CCB7 | | | |
| | | STD 3 | | | |
| | | CCV8 | | | Si high |
| | | CCB8 | | | |
| | | RG84 D | SWC | 10 | |
| | | ↓ G | ↓ | ↓ | |
| | | ↓ H | ↓ | ↓ | |
| | | ↓ I | ↓ | ↓ | |
| | | ↓ J | ↓ | ↓ | |
| | | ↓ K | ↓ | ↓ | |
| | | ↓ A | ↓ | 20 | CAF |
| | | ↓ Aspl | ↓ | ↓ | Cr Cu Zn Si |
| | | ↓ ADup | ↓ | ↓ | Cu high RPD |



IEC Date: _____

Analysis Date: 8-6-10

Analyst: MA

LR Date: _____

Page: 5 of 17

All corrections made by analyst unless otherwise noted.

MA 89-10

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|------------|-------------|-----------------|------------|----------|-----------------------------------|
| | | DIL | | | |
| | | CCV9 | | | |
| | | CCV9 | | | |
| | | RG51 WBI | SWE | 2 | |
| | | B | | | |
| | | C | | | |
| | | D | | | |
| | | ADup | | | |
| | | A | | | |
| | | Aspl | | | |
| 222 | | RF71 | | | Cont |
| | | RG51 Ref1 | | | Scr noisy (NR) |
| | | ↓ WBI SPL | ↓ | ↓ | Scr sl noisy (NR) |
| | | CCV10 | | | cancel k Mg Na 320 Db Si. Se wash |
| | | CCV10 | | | |
| | | RG51 F | SWE | 2 | |
| | | ↓ G | | | |
| | | RG51 A | | | |
| | | B | | | |
| | | C | | | |
| | | E | | | |
| | | F | | | |
| | | H | | | |
| | | ↓ I | ↓ | ↓ | |



IEC Date: _____ Analysis Date: 8-6-10 Analyst: AT
LR Date: _____ Page: 6 of 7

All corrections made by analyst unless otherwise noted. AS 9-10

| Edit Label | Delete Data | ARI Sample ID | Prep. Code | Dilution | Comments |
|------------|-------------|---------------|------------|----------|-----------------------------------|
| | | RG54 J | SWC | 2 | |
| | | CCV11 | | | Ca Cd K Mg Sb Si Sn high |
| | | CCB34 | | | end pkg |
| | ✓ | RG42 MB | SWC | 2 | CV out |
| | | RG51 E | SWC | 2 | |
| | ✓ | RG42 A | SWC | | CV out |
| | | B | | | |
| | | C | | | |
| | | D | | | |
| | | E | | | |
| etc | | RG47 A | | 5 | |
| RG | | MB spk | | 2 | |
| b | ↓ | RG42 MB spk | | ↓ | ↓ |
| | | CCV2 | | | Ca Cd Fe K Mg Na330 Sb Si Sn high |
| | | CCB12 | | | end pkg |
| | ✓ | RG47 MB | SWC | 2 | CV out |
| | | RG24 MB | WMS | | |
| | | A | | | |
| | | B | | | |
| | | C | | | |
| | | D | | | |
| | | E | | | |
| | | F | | | |
| | ↓ | G | | | ↓ |

AT 8/10

Metals Data Review Checklist

Method: ICP ICP-MS GFA CVA

Analysis Date: 8-6-10

| | Analyst <u>AB-9</u> | Peer <u>BW89</u> | Comment |
|---|------------------------|---------------------|-----------------------------------|
| <u>OPT II</u> | | | |
| Logbook: | | | |
| Analyst, Date, Method info | ✓ | ✓ | |
| Sample ID's | ✓ | ✓ | |
| Standard/QC solution ID's recorded | ✓ | ✓ | |
| Prep codes | ✓ | ✓ | |
| Dilution factors | ✓ | ✓ | |
| Crossouts/Corrections/Deletions | ✓ | ✓ | |
| Calibration: | | | |
| Blank & Standard intensities | ✓ | ✓ | |
| Standard deviations | ✓ | ✓ | |
| Curve fit | ✓ | ✓ | |
| Calibration Verification: | | | |
| ICV/CCV | ✓ | ✓ | see log |
| ICB/CCB | ✓ | ✓ | |
| Samples: | | | |
| RSD's & SD's | ✓ | ✓ | see log |
| Internal Standards | ✓ | ✓ | |
| Carry-over | ✓ | ✓ | |
| Method QC: | | | |
| CRI/CRA | ✓ | ✓ | |
| ICSA/ICSAB | ✓ | ✓ | |
| Post Spikes/Serial Dilutions | ✓ | ✓ | |
| Analytic Spikes | ✓ | ✓ | |
| Matrix QC: | | | |
| SRM/LCS | ✓ | ✓ | |
| Matrix Spikes | ✓ | ✓ | |
| Matrix Duplicates | ✓ | ✓ | |
| Method Blanks | ✓ | ✓ | |
| Data Distribution: | | | |
| Requested elements/isotope identified | ✓ | ✓ | |
| Correct samples identified for distribution | ✓ | ✓ | |
| Raw data match distributed data | ✓ | ✓ | |
| Data filename correct | ✓ | ✓ | |
| Necessary Analysts Notes and CAF's | ✓ | ✓ | A.W. RG83, RG30 CAF RG87, RG71 |

=====
Analysis Begun

Start Time: 8/6/2010 9:16:14 AM
Logged In Analyst: metals
Spectrometer Model: Optima 7300 DV, S/N 077C8121202

Plasma On Time: 8/6/2010 7:12:02 AM
Technique: ICP Continuous
Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif
Batch ID:
Results Data Set: I2100806
Results Library: C:\pe\metals\Results\Results.mdb

=====
Sequence No.: 1
Sample ID: Calib Blank 1

Autosampler Location: 1
Date Collected: 8/6/2010 9:16:15 AM
Data Type: Original

Nebulizer Parameters: Calib Blank 1

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: Calib Blank 1

| Analyte | Mean Corrected Intensity | Std.Dev. | RSD | Calib Conc. | Units |
|-------------|--------------------------|----------|--------|-------------|-------|
| ScA 357.253 | 1901694.7 | 13813.30 | 0.73% | 100.0 | % |
| ScR 361.383 | 292682.5 | 2628.77 | 0.90% | 100.0 | % |
| Ag 328.068† | -308.7 | 46.44 | 15.04% | [0.00] | mg/L |
| Al 308.215† | -39.4 | 3.75 | 9.51% | [0.00] | mg/L |
| As 188.979† | -17.3 | 2.85 | 16.52% | [0.00] | mg/L |
| B 249.677† | -26.3 | 6.28 | 23.88% | [0.00] | mg/L |
| Ba 233.527† | 39.3 | 0.90 | 2.29% | [0.00] | mg/L |
| Be 313.042† | 1086.5 | 19.65 | 1.81% | [0.00] | mg/L |
| Ca 317.933† | 96.9 | 28.75 | 29.67% | [0.00] | mg/L |
| Cd 228.802† | 72.2 | 4.48 | 6.21% | [0.00] | mg/L |
| Co 228.616† | -82.3 | 3.19 | 3.87% | [0.00] | mg/L |
| Cr 267.716† | -78.5 | 2.38 | 3.03% | [0.00] | mg/L |
| Cu 324.752† | 8508.7 | 51.87 | 0.61% | [0.00] | mg/L |
| Fe 273.955† | 10.9 | 1.16 | 10.59% | [0.00] | mg/L |
| K 766.490† | -74.4 | 43.61 | 58.59% | [0.00] | mg/L |
| Mg 279.077† | -70.9 | 3.88 | 5.47% | [0.00] | mg/L |
| Mn 257.610† | 46.4 | 5.19 | 11.20% | [0.00] | mg/L |
| Mo 202.031† | 100.3 | 2.47 | 2.47% | [0.00] | mg/L |
| Na 589.592† | -331.8 | 17.52 | 5.28% | [0.00] | mg/L |
| Na 330.237† | -77.2 | 1.59 | 2.06% | [0.00] | mg/L |
| Ni 231.604† | -8.0 | 1.89 | 23.68% | [0.00] | mg/L |
| Pb 220.353† | -73.9 | 7.42 | 10.04% | [0.00] | mg/L |
| Sb 206.836† | 98.8 | 7.15 | 7.23% | [0.00] | mg/L |
| Se 196.026† | -65.3 | 0.71 | 1.08% | [0.00] | mg/L |
| Si 288.158† | 76.3 | 1.82 | 2.38% | [0.00] | mg/L |
| Sn 189.927† | -10.4 | 0.83 | 7.91% | [0.00] | mg/L |
| Sr 421.552† | 262.0 | 8.24 | 3.14% | [0.00] | mg/L |
| Ti 334.903† | -64.7 | 3.33 | 5.15% | [0.00] | mg/L |
| Tl 190.801† | -39.1 | 2.89 | 7.40% | [0.00] | mg/L |
| V 292.402† | 307.8 | 23.97 | 7.79% | [0.00] | mg/L |
| Zn 206.200† | 2.5 | 0.28 | 11.40% | [0.00] | mg/L |

Sequence No.: 2
Sample ID: STD2

Autosampler Location: 2
Date Collected: 8/6/2010 9:20:26 AM
Data Type: Original

Nebulizer Parameters: STD2

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: STD2

| Analyte | Mean Corrected | | RSD | Calib | |
|-------------|----------------|----------|-------|-------|-------|
| | Intensity | Std.Dev. | | Conc. | Units |
| ScA 357.253 | 1939918.3 | 5780.58 | 0.30% | 102.0 | % |
| ScR 361.383 | 295499.5 | 2573.48 | 0.87% | 101.0 | % |
| Ba 233.527† | 30826.9 | 202.74 | 0.66% | [10] | mg/L |
| Cd 228.802† | 210506.4 | 1462.86 | 0.69% | [10] | mg/L |
| Co 228.616† | 295454.6 | 1388.64 | 0.47% | [10] | mg/L |
| Cr 267.716† | 47137.9 | 301.75 | 0.64% | [10] | mg/L |
| Cu 324.752† | 2771035.9 | 2210.85 | 0.08% | [10] | mg/L |
| Mn 257.610† | 293173.6 | 1742.54 | 0.59% | [10] | mg/L |
| V 292.402† | 963014.9 | 2487.89 | 0.26% | [10] | mg/L |

Sequence No.: 3
Sample ID: STD3

Autosampler Location: 3
Date Collected: 8/6/2010 9:22:22 AM
Data Type: Original

Nebulizer Parameters: STD3

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: STD3

| Analyte | Mean Corrected Intensity | Std.Dev. | RSD | Calib Conc. Units |
|-------------|--------------------------|----------|-------|-------------------|
| ScA 357.253 | 1911947.0 | 9470.44 | 0.50% | 100.5 % |
| ScR 361.383 | 287119.4 | 1408.49 | 0.49% | 98.10 % |
| Ag 328.068† | 173230.5 | 724.62 | 0.42% | [1.0] mg/L |
| As 188.979† | 13799.9 | 59.29 | 0.43% | [10] mg/L |
| B 249.677† | 33101.0 | 220.79 | 0.67% | [10] mg/L |
| Be 313.042† | 2747545.2 | 12271.89 | 0.45% | [5.0] mg/L |
| Na 589.592† | 593348.7 | 1683.23 | 0.28% | [50] mg/L |
| Ni 231.604† | 16190.4 | 108.29 | 0.67% | [10] mg/L |
| Pb 220.353† | 68969.7 | 302.79 | 0.44% | [10] mg/L |
| Se 196.026† | 11905.4 | 55.38 | 0.47% | [10] mg/L |
| Sr 421.552† | 3161764.0 | 21881.79 | 0.69% | [5] mg/L |
| Tl 190.801† | 17199.8 | 109.97 | 0.64% | [10] mg/L |
| Zn 206.200† | 6199.9 | 43.31 | 0.70% | [10] mg/L |

Sequence No.: 4
Sample ID: STD4

Autosampler Location: 4
Date Collected: 8/6/2010 9:24:51 AM
Data Type: Original

Nebulizer Parameters: STD4

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: STD4

| Analyte | Mean Corrected Intensity | Std.Dev. | RSD | Calib Conc. | Units |
|-------------|--------------------------|----------|-------|-------------|-------|
| ScA 357.253 | 1931680.4 | 8059.19 | 0.42% | 101.6 | % |
| ScR 361.383 | 294713.8 | 1276.62 | 0.43% | 100.7 | % |
| Mo 202.031† | 171903.3 | 1189.02 | 0.69% | [10] | mg/L |
| Sb 206.836† | 26845.3 | 141.08 | 0.53% | [10] | mg/L |
| Si 288.158† | 14767.8 | 22.92 | 0.16% | [10] | mg/L |
| Sn 189.927† | 36766.5 | 241.76 | 0.66% | [10] | mg/L |
| Ti 334.903† | 219593.7 | 120.79 | 0.06% | [10] | mg/L |

Sequence No.: 5
Sample ID: STD5

Autosampler Location: 5
Date Collected: 8/6/2010 9:27:01 AM
Data Type: Original

Nebulizer Parameters: STD5

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: STD5

| Analyte | Mean Corrected Intensity | Std.Dev. | RSD | Conc. | Calib Units |
|-------------|--------------------------|----------|-------|-------|-------------|
| ScA 357.253 | 1825905.4 | 26915.81 | 1.47% | 96.01 | % |
| ScR 361.383 | 290148.4 | 1529.84 | 0.53% | 99.13 | % |
| Al 308.215† | 37889.0 | 50.64 | 0.13% | [30] | mg/L |
| Ca 317.933† | 431183.3 | 1568.55 | 0.36% | [30] | mg/L |
| Fe 273.955† | 113290.3 | 543.90 | 0.48% | [100] | mg/L |
| K 766.490† | 143026.9 | 1263.39 | 0.88% | [100] | mg/L |
| Mg 279.077† | 27720.9 | 121.41 | 0.44% | [30] | mg/L |
| Na 330.237† | 2893.7 | 17.63 | 0.61% | [100] | mg/L |

Calibration Summary

| Analyte | Stds. | Equation | Intercept | Slope | Curvature | Corr. Coef. | Reslope |
|------------|-------|------------|-----------|--------|-----------|-------------|---------|
| Ag 328.068 | 1 | Lin Thru 0 | 0.0 | 173200 | 0.00000 | 1.000000 | |
| Al 308.215 | 1 | Lin Thru 0 | 0.0 | 1263 | 0.00000 | 1.000000 | |
| As 188.979 | 1 | Lin Thru 0 | 0.0 | 1380 | 0.00000 | 1.000000 | |
| B 249.677 | 1 | Lin Thru 0 | 0.0 | 3310 | 0.00000 | 1.000000 | |
| Ba 233.527 | 1 | Lin Thru 0 | 0.0 | 3083 | 0.00000 | 1.000000 | |
| Be 313.042 | 1 | Lin Thru 0 | 0.0 | 549500 | 0.00000 | 1.000000 | |
| Ca 317.933 | 1 | Lin Thru 0 | 0.0 | 14370 | 0.00000 | 1.000000 | |
| Cd 228.802 | 1 | Lin Thru 0 | 0.0 | 21050 | 0.00000 | 1.000000 | |
| Co 228.616 | 1 | Lin Thru 0 | 0.0 | 29550 | 0.00000 | 1.000000 | |
| Cr 267.716 | 1 | Lin Thru 0 | 0.0 | 4714 | 0.00000 | 1.000000 | |
| Cu 324.752 | 1 | Lin Thru 0 | 0.0 | 277100 | 0.00000 | 1.000000 | |
| Fe 273.955 | 1 | Lin Thru 0 | 0.0 | 1133 | 0.00000 | 1.000000 | |
| K 766.490 | 1 | Lin Thru 0 | 0.0 | 1430 | 0.00000 | 1.000000 | |
| Mg 279.077 | 1 | Lin Thru 0 | 0.0 | 924.0 | 0.00000 | 1.000000 | |
| Mn 257.610 | 1 | Lin Thru 0 | 0.0 | 29320 | 0.00000 | 1.000000 | |
| Mo 202.031 | 1 | Lin Thru 0 | 0.0 | 17190 | 0.00000 | 1.000000 | |
| Na 589.592 | 1 | Lin Thru 0 | 0.0 | 11870 | 0.00000 | 1.000000 | |
| Na 330.237 | 1 | Lin Thru 0 | 0.0 | 28.94 | 0.00000 | 1.000000 | |
| Ni 231.604 | 1 | Lin Thru 0 | 0.0 | 1619 | 0.00000 | 1.000000 | |
| Pb 220.353 | 1 | Lin Thru 0 | 0.0 | 6897 | 0.00000 | 1.000000 | |
| Sb 206.836 | 1 | Lin Thru 0 | 0.0 | 2685 | 0.00000 | 1.000000 | |
| Se 196.026 | 1 | Lin Thru 0 | 0.0 | 1191 | 0.00000 | 1.000000 | |
| Si 288.158 | 1 | Lin Thru 0 | 0.0 | 1477 | 0.00000 | 1.000000 | |
| Sn 189.927 | 1 | Lin Thru 0 | 0.0 | 3677 | 0.00000 | 1.000000 | |
| Sr 421.552 | 1 | Lin Thru 0 | 0.0 | 632400 | 0.00000 | 1.000000 | |
| Ti 334.903 | 1 | Lin Thru 0 | 0.0 | 21960 | 0.00000 | 1.000000 | |
| Tl 190.801 | 1 | Lin Thru 0 | 0.0 | 1720 | 0.00000 | 1.000000 | |
| V 292.402 | 1 | Lin Thru 0 | 0.0 | 96300 | 0.00000 | 1.000000 | |
| Zn 206.200 | 1 | Lin Thru 0 | 0.0 | 620.0 | 0.00000 | 1.000000 | |

=====
Analysis Begun

Start Time: 8/6/2010 9:29:53 AM

Plasma On Time: 8/6/2010 7:12:02 AM

Logged In Analyst: metals

Technique: ICP Continuous

Spectrometer Model: Optima 7300 DV, S/N 077C8121202 Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif

Batch ID:

Results Data Set: I2100806

Results Library: C:\pe\metals\Results\Results.mdb

=====
Sequence No.: 1

Autosampler Location: 7

Sample ID: CV

Data Collected: 8/6/2010 9:29:54 AM

Analyst: ALA

Data Type: Original

Dilution: 1X

Nebulizer Parameters: CV

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: CV

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------|----------|--------------------|----------|-------|
| ScA 357.253 | 1919699.5 | 100.9 | % | 0.51 | | | 0.50% |
| ScR 361.383 | 289156.1 | 98.80 | % | 0.716 | | | 0.72% |
| Ag 328.068† | 179266.0 | 1.035 | mg/L | 0.0063 | 1.035 mg/L | 0.0063 | 0.61% |
| Al 308.215† | 2684.1 | 2.093 | mg/L | 0.0187 | 2.093 mg/L | 0.0187 | 0.90% |
| As 188.979† | 2776.4 | 2.029 | mg/L | 0.0088 | 2.029 mg/L | 0.0088 | 0.44% |
| B 249.677† | 3311.0 | 0.9985 | mg/L | 0.00654 | 0.9985 mg/L | 0.00654 | 0.65% |
| Ba 233.527† | 3204.3 | 1.039 | mg/L | 0.0101 | 1.039 mg/L | 0.0101 | 0.97% |
| Be 313.042† | 541467.3 | 0.9848 | mg/L | 0.00710 | 0.9848 mg/L | 0.00710 | 0.72% |
| Ca 317.933† | 30473.5 | 2.120 | mg/L | 0.0086 | 2.120 mg/L | 0.0086 | 0.41% |
| Cd 228.802† | 22001.2 | 1.039 | mg/L | 0.0041 | 1.039 mg/L | 0.0041 | 0.39% |
| Co 228.616† | 29893.8 | 1.010 | mg/L | 0.0055 | 1.010 mg/L | 0.0055 | 0.54% |
| Cr 267.716† | 4956.9 | 1.051 | mg/L | 0.0069 | 1.051 mg/L | 0.0069 | 0.66% |
| Cu 324.752† | 287003.5 | 1.035 | mg/L | 0.0065 | 1.035 mg/L | 0.0065 | 0.62% |
| Fe 273.955† | 2321.6 | 2.044 | mg/L | 0.0147 | 2.044 mg/L | 0.0147 | 0.72% |
| K 766.490† | 29239.7 | 20.44 | mg/L | 0.121 | 20.44 mg/L | 0.121 | 0.59% |
| Mg 279.077† | 1918.3 | 2.081 | mg/L | 0.0173 | 2.081 mg/L | 0.0173 | 0.83% |
| Mn 257.610† | 29614.8 | 1.011 | mg/L | 0.0059 | 1.011 mg/L | 0.0059 | 0.58% |
| Mo 202.031† | 17281.2 | 1.005 | mg/L | 0.0052 | 1.005 mg/L | 0.0052 | 0.52% |
| Na 589.592† | 599623.4 | 50.53 | mg/L | 0.353 | 50.53 mg/L | 0.353 | 0.70% |
| Na 330.237† | 1487.3 | 51.46 | mg/L | 0.299 | 51.46 mg/L | 0.299 | 0.58% |
| Ni 231.604† | 1634.8 | 1.011 | mg/L | 0.0049 | 1.011 mg/L | 0.0049 | 0.48% |
| Pb 220.353† | 13915.1 | 2.019 | mg/L | 0.0063 | 2.019 mg/L | 0.0063 | 0.31% |
| Sb 206.836† | 5574.8 | 2.082 | mg/L | 0.0126 | 2.082 mg/L | 0.0126 | 0.60% |
| Se 196.026† | 2415.9 | 2.029 | mg/L | 0.0114 | 2.029 mg/L | 0.0114 | 0.56% |
| Si 288.158† | 3154.0 | 2.139 | mg/L | 0.0116 | 2.139 mg/L | 0.0116 | 0.54% |
| Sn 189.927† | 3697.2 | 1.007 | mg/L | 0.0062 | 1.007 mg/L | 0.0062 | 0.62% |
| Sr 421.552† | 638679.4 | 1.010 | mg/L | 0.0071 | 1.010 mg/L | 0.0071 | 0.70% |
| Ti 334.903† | 22384.4 | 1.018 | mg/L | 0.0080 | 1.018 mg/L | 0.0080 | 0.78% |
| Tl 190.801† | 3467.5 | 2.016 | mg/L | 0.0117 | 2.016 mg/L | 0.0117 | 0.58% |
| V 292.402† | 97120.9 | 1.013 | mg/L | 0.0061 | 1.013 mg/L | 0.0061 | 0.60% |
| Zn 206.200† | 615.0 | 0.9915 | mg/L | 0.00774 | 0.9915 mg/L | 0.00774 | 0.78% |

Sequence No.: 2
 Sample ID: CB
 Analyst: A/A
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 9:34:07 AM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 198.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1920093.2 | 101.0 | % | 0.51 | | | 0.51% |
| ScR 361.383 | 274885.6 | 93.92 | % | 0.273 | | | 0.29% |
| Ag 328.068† | -14.0 | -0.00008 | mg/L | 0.000094 | -0.00008 mg/L | 0.000094 | 116.43% |
| Al 308.215† | -7.9 | -0.00624 | mg/L | 0.005167 | -0.00624 mg/L | 0.005167 | 82.85% |
| As 188.979† | 4.3 | 0.00311 | mg/L | 0.001713 | 0.00311 mg/L | 0.001713 | 55.04% |
| B 249.677† | 4.2 | 0.00126 | mg/L | 0.002518 | 0.00126 mg/L | 0.002518 | 200.54% |
| Ba 233.527† | 3.3 | 0.00108 | mg/L | 0.000847 | 0.00108 mg/L | 0.000847 | 78.37% |
| Be 313.042† | 55.7 | 0.00010 | mg/L | 0.000049 | 0.00010 mg/L | 0.000049 | 48.29% |
| Ca 317.933† | 10.8 | 0.00075 | mg/L | 0.002432 | 0.00075 mg/L | 0.002432 | 323.25% |
| Cd 228.802† | -1.7 | -0.00009 | mg/L | 0.000165 | -0.00009 mg/L | 0.000165 | 182.43% |
| Co 228.616† | 2.3 | 0.00008 | mg/L | 0.000220 | 0.00008 mg/L | 0.000220 | 285.33% |
| Cr 267.716† | -0.7 | -0.00015 | mg/L | 0.001140 | -0.00015 mg/L | 0.001140 | 738.40% |
| Cu 324.752† | -52.5 | -0.00019 | mg/L | 0.000361 | -0.00019 mg/L | 0.000361 | 190.29% |
| Fe 273.955† | -1.7 | -0.00152 | mg/L | 0.002196 | -0.00152 mg/L | 0.002196 | 144.43% |
| K 766.490† | 45.6 | 0.03187 | mg/L | 0.020405 | 0.03187 mg/L | 0.020405 | 64.02% |
| Mg 279.077† | -2.9 | -0.00312 | mg/L | 0.002210 | -0.00312 mg/L | 0.002210 | 70.88% |
| Mn 257.610† | 4.9 | 0.00017 | mg/L | 0.000050 | 0.00017 mg/L | 0.000050 | 30.23% |
| Mo 202.031† | 0.2 | 0.00001 | mg/L | 0.000065 | 0.00001 mg/L | 0.000065 | 596.14% |
| Na 589.592† | 64.1 | 0.00540 | mg/L | 0.003285 | 0.00540 mg/L | 0.003285 | 60.80% |
| Na 330.237† | -5.1 | -0.1763 | mg/L | 0.13025 | -0.1763 mg/L | 0.13025 | 73.89% |
| Ni 231.604† | 6.9 | 0.00428 | mg/L | 0.001189 | 0.00428 mg/L | 0.001189 | 27.78% |
| Pb 220.353† | 0.1 | 0.00002 | mg/L | 0.000213 | 0.00002 mg/L | 0.000213 | >999.9% |
| Sb 206.836† | 8.1 | 0.00303 | mg/L | 0.002451 | 0.00303 mg/L | 0.002451 | 80.87% |
| Se 196.026† | 5.0 | 0.00418 | mg/L | 0.003761 | 0.00418 mg/L | 0.003761 | 89.91% |
| Si 288.158† | 12.0 | 0.00810 | mg/L | 0.003591 | 0.00810 mg/L | 0.003591 | 44.34% |
| Sn 189.927† | 1.5 | 0.00042 | mg/L | 0.000959 | 0.00042 mg/L | 0.000959 | 227.28% |
| Sr 421.552† | 49.9 | 0.00008 | mg/L | 0.000039 | 0.00008 mg/L | 0.000039 | 48.94% |
| Ti 334.903† | -0.2 | -0.00001 | mg/L | 0.001087 | -0.00001 mg/L | 0.001087 | >999.9% |
| Tl 190.801† | 1.6 | 0.00094 | mg/L | 0.000489 | 0.00094 mg/L | 0.000489 | 51.78% |
| V 292.402† | -6.1 | -0.00006 | mg/L | 0.000081 | -0.00006 mg/L | 0.000081 | 127.96% |
| Zn 206.200† | -0.0 | -0.00005 | mg/L | 0.002159 | -0.00005 mg/L | 0.002159 | >999.9% |

Sequence No.: 3
Sample ID: CRI
Analyst: ALA
Dilution: 1X

Autosampler Location: 301
Date Collected: 8/6/2010 9:38:03 AM
Data Type: Original

Nebulizer Parameters: CRI

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: CRI

Table with 8 columns: Analyte, Mean Corrected Intensity, Calib. Conc. Units, Std.Dev., Sample Conc. Units, Std.Dev., RSD. Lists various elements like ScA, ScR, Ag, Al, As, B, Ba, Be, Ca, Cd, Co, Cr, Cu, Fe, K, Mg, Mn, Mo, Na, Ni, Pb, Sb, Se, Si, Sn, Sr, Ti, Tl, V, Zn with their respective intensity, concentration, and RSD values.

Sequence No.: 4
 Sample ID: ICSA
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 302
 Date Collected: 8/6/2010 9:42:14 AM
 Data Type: Original

Nebulizer Parameters: ICSA

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: ICSA

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|-----------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1870069.2 | 98.34 | % | 0.875 | | | | 0.89% |
| ScR 361.383 | 290138.9 | 99.13 | % | 0.616 | | | | 0.62% |
| Ag 328.068† | -177.5 | -0.00102 | mg/L | 0.000239 | -0.00102 | mg/L | 0.000239 | 23.40% |
| Al 308.215† | 255190.8 | 202.1 | mg/L | 0.53 | 202.1 | mg/L | 0.53 | 0.26% |
| As 188.979† | 16.2 | 0.00879 | mg/L | 0.000890 | 0.00879 | mg/L | 0.000890 | 10.12% |
| B 249.677† | -19.6 | -0.00591 | mg/L | 0.001857 | -0.00591 | mg/L | 0.001857 | 31.42% |
| Ba 233.527† | 63.3 | 0.00156 | mg/L | 0.000492 | 0.00156 | mg/L | 0.000492 | 31.62% |
| Be 313.042† | -1.6 | -0.00002 | mg/L | 0.000026 | -0.00002 | mg/L | 0.000026 | 168.35% |
| Ca 317.933† | 1446765.9 | 100.7 | mg/L | 0.55 | 100.7 | mg/L | 0.55 | 0.54% |
| Cd 228.802† | 44.9 | 0.00210 | mg/L | 0.000185 | 0.00210 | mg/L | 0.000185 | 8.84% |
| Co 228.616† | 56.2 | -0.00057 | mg/L | 0.000162 | -0.00057 | mg/L | 0.000162 | 28.51% |
| Cr 267.716† | 34.3 | 0.00159 | mg/L | 0.001212 | 0.00159 | mg/L | 0.001212 | 76.39% |
| Cu 324.752† | -3687.1 | -0.00147 | mg/L | 0.000391 | -0.00147 | mg/L | 0.000391 | 26.54% |
| Fe 273.955† | 223019.7 | 196.9 | mg/L | 0.87 | 196.9 | mg/L | 0.87 | 0.44% |
| K 766.490† | 19.0 | 0.01328 | mg/L | 0.011046 | 0.01328 | mg/L | 0.011046 | 83.16% |
| Mg 279.077† | 92019.1 | 99.47 | mg/L | 0.479 | 99.47 | mg/L | 0.479 | 0.48% |
| Mn 257.610† | 46.8 | 0.00101 | mg/L | 0.000283 | 0.00101 | mg/L | 0.000283 | 28.14% |
| Mo 202.031† | 105.1 | 0.00437 | mg/L | 0.000422 | 0.00437 | mg/L | 0.000422 | 9.65% |
| Na 589.592† | 98.0 | 0.00826 | mg/L | 0.000669 | 0.00826 | mg/L | 0.000669 | 8.10% |
| Na 330.237† | 1.3 | 0.6518 | mg/L | 0.13949 | 0.6518 | mg/L | 0.13949 | 21.40% |
| Ni 231.604† | 3.5 | 0.00220 | mg/L | 0.004025 | 0.00220 | mg/L | 0.004025 | 183.18% |
| Pb 220.353† | -205.9 | -0.00938 | mg/L | 0.000804 | -0.00938 | mg/L | 0.000804 | 8.57% |
| Sb 206.836† | 69.2 | 0.02563 | mg/L | 0.002142 | 0.02563 | mg/L | 0.002142 | 8.36% |
| Se 196.026† | 62.5 | 0.04568 | mg/L | 0.005316 | 0.04568 | mg/L | 0.005316 | 11.64% |
| Si 288.158† | -26.6 | -0.01798 | mg/L | 0.011587 | -0.01798 | mg/L | 0.011587 | 64.44% |
| Sn 189.927† | -55.2 | -0.01033 | mg/L | 0.001424 | -0.01033 | mg/L | 0.001424 | 13.79% |
| Sr 421.552† | 2288.6 | 0.00362 | mg/L | 0.000038 | 0.00362 | mg/L | 0.000038 | 1.04% |
| Ti 334.903† | 161.3 | 0.00106 | mg/L | 0.000544 | 0.00106 | mg/L | 0.000544 | 51.23% |
| Tl 190.801† | -33.4 | 0.01017 | mg/L | 0.002501 | 0.01017 | mg/L | 0.002501 | 24.59% |
| V 292.402† | 2275.7 | 0.00259 | mg/L | 0.000403 | 0.00259 | mg/L | 0.000403 | 15.58% |
| Zn 206.200† | -2.6 | -0.00982 | mg/L | 0.002657 | -0.00982 | mg/L | 0.002657 | 27.05% |

Sequence No.: 5
 Sample ID: ICSAB
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 303
 Date Collected: 8/6/2010 9:46:25 AM
 Data Type: Original

Nebulizer Parameters: ICSAB

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: ICSAB

| Analyte | Mean Corrected | | Calib. | | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | Units | Std.Dev. | Conc. | Units | | |
| ScA 357.253 | 1886771.3 | 99.22 | % | 0.973 | | | | 0.98% |
| ScR 361.383 | 287580.3 | 98.26 | % | 0.884 | | | | 0.90% |
| Ag 328.068† | 177635.6 | 1.025 | mg/L | 0.0147 | 1.025 | mg/L | 0.0147 | 1.43% |
| Al 308.215† | 260071.3 | 205.9 | mg/L | 0.41 | 205.9 | mg/L | 0.41 | 0.20% |
| As 188.979† | 1409.0 | 1.018 | mg/L | 0.0100 | 1.018 | mg/L | 0.0100 | 0.98% |
| B 249.677† | -24.0 | -0.00970 | mg/L | 0.001187 | -0.00970 | mg/L | 0.001187 | 12.24% |
| Ba 233.527† | 3214.8 | 1.023 | mg/L | 0.0051 | 1.023 | mg/L | 0.0051 | 0.50% |
| Be 313.042† | 551747.9 | 1.004 | mg/L | 0.0021 | 1.004 | mg/L | 0.0021 | 0.21% |
| Ca 317.933† | 1468892.5 | 102.2 | mg/L | 0.21 | 102.2 | mg/L | 0.21 | 0.21% |
| Cd 228.802† | 22262.2 | 1.055 | mg/L | 0.0129 | 1.055 | mg/L | 0.0129 | 1.22% |
| Co 228.616† | 28742.1 | 0.9699 | mg/L | 0.01244 | 0.9699 | mg/L | 0.01244 | 1.28% |
| Cr 267.716† | 4925.8 | 1.039 | mg/L | 0.0048 | 1.039 | mg/L | 0.0048 | 0.46% |
| Cu 324.752† | 285018.5 | 1.041 | mg/L | 0.0133 | 1.041 | mg/L | 0.0133 | 1.28% |
| Fe 273.955† | 226418.6 | 199.9 | mg/L | 0.16 | 199.9 | mg/L | 0.16 | 0.08% |
| K 766.490† | -70.1 | -0.04899 | mg/L | 0.050312 | -0.04899 | mg/L | 0.050312 | 102.70% |
| Mg 279.077† | 93245.9 | 100.8 | mg/L | 0.43 | 100.8 | mg/L | 0.43 | 0.43% |
| Mn 257.610† | 28549.4 | 0.9734 | mg/L | 0.00363 | 0.9734 | mg/L | 0.00363 | 0.37% |
| Mo 202.031† | 98.3 | 0.00395 | mg/L | 0.000404 | 0.00395 | mg/L | 0.000404 | 10.24% |
| Na 589.592† | 254.2 | 0.02142 | mg/L | 0.004104 | 0.02142 | mg/L | 0.004104 | 19.16% |
| Na 330.237† | -2.8 | 0.2889 | mg/L | 0.11678 | 0.2889 | mg/L | 0.11678 | 40.43% |
| Ni 231.604† | 1557.4 | 0.9627 | mg/L | 0.00535 | 0.9627 | mg/L | 0.00535 | 0.56% |
| Pb 220.353† | 6466.6 | 0.9592 | mg/L | 0.01034 | 0.9592 | mg/L | 0.01034 | 1.08% |
| Sb 206.836† | 2835.2 | 1.048 | mg/L | 0.0135 | 1.048 | mg/L | 0.0135 | 1.29% |
| Se 196.026† | 1277.5 | 1.066 | mg/L | 0.0061 | 1.066 | mg/L | 0.0061 | 0.57% |
| Si 288.158† | -35.4 | -0.02024 | mg/L | 0.003071 | -0.02024 | mg/L | 0.003071 | 15.17% |
| Sn 189.927† | -55.7 | -0.00974 | mg/L | 0.002688 | -0.00974 | mg/L | 0.002688 | 27.60% |
| Sr 421.552† | 2354.3 | 0.00372 | mg/L | 0.000042 | 0.00372 | mg/L | 0.000042 | 1.12% |
| Ti 334.903† | 179.1 | 0.00159 | mg/L | 0.000359 | 0.00159 | mg/L | 0.000359 | 22.65% |
| Tl 190.801† | 1629.1 | 0.9740 | mg/L | 0.00881 | 0.9740 | mg/L | 0.00881 | 0.90% |
| V 292.402† | 96755.5 | 0.9878 | mg/L | 0.01033 | 0.9878 | mg/L | 0.01033 | 1.05% |
| Zn 206.200† | 593.5 | 0.9513 | mg/L | 0.00369 | 0.9513 | mg/L | 0.00369 | 0.39% |

Sequence No.: 6
Sample ID: CV
Analyst: ALA
Dilution: 1X

Autosampler Location: 7
Date Collected: 8/6/2010 9:50:08 AM
Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1905842.6 | 100.2 % | 0.81 | | | 0.81% |
| ScR 361.383 | 275838.7 | 94.25 % | 0.469 | | | 0.50% |
| Ag 328.068† | 181213.7 | 1.046 mg/L | 0.0028 | 1.046 mg/L | 0.0028 | 0.26% |
| Al 308.215† | 2841.4 | 2.217 mg/L | 0.0050 | 2.217 mg/L | 0.0050 | 0.23% |
| As 188.979† | 2829.6 | 2.068 mg/L | 0.0184 | 2.068 mg/L | 0.0184 | 0.89% |
| B 249.677† | 3461.7 | 1.044 mg/L | 0.0023 | 1.044 mg/L | 0.0023 | 0.22% |
| Ba 233.527† | 3351.1 | 1.086 mg/L | 0.0029 | 1.086 mg/L | 0.0029 | 0.26% |
| Be 313.042† | 562156.0 | 1.022 mg/L | 0.0081 | 1.022 mg/L | 0.0081 | 0.79% |
| Ca 317.933† | 31369.4 | 2.183 mg/L | 0.0117 | 2.183 mg/L | 0.0117 | 0.54% |
| Cd 228.802† | 22235.5 | 1.050 mg/L | 0.0092 | 1.050 mg/L | 0.0092 | 0.87% |
| Co 228.616† | 30212.5 | 1.021 mg/L | 0.0072 | 1.021 mg/L | 0.0072 | 0.71% |
| Cr 267.716† | 5185.8 | 1.100 mg/L | 0.0030 | 1.100 mg/L | 0.0030 | 0.28% |
| Cu 324.752† | 289540.6 | 1.044 mg/L | 0.0080 | 1.044 mg/L | 0.0080 | 0.77% |
| Fe 273.955† | 2442.1 | 2.150 mg/L | 0.0013 | 2.150 mg/L | 0.0013 | 0.06% |
| K 766.490† | 30647.7 | 21.43 mg/L | 0.057 | 21.43 mg/L | 0.057 | 0.26% |
| Mg 279.077† | 1999.9 | 2.169 mg/L | 0.0027 | 2.169 mg/L | 0.0027 | 0.12% |
| Mn 257.610† | 30572.0 | 1.043 mg/L | 0.0066 | 1.043 mg/L | 0.0066 | 0.63% |
| Mo 202.031† | 17554.2 | 1.021 mg/L | 0.0089 | 1.021 mg/L | 0.0089 | 0.87% |
| Na 589.592† | 624394.6 | 52.62 mg/L | 0.310 | 52.62 mg/L | 0.310 | 0.59% |
| Na 330.237† | 1594.6 | 55.16 mg/L | 0.237 | 55.16 mg/L | 0.237 | 0.43% |
| Ni 231.604† | 1705.1 | 1.055 mg/L | 0.0010 | 1.055 mg/L | 0.0010 | 0.10% |
| Pb 220.353† | 14179.1 | 2.057 mg/L | 0.0192 | 2.057 mg/L | 0.0192 | 0.93% |
| Sb 206.836† | 5666.5 | 2.116 mg/L | 0.0213 | 2.116 mg/L | 0.0213 | 1.01% |
| Se 196.026† | 2466.0 | 2.071 mg/L | 0.0178 | 2.071 mg/L | 0.0178 | 0.86% |
| Si 288.158† | 3326.4 | 2.256 mg/L | 0.0092 | 2.256 mg/L | 0.0092 | 0.41% |
| Sn 189.927† | 3778.0 | 1.029 mg/L | 0.0124 | 1.029 mg/L | 0.0124 | 1.20% |
| Sr 421.552† | 666444.3 | 1.054 mg/L | 0.0046 | 1.054 mg/L | 0.0046 | 0.44% |
| Ti 334.903† | 23150.0 | 1.053 mg/L | 0.0056 | 1.053 mg/L | 0.0056 | 0.53% |
| Tl 190.801† | 3525.8 | 2.050 mg/L | 0.0213 | 2.050 mg/L | 0.0213 | 1.04% |
| V 292.402† | 98599.5 | 1.029 mg/L | 0.0094 | 1.029 mg/L | 0.0094 | 0.91% |
| Zn 206.200† | 645.4 | 1.041 mg/L | 0.0040 | 1.041 mg/L | 0.0040 | 0.38% |

Sequence No.: 7
 Sample ID: CB
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 9:54:21 AM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1922942.6 | 101.1 | % | 0.99 | | | 0.98% |
| ScR 361.383 | 274349.7 | 93.74 | % | 0.319 | | | 0.34% |
| Ag 328.068† | -26.6 | -0.00015 | mg/L | 0.000267 | -0.00015 mg/L | 0.000267 | 174.16% |
| Al 308.215† | 0.5 | 0.00043 | mg/L | 0.002215 | 0.00043 mg/L | 0.002215 | 517.86% |
| As 188.979† | -4.5 | -0.00329 | mg/L | 0.000810 | -0.00329 mg/L | 0.000810 | 24.66% |
| B 249.677† | 1.4 | 0.00041 | mg/L | 0.002350 | 0.00041 mg/L | 0.002350 | 573.64% |
| Ba 233.527† | 3.4 | 0.00111 | mg/L | 0.001190 | 0.00111 mg/L | 0.001190 | 107.49% |
| Be 313.042† | 96.9 | 0.00018 | mg/L | 0.000056 | 0.00018 mg/L | 0.000056 | 31.61% |
| Ca 317.933† | 22.8 | 0.00158 | mg/L | 0.000780 | 0.00158 mg/L | 0.000780 | 49.26% |
| Cd 228.802† | -1.4 | -0.00005 | mg/L | 0.000254 | -0.00005 mg/L | 0.000254 | 467.92% |
| Co 228.616† | -0.0 | 0.00000 | mg/L | 0.000039 | 0.00000 mg/L | 0.000039 | >999.9% |
| Cr 267.716† | -0.1 | -0.00003 | mg/L | 0.000974 | -0.00003 mg/L | 0.000974 | >999.9% |
| Cu 324.752† | 7.9 | 0.00003 | mg/L | 0.000235 | 0.00003 mg/L | 0.000235 | 821.65% |
| Fe 273.955† | 1.2 | 0.00110 | mg/L | 0.001478 | 0.00110 mg/L | 0.001478 | 134.07% |
| K 766.490† | 60.9 | 0.04258 | mg/L | 0.027136 | 0.04258 mg/L | 0.027136 | 63.72% |
| Mg 279.077† | -0.7 | -0.00076 | mg/L | 0.012151 | -0.00076 mg/L | 0.012151 | >999.9% |
| Mn 257.610† | 5.6 | 0.00019 | mg/L | 0.000118 | 0.00019 mg/L | 0.000118 | 61.67% |
| Mo 202.031† | 4.0 | 0.00024 | mg/L | 0.000210 | 0.00024 mg/L | 0.000210 | 89.14% |
| Na 589.592† | 22.6 | 0.00191 | mg/L | 0.003293 | 0.00191 mg/L | 0.003293 | 172.82% |
| Na 330.237† | -4.2 | -0.1459 | mg/L | 0.11158 | -0.1459 mg/L | 0.11158 | 76.49% |
| Ni 231.604† | 4.6 | 0.00282 | mg/L | 0.001610 | 0.00282 mg/L | 0.001610 | 57.10% |
| Pb 220.353† | -4.6 | -0.00067 | mg/L | 0.000465 | -0.00067 mg/L | 0.000465 | 69.53% |
| Sb 206.836† | 3.1 | 0.00116 | mg/L | 0.001963 | 0.00116 mg/L | 0.001963 | 169.48% |
| Se 196.026† | 4.2 | 0.00351 | mg/L | 0.002781 | 0.00351 mg/L | 0.002781 | 79.16% |
| Si 288.158† | 9.7 | 0.00654 | mg/L | 0.004024 | 0.00654 mg/L | 0.004024 | 61.54% |
| Sn 189.927† | 3.9 | 0.00107 | mg/L | 0.001045 | 0.00107 mg/L | 0.001045 | 97.60% |
| Sr 421.552† | 66.0 | 0.00010 | mg/L | 0.000049 | 0.00010 mg/L | 0.000049 | 46.84% |
| Ti 334.903† | -8.3 | -0.00038 | mg/L | 0.000499 | -0.00038 mg/L | 0.000499 | 131.37% |
| Tl 190.801† | 3.7 | 0.00212 | mg/L | 0.001605 | 0.00212 mg/L | 0.001605 | 75.55% |
| V 292.402† | -8.3 | -0.00009 | mg/L | 0.000241 | -0.00009 mg/L | 0.000241 | 280.50% |
| Zn 206.200† | 0.4 | 0.00064 | mg/L | 0.002043 | 0.00064 mg/L | 0.002043 | 319.40% |

Sequence No.: 8
Sample ID: RF71 MB1 SWC
Analyst: ALA
Dilution: 2X

Del

Autosampler Location: 304
Date Collected: 8/6/2010 9:58:17 AM
Data Type: Original

Nebulizer Parameters: RF71 MB1 SWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RF71 MB1 SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1948105.1 | 102.4 | % | 0.75 | | | | 0.73% |
| ScR 361.383 | 292462.1 | 99.92 | % | 2.909 | | | | 2.91% |
| Ag 328.068† | -18.5 | -0.00011 | mg/L | 0.000189 | -0.00021 | mg/L | 0.000378 | 176.95% |
| Al 308.215† | 4.1 | 0.00328 | mg/L | 0.006860 | 0.00656 | mg/L | 0.013719 | 209.18% |
| As 188.979† | -0.6 | -0.00045 | mg/L | 0.001666 | -0.00089 | mg/L | 0.003333 | 373.88% |
| B 249.677† | -2.7 | -0.00082 | mg/L | 0.001528 | -0.00164 | mg/L | 0.003056 | 186.90% |
| Ba 233.527† | 0.7 | 0.00022 | mg/L | 0.000692 | 0.00044 | mg/L | 0.001383 | 314.76% |
| Be 313.042† | -22.8 | -0.00004 | mg/L | 0.000056 | -0.00008 | mg/L | 0.000113 | 135.97% |
| Ca 317.933† | 134.8 | 0.00938 | mg/L | 0.001124 | 0.01876 | mg/L | 0.002247 | 11.98% |
| Cd 228.802† | -2.6 | -0.00012 | mg/L | 0.000132 | -0.00024 | mg/L | 0.000264 | 109.28% |
| Co 228.616† | 1.5 | 0.00005 | mg/L | 0.000122 | 0.00010 | mg/L | 0.000243 | 239.44% |
| Cr 267.716† | 1.2 | 0.00026 | mg/L | 0.001019 | 0.00052 | mg/L | 0.002037 | 390.40% |
| Cu 324.752† | -55.0 | -0.00020 | mg/L | 0.000161 | -0.00040 | mg/L | 0.000322 | 81.11% |
| Fe 273.955† | 0.2 | 0.00014 | mg/L | 0.003707 | 0.00028 | mg/L | 0.007414 | >999.9% |
| K 766.490† | -19.8 | -0.01383 | mg/L | 0.011765 | -0.02765 | mg/L | 0.023531 | 85.09% |
| Mg 279.077† | 5.2 | 0.00559 | mg/L | 0.009401 | 0.01118 | mg/L | 0.018802 | 168.23% |
| Mn 257.610† | -5.9 | -0.00020 | mg/L | 0.000095 | -0.00040 | mg/L | 0.000191 | 47.70% |
| Mo 202.031† | -6.7 | -0.00039 | mg/L | 0.000198 | -0.00078 | mg/L | 0.000396 | 51.03% |
| Na 589.592† | 29.4 | 0.00248 | mg/L | 0.003401 | 0.00496 | mg/L | 0.006802 | 137.12% |
| Na 330.237† | 6.2 | 0.2155 | mg/L | 0.31297 | 0.4310 | mg/L | 0.62593 | 145.22% |
| Ni 231.604† | 4.5 | 0.00278 | mg/L | 0.001182 | 0.00556 | mg/L | 0.002364 | 42.52% |
| Pb 220.353† | 2.9 | 0.00042 | mg/L | 0.001131 | 0.00084 | mg/L | 0.002261 | 267.74% |
| Sb 206.836† | -0.9 | -0.00033 | mg/L | 0.000110 | -0.00066 | mg/L | 0.000221 | 33.54% |
| Se 196.026† | 10.4 | 0.00870 | mg/L | 0.005925 | 0.01739 | mg/L | 0.011849 | 68.13% |
| Si 288.158† | -1.6 | -0.00106 | mg/L | 0.003415 | -0.00212 | mg/L | 0.006831 | 322.16% |
| Sn 189.927† | 2.8 | 0.00077 | mg/L | 0.000558 | 0.00154 | mg/L | 0.001115 | 72.53% |
| Sr 421.552† | -16.8 | -0.00003 | mg/L | 0.000064 | -0.00005 | mg/L | 0.000129 | 241.27% |
| Ti 334.903† | 2.0 | 0.00009 | mg/L | 0.000719 | 0.00018 | mg/L | 0.001437 | 809.25% |
| Tl 190.801† | 5.9 | 0.00342 | mg/L | 0.002256 | 0.00685 | mg/L | 0.004513 | 65.89% |
| V 292.402† | -5.2 | -0.00005 | mg/L | 0.000174 | -0.00011 | mg/L | 0.000347 | 325.74% |
| Zn 206.200† | 0.4 | 0.00057 | mg/L | 0.000343 | 0.00115 | mg/L | 0.000686 | 59.87% |

Sequence No.: 9
Sample ID: RG11 MB1 SWC
Analyst: ALA
Dilution: 2X

DL

Autosampler Location: 305
Date Collected: 8/6/2010 10:02:29 AM
Data Type: Original

Nebulizer Parameters: RG11 MB1 SWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG11 MB1 SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|------------------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1950662.5 | 102.6 | % | 1.04 | | | 1.01% |
| ScR 361.383 | 295484.0 | 101.0 | % | 2.92 | | | 2.89% |
| Ag 328.068† | 2.7 | 0.00002 | mg/L | 0.000312 | 0.00003 | mg/L | 0.000624 >999.9% |
| Al 308.215† | 1.2 | 0.00099 | mg/L | 0.004016 | 0.00198 | mg/L | 0.008033 405.31% |
| As 188.979† | 0.8 | 0.00062 | mg/L | 0.002395 | 0.00124 | mg/L | 0.004790 387.51% |
| B 249.677† | -5.1 | -0.00155 | mg/L | 0.001520 | -0.00311 | mg/L | 0.003040 97.87% |
| Ba 233.527† | 0.4 | 0.00014 | mg/L | 0.000651 | 0.00028 | mg/L | 0.001303 464.67% |
| Be 313.042† | -46.7 | -0.00008 | mg/L | 0.000075 | -0.00017 | mg/L | 0.000151 88.83% |
| Ca 317.933† | 123.3 | 0.00858 | mg/L | 0.001351 | 0.01715 | mg/L | 0.002703 15.76% |
| Cd 228.802† | 0.3 | 0.00002 | mg/L | 0.000179 | 0.00003 | mg/L | 0.000358 >999.9% |
| Co 228.616† | 0.4 | 0.00001 | mg/L | 0.000111 | 0.00002 | mg/L | 0.000222 >999.9% |
| Cr 267.716† | 6.9 | 0.00145 | mg/L | 0.000947 | 0.00291 | mg/L | 0.001894 65.11% |
| Cu 324.752† | -69.1 | -0.00025 | mg/L | 0.000383 | -0.00050 | mg/L | 0.000766 153.45% |
| Fe 273.955† | -0.6 | -0.00055 | mg/L | 0.001553 | -0.00111 | mg/L | 0.003106 280.09% |
| K 766.490† | 18.1 | 0.01263 | mg/L | 0.018316 | 0.02527 | mg/L | 0.036632 144.97% |
| Mg 279.077† | 0.2 | 0.00027 | mg/L | 0.004795 | 0.00053 | mg/L | 0.009591 >999.9% |
| Mn 257.610† | -1.9 | -0.00006 | mg/L | 0.000070 | -0.00013 | mg/L | 0.000140 110.80% |
| Mo 202.031† | -5.4 | -0.00031 | mg/L | 0.000297 | -0.00063 | mg/L | 0.000595 95.03% |
| Na 589.592† | 19.5 | 0.00164 | mg/L | 0.003087 | 0.00329 | mg/L | 0.006173 187.66% |
| Na 330.237† | 0.7 | 0.02327 | mg/L | 0.096014 | 0.04654 | mg/L | 0.192029 412.64% |
| Ni 231.604† | 4.3 | 0.00266 | mg/L | 0.000669 | 0.00532 | mg/L | 0.001337 25.13% |
| Pb 220.353† | -3.1 | -0.00045 | mg/L | 0.000209 | -0.00090 | mg/L | 0.000419 46.48% |
| Sb 206.836† | 1.2 | 0.00044 | mg/L | 0.001260 | 0.00089 | mg/L | 0.002519 284.26% |
| Se 196.026† | 8.3 | 0.00697 | mg/L | 0.001442 | 0.01394 | mg/L | 0.002883 20.68% |
| Si 288.158† | 9.0 | 0.00606 | mg/L | 0.000946 | 0.01212 | mg/L | 0.001891 15.60% |
| Sn 189.927† | 4.2 | 0.00113 | mg/L | 0.000314 | 0.00227 | mg/L | 0.000628 27.70% |
| Sr 421.552† | -30.3 | -0.00005 | mg/L | 0.000007 | -0.00010 | mg/L | 0.000013 13.92% |
| Ti 334.903† | 15.3 | 0.00070 | mg/L | 0.000369 | 0.00139 | mg/L | 0.000738 53.00% |
| Tl 190.801† | 3.1 | 0.00180 | mg/L | 0.002141 | 0.00360 | mg/L | 0.004281 118.77% |
| V 292.402† | -19.7 | -0.00020 | mg/L | 0.000018 | -0.00040 | mg/L | 0.000037 9.18% |
| Zn 206.200† | -0.5 | -0.00076 | mg/L | 0.001164 | -0.00151 | mg/L | 0.002329 153.92% |

Sequence No.: 10
Sample ID: RG11 A SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 306
Date Collected: 8/6/2010 10:06:39 AM
Data Type: Original

ER 1/5

Nebulizer Parameters: RG11 A SWC

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG11 A SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|----------|--------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1969031.6 | 103.5 | % | 1.76 | | | | 1.70% |
| ScR 361.383 | 303919.5 | 103.8 | % | 1.28 | | | | 1.23% |
| Ag 328.068† | 336.3 | 0.00153 | mg/L | 0.000181 | 0.00306 | mg/L | 0.000362 | 11.84% |
| Al 308.215† | 123001.2 | 97.36 | mg/L | 0.383 | 194.7 | mg/L | 0.77 | 0.39% |
| As 188.979† | -106.1 | 0.04896 | mg/L | 0.003118 | 0.09792 | mg/L | 0.006236 | 6.37% |
| B 249.677† | 350.7 | 0.1060 | mg/L | 0.00182 | 0.2120 | mg/L | 0.00364 | 1.72% |
| Ba 233.527† | 2351.0 | 0.7366 | mg/L | 0.00802 | 1.473 | mg/L | 0.0160 | 1.09% |
| Be 313.042† | 644.4 | 0.00086 | mg/L | 0.000027 | 0.00171 | mg/L | 0.000054 | 3.15% |
| Ca 317.933† | 1096563.4 | 76.29 | mg/L | 0.844 | 152.6 | mg/L | 1.69 | 1.11% |
| Cd 228.802† | 31.5 | 0.00682 | mg/L | 0.000282 | 0.01364 | mg/L | 0.000565 | 4.14% |
| Co 228.616† | 5176.4 | 0.1577 | mg/L | 0.00244 | 0.3155 | mg/L | 0.00488 | 1.55% |
| Cr 267.716† | 35038.8 | 7.437 | mg/L | 0.0327 | 14.87 | mg/L | 0.065 | 0.44% |
| Cu 324.752† | 3121499.1 | 11.28 | mg/L | 0.215 | 22.56 | mg/L | 0.429 | 1.90% |
| Fe 273.955† | 299813.7 | 264.6 | mg/L | 1.61 | 529.3 | mg/L | 3.23 | 0.61% |
| K 766.490† | 7627.0 | 5.333 | mg/L | 0.0247 | 10.67 | mg/L | 0.049 | 0.46% |
| Mg 279.077† | 48310.0 | 52.15 | mg/L | 0.293 | 104.3 | mg/L | 0.59 | 0.56% |
| Mn 257.610† | 103635.1 | 3.536 | mg/L | 0.0431 | 7.071 | mg/L | 0.0862 | 1.22% |
| Mo 202.031† | 10609.6 | 0.6159 | mg/L | 0.01002 | 1.232 | mg/L | 0.0200 | 1.63% |
| Na 589.592† | 38660.0 | 3.258 | mg/L | 0.0275 | 6.516 | mg/L | 0.0551 | 0.85% |
| Na 330.237† | 37.2 | 3.295 | mg/L | 0.0890 | 6.590 | mg/L | 0.1781 | 2.70% |
| Ni 231.604† | 12663.5 | 7.822 | mg/L | 0.0944 | 15.64 | mg/L | 0.189 | 1.21% |
| Pb 220.353† | 2227.2 | 0.3214 | mg/L | 0.00545 | 0.6428 | mg/L | 0.01089 | 1.69% |
| Sb 206.836† | 247.1 | 0.02749 | mg/L | 0.002804 | 0.05499 | mg/L | 0.005608 | 10.20% |
| Se 196.026† | 41.4 | 0.02960 | mg/L | 0.003400 | 0.05920 | mg/L | 0.006799 | 11.49% |
| Si 288.158† | 3210.6 | 2.174 | mg/L | 0.0322 | 4.348 | mg/L | 0.0645 | 1.48% |
| Sn 189.927† | 160.9 | 0.05080 | mg/L | 0.001812 | 0.1016 | mg/L | 0.00362 | 3.57% |
| Sr 421.552† | 177813.6 | 0.2812 | mg/L | 0.00119 | 0.5624 | mg/L | 0.00237 | 0.42% |
| Ti 334.903† | 165991.7 | 7.552 | mg/L | 0.0567 | 15.10 | mg/L | 0.113 | 0.75% |
| Tl 190.801† | -47.7 | 0.01394 | mg/L | 0.004894 | 0.02787 | mg/L | 0.009788 | 35.12% |
| V 292.402† | 43027.6 | 0.4460 | mg/L | 0.00749 | 0.8919 | mg/L | 0.01498 | 1.68% |
| Zn 206.200† | 1380.8 | 2.222 | mg/L | 0.0235 | 4.444 | mg/L | 0.0470 | 1.06% |

Sequence No.: 11
 Sample ID: RF71 ADUP SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 307
 Date Collected: 8/6/2010 10:10:22 AM
 Data Type: Original

Del

Nebulizer Parameters: RF71 ADUP SWC

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RF71 ADUP SWC

| Analyte | Mean Corrected | | Calib. | | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------|----------|---------|-------|----------|---------|
| | Intensity | Conc. | Units | Std.Dev. | Conc. | Units | | |
| ScA 357.253 | 1940833.7 | 102.1 | % | 0.62 | | | | 0.61% |
| ScR 361.383 | 293686.2 | 100.3 | % | 0.78 | | | | 0.78% |
| Ag 328.068† | 30.1 | 0.00004 | mg/L | 0.000273 | 0.00007 | mg/L | 0.000546 | 737.43% |
| Al 308.215† | 146057.3 | 115.6 | mg/L | 1.14 | 231.3 | mg/L | 2.29 | 0.99% |
| As 188.979† | -55.4 | 0.05587 | mg/L | 0.001883 | 0.1117 | mg/L | 0.00377 | 3.37% |
| B 249.677† | 239.5 | 0.07218 | mg/L | 0.002896 | 0.1444 | mg/L | 0.00579 | 4.01% |
| Ba 233.527† | 996.2 | 0.3069 | mg/L | 0.00376 | 0.6138 | mg/L | 0.00753 | 1.23% |
| Be 313.042† | 1030.8 | 0.00164 | mg/L | 0.000045 | 0.00327 | mg/L | 0.000090 | 2.76% |
| Ca 317.933† | 432545.3 | 30.09 | mg/L | 0.387 | 60.19 | mg/L | 0.775 | 1.29% |
| Cd 228.802† | 84.5 | 0.00432 | mg/L | 0.000019 | 0.00864 | mg/L | 0.000037 | 0.43% |
| Co 228.616† | 2329.0 | 0.06752 | mg/L | 0.000403 | 0.1350 | mg/L | 0.00081 | 0.60% |
| Cr 267.716† | 1352.6 | 0.2867 | mg/L | 0.00368 | 0.5733 | mg/L | 0.00737 | 1.29% |
| Cu 324.752† | 88482.6 | 0.3283 | mg/L | 0.00355 | 0.6566 | mg/L | 0.00709 | 1.08% |
| Fe 273.955† | 194488.1 | 171.7 | mg/L | 1.98 | 343.3 | mg/L | 3.97 | 1.16% |
| K 766.490† | 13935.7 | 9.743 | mg/L | 0.1511 | 19.49 | mg/L | 0.302 | 1.55% |
| Mg 279.077† | 54580.2 | 58.98 | mg/L | 0.793 | 118.0 | mg/L | 1.59 | 1.35% |
| Mn 257.610† | 60088.4 | 2.050 | mg/L | 0.0294 | 4.099 | mg/L | 0.0587 | 1.43% |
| Mo 202.031† | 186.7 | 0.01034 | mg/L | 0.000047 | 0.02068 | mg/L | 0.000094 | 0.45% |
| Na 589.592† | 198397.1 | 16.72 | mg/L | 0.207 | 33.44 | mg/L | 0.414 | 1.24% |
| Na 330.237† | 454.7 | 17.23 | mg/L | 0.251 | 34.46 | mg/L | 0.502 | 1.46% |
| Ni 231.604† | 447.2 | 0.2762 | mg/L | 0.00447 | 0.5525 | mg/L | 0.00894 | 1.62% |
| Pb 220.353† | 925.6 | 0.1419 | mg/L | 0.00017 | 0.2839 | mg/L | 0.00035 | 0.12% |
| Sb 206.836† | 23.8 | 0.01395 | mg/L | 0.001746 | 0.02789 | mg/L | 0.003491 | 12.52% |
| Se 196.026† | 44.8 | 0.03559 | mg/L | 0.001748 | 0.07118 | mg/L | 0.003496 | 4.91% |
| Si 288.158† | 10946.0 | 7.412 | mg/L | 0.0669 | 14.82 | mg/L | 0.134 | 0.90% |
| Sn 189.927† | 13.9 | 0.00763 | mg/L | 0.000791 | 0.01526 | mg/L | 0.001583 | 10.37% |
| Sr 421.552† | 157880.1 | 0.2497 | mg/L | 0.00337 | 0.4993 | mg/L | 0.00674 | 1.35% |
| Ti 334.903† | 117921.9 | 5.368 | mg/L | 0.0714 | 10.74 | mg/L | 0.143 | 1.33% |
| Tl 190.801† | -34.8 | 0.00681 | mg/L | 0.001641 | 0.01362 | mg/L | 0.003281 | 24.09% |
| V 292.402† | 33574.2 | 0.3286 | mg/L | 0.00359 | 0.6573 | mg/L | 0.00718 | 1.09% |
| Zn 206.200† | 372.5 | 0.5975 | mg/L | 0.00527 | 1.195 | mg/L | 0.0105 | 0.88% |

Sequence No.: 12
Sample ID: RF71 A SWC
Analyst: ALA
Dilution: 2X

DEL

Autosampler Location: 308
Date Collected: 8/6/2010 10:14:18 AM
Data Type: Original

Nebulizer Parameters: RF71 A SWC

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RF71 A SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|------------------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1935116.0 | 101.8 | % | 1.28 | | | 1.26% |
| ScR 361.383 | 296773.6 | 101.4 | % | 0.70 | | | 0.69% |
| Ag 328.068† | 42.6 | 0.00013 | mg/L | 0.000171 | 0.00026 | mg/L | 0.000342 131.39% |
| Al 308.215† | 158364.6 | 125.4 | mg/L | 0.85 | 250.7 | mg/L | 1.70 0.68% |
| As 188.979† | -72.1 | 0.05526 | mg/L | 0.002437 | 0.1105 | mg/L | 0.00487 4.41% |
| B 249.677† | 266.2 | 0.08020 | mg/L | 0.001474 | 0.1604 | mg/L | 0.00295 1.84% |
| Ba 233.527† | 1075.6 | 0.3316 | mg/L | 0.00215 | 0.6631 | mg/L | 0.00429 0.65% |
| Be 313.042† | 1079.8 | 0.00169 | mg/L | 0.000046 | 0.00338 | mg/L | 0.000092 2.71% |
| Ca 317.933† | 472819.8 | 32.90 | mg/L | 0.254 | 65.79 | mg/L | 0.507 0.77% |
| Cd 228.802† | 88.9 | 0.00458 | mg/L | 0.000449 | 0.00916 | mg/L | 0.000897 9.80% |
| Co 228.616† | 2548.5 | 0.07372 | mg/L | 0.000919 | 0.1474 | mg/L | 0.00184 1.25% |
| Cr 267.716† | 1483.4 | 0.3142 | mg/L | 0.00205 | 0.6284 | mg/L | 0.00410 0.65% |
| Cu 324.752† | 95159.4 | 0.3529 | mg/L | 0.00406 | 0.7057 | mg/L | 0.00812 1.15% |
| Fe 273.955† | 207505.3 | 183.2 | mg/L | 1.21 | 366.3 | mg/L | 2.42 0.66% |
| K 766.490† | 14925.0 | 10.44 | mg/L | 0.096 | 20.87 | mg/L | 0.193 0.92% |
| Mg 279.077† | 59318.2 | 64.10 | mg/L | 0.476 | 128.2 | mg/L | 0.95 0.74% |
| Mn 257.610† | 62128.7 | 2.119 | mg/L | 0.0132 | 4.238 | mg/L | 0.0264 0.62% |
| Mo 202.031† | 210.7 | 0.01168 | mg/L | 0.000198 | 0.02337 | mg/L | 0.000397 1.70% |
| Na 589.592† | 207784.6 | 17.51 | mg/L | 0.096 | 35.02 | mg/L | 0.192 0.55% |
| Na 330.237† | 482.0 | 18.36 | mg/L | 0.137 | 36.72 | mg/L | 0.275 0.75% |
| Ni 231.604† | 477.0 | 0.2946 | mg/L | 0.00290 | 0.5893 | mg/L | 0.00580 0.98% |
| Pb 220.353† | 1003.9 | 0.1542 | mg/L | 0.00186 | 0.3083 | mg/L | 0.00372 1.21% |
| Sb 206.836† | 34.2 | 0.01854 | mg/L | 0.001025 | 0.03709 | mg/L | 0.002050 5.53% |
| Se 196.026† | 38.8 | 0.03036 | mg/L | 0.005474 | 0.06073 | mg/L | 0.010948 18.03% |
| Si 288.158† | 10940.5 | 7.408 | mg/L | 0.0629 | 14.82 | mg/L | 0.126 0.85% |
| Sn 189.927† | 17.9 | 0.00914 | mg/L | 0.000924 | 0.01829 | mg/L | 0.001848 10.10% |
| Sr 421.552† | 169060.7 | 0.2674 | mg/L | 0.00252 | 0.5347 | mg/L | 0.00503 0.94% |
| Ti 334.903† | 132058.6 | 6.012 | mg/L | 0.0407 | 12.02 | mg/L | 0.081 0.68% |
| Tl 190.801† | -33.8 | 0.00905 | mg/L | 0.002683 | 0.01810 | mg/L | 0.005366 29.64% |
| V 292.402† | 38812.4 | 0.3816 | mg/L | 0.00683 | 0.7631 | mg/L | 0.01365 1.79% |
| Zn 206.200† | 397.9 | 0.6382 | mg/L | 0.00860 | 1.276 | mg/L | 0.0172 1.35% |

Sequence No.: 13
 Sample ID: RF71 ASPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 309
 Date Collected: 8/6/2010 10:18:14 AM
 Data Type: Original

Nebulizer Parameters: RF71 ASPK SWC

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RF71 ASPK SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------|----------|--------|
| ScA 357.253 | 1935544.1 | 101.8 | % | 1.31 | | | 1.29% |
| ScR 361.383 | 296252.8 | 101.2 | % | 1.57 | | | 1.55% |
| Ag 328.068† | 85187.9 | 0.4917 | mg/L | 0.00849 | 0.9833 mg/L | 0.01699 | 1.73% |
| Al 308.215† | 155584.6 | 123.2 | mg/L | 2.60 | 246.3 mg/L | 5.20 | 2.11% |
| As 188.979† | 2683.0 | 2.049 | mg/L | 0.0336 | 4.097 mg/L | 0.0671 | 1.64% |
| B 249.677† | 283.4 | 0.08420 | mg/L | 0.001285 | 0.1684 mg/L | 0.00257 | 1.53% |
| Ba 233.527† | 7250.2 | 2.335 | mg/L | 0.0383 | 4.669 mg/L | 0.0766 | 1.64% |
| Be 313.042† | 267105.3 | 0.4856 | mg/L | 0.01274 | 0.9712 mg/L | 0.02548 | 2.62% |
| Ca 317.933† | 622544.5 | 43.31 | mg/L | 1.104 | 86.63 mg/L | 2.207 | 2.55% |
| Cd 228.802† | 11046.7 | 0.5186 | mg/L | 0.00810 | 1.037 mg/L | 0.0162 | 1.56% |
| Co 228.616† | 16738.4 | 0.5538 | mg/L | 0.00830 | 1.108 mg/L | 0.0166 | 1.50% |
| Cr 267.716† | 3826.1 | 0.8098 | mg/L | 0.01339 | 1.620 mg/L | 0.0268 | 1.65% |
| Cu 324.752† | 228301.1 | 0.8331 | mg/L | 0.01445 | 1.666 mg/L | 0.0289 | 1.73% |
| Fe 273.955† | 201940.8 | 178.2 | mg/L | 4.22 | 356.5 mg/L | 8.43 | 2.37% |
| K 766.490† | 29008.4 | 20.28 | mg/L | 0.427 | 40.56 mg/L | 0.854 | 2.11% |
| Mg 279.077† | 65468.9 | 70.76 | mg/L | 1.601 | 141.5 mg/L | 3.20 | 2.26% |
| Mn 257.610† | 73242.0 | 2.499 | mg/L | 0.0639 | 4.997 mg/L | 0.1278 | 2.56% |
| Mo 202.031† | 209.7 | 0.01145 | mg/L | 0.000226 | 0.02290 mg/L | 0.000451 | 1.97% |
| Na 589.592† | 327164.0 | 27.57 | mg/L | 0.604 | 55.14 mg/L | 1.207 | 2.19% |
| Na 330.237† | 785.4 | 28.76 | mg/L | 0.562 | 57.52 mg/L | 1.124 | 1.95% |
| Ni 231.604† | 1215.2 | 0.7509 | mg/L | 0.01343 | 1.502 mg/L | 0.0269 | 1.79% |
| Pb 220.353† | 14286.0 | 2.080 | mg/L | 0.0300 | 4.161 mg/L | 0.0599 | 1.44% |
| Sb 206.836† | 1014.4 | 0.3797 | mg/L | 0.00438 | 0.7595 mg/L | 0.00876 | 1.15% |
| Se 196.026† | 2443.5 | 2.050 | mg/L | 0.0333 | 4.099 mg/L | 0.0666 | 1.62% |
| Si 288.158† | 11372.0 | 7.702 | mg/L | 0.1187 | 15.40 mg/L | 0.237 | 1.54% |
| Sn 189.927† | 6.7 | 0.00676 | mg/L | 0.002135 | 0.01351 mg/L | 0.004270 | 31.60% |
| Sr 421.552† | 481853.3 | 0.7620 | mg/L | 0.01693 | 1.524 mg/L | 0.0339 | 2.22% |
| Ti 334.903† | 128811.4 | 5.863 | mg/L | 0.1290 | 11.73 mg/L | 0.258 | 2.20% |
| Tl 190.801† | 3265.5 | 1.925 | mg/L | 0.0304 | 3.850 mg/L | 0.0609 | 1.58% |
| V 292.402† | 81592.6 | 0.8285 | mg/L | 0.01035 | 1.657 mg/L | 0.0207 | 1.25% |
| Zn 206.200† | 675.2 | 1.085 | mg/L | 0.0172 | 2.171 mg/L | 0.0344 | 1.58% |

Sequence No.: 14 *RF71 APOST SWC*
 Sample ID: RF71 APOST SWC *222222*
 Analyst: ALA
 Dilution: 2X
use #89-10

Autosampler Location: 310
 Date Collected: 8/6/2010 10:21:59 AM
 Data Type: Original

Nebulizer Parameters: RF71 APOST SWC
 Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RF71 APOST SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1945358.4 | 102.3 | % | 0.76 | | | 0.75% |
| ScR 361.383 | 299180.8 | 102.2 | % | 0.74 | | | 0.72% |
| Ag 328.068† | 85858.9 | 0.4955 | mg/L | 0.00175 | 0.9911 mg/L | 0.00350 | 0.35% |
| Al 308.215† | 156169.7 | 123.6 | mg/L | 0.25 | 247.2 mg/L | 0.51 | 0.20% |
| As 188.979† | 2737.8 | 2.088 | mg/L | 0.0161 | 4.176 mg/L | 0.0321 | 0.77% |
| B 249.677† | 264.0 | 0.07833 | mg/L | 0.001573 | 0.1567 mg/L | 0.00315 | 2.01% |
| Ba 233.527† | 7253.1 | 2.335 | mg/L | 0.0148 | 4.671 mg/L | 0.0295 | 0.63% |
| Be 313.042† | 266419.4 | 0.4843 | mg/L | 0.00143 | 0.9686 mg/L | 0.00286 | 0.30% |
| Ca 317.933† | 603300.5 | 41.98 | mg/L | 0.139 | 83.95 mg/L | 0.278 | 0.33% |
| Cd 228.802† | 11146.4 | 0.5232 | mg/L | 0.00505 | 1.046 mg/L | 0.0101 | 0.96% |
| Co 228.616† | 16949.7 | 0.5610 | mg/L | 0.00502 | 1.122 mg/L | 0.0100 | 0.90% |
| Cr 267.716† | 3815.3 | 0.8074 | mg/L | 0.00605 | 1.615 mg/L | 0.0121 | 0.75% |
| Cu 324.752† | 228689.1 | 0.8345 | mg/L | 0.00591 | 1.669 mg/L | 0.0118 | 0.71% |
| Fe 273.955† | 203762.5 | 179.9 | mg/L | 0.82 | 359.7 mg/L | 1.64 | 0.46% |
| K 766.490† | 28958.5 | 20.25 | mg/L | 0.018 | 40.49 mg/L | 0.037 | 0.09% |
| Mg 279.077† | 66988.2 | 72.40 | mg/L | 0.191 | 144.8 mg/L | 0.38 | 0.26% |
| Mn 257.610† | 74258.5 | 2.533 | mg/L | 0.0066 | 5.067 mg/L | 0.0132 | 0.26% |
| Mo 202.031† | 202.9 | 0.01108 | mg/L | 0.000287 | 0.02215 mg/L | 0.000573 | 2.59% |
| Na 589.592† | 319113.9 | 26.89 | mg/L | 0.059 | 53.78 mg/L | 0.117 | 0.22% |
| Na 330.237† | 769.8 | 28.20 | mg/L | 0.270 | 56.41 mg/L | 0.540 | 0.96% |
| Ni 231.604† | 1220.0 | 0.7550 | mg/L | 0.00570 | 1.510 mg/L | 0.0114 | 0.75% |
| Pb 220.353† | 14424.6 | 2.100 | mg/L | 0.0153 | 4.201 mg/L | 0.0306 | 0.73% |
| Sb 206.836† | 5550.7 | 2.070 | mg/L | 0.0172 | 4.139 mg/L | 0.0343 | 0.83% |
| Se 196.026† | 2510.8 | 2.106 | mg/L | 0.0216 | 4.212 mg/L | 0.0431 | 1.02% |
| Si 288.158† | 10979.3 | 7.436 | mg/L | 0.0555 | 14.87 mg/L | 0.111 | 0.75% |
| Sn 189.927† | 2.7 | 0.00666 | mg/L | 0.000348 | 0.01333 mg/L | 0.000696 | 5.22% |
| Sr 421.552† | 474377.4 | 0.7502 | mg/L | 0.00207 | 1.500 mg/L | 0.0041 | 0.28% |
| Ti 334.903† | 128325.1 | 5.841 | mg/L | 0.0133 | 11.68 mg/L | 0.027 | 0.23% |
| Tl 190.801† | 3295.4 | 1.943 | mg/L | 0.0148 | 3.885 mg/L | 0.0295 | 0.76% |
| V 292.402† | 83871.7 | 0.8520 | mg/L | 0.01263 | 1.704 mg/L | 0.0253 | 1.48% |
| Zn 206.200† | 677.4 | 1.089 | mg/L | 0.0142 | 2.178 mg/L | 0.0284 | 1.30% |

Sequence No.: 15
 Sample ID: RF71 MB1SPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 311
 Date Collected: 8/6/2010 10:25:42 AM
 Data Type: Original

Del

Nebulizer Parameters: RF71 MB1SPK SWC
 Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RF71 MB1SPK SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1937689.8 | 101.9 | % | 0.32 | | | | 0.32% |
| ScR 361.383 | 296376.3 | 101.3 | % | 0.39 | | | | 0.38% |
| Ag 328.068† | 93882.6 | 0.5420 | mg/L | 0.00234 | 1.084 | mg/L | 0.0047 | 0.43% |
| Al 308.215† | 2713.8 | 2.139 | mg/L | 0.0058 | 4.278 | mg/L | 0.0115 | 0.27% |
| As 188.979† | 2923.3 | 2.118 | mg/L | 0.0074 | 4.236 | mg/L | 0.0149 | 0.35% |
| B 249.677† | -3.5 | -0.00235 | mg/L | 0.000760 | -0.00470 | mg/L | 0.001519 | 32.34% |
| Ba 233.527† | 6536.8 | 2.120 | mg/L | 0.0086 | 4.240 | mg/L | 0.0172 | 0.41% |
| Be 313.042† | 275757.6 | 0.5016 | mg/L | 0.00257 | 1.003 | mg/L | 0.0051 | 0.51% |
| Ca 317.933† | 146668.3 | 10.20 | mg/L | 0.051 | 20.41 | mg/L | 0.102 | 0.50% |
| Cd 228.802† | 11272.5 | 0.5286 | mg/L | 0.00064 | 1.057 | mg/L | 0.0013 | 0.12% |
| Co 228.616† | 15317.7 | 0.5179 | mg/L | 0.00176 | 1.036 | mg/L | 0.0035 | 0.34% |
| Cr 267.716† | 2537.0 | 0.5367 | mg/L | 0.00289 | 1.073 | mg/L | 0.0058 | 0.54% |
| Cu 324.752† | 138824.8 | 0.5011 | mg/L | 0.00292 | 1.002 | mg/L | 0.0058 | 0.58% |
| Fe 273.955† | 2441.0 | 2.152 | mg/L | 0.0060 | 4.304 | mg/L | 0.0121 | 0.28% |
| K 766.490† | 14780.1 | 10.33 | mg/L | 0.031 | 20.67 | mg/L | 0.063 | 0.30% |
| Mg 279.077† | 9585.6 | 10.37 | mg/L | 0.026 | 20.75 | mg/L | 0.051 | 0.25% |
| Mn 257.610† | 14701.3 | 0.5019 | mg/L | 0.00420 | 1.004 | mg/L | 0.0084 | 0.84% |
| Mo 202.031† | 19.7 | 0.00097 | mg/L | 0.000388 | 0.00193 | mg/L | 0.000777 | 40.14% |
| Na 589.592† | 120061.4 | 10.12 | mg/L | 0.039 | 20.23 | mg/L | 0.078 | 0.38% |
| Na 330.237† | 320.6 | 11.02 | mg/L | 0.265 | 22.04 | mg/L | 0.529 | 2.40% |
| Ni 231.604† | 821.0 | 0.5087 | mg/L | 0.00345 | 1.017 | mg/L | 0.0069 | 0.68% |
| Pb 220.353† | 14114.1 | 2.047 | mg/L | 0.0135 | 4.094 | mg/L | 0.0271 | 0.66% |
| Sb 206.836† | 5823.4 | 2.165 | mg/L | 0.0088 | 4.331 | mg/L | 0.0177 | 0.41% |
| Se 196.026† | 2527.9 | 2.123 | mg/L | 0.0086 | 4.245 | mg/L | 0.0173 | 0.41% |
| Si 288.158† | 9.3 | 0.00821 | mg/L | 0.008348 | 0.01641 | mg/L | 0.016695 | 101.73% |
| Sn 189.927† | -13.7 | -0.00187 | mg/L | 0.000890 | -0.00374 | mg/L | 0.001780 | 47.64% |
| Sr 421.552† | 323572.9 | 0.5117 | mg/L | 0.00125 | 1.023 | mg/L | 0.0025 | 0.25% |
| Ti 334.903† | 52.5 | 0.00166 | mg/L | 0.000406 | 0.00331 | mg/L | 0.000811 | 24.49% |
| Tl 190.801† | 3607.4 | 2.096 | mg/L | 0.0147 | 4.192 | mg/L | 0.0293 | 0.70% |
| V 292.402† | 51162.2 | 0.5334 | mg/L | 0.00454 | 1.067 | mg/L | 0.0091 | 0.85% |
| Zn 206.200† | 316.2 | 0.5100 | mg/L | 0.00392 | 1.020 | mg/L | 0.0078 | 0.77% |

Sequence No.: 16
Sample ID: RG11 MB1SPK SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 312
Date Collected: 8/6/2010 10:29:53 AM
Data Type: Original

DEL

Nebulizer Parameters: RG11 MB1SPK SWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG11 MB1SPK SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|------------------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1939033.5 | 102.0 | % | 2.17 | | | 2.12% |
| ScR 361.383 | 295863.1 | 101.1 | % | 1.65 | | | 1.63% |
| Ag 328.068† | 92091.3 | 0.5316 | mg/L | 0.01036 | 1.063 | mg/L | 0.0207 1.95% |
| Al 308.215† | 2649.8 | 2.088 | mg/L | 0.0462 | 4.177 | mg/L | 0.0924 2.21% |
| As 188.979† | 2868.0 | 2.078 | mg/L | 0.0508 | 4.156 | mg/L | 0.1016 2.45% |
| B 249.677† | -0.8 | -0.00153 | mg/L | 0.000750 | -0.00306 | mg/L | 0.001499 48.94% |
| Ba 233.527† | 6409.4 | 2.079 | mg/L | 0.0389 | 4.157 | mg/L | 0.0778 1.87% |
| Be 313.042† | 269592.0 | 0.4903 | mg/L | 0.00485 | 0.9807 | mg/L | 0.00970 0.99% |
| Ca 317.933† | 149100.3 | 10.37 | mg/L | 0.213 | 20.75 | mg/L | 0.425 2.05% |
| Cd 228.802† | 11113.1 | 0.5211 | mg/L | 0.00900 | 1.042 | mg/L | 0.0180 1.73% |
| Co 228.616† | 15046.0 | 0.5087 | mg/L | 0.00894 | 1.017 | mg/L | 0.0179 1.76% |
| Cr 267.716† | 2487.0 | 0.5261 | mg/L | 0.00916 | 1.052 | mg/L | 0.0183 1.74% |
| Cu 324.752† | 137265.7 | 0.4954 | mg/L | 0.01630 | 0.9909 | mg/L | 0.03259 3.29% |
| Fe 273.955† | 2384.7 | 2.102 | mg/L | 0.0404 | 4.204 | mg/L | 0.0809 1.92% |
| K 766.490† | 14825.3 | 10.37 | mg/L | 0.112 | 20.73 | mg/L | 0.225 1.09% |
| Mg 279.077† | 9489.4 | 10.27 | mg/L | 0.192 | 20.54 | mg/L | 0.384 1.87% |
| Mn 257.610† | 14530.2 | 0.4961 | mg/L | 0.00675 | 0.9921 | mg/L | 0.01350 1.36% |
| Mo 202.031† | 18.7 | 0.00091 | mg/L | 0.000281 | 0.00182 | mg/L | 0.000563 30.91% |
| Na 589.592† | 117703.8 | 9.919 | mg/L | 0.1321 | 19.84 | mg/L | 0.264 1.33% |
| Na 330.237† | 314.9 | 10.83 | mg/L | 0.385 | 21.66 | mg/L | 0.770 3.56% |
| Ni 231.604† | 807.3 | 0.4986 | mg/L | 0.00748 | 0.9972 | mg/L | 0.01497 1.50% |
| Pb 220.353† | 13839.0 | 2.007 | mg/L | 0.0311 | 4.014 | mg/L | 0.0621 1.55% |
| Sb 206.836† | 27.9 | 0.00656 | mg/L | 0.003094 | 0.01311 | mg/L | 0.006188 47.19% |
| Se 196.026† | 2498.7 | 2.098 | mg/L | 0.0544 | 4.196 | mg/L | 0.1088 2.59% |
| Si 288.158† | 4.8 | 0.00514 | mg/L | 0.004635 | -0.01027 | mg/L | 0.009270 90.24% |
| Sn 189.927† | -9.7 | -0.00215 | mg/L | 0.000310 | -0.00429 | mg/L | 0.000620 14.44% |
| Sr 421.552† | 317884.3 | 0.5027 | mg/L | 0.00408 | 1.005 | mg/L | 0.0082 0.81% |
| Ti 334.903† | 25.2 | 0.00041 | mg/L | 0.000458 | 0.00081 | mg/L | 0.000917 112.98% |
| Tl 190.801† | 3542.2 | 2.058 | mg/L | 0.0544 | 4.116 | mg/L | 0.1087 2.64% |
| V 292.402† | 49964.2 | 0.5209 | mg/L | 0.00768 | 1.042 | mg/L | 0.0154 1.47% |
| Zn 206.200† | 305.0 | 0.4918 | mg/L | 0.00734 | 0.9836 | mg/L | 0.01469 1.49% |

Sequence No.: 17

Sample ID: RG11 MB1SPD *Silic*

Analyst: ALA

Dilution: 2X

48-b DEL

Autosampler Location: 313

Date Collected: 8/6/2010 10:34:04 AM

Data Type: Original

Nebulizer Parameters: RG11 MB1SPD

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG11 MB1SPD

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1930298.4 | 101.5 % | 3.25 | | | 3.20% |
| ScR 361.383 | 294099.1 | 100.5 % | 0.96 | | | 0.96% |
| Ag 328.068† | 92155.4 | 0.5320 mg/L | 0.01265 | 1.064 mg/L | 0.0253 | 2.38% |
| Al 308.215† | 2661.6 | 2.098 mg/L | 0.0170 | 4.195 mg/L | 0.0340 | 0.81% |
| As 188.979† | 2873.6 | 2.082 mg/L | 0.0638 | 4.164 mg/L | 0.1276 | 3.06% |
| B 249.677† | -6.6 | -0.00328 mg/L | 0.001527 | -0.00655 mg/L | 0.003053 | 46.60% |
| Ba 233.527† | 6414.4 | 2.080 mg/L | 0.0207 | 4.160 mg/L | 0.0414 | 1.00% |
| Be 313.042† | 270602.8 | 0.4922 mg/L | 0.00382 | 0.9843 mg/L | 0.00765 | 0.78% |
| Ca 317.933† | 143945.0 | 10.02 mg/L | 0.082 | 20.03 mg/L | 0.163 | 0.82% |
| Cd 228.802† | 11146.6 | 0.5227 mg/L | 0.01554 | 1.045 mg/L | 0.0311 | 2.97% |
| Co 228.616† | 15039.3 | 0.5085 mg/L | 0.01451 | 1.017 mg/L | 0.0290 | 2.85% |
| Cr 267.716† | 2495.1 | 0.5278 mg/L | 0.00614 | 1.056 mg/L | 0.0123 | 1.16% |
| Cu 324.752† | 137393.9 | 0.4959 mg/L | 0.01822 | 0.9918 mg/L | 0.03645 | 3.68% |
| Fe 273.955† | 2410.9 | 2.125 mg/L | 0.0183 | 4.251 mg/L | 0.0366 | 0.86% |
| K 766.490† | 14924.1 | 10.43 mg/L | 0.032 | 20.87 mg/L | 0.064 | 0.31% |
| Mg 279.077† | 9531.0 | 10.31 mg/L | 0.031 | 20.63 mg/L | 0.063 | 0.30% |
| Mn 257.610† | 14608.5 | 0.4987 mg/L | 0.00297 | 0.9975 mg/L | 0.00595 | 0.60% |
| Mo 202.031† | 18.1 | 0.00088 mg/L | 0.000297 | 0.00175 mg/L | 0.000595 | 33.90% |
| Na 589.592† | 118218.4 | 9.962 mg/L | 0.0596 | 19.92 mg/L | 0.119 | 0.60% |
| Na 330.237† | 308.2 | 10.59 mg/L | 0.057 | 21.19 mg/L | 0.114 | 0.54% |
| Ni 231.604† | 810.2 | 0.5004 mg/L | 0.00630 | 1.001 mg/L | 0.0126 | 1.26% |
| Pb 220.353† | 13863.6 | 2.011 mg/L | 0.0484 | 4.021 mg/L | 0.0967 | 2.41% |
| Sb 206.836† | 17.2 | 0.00258 mg/L | 0.002075 | 0.00515 mg/L | 0.004149 | 80.49% |
| Se 196.026† | 2502.7 | 2.101 mg/L | 0.0643 | 4.203 mg/L | 0.1285 | 3.06% |
| Si 288.158† | 3.5 | 0.00423 mg/L | 0.001894 | 0.00846 mg/L | 0.003788 | 44.78% |
| Sn 189.927† | -8.8 | -0.00193 mg/L | 0.000320 | -0.00386 mg/L | 0.000639 | 16.56% |
| Sr 421.552† | 319716.2 | 0.5056 mg/L | 0.00414 | 1.011 mg/L | 0.0083 | 0.82% |
| Ti 334.903† | 18.3 | 0.00011 mg/L | 0.000410 | 0.00022 mg/L | 0.000821 | 367.90% |
| Tl 190.801† | 3544.0 | 2.059 mg/L | 0.0666 | 4.118 mg/L | 0.1333 | 3.24% |
| V 292.402† | 50199.9 | 0.5233 mg/L | 0.01181 | 1.047 mg/L | 0.0236 | 2.26% |
| Zn 206.200† | 307.4 | 0.4957 mg/L | 0.00869 | 0.9914 mg/L | 0.01738 | 1.75% |

Sequence No.: 18
 Sample ID: CV *2*
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 7
 Date Collected: 8/6/2010 10:38:15 AM
 Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1929390.4 | 101.5 % | 0.96 | | | 0.95% |
| ScR 361.383 | 279806.6 | 95.60 % | 0.680 | | | 0.71% |
| Ag 328.068† | 181722.2 | 1.049 mg/L | 0.0122 | 1.049 mg/L | 0.0122 | 1.16% |
| Al 308.215† | 2836.5 | 2.213 mg/L | 0.0129 | 2.213 mg/L | 0.0129 | 0.58% |
| As 188.979† | 2830.2 | 2.068 mg/L | 0.0173 | 2.068 mg/L | 0.0173 | 0.83% |
| B 249.677† | 3485.0 | 1.051 mg/L | 0.0059 | 1.051 mg/L | 0.0059 | 0.56% |
| Ba 233.527† | 3365.1 | 1.091 mg/L | 0.0059 | 1.091 mg/L | 0.0059 | 0.54% |
| Be 313.042† | 569051.9 | 1.035 mg/L | 0.0085 | 1.035 mg/L | 0.0085 | 0.82% |
| Ca 317.933† | 31741.7 | 2.208 mg/L | 0.0138 | 2.208 mg/L | 0.0138 | 0.62% |
| Cd 228.802† | 22644.5 | 1.069 mg/L | 0.0145 | 1.069 mg/L | 0.0145 | 1.35% |
| Co 228.616† | 30798.1 | 1.040 mg/L | 0.0153 | 1.040 mg/L | 0.0153 | 1.47% |
| Cr 267.716† | 5245.7 | 1.112 mg/L | 0.0083 | 1.112 mg/L | 0.0083 | 0.74% |
| Cu 324.752† | 290964.3 | 1.049 mg/L | 0.0114 | 1.049 mg/L | 0.0114 | 1.09% |
| Fe 273.955† | 2445.3 | 2.153 mg/L | 0.0188 | 2.153 mg/L | 0.0188 | 0.87% |
| K 766.490† | 31074.9 | 21.73 mg/L | 0.004 | 21.73 mg/L | 0.004 | 0.02% |
| Mg 279.077† | 2012.1 | 2.183 mg/L | 0.0198 | 2.183 mg/L | 0.0198 | 0.91% |
| Mn 257.610† | 30875.4 | 1.054 mg/L | 0.0043 | 1.054 mg/L | 0.0043 | 0.41% |
| Mo 202.031† | 17549.3 | 1.021 mg/L | 0.0120 | 1.021 mg/L | 0.0120 | 1.18% |
| Na 589.592† | 624705.6 | 52.64 mg/L | 0.478 | 52.64 mg/L | 0.478 | 0.91% |
| Na 330.237† | 1605.2 | 55.53 mg/L | 0.466 | 55.53 mg/L | 0.466 | 0.84% |
| Ni 231.604† | 1716.5 | 1.062 mg/L | 0.0079 | 1.062 mg/L | 0.0079 | 0.74% |
| Pb 220.353† | 14186.1 | 2.058 mg/L | 0.0214 | 2.058 mg/L | 0.0214 | 1.04% |
| Sb 206.836† | 5669.7 | 2.117 mg/L | 0.0231 | 2.117 mg/L | 0.0231 | 1.09% |
| Se 196.026† | 2466.7 | 2.072 mg/L | 0.0268 | 2.072 mg/L | 0.0268 | 1.29% |
| Si 288.158† | 3333.4 | 2.261 mg/L | 0.0140 | 2.261 mg/L | 0.0140 | 0.62% |
| Sn 189.927† | 3770.6 | 1.027 mg/L | 0.0119 | 1.027 mg/L | 0.0119 | 1.16% |
| Sr 421.552† | 673626.6 | 1.065 mg/L | 0.0104 | 1.065 mg/L | 0.0104 | 0.98% |
| Ti 334.903† | 23447.7 | 1.066 mg/L | 0.0016 | 1.066 mg/L | 0.0016 | 0.15% |
| Tl 190.801† | 3527.1 | 2.051 mg/L | 0.0247 | 2.051 mg/L | 0.0247 | 1.20% |
| V 292.402† | 99594.0 | 1.039 mg/L | 0.0075 | 1.039 mg/L | 0.0075 | 0.72% |
| Zn 206.200† | 655.4 | 1.057 mg/L | 0.0065 | 1.057 mg/L | 0.0065 | 0.61% |

Sequence No.: 19
 Sample ID: CB 2
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 10:42:28 AM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1941046.8 | 102.1 | % | 0.70 | | | 0.68% |
| ScR 361.383 | 279669.7 | 95.55 | % | 0.726 | | | 0.76% |
| Ag 328.068† | -20.1 | -0.00012 | mg/L | 0.000102 | -0.00012 mg/L | 0.000102 | 87.87% |
| Al 308.215† | -6.5 | -0.00517 | mg/L | 0.004567 | -0.00517 mg/L | 0.004567 | 88.34% |
| As 188.979† | -1.2 | -0.00090 | mg/L | 0.000314 | -0.00090 mg/L | 0.000314 | 34.95% |
| B 249.677† | -3.2 | -0.00096 | mg/L | 0.001306 | -0.00096 mg/L | 0.001306 | 135.64% |
| Ba 233.527† | 2.5 | 0.00081 | mg/L | 0.000587 | 0.00081 mg/L | 0.000587 | 72.38% |
| Be 313.042† | 99.1 | 0.00018 | mg/L | 0.000075 | 0.00018 mg/L | 0.000075 | 41.63% |
| Ca 317.933† | 23.4 | 0.00163 | mg/L | 0.001235 | 0.00163 mg/L | 0.001235 | 75.86% |
| Cd 228.802† | 1.9 | 0.00009 | mg/L | 0.000034 | 0.00009 mg/L | 0.000034 | 35.89% |
| Co 228.616† | 1.2 | 0.00004 | mg/L | 0.000116 | 0.00004 mg/L | 0.000116 | 293.25% |
| Cr 267.716† | -3.5 | -0.00074 | mg/L | 0.000812 | -0.00074 mg/L | 0.000812 | 109.39% |
| Cu 324.752† | -10.2 | -0.00004 | mg/L | 0.000322 | -0.00004 mg/L | 0.000322 | 864.49% |
| Fe 273.955† | -3.7 | -0.00328 | mg/L | 0.001436 | -0.00328 mg/L | 0.001436 | 43.76% |
| K 766.490† | 98.9 | 0.06914 | mg/L | 0.018016 | 0.06914 mg/L | 0.018016 | 26.06% |
| Mg 279.077† | 1.8 | 0.00198 | mg/L | 0.016643 | 0.00198 mg/L | 0.016643 | 839.10% |
| Mn 257.610† | -0.3 | -0.00001 | mg/L | 0.000122 | -0.00001 mg/L | 0.000122 | >999.9% |
| Mo 202.031† | 3.7 | 0.00021 | mg/L | 0.000138 | 0.00021 mg/L | 0.000138 | 64.79% |
| Na 589.592† | 43.8 | 0.00369 | mg/L | 0.003599 | 0.00369 mg/L | 0.003599 | 97.54% |
| Na 330.237† | -6.6 | -0.2262 | mg/L | 0.78478 | -0.2262 mg/L | 0.78478 | 346.98% |
| Ni 231.604† | 3.9 | 0.00241 | mg/L | 0.001615 | 0.00241 mg/L | 0.001615 | 66.97% |
| Pb 220.353† | -6.7 | -0.00097 | mg/L | 0.000111 | -0.00097 mg/L | 0.000111 | 11.35% |
| Sb 206.836† | 7.6 | 0.00287 | mg/L | 0.000990 | 0.00287 mg/L | 0.000990 | 34.48% |
| Se 196.026† | 1.7 | 0.00145 | mg/L | 0.001260 | 0.00145 mg/L | 0.001260 | 87.06% |
| Si 288.158† | 6.9 | 0.00465 | mg/L | 0.005720 | 0.00465 mg/L | 0.005720 | 122.94% |
| Sn 189.927† | 5.3 | 0.00144 | mg/L | 0.000421 | 0.00144 mg/L | 0.000421 | 29.19% |
| Sr 421.552† | 60.9 | 0.00010 | mg/L | 0.000018 | 0.00010 mg/L | 0.000018 | 18.67% |
| Ti 334.903† | 0.7 | 0.00003 | mg/L | 0.000254 | 0.00003 mg/L | 0.000254 | 768.34% |
| Tl 190.801† | 5.4 | 0.00315 | mg/L | 0.003419 | 0.00315 mg/L | 0.003419 | 108.43% |
| V 292.402† | -3.0 | -0.00003 | mg/L | 0.000038 | -0.00003 mg/L | 0.000038 | 109.95% |
| Zn 206.200† | -0.8 | -0.00135 | mg/L | 0.003625 | -0.00135 mg/L | 0.003625 | 269.41% |

=====
Analysis Begun

Start Time: 8/6/2010 10:48:39 AM

Plasma On Time: 8/6/2010 7:12:02 AM

Logged In Analyst: metals

Technique: ICP Continuous

Spectrometer Model: Optima 7300 DV, S/N 077C8121202 Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif

Batch ID:

Results Data Set: I2100806

Results Library: C:\pe\metals\Results\Results.mdb
=====

Sequence No.: 1

Sample ID: STD2

Date Collected: 8/6/2010 10:48:40 AM

Data Type: Original

Nebulizer Parameters: STD2

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: STD2

| Analyte | Mean Corrected | | | Calib Conc. Units |
|-------------|----------------|----------|-------|----------------------|
| | Intensity | Std.Dev. | RSD | |
| ScA 357.253 | 1960937.8 | 24545.63 | 1.25% | 103.1 % |
| ScR 361.383 | 279697.4 | 1432.83 | 0.51% | 95.56 % |
| Ba 233.527† | 33335.7 | 55.71 | 0.17% | [10] mg/L |
| Cd 228.802† | 213318.0 | 3295.79 | 1.55% | [10] mg/L |
| Co 228.616† | 301306.6 | 5113.68 | 1.70% | [10] mg/L |
| Cr 267.716† | 51381.4 | 154.99 | 0.30% | [10] mg/L |
| Cu 324.752† | 2788430.0 | 54663.57 | 1.96% | [10] mg/L |
| Mn 257.610† | 315116.4 | 469.25 | 0.15% | [10] mg/L |
| V 292.402† | 983433.1 | 17328.86 | 1.76% | [10] mg/L |

Sequence No.: 2
Sample ID: STD5

Date Collected: 8/6/2010 10:50:31 AM
Data Type: Original

Nebulizer Parameters: STD5

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: STD5

| Analyte | Mean Corrected Intensity | Std.Dev. | RSD | Conc. | Calib Units |
|-------------|--------------------------|----------|-------|-------|-------------|
| ScA 357.253 | 1831252.8 | 28627.53 | 1.56% | 96.30 | % |
| ScR 361.383 | 295220.7 | 2321.17 | 0.79% | 100.9 | % |
| Al 308.215† | 38023.1 | 530.05 | 1.39% | [30] | mg/L |
| Ca 317.933† | 435603.2 | 2148.96 | 0.49% | [30] | mg/L |
| Fe 273.955† | 114343.3 | 551.89 | 0.48% | [100] | mg/L |
| K 766.490† | 145316.8 | 1012.11 | 0.70% | [100] | mg/L |
| Mg 279.077† | 28155.8 | 250.41 | 0.89% | [30] | mg/L |
| Na 330.237† | 2908.8 | 34.15 | 1.17% | [100] | mg/L |

Calibration Summary

| Analyte | Stds. | Equation | Intercept | Slope | Curvature | Corr. Coef. | Reslope |
|------------|-------|------------|-----------|--------|-----------|-------------|---------|
| Ag 328.068 | 1 | Lin Thru 0 | 0.0 | 173200 | 0.00000 | 1.000000 | |
| Al 308.215 | 1 | Lin Thru 0 | 0.0 | 1267 | 0.00000 | 1.000000 | |
| As 188.979 | 1 | Lin Thru 0 | 0.0 | 1380 | 0.00000 | 1.000000 | |
| B 249.677 | 1 | Lin Thru 0 | 0.0 | 3310 | 0.00000 | 1.000000 | |
| Ba 233.527 | 1 | Lin Thru 0 | 0.0 | 3334 | 0.00000 | 1.000000 | |
| Be 313.042 | 1 | Lin Thru 0 | 0.0 | 549500 | 0.00000 | 1.000000 | |
| Ca 317.933 | 1 | Lin Thru 0 | 0.0 | 14520 | 0.00000 | 1.000000 | |
| Cd 228.802 | 1 | Lin Thru 0 | 0.0 | 21330 | 0.00000 | 1.000000 | |
| Co 228.616 | 1 | Lin Thru 0 | 0.0 | 30130 | 0.00000 | 1.000000 | |
| Cr 267.716 | 1 | Lin Thru 0 | 0.0 | 5138 | 0.00000 | 1.000000 | |
| Cu 324.752 | 1 | Lin Thru 0 | 0.0 | 278800 | 0.00000 | 1.000000 | |
| Fe 273.955 | 1 | Lin Thru 0 | 0.0 | 1143 | 0.00000 | 1.000000 | |
| K 766.490 | 1 | Lin Thru 0 | 0.0 | 1453 | 0.00000 | 1.000000 | |
| Mg 279.077 | 1 | Lin Thru 0 | 0.0 | 938.5 | 0.00000 | 1.000000 | |
| Mn 257.610 | 1 | Lin Thru 0 | 0.0 | 31510 | 0.00000 | 1.000000 | |
| Mo 202.031 | 1 | Lin Thru 0 | 0.0 | 17190 | 0.00000 | 1.000000 | |
| Na 589.592 | 1 | Lin Thru 0 | 0.0 | 11870 | 0.00000 | 1.000000 | |
| Na 330.237 | 1 | Lin Thru 0 | 0.0 | 29.09 | 0.00000 | 1.000000 | |
| Ni 231.604 | 1 | Lin Thru 0 | 0.0 | 1619 | 0.00000 | 1.000000 | |
| Pb 220.353 | 1 | Lin Thru 0 | 0.0 | 6897 | 0.00000 | 1.000000 | |
| Sb 206.836 | 1 | Lin Thru 0 | 0.0 | 2685 | 0.00000 | 1.000000 | |
| Se 196.026 | 1 | Lin Thru 0 | 0.0 | 1191 | 0.00000 | 1.000000 | |
| Si 288.158 | 1 | Lin Thru 0 | 0.0 | 1477 | 0.00000 | 1.000000 | |
| Sn 189.927 | 1 | Lin Thru 0 | 0.0 | 3677 | 0.00000 | 1.000000 | |
| Sr 421.552 | 1 | Lin Thru 0 | 0.0 | 632400 | 0.00000 | 1.000000 | |
| Ti 334.903 | 1 | Lin Thru 0 | 0.0 | 21960 | 0.00000 | 1.000000 | |
| Tl 190.801 | 1 | Lin Thru 0 | 0.0 | 1720 | 0.00000 | 1.000000 | |
| V 292.402 | 1 | Lin Thru 0 | 0.0 | 98340 | 0.00000 | 1.000000 | |
| Zn 206.200 | 1 | Lin Thru 0 | 0.0 | 620.0 | 0.00000 | 1.000000 | |

=====
Analysis Begun

Start Time: 8/6/2010 10:53:42 AM

Plasma On Time: 8/6/2010 7:12:02 AM

Logged In Analyst: metals

Technique: ICP Continuous

Spectrometer Model: Optima 7300 DV, S/N 077C8121202Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif

Batch ID:

Results Data Set: I2100806

Results Library: C:\pe\metals\Results\Results.mdb

=====
Sequence No.: 1

Autosampler Location: 7

Sample ID: CV

Date Collected: 8/6/2010 10:53:43 AM

Analyst: ALA

Data Type: Original

Dilution: 1X

Nebulizer Parameters: CV

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 199.0 kPa | 0.75 L/min |

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1916554.3 | 100.8 % | 0.88 | | | 0.88% |
| ScR 361.383 | 290969.8 | 99.41 % | 1.268 | | | 1.28% |
| Ag 328.068† | 182817.8 | 1.055 mg/L | 0.0082 | 1.055 mg/L | 0.0082 | 0.77% |
| Al 308.215† | 2731.4 | 2.123 mg/L | 0.0263 | 2.123 mg/L | 0.0263 | 1.24% |
| As 188.979† | 2868.1 | 2.095 mg/L | 0.0222 | 2.095 mg/L | 0.0222 | 1.06% |
| B 249.677† | 3376.3 | 1.018 mg/L | 0.0113 | 1.018 mg/L | 0.0113 | 1.11% |
| Ba 233.527† | 3267.4 | 0.9794 mg/L | 0.01398 | 0.9794 mg/L | 0.01398 | 1.43% |
| Be 313.042† | 549400.9 | 0.9993 mg/L | 0.00527 | 0.9993 mg/L | 0.00527 | 0.53% |
| Ca 317.933† | 30758.3 | 2.118 mg/L | 0.0292 | 2.118 mg/L | 0.0292 | 1.38% |
| Cd 228.802† | 22610.8 | 1.053 mg/L | 0.0029 | 1.053 mg/L | 0.0029 | 0.28% |
| Co 228.616† | 30913.3 | 1.024 mg/L | 0.0027 | 1.024 mg/L | 0.0027 | 0.27% |
| Cr 267.716† | 5091.4 | 0.9903 mg/L | 0.01265 | 0.9903 mg/L | 0.01265 | 1.28% |
| Cu 324.752† | 291831.7 | 1.046 mg/L | 0.0066 | 1.046 mg/L | 0.0066 | 0.63% |
| Fe 273.955† | 2379.9 | 2.076 mg/L | 0.0333 | 2.076 mg/L | 0.0333 | 1.60% |
| K 766.490† | 29986.5 | 20.64 mg/L | 0.127 | 20.64 mg/L | 0.127 | 0.62% |
| Mg 279.077† | 1960.4 | 2.094 mg/L | 0.0229 | 2.094 mg/L | 0.0229 | 1.09% |
| Mn 257.610† | 29709.8 | 0.9433 mg/L | 0.01003 | 0.9433 mg/L | 0.01003 | 1.06% |
| Mo 202.031† | 17734.0 | 1.032 mg/L | 0.0090 | 1.032 mg/L | 0.0090 | 0.87% |
| Na 589.592† | 598481.1 | 50.43 mg/L | 0.413 | 50.43 mg/L | 0.413 | 0.82% |
| Na 330.237† | 1546.9 | 53.23 mg/L | 0.924 | 53.23 mg/L | 0.924 | 1.74% |
| Ni 231.604† | 1671.4 | 1.034 mg/L | 0.0128 | 1.034 mg/L | 0.0128 | 1.24% |
| Pb 220.353† | 14388.7 | 2.087 mg/L | 0.0174 | 2.087 mg/L | 0.0174 | 0.83% |
| Sb 206.836† | 5722.0 | 2.138 mg/L | 0.0173 | 2.138 mg/L | 0.0173 | 0.81% |
| Se 196.026† | 2501.1 | 2.101 mg/L | 0.0163 | 2.101 mg/L | 0.0163 | 0.77% |
| Si 288.158† | 3227.5 | 2.189 mg/L | 0.0257 | 2.189 mg/L | 0.0257 | 1.18% |
| Sn 189.927† | 3826.2 | 1.043 mg/L | 0.0107 | 1.043 mg/L | 0.0107 | 1.03% |
| Sr 421.552† | 648206.0 | 1.025 mg/L | 0.0037 | 1.025 mg/L | 0.0037 | 0.36% |
| Ti 334.903† | 22498.2 | 1.023 mg/L | 0.0094 | 1.023 mg/L | 0.0094 | 0.92% |
| Tl 190.801† | 3568.3 | 2.075 mg/L | 0.0211 | 2.075 mg/L | 0.0211 | 1.02% |
| V 292.402† | 100301.1 | 1.024 mg/L | 0.0045 | 1.024 mg/L | 0.0045 | 0.44% |
| Zn 206.200† | 641.1 | 1.033 mg/L | 0.0154 | 1.033 mg/L | 0.0154 | 1.49% |

Sequence No.: 2
Sample ID: CB 3
Analyst: ALA
Dilution: 1X

Autosampler Location: 1
Date Collected: 8/6/2010 10:57:56 AM
Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1935027.4 | 101.8 | % | 0.51 | | | 0.50% |
| ScR 361.383 | 297442.3 | 101.6 | % | 0.64 | | | 0.63% |
| Ag 328.068† | -15.7 | -0.00009 | mg/L | 0.000091 | -0.00009 mg/L | 0.000091 | 100.68% |
| Al 308.215† | 2.9 | 0.00231 | mg/L | 0.006753 | 0.00231 mg/L | 0.006753 | 292.60% |
| As 188.979† | 2.6 | 0.00187 | mg/L | 0.001131 | 0.00187 mg/L | 0.001131 | 60.54% |
| B 249.677† | -1.8 | -0.00053 | mg/L | 0.002307 | -0.00053 mg/L | 0.002307 | 435.59% |
| Ba 233.527† | 1.3 | 0.00039 | mg/L | 0.000608 | 0.00039 mg/L | 0.000608 | 155.29% |
| Be 313.042† | -2.2 | 0.00000 | mg/L | 0.000032 | 0.00000 mg/L | 0.000032 | 805.50% |
| Ca 317.933† | 6.5 | 0.00045 | mg/L | 0.001185 | 0.00045 mg/L | 0.001185 | 266.00% |
| Cd 228.802† | -1.2 | -0.00006 | mg/L | 0.000202 | -0.00006 mg/L | 0.000202 | 328.60% |
| Co 228.616† | -0.9 | -0.00003 | mg/L | 0.000197 | -0.00003 mg/L | 0.000197 | 635.75% |
| Cr 267.716† | 4.0 | 0.00077 | mg/L | 0.000710 | 0.00077 mg/L | 0.000710 | 92.01% |
| Cu 324.752† | -22.0 | -0.00008 | mg/L | 0.000153 | -0.00008 mg/L | 0.000153 | 193.20% |
| Fe 273.955† | -0.5 | -0.00041 | mg/L | 0.000253 | -0.00041 mg/L | 0.000253 | 61.75% |
| K 766.490† | 7.2 | 0.00498 | mg/L | 0.013775 | 0.00498 mg/L | 0.013775 | 276.52% |
| Mg 279.077† | 6.8 | 0.00725 | mg/L | 0.005082 | 0.00725 mg/L | 0.005082 | 70.07% |
| Mn 257.610† | -1.2 | -0.00004 | mg/L | 0.000120 | -0.00004 mg/L | 0.000120 | 314.89% |
| Mo 202.031† | 0.1 | 0.00000 | mg/L | 0.000463 | 0.00000 mg/L | 0.000463 | >999.9% |
| Na 589.592† | 97.0 | 0.00818 | mg/L | 0.004493 | 0.00818 mg/L | 0.004493 | 54.96% |
| Na 330.237† | 3.2 | 0.1106 | mg/L | 0.34940 | 0.1106 mg/L | 0.34940 | 316.02% |
| Ni 231.604† | 5.0 | 0.00311 | mg/L | 0.001262 | 0.00311 mg/L | 0.001262 | 40.61% |
| Pb 220.353† | -7.9 | -0.00115 | mg/L | 0.000492 | -0.00115 mg/L | 0.000492 | 42.82% |
| Sb 206.836† | 7.2 | 0.00269 | mg/L | 0.001302 | 0.00269 mg/L | 0.001302 | 48.41% |
| Se 196.026† | 7.5 | 0.00626 | mg/L | 0.001597 | 0.00626 mg/L | 0.001597 | 25.51% |
| Si 288.158† | 6.8 | 0.00463 | mg/L | 0.000576 | 0.00463 mg/L | 0.000576 | 12.46% |
| Sn 189.927† | 5.1 | 0.00139 | mg/L | 0.000683 | 0.00139 mg/L | 0.000683 | 49.12% |
| Sr 421.552† | -1.0 | 0.00000 | mg/L | 0.000073 | 0.00000 mg/L | 0.000073 | >999.9% |
| Ti 334.903† | 6.8 | 0.00031 | mg/L | 0.000299 | 0.00031 mg/L | 0.000299 | 96.57% |
| Tl 190.801† | 0.6 | 0.00038 | mg/L | 0.001184 | 0.00038 mg/L | 0.001184 | 314.55% |
| V 292.402† | -9.0 | -0.00009 | mg/L | 0.000432 | -0.00009 mg/L | 0.000432 | 486.61% |
| Zn 206.200† | -0.7 | -0.00112 | mg/L | 0.002471 | -0.00112 mg/L | 0.002471 | 220.63% |

Sequence No.: 3
Sample ID: RG30 MB1 TWC
Analyst: ALA
Dilution: 1X

Autosampler Location: 314
Date Collected: 8/6/2010 11:02:07 AM
Data Type: Original

Nebulizer Parameters: RG30 MB1 TWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG30 MB1 TWC

Table with 8 columns: Analyte, Mean Corrected Intensity, Conc., Calib. Units, Std.Dev., Sample Conc., Units, Std.Dev., RSD. Lists various elements like ScA, ScR, Ag, Al, As, B, Ba, Be, Ca, Cd, Co, Cr, Cu, Fe, K, Mg, Mn, Mo, Na, Ni, Pb, Sb, Se, Si, Sn, Sr, Ti, Tl, V, Zn with their respective values.

Sequence No.: 4
 Sample ID: RG30 F TWC
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 315
 Date Collected: 8/6/2010 11:06:04 AM
 Data Type: Original

Nebulizer Parameters: RG30 F TWC

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RG30 F TWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1910460.4 | 100.5 | % | 1.08 | | | 1.07% |
| ScR 361.383 | 293466.0 | 100.3 | % | 0.43 | | | 0.43% |
| Ag 328.068† | -40.9 | -0.00024 | mg/L | 0.000106 | -0.00024 mg/L | 0.000106 | 43.99% |
| Al 308.215† | 100.8 | 0.07939 | mg/L | 0.006996 | 0.07939 mg/L | 0.006996 | 8.81% |
| As 188.979† | 18.4 | 0.01090 | mg/L | 0.002826 | 0.01090 mg/L | 0.002826 | 25.93% |
| B 249.677† | 127.7 | 0.03859 | mg/L | 0.000358 | 0.03859 mg/L | 0.000358 | 0.93% |
| Ba 233.527† | 462.2 | 0.1379 | mg/L | 0.00074 | 0.1379 mg/L | 0.00074 | 0.54% |
| Be 313.042† | 36.9 | 0.00007 | mg/L | 0.000015 | 0.00007 mg/L | 0.000015 | 22.77% |
| Ca 317.933† | 1227050.5 | 84.51 | mg/L | 0.607 | 84.51 mg/L | 0.607 | 0.72% |
| Cd 228.802† | 5.6 | 0.00022 | mg/L | 0.000131 | 0.00022 mg/L | 0.000131 | 58.60% |
| Co 228.616† | 16.9 | 0.00052 | mg/L | 0.000186 | 0.00052 mg/L | 0.000186 | 35.77% |
| Cr 267.716† | 44.2 | 0.00473 | mg/L | 0.001149 | 0.00473 mg/L | 0.001149 | 24.27% |
| Cu 324.752† | 716.3 | 0.00218 | mg/L | 0.000417 | 0.00218 mg/L | 0.000417 | 19.14% |
| Fe 273.955† | 77.7 | 0.06796 | mg/L | 0.001112 | 0.06796 mg/L | 0.001112 | 1.64% |
| K 766.490† | 8995.3 | 6.190 | mg/L | 0.0572 | 6.190 mg/L | 0.0572 | 0.92% |
| Mg 279.077† | 16068.5 | 17.11 | mg/L | 0.170 | 17.11 mg/L | 0.170 | 0.99% |
| Mn 257.610† | 921.3 | 0.02904 | mg/L | 0.000156 | 0.02904 mg/L | 0.000156 | 0.54% |
| Mo 202.031† | 102.6 | 0.00450 | mg/L | 0.000142 | 0.00450 mg/L | 0.000142 | 3.16% |
| Na 589.592† | 108123.2 | 9.111 | mg/L | 0.0395 | 9.111 mg/L | 0.0395 | 0.43% |
| Na 330.237† | 281.1 | 10.05 | mg/L | 0.190 | 10.05 mg/L | 0.190 | 1.89% |
| Ni 231.604† | 12.9 | 0.00798 | mg/L | 0.001737 | 0.00798 mg/L | 0.001737 | 21.76% |
| Pb 220.353† | -45.2 | -0.00653 | mg/L | 0.000465 | -0.00653 mg/L | 0.000465 | 7.12% |
| Sb 206.836† | 10.7 | 0.00378 | mg/L | 0.001783 | 0.00378 mg/L | 0.001783 | 47.14% |
| Se 196.026† | 65.7 | 0.04945 | mg/L | 0.004765 | 0.04945 mg/L | 0.004765 | 9.64% |
| Si 288.158† | 25726.7 | 17.42 | mg/L | 0.223 | 17.42 mg/L | 0.223 | 1.28% |
| Sn 189.927† | -43.2 | -0.00783 | mg/L | 0.000616 | -0.00783 mg/L | 0.000616 | 7.88% |
| Sr 421.552† | 243016.1 | 0.3843 | mg/L | 0.00171 | 0.3843 mg/L | 0.00171 | 0.44% |
| Ti 334.903† | 178.5 | 0.00285 | mg/L | 0.000434 | 0.00285 mg/L | 0.000434 | 15.22% |
| Tl 190.801† | 25.0 | 0.01458 | mg/L | 0.000596 | 0.01458 mg/L | 0.000596 | 4.09% |
| V 292.402† | 333.0 | 0.00342 | mg/L | 0.000164 | 0.00342 mg/L | 0.000164 | 4.80% |
| Zn 206.200† | 325.9 | 0.5256 | mg/L | 0.00328 | 0.5256 mg/L | 0.00328 | 0.62% |

Sequence No.: 5
Sample ID: RG30 G TWC
Analyst: ALA
Dilution: 1X

Autosampler Location: 316
Date Collected: 8/6/2010 11:10:15 AM
Data Type: Original

Nebulizer Parameters: RG30 G TWC
Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG30 G TWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|------------------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1898995.8 | 99.86 | % | 0.214 | | | 0.21% |
| ScR 361.383 | 288586.1 | 98.60 | % | 0.636 | | | 0.64% |
| Ag 328.068† | -37.3 | -0.00022 | mg/L | 0.000146 | -0.00022 | mg/L | 0.000146 67.94% |
| Al 308.215† | 18.4 | 0.01438 | mg/L | 0.004439 | 0.01438 | mg/L | 0.004439 30.88% |
| As 188.979† | 24.8 | 0.01463 | mg/L | 0.003511 | 0.01463 | mg/L | 0.003511 24.00% |
| B 249.677† | 200.6 | 0.06059 | mg/L | 0.001843 | 0.06059 | mg/L | 0.001843 3.04% |
| Ba 233.527† | 378.6 | 0.1125 | mg/L | 0.00202 | 0.1125 | mg/L | 0.00202 1.80% |
| Be 313.042† | 52.4 | 0.00009 | mg/L | 0.000030 | 0.00009 | mg/L | 0.000030 32.73% |
| Ca 317.933† | 1679774.9 | 115.7 | mg/L | 0.92 | 115.7 | mg/L | 0.92 0.80% |
| Cd 228.802† | 9.8 | 0.00041 | mg/L | 0.000186 | 0.00041 | mg/L | 0.000186 45.89% |
| Co 228.616† | 19.7 | 0.00062 | mg/L | 0.000334 | 0.00062 | mg/L | 0.000334 54.00% |
| Cr 267.716† | 22.1 | -0.00032 | mg/L | 0.001216 | -0.00032 | mg/L | 0.001216 384.35% |
| Cu 324.752† | 797.3 | 0.00244 | mg/L | 0.000165 | 0.00244 | mg/L | 0.000165 6.75% |
| Fe 273.955† | 4.2 | 0.00366 | mg/L | 0.001603 | 0.00366 | mg/L | 0.001603 43.77% |
| K 766.490† | 8912.9 | 6.133 | mg/L | 0.0765 | 6.133 | mg/L | 0.0765 1.25% |
| Mg 279.077† | 16990.9 | 18.09 | mg/L | 0.168 | 18.09 | mg/L | 0.168 0.93% |
| Mn 257.610† | 113.3 | 0.00332 | mg/L | 0.000158 | 0.00332 | mg/L | 0.000158 4.75% |
| Mo 202.031† | 108.8 | 0.00433 | mg/L | 0.000490 | 0.00433 | mg/L | 0.000490 11.33% |
| Na 589.592† | 185305.1 | 15.62 | mg/L | 0.118 | 15.62 | mg/L | 0.118 0.76% |
| Na 330.237† | 478.4 | 17.00 | mg/L | 0.266 | 17.00 | mg/L | 0.266 1.56% |
| Ni 231.604† | 12.4 | 0.00767 | mg/L | 0.003635 | 0.00767 | mg/L | 0.003635 47.40% |
| Pb 220.353† | -51.1 | -0.00740 | mg/L | 0.000965 | -0.00740 | mg/L | 0.000965 13.05% |
| Sb 206.836† | 12.8 | 0.00457 | mg/L | 0.001391 | 0.00457 | mg/L | 0.001391 30.41% |
| Se 196.026† | 62.7 | 0.04479 | mg/L | 0.004020 | 0.04479 | mg/L | 0.004020 8.97% |
| Si 288.158† | 26841.9 | 18.18 | mg/L | 0.072 | 18.18 | mg/L | 0.072 0.40% |
| Sn 189.927† | -54.4 | -0.00944 | mg/L | 0.000368 | -0.00944 | mg/L | 0.000368 3.90% |
| Sr 421.552† | 348343.9 | 0.5509 | mg/L | 0.00278 | 0.5509 | mg/L | 0.00278 0.51% |
| Ti 334.903† | 173.0 | 0.00066 | mg/L | 0.000165 | 0.00066 | mg/L | 0.000165 25.12% |
| Tl 190.801† | 21.8 | 0.01272 | mg/L | 0.001407 | 0.01272 | mg/L | 0.001407 11.06% |
| V 292.402† | 419.2 | 0.00428 | mg/L | 0.000083 | 0.00428 | mg/L | 0.000083 1.94% |
| Zn 206.200† | 374.5 | 0.6040 | mg/L | 0.00860 | 0.6040 | mg/L | 0.00860 1.42% |

Sequence No.: 6
 Sample ID: RG30 H TWC
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 317
 Date Collected: 8/6/2010 11:14:27 AM
 Data Type: Original

Nebulizer Parameters: RG30 H TWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG30 H TWC

| Analyte | Mean Corrected | | Calib. Conc. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|-----------------------|----------|-------------|------|----------|--------|
| | Intensity | | | | Conc. Units | | | |
| ScA 357.253 | 1878036.6 | | 98.76 % | 0.469 | | | | 0.47% |
| ScR 361.383 | 287978.5 | | 98.39 % | 0.589 | | | | 0.60% |
| Ag 328.068† | -54.8 | -0.00034 | mg/L | 0.000126 | -0.00034 | mg/L | 0.000126 | 37.09% |
| Al 308.215† | 113.3 | 0.08920 | mg/L | 0.002615 | 0.08920 | mg/L | 0.002615 | 2.93% |
| As 188.979† | 22.4 | 0.01235 | mg/L | 0.003378 | 0.01235 | mg/L | 0.003378 | 27.36% |
| B 249.677† | 407.2 | 0.1230 | mg/L | 0.00100 | 0.1230 | mg/L | 0.00100 | 0.81% |
| Ba 233.527† | 1345.9 | 0.4026 | mg/L | 0.00333 | 0.4026 | mg/L | 0.00333 | 0.83% |
| Be 313.042† | 37.9 | 0.00007 | mg/L | 0.000056 | 0.00007 | mg/L | 0.000056 | 83.35% |
| Ca 317.933† | 1939469.2 | 133.6 | mg/L | 0.23 | 133.6 | mg/L | 0.23 | 0.17% |
| Cd 228.802† | 6.0 | 0.00024 | mg/L | 0.000150 | 0.00024 | mg/L | 0.000150 | 63.87% |
| Co 228.616† | 43.0 | 0.00133 | mg/L | 0.000050 | 0.00133 | mg/L | 0.000050 | 3.77% |
| Cr 267.716† | 79.9 | 0.00888 | mg/L | 0.001490 | 0.00888 | mg/L | 0.001490 | 16.78% |
| Cu 324.752† | 1278.8 | 0.00388 | mg/L | 0.000118 | 0.00388 | mg/L | 0.000118 | 3.06% |
| Fe 273.955† | 175.7 | 0.1537 | mg/L | 0.00407 | 0.1537 | mg/L | 0.00407 | 2.65% |
| K 766.490† | 14790.0 | 10.18 | mg/L | 0.031 | 10.18 | mg/L | 0.031 | 0.30% |
| Mg 279.077† | 29297.0 | 31.20 | mg/L | 0.201 | 31.20 | mg/L | 0.201 | 0.65% |
| Mn 257.610† | 3852.8 | 0.1220 | mg/L | 0.00099 | 0.1220 | mg/L | 0.00099 | 0.81% |
| Mo 202.031† | 128.0 | 0.00513 | mg/L | 0.000123 | 0.00513 | mg/L | 0.000123 | 2.39% |
| Na 589.592† | 459765.3 | 38.74 | mg/L | 0.069 | 38.74 | mg/L | 0.069 | 0.18% |
| Na 330.237† | 1142.5 | 40.05 | mg/L | 0.544 | 40.05 | mg/L | 0.544 | 1.36% |
| Ni 231.604† | 17.1 | 0.01054 | mg/L | 0.001493 | 0.01054 | mg/L | 0.001493 | 14.17% |
| Pb 220.353† | -57.2 | -0.00826 | mg/L | 0.001168 | -0.00826 | mg/L | 0.001168 | 14.14% |
| Sb 206.836† | 18.0 | 0.00637 | mg/L | 0.001215 | 0.00637 | mg/L | 0.001215 | 19.09% |
| Se 196.026† | 60.9 | 0.04204 | mg/L | 0.005278 | 0.04204 | mg/L | 0.005278 | 12.55% |
| Si 288.158† | 32057.4 | 21.71 | mg/L | 0.114 | 21.71 | mg/L | 0.114 | 0.52% |
| Sn 189.927† | -60.0 | -0.01013 | mg/L | 0.001216 | -0.01013 | mg/L | 0.001216 | 12.00% |
| Sr 421.552† | 334787.9 | 0.5294 | mg/L | 0.00165 | 0.5294 | mg/L | 0.00165 | 0.31% |
| Ti 334.903† | 236.5 | 0.00243 | mg/L | 0.000145 | 0.00243 | mg/L | 0.000145 | 5.98% |
| Tl 190.801† | 27.6 | 0.01619 | mg/L | 0.003086 | 0.01619 | mg/L | 0.003086 | 19.06% |
| V 292.402† | 335.3 | 0.00348 | mg/L | 0.000403 | 0.00348 | mg/L | 0.000403 | 11.59% |
| Zn 206.200† | 71.3 | 0.1150 | mg/L | 0.00463 | 0.1150 | mg/L | 0.00463 | 4.03% |

Sequence No.: 7
 Sample ID: RG30 ADUP TWC
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 318
 Date Collected: 8/6/2010 11:18:39 AM
 Data Type: Original

Nebulizer Parameters: RG30 ADUP TWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG30 ADUP TWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|-----------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1886535.5 | 99.20 | % | 1.376 | | | | 1.39% |
| ScR 361.383 | 287745.4 | 98.31 | % | 0.448 | | | | 0.46% |
| Ag 328.068† | -56.1 | -0.00035 | mg/L | 0.000210 | -0.00035 | mg/L | 0.000210 | 60.46% |
| Al 308.215† | 103.1 | 0.08119 | mg/L | 0.006807 | 0.08119 | mg/L | 0.006807 | 8.38% |
| As 188.979† | 24.5 | 0.01373 | mg/L | 0.000947 | 0.01373 | mg/L | 0.000947 | 6.90% |
| B 249.677† | 423.1 | 0.1278 | mg/L | 0.00355 | 0.1278 | mg/L | 0.00355 | 2.78% |
| Ba 233.527† | 1388.8 | 0.4154 | mg/L | 0.00349 | 0.4154 | mg/L | 0.00349 | 0.84% |
| Be 313.042† | 23.4 | 0.00004 | mg/L | 0.000023 | 0.00004 | mg/L | 0.000023 | 56.19% |
| Ca 317.933† | 1994567.0 | 137.4 | mg/L | 0.98 | 137.4 | mg/L | 0.98 | 0.71% |
| Cd 228.802† | 5.6 | 0.00021 | mg/L | 0.000233 | 0.00021 | mg/L | 0.000233 | 111.81% |
| Co 228.616† | 36.1 | 0.00110 | mg/L | 0.000042 | 0.00110 | mg/L | 0.000042 | 3.84% |
| Cr 267.716† | 83.2 | 0.00929 | mg/L | 0.001061 | 0.00929 | mg/L | 0.001061 | 11.41% |
| Cu 324.752† | 1066.4 | 0.00309 | mg/L | 0.000448 | 0.00309 | mg/L | 0.000448 | 14.51% |
| Fe 273.955† | 153.1 | 0.1339 | mg/L | 0.00170 | 0.1339 | mg/L | 0.00170 | 1.27% |
| K 766.490† | 15350.6 | 10.56 | mg/L | 0.133 | 10.56 | mg/L | 0.133 | 1.25% |
| Mg 279.077† | 30441.1 | 32.42 | mg/L | 0.286 | 32.42 | mg/L | 0.286 | 0.88% |
| Mn 257.610† | 3761.5 | 0.1190 | mg/L | 0.00053 | 0.1190 | mg/L | 0.00053 | 0.45% |
| Mo 202.031† | 119.2 | 0.00456 | mg/L | 0.000282 | 0.00456 | mg/L | 0.000282 | 6.19% |
| Na 589.592† | 475049.4 | 40.03 | mg/L | 0.226 | 40.03 | mg/L | 0.226 | 0.57% |
| Na 330.237† | 1201.3 | 42.10 | mg/L | 0.733 | 42.10 | mg/L | 0.733 | 1.74% |
| Ni 231.604† | 17.2 | 0.01060 | mg/L | 0.001240 | 0.01060 | mg/L | 0.001240 | 11.69% |
| Pb 220.353† | -56.2 | -0.00812 | mg/L | 0.001064 | -0.00812 | mg/L | 0.001064 | 13.12% |
| Sb 206.836† | 18.1 | 0.00641 | mg/L | 0.002750 | 0.00641 | mg/L | 0.002750 | 42.89% |
| Se 196.026† | 64.8 | 0.04509 | mg/L | 0.003819 | 0.04509 | mg/L | 0.003819 | 8.47% |
| Si 288.158† | 33621.6 | 22.77 | mg/L | 0.205 | 22.77 | mg/L | 0.205 | 0.90% |
| Sn 189.927† | -56.3 | -0.00894 | mg/L | 0.000707 | -0.00894 | mg/L | 0.000707 | 7.91% |
| Sr 421.552† | 343866.8 | 0.5438 | mg/L | 0.00415 | 0.5438 | mg/L | 0.00415 | 0.76% |
| Ti 334.903† | 213.9 | 0.00117 | mg/L | 0.000310 | 0.00117 | mg/L | 0.000310 | 26.59% |
| Tl 190.801† | 28.3 | 0.01661 | mg/L | 0.000590 | 0.01661 | mg/L | 0.000590 | 3.55% |
| V 292.402† | 361.5 | 0.00375 | mg/L | 0.000076 | 0.00375 | mg/L | 0.000076 | 2.03% |
| Zn 206.200† | 72.0 | 0.1162 | mg/L | 0.00534 | 0.1162 | mg/L | 0.00534 | 4.60% |

Sequence No.: 8
 Sample ID: RG30 A TWC
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 319
 Date Collected: 8/6/2010 11:22:51 AM
 Data Type: Original

Nebulizer Parameters: RG30 A TWC

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RG30 A TWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1890477.9 | 99.41 | % | 0.550 | | | 0.55% |
| ScR 361.383 | 288515.3 | 98.58 | % | 0.131 | | | 0.13% |
| Ag 328.068† | -1.7 | -0.00003 | mg/L | 0.000176 | -0.00003 mg/L | 0.000176 | 576.24% |
| Al 308.215† | 102.4 | 0.08065 | mg/L | 0.001335 | 0.08065 mg/L | 0.001335 | 1.66% |
| As 188.979† | 24.8 | 0.01398 | mg/L | 0.001159 | 0.01398 mg/L | 0.001159 | 8.29% |
| B 249.677† | 418.9 | 0.1266 | mg/L | 0.00095 | 0.1266 mg/L | 0.00095 | 0.75% |
| Ba 233.527† | 1382.4 | 0.4135 | mg/L | 0.00069 | 0.4135 mg/L | 0.00069 | 0.17% |
| Be 313.042† | 13.5 | 0.00002 | mg/L | 0.000015 | 0.00002 mg/L | 0.000015 | 66.10% |
| Ca 317.933† | 1999500.8 | 137.7 | mg/L | 0.35 | 137.7 mg/L | 0.35 | 0.25% |
| Cd 228.802† | 2.9 | 0.00008 | mg/L | 0.000234 | 0.00008 mg/L | 0.000234 | 285.21% |
| Co 228.616† | 38.8 | 0.00119 | mg/L | 0.000179 | 0.00119 mg/L | 0.000179 | 15.03% |
| Cr 267.716† | 82.6 | 0.00921 | mg/L | 0.000457 | 0.00921 mg/L | 0.000457 | 4.96% |
| Cu 324.752† | 1219.0 | 0.00364 | mg/L | 0.000325 | 0.00364 mg/L | 0.000325 | 8.93% |
| Fe 273.955† | 148.2 | 0.1296 | mg/L | 0.00173 | 0.1296 mg/L | 0.00173 | 1.33% |
| K 766.490† | 15219.8 | 10.47 | mg/L | 0.034 | 10.47 mg/L | 0.034 | 0.33% |
| Mg 279.077† | 30178.5 | 32.14 | mg/L | 0.033 | 32.14 mg/L | 0.033 | 0.10% |
| Mn 257.610† | 3386.1 | 0.1071 | mg/L | 0.00045 | 0.1071 mg/L | 0.00045 | 0.42% |
| Mo 202.031† | 126.9 | 0.00500 | mg/L | 0.000415 | 0.00500 mg/L | 0.000415 | 8.30% |
| Na 589.592† | 476333.2 | 40.14 | mg/L | 0.064 | 40.14 mg/L | 0.064 | 0.16% |
| Na 330.237† | 1172.3 | 41.10 | mg/L | 0.129 | 41.10 mg/L | 0.129 | 0.31% |
| Ni 231.604† | 19.4 | 0.01197 | mg/L | 0.001870 | 0.01197 mg/L | 0.001870 | 15.62% |
| Pb 220.353† | -55.6 | -0.00804 | mg/L | 0.001026 | -0.00804 mg/L | 0.001026 | 12.77% |
| Sb 206.836† | 16.8 | 0.00594 | mg/L | 0.000881 | 0.00594 mg/L | 0.000881 | 14.83% |
| Se 196.026† | 61.0 | 0.04188 | mg/L | 0.005476 | 0.04188 mg/L | 0.005476 | 13.08% |
| Si 288.158† | 31944.2 | 21.63 | mg/L | 0.039 | 21.63 mg/L | 0.039 | 0.18% |
| Sn 189.927† | -57.1 | -0.00915 | mg/L | 0.000717 | -0.00915 mg/L | 0.000717 | 7.84% |
| Sr 421.552† | 345649.0 | 0.5466 | mg/L | 0.00230 | 0.5466 mg/L | 0.00230 | 0.42% |
| Ti 334.903† | 232.5 | 0.00199 | mg/L | 0.000133 | 0.00199 mg/L | 0.000133 | 6.69% |
| Tl 190.801† | 27.8 | 0.01628 | mg/L | 0.002405 | 0.01628 mg/L | 0.002405 | 14.78% |
| V 292.402† | 384.6 | 0.00398 | mg/L | 0.000238 | 0.00398 mg/L | 0.000238 | 5.99% |
| Zn 206.200† | 71.8 | 0.1158 | mg/L | 0.00536 | 0.1158 mg/L | 0.00536 | 4.63% |

Sequence No.: 9
Sample ID: RG30 ASPK TWC
Analyst: ALA
Dilution: 1X

Autosampler Location: 320
Date Collected: 8/6/2010 11:27:03 AM
Data Type: Original

Nebulizer Parameters: RG30 ASPK TWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG30 ASPK TWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|----------|--------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1882937.6 | 99.01 | % | 0.302 | | | | 0.30% |
| ScR 361.383 | 285206.5 | 97.45 | % | 0.340 | | | | 0.35% |
| Ag 328.068† | 94212.9 | 0.5439 | mg/L | 0.00434 | 0.5439 | mg/L | 0.00434 | 0.80% |
| Al 308.215† | 2920.7 | 2.295 | mg/L | 0.0055 | 2.295 | mg/L | 0.0055 | 0.24% |
| As 188.979† | 3034.1 | 2.194 | mg/L | 0.0058 | 2.194 | mg/L | 0.0058 | 0.26% |
| B 249.677† | 423.7 | 0.1267 | mg/L | 0.00133 | 0.1267 | mg/L | 0.00133 | 1.05% |
| Ba 233.527† | 8095.8 | 2.427 | mg/L | 0.0113 | 2.427 | mg/L | 0.0113 | 0.47% |
| Be 313.042† | 282722.2 | 0.5142 | mg/L | 0.00268 | 0.5142 | mg/L | 0.00268 | 0.52% |
| Ca 317.933† | 2179740.1 | 150.1 | mg/L | 0.63 | 150.1 | mg/L | 0.63 | 0.42% |
| Cd 228.802† | 11441.9 | 0.5292 | mg/L | 0.00174 | 0.5292 | mg/L | 0.00174 | 0.33% |
| Co 228.616† | 14999.1 | 0.4972 | mg/L | 0.00182 | 0.4972 | mg/L | 0.00182 | 0.37% |
| Cr 267.716† | 2677.0 | 0.5124 | mg/L | 0.00253 | 0.5124 | mg/L | 0.00253 | 0.49% |
| Cu 324.752† | 149644.5 | 0.5360 | mg/L | 0.00490 | 0.5360 | mg/L | 0.00490 | 0.91% |
| Fe 273.955† | 2659.7 | 2.323 | mg/L | 0.0089 | 2.323 | mg/L | 0.0089 | 0.38% |
| K 766.490† | 31158.1 | 21.44 | mg/L | 0.171 | 21.44 | mg/L | 0.171 | 0.80% |
| Mg 279.077† | 40906.8 | 43.57 | mg/L | 0.217 | 43.57 | mg/L | 0.217 | 0.50% |
| Mn 257.610† | 19017.1 | 0.6036 | mg/L | 0.00360 | 0.6036 | mg/L | 0.00360 | 0.60% |
| Mo 202.031† | 130.8 | 0.00501 | mg/L | 0.000463 | 0.00501 | mg/L | 0.000463 | 9.24% |
| Na 589.592† | 606915.5 | 51.14 | mg/L | 0.256 | 51.14 | mg/L | 0.256 | 0.50% |
| Na 330.237† | 1529.3 | 53.33 | mg/L | 0.150 | 53.33 | mg/L | 0.150 | 0.28% |
| Ni 231.604† | 842.3 | 0.5203 | mg/L | 0.00404 | 0.5203 | mg/L | 0.00404 | 0.78% |
| Pb 220.353† | 14026.9 | 2.034 | mg/L | 0.0140 | 2.034 | mg/L | 0.0140 | 0.69% |
| Sb 206.836† | 27.0 | 0.00618 | mg/L | 0.002049 | 0.00618 | mg/L | 0.002049 | 33.13% |
| Se 196.026† | 2636.7 | 2.205 | mg/L | 0.0120 | 2.205 | mg/L | 0.0120 | 0.54% |
| Si 288.158† | 31719.8 | 21.48 | mg/L | 0.101 | 21.48 | mg/L | 0.101 | 0.47% |
| Sn 189.927† | -62.7 | -0.01010 | mg/L | 0.000790 | -0.01010 | mg/L | 0.000790 | 7.82% |
| Sr 421.552† | 683046.2 | 1.080 | mg/L | 0.0094 | 1.080 | mg/L | 0.0094 | 0.87% |
| Ti 334.903† | 250.8 | 0.00196 | mg/L | 0.000365 | 0.00196 | mg/L | 0.000365 | 18.63% |
| Tl 190.801† | 3617.7 | 2.102 | mg/L | 0.0110 | 2.102 | mg/L | 0.0110 | 0.52% |
| V 292.402† | 51531.0 | 0.5260 | mg/L | 0.00481 | 0.5260 | mg/L | 0.00481 | 0.91% |
| Zn 206.200† | 392.2 | 0.6325 | mg/L | 0.00951 | 0.6325 | mg/L | 0.00951 | 1.50% |

Sequence No.: 10
 Sample ID: RG30 MB1SPK TWC
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 321
 Date Collected: 8/6/2010 11:31:15 AM
 Data Type: Original

Nebulizer Parameters: RG30 MB1SPK TWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG30 MB1SPK TWC

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1920114.0 | 101.0 % | 0.59 | | | 0.59% |
| ScR 361.383 | 296714.4 | 101.4 % | 0.59 | | | 0.59% |
| Ag 328.068† | 90837.1 | 0.5244 mg/L | 0.00282 | 0.5244 mg/L | 0.00282 | 0.54% |
| Al 308.215† | 2646.6 | 2.079 mg/L | 0.0039 | 2.079 mg/L | 0.0039 | 0.19% |
| As 188.979† | 2869.6 | 2.079 mg/L | 0.0200 | 2.079 mg/L | 0.0200 | 0.96% |
| B 249.677† | -5.0 | -0.00278 mg/L | 0.001174 | -0.00278 mg/L | 0.001174 | 42.15% |
| Ba 233.527† | 6454.5 | 1.936 mg/L | 0.0132 | 1.936 mg/L | 0.0132 | 0.68% |
| Be 313.042† | 272778.9 | 0.4961 mg/L | 0.00029 | 0.4961 mg/L | 0.00029 | 0.06% |
| Ca 317.933† | 145477.2 | 10.02 mg/L | 0.016 | 10.02 mg/L | 0.016 | 0.16% |
| Cd 228.802† | 11153.2 | 0.5161 mg/L | 0.00476 | 0.5161 mg/L | 0.00476 | 0.92% |
| Co 228.616† | 15150.6 | 0.5024 mg/L | 0.00435 | 0.5024 mg/L | 0.00435 | 0.87% |
| Cr 267.716† | 2511.6 | 0.4873 mg/L | 0.00212 | 0.4873 mg/L | 0.00212 | 0.43% |
| Cu 324.752† | 141736.5 | 0.5084 mg/L | 0.00274 | 0.5084 mg/L | 0.00274 | 0.54% |
| Fe 273.955† | 2400.2 | 2.096 mg/L | 0.0100 | 2.096 mg/L | 0.0100 | 0.48% |
| K 766.490† | 14781.2 | 10.17 mg/L | 0.041 | 10.17 mg/L | 0.041 | 0.40% |
| Mg 279.077† | 9471.9 | 10.09 mg/L | 0.023 | 10.09 mg/L | 0.023 | 0.23% |
| Mn 257.610† | 14602.3 | 0.4639 mg/L | 0.00237 | 0.4639 mg/L | 0.00237 | 0.51% |
| Mo 202.031† | 22.4 | 0.00113 mg/L | 0.000212 | 0.00113 mg/L | 0.000212 | 18.83% |
| Na 589.592† | 117733.8 | 9.921 mg/L | 0.0256 | 9.921 mg/L | 0.0256 | 0.26% |
| Na 330.237† | 315.0 | 10.77 mg/L | 0.109 | 10.77 mg/L | 0.109 | 1.01% |
| Ni 231.604† | 812.8 | 0.5020 mg/L | 0.00443 | 0.5020 mg/L | 0.00443 | 0.88% |
| Pb 220.353† | 14288.0 | 2.072 mg/L | 0.0191 | 2.072 mg/L | 0.0191 | 0.92% |
| Sb 206.836† | 12.9 | 0.00138 mg/L | 0.001607 | 0.00138 mg/L | 0.001607 | 116.33% |
| Se 196.026† | 2468.0 | 2.072 mg/L | 0.0183 | 2.072 mg/L | 0.0183 | 0.88% |
| Si 288.158† | 80.2 | 0.05615 mg/L | 0.019761 | 0.05615 mg/L | 0.019761 | 35.19% |
| Sn 189.927† | -7.0 | -0.00145 mg/L | 0.000475 | -0.00145 mg/L | 0.000475 | 32.84% |
| Sr 421.552† | 320350.8 | 0.5066 mg/L | 0.00126 | 0.5066 mg/L | 0.00126 | 0.25% |
| Ti 334.903† | 14.1 | -0.00007 mg/L | 0.000413 | -0.00007 mg/L | 0.000413 | 557.48% |
| Tl 190.801† | 3565.0 | 2.071 mg/L | 0.0123 | 2.071 mg/L | 0.0123 | 0.59% |
| V 292.402† | 49997.1 | 0.5103 mg/L | 0.00183 | 0.5103 mg/L | 0.00183 | 0.36% |
| Zn 206.200† | 310.5 | 0.5007 mg/L | 0.00127 | 0.5007 mg/L | 0.00127 | 0.25% |

Sequence No.: 11
 Sample ID: CV
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 7
 Date Collected: 8/6/2010 11:35:26 AM
 Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected | | Calib. Conc. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|--|-----------------------|----------|-------------|---------|----------|-------|
| | Intensity | | | | Conc. Units | | | |
| ScA 357.253 | 1927229.0 | | 101.3 % | 0.87 | | | | 0.86% |
| ScR 361.383 | 292127.1 | | 99.81 % | 1.239 | | | | 1.24% |
| Ag 328.068† | 181866.3 | | 1.050 mg/L | 0.0073 | 1.050 mg/L | 0.0073 | | 0.69% |
| Al 308.215† | 2735.0 | | 2.126 mg/L | 0.0248 | 2.126 mg/L | 0.0248 | | 1.17% |
| As 188.979† | 2877.8 | | 2.102 mg/L | 0.0209 | 2.102 mg/L | 0.0209 | | 0.99% |
| B 249.677† | 3368.8 | | 1.016 mg/L | 0.0139 | 1.016 mg/L | 0.0139 | | 1.37% |
| Ba 233.527† | 3274.0 | | 0.9814 mg/L | 0.01376 | 0.9814 mg/L | 0.01376 | | 1.40% |
| Be 313.042† | 548462.7 | | 0.9976 mg/L | 0.00966 | 0.9976 mg/L | 0.00966 | | 0.97% |
| Ca 317.933† | 31037.5 | | 2.138 mg/L | 0.0291 | 2.138 mg/L | 0.0291 | | 1.36% |
| Cd 228.802† | 22398.8 | | 1.043 mg/L | 0.0110 | 1.043 mg/L | 0.0110 | | 1.05% |
| Co 228.616† | 30606.6 | | 1.014 mg/L | 0.0109 | 1.014 mg/L | 0.0109 | | 1.08% |
| Cr 267.716† | 5094.0 | | 0.9908 mg/L | 0.01587 | 0.9908 mg/L | 0.01587 | | 1.60% |
| Cu 324.752† | 291088.8 | | 1.043 mg/L | 0.0066 | 1.043 mg/L | 0.0066 | | 0.64% |
| Fe 273.955† | 2384.5 | | 2.080 mg/L | 0.0255 | 2.080 mg/L | 0.0255 | | 1.23% |
| K 766.490† | 30157.9 | | 20.75 mg/L | 0.056 | 20.75 mg/L | 0.056 | | 0.27% |
| Mg 279.077† | 1970.5 | | 2.105 mg/L | 0.0364 | 2.105 mg/L | 0.0364 | | 1.73% |
| Mn 257.610† | 30032.1 | | 0.9535 mg/L | 0.01080 | 0.9535 mg/L | 0.01080 | | 1.13% |
| Mo 202.031† | 17729.9 | | 1.031 mg/L | 0.0105 | 1.031 mg/L | 0.0105 | | 1.02% |
| Na 589.592† | 596775.7 | | 50.29 mg/L | 0.497 | 50.29 mg/L | 0.497 | | 0.99% |
| Na 330.237† | 1554.3 | | 53.49 mg/L | 1.067 | 53.49 mg/L | 1.067 | | 1.99% |
| Ni 231.604† | 1670.1 | | 1.033 mg/L | 0.0119 | 1.033 mg/L | 0.0119 | | 1.16% |
| Pb 220.353† | 14380.9 | | 2.086 mg/L | 0.0236 | 2.086 mg/L | 0.0236 | | 1.13% |
| Sb 206.836† | 5741.6 | | 2.145 mg/L | 0.0258 | 2.145 mg/L | 0.0258 | | 1.20% |
| Se 196.026† | 2514.0 | | 2.111 mg/L | 0.0213 | 2.111 mg/L | 0.0213 | | 1.01% |
| Si 288.158† | 3266.1 | | 2.215 mg/L | 0.0241 | 2.215 mg/L | 0.0241 | | 1.09% |
| Sn 189.927† | 3836.3 | | 1.045 mg/L | 0.0098 | 1.045 mg/L | 0.0098 | | 0.94% |
| Sr 421.552† | 649413.3 | | 1.027 mg/L | 0.0022 | 1.027 mg/L | 0.0022 | | 0.21% |
| Ti 334.903† | 22709.9 | | 1.033 mg/L | 0.0141 | 1.033 mg/L | 0.0141 | | 1.37% |
| Tl 190.801† | 3568.3 | | 2.075 mg/L | 0.0239 | 2.075 mg/L | 0.0239 | | 1.15% |
| V 292.402† | 100016.6 | | 1.021 mg/L | 0.0059 | 1.021 mg/L | 0.0059 | | 0.58% |
| Zn 206.200† | 640.0 | | 1.032 mg/L | 0.0155 | 1.032 mg/L | 0.0155 | | 1.50% |

Sequence No.: 12
 Sample ID: CB
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 11:39:39 AM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected | | Calib. Conc. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|----------|-----------------------|----------|-------------|----------|------------------|
| | Intensity | | | | Conc. Units | Std.Dev. | |
| ScA 357.253 | 1935242.1 | | 101.8 % | 0.73 | | | 0.72% |
| ScR 361.383 | 277577.8 | | 94.84 % | 0.280 | | | 0.30% |
| Ag 328.068† | -5.5 | -0.00003 | mg/L | 0.000083 | -0.00003 | mg/L | 0.000083 262.61% |
| Al 308.215† | -6.5 | -0.00514 | mg/L | 0.001615 | -0.00514 | mg/L | 0.001615 31.42% |
| As 188.979† | 0.8 | 0.00057 | mg/L | 0.001529 | 0.00057 | mg/L | 0.001529 266.94% |
| B 249.677† | -1.3 | -0.00039 | mg/L | 0.001785 | -0.00039 | mg/L | 0.001785 461.46% |
| Ba 233.527† | 4.8 | 0.00145 | mg/L | 0.000990 | 0.00145 | mg/L | 0.000990 68.16% |
| Be 313.042† | 91.9 | 0.00017 | mg/L | 0.000057 | 0.00017 | mg/L | 0.000057 33.86% |
| Ca 317.933† | 11.0 | 0.00076 | mg/L | 0.000463 | 0.00076 | mg/L | 0.000463 61.09% |
| Cd 228.802† | 2.2 | 0.00010 | mg/L | 0.000142 | 0.00010 | mg/L | 0.000142 139.01% |
| Co 228.616† | 4.9 | 0.00016 | mg/L | 0.000115 | 0.00016 | mg/L | 0.000115 70.94% |
| Cr 267.716† | -1.4 | -0.00026 | mg/L | 0.001017 | -0.00026 | mg/L | 0.001017 386.71% |
| Cu 324.752† | 149.5 | 0.00054 | mg/L | 0.000297 | 0.00054 | mg/L | 0.000297 55.41% |
| Fe 273.955† | 0.7 | 0.00064 | mg/L | 0.003288 | 0.00064 | mg/L | 0.003288 515.24% |
| K 766.490† | 89.5 | 0.06156 | mg/L | 0.027133 | 0.06156 | mg/L | 0.027133 44.08% |
| Mg 279.077† | -3.3 | -0.00352 | mg/L | 0.001964 | -0.00352 | mg/L | 0.001964 55.76% |
| Mn 257.610† | -1.7 | -0.00005 | mg/L | 0.000052 | -0.00005 | mg/L | 0.000052 95.88% |
| Mo 202.031† | 0.7 | 0.00004 | mg/L | 0.000236 | 0.00004 | mg/L | 0.000236 617.34% |
| Na 589.592† | 93.2 | 0.00785 | mg/L | 0.003526 | 0.00785 | mg/L | 0.003526 44.92% |
| Na 330.237† | -1.3 | -0.04371 | mg/L | 0.189833 | -0.04371 | mg/L | 0.189833 434.26% |
| Ni 231.604† | 4.6 | 0.00283 | mg/L | 0.000364 | 0.00283 | mg/L | 0.000364 12.89% |
| Pb 220.353† | -2.9 | -0.00042 | mg/L | 0.000559 | -0.00042 | mg/L | 0.000559 134.02% |
| Sb 206.836† | 4.9 | 0.00184 | mg/L | 0.001181 | 0.00184 | mg/L | 0.001181 64.29% |
| Se 196.026† | 0.6 | 0.00054 | mg/L | 0.002971 | 0.00054 | mg/L | 0.002971 545.37% |
| Si 288.158† | 32.2 | 0.02180 | mg/L | 0.004344 | 0.02180 | mg/L | 0.004344 19.93% |
| Sn 189.927† | 2.8 | 0.00076 | mg/L | 0.000636 | 0.00076 | mg/L | 0.000636 83.97% |
| Sr 421.552† | 43.5 | 0.00007 | mg/L | 0.000112 | 0.00007 | mg/L | 0.000112 162.42% |
| Ti 334.903† | -0.1 | -0.00001 | mg/L | 0.000492 | -0.00001 | mg/L | 0.000492 >999.9% |
| Tl 190.801† | 2.6 | 0.00151 | mg/L | 0.000633 | 0.00151 | mg/L | 0.000633 41.95% |
| V 292.402† | 2.3 | 0.00002 | mg/L | 0.000155 | 0.00002 | mg/L | 0.000155 701.58% |
| Zn 206.200† | 0.1 | 0.00016 | mg/L | 0.003070 | 0.00016 | mg/L | 0.003070 >999.9% |

Sequence No.: 13
 Sample ID: RF71 MB1 SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 304
 Date Collected: 8/6/2010 11:43:35 AM
 Data Type: Original

Nebulizer Parameters: RF71 MB1 SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RF71 MB1 SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1930856.3 | 101.5 % | | 1.51 | | | 1.48% |
| ScR 361.383 | 294341.3 | 100.6 % | | 2.39 | | | 2.38% |
| Ag 328.068† | 18.5 | 0.00011 mg/L | | 0.000332 | 0.00021 mg/L | 0.000664 | 310.59% |
| Al 308.215† | 6.6 | 0.00522 mg/L | | 0.004598 | 0.01044 mg/L | 0.009196 | 88.13% |
| As 188.979† | 1.6 | 0.00115 mg/L | | 0.003047 | 0.00230 mg/L | 0.006094 | 265.05% |
| B 249.677† | -6.5 | -0.00195 mg/L | | 0.000605 | -0.00390 mg/L | 0.001210 | 31.05% |
| Ba 233.527† | 3.5 | 0.00103 mg/L | | 0.000191 | 0.00207 mg/L | 0.000382 | 18.45% |
| Be 313.042† | 18.9 | 0.00003 mg/L | | 0.000064 | 0.00007 mg/L | 0.000127 | 185.21% |
| Ca 317.933† | 198.0 | 0.01364 mg/L | | 0.002249 | 0.02727 mg/L | 0.004497 | 16.49% |
| Cd 228.802† | 0.5 | 0.00002 mg/L | | 0.000247 | 0.00004 mg/L | 0.000494 | >999.9% |
| Co 228.616† | -1.3 | -0.00005 mg/L | | 0.000165 | -0.00009 mg/L | 0.000330 | 362.13% |
| Cr 267.716† | 2.6 | 0.00050 mg/L | | 0.000724 | 0.00100 mg/L | 0.001448 | 144.59% |
| Cu 324.752† | 212.7 | 0.00076 mg/L | | 0.000240 | 0.00152 mg/L | 0.000480 | 31.50% |
| Fe 273.955† | -0.3 | -0.00024 mg/L | | 0.002398 | -0.00047 mg/L | 0.004795 | >999.9% |
| K 766.490† | 28.9 | 0.01987 mg/L | | 0.011694 | 0.03975 mg/L | 0.023388 | 58.84% |
| Mg 279.077† | 8.9 | 0.00946 mg/L | | 0.000841 | 0.01892 mg/L | 0.001681 | 8.88% |
| Mn 257.610† | -2.5 | -0.00008 mg/L | | 0.000060 | -0.00016 mg/L | 0.000119 | 75.22% |
| Mo 202.031† | -0.0 | 0.00000 mg/L | | 0.000315 | -0.00001 mg/L | 0.000631 | >999.9% |
| Na 589.592† | 75.3 | 0.00635 mg/L | | 0.004026 | 0.01270 mg/L | 0.008051 | 63.41% |
| Na 330.237† | -1.4 | -0.04929 mg/L | | 0.246166 | -0.09859 mg/L | 0.492333 | 499.40% |
| Ni 231.604† | 6.8 | 0.00418 mg/L | | 0.001147 | 0.00837 mg/L | 0.002294 | 27.42% |
| Pb 220.353† | 0.1 | 0.00001 mg/L | | 0.000547 | 0.00003 mg/L | 0.001094 | >999.9% |
| Sb 206.836† | 0.6 | 0.00025 mg/L | | 0.002819 | 0.00050 mg/L | 0.005639 | >999.9% |
| Se 196.026† | 7.1 | 0.00598 mg/L | | 0.002433 | 0.01196 mg/L | 0.004867 | 40.70% |
| Si 288.158† | 25.8 | 0.01748 mg/L | | 0.002732 | 0.03496 mg/L | 0.005464 | 15.63% |
| Sn 189.927† | 4.1 | 0.00112 mg/L | | 0.000406 | 0.00224 mg/L | 0.000813 | 36.35% |
| Sr 421.552† | -0.9 | 0.00000 mg/L | | 0.000018 | 0.00000 mg/L | 0.000036 | >999.9% |
| Ti 334.903† | 24.4 | 0.00111 mg/L | | 0.000844 | 0.00222 mg/L | 0.001689 | 75.94% |
| Tl 190.801† | 2.6 | 0.00150 mg/L | | 0.002423 | 0.00301 mg/L | 0.004846 | 161.23% |
| V 292.402† | 11.8 | 0.00012 mg/L | | 0.000214 | 0.00024 mg/L | 0.000427 | 176.71% |
| Zn 206.200† | -0.4 | -0.00064 mg/L | | 0.001942 | -0.00128 mg/L | 0.003884 | 302.92% |

Sequence No.: 14
Sample ID: RG11 MB1 SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 305
Date Collected: 8/6/2010 11:47:47 AM
Data Type: Original

Nebulizer Parameters: RG11 MB1 SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG11 MB1 SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1945686.8 | 102.3 | % | 0.49 | | | 0.48% |
| ScR 361.383 | 276052.4 | 94.32 | % | 0.327 | | | 0.35% |
| Ag 328.068† | 22.8 | 0.00013 | mg/L | 0.000321 | 0.00026 mg/L | 0.000641 | 243.63% |
| Al 308.215† | -3.2 | -0.00255 | mg/L | 0.000838 | -0.00510 mg/L | 0.001677 | 32.88% |
| As 188.979† | -2.5 | -0.00178 | mg/L | 0.001661 | -0.00356 mg/L | 0.003322 | 93.38% |
| B 249.677† | -12.9 | -0.00389 | mg/L | 0.000160 | -0.00777 mg/L | 0.000320 | 4.12% |
| Ba 233.527† | 1.5 | 0.00045 | mg/L | 0.000863 | 0.00089 mg/L | 0.001726 | 193.08% |
| Be 313.042† | 58.5 | 0.00011 | mg/L | 0.000028 | 0.00021 mg/L | 0.000056 | 26.41% |
| Ca 317.933† | 156.4 | 0.01077 | mg/L | 0.000134 | 0.02154 mg/L | 0.000268 | 1.25% |
| Cd 228.802† | -2.5 | -0.00011 | mg/L | 0.000169 | -0.00022 mg/L | 0.000338 | 154.15% |
| Co 228.616† | -3.3 | -0.00011 | mg/L | 0.000181 | -0.00022 mg/L | 0.000361 | 163.99% |
| Cr 267.716† | 2.2 | 0.00043 | mg/L | 0.001366 | 0.00086 mg/L | 0.002733 | 318.08% |
| Cu 324.752† | 129.8 | 0.00047 | mg/L | 0.000261 | 0.00093 mg/L | 0.000522 | 56.06% |
| Fe 273.955† | 0.7 | 0.00061 | mg/L | 0.003538 | 0.00122 mg/L | 0.007076 | 581.31% |
| K 766.490† | 80.5 | 0.05540 | mg/L | 0.031287 | 0.1108 mg/L | 0.06257 | 56.47% |
| Mg 279.077† | 0.9 | 0.00093 | mg/L | 0.003559 | 0.00186 mg/L | 0.007117 | 381.84% |
| Mn 257.610† | -1.0 | -0.00003 | mg/L | 0.000084 | -0.00006 mg/L | 0.000168 | 276.31% |
| Mo 202.031† | -1.3 | -0.00008 | mg/L | 0.000269 | -0.00015 mg/L | 0.000538 | 349.24% |
| Na 589.592† | 44.9 | 0.00378 | mg/L | 0.003732 | 0.00757 mg/L | 0.007464 | 98.61% |
| Na 330.237† | -12.8 | -0.4403 | mg/L | 0.38070 | -0.8806 mg/L | 0.76140 | 86.46% |
| Ni 231.604† | 4.1 | 0.00255 | mg/L | 0.003254 | 0.00511 mg/L | 0.006509 | 127.38% |
| Pb 220.353† | -0.8 | -0.00011 | mg/L | 0.000971 | -0.00023 mg/L | 0.001942 | 852.11% |
| Sb 206.836† | -3.8 | -0.00139 | mg/L | 0.000717 | -0.00279 mg/L | 0.001435 | 51.45% |
| Se 196.026† | 3.7 | 0.00311 | mg/L | 0.005111 | 0.00623 mg/L | 0.010222 | 164.18% |
| Si 288.158† | 20.8 | 0.01410 | mg/L | 0.007360 | 0.02821 mg/L | 0.014720 | 52.19% |
| Sn 189.927† | 2.8 | 0.00075 | mg/L | 0.000352 | 0.00150 mg/L | 0.000705 | 46.88% |
| Sr 421.552† | 27.2 | 0.00004 | mg/L | 0.000071 | 0.00009 mg/L | 0.000141 | 163.92% |
| Ti 334.903† | 1.4 | 0.00006 | mg/L | 0.000450 | 0.00012 mg/L | 0.000899 | 738.87% |
| Tl 190.801† | 4.5 | 0.00262 | mg/L | 0.002572 | 0.00524 mg/L | 0.005143 | 98.21% |
| V 292.402† | -15.1 | -0.00015 | mg/L | 0.000503 | -0.00030 mg/L | 0.001007 | 330.98% |
| Zn 206.200† | 1.9 | 0.00303 | mg/L | 0.001717 | 0.00607 mg/L | 0.003434 | 56.59% |

Sequence No.: 15
 Sample ID: RG11 A SWC
 Analyst: ALA
 Dilution: 5X

Autosampler Location: 306
 Date Collected: 8/6/2010 11:51:43 AM
 Data Type: Original

Nebulizer Parameters: RG11 A SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG11 A SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1965228.8 | 103.3 | % | 0.99 | | | 0.96% |
| ScR 361.383 | 301199.1 | 102.9 | % | 1.58 | | | 1.54% |
| Ag 328.068† | 126.8 | 0.00058 | mg/L | 0.000118 | 0.00289 mg/L | 0.000592 | 20.49% |
| Al 308.215† | 50513.5 | 39.84 | mg/L | 0.720 | 199.2 mg/L | 3.60 | 1.81% |
| As 188.979† | -45.5 | 0.01962 | mg/L | 0.004217 | 0.09808 mg/L | 0.021083 | 21.50% |
| B 249.677† | 138.4 | 0.04184 | mg/L | 0.001239 | 0.2092 mg/L | 0.00620 | 2.96% |
| Ba 233.527† | 988.1 | 0.2856 | mg/L | 0.00468 | 1.428 mg/L | 0.0234 | 1.64% |
| Be 313.042† | 298.5 | 0.00041 | mg/L | 0.000040 | 0.00207 mg/L | 0.000198 | 9.58% |
| Ca 317.933† | 456985.0 | 31.47 | mg/L | 0.501 | 157.4 mg/L | 2.51 | 1.59% |
| Cd 228.802† | 9.5 | 0.00270 | mg/L | 0.000067 | 0.01349 mg/L | 0.000337 | 2.50% |
| Co 228.616† | 2183.9 | 0.06521 | mg/L | 0.001153 | 0.3260 mg/L | 0.00576 | 1.77% |
| Cr 267.716† | 14717.5 | 2.866 | mg/L | 0.0613 | 14.33 mg/L | 0.307 | 2.14% |
| Cu 324.752† | 1241346.7 | 4.458 | mg/L | 0.0608 | 22.29 mg/L | 0.304 | 1.36% |
| Fe 273.955† | 125770.9 | 110.0 | mg/L | 1.94 | 550.0 mg/L | 9.69 | 1.76% |
| K 766.490† | 3195.1 | 2.199 | mg/L | 0.0296 | 10.99 mg/L | 0.148 | 1.34% |
| Mg 279.077† | 20155.2 | 21.42 | mg/L | 0.425 | 107.1 mg/L | 2.13 | 1.99% |
| Mn 257.610† | 43397.6 | 1.377 | mg/L | 0.0272 | 6.887 mg/L | 0.1360 | 1.97% |
| Mo 202.031† | 4446.6 | 0.2581 | mg/L | 0.00329 | 1.291 mg/L | 0.0165 | 1.27% |
| Na 589.592† | 15814.7 | 1.333 | mg/L | 0.0251 | 6.663 mg/L | 0.1257 | 1.89% |
| Na 330.237† | 12.0 | 1.241 | mg/L | 0.1208 | 6.205 mg/L | 0.6042 | 9.74% |
| Ni 231.604† | 5354.1 | 3.307 | mg/L | 0.0546 | 16.53 mg/L | 0.273 | 1.65% |
| Pb 220.353† | 930.7 | 0.1341 | mg/L | 0.00142 | 0.6703 mg/L | 0.00712 | 1.06% |
| Sb 206.836† | 96.4 | 0.01148 | mg/L | 0.000426 | 0.05739 mg/L | 0.002128 | 3.71% |
| Se 196.026† | 29.7 | 0.02278 | mg/L | 0.003318 | 0.1139 mg/L | 0.01659 | 14.56% |
| Si 288.158† | 1411.9 | 0.9560 | mg/L | 0.01663 | 4.780 mg/L | 0.0831 | 1.74% |
| Sn 189.927† | 62.9 | 0.02002 | mg/L | 0.000878 | 0.1001 mg/L | 0.00439 | 4.38% |
| Sr 421.552† | 74377.5 | 0.1176 | mg/L | 0.00225 | 0.5881 mg/L | 0.01123 | 1.91% |
| Ti 334.903† | 69041.2 | 3.141 | mg/L | 0.0558 | 15.71 mg/L | 0.279 | 1.78% |
| Tl 190.801† | -18.7 | 0.00645 | mg/L | 0.000723 | 0.03227 mg/L | 0.003617 | 11.21% |
| V 292.402† | 17957.4 | 0.1813 | mg/L | 0.00132 | 0.9065 mg/L | 0.00658 | 0.73% |
| Zn 206.200† | 590.1 | 0.9498 | mg/L | 0.01146 | 4.749 mg/L | 0.0573 | 1.21% |

Sequence No.: 16
 Sample ID: RF71 ADUP SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 307
 Date Collected: 8/6/2010 11:55:40 AM
 Data Type: Original

Nebulizer Parameters: RF71 ADUP SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RF71 ADUP SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1965799.5 | 103.4 | % | 0.39 | | | | 0.38% |
| ScR 361.383 | 301290.6 | 102.9 | % | 0.71 | | | | 0.69% |
| Ag 328.068† | 44.9 | 0.00015 | mg/L | 0.000355 | 0.00029 | mg/L | 0.000711 | 241.50% |
| Al 308.215† | 146723.6 | 115.7 | mg/L | 0.90 | 231.5 | mg/L | 1.79 | 0.78% |
| As 188.979† | -54.9 | 0.05757 | mg/L | 0.002747 | 0.1151 | mg/L | 0.00549 | 4.77% |
| B 249.677† | 230.9 | 0.06957 | mg/L | 0.000947 | 0.1391 | mg/L | 0.00189 | 1.36% |
| Ba 233.527† | 1003.7 | 0.2848 | mg/L | 0.00229 | 0.5695 | mg/L | 0.00458 | 0.80% |
| Be 313.042† | 1042.6 | 0.00166 | mg/L | 0.000055 | 0.00331 | mg/L | 0.000110 | 3.32% |
| Ca 317.933† | 439281.8 | 30.25 | mg/L | 0.245 | 60.51 | mg/L | 0.490 | 0.81% |
| Cd 228.802† | 87.7 | 0.00442 | mg/L | 0.000047 | 0.00884 | mg/L | 0.000095 | 1.08% |
| Co 228.616† | 2382.3 | 0.06763 | mg/L | 0.000671 | 0.1353 | mg/L | 0.00134 | 0.99% |
| Cr 267.716† | 1369.7 | 0.2663 | mg/L | 0.00234 | 0.5326 | mg/L | 0.00468 | 0.88% |
| Cu 324.752† | 90685.3 | 0.3343 | mg/L | 0.00383 | 0.6685 | mg/L | 0.00767 | 1.15% |
| Fe 273.955† | 197419.3 | 172.7 | mg/L | 0.89 | 345.3 | mg/L | 1.78 | 0.52% |
| K 766.490† | 14412.9 | 9.918 | mg/L | 0.0260 | 19.84 | mg/L | 0.052 | 0.26% |
| Mg 279.077† | 55433.9 | 58.97 | mg/L | 0.254 | 117.9 | mg/L | 0.51 | 0.43% |
| Mn 257.610† | 61123.6 | 1.940 | mg/L | 0.0155 | 3.880 | mg/L | 0.0310 | 0.80% |
| Mo 202.031† | 189.5 | 0.01050 | mg/L | 0.000228 | 0.02100 | mg/L | 0.000456 | 2.17% |
| Na 589.592† | 198536.5 | 16.73 | mg/L | 0.132 | 33.46 | mg/L | 0.264 | 0.79% |
| Na 330.237† | 465.2 | 17.53 | mg/L | 0.310 | 35.06 | mg/L | 0.620 | 1.77% |
| Ni 231.604† | 454.6 | 0.2808 | mg/L | 0.00313 | 0.5615 | mg/L | 0.00627 | 1.12% |
| Pb 220.353† | 946.5 | 0.1449 | mg/L | 0.00084 | 0.2897 | mg/L | 0.00168 | 0.58% |
| Sb 206.836† | 25.5 | 0.01491 | mg/L | 0.000969 | 0.02981 | mg/L | 0.001937 | 6.50% |
| Se 196.026† | 32.5 | 0.02527 | mg/L | 0.005243 | 0.05053 | mg/L | 0.010486 | 20.75% |
| Si 288.158† | 11300.5 | 7.652 | mg/L | 0.0644 | 15.30 | mg/L | 0.129 | 0.84% |
| Sn 189.927† | 9.5 | 0.00648 | mg/L | 0.001192 | 0.01297 | mg/L | 0.002384 | 18.38% |
| Sr 421.552† | 161675.1 | 0.2557 | mg/L | 0.00079 | 0.5113 | mg/L | 0.00159 | 0.31% |
| Ti 334.903† | 119521.9 | 5.441 | mg/L | 0.0333 | 10.88 | mg/L | 0.067 | 0.61% |
| Tl 190.801† | -33.9 | 0.00733 | mg/L | 0.002841 | 0.01465 | mg/L | 0.005683 | 38.78% |
| V 292.402† | 34359.5 | 0.3291 | mg/L | 0.00173 | 0.6583 | mg/L | 0.00346 | 0.53% |
| Zn 206.200† | 378.5 | 0.6071 | mg/L | 0.00536 | 1.214 | mg/L | 0.0107 | 0.88% |

Sequence No.: 17
 Sample ID: RF71 A SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 308
 Date Collected: 8/6/2010 11:59:36 AM
 Data Type: Original

Nebulizer Parameters: RF71 A SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RF71 A SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Conc. Units | Sample Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------|-----------------|--------|
| ScA 357.253 | 1951269.6 | 102.6 | % | 1.56 | | | 1.52% |
| ScR 361.383 | 304525.1 | 104.0 | % | 0.51 | | | 0.49% |
| Ag 328.068† | 99.9 | 0.00049 | mg/L | 0.000351 | 0.00098 mg/L | 0.000702 | 71.72% |
| Al 308.215† | 155423.3 | 122.6 | mg/L | 1.02 | 245.2 mg/L | 2.05 | 0.84% |
| As 188.979† | -67.4 | 0.05807 | mg/L | 0.006236 | 0.1161 mg/L | 0.01247 | 10.74% |
| B 249.677† | 265.4 | 0.07997 | mg/L | 0.001479 | 0.1599 mg/L | 0.00296 | 1.85% |
| Ba 233.527† | 1062.5 | 0.3017 | mg/L | 0.00211 | 0.6034 mg/L | 0.00422 | 0.70% |
| Be 313.042† | 1376.0 | 0.00223 | mg/L | 0.000035 | 0.00447 mg/L | 0.000069 | 1.55% |
| Ca 317.933† | 471352.8 | 32.46 | mg/L | 0.297 | 64.92 mg/L | 0.594 | 0.92% |
| Cd 228.802† | 109.1 | 0.00546 | mg/L | 0.000334 | 0.01092 mg/L | 0.000669 | 6.13% |
| Co 228.616† | 2591.8 | 0.07359 | mg/L | 0.001465 | 0.1472 mg/L | 0.00293 | 1.99% |
| Cr 267.716† | 1470.0 | 0.2856 | mg/L | 0.00184 | 0.5712 mg/L | 0.00367 | 0.64% |
| Cu 324.752† | 94601.0 | 0.3485 | mg/L | 0.00243 | 0.6971 mg/L | 0.00487 | 0.70% |
| Fe 273.955† | 205677.9 | 179.9 | mg/L | 1.76 | 359.8 mg/L | 3.52 | 0.98% |
| K 766.490† | 15050.8 | 10.36 | mg/L | 0.084 | 20.71 mg/L | 0.169 | 0.81% |
| Mg 279.077† | 59157.0 | 62.94 | mg/L | 0.607 | 125.9 mg/L | 1.21 | 0.96% |
| Mn 257.610† | 61771.7 | 1.960 | mg/L | 0.0190 | 3.921 mg/L | 0.0381 | 0.97% |
| Mo 202.031† | 208.2 | 0.01155 | mg/L | 0.000034 | 0.02310 mg/L | 0.000068 | 0.30% |
| Na 589.592† | 203278.3 | 17.13 | mg/L | 0.141 | 34.26 mg/L | 0.281 | 0.82% |
| Na 330.237† | 474.2 | 17.99 | mg/L | 0.103 | 35.98 mg/L | 0.206 | 0.57% |
| Ni 231.604† | 474.4 | 0.2930 | mg/L | 0.00290 | 0.5860 mg/L | 0.00581 | 0.99% |
| Pb 220.353† | 1020.6 | 0.1563 | mg/L | 0.00242 | 0.3126 mg/L | 0.00484 | 1.55% |
| Sb 206.836† | 47.4 | 0.02371 | mg/L | 0.005055 | 0.04743 mg/L | 0.010110 | 21.32% |
| Se 196.026† | 47.2 | 0.03743 | mg/L | 0.011463 | 0.07485 mg/L | 0.022926 | 30.63% |
| Si 288.158† | 11425.1 | 7.737 | mg/L | 0.0627 | 15.47 mg/L | 0.125 | 0.81% |
| Sn 189.927† | 19.5 | 0.00954 | mg/L | 0.000586 | 0.01909 mg/L | 0.001172 | 6.14% |
| Sr 421.552† | 169030.4 | 0.2673 | mg/L | 0.00306 | 0.5346 mg/L | 0.00612 | 1.14% |
| Ti 334.903† | 131243.0 | 5.975 | mg/L | 0.0545 | 11.95 mg/L | 0.109 | 0.91% |
| Tl 190.801† | -35.8 | 0.00727 | mg/L | 0.004061 | 0.01454 mg/L | 0.008123 | 55.88% |
| V 292.402† | 38841.7 | 0.3737 | mg/L | 0.00172 | 0.7474 mg/L | 0.00345 | 0.46% |
| Zn 206.200† | 394.4 | 0.6327 | mg/L | 0.00978 | 1.265 mg/L | 0.0196 | 1.55% |

Sequence No.: 18
 Sample ID: RF71 ASPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 309
 Date Collected: 8/6/2010 12:03:32 PM
 Data Type: Original

Nebulizer Parameters: RF71 ASPK SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RF71 ASPK SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1921574.6 | 101.0 | % | 0.85 | | | 0.84% |
| ScR 361.383 | 301838.7 | 103.1 | % | 0.28 | | | 0.27% |
| Ag 328.068† | 87839.2 | 0.5070 | mg/L | 0.00381 | 1.014 mg/L | 0.0076 | 0.75% |
| Al 308.215† | 156663.8 | 123.6 | mg/L | 0.79 | 247.2 mg/L | 1.58 | 0.64% |
| As 188.979† | 2798.2 | 2.134 | mg/L | 0.0274 | 4.267 mg/L | 0.0548 | 1.28% |
| B 249.677† | 275.4 | 0.08176 | mg/L | 0.002280 | 0.1635 mg/L | 0.00456 | 2.79% |
| Ba 233.527† | 7392.3 | 2.200 | mg/L | 0.0021 | 4.400 mg/L | 0.0041 | 0.09% |
| Be 313.042† | 271853.9 | 0.4942 | mg/L | 0.00197 | 0.9884 mg/L | 0.00393 | 0.40% |
| Ca 317.933† | 634390.1 | 43.69 | mg/L | 0.141 | 87.38 mg/L | 0.282 | 0.32% |
| Cd 228.802† | 11470.9 | 0.5313 | mg/L | 0.00477 | 1.063 mg/L | 0.0095 | 0.90% |
| Co 228.616† | 17467.0 | 0.5669 | mg/L | 0.00528 | 1.134 mg/L | 0.0106 | 0.93% |
| Cr 267.716† | 3931.4 | 0.7633 | mg/L | 0.00324 | 1.527 mg/L | 0.0065 | 0.42% |
| Cu 324.752† | 235767.2 | 0.8548 | mg/L | 0.00824 | 1.710 mg/L | 0.0165 | 0.96% |
| Fe 273.955† | 205520.5 | 179.7 | mg/L | 0.58 | 359.5 mg/L | 1.16 | 0.32% |
| K 766.490† | 29597.1 | 20.37 | mg/L | 0.243 | 40.73 mg/L | 0.485 | 1.19% |
| Mg 279.077† | 66737.6 | 71.01 | mg/L | 0.240 | 142.0 mg/L | 0.48 | 0.34% |
| Mn 257.610† | 74257.5 | 2.357 | mg/L | 0.0045 | 4.714 mg/L | 0.0091 | 0.19% |
| Mo 202.031† | 226.3 | 0.01241 | mg/L | 0.000139 | 0.02482 mg/L | 0.000279 | 1.12% |
| Na 589.592† | 326351.1 | 27.50 | mg/L | 0.097 | 55.00 mg/L | 0.194 | 0.35% |
| Na 330.237† | 791.4 | 28.84 | mg/L | 0.084 | 57.68 mg/L | 0.169 | 0.29% |
| Ni 231.604† | 1242.2 | 0.7675 | mg/L | 0.00077 | 1.535 mg/L | 0.0015 | 0.10% |
| Pb 220.353† | 14929.9 | 2.173 | mg/L | 0.0200 | 4.347 mg/L | 0.0400 | 0.92% |
| Sb 206.836† | 1056.2 | 0.3960 | mg/L | 0.00637 | 0.7920 mg/L | 0.01275 | 1.61% |
| Se 196.026† | 2557.1 | 2.145 | mg/L | 0.0271 | 4.290 mg/L | 0.0542 | 1.26% |
| Si 288.158† | 11582.1 | 7.845 | mg/L | 0.0105 | 15.69 mg/L | 0.021 | 0.13% |
| Sn 189.927† | 0.8 | 0.00520 | mg/L | 0.000525 | 0.01039 mg/L | 0.001050 | 10.10% |
| Sr 421.552† | 493651.6 | 0.7807 | mg/L | 0.00505 | 1.561 mg/L | 0.0101 | 0.65% |
| Ti 334.903† | 130521.7 | 5.941 | mg/L | 0.0193 | 11.88 mg/L | 0.039 | 0.33% |
| Tl 190.801† | 3385.7 | 1.995 | mg/L | 0.0261 | 3.990 mg/L | 0.0523 | 1.31% |
| V 292.402† | 85384.5 | 0.8491 | mg/L | 0.00779 | 1.698 mg/L | 0.0156 | 0.92% |
| Zn 206.200† | 702.5 | 1.129 | mg/L | 0.0035 | 2.259 mg/L | 0.0071 | 0.31% |

Sequence No.: 19

Sample ID: ~~RF71 APOST SWC~~ *ZZZZZZ*

Analyst: ALA

Dilution: 2X

Autosampler Location: 310

Date Collected: 8/6/2010 12:07:15 PM

Data Type: Original

Nebulizer Parameters: RF71 APOST SWC

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 200.0 kPa | 0.75 L/min |

Mean Data: RF71 APOST SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|----------|--------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1974501.7 | 103.8 | % | 1.41 | | | | 1.36% |
| ScR 361.383 | 301567.4 | 103.0 | % | 0.93 | | | | 0.90% |
| Ag 328.068† | 698.8 | 0.00394 | mg/L | 0.000029 | 0.00789 | mg/L | 0.000058 | 0.74% |
| Al 308.215† | 159018.3 | 125.4 | mg/L | 1.39 | 250.9 | mg/L | 2.77 | 1.10% |
| As 188.979† | -49.1 | 0.07356 | mg/L | 0.005336 | 0.1471 | mg/L | 0.01067 | 7.25% |
| B 249.677† | 268.1 | 0.08077 | mg/L | 0.001926 | 0.1615 | mg/L | 0.00385 | 2.38% |
| Ba 233.527† | 1130.4 | 0.3216 | mg/L | 0.00417 | 0.6433 | mg/L | 0.00834 | 1.30% |
| Be 313.042† | 3145.4 | 0.00545 | mg/L | 0.000070 | 0.01090 | mg/L | 0.000139 | 1.28% |
| Ca 317.933† | 482608.9 | 33.24 | mg/L | 0.396 | 66.47 | mg/L | 0.792 | 1.19% |
| Cd 228.802† | 177.7 | 0.00864 | mg/L | 0.000165 | 0.01727 | mg/L | 0.000329 | 1.91% |
| Co 228.616† | 2704.7 | 0.07706 | mg/L | 0.001367 | 0.1541 | mg/L | 0.00273 | 1.77% |
| Cr 267.716† | 1522.7 | 0.2959 | mg/L | 0.00339 | 0.5918 | mg/L | 0.00678 | 1.15% |
| Cu 324.752† | 95444.3 | 0.3518 | mg/L | 0.00355 | 0.7036 | mg/L | 0.00709 | 1.01% |
| Fe 273.955† | 210875.6 | 184.4 | mg/L | 2.29 | 368.8 | mg/L | 4.58 | 1.24% |
| K 766.490† | 15533.5 | 10.69 | mg/L | 0.091 | 21.38 | mg/L | 0.183 | 0.85% |
| Mg 279.077† | 60515.2 | 64.38 | mg/L | 0.659 | 128.8 | mg/L | 1.32 | 1.02% |
| Mn 257.610† | 63100.9 | 2.003 | mg/L | 0.0268 | 4.005 | mg/L | 0.0536 | 1.34% |
| Mo 202.031† | 208.6 | 0.01156 | mg/L | 0.000079 | 0.02312 | mg/L | 0.000159 | 0.69% |
| Na 589.592† | 207796.9 | 17.51 | mg/L | 0.191 | 35.02 | mg/L | 0.381 | 1.09% |
| Na 330.237† | 494.7 | 18.73 | mg/L | 0.389 | 37.47 | mg/L | 0.777 | 2.07% |
| Ni 231.604† | 490.1 | 0.3027 | mg/L | 0.00492 | 0.6054 | mg/L | 0.00983 | 1.62% |
| Pb 220.353† | 1114.5 | 0.1701 | mg/L | 0.00230 | 0.3402 | mg/L | 0.00460 | 1.35% |
| Sb 206.836† | 73.3 | 0.03344 | mg/L | 0.000590 | 0.06687 | mg/L | 0.001180 | 1.76% |
| Se 196.026† | 59.8 | 0.04798 | mg/L | 0.003271 | 0.09595 | mg/L | 0.006543 | 6.82% |
| Si 288.158† | 11774.4 | 7.973 | mg/L | 0.0828 | 15.95 | mg/L | 0.166 | 1.04% |
| Sn 189.927† | 18.0 | 0.00924 | mg/L | 0.002102 | 0.01848 | mg/L | 0.004204 | 22.75% |
| Sr 421.552† | 174957.1 | 0.2767 | mg/L | 0.00277 | 0.5534 | mg/L | 0.00554 | 1.00% |
| Ti 334.903† | 134018.0 | 6.101 | mg/L | 0.0685 | 12.20 | mg/L | 0.137 | 1.12% |
| Tl 190.801† | -19.5 | 0.01744 | mg/L | 0.006935 | 0.03487 | mg/L | 0.013871 | 39.77% |
| V 292.402† | 39135.4 | 0.3762 | mg/L | 0.00483 | 0.7524 | mg/L | 0.00966 | 1.28% |
| Zn 206.200† | 406.7 | 0.6525 | mg/L | 0.01045 | 1.305 | mg/L | 0.0209 | 1.60% |

Sequence No.: 20
Sample ID: RF71 MB1SPK SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 311
Date Collected: 8/6/2010 12:11:11 PM
Data Type: Original

Nebulizer Parameters: RF71 MB1SPK SWC
Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RF71 MB1SPK SWC

Table with 8 columns: Analyte, Mean Corrected Intensity, Conc. Units, Calib. Units, Std.Dev., Sample Conc. Units, Std.Dev., RSD. Lists various elements like ScA, ScR, Ag, Al, As, B, Ba, Be, Ca, Cd, Co, Cr, Cu, Fe, K, Mg, Mn, Mo, Na, Ni, Pb, Sb, Se, Si, Sn, Sr, Ti, Tl, V, Zn with their respective values.

Sequence No.: 21
 Sample ID: RG11 MB1SPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 312
 Date Collected: 8/6/2010 12:15:22 PM
 Data Type: Original

Nebulizer Parameters: RG11 MB1SPK SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG11 MB1SPK SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|-----------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1963065.4 | 103.2 | % | 1.44 | | | | 1.40% |
| ScR 361.383 | 297173.7 | 101.5 | % | 2.63 | | | | 2.60% |
| Ag 328.068† | 92795.6 | 0.5357 | mg/L | 0.00815 | 1.071 | mg/L | 0.0163 | 1.52% |
| Al 308.215† | 2714.1 | 2.132 | mg/L | 0.0563 | 4.263 | mg/L | 0.1126 | 2.64% |
| As 188.979† | 2934.7 | 2.126 | mg/L | 0.0360 | 4.253 | mg/L | 0.0719 | 1.69% |
| B 249.677† | -5.1 | -0.00282 | mg/L | 0.001698 | -0.00564 | mg/L | 0.003396 | 60.21% |
| Ba 233.527† | 6589.1 | 1.976 | mg/L | 0.0509 | 3.952 | mg/L | 0.1017 | 2.57% |
| Be 313.042† | 280211.5 | 0.5097 | mg/L | 0.01414 | 1.019 | mg/L | 0.0283 | 2.77% |
| Ca 317.933† | 149069.0 | 10.27 | mg/L | 0.286 | 20.53 | mg/L | 0.572 | 2.79% |
| Cd 228.802† | 11332.0 | 0.5243 | mg/L | 0.00684 | 1.049 | mg/L | 0.0137 | 1.31% |
| Co 228.616† | 15386.7 | 0.5102 | mg/L | 0.00712 | 1.020 | mg/L | 0.0142 | 1.40% |
| Cr 267.716† | 2561.4 | 0.4970 | mg/L | 0.01077 | 0.9939 | mg/L | 0.02153 | 2.17% |
| Cu 324.752† | 137625.4 | 0.4936 | mg/L | 0.00773 | 0.9873 | mg/L | 0.01546 | 1.57% |
| Fe 273.955† | 2460.8 | 2.149 | mg/L | 0.0545 | 4.299 | mg/L | 0.1090 | 2.54% |
| K 766.490† | 15240.6 | 10.49 | mg/L | 0.254 | 20.98 | mg/L | 0.508 | 2.42% |
| Mg 279.077† | 9767.1 | 10.41 | mg/L | 0.221 | 20.81 | mg/L | 0.442 | 2.13% |
| Mn 257.610† | 14863.0 | 0.4721 | mg/L | 0.00988 | 0.9443 | mg/L | 0.01976 | 2.09% |
| Mo 202.031† | 18.9 | 0.00092 | mg/L | 0.000300 | 0.00184 | mg/L | 0.000599 | 32.54% |
| Na 589.592† | 119784.2 | 10.09 | mg/L | 0.245 | 20.19 | mg/L | 0.489 | 2.42% |
| Na 330.237† | 313.6 | 10.72 | mg/L | 0.258 | 21.44 | mg/L | 0.516 | 2.40% |
| Ni 231.604† | 838.3 | 0.5178 | mg/L | 0.01232 | 1.036 | mg/L | 0.0246 | 2.38% |
| Pb 220.353† | 14163.5 | 2.054 | mg/L | 0.0342 | 4.108 | mg/L | 0.0684 | 1.66% |
| Sb 206.836† | 26.7 | 0.00644 | mg/L | 0.000894 | 0.01287 | mg/L | 0.001787 | 13.88% |
| Se 196.026† | 2557.0 | 2.147 | mg/L | 0.0344 | 4.294 | mg/L | 0.0689 | 1.60% |
| Si 288.158† | 16.1 | 0.01275 | mg/L | 0.007008 | 0.02551 | mg/L | 0.014015 | 54.95% |
| Sn 189.927† | -8.9 | -0.00193 | mg/L | 0.000507 | -0.00386 | mg/L | 0.001014 | 26.26% |
| Sr 421.552† | 330006.0 | 0.5219 | mg/L | 0.01143 | 1.044 | mg/L | 0.0229 | 2.19% |
| Ti 334.903† | 33.0 | 0.00077 | mg/L | 0.000817 | 0.00154 | mg/L | 0.001634 | 106.18% |
| Tl 190.801† | 3594.3 | 2.088 | mg/L | 0.0388 | 4.177 | mg/L | 0.0775 | 1.86% |
| V 292.402† | 50992.2 | 0.5204 | mg/L | 0.00834 | 1.041 | mg/L | 0.0167 | 1.60% |
| Zn 206.200† | 318.8 | 0.5141 | mg/L | 0.01251 | 1.028 | mg/L | 0.0250 | 2.43% |

Sequence No.: 22

Sample ID: RG11 MB1SPD

Analyst: ALA

Dilution: 2X

320
489-10

Autosampler Location: 313

Date Collected: 8/6/2010 12:19:33 PM

Data Type: Original

Nebulizer Parameters: RG11 MB1SPD

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 200.0 kPa | 0.75 L/min |

Mean Data: RG11 MB1SPD

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1962901.1 | 103.2 | % | 0.97 | | | | 0.94% |
| ScR 361.383 | 299966.7 | 102.5 | % | 1.16 | | | | 1.13% |
| Ag 328.068† | 92724.3 | 0.5353 | mg/L | 0.00239 | 1.071 | mg/L | 0.0048 | 0.45% |
| Al 308.215† | 2699.5 | 2.120 | mg/L | 0.0187 | 4.240 | mg/L | 0.0374 | 0.88% |
| As 188.979† | 2928.2 | 2.122 | mg/L | 0.0195 | 4.243 | mg/L | 0.0390 | 0.92% |
| B 249.677† | 1.8 | -0.00074 | mg/L | 0.001313 | -0.00148 | mg/L | 0.002626 | 177.01% |
| Ba 233.527† | 6530.5 | 1.958 | mg/L | 0.0182 | 3.917 | mg/L | 0.0364 | 0.93% |
| Be 313.042† | 275484.7 | 0.5011 | mg/L | 0.00325 | 1.002 | mg/L | 0.0065 | 0.65% |
| Ca 317.933† | 146736.5 | 10.11 | mg/L | 0.055 | 20.21 | mg/L | 0.111 | 0.55% |
| Cd 228.802† | 11294.6 | 0.5225 | mg/L | 0.00468 | 1.045 | mg/L | 0.0094 | 0.89% |
| Co 228.616† | 15335.5 | 0.5085 | mg/L | 0.00418 | 1.017 | mg/L | 0.0084 | 0.82% |
| Cr 267.716† | 2548.0 | 0.4944 | mg/L | 0.00537 | 0.9887 | mg/L | 0.01074 | 1.09% |
| Cu 324.752† | 138107.6 | 0.4954 | mg/L | 0.00890 | 0.9907 | mg/L | 0.01780 | 1.80% |
| Fe 273.955† | 2457.4 | 2.146 | mg/L | 0.0197 | 4.293 | mg/L | 0.0393 | 0.92% |
| K 766.490† | 15128.0 | 10.41 | mg/L | 0.137 | 20.82 | mg/L | 0.273 | 1.31% |
| Mg 279.077† | 9610.8 | 10.24 | mg/L | 0.116 | 20.48 | mg/L | 0.233 | 1.14% |
| Mn 257.610† | 14666.1 | 0.4659 | mg/L | 0.00710 | 0.9318 | mg/L | 0.01419 | 1.52% |
| Mo 202.031† | 16.1 | 0.00076 | mg/L | 0.000125 | 0.00152 | mg/L | 0.000250 | 16.45% |
| Na 589.592† | 118248.8 | 9.965 | mg/L | 0.0822 | 19.93 | mg/L | 0.164 | 0.83% |
| Na 330.237† | 311.4 | 10.64 | mg/L | 0.129 | 21.29 | mg/L | 0.258 | 1.21% |
| Ni 231.604† | 822.4 | 0.5080 | mg/L | 0.00486 | 1.016 | mg/L | 0.0097 | 0.96% |
| Pb 220.353† | 14153.5 | 2.053 | mg/L | 0.0100 | 4.105 | mg/L | 0.0200 | 0.49% |
| Sb 206.836† | 14.1 | 0.00177 | mg/L | 0.000403 | 0.00353 | mg/L | 0.000806 | 22.83% |
| Se 196.026† | 2557.1 | 2.147 | mg/L | 0.0175 | 4.294 | mg/L | 0.0350 | 0.82% |
| Si 288.158† | 11.6 | 0.00973 | mg/L | 0.007666 | 0.01947 | mg/L | 0.015331 | 78.75% |
| Sn 189.927† | -15.0 | -0.00361 | mg/L | 0.000444 | -0.00722 | mg/L | 0.000888 | 12.31% |
| Sr 421.552† | 327395.5 | 0.5177 | mg/L | 0.00265 | 1.035 | mg/L | 0.0053 | 0.51% |
| Ti 334.903† | 21.6 | 0.00026 | mg/L | 0.000585 | 0.00053 | mg/L | 0.001170 | 222.05% |
| Tl 190.801† | 3600.5 | 2.092 | mg/L | 0.0157 | 4.184 | mg/L | 0.0313 | 0.75% |
| V 292.402† | 50934.0 | 0.5198 | mg/L | 0.00302 | 1.040 | mg/L | 0.0060 | 0.58% |
| Zn 206.200† | 316.6 | 0.5106 | mg/L | 0.00561 | 1.021 | mg/L | 0.0112 | 1.10% |

Sequence No.: 23
 Sample ID: CV
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 7
 Date Collected: 8/6/2010 12:23:44 PM
 Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|--------|--------------|----------|--------|-------|----------|-------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1933980.8 | 101.7 | % | 0.33 | | | | 0.32% |
| ScR 361.383 | 296410.3 | 101.3 | % | 1.02 | | | | 1.00% |
| Ag 328.068† | 183614.6 | 1.060 | mg/L | 0.0038 | 1.060 | mg/L | 0.0038 | 0.36% |
| Al 308.215† | 2743.2 | 2.132 | mg/L | 0.0182 | 2.132 | mg/L | 0.0182 | 0.85% |
| As 188.979† | 2919.5 | 2.133 | mg/L | 0.0107 | 2.133 | mg/L | 0.0107 | 0.50% |
| B 249.677† | 3386.2 | 1.021 | mg/L | 0.0134 | 1.021 | mg/L | 0.0134 | 1.31% |
| Ba 233.527† | 3285.4 | 0.9848 | mg/L | 0.01161 | 0.9848 | mg/L | 0.01161 | 1.18% |
| Be 313.042† | 557170.4 | 1.013 | mg/L | 0.0051 | 1.013 | mg/L | 0.0051 | 0.50% |
| Ca 317.933† | 30976.0 | 2.133 | mg/L | 0.0212 | 2.133 | mg/L | 0.0212 | 0.99% |
| Cd 228.802† | 22892.0 | 1.067 | mg/L | 0.0054 | 1.067 | mg/L | 0.0054 | 0.51% |
| Co 228.616† | 31402.6 | 1.040 | mg/L | 0.0041 | 1.040 | mg/L | 0.0041 | 0.40% |
| Cr 267.716† | 5138.0 | 0.9994 | mg/L | 0.01089 | 0.9994 | mg/L | 0.01089 | 1.09% |
| Cu 324.752† | 294046.6 | 1.054 | mg/L | 0.0055 | 1.054 | mg/L | 0.0055 | 0.52% |
| Fe 273.955† | 2388.9 | 2.084 | mg/L | 0.0243 | 2.084 | mg/L | 0.0243 | 1.17% |
| K 766.490† | 30443.7 | 20.95 | mg/L | 0.168 | 20.95 | mg/L | 0.168 | 0.80% |
| Mg 279.077† | 1977.0 | 2.112 | mg/L | 0.0223 | 2.112 | mg/L | 0.0223 | 1.06% |
| Mn 257.610† | 29890.7 | 0.9491 | mg/L | 0.01041 | 0.9491 | mg/L | 0.01041 | 1.10% |
| Mo 202.031† | 17113.8 | 0.9955 | mg/L | 0.00147 | 0.9955 | mg/L | 0.00147 | 0.15% |
| Na 589.592† | 599310.5 | 50.50 | mg/L | 0.279 | 50.50 | mg/L | 0.279 | 0.55% |
| Na 330.237† | 1560.8 | 53.71 | mg/L | 0.500 | 53.71 | mg/L | 0.500 | 0.93% |
| Ni 231.604† | 1684.7 | 1.042 | mg/L | 0.0069 | 1.042 | mg/L | 0.0069 | 0.66% |
| Pb 220.353† | 14606.1 | 2.119 | mg/L | 0.0072 | 2.119 | mg/L | 0.0072 | 0.34% |
| Sb 206.836† | 5800.3 | 2.167 | mg/L | 0.0092 | 2.167 | mg/L | 0.0092 | 0.42% |
| Se 196.026† | 2536.1 | 2.130 | mg/L | 0.0101 | 2.130 | mg/L | 0.0101 | 0.47% |
| Si 288.158† | 3245.5 | 2.201 | mg/L | 0.0229 | 2.201 | mg/L | 0.0229 | 1.04% |
| Sn 189.927† | 3877.1 | 1.056 | mg/L | 0.0050 | 1.056 | mg/L | 0.0050 | 0.47% |
| Sr 421.552† | 661933.9 | 1.047 | mg/L | 0.0068 | 1.047 | mg/L | 0.0068 | 0.65% |
| Ti 334.903† | 22646.5 | 1.030 | mg/L | 0.0137 | 1.030 | mg/L | 0.0137 | 1.33% |
| Tl 190.801† | 3618.6 | 2.104 | mg/L | 0.0067 | 2.104 | mg/L | 0.0067 | 0.32% |
| V 292.402† | 101970.0 | 1.041 | mg/L | 0.0077 | 1.041 | mg/L | 0.0077 | 0.74% |
| Zn 206.200† | 647.4 | 1.044 | mg/L | 0.0093 | 1.044 | mg/L | 0.0093 | 0.89% |

Sequence No.: 24
Sample ID: CB
Analyst: ALA
Dilution: 1X

Autosampler Location: 1
Date Collected: 8/6/2010 12:27:57 PM
Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1944308.2 | 102.2 % | 0.36 | | | 0.35% |
| ScR 361.383 | 301689.0 | 103.1 % | 1.39 | | | 1.35% |
| Ag 328.068† | -54.0 | -0.00031 mg/L | 0.000506 | -0.00031 mg/L | 0.000506 | 162.45% |
| Al 308.215† | 1.5 | 0.00122 mg/L | 0.001022 | 0.00122 mg/L | 0.001022 | 83.94% |
| As 188.979† | -0.4 | -0.00032 mg/L | 0.001071 | -0.00032 mg/L | 0.001071 | 337.02% |
| B 249.677† | -2.3 | -0.00068 mg/L | 0.001529 | -0.00068 mg/L | 0.001529 | 224.75% |
| Ba 233.527† | 2.4 | 0.00073 mg/L | 0.000656 | 0.00073 mg/L | 0.000656 | 90.23% |
| Be 313.042† | 0.4 | 0.00000 mg/L | 0.000036 | 0.00000 mg/L | 0.000036 | >999.9% |
| Ca 317.933† | 13.1 | 0.00090 mg/L | 0.002627 | 0.00090 mg/L | 0.002627 | 290.65% |
| Cd 228.802† | -1.8 | -0.00008 mg/L | 0.000087 | -0.00008 mg/L | 0.000087 | 105.65% |
| Co 228.616† | -4.7 | -0.00016 mg/L | 0.000033 | -0.00016 mg/L | 0.000033 | 20.88% |
| Cr 267.716† | 4.0 | 0.00078 mg/L | 0.001342 | 0.00078 mg/L | 0.001342 | 171.57% |
| Cu 324.752† | 209.2 | 0.00075 mg/L | 0.000151 | 0.00075 mg/L | 0.000151 | 20.17% |
| Fe 273.955† | -3.4 | -0.00298 mg/L | 0.003630 | -0.00298 mg/L | 0.003630 | 121.98% |
| K 766.490† | 23.8 | 0.01640 mg/L | 0.026136 | 0.01640 mg/L | 0.026136 | 159.39% |
| Mg 279.077† | 9.2 | 0.00983 mg/L | 0.001503 | 0.00983 mg/L | 0.001503 | 15.29% |
| Mn 257.610† | -1.4 | -0.00005 mg/L | 0.000028 | -0.00005 mg/L | 0.000028 | 62.56% |
| Mo 202.031† | -3.1 | -0.00018 mg/L | 0.000341 | -0.00018 mg/L | 0.000341 | 188.02% |
| Na 589.592† | 72.2 | 0.00608 mg/L | 0.004339 | 0.00608 mg/L | 0.004339 | 71.34% |
| Na 330.237† | 1.2 | 0.04001 mg/L | 0.119348 | 0.04001 mg/L | 0.119348 | 298.33% |
| Ni 231.604† | 3.5 | 0.00215 mg/L | 0.001714 | 0.00215 mg/L | 0.001714 | 79.66% |
| Pb 220.353† | 1.3 | 0.00019 mg/L | 0.000606 | 0.00019 mg/L | 0.000606 | 311.46% |
| Sb 206.836† | 10.4 | 0.00387 mg/L | 0.001257 | 0.00387 mg/L | 0.001257 | 32.48% |
| Se 196.026† | 9.1 | 0.00763 mg/L | 0.002000 | 0.00763 mg/L | 0.002000 | 26.21% |
| Si 288.158† | 6.5 | 0.00441 mg/L | 0.004450 | 0.00441 mg/L | 0.004450 | 100.81% |
| Sn 189.927† | 3.7 | 0.00101 mg/L | 0.000757 | 0.00101 mg/L | 0.000757 | 75.20% |
| Sr 421.552† | -8.7 | -0.00001 mg/L | 0.000054 | -0.00001 mg/L | 0.000054 | 390.91% |
| Ti 334.903† | 9.4 | 0.00043 mg/L | 0.001099 | 0.00043 mg/L | 0.001099 | 257.32% |
| Tl 190.801† | 5.7 | 0.00331 mg/L | 0.000478 | 0.00331 mg/L | 0.000478 | 14.44% |
| V 292.402† | 22.3 | 0.00023 mg/L | 0.000068 | 0.00023 mg/L | 0.000068 | 29.31% |
| Zn 206.200† | 0.8 | 0.00130 mg/L | 0.000422 | 0.00130 mg/L | 0.000422 | 32.48% |

Sequence No.: 25
 Sample ID: RG84 D SWC
 Analyst: ALA
 Dilution: 10X

Autosampler Location: 322
 Date Collected: 8/6/2010 12:32:08 PM
 Data Type: Original

DEL

Nebulizer Parameters: RG84 D SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG84 D SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1967540.2 | 103.5 | % | 0.41 | | | 0.39% |
| ScR 361.383 | 304209.8 | 103.9 | % | 0.18 | | | 0.17% |
| Ag 328.068† | 184.9 | 0.00087 | mg/L | 0.000147 | 0.00870 mg/L | 0.001470 | 16.90% |
| Al 308.215† | 28572.8 | 22.54 | mg/L | 0.181 | 225.4 mg/L | 1.81 | 0.80% |
| As 188.979† | 42.9 | 0.05500 | mg/L | 0.005122 | 0.5500 mg/L | 0.05122 | 9.31% |
| B 249.677† | 106.0 | 0.03194 | mg/L | 0.002379 | 0.3194 mg/L | 0.02379 | 7.45% |
| Ba 233.527† | 892.2 | 0.2556 | mg/L | 0.00132 | 2.556 mg/L | 0.0132 | 0.52% |
| Be 313.042† | 275.0 | 0.00041 | mg/L | 0.000007 | 0.00412 mg/L | 0.000073 | 1.76% |
| Ca 317.933† | 173691.4 | 11.96 | mg/L | 0.096 | 119.6 mg/L | 0.96 | 0.81% |
| Cd 228.802† | 1222.1 | 0.05729 | mg/L | 0.000445 | 0.5729 mg/L | 0.00445 | 0.78% |
| Co 228.616† | 1361.1 | 0.04120 | mg/L | 0.000487 | 0.4120 mg/L | 0.00487 | 1.18% |
| Cr 267.716† | 1367.2 | 0.2708 | mg/L | 0.00089 | 2.708 mg/L | 0.0089 | 0.33% |
| Cu 324.752† | 160267.3 | 0.5833 | mg/L | 0.00023 | 5.833 mg/L | 0.0023 | 0.04% |
| Fe 273.955† | 147224.8 | 128.8 | mg/L | 1.03 | 1288 mg/L | 10.3 | 0.80% |
| K 766.490† | 2002.3 | 1.378 | mg/L | 0.0051 | 13.78 mg/L | 0.051 | 0.37% |
| Mg 279.077† | 7381.2 | 7.799 | mg/L | 0.0035 | 77.99 mg/L | 0.035 | 0.05% |
| Mn 257.610† | 43737.6 | 1.389 | mg/L | 0.0068 | 13.89 mg/L | 0.068 | 0.49% |
| Mo 202.031† | 549.2 | 0.03174 | mg/L | 0.000457 | 0.3174 mg/L | 0.00457 | 1.44% |
| Na 589.592† | 12932.3 | 1.090 | mg/L | 0.0049 | 10.90 mg/L | 0.049 | 0.45% |
| Na 330.237† | 47.8 | 1.074 | mg/L | 0.2213 | 10.74 mg/L | 2.213 | 20.60% |
| Ni 231.604† | 283.6 | 0.1752 | mg/L | 0.00431 | 1.752 mg/L | 0.0431 | 2.46% |
| Pb 220.353† | 7940.7 | 1.146 | mg/L | 0.0082 | 11.46 mg/L | 0.082 | 0.71% |
| Sb 206.836† | 56.6 | 0.02083 | mg/L | 0.002735 | 0.2083 mg/L | 0.02735 | 13.13% |
| Se 196.026† | 14.0 | 0.01095 | mg/L | 0.005616 | 0.1095 mg/L | 0.05616 | 51.28% |
| Si 288.158† | 329.1 | 0.2231 | mg/L | 0.00110 | 2.231 mg/L | 0.0110 | 0.49% |
| Sn 189.927† | 105.7 | 0.02995 | mg/L | 0.001119 | 0.2995 mg/L | 0.01119 | 3.74% |
| Sr 421.552† | 43903.2 | 0.06943 | mg/L | 0.000639 | 0.6943 mg/L | 0.00639 | 0.92% |
| Ti 334.903† | 29837.3 | 1.358 | mg/L | 0.0075 | 13.58 mg/L | 0.075 | 0.55% |
| Tl 190.801† | -27.6 | 0.00438 | mg/L | 0.001659 | 0.04382 mg/L | 0.016593 | 37.87% |
| V 292.402† | 13842.2 | 0.1275 | mg/L | 0.00103 | 1.275 mg/L | 0.0103 | 0.81% |
| Zn 206.200† | 2634.4 | 4.248 | mg/L | 0.0175 | 42.48 mg/L | 0.175 | 0.41% |

Sequence No.: 26
Sample ID: RG84 G SWC
Analyst: ALA
Dilution: 10X

Autosampler Location: 323
Date Collected: 8/6/2010 12:36:06 PM
Data Type: Original

DEL

Nebulizer Parameters: RG84 G SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG84 G SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1977300.0 | 104.0 % | % | 0.74 | | | 0.71% |
| ScR 361.383 | 281667.1 | 96.24 % | % | 0.230 | | | 0.24% |
| Ag 328.068† | 462.7 | 0.00250 mg/L | mg/L | 0.000117 | 0.02501 mg/L | 0.001170 | 4.68% |
| Al 308.215† | 36451.9 | 28.75 mg/L | mg/L | 0.232 | 287.5 mg/L | 2.32 | 0.81% |
| As 188.979† | -16.1 | 0.01805 mg/L | mg/L | 0.002337 | 0.1805 mg/L | 0.02337 | 12.95% |
| B 249.677† | 37.9 | 0.01138 mg/L | mg/L | 0.000951 | 0.1138 mg/L | 0.00951 | 8.36% |
| Ba 233.527† | 1320.2 | 0.3822 mg/L | mg/L | 0.00040 | 3.822 mg/L | 0.0040 | 0.10% |
| Be 313.042† | 332.7 | 0.00053 mg/L | mg/L | 0.000010 | 0.00533 mg/L | 0.000097 | 1.83% |
| Ca 317.933† | 276736.1 | 19.06 mg/L | mg/L | 0.211 | 190.6 mg/L | 2.11 | 1.11% |
| Cd 228.802† | 676.2 | 0.03191 mg/L | mg/L | 0.000303 | 0.3191 mg/L | 0.00303 | 0.95% |
| Co 228.616† | 1314.1 | 0.03878 mg/L | mg/L | 0.000191 | 0.3878 mg/L | 0.00191 | 0.49% |
| Cr 267.716† | 2245.5 | 0.4424 mg/L | mg/L | 0.00385 | 4.424 mg/L | 0.0385 | 0.87% |
| Cu 324.752† | 111463.5 | 0.4096 mg/L | mg/L | 0.00428 | 4.096 mg/L | 0.0428 | 1.05% |
| Fe 273.955† | 169887.1 | 148.6 mg/L | mg/L | 0.91 | 1486 mg/L | 9.1 | 0.61% |
| K 766.490† | 2954.4 | 2.033 mg/L | mg/L | 0.0057 | 20.33 mg/L | 0.057 | 0.28% |
| Mg 279.077† | 8376.3 | 8.849 mg/L | mg/L | 0.0254 | 88.49 mg/L | 0.254 | 0.29% |
| Mn 257.610† | 39741.2 | 1.262 mg/L | mg/L | 0.0095 | 12.62 mg/L | 0.095 | 0.75% |
| Mo 202.031† | 609.4 | 0.03512 mg/L | mg/L | 0.000303 | 0.3512 mg/L | 0.00303 | 0.86% |
| Na 589.592† | 13865.8 | 1.168 mg/L | mg/L | 0.0105 | 11.68 mg/L | 0.105 | 0.90% |
| Na 330.237† | 28.9 | 1.126 mg/L | mg/L | 0.3349 | 11.26 mg/L | 3.349 | 29.74% |
| Ni 231.604† | 430.3 | 0.2658 mg/L | mg/L | 0.00482 | 2.658 mg/L | 0.0482 | 1.82% |
| Pb 220.353† | 1767.8 | 0.2511 mg/L | mg/L | 0.00183 | 2.511 mg/L | 0.0183 | 0.73% |
| Sb 206.836† | 43.7 | 0.01440 mg/L | mg/L | 0.002250 | 0.1440 mg/L | 0.02250 | 15.63% |
| Se 196.026† | 16.9 | 0.01292 mg/L | mg/L | 0.001643 | 0.1292 mg/L | 0.01643 | 12.72% |
| Si 288.158† | 330.4 | 0.2238 mg/L | mg/L | 0.00387 | 2.238 mg/L | 0.0387 | 1.73% |
| Sn 189.927† | 52.1 | 0.01583 mg/L | mg/L | 0.001624 | 0.1583 mg/L | 0.01624 | 10.26% |
| Sr 421.552† | 83682.6 | 0.1323 mg/L | mg/L | 0.00080 | 1.323 mg/L | 0.0080 | 0.60% |
| Ti 334.903† | 37387.3 | 1.701 mg/L | mg/L | 0.0134 | 17.01 mg/L | 0.134 | 0.79% |
| Tl 190.801† | -23.0 | 0.00993 mg/L | mg/L | 0.002370 | 0.09928 mg/L | 0.023698 | 23.87% |
| V 292.402† | 10164.4 | 0.08849 mg/L | mg/L | 0.001015 | 0.8849 mg/L | 0.01015 | 1.15% |
| Zn 206.200† | 1170.8 | 1.888 mg/L | mg/L | 0.0114 | 18.88 mg/L | 0.114 | 0.61% |

Sequence No.: 27
Sample ID: RG84 H SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 324
Date Collected: 8/6/2010 12:40:02 PM
Data Type: Original

DEL

Nebulizer Parameters: RG84 H SWC

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG84 H SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1966180.5 | 103.4 | % | 0.64 | | | 0.61% |
| ScR 361.383 | 305771.5 | 104.5 | % | 1.71 | | | 1.64% |
| Ag 328.068† | 206.4 | 0.00068 | mg/L | 0.000128 | 0.00137 mg/L | 0.000255 | 18.65% |
| Al 308.215† | 143636.3 | 113.3 | mg/L | 1.68 | 226.6 mg/L | 3.36 | 1.48% |
| As 188.979† | -86.6 | 0.03620 | mg/L | 0.002474 | 0.07241 mg/L | 0.004949 | 6.83% |
| B 249.677† | 312.1 | 0.09406 | mg/L | 0.003234 | 0.1881 mg/L | 0.00647 | 3.44% |
| Ba 233.527† | 6299.4 | 1.869 | mg/L | 0.0400 | 3.739 mg/L | 0.0800 | 2.14% |
| Be 313.042† | 1195.8 | 0.00188 | mg/L | 0.000072 | 0.00375 mg/L | 0.000143 | 3.82% |
| Ca 317.933† | 1454755.7 | 100.2 | mg/L | 1.41 | 200.4 mg/L | 2.83 | 1.41% |
| Cd 228.802† | 640.2 | 0.03043 | mg/L | 0.000164 | 0.06087 mg/L | 0.000328 | 0.54% |
| Co 228.616† | 3284.8 | 0.09644 | mg/L | 0.001006 | 0.1929 mg/L | 0.00201 | 1.04% |
| Cr 267.716† | 3358.9 | 0.6560 | mg/L | 0.01116 | 1.312 mg/L | 0.0223 | 1.70% |
| Cu 324.752† | 529140.1 | 1.910 | mg/L | 0.0009 | 3.819 mg/L | 0.0018 | 0.05% |
| Fe 273.955† | 239710.9 | 209.6 | mg/L | 2.73 | 419.3 mg/L | 5.45 | 1.30% |
| K 766.490† | 13387.2 | 9.212 | mg/L | 0.1072 | 18.42 mg/L | 0.214 | 1.16% |
| Mg 279.077† | 39765.2 | 42.25 | mg/L | 0.484 | 84.51 mg/L | 0.967 | 1.14% |
| Mn 257.610† | 128731.9 | 4.086 | mg/L | 0.0598 | 8.172 mg/L | 0.1197 | 1.46% |
| Mo 202.031† | 1000.0 | 0.05643 | mg/L | 0.000110 | 0.1129 mg/L | 0.00022 | 0.20% |
| Na 589.592† | 70276.9 | 5.922 | mg/L | 0.0858 | 11.84 mg/L | 0.172 | 1.45% |
| Na 330.237† | 277.5 | 6.509 | mg/L | 0.1579 | 13.02 mg/L | 0.316 | 2.43% |
| Ni 231.604† | 552.1 | 0.3410 | mg/L | 0.00696 | 0.6821 mg/L | 0.01393 | 2.04% |
| Pb 220.353† | 13726.3 | 1.994 | mg/L | 0.0086 | 3.987 mg/L | 0.0171 | 0.43% |
| Sb 206.836† | 73.2 | 0.02953 | mg/L | 0.003560 | 0.05906 mg/L | 0.007120 | 12.06% |
| Se 196.026† | 56.1 | 0.04029 | mg/L | 0.004791 | 0.08058 mg/L | 0.009582 | 11.89% |
| Si 288.158† | 1514.7 | 1.026 | mg/L | 0.0193 | 2.052 mg/L | 0.0385 | 1.88% |
| Sn 189.927† | 118.1 | 0.03937 | mg/L | 0.001763 | 0.07874 mg/L | 0.003525 | 4.48% |
| Sr 421.552† | 384542.0 | 0.6081 | mg/L | 0.00797 | 1.216 mg/L | 0.0159 | 1.31% |
| Ti 334.903† | 124580.3 | 5.667 | mg/L | 0.0775 | 11.33 mg/L | 0.155 | 1.37% |
| Tl 190.801† | -33.5 | 0.01500 | mg/L | 0.005042 | 0.02999 mg/L | 0.010085 | 33.63% |
| V 292.402† | 44953.8 | 0.4347 | mg/L | 0.00113 | 0.8695 mg/L | 0.00226 | 0.26% |
| Zn 206.200† | 13497.5 | 21.77 | mg/L | 0.231 | 43.53 mg/L | 0.462 | 1.06% |

Sequence No.: 28
Sample ID: RG84 I SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 325
Date Collected: 8/6/2010 12:43:44 PM
Data Type: Original

DL

Nebulizer Parameters: RG84 I SWC
Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG84 I SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1996013.9 | 105.0 | % | 0.85 | | | 0.81% |
| ScR 361.383 | 305088.6 | 104.2 | % | 1.18 | | | 1.14% |
| Ag 328.068† | -118.3 | -0.00080 | mg/L | 0.000212 | -0.00160 mg/L | 0.000423 | 26.53% |
| Al 308.215† | 198307.6 | 156.4 | mg/L | 1.85 | 312.9 mg/L | 3.70 | 1.18% |
| As 188.979† | -172.4 | 0.03656 | mg/L | 0.003746 | 0.07312 mg/L | 0.007492 | 10.25% |
| B 249.677† | 39.7 | 0.01174 | mg/L | 0.002944 | 0.02348 mg/L | 0.005888 | 25.08% |
| Ba 233.527† | 1807.7 | 0.5204 | mg/L | 0.00494 | 1.041 mg/L | 0.0099 | 0.95% |
| Be 313.042† | 1649.9 | 0.00261 | mg/L | 0.000045 | 0.00521 mg/L | 0.000091 | 1.74% |
| Ca 317.933† | 932498.3 | 64.22 | mg/L | 0.755 | 128.4 mg/L | 1.51 | 1.18% |
| Cd 228.802† | 122.0 | 0.00626 | mg/L | 0.000171 | 0.01252 mg/L | 0.000342 | 2.73% |
| Co 228.616† | 2944.9 | 0.07951 | mg/L | 0.000473 | 0.1590 mg/L | 0.00095 | 0.59% |
| Cr 267.716† | 1050.6 | 0.2065 | mg/L | 0.00300 | 0.4131 mg/L | 0.00599 | 1.45% |
| Cu 324.752† | 85291.8 | 0.3176 | mg/L | 0.00393 | 0.6353 mg/L | 0.00786 | 1.24% |
| Fe 273.955† | 260893.4 | 228.2 | mg/L | 3.19 | 456.3 mg/L | 6.39 | 1.40% |
| K 766.490† | 14842.0 | 10.21 | mg/L | 0.139 | 20.43 mg/L | 0.278 | 1.36% |
| Mg 279.077† | 52382.5 | 55.69 | mg/L | 0.877 | 111.4 mg/L | 1.75 | 1.57% |
| Mn 257.610† | 89828.5 | 2.851 | mg/L | 0.0455 | 5.701 mg/L | 0.0911 | 1.60% |
| Mo 202.031† | 112.3 | 0.00542 | mg/L | 0.000609 | 0.01084 mg/L | 0.001217 | 11.23% |
| Na 589.592† | 73884.6 | 6.226 | mg/L | 0.0816 | 12.45 mg/L | 0.163 | 1.31% |
| Na 330.237† | 130.2 | 6.583 | mg/L | 0.3153 | 13.17 mg/L | 0.631 | 4.79% |
| Ni 231.604† | 322.0 | 0.1989 | mg/L | 0.00522 | 0.3978 mg/L | 0.01045 | 2.63% |
| Pb 220.353† | 450.2 | 0.07582 | mg/L | 0.001042 | 0.1516 mg/L | 0.00208 | 1.37% |
| Sb 206.836† | 32.1 | 0.02314 | mg/L | 0.002199 | 0.04628 mg/L | 0.004398 | 9.50% |
| Se 196.026† | 46.7 | 0.03488 | mg/L | 0.002704 | 0.06977 mg/L | 0.005407 | 7.75% |
| Si 288.158† | 1385.2 | 0.9380 | mg/L | 0.01028 | 1.876 mg/L | 0.0206 | 1.10% |
| Sn 189.927† | -34.1 | -0.00215 | mg/L | 0.000144 | -0.00430 mg/L | 0.000288 | 6.70% |
| Sr 421.552† | 291976.8 | 0.4617 | mg/L | 0.00574 | 0.9235 mg/L | 0.01148 | 1.24% |
| Ti 334.903† | 198521.4 | 9.036 | mg/L | 0.1292 | 18.07 mg/L | 0.258 | 1.43% |
| Tl 190.801† | -38.4 | 0.01358 | mg/L | 0.000902 | 0.02715 mg/L | 0.001804 | 6.64% |
| V 292.402† | 55849.7 | 0.5395 | mg/L | 0.00528 | 1.079 mg/L | 0.0106 | 0.98% |
| Zn 206.200† | 2001.8 | 3.224 | mg/L | 0.0372 | 6.449 mg/L | 0.0744 | 1.15% |

Sequence No.: 29
 Sample ID: RG84 J SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 326
 Date Collected: 8/6/2010 12:47:26 PM
 Data Type: Original

DEL

Nebulizer Parameters: RG84 J SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG84 J SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1992117.3 | 104.8 | % | 2.28 | | | 2.18% |
| ScR 361.383 | 310789.5 | 106.2 | % | 1.65 | | | 1.56% |
| Ag 328.068† | -17.8 | -0.00016 | mg/L | 0.000191 | -0.00032 mg/L | 0.000382 | 118.55% |
| Al 308.215† | 162837.8 | 128.4 | mg/L | 1.88 | 256.9 mg/L | 3.75 | 1.46% |
| As 188.979† | -195.6 | 0.01839 | mg/L | 0.007163 | 0.03678 mg/L | 0.014327 | 38.96% |
| B 249.677† | 35.4 | 0.01049 | mg/L | 0.000524 | 0.02098 mg/L | 0.001048 | 5.00% |
| Ba 233.527† | 1684.6 | 0.4860 | mg/L | 0.00600 | 0.9720 mg/L | 0.01199 | 1.23% |
| Be 313.042† | 1214.6 | 0.00186 | mg/L | 0.000057 | 0.00373 mg/L | 0.000115 | 3.08% |
| Ca 317.933† | 901800.8 | 62.11 | mg/L | 1.000 | 124.2 mg/L | 2.00 | 1.61% |
| Cd 228.802† | 141.4 | 0.00726 | mg/L | 0.000464 | 0.01453 mg/L | 0.000928 | 6.39% |
| Co 228.616† | 2575.0 | 0.06768 | mg/L | 0.001693 | 0.1354 mg/L | 0.00339 | 2.50% |
| Cr 267.716† | 1477.9 | 0.2894 | mg/L | 0.00360 | 0.5788 mg/L | 0.00721 | 1.25% |
| Cu 324.752† | 127721.1 | 0.4681 | mg/L | 0.01104 | 0.9362 mg/L | 0.02209 | 2.36% |
| Fe 273.955† | 230714.5 | 201.8 | mg/L | 3.25 | 403.5 mg/L | 6.49 | 1.61% |
| K 766.490† | 11386.3 | 7.835 | mg/L | 0.1206 | 15.67 mg/L | 0.241 | 1.54% |
| Mg 279.077† | 46023.2 | 48.93 | mg/L | 0.875 | 97.86 mg/L | 1.749 | 1.79% |
| Mn 257.610† | 76682.4 | 2.434 | mg/L | 0.0419 | 4.867 mg/L | 0.0838 | 1.72% |
| Mo 202.031† | 235.8 | 0.01264 | mg/L | 0.000687 | 0.02528 mg/L | 0.001373 | 5.43% |
| Na 589.592† | 73404.5 | 6.186 | mg/L | 0.1001 | 12.37 mg/L | 0.200 | 1.62% |
| Na 330.237† | 268.5 | 6.641 | mg/L | 0.3089 | 13.28 mg/L | 0.618 | 4.65% |
| Ni 231.604† | 412.6 | 0.2549 | mg/L | 0.00231 | 0.5097 mg/L | 0.00462 | 0.91% |
| Pb 220.353† | 5338.1 | 0.7816 | mg/L | 0.01766 | 1.563 mg/L | 0.0353 | 2.26% |
| Sb 206.836† | 29.1 | 0.02087 | mg/L | 0.001930 | 0.04173 mg/L | 0.003859 | 9.25% |
| Se 196.026† | 51.5 | 0.03905 | mg/L | 0.002130 | 0.07811 mg/L | 0.004260 | 5.45% |
| Si 288.158† | 1708.7 | 1.157 | mg/L | 0.0189 | 2.314 mg/L | 0.0378 | 1.63% |
| Sn 189.927† | -3.1 | 0.00614 | mg/L | 0.001033 | 0.01227 mg/L | 0.002066 | 16.84% |
| Sr 421.552† | 182197.7 | 0.2881 | mg/L | 0.00480 | 0.5763 mg/L | 0.00961 | 1.67% |
| Ti 334.903† | 196954.9 | 8.965 | mg/L | 0.1506 | 17.93 mg/L | 0.301 | 1.68% |
| Tl 190.801† | -30.8 | 0.01382 | mg/L | 0.002165 | 0.02765 mg/L | 0.004330 | 15.66% |
| V 292.402† | 46598.5 | 0.4486 | mg/L | 0.01061 | 0.8972 mg/L | 0.02123 | 2.37% |
| Zn 206.200† | 14113.9 | 22.76 | mg/L | 0.436 | 45.52 mg/L | 0.872 | 1.92% |

Sequence No.: 30
Sample ID: RG84 K SWC
Analyst: ALA
Dilution: 2X

DEL

Autosampler Location: 327
Date Collected: 8/6/2010 12:51:08 PM
Data Type: Original

Nebulizer Parameters: RG84 K SWC

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG84 K SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|--------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1987646.8 | 104.5 | % | 1.53 | | | | 1.47% |
| ScR 361.383 | 308043.1 | 105.2 | % | 0.88 | | | | 0.84% |
| Ag 328.068† | -29.4 | -0.00024 | mg/L | 0.000382 | -0.00048 | mg/L | 0.000764 | 158.59% |
| Al 308.215† | 141239.2 | 111.4 | mg/L | 1.31 | 222.8 | mg/L | 2.62 | 1.18% |
| As 188.979† | -152.8 | 0.02784 | mg/L | 0.004730 | 0.05568 | mg/L | 0.009460 | 16.99% |
| B 249.677† | 220.2 | 0.06631 | mg/L | 0.002430 | 0.1326 | mg/L | 0.00486 | 3.66% |
| Ba 233.527† | 2217.4 | 0.6481 | mg/L | 0.00524 | 1.296 | mg/L | 0.0105 | 0.81% |
| Be 313.042† | 1217.3 | 0.00188 | mg/L | 0.000007 | 0.00376 | mg/L | 0.000013 | 0.35% |
| Ca 317.933† | 890332.3 | 61.32 | mg/L | 0.939 | 122.6 | mg/L | 1.88 | 1.53% |
| Cd 228.802† | 175.4 | 0.00874 | mg/L | 0.000284 | 0.01747 | mg/L | 0.000568 | 3.25% |
| Co 228.616† | 2814.7 | 0.07793 | mg/L | 0.001008 | 0.1559 | mg/L | 0.00202 | 1.29% |
| Cr 267.716† | 1361.1 | 0.2665 | mg/L | 0.00181 | 0.5331 | mg/L | 0.00362 | 0.68% |
| Cu 324.752† | 139043.9 | 0.5076 | mg/L | 0.01221 | 1.015 | mg/L | 0.0244 | 2.41% |
| Fe 273.955† | 202787.1 | 177.3 | mg/L | 2.78 | 354.7 | mg/L | 5.57 | 1.57% |
| K 766.490† | 10175.3 | 7.002 | mg/L | 0.0386 | 14.00 | mg/L | 0.077 | 0.55% |
| Mg 279.077† | 38812.6 | 41.26 | mg/L | 0.599 | 82.52 | mg/L | 1.197 | 1.45% |
| Mn 257.610† | 72287.3 | 2.294 | mg/L | 0.0309 | 4.588 | mg/L | 0.0618 | 1.35% |
| Mo 202.031† | 219.3 | 0.01169 | mg/L | 0.000562 | 0.02339 | mg/L | 0.001124 | 4.81% |
| Na 589.592† | 73011.8 | 6.153 | mg/L | 0.0700 | 12.31 | mg/L | 0.140 | 1.14% |
| Na 330.237† | 146.9 | 6.337 | mg/L | 0.2264 | 12.67 | mg/L | 0.453 | 3.57% |
| Ni 231.604† | 373.1 | 0.2304 | mg/L | 0.00145 | 0.4609 | mg/L | 0.00290 | 0.63% |
| Pb 220.353† | 3204.9 | 0.4710 | mg/L | 0.00596 | 0.9421 | mg/L | 0.01192 | 1.27% |
| Sb 206.836† | 26.3 | 0.01866 | mg/L | 0.000264 | 0.03733 | mg/L | 0.000529 | 1.42% |
| Se 196.026† | 39.0 | 0.02855 | mg/L | 0.003156 | 0.05711 | mg/L | 0.006312 | 11.05% |
| Si 288.158† | 1912.2 | 1.295 | mg/L | 0.0118 | 2.590 | mg/L | 0.0236 | 0.91% |
| Sn 189.927† | 28.5 | 0.01417 | mg/L | 0.000513 | 0.02833 | mg/L | 0.001025 | 3.62% |
| Sr 421.552† | 380969.7 | 0.6025 | mg/L | 0.00745 | 1.205 | mg/L | 0.0149 | 1.24% |
| Ti 334.903† | 170692.0 | 7.769 | mg/L | 0.1084 | 15.54 | mg/L | 0.217 | 1.40% |
| Tl 190.801† | -26.9 | 0.01222 | mg/L | 0.002012 | 0.02443 | mg/L | 0.004024 | 16.47% |
| V 292.402† | 47187.0 | 0.4578 | mg/L | 0.01016 | 0.9155 | mg/L | 0.02033 | 2.22% |
| Zn 206.200† | 3180.0 | 5.126 | mg/L | 0.0327 | 10.25 | mg/L | 0.065 | 0.64% |

Sequence No.: 31
Sample ID: RG84 ADUP SWC
Analyst: ALA
Dilution: 20X

DEL

Autosampler Location: 328
Date Collected: 8/6/2010 12:54:50 PM
Data Type: Original

Nebulizer Parameters: RG84 ADUP SWC
Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG84 ADUP SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|----------|--------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1936804.8 | 101.8 | % | 0.56 | | | | 0.55% |
| ScR 361.383 | 280699.4 | 95.91 | % | 0.426 | | | | 0.44% |
| Ag 328.068† | 662.3 | 0.00372 | mg/L | 0.000110 | 0.07447 | mg/L | 0.002206 | 2.96% |
| Al 308.215† | 23691.3 | 18.69 | mg/L | 0.119 | 373.8 | mg/L | 2.38 | 0.64% |
| As 188.979† | 32.7 | 0.03799 | mg/L | 0.000503 | 0.7598 | mg/L | 0.01006 | 1.32% |
| B 249.677† | 32.7 | 0.00985 | mg/L | 0.001030 | 0.1970 | mg/L | 0.02060 | 10.46% |
| Ba 233.527† | 559.6 | 0.1615 | mg/L | 0.00044 | 3.230 | mg/L | 0.0088 | 0.27% |
| Be 313.042† | 303.2 | 0.00051 | mg/L | 0.000013 | 0.01029 | mg/L | 0.000253 | 2.46% |
| Ca 317.933† | 154513.7 | 10.64 | mg/L | 0.054 | 212.8 | mg/L | 1.09 | 0.51% |
| Cd 228.802† | 715.7 | 0.03366 | mg/L | 0.000250 | 0.6732 | mg/L | 0.00500 | 0.74% |
| Co 228.616† | 831.8 | 0.02528 | mg/L | 0.000316 | 0.5056 | mg/L | 0.00631 | 1.25% |
| Cr 267.716† | 2424.5 | 0.4742 | mg/L | 0.00092 | 9.483 | mg/L | 0.0183 | 0.19% |
| Cu 324.752† | 9035186.5 | 32.41 | mg/L | 0.306 | 648.1 | mg/L | 6.12 | 0.94% |
| Fe 273.955† | 77150.1 | 67.47 | mg/L | 0.318 | 1349 | mg/L | 6.4 | 0.47% |
| K 766.490† | 1344.5 | 0.9252 | mg/L | 0.01435 | 18.50 | mg/L | 0.287 | 1.55% |
| Mg 279.077† | 4779.8 | 5.058 | mg/L | 0.0136 | 101.2 | mg/L | 0.27 | 0.27% |
| Mn 257.610† | 21969.5 | 0.6974 | mg/L | 0.00439 | 13.95 | mg/L | 0.088 | 0.63% |
| Mo 202.031† | 596.6 | 0.03452 | mg/L | 0.000336 | 0.6905 | mg/L | 0.00672 | 0.97% |
| Na 589.592† | 6361.2 | 0.5360 | mg/L | 0.00493 | 10.72 | mg/L | 0.099 | 0.92% |
| Na 330.237† | 23.5 | 0.3125 | mg/L | 0.23749 | 6.251 | mg/L | 4.7497 | 75.98% |
| Ni 231.604† | 476.2 | 0.2941 | mg/L | 0.00077 | 5.883 | mg/L | 0.0153 | 0.26% |
| Pb 220.353† | 1608.5 | 0.1913 | mg/L | 0.00054 | 3.826 | mg/L | 0.0109 | 0.28% |
| Sb 206.836† | 35.6 | 0.00975 | mg/L | 0.000816 | 0.1951 | mg/L | 0.01633 | 8.37% |
| Se 196.026† | 16.1 | 0.01276 | mg/L | 0.009144 | 0.2552 | mg/L | 0.18288 | 71.67% |
| Si 288.158† | 177.6 | 0.1204 | mg/L | 0.00380 | 2.408 | mg/L | 0.0760 | 3.16% |
| Sn 189.927† | 55.4 | 0.01595 | mg/L | 0.000488 | 0.3190 | mg/L | 0.00976 | 3.06% |
| Sr 421.552† | 39067.4 | 0.06178 | mg/L | 0.000544 | 1.236 | mg/L | 0.0109 | 0.88% |
| Ti 334.903† | 18351.1 | 0.8349 | mg/L | 0.00582 | 16.70 | mg/L | 0.116 | 0.70% |
| Tl 190.801† | -11.4 | 0.00401 | mg/L | 0.002340 | 0.08010 | mg/L | 0.046795 | 58.42% |
| V 292.402† | 5329.1 | 0.04857 | mg/L | 0.000285 | 0.9715 | mg/L | 0.00569 | 0.59% |
| Zn 206.200† | 2052.2 | 3.309 | mg/L | 0.0082 | 66.19 | mg/L | 0.164 | 0.25% |

Sequence No.: 32
 Sample ID: DIL
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 329
 Date Collected: 8/6/2010 12:59:03 PM
 Data Type: Original

Nebulizer Parameters: DIL

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: DIL

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. | Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------|-------|----------|---------|
| ScA 357.253 | 1941724.3 | 102.1 | % | 0.41 | | | | 0.40% |
| ScR 361.383 | 301759.1 | 103.1 | % | 0.19 | | | | 0.19% |
| Ag 328.068† | -18.7 | -0.00011 | mg/L | 0.000218 | -0.00011 | mg/L | 0.000218 | 202.54% |
| Al 308.215† | 4.5 | 0.00352 | mg/L | 0.010087 | 0.00352 | mg/L | 0.010087 | 286.95% |
| As 188.979† | 0.3 | 0.00020 | mg/L | 0.000795 | 0.00020 | mg/L | 0.000795 | 390.00% |
| B 249.677† | -12.7 | -0.00385 | mg/L | 0.001251 | -0.00385 | mg/L | 0.001251 | 32.49% |
| Ba 233.527† | 1.3 | 0.00038 | mg/L | 0.000311 | 0.00038 | mg/L | 0.000311 | 81.98% |
| Be 313.042† | -10.2 | -0.00002 | mg/L | 0.000026 | -0.00002 | mg/L | 0.000026 | 141.44% |
| Ca 317.933† | 43.0 | 0.00296 | mg/L | 0.002042 | 0.00296 | mg/L | 0.002042 | 68.90% |
| Cd 228.802† | 0.9 | 0.00004 | mg/L | 0.000132 | 0.00004 | mg/L | 0.000132 | 300.76% |
| Co 228.616† | 3.3 | 0.00011 | mg/L | 0.000058 | 0.00011 | mg/L | 0.000058 | 53.03% |
| Cr 267.716† | 4.3 | 0.00084 | mg/L | 0.000896 | 0.00084 | mg/L | 0.000896 | 106.41% |
| Cu 324.752† | 666.7 | 0.00239 | mg/L | 0.000892 | 0.00239 | mg/L | 0.000892 | 37.31% |
| Fe 273.955† | 7.0 | 0.00613 | mg/L | 0.000321 | 0.00613 | mg/L | 0.000321 | 5.23% |
| K 766.490† | 13.2 | 0.00908 | mg/L | 0.018160 | 0.00908 | mg/L | 0.018160 | 199.89% |
| Mg 279.077† | 1.0 | 0.00111 | mg/L | 0.010984 | 0.00111 | mg/L | 0.010984 | 985.28% |
| Mn 257.610† | 0.8 | 0.00002 | mg/L | 0.000053 | 0.00002 | mg/L | 0.000053 | 216.75% |
| Mo 202.031† | -4.4 | -0.00025 | mg/L | 0.000322 | -0.00025 | mg/L | 0.000322 | 126.26% |
| Na 589.592† | -35.8 | -0.00302 | mg/L | 0.003978 | -0.00302 | mg/L | 0.003978 | 131.83% |
| Na 330.237† | -1.6 | -0.05614 | mg/L | 0.329847 | -0.05614 | mg/L | 0.329847 | 587.51% |
| Ni 231.604† | 3.9 | 0.00243 | mg/L | 0.000641 | 0.00243 | mg/L | 0.000641 | 26.35% |
| Pb 220.353† | -10.3 | -0.00150 | mg/L | 0.000946 | -0.00150 | mg/L | 0.000946 | 63.25% |
| Sb 206.836† | 0.7 | 0.00028 | mg/L | 0.001241 | 0.00028 | mg/L | 0.001241 | 449.34% |
| Se 196.026† | 5.3 | 0.00447 | mg/L | 0.002395 | 0.00447 | mg/L | 0.002395 | 53.57% |
| Si 288.158† | 6.8 | 0.00458 | mg/L | 0.005693 | 0.00458 | mg/L | 0.005693 | 124.18% |
| Sn 189.927† | 4.9 | 0.00133 | mg/L | 0.001107 | 0.00133 | mg/L | 0.001107 | 83.24% |
| Sr 421.552† | 2.6 | 0.00000 | mg/L | 0.000049 | 0.00000 | mg/L | 0.000049 | >999.9% |
| Ti 334.903† | 9.1 | 0.00042 | mg/L | 0.000829 | 0.00042 | mg/L | 0.000829 | 199.37% |
| Tl 190.801† | 0.9 | 0.00053 | mg/L | 0.000554 | 0.00053 | mg/L | 0.000554 | 104.76% |
| V 292.402† | 17.1 | 0.00018 | mg/L | 0.000077 | 0.00018 | mg/L | 0.000077 | 43.36% |
| Zn 206.200† | -0.0 | 0.00000 | mg/L | 0.000342 | 0.00000 | mg/L | 0.000342 | >999.9% |

Sequence No.: 33
Sample ID: RG84 A SWC
Analyst: ALA
Dilution: 20X

DEL

Autosampler Location: 330
Date Collected: 8/6/2010 1:03:13 PM
Data Type: Original

Nebulizer Parameters: RG84 A SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG84 A SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|---------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1962171.8 | 103.2 | % | 0.50 | | | | 0.49% |
| ScR 361.383 | 301260.1 | 102.9 | % | 0.25 | | | | 0.24% |
| Ag 328.068† | 115.5 | 0.00058 | mg/L | 0.000040 | 0.01165 | mg/L | 0.000793 | 6.81% |
| Al 308.215† | 18074.9 | 14.26 | mg/L | 0.108 | 285.2 | mg/L | 2.16 | 0.76% |
| As 188.979† | 25.4 | 0.03054 | mg/L | 0.001890 | 0.6108 | mg/L | 0.03780 | 6.19% |
| B 249.677† | 26.8 | 0.00808 | mg/L | 0.001211 | 0.1615 | mg/L | 0.02423 | 15.00% |
| Ba 233.527† | 477.5 | 0.1379 | mg/L | 0.00028 | 2.759 | mg/L | 0.0057 | 0.21% |
| Be 313.042† | 141.1 | 0.00022 | mg/L | 0.000030 | 0.00443 | mg/L | 0.000610 | 13.75% |
| Ca 317.933† | 138003.7 | 9.504 | mg/L | 0.0363 | 190.1 | mg/L | 0.73 | 0.38% |
| Cd 228.802† | 679.0 | 0.03194 | mg/L | 0.000262 | 0.6387 | mg/L | 0.00525 | 0.82% |
| Co 228.616† | 669.2 | 0.02023 | mg/L | 0.000241 | 0.4047 | mg/L | 0.00481 | 1.19% |
| Cr 267.716† | 2212.8 | 0.4325 | mg/L | 0.00111 | 8.650 | mg/L | 0.0221 | 0.26% |
| Cu 324.752† | 93424.3 | 0.3387 | mg/L | 0.00226 | 6.774 | mg/L | 0.0452 | 0.67% |
| Fe 273.955† | 64541.1 | 56.44 | mg/L | 0.210 | 1129 | mg/L | 4.2 | 0.37% |
| K 766.490† | 1137.0 | 0.7825 | mg/L | 0.00681 | 15.65 | mg/L | 0.136 | 0.87% |
| Mg 279.077† | 4300.5 | 4.553 | mg/L | 0.0237 | 91.06 | mg/L | 0.473 | 0.52% |
| Mn 257.610† | 18760.5 | 0.5956 | mg/L | 0.00225 | 11.91 | mg/L | 0.045 | 0.38% |
| Mo 202.031† | 554.8 | 0.03211 | mg/L | 0.000394 | 0.6422 | mg/L | 0.00788 | 1.23% |
| Na 589.592† | 5496.6 | 0.4632 | mg/L | 0.00188 | 9.264 | mg/L | 0.0376 | 0.41% |
| Na 330.237† | 22.4 | 0.3814 | mg/L | 0.09533 | 7.628 | mg/L | 1.9066 | 24.99% |
| Ni 231.604† | 430.9 | 0.2662 | mg/L | 0.00055 | 5.324 | mg/L | 0.0110 | 0.21% |
| Pb 220.353† | 1242.8 | 0.1791 | mg/L | 0.00069 | 3.582 | mg/L | 0.0137 | 0.38% |
| Sb 206.836† | 33.8 | 0.00947 | mg/L | 0.001252 | 0.1895 | mg/L | 0.02505 | 13.22% |
| Se 196.026† | 10.2 | 0.00789 | mg/L | 0.002607 | 0.1577 | mg/L | 0.05213 | 33.06% |
| Si 288.158† | 150.6 | 0.1021 | mg/L | 0.00088 | 2.042 | mg/L | 0.0177 | 0.87% |
| Sn 189.927† | 88.6 | 0.02488 | mg/L | 0.001482 | 0.4975 | mg/L | 0.02964 | 5.96% |
| Sr 421.552† | 34155.2 | 0.05401 | mg/L | 0.000194 | 1.080 | mg/L | 0.0039 | 0.36% |
| Ti 334.903† | 15689.2 | 0.7138 | mg/L | 0.00235 | 14.28 | mg/L | 0.047 | 0.33% |
| Tl 190.801† | -10.8 | 0.00260 | mg/L | 0.002904 | 0.05194 | mg/L | 0.058076 | 111.82% |
| V 292.402† | 5141.8 | 0.04773 | mg/L | 0.000359 | 0.9546 | mg/L | 0.00717 | 0.75% |
| Zn 206.200† | 1672.0 | 2.696 | mg/L | 0.0196 | 53.93 | mg/L | 0.393 | 0.73% |

Sequence No.: 34
Sample ID: RG84 ASPK SWC
Analyst: ALA
Dilution: 20X

DEL

Autosampler Location: 331
Date Collected: 8/6/2010 1:07:08 PM
Data Type: Original

Nebulizer Parameters: RG84 ASPK SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG84 ASPK SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|---------|--------------|----------|--------|-------|----------|--------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1950212.0 | 102.6 | % | 1.68 | | | | 1.64% |
| ScR 361.383 | 280681.3 | 95.90 | % | 0.196 | | | | 0.20% |
| Ag 328.068† | 8956.2 | 0.05158 | mg/L | 0.000822 | 1.032 | mg/L | 0.0164 | 1.59% |
| Al 308.215† | 22207.1 | 17.52 | mg/L | 0.093 | 350.3 | mg/L | 1.85 | 0.53% |
| As 188.979† | 293.7 | 0.2269 | mg/L | 0.00479 | 4.538 | mg/L | 0.0958 | 2.11% |
| B 249.677† | 41.7 | 0.01244 | mg/L | 0.001994 | 0.2488 | mg/L | 0.03989 | 16.03% |
| Ba 233.527† | 1305.3 | 0.3853 | mg/L | 0.00067 | 7.705 | mg/L | 0.0134 | 0.17% |
| Be 313.042† | 28059.8 | 0.05100 | mg/L | 0.000348 | 1.020 | mg/L | 0.0070 | 0.68% |
| Ca 317.933† | 171729.9 | 11.83 | mg/L | 0.079 | 236.5 | mg/L | 1.58 | 0.67% |
| Cd 228.802† | 1813.3 | 0.08451 | mg/L | 0.001402 | 1.690 | mg/L | 0.0280 | 1.66% |
| Co 228.616† | 2303.5 | 0.07409 | mg/L | 0.001440 | 1.482 | mg/L | 0.0288 | 1.94% |
| Cr 267.716† | 2845.2 | 0.5558 | mg/L | 0.00248 | 11.12 | mg/L | 0.050 | 0.45% |
| Cu 324.752† | 129128.7 | 0.4674 | mg/L | 0.00684 | 9.349 | mg/L | 0.1368 | 1.46% |
| Fe 273.955† | 76263.4 | 66.70 | mg/L | 0.342 | 1334 | mg/L | 6.8 | 0.51% |
| K 766.490† | 2845.5 | 1.958 | mg/L | 0.0137 | 39.16 | mg/L | 0.274 | 0.70% |
| Mg 279.077† | 5976.0 | 6.333 | mg/L | 0.0150 | 126.7 | mg/L | 0.30 | 0.24% |
| Mn 257.610† | 26447.7 | 0.8396 | mg/L | 0.00498 | 16.79 | mg/L | 0.100 | 0.59% |
| Mo 202.031† | 675.2 | 0.03907 | mg/L | 0.001223 | 0.7815 | mg/L | 0.02446 | 3.13% |
| Na 589.592† | 18521.4 | 1.561 | mg/L | 0.0080 | 31.22 | mg/L | 0.161 | 0.52% |
| Na 330.237† | 57.2 | 1.479 | mg/L | 0.1455 | 29.59 | mg/L | 2.910 | 9.83% |
| Ni 231.604† | 602.3 | 0.3720 | mg/L | 0.00096 | 7.440 | mg/L | 0.0192 | 0.26% |
| Pb 220.353† | 2831.8 | 0.4094 | mg/L | 0.00754 | 8.188 | mg/L | 0.1508 | 1.84% |
| Sb 206.836† | 33.2 | 0.00819 | mg/L | 0.001985 | 0.1639 | mg/L | 0.03971 | 24.23% |
| Se 196.026† | 242.6 | 0.2030 | mg/L | 0.00245 | 4.060 | mg/L | 0.0490 | 1.21% |
| Si 288.158† | 183.7 | 0.1247 | mg/L | 0.00672 | 2.494 | mg/L | 0.1344 | 5.39% |
| Sn 189.927† | 63.0 | 0.01807 | mg/L | 0.000280 | 0.3613 | mg/L | 0.00561 | 1.55% |
| Sr 421.552† | 73369.0 | 0.1160 | mg/L | 0.00069 | 2.321 | mg/L | 0.0139 | 0.60% |
| Ti 334.903† | 18172.9 | 0.8267 | mg/L | 0.00205 | 16.53 | mg/L | 0.041 | 0.25% |
| Tl 190.801† | 325.3 | 0.1996 | mg/L | 0.00508 | 3.991 | mg/L | 0.1016 | 2.54% |
| V 292.402† | 9996.8 | 0.09649 | mg/L | 0.001394 | 1.930 | mg/L | 0.0279 | 1.44% |
| Zn 206.200† | 2045.6 | 3.299 | mg/L | 0.0015 | 65.98 | mg/L | 0.031 | 0.05% |

Sequence No.: 35
Sample ID: CV
Analyst: ALA
Dilution: 1X

Autosampler Location: 7
Date Collected: 8/6/2010 1:11:04 PM
Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1957447.6 | 102.9 % | 0.54 | | | 0.52% |
| ScR 361.383 | 279819.4 | 95.61 % | 0.434 | | | 0.45% |
| Ag 328.068† | 182737.1 | 1.055 mg/L | 0.0086 | 1.055 mg/L | 0.0086 | 0.81% |
| Al 308.215† | 2932.8 | 2.281 mg/L | 0.0221 | 2.281 mg/L | 0.0221 | 0.97% |
| As 188.979† | 2929.9 | 2.141 mg/L | 0.0094 | 2.141 mg/L | 0.0094 | 0.44% |
| B 249.677† | 3642.5 | 1.099 mg/L | 0.0085 | 1.099 mg/L | 0.0085 | 0.77% |
| Ba 233.527† | 3554.8 | 1.066 mg/L | 0.0095 | 1.066 mg/L | 0.0095 | 0.90% |
| Be 313.042† | 598145.8 | 1.088 mg/L | 0.0045 | 1.088 mg/L | 0.0045 | 0.41% |
| Ca 317.933† | 33303.2 | 2.294 mg/L | 0.0084 | 2.294 mg/L | 0.0084 | 0.37% |
| Cd 228.802† | 22863.0 | 1.065 mg/L | 0.0088 | 1.065 mg/L | 0.0088 | 0.82% |
| Co 228.616† | 31410.3 | 1.040 mg/L | 0.0064 | 1.040 mg/L | 0.0064 | 0.61% |
| Cr 267.716† | 5532.1 | 1.076 mg/L | 0.0076 | 1.076 mg/L | 0.0076 | 0.71% |
| Cu 324.752† | 292531.9 | 1.048 mg/L | 0.0070 | 1.048 mg/L | 0.0070 | 0.67% |
| Fe 273.955† | 2587.3 | 2.257 mg/L | 0.0106 | 2.257 mg/L | 0.0106 | 0.47% |
| K 766.490† | 32808.6 | 22.58 mg/L | 0.127 | 22.58 mg/L | 0.127 | 0.56% |
| Mg 279.077† | 2131.3 | 2.276 mg/L | 0.0148 | 2.276 mg/L | 0.0148 | 0.65% |
| Mn 257.610† | 32116.3 | 1.020 mg/L | 0.0049 | 1.020 mg/L | 0.0049 | 0.48% |
| Mo 202.031† | 17832.2 | 1.037 mg/L | 0.0045 | 1.037 mg/L | 0.0045 | 0.43% |
| Na 589.592† | 635507.5 | 53.55 mg/L | 0.240 | 53.55 mg/L | 0.240 | 0.45% |
| Na 330.237† | 1666.3 | 57.33 mg/L | 0.209 | 57.33 mg/L | 0.209 | 0.37% |
| Ni 231.604† | 1820.0 | 1.126 mg/L | 0.0098 | 1.126 mg/L | 0.0098 | 0.87% |
| Pb 220.353† | 14593.5 | 2.117 mg/L | 0.0068 | 2.117 mg/L | 0.0068 | 0.32% |
| Sb 206.836† | 5810.9 | 2.171 mg/L | 0.0052 | 2.171 mg/L | 0.0052 | 0.24% |
| Se 196.026† | 2555.2 | 2.146 mg/L | 0.0007 | 2.146 mg/L | 0.0007 | 0.03% |
| Si 288.158† | 3484.1 | 2.363 mg/L | 0.0167 | 2.363 mg/L | 0.0167 | 0.71% |
| Sn 189.927† | 3895.9 | 1.062 mg/L | 0.0039 | 1.062 mg/L | 0.0039 | 0.37% |
| Sr 421.552† | 708433.6 | 1.120 mg/L | 0.0022 | 1.120 mg/L | 0.0022 | 0.19% |
| Ti 334.903† | 24224.2 | 1.102 mg/L | 0.0037 | 1.102 mg/L | 0.0037 | 0.34% |
| Tl 190.801† | 3614.7 | 2.102 mg/L | 0.0083 | 2.102 mg/L | 0.0083 | 0.39% |
| V 292.402† | 102010.2 | 1.042 mg/L | 0.0050 | 1.042 mg/L | 0.0050 | 0.48% |
| Zn 206.200† | 708.4 | 1.142 mg/L | 0.0076 | 1.142 mg/L | 0.0076 | 0.67% |

Sequence No.: 36
 Sample ID: CB
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 1:15:17 PM
 Data Type: Original

Nebulizer Parameters: CB

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 201.0 kPa | 0.75 L/min |

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1933164.1 | 101.7 | % | 0.47 | | | 0.46% |
| ScR 361.383 | 298093.0 | 101.8 | % | 1.07 | | | 1.05% |
| Ag 328.068† | -47.1 | -0.00027 | mg/L | 0.000241 | -0.00027 mg/L | 0.000241 | 88.43% |
| Al 308.215† | -4.5 | -0.00354 | mg/L | 0.007758 | -0.00354 mg/L | 0.007758 | 219.32% |
| As 188.979† | 2.8 | 0.00201 | mg/L | 0.000846 | 0.00201 mg/L | 0.000846 | 42.17% |
| B 249.677† | -2.3 | -0.00070 | mg/L | 0.001169 | -0.00070 mg/L | 0.001169 | 167.83% |
| Ba 233.527† | 0.2 | 0.00005 | mg/L | 0.000860 | 0.00005 mg/L | 0.000860 | >999.9% |
| Be 313.042† | 44.9 | 0.00008 | mg/L | 0.000069 | 0.00008 mg/L | 0.000069 | 84.36% |
| Ca 317.933† | 3.6 | 0.00025 | mg/L | 0.000311 | 0.00025 mg/L | 0.000311 | 123.74% |
| Cd 228.802† | -0.2 | -0.00001 | mg/L | 0.000129 | -0.00001 mg/L | 0.000129 | 891.87% |
| Co 228.616† | 1.2 | 0.00004 | mg/L | 0.000179 | 0.00004 mg/L | 0.000179 | 451.45% |
| Cr 267.716† | 2.1 | 0.00040 | mg/L | 0.000978 | 0.00040 mg/L | 0.000978 | 242.98% |
| Cu 324.752† | 288.8 | 0.00104 | mg/L | 0.000110 | 0.00104 mg/L | 0.000110 | 10.57% |
| Fe 273.955† | 2.1 | 0.00185 | mg/L | 0.000772 | 0.00185 mg/L | 0.000772 | 41.75% |
| K 766.490† | -1.6 | -0.00108 | mg/L | 0.011203 | -0.00108 mg/L | 0.011203 | >999.9% |
| Mg 279.077† | 5.7 | 0.00608 | mg/L | 0.003921 | 0.00608 mg/L | 0.003921 | 64.46% |
| Mn 257.610† | 2.0 | 0.00006 | mg/L | 0.000121 | 0.00006 mg/L | 0.000121 | 189.06% |
| Mo 202.031† | 3.7 | 0.00022 | mg/L | 0.000185 | 0.00022 mg/L | 0.000185 | 85.12% |
| Na 589.592† | 60.8 | 0.00512 | mg/L | 0.005848 | 0.00512 mg/L | 0.005848 | 114.15% |
| Na 330.237† | 10.7 | 0.3683 | mg/L | 0.57800 | 0.3683 mg/L | 0.57800 | 156.94% |
| Ni 231.604† | 4.5 | 0.00279 | mg/L | 0.001834 | 0.00279 mg/L | 0.001834 | 65.68% |
| Pb 220.353† | -7.5 | -0.00109 | mg/L | 0.000947 | -0.00109 mg/L | 0.000947 | 87.13% |
| Sb 206.836† | 7.3 | 0.00271 | mg/L | 0.002238 | 0.00271 mg/L | 0.002238 | 82.55% |
| Se 196.026† | 5.0 | 0.00423 | mg/L | 0.003564 | 0.00423 mg/L | 0.003564 | 84.31% |
| Si 288.158† | 13.1 | 0.00887 | mg/L | 0.002571 | 0.00887 mg/L | 0.002571 | 28.98% |
| Sn 189.927† | 1.8 | 0.00050 | mg/L | 0.000693 | 0.00050 mg/L | 0.000693 | 139.66% |
| Sr 421.552† | 26.2 | 0.00004 | mg/L | 0.000067 | 0.00004 mg/L | 0.000067 | 162.79% |
| Ti 334.903† | 2.3 | 0.00011 | mg/L | 0.000727 | 0.00011 mg/L | 0.000727 | 688.12% |
| Tl 190.801† | -1.3 | -0.00077 | mg/L | 0.002644 | -0.00077 mg/L | 0.002644 | 342.04% |
| V 292.402† | -8.9 | -0.00009 | mg/L | 0.000257 | -0.00009 mg/L | 0.000257 | 288.58% |
| Zn 206.200† | -0.0 | -0.00002 | mg/L | 0.002701 | -0.00002 mg/L | 0.002701 | >999.9% |

Sequence No.: 37
Sample ID: RG83 MB LEN
Analyst: ALA
Dilution: 5X

Autosampler Location: 332
Date Collected: 8/6/2010 1:19:28 PM
Data Type: Original

Nebulizer Parameters: RG83 MB LEN

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG83 MB LEN

Table with 9 columns: Analyte, Mean Corrected Intensity, Calib. Conc. Units, Std.Dev., Sample Conc. Units, Std.Dev., RSD. Lists various elements like ScA, ScR, Ag, Al, As, B, Ba, Be, Ca, Cd, Co, Cr, Cu, Fe, K, Mg, Mn, Mo, Na, Ni, Pb, Sb, Se, Si, Sn, Sr, Ti, Tl, V, Zn with their respective intensity, concentration, and RSD values.

Sequence No.: 38
 Sample ID: RG83 ADUP LEN
 Analyst: ALA
 Dilution: 5X

Autosampler Location: 333
 Date Collected: 8/6/2010 1:23:41 PM
 Data Type: Original

Nebulizer Parameters: RG83 ADUP LEN

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG83 ADUP LEN

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1882751.0 | 99.00 % | 1.087 | | | 1.10% |
| ScR 361.383 | 290717.3 | 99.33 % | 0.732 | | | 0.74% |
| Ag 328.068† | 49.7 | -0.00005 mg/L | 0.000331 | -0.00025 mg/L | 0.001657 | 664.59% |
| Al 308.215† | 175.5 | 0.1384 mg/L | 0.00129 | 0.6920 mg/L | 0.00643 | 0.93% |
| As 188.979† | 11.4 | 0.00628 mg/L | 0.002026 | 0.03141 mg/L | 0.010129 | 32.25% |
| B 249.677† | 223.6 | 0.06753 mg/L | 0.000492 | 0.3377 mg/L | 0.00246 | 0.73% |
| Ba 233.527† | 1131.7 | 0.3389 mg/L | 0.00328 | 1.694 mg/L | 0.0164 | 0.97% |
| Be 313.042† | 80.9 | 0.00015 mg/L | 0.000009 | 0.00074 mg/L | 0.000044 | 5.94% |
| Ca 317.933† | 994249.4 | 68.47 mg/L | 0.706 | 342.4 mg/L | 3.53 | 1.03% |
| Cd 228.802† | 1463.6 | 0.06864 mg/L | 0.000808 | 0.3432 mg/L | 0.00404 | 1.18% |
| Co 228.616† | 325.3 | 0.01071 mg/L | 0.000155 | 0.05354 mg/L | 0.000774 | 1.45% |
| Cr 267.716† | 16.0 | 0.00118 mg/L | 0.000931 | 0.00592 mg/L | 0.004654 | 78.56% |
| Cu 324.752† | 221136.7 | 0.7929 mg/L | 0.00381 | 3.965 mg/L | 0.0190 | 0.48% |
| Fe 273.955† | 70.7 | 0.06181 mg/L | 0.000935 | 0.3091 mg/L | 0.00467 | 1.51% |
| K 766.490† | 5659.4 | 3.894 mg/L | 0.0412 | 19.47 mg/L | 0.206 | 1.06% |
| Mg 279.077† | 4346.8 | 4.623 mg/L | 0.0396 | 23.11 mg/L | 0.198 | 0.86% |
| Mn 257.610† | 53984.2 | 1.713 mg/L | 0.0167 | 8.565 mg/L | 0.0833 | 0.97% |
| Mo 202.031† | 72.2 | 0.00302 mg/L | 0.000232 | 0.01508 mg/L | 0.001162 | 7.71% |
| Na 589.592† | 3448448.0 | 290.6 mg/L | 2.88 | 1453 mg/L | 14.4 | 0.99% |
| Na 330.237† | 8744.5 | 300.4 mg/L | 5.31 | 1502 mg/L | 26.5 | 1.77% |
| Ni 231.604† | 150.7 | 0.09308 mg/L | 0.001757 | 0.4654 mg/L | 0.00878 | 1.89% |
| Pb 220.353† | 2735.8 | 0.3957 mg/L | 0.00393 | 1.978 mg/L | 0.0197 | 0.99% |
| Sb 206.836† | 12.8 | 0.00466 mg/L | 0.000464 | 0.02330 mg/L | 0.002318 | 9.95% |
| Se 196.026† | 38.4 | 0.02762 mg/L | 0.000839 | 0.1381 mg/L | 0.00419 | 3.04% |
| Si 288.158† | 2249.9 | 1.524 mg/L | 0.0316 | 7.619 mg/L | 0.1582 | 2.08% |
| Sn 189.927† | -42.0 | -0.00824 mg/L | 0.001003 | -0.04119 mg/L | 0.005016 | 12.18% |
| Sr 421.552† | 103446.5 | 0.1636 mg/L | 0.00209 | 0.8179 mg/L | 0.01045 | 1.28% |
| Ti 334.903† | 103.8 | 0.00045 mg/L | 0.000157 | 0.00226 mg/L | 0.000787 | 34.75% |
| Tl 190.801† | 16.3 | 0.01109 mg/L | 0.003238 | 0.05546 mg/L | 0.016189 | 29.19% |
| V 292.402† | -18.4 | 0.00008 mg/L | 0.000182 | 0.00041 mg/L | 0.000909 | 223.86% |
| Zn 206.200† | 1546.6 | 2.495 mg/L | 0.0184 | 12.47 mg/L | 0.092 | 0.74% |

Sequence No.: 39
 Sample ID: RG83 A LEN
 Analyst: ALA
 Dilution: 5X

Autosampler Location: 334
 Date Collected: 8/6/2010 1:27:54 PM
 Data Type: Original

Nebulizer Parameters: RG83 A LEN

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG83 A LEN

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1882427.8 | 98.99 | % | 0.333 | | | 0.34% |
| ScR 361.383 | 288335.4 | 98.51 | % | 1.608 | | | 1.63% |
| Ag 328.068† | 38.6 | -0.00011 | mg/L | 0.000294 | -0.00057 mg/L | 0.001468 | 255.79% |
| Al 308.215† | 175.8 | 0.1387 | mg/L | 0.00094 | 0.6934 mg/L | 0.00470 | 0.68% |
| As 188.979† | 13.1 | 0.00748 | mg/L | 0.003859 | 0.03740 mg/L | 0.019293 | 51.58% |
| B 249.677† | 224.0 | 0.06766 | mg/L | 0.002805 | 0.3383 mg/L | 0.01403 | 4.15% |
| Ba 233.527† | 1129.8 | 0.3383 | mg/L | 0.00526 | 1.691 mg/L | 0.0263 | 1.55% |
| Be 313.042† | 78.0 | 0.00014 | mg/L | 0.000027 | 0.00071 mg/L | 0.000133 | 18.74% |
| Ca 317.933† | 999440.9 | 68.83 | mg/L | 1.146 | 344.2 mg/L | 5.73 | 1.67% |
| Cd 228.802† | 1466.4 | 0.06877 | mg/L | 0.000815 | 0.3438 mg/L | 0.00408 | 1.19% |
| Co 228.616† | 329.7 | 0.01086 | mg/L | 0.000084 | 0.05428 mg/L | 0.000422 | 0.78% |
| Cr 267.716† | 13.4 | 0.00068 | mg/L | 0.000525 | 0.00338 mg/L | 0.002623 | 77.55% |
| Cu 324.752† | 220098.7 | 0.7892 | mg/L | 0.00531 | 3.946 mg/L | 0.0265 | 0.67% |
| Fe 273.955† | 71.9 | 0.06289 | mg/L | 0.002212 | 0.3144 mg/L | 0.01106 | 3.52% |
| K 766.490† | 5658.7 | 3.894 | mg/L | 0.1245 | 19.47 mg/L | 0.623 | 3.20% |
| Mg 279.077† | 4352.0 | 4.628 | mg/L | 0.0884 | 23.14 mg/L | 0.442 | 1.91% |
| Mn 257.610† | 54137.1 | 1.718 | mg/L | 0.0313 | 8.590 mg/L | 0.1565 | 1.82% |
| Mo 202.031† | 72.6 | 0.00303 | mg/L | 0.000458 | 0.01516 mg/L | 0.002292 | 15.12% |
| Na 589.592† | 3442564.7 | 290.1 | mg/L | 4.42 | 1450 mg/L | 22.1 | 1.52% |
| Na 330.237† | 8773.3 | 301.4 | mg/L | 3.67 | 1507 mg/L | 18.4 | 1.22% |
| Ni 231.604† | 149.0 | 0.09201 | mg/L | 0.002551 | 0.4601 mg/L | 0.01276 | 2.77% |
| Pb 220.353† | 2744.3 | 0.3969 | mg/L | 0.00207 | 1.985 mg/L | 0.0104 | 0.52% |
| Sb 206.836† | 12.5 | 0.00454 | mg/L | 0.000449 | 0.02272 mg/L | 0.002244 | 9.88% |
| Se 196.026† | 38.0 | 0.02725 | mg/L | 0.006303 | 0.1363 mg/L | 0.03151 | 23.13% |
| Si 288.158† | 2348.2 | 1.590 | mg/L | 0.0075 | 7.952 mg/L | 0.0376 | 0.47% |
| Sn 189.927† | -40.2 | -0.00773 | mg/L | 0.000134 | -0.03867 mg/L | 0.000670 | 1.73% |
| Sr 421.552† | 103937.3 | 0.1644 | mg/L | 0.00279 | 0.8218 mg/L | 0.01393 | 1.69% |
| Ti 334.903† | 101.6 | 0.00033 | mg/L | 0.000386 | 0.00166 mg/L | 0.001929 | 116.20% |
| Tl 190.801† | 21.4 | 0.01409 | mg/L | 0.002590 | 0.07043 mg/L | 0.012948 | 18.38% |
| V 292.402† | -16.8 | 0.00010 | mg/L | 0.000038 | 0.00048 mg/L | 0.000188 | 39.32% |
| Zn 206.200† | 1546.7 | 2.495 | mg/L | 0.0431 | 12.47 mg/L | 0.215 | 1.73% |

Sequence No.: 40
 Sample ID: RG83 ASPK LEN
 Analyst: ALA
 Dilution: 5X

Autosampler Location: 335
 Date Collected: 8/6/2010 1:32:07 PM
 Data Type: Original

Nebulizer Parameters: RG83 ASPK LEN

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG83 ASPK LEN

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| SCA 357.253 | 1871754.1 | 98.43 | % | 0.711 | | | 0.72% |
| SCR 361.383 | 286845.7 | 98.01 | % | 1.373 | | | 1.40% |
| Ag 328.068† | 35218.4 | 0.2030 | mg/L | 0.00120 | 1.015 mg/L | 0.0060 | 0.59% |
| Al 308.215† | 1288.2 | 1.012 | mg/L | 0.0115 | 5.062 mg/L | 0.0576 | 1.14% |
| As 188.979† | 1228.7 | 0.8883 | mg/L | 0.00991 | 4.441 mg/L | 0.0496 | 1.12% |
| B 249.677† | 224.4 | 0.06725 | mg/L | 0.001814 | 0.3362 mg/L | 0.00907 | 2.70% |
| Ba 233.527† | 3821.6 | 1.146 | mg/L | 0.0144 | 5.728 mg/L | 0.0722 | 1.26% |
| Be 313.042† | 115132.0 | 0.2094 | mg/L | 0.00320 | 1.047 mg/L | 0.0160 | 1.53% |
| Ca 317.933† | 1061669.3 | 73.12 | mg/L | 1.121 | 365.6 mg/L | 5.60 | 1.53% |
| Cd 228.802† | 6223.7 | 0.2889 | mg/L | 0.00172 | 1.445 mg/L | 0.0086 | 0.59% |
| Co 228.616† | 6593.6 | 0.2185 | mg/L | 0.00090 | 1.093 mg/L | 0.0045 | 0.41% |
| Cr 267.716† | 1039.8 | 0.1998 | mg/L | 0.00195 | 0.9989 mg/L | 0.00973 | 0.97% |
| Cu 324.752† | 288882.4 | 1.036 | mg/L | 0.0048 | 5.180 mg/L | 0.0240 | 0.46% |
| Fe 273.955† | 1057.7 | 0.9239 | mg/L | 0.01206 | 4.619 mg/L | 0.0603 | 1.31% |
| K 766.490† | 12010.6 | 8.265 | mg/L | 0.1427 | 41.33 mg/L | 0.714 | 1.73% |
| Mg 279.077† | 8461.8 | 9.007 | mg/L | 0.1187 | 45.03 mg/L | 0.593 | 1.32% |
| Mn 257.610† | 60714.2 | 1.927 | mg/L | 0.0300 | 9.634 mg/L | 0.1502 | 1.56% |
| Mo 202.031† | 76.2 | 0.00316 | mg/L | 0.000399 | 0.01582 mg/L | 0.001993 | 12.60% |
| Na 589.592† | 3507979.7 | 295.6 | mg/L | 3.94 | 1478 mg/L | 19.7 | 1.33% |
| Na 330.237† | 8935.2 | 307.0 | mg/L | 3.40 | 1535 mg/L | 17.0 | 1.11% |
| Ni 231.604† | 487.3 | 0.3010 | mg/L | 0.00156 | 1.505 mg/L | 0.0078 | 0.52% |
| Pb 220.353† | 8590.5 | 1.245 | mg/L | 0.0103 | 6.224 mg/L | 0.0517 | 0.83% |
| Sb 206.836† | 19.7 | 0.00583 | mg/L | 0.002538 | 0.02917 mg/L | 0.012688 | 43.49% |
| Se 196.026† | 1094.8 | 0.9146 | mg/L | 0.00572 | 4.573 mg/L | 0.0286 | 0.63% |
| Si 288.158† | 2439.6 | 1.653 | mg/L | 0.0170 | 8.265 mg/L | 0.0850 | 1.03% |
| Sn 189.927† | -39.2 | -0.00728 | mg/L | 0.001234 | -0.03641 mg/L | 0.006168 | 16.94% |
| Sr 421.552† | 239641.9 | 0.3790 | mg/L | 0.00649 | 1.895 mg/L | 0.0324 | 1.71% |
| Ti 334.903† | 114.1 | 0.00060 | mg/L | 0.000600 | 0.00298 mg/L | 0.003000 | 100.76% |
| Tl 190.801† | 1447.9 | 0.8429 | mg/L | 0.00965 | 4.215 mg/L | 0.0483 | 1.15% |
| V 292.402† | 20345.5 | 0.2079 | mg/L | 0.00078 | 1.040 mg/L | 0.0039 | 0.37% |
| Zn 206.200† | 1670.6 | 2.695 | mg/L | 0.0439 | 13.47 mg/L | 0.220 | 1.63% |

Sequence No.: 41
 Sample ID: RG54 K SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 336
 Date Collected: 8/6/2010 1:36:20 PM
 Data Type: Original

Nebulizer Parameters: RG54 K SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG54 K SWC

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1973145.2 | 103.8 % | 1.00 | | | 0.96% |
| ScR 361.383 | 309877.1 | 105.9 % | 1.07 | | | 1.01% |
| Ag 328.068† | -194.2 | -0.00117 mg/L | 0.000057 | -0.00234 mg/L | 0.000114 | 4.89% |
| Al 308.215† | 244318.3 | 192.7 mg/L | 2.09 | 385.5 mg/L | 4.17 | 1.08% |
| As 188.979† | -264.8 | -0.00255 mg/L | 0.007005 | -0.00511 mg/L | 0.014011 | 274.36% |
| B 249.677† | 26.5 | 0.00777 mg/L | 0.002450 | 0.01555 mg/L | 0.004899 | 31.51% |
| Ba 233.527† | 2246.1 | 0.6556 mg/L | 0.00819 | 1.311 mg/L | 0.0164 | 1.25% |
| Be 313.042† | 1358.0 | 0.00210 mg/L | 0.000054 | 0.00420 mg/L | 0.000108 | 2.57% |
| Ca 317.933† | 594221.3 | 40.92 mg/L | 0.524 | 81.85 mg/L | 1.048 | 1.28% |
| Cd 228.802† | 40.4 | 0.00276 mg/L | 0.000249 | 0.00552 mg/L | 0.000498 | 9.02% |
| Co 228.616† | 2865.5 | 0.07475 mg/L | 0.001023 | 0.1495 mg/L | 0.00205 | 1.37% |
| Cr 267.716† | 1669.3 | 0.3257 mg/L | 0.00194 | 0.6513 mg/L | 0.00389 | 0.60% |
| Cu 324.752† | 44150.4 | 0.1669 mg/L | 0.00218 | 0.3337 mg/L | 0.00437 | 1.31% |
| Fe 273.955† | 218225.9 | 190.8 mg/L | 2.35 | 381.7 mg/L | 4.69 | 1.23% |
| K 766.490† | 10812.4 | 7.441 mg/L | 0.1141 | 14.88 mg/L | 0.228 | 1.53% |
| Mg 279.077† | 52457.7 | 55.79 mg/L | 0.734 | 111.6 mg/L | 1.47 | 1.31% |
| Mn 257.610† | 84670.7 | 2.687 mg/L | 0.0386 | 5.373 mg/L | 0.0772 | 1.44% |
| Mo 202.031† | 133.8 | 0.00707 mg/L | 0.000051 | 0.01414 mg/L | 0.000101 | 0.72% |
| Na 589.592† | 24182.3 | 2.038 mg/L | 0.0230 | 4.076 mg/L | 0.0460 | 1.13% |
| Na 330.237† | -28.1 | 2.110 mg/L | 0.1689 | 4.221 mg/L | 0.3378 | 8.00% |
| Ni 231.604† | 564.6 | 0.3487 mg/L | 0.00380 | 0.6975 mg/L | 0.00761 | 1.09% |
| Pb 220.353† | -13.6 | 0.01776 mg/L | 0.000837 | 0.03552 mg/L | 0.001675 | 4.71% |
| Sb 206.836† | 29.2 | 0.02246 mg/L | 0.002471 | 0.04493 mg/L | 0.004941 | 11.00% |
| Se 196.026† | 47.5 | 0.03712 mg/L | 0.000275 | 0.07423 mg/L | 0.000551 | 0.74% |
| Si 288.158† | 8681.6 | 5.879 mg/L | 0.0718 | 11.76 mg/L | 0.144 | 1.22% |
| Sn 189.927† | -47.3 | -0.00614 mg/L | 0.000966 | -0.01227 mg/L | 0.001932 | 15.74% |
| Sr 421.552† | 176016.1 | 0.2784 mg/L | 0.00345 | 0.5567 mg/L | 0.00689 | 1.24% |
| Ti 334.903† | 231642.5 | 10.55 mg/L | 0.130 | 21.09 mg/L | 0.260 | 1.23% |
| Tl 190.801† | -40.5 | 0.00672 mg/L | 0.003270 | 0.01343 mg/L | 0.006539 | 48.68% |
| V 292.402† | 47645.7 | 0.4597 mg/L | 0.00833 | 0.9194 mg/L | 0.01666 | 1.81% |
| Zn 206.200† | 202.0 | 0.3203 mg/L | 0.00537 | 0.6407 mg/L | 0.01074 | 1.68% |

Sequence No.: 42
 Sample ID: RG54 L SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 337
 Date Collected: 8/6/2010 1:40:02 PM
 Data Type: Original

Nebulizer Parameters: RG54 L SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG54 L SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1959946.8 | 103.1 | % | 0.67 | | | 0.65% |
| ScR 361.383 | 305557.1 | 104.4 | % | 2.06 | | | 1.97% |
| Ag 328.068† | -135.7 | -0.00096 | mg/L | 0.000119 | -0.00192 mg/L | 0.000237 | 12.38% |
| Al 308.215† | 144242.5 | 113.8 | mg/L | 2.24 | 227.6 mg/L | 4.49 | 1.97% |
| As 188.979† | -215.7 | 0.00393 | mg/L | 0.004534 | 0.00787 mg/L | 0.009067 | 115.27% |
| B 249.677† | 37.9 | 0.01124 | mg/L | 0.000908 | 0.02248 mg/L | 0.001817 | 8.08% |
| Ba 233.527† | 1696.4 | 0.4930 | mg/L | 0.01031 | 0.9859 mg/L | 0.02062 | 2.09% |
| Be 313.042† | 993.9 | 0.00149 | mg/L | 0.000084 | 0.00298 mg/L | 0.000168 | 5.66% |
| Ca 317.933† | 859841.4 | 59.22 | mg/L | 1.264 | 118.4 mg/L | 2.53 | 2.13% |
| Cd 228.802† | 49.0 | 0.00308 | mg/L | 0.000050 | 0.00616 mg/L | 0.000099 | 1.61% |
| Co 228.616† | 2718.8 | 0.07288 | mg/L | 0.000667 | 0.1458 mg/L | 0.00133 | 0.91% |
| Cr 267.716† | 1529.9 | 0.2965 | mg/L | 0.00590 | 0.5931 mg/L | 0.01179 | 1.99% |
| Cu 324.752† | 33503.7 | 0.1273 | mg/L | 0.00090 | 0.2547 mg/L | 0.00180 | 0.70% |
| Fe 273.955† | 188748.7 | 165.1 | mg/L | 3.06 | 330.1 mg/L | 6.12 | 1.85% |
| K 766.490† | 10729.5 | 7.384 | mg/L | 0.1049 | 14.77 mg/L | 0.210 | 1.42% |
| Mg 279.077† | 55666.9 | 59.22 | mg/L | 1.060 | 118.4 mg/L | 2.12 | 1.79% |
| Mn 257.610† | 93698.3 | 2.973 | mg/L | 0.0699 | 5.947 mg/L | 0.1398 | 2.35% |
| Mo 202.031† | 96.2 | 0.00457 | mg/L | 0.000259 | 0.00914 mg/L | 0.000517 | 5.66% |
| Na 589.592† | 42116.1 | 3.549 | mg/L | 0.0710 | 7.098 mg/L | 0.1420 | 2.00% |
| Na 330.237† | 29.9 | 3.784 | mg/L | 0.3565 | 7.568 mg/L | 0.7130 | 9.42% |
| Ni 231.604† | 658.4 | 0.4066 | mg/L | 0.01196 | 0.8133 mg/L | 0.02391 | 2.94% |
| Pb 220.353† | 35.3 | 0.01327 | mg/L | 0.001704 | 0.02654 mg/L | 0.003409 | 12.85% |
| Sb 206.836† | 20.6 | 0.01736 | mg/L | 0.002733 | 0.03472 mg/L | 0.005465 | 15.74% |
| Se 196.026† | 45.9 | 0.03457 | mg/L | 0.002300 | 0.06914 mg/L | 0.004600 | 6.65% |
| Si 288.158† | 6197.1 | 4.196 | mg/L | 0.0745 | 8.393 mg/L | 0.1489 | 1.77% |
| Sn 189.927† | -46.6 | -0.00582 | mg/L | 0.000279 | -0.01164 mg/L | 0.000558 | 4.80% |
| Sr 421.552† | 234289.5 | 0.3705 | mg/L | 0.00611 | 0.7410 mg/L | 0.01223 | 1.65% |
| Ti 334.903† | 196984.8 | 8.967 | mg/L | 0.1691 | 17.93 mg/L | 0.338 | 1.89% |
| Tl 190.801† | -27.9 | 0.01053 | mg/L | 0.001496 | 0.02106 mg/L | 0.002991 | 14.20% |
| V 292.402† | 41556.5 | 0.4014 | mg/L | 0.00107 | 0.8027 mg/L | 0.00214 | 0.27% |
| Zn 206.200† | 189.9 | 0.3031 | mg/L | 0.00644 | 0.6062 mg/L | 0.01289 | 2.13% |

Sequence No.: 43
Sample ID: CV 7
Analyst: ALA
Dilution: 1x

Autosampler Location: 7
Date Collected: 8/6/2010 1:44:00 PM
Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1954719.7 | 102.8 % | 0.44 | | | 0.43% |
| ScR 361.383 | 299087.4 | 102.2 % | 0.43 | | | 0.78% |
| Ag 328.068† | 184664.4 | 1.066 mg/L | 0.0084 | 1.066 mg/L | 0.0084 | 0.78% |
| Al 308.215† | 2793.6 | 2.171 mg/L | 0.0124 | 2.171 mg/L | 0.0124 | 0.57% |
| As 188.979† | 2967.0 | 2.167 mg/L | 0.0035 | 2.167 mg/L | 0.0035 | 0.16% |
| B 249.677† | 3428.6 | 1.034 mg/L | 0.0050 | 1.034 mg/L | 0.0050 | 0.48% |
| Ba 233.527† | 3342.7 | 1.002 mg/L | 0.0045 | 1.002 mg/L | 0.0045 | 0.45% |
| Be 313.042† | 563352.2 | 1.025 mg/L | 0.0075 | 1.025 mg/L | 0.0075 | 0.73% |
| Ca 317.933† | 31724.5 | 2.185 mg/L | 0.0025 | 2.185 mg/L | 0.0025 | 0.12% |
| Cd 228.802† | 23169.3 | 1.079 mg/L | 0.0044 | 1.079 mg/L | 0.0044 | 0.41% |
| Co 228.616† | 31913.6 | 1.057 mg/L | 0.0049 | 1.057 mg/L | 0.0049 | 0.46% |
| Cr 267.716† | 5232.7 | 1.018 mg/L | 0.0057 | 1.018 mg/L | 0.0057 | 0.56% |
| Cu 324.752† | 295258.4 | 1.058 mg/L | 0.0066 | 1.058 mg/L | 0.0066 | 0.62% |
| Fe 273.955† | 2461.2 | 2.147 mg/L | 0.0076 | 2.147 mg/L | 0.0076 | 0.36% |
| K 766.490† | 31295.4 | 21.54 mg/L | 0.086 | 21.54 mg/L | 0.086 | 0.40% |
| Mg 279.077† | 2021.6 | 2.159 mg/L | 0.0069 | 2.159 mg/L | 0.0069 | 0.32% |
| Mn 257.610† | 30470.2 | 0.9675 mg/L | 0.00241 | 0.9675 mg/L | 0.00241 | 0.25% |
| Mo 202.031† | 17958.3 | 1.045 mg/L | 0.0038 | 1.045 mg/L | 0.0038 | 0.37% |
| Na 589.592† | 597395.7 | 50.34 mg/L | 0.330 | 50.34 mg/L | 0.330 | 0.66% |
| Na 330.237† | 1575.4 | 54.20 mg/L | 0.218 | 54.20 mg/L | 0.218 | 0.40% |
| Ni 231.604† | 1716.9 | 1.062 mg/L | 0.0057 | 1.062 mg/L | 0.0057 | 0.54% |
| Pb 220.353† | 14763.6 | 2.142 mg/L | 0.0066 | 2.142 mg/L | 0.0066 | 0.31% |
| Sb 206.836† | 5867.6 | 2.192 mg/L | 0.0089 | 2.192 mg/L | 0.0089 | 0.41% |
| Se 196.026† | 2584.8 | 2.171 mg/L | 0.0144 | 2.171 mg/L | 0.0144 | 0.66% |
| Si 288.158† | 3299.2 | 2.238 mg/L | 0.0120 | 2.238 mg/L | 0.0120 | 0.53% |
| Sn 189.927† | 3935.6 | 1.072 mg/L | 0.0064 | 1.072 mg/L | 0.0064 | 0.59% |
| Sr 421.552† | 671040.1 | 1.061 mg/L | 0.0048 | 1.061 mg/L | 0.0048 | 0.46% |
| Ti 334.903† | 23058.0 | 1.048 mg/L | 0.0005 | 1.048 mg/L | 0.0005 | 0.05% |
| Tl 190.801† | 3656.6 | 2.126 mg/L | 0.0095 | 2.126 mg/L | 0.0095 | 0.45% |
| V 292.402† | 103182.3 | 1.054 mg/L | 0.0040 | 1.054 mg/L | 0.0040 | 0.38% |
| Zn 206.200† | 664.0 | 1.070 mg/L | 0.0054 | 1.070 mg/L | 0.0054 | 0.50% |

Sequence No.: 44
 Sample ID: CB 7
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 1:48:14 PM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1965201.6 | 103.3 | % | 0.56 | | | 0.54% |
| ScR 361.383 | 277407.8 | 94.78 | % | 2.560 | | | 2.70% |
| Ag 328.068† | 9.5 | 0.00006 | mg/L | 0.000171 | 0.00006 mg/L | 0.000171 | 310.61% |
| Al 308.215† | 4.3 | 0.00339 | mg/L | 0.002702 | 0.00339 mg/L | 0.002702 | 79.71% |
| As 188.979† | 2.2 | 0.00161 | mg/L | 0.001778 | 0.00161 mg/L | 0.001778 | 110.35% |
| B 249.677† | -6.9 | -0.00208 | mg/L | 0.000991 | -0.00208 mg/L | 0.000991 | 47.71% |
| Ba 233.527† | 6.4 | 0.00193 | mg/L | 0.000783 | 0.00193 mg/L | 0.000783 | 40.51% |
| Be 313.042† | 88.9 | 0.00016 | mg/L | 0.000089 | 0.00016 mg/L | 0.000089 | 55.12% |
| Ca 317.933† | 4.8 | 0.00033 | mg/L | 0.000303 | 0.00033 mg/L | 0.000303 | 91.71% |
| Cd 228.802† | -3.2 | -0.00015 | mg/L | 0.000112 | -0.00015 mg/L | 0.000112 | 72.43% |
| Co 228.616† | 1.3 | 0.00004 | mg/L | 0.000370 | 0.00004 mg/L | 0.000370 | 895.00% |
| Cr 267.716† | -9.0 | -0.00176 | mg/L | 0.000737 | -0.00176 mg/L | 0.000737 | 41.86% |
| Cu 324.752† | 299.1 | 0.00107 | mg/L | 0.000240 | 0.00107 mg/L | 0.000240 | 22.41% |
| Fe 273.955† | 3.9 | 0.00345 | mg/L | 0.004478 | 0.00345 mg/L | 0.004478 | 129.89% |
| K 766.490† | 64.3 | 0.04422 | mg/L | 0.030457 | 0.04422 mg/L | 0.030457 | 68.87% |
| Mg 279.077† | 3.6 | 0.00386 | mg/L | 0.003535 | 0.00386 mg/L | 0.003535 | 91.52% |
| Mn 257.610† | 1.3 | 0.00004 | mg/L | 0.000082 | 0.00004 mg/L | 0.000082 | 198.93% |
| Mo 202.031† | 1.4 | 0.00008 | mg/L | 0.000218 | 0.00008 mg/L | 0.000218 | 267.40% |
| Na 589.592† | 231.5 | 0.01950 | mg/L | 0.001391 | 0.01950 mg/L | 0.001391 | 7.13% |
| Na 330.237† | -12.1 | -0.4176 | mg/L | 0.64153 | -0.4176 mg/L | 0.64153 | 153.61% |
| Ni 231.604† | 5.0 | 0.00311 | mg/L | 0.000803 | 0.00311 mg/L | 0.000803 | 25.84% |
| Pb 220.353† | -5.0 | -0.00073 | mg/L | 0.001208 | -0.00073 mg/L | 0.001208 | 166.14% |
| Sb 206.836† | 10.5 | 0.00393 | mg/L | 0.000878 | 0.00393 mg/L | 0.000878 | 22.32% |
| Se 196.026† | 10.2 | 0.00853 | mg/L | 0.005833 | 0.00853 mg/L | 0.005833 | 68.42% |
| Si 288.158† | 19.9 | 0.01349 | mg/L | 0.002696 | 0.01349 mg/L | 0.002696 | 19.99% |
| Sn 189.927† | 2.6 | 0.00071 | mg/L | 0.000573 | 0.00071 mg/L | 0.000573 | 80.34% |
| Sr 421.552† | 85.7 | 0.00014 | mg/L | 0.000062 | 0.00014 mg/L | 0.000062 | 45.49% |
| Ti 334.903† | -0.9 | -0.00004 | mg/L | 0.000678 | -0.00004 mg/L | 0.000678 | >999.9% |
| Tl 190.801† | 4.5 | 0.00261 | mg/L | 0.001090 | 0.00261 mg/L | 0.001090 | 41.78% |
| V 292.402† | 23.3 | 0.00023 | mg/L | 0.000155 | 0.00023 mg/L | 0.000155 | 67.28% |
| Zn 206.200† | 0.3 | 0.00042 | mg/L | 0.001796 | 0.00042 mg/L | 0.001796 | 427.81% |

=====
Analysis Begun

Start Time: 8/6/2010 1:52:18 PM Plasma On Time: 8/6/2010 7:12:02 AM
Logged In Analyst: metals Technique: ICP Continuous
Spectrometer Model: Optima 7300 DV, S/N 077C8121202 Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif
Batch ID:
Results Data Set: I2100806
Results Library: C:\pe\metals\Results\Results.mdb

=====
Sequence No.: 1 Date Collected: 8/6/2010 1:52:19 PM
Sample ID: STD3 Data Type: Original

Nebulizer Parameters: STD3
Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: STD3

| Analyte | Mean Corrected | | | Calib | |
|-------------|----------------|----------|-------|-------|-------|
| | Intensity | Std.Dev. | RSD | Conc. | Units |
| ScA 357.253 | 1954813.3 | 5813.40 | 0.30% | 102.8 | % |
| ScR 361.383 | 295724.9 | 315.66 | 0.11% | 101.0 | % |
| Ag 328.068† | 177312.5 | 765.91 | 0.43% | [1.0] | mg/L |
| As 188.979† | 14742.9 | 35.10 | 0.24% | [10] | mg/L |
| B 249.677† | 34675.4 | 194.94 | 0.56% | [10] | mg/L |
| Be 313.042† | 2888680.3 | 7581.16 | 0.26% | [5.0] | mg/L |
| Na 589.592† | 596114.2 | 1019.54 | 0.17% | [50] | mg/L |
| Ni 231.604† | 17029.6 | 43.01 | 0.25% | [10] | mg/L |
| Pb 220.353† | 73686.8 | 28.65 | 0.04% | [10] | mg/L |
| Se 196.026† | 12698.7 | 37.82 | 0.30% | [10] | mg/L |
| Sr 421.552† | 3349510.2 | 40161.81 | 1.20% | [5] | mg/L |
| Tl 190.801† | 18095.1 | 13.81 | 0.08% | [10] | mg/L |
| Zn 206.200† | 6788.1 | 42.17 | 0.62% | [10] | mg/L |

=====
Analysis Begun

Start Time: 8/6/2010 1:57:52 PM Plasma On Time: 8/6/2010 7:12:02 AM
Logged In Analyst: metals Technique: ICP Continuous
Spectrometer Model: Optima 7300 DV, S/N 077C8121202 Autosampler Model: AS-93plus

Sample Information File: C:\pe\metals\Sample Information\0806.sif
Batch ID:
Results Data Set: I2100806
Results Library: C:\pe\metals\Results\Results.mdb

=====
Sequence No.: 1 Autosampler Location: 7
Sample ID: CV Date Collected: 8/6/2010 1:57:54 PM
Analyst: ALA Data Type: Original
Dilution: 1X

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|--------|--------------|----------|--------|-------|----------|-------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1967341.3 | 103.5 | % | 1.14 | | | | 1.10% |
| ScR 361.383 | 299324.1 | 102.3 | % | 0.81 | | | | 0.80% |
| Ag 328.068† | 182746.7 | 1.031 | mg/L | 0.0142 | 1.031 | mg/L | 0.0142 | 1.38% |
| Al 308.215† | 2762.0 | 2.146 | mg/L | 0.0161 | 2.146 | mg/L | 0.0161 | 0.75% |
| As 188.979† | 2954.2 | 2.021 | mg/L | 0.0290 | 2.021 | mg/L | 0.0290 | 1.43% |
| B 249.677† | 3457.4 | 0.9953 | mg/L | 0.00969 | 0.9953 | mg/L | 0.00969 | 0.97% |
| Ba 233.527† | 3328.7 | 0.9978 | mg/L | 0.01040 | 0.9978 | mg/L | 0.01040 | 1.04% |
| Be 313.042† | 564286.9 | 0.9762 | mg/L | 0.00558 | 0.9762 | mg/L | 0.00558 | 0.57% |
| Ca 317.933† | 31389.1 | 2.162 | mg/L | 0.0118 | 2.162 | mg/L | 0.0118 | 0.55% |
| Cd 228.802† | 22976.8 | 1.071 | mg/L | 0.0108 | 1.071 | mg/L | 0.0108 | 1.01% |
| Co 228.616† | 31594.0 | 1.047 | mg/L | 0.0117 | 1.047 | mg/L | 0.0117 | 1.12% |
| Cr 267.716† | 5208.9 | 1.013 | mg/L | 0.0079 | 1.013 | mg/L | 0.0079 | 0.78% |
| Cu 324.752† | 293301.8 | 1.051 | mg/L | 0.0115 | 1.051 | mg/L | 0.0115 | 1.09% |
| Fe 273.955† | 2415.4 | 2.107 | mg/L | 0.0146 | 2.107 | mg/L | 0.0146 | 0.69% |
| K 766.490† | 31344.8 | 21.57 | mg/L | 0.066 | 21.57 | mg/L | 0.066 | 0.30% |
| Mg 279.077† | 2008.9 | 2.146 | mg/L | 0.0181 | 2.146 | mg/L | 0.0181 | 0.84% |
| Mn 257.610† | 30254.6 | 0.9606 | mg/L | 0.00372 | 0.9606 | mg/L | 0.00372 | 0.39% |
| Mo 202.031† | 17855.0 | 1.039 | mg/L | 0.0126 | 1.039 | mg/L | 0.0126 | 1.21% |
| Na 589.592† | 596062.8 | 50.00 | mg/L | 0.359 | 50.00 | mg/L | 0.359 | 0.72% |
| Na 330.237† | 1569.0 | 54.01 | mg/L | 0.150 | 54.01 | mg/L | 0.150 | 0.28% |
| Ni 231.604† | 1707.3 | 1.004 | mg/L | 0.0065 | 1.004 | mg/L | 0.0065 | 0.65% |
| Pb 220.353† | 14675.0 | 1.993 | mg/L | 0.0214 | 1.993 | mg/L | 0.0214 | 1.08% |
| Sb 206.836† | 5845.6 | 2.184 | mg/L | 0.0245 | 2.184 | mg/L | 0.0245 | 1.12% |
| Se 196.026† | 2571.4 | 2.025 | mg/L | 0.0243 | 2.025 | mg/L | 0.0243 | 1.20% |
| Si 288.158† | 3272.1 | 2.219 | mg/L | 0.0183 | 2.219 | mg/L | 0.0183 | 0.83% |
| Sn 189.927† | 3916.4 | 1.067 | mg/L | 0.0135 | 1.067 | mg/L | 0.0135 | 1.26% |
| Sr 421.552† | 671435.4 | 1.002 | mg/L | 0.0109 | 1.002 | mg/L | 0.0109 | 1.08% |
| Ti 334.903† | 22961.0 | 1.044 | mg/L | 0.0061 | 1.044 | mg/L | 0.0061 | 0.58% |
| Tl 190.801† | 3633.6 | 2.008 | mg/L | 0.0238 | 2.008 | mg/L | 0.0238 | 1.18% |
| V 292.402† | 102865.0 | 1.050 | mg/L | 0.0099 | 1.050 | mg/L | 0.0099 | 0.94% |
| Zn 206.200† | 662.8 | 0.9759 | mg/L | 0.01387 | 0.9759 | mg/L | 0.01387 | 1.42% |

Sequence No.: 2
 Sample ID: CB
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 2:02:07 PM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1962395.3 | 103.2 | % | 0.28 | | | 0.27% |
| ScR 361.383 | 304299.9 | 104.0 | % | 0.33 | | | 0.32% |
| Ag 328.068† | -44.9 | -0.00025 | mg/L | 0.000065 | -0.00025 mg/L | 0.000065 | 25.57% |
| Al 308.215† | 8.0 | 0.00629 | mg/L | 0.004634 | 0.00629 mg/L | 0.004634 | 73.64% |
| As 188.979† | 2.4 | 0.00159 | mg/L | 0.001397 | 0.00159 mg/L | 0.001397 | 88.01% |
| B 249.677† | 11.1 | 0.00320 | mg/L | 0.002945 | 0.00320 mg/L | 0.002945 | 92.05% |
| Ba 233.527† | 0.3 | 0.00008 | mg/L | 0.000613 | 0.00008 mg/L | 0.000613 | 724.51% |
| Be 313.042† | 62.2 | 0.00011 | mg/L | 0.000180 | 0.00011 mg/L | 0.000180 | 167.05% |
| Ca 317.933† | 14.0 | 0.00096 | mg/L | 0.001427 | 0.00096 mg/L | 0.001427 | 148.09% |
| Cd 228.802† | -3.2 | -0.00016 | mg/L | 0.000127 | -0.00016 mg/L | 0.000127 | 81.75% |
| Co 228.616† | 4.8 | 0.00016 | mg/L | 0.000034 | 0.00016 mg/L | 0.000034 | 21.50% |
| Cr 267.716† | 1.2 | 0.00022 | mg/L | 0.001031 | 0.00022 mg/L | 0.001031 | 462.69% |
| Cu 324.752† | 323.3 | 0.00116 | mg/L | 0.000059 | 0.00116 mg/L | 0.000059 | 5.06% |
| Fe 273.955† | -2.5 | -0.00216 | mg/L | 0.001573 | -0.00216 mg/L | 0.001573 | 72.78% |
| K 766.490† | 45.0 | 0.03095 | mg/L | 0.040942 | 0.03095 mg/L | 0.040942 | 132.26% |
| Mg 279.077† | 9.9 | 0.01060 | mg/L | 0.001830 | 0.01060 mg/L | 0.001830 | 17.27% |
| Mn 257.610† | -1.7 | -0.00005 | mg/L | 0.000271 | -0.00005 mg/L | 0.000271 | 502.30% |
| Mo 202.031† | -1.7 | -0.00010 | mg/L | 0.000156 | -0.00010 mg/L | 0.000156 | 157.16% |
| Na 589.592† | 239.6 | 0.02009 | mg/L | 0.009554 | 0.02009 mg/L | 0.009554 | 47.54% |
| Na 330.237† | 4.2 | 0.1429 | mg/L | 0.24819 | 0.1429 mg/L | 0.24819 | 173.74% |
| Ni 231.604† | 4.6 | 0.00268 | mg/L | 0.001059 | 0.00268 mg/L | 0.001059 | 39.57% |
| Pb 220.353† | -8.7 | -0.00118 | mg/L | 0.000556 | -0.00118 mg/L | 0.000556 | 47.05% |
| Sb 206.836† | 8.3 | 0.00309 | mg/L | 0.001153 | 0.00309 mg/L | 0.001153 | 37.25% |
| Se 196.026† | 7.2 | 0.00568 | mg/L | 0.005404 | 0.00568 mg/L | 0.005404 | 95.16% |
| Si 288.158† | 10.2 | 0.00689 | mg/L | 0.001605 | 0.00689 mg/L | 0.001605 | 23.28% |
| Sn 189.927† | 3.8 | 0.00103 | mg/L | 0.000175 | 0.00103 mg/L | 0.000175 | 17.01% |
| Sr 421.552† | 76.1 | 0.00011 | mg/L | 0.000130 | 0.00011 mg/L | 0.000130 | 114.20% |
| Ti 334.903† | -10.8 | -0.00049 | mg/L | 0.000872 | -0.00049 mg/L | 0.000872 | 176.65% |
| Tl 190.801† | 4.5 | 0.00251 | mg/L | 0.000759 | 0.00251 mg/L | 0.000759 | 30.25% |
| V 292.402† | -2.2 | -0.00002 | mg/L | 0.000158 | -0.00002 mg/L | 0.000158 | 762.20% |
| Zn 206.200† | -0.2 | -0.00028 | mg/L | 0.001622 | -0.00028 mg/L | 0.001622 | 579.73% |

Sequence No.: 3
 Sample ID: RG84 D SWC
 Analyst: ALA
 Dilution: 10X

Autosampler Location: 322
 Date Collected: 8/6/2010 2:06:18 PM
 Data Type: Original

Nebulizer Parameters: RG84 D SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 D SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1986927.7 | 104.5 | % | 0.36 | | | 0.34% |
| ScR 361.383 | 308196.1 | 105.3 | % | 1.56 | | | 1.48% |
| Ag 328.068† | 244.9 | 0.00118 | mg/L | 0.000143 | 0.01184 mg/L | 0.001433 | 12.11% |
| Al 308.215† | 28418.4 | 22.42 | mg/L | 0.359 | 224.2 mg/L | 3.59 | 1.60% |
| As 188.979† | 39.7 | 0.05091 | mg/L | 0.000375 | 0.5091 mg/L | 0.00375 | 0.74% |
| B 249.677† | 113.1 | 0.03253 | mg/L | 0.000718 | 0.3253 mg/L | 0.00718 | 2.21% |
| Ba 233.527† | 903.6 | 0.2590 | mg/L | 0.00539 | 2.590 mg/L | 0.0539 | 2.08% |
| Be 313.042† | 293.5 | 0.00042 | mg/L | 0.000028 | 0.00420 mg/L | 0.000283 | 6.75% |
| Ca 317.933† | 174257.4 | 12.00 | mg/L | 0.193 | 120.0 mg/L | 1.93 | 1.61% |
| Cd 228.802† | 1214.0 | 0.05692 | mg/L | 0.000450 | 0.5692 mg/L | 0.00450 | 0.79% |
| Co 228.616† | 1363.4 | 0.04127 | mg/L | 0.000417 | 0.4127 mg/L | 0.00417 | 1.01% |
| Cr 267.716† | 1385.0 | 0.2743 | mg/L | 0.00496 | 2.743 mg/L | 0.0496 | 1.81% |
| Cu 324.752† | 158188.8 | 0.5759 | mg/L | 0.00199 | 5.759 mg/L | 0.0199 | 0.35% |
| Fe 273.955† | 147624.4 | 129.1 | mg/L | 2.35 | 1291 mg/L | 23.5 | 1.82% |
| K 766.490† | 2075.9 | 1.429 | mg/L | 0.0637 | 14.29 mg/L | 0.637 | 4.46% |
| Mg 279.077† | 7437.7 | 7.859 | mg/L | 0.1220 | 78.59 mg/L | 1.220 | 1.55% |
| Mn 257.610† | 43791.3 | 1.390 | mg/L | 0.0276 | 13.90 mg/L | 0.276 | 1.99% |
| Mo 202.031† | 558.1 | 0.03226 | mg/L | 0.000507 | 0.3226 mg/L | 0.00507 | 1.57% |
| Na 589.592† | 12909.6 | 1.083 | mg/L | 0.0184 | 10.83 mg/L | 0.184 | 1.70% |
| Na 330.237† | 53.4 | 1.337 | mg/L | 0.1554 | 13.37 mg/L | 1.554 | 11.62% |
| Ni 231.604† | 286.4 | 0.1682 | mg/L | 0.00346 | 1.682 mg/L | 0.0346 | 2.06% |
| Pb 220.353† | 7931.5 | 1.071 | mg/L | 0.0062 | 10.71 mg/L | 0.062 | 0.58% |
| Sb 206.836† | 56.4 | 0.02074 | mg/L | 0.001615 | 0.2074 mg/L | 0.01615 | 7.79% |
| Se 196.026† | 12.3 | 0.00891 | mg/L | 0.001111 | 0.08906 mg/L | 0.011113 | 12.48% |
| Si 288.158† | 351.5 | 0.2382 | mg/L | 0.00975 | 2.382 mg/L | 0.0975 | 4.09% |
| Sn 189.927† | 104.1 | 0.02951 | mg/L | 0.000907 | 0.2951 mg/L | 0.00907 | 3.07% |
| Sr 421.552† | 44252.8 | 0.06606 | mg/L | 0.001153 | 0.6606 mg/L | 0.01153 | 1.74% |
| Ti 334.903† | 29921.6 | 1.362 | mg/L | 0.0246 | 13.62 mg/L | 0.246 | 1.81% |
| Tl 190.801† | -22.1 | 0.00825 | mg/L | 0.001675 | 0.08252 mg/L | 0.016755 | 20.30% |
| V 292.402† | 13881.6 | 0.1279 | mg/L | 0.00032 | 1.279 mg/L | 0.0032 | 0.25% |
| Zn 206.200† | 2688.3 | 3.960 | mg/L | 0.0722 | 39.60 mg/L | 0.722 | 1.82% |

Sequence No.: 4
 Sample ID: RG84 G SWC
 Analyst: ALA
 Dilution: 10X

Autosampler Location: 323
 Date Collected: 8/6/2010 2:10:15 PM
 Data Type: Original

Nebulizer Parameters: RG84 G SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 G SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1976214.2 | 103.9 | % | 0.97 | | | 0.93% |
| ScR 361.383 | 283449.6 | 96.85 | % | 0.846 | | | 0.87% |
| Ag 328.068† | 448.6 | 0.00236 | mg/L | 0.000172 | 0.02358 mg/L | 0.001717 | 7.28% |
| Al 308.215† | 36994.1 | 29.18 | mg/L | 0.259 | 291.8 mg/L | 2.59 | 0.89% |
| As 188.979† | -18.5 | 0.01772 | mg/L | 0.002215 | 0.1772 mg/L | 0.02215 | 12.50% |
| B 249.677† | 43.3 | 0.01239 | mg/L | 0.003048 | 0.1239 mg/L | 0.03048 | 24.60% |
| Ba 233.527† | 1348.8 | 0.3904 | mg/L | 0.00266 | 3.904 mg/L | 0.0266 | 0.68% |
| Be 313.042† | 360.5 | 0.00055 | mg/L | 0.000022 | 0.00550 mg/L | 0.000217 | 3.95% |
| Ca 317.933† | 282649.8 | 19.47 | mg/L | 0.211 | 194.7 mg/L | 2.11 | 1.09% |
| Cd 228.802† | 686.7 | 0.03240 | mg/L | 0.000398 | 0.3240 mg/L | 0.00398 | 1.23% |
| Co 228.616† | 1350.0 | 0.03988 | mg/L | 0.000438 | 0.3988 mg/L | 0.00438 | 1.10% |
| Cr 267.716† | 2301.0 | 0.4534 | mg/L | 0.00339 | 4.534 mg/L | 0.0339 | 0.75% |
| Cu 324.752† | 113410.3 | 0.4167 | mg/L | 0.00526 | 4.167 mg/L | 0.0526 | 1.26% |
| Fe 273.955† | 173188.1 | 151.5 | mg/L | 1.24 | 1515 mg/L | 12.4 | 0.82% |
| K 766.490† | 2952.4 | 2.032 | mg/L | 0.0250 | 20.32 mg/L | 0.250 | 1.23% |
| Mg 279.077† | 8550.1 | 9.032 | mg/L | 0.0515 | 90.32 mg/L | 0.515 | 0.57% |
| Mn 257.610† | 40416.9 | 1.283 | mg/L | 0.0130 | 12.83 mg/L | 0.130 | 1.01% |
| Mo 202.031† | 622.5 | 0.03587 | mg/L | 0.000577 | 0.3587 mg/L | 0.00577 | 1.61% |
| Na 589.592† | 14011.5 | 1.175 | mg/L | 0.0162 | 11.75 mg/L | 0.162 | 1.38% |
| Na 330.237† | 23.6 | 0.9842 | mg/L | 0.08704 | 9.842 mg/L | 0.8704 | 8.84% |
| Ni 231.604† | 441.3 | 0.2591 | mg/L | 0.00160 | 2.591 mg/L | 0.0160 | 0.62% |
| Pb 220.353† | 1807.9 | 0.2401 | mg/L | 0.00142 | 2.401 mg/L | 0.0142 | 0.59% |
| Sb 206.836† | 46.6 | 0.01542 | mg/L | 0.001103 | 0.1542 mg/L | 0.01103 | 7.15% |
| Se 196.026† | 13.2 | 0.00905 | mg/L | 0.003014 | 0.09052 mg/L | 0.030136 | 33.29% |
| Si 288.158† | 334.5 | 0.2266 | mg/L | 0.00249 | 2.266 mg/L | 0.0249 | 1.10% |
| Sn 189.927† | 51.0 | 0.01559 | mg/L | 0.001114 | 0.1559 mg/L | 0.01114 | 7.14% |
| Sr 421.552† | 85663.6 | 0.1279 | mg/L | 0.00089 | 1.279 mg/L | 0.0089 | 0.70% |
| Ti 334.903† | 38077.7 | 1.733 | mg/L | 0.0181 | 17.33 mg/L | 0.181 | 1.05% |
| Tl 190.801† | -24.4 | 0.01026 | mg/L | 0.002924 | 0.1026 mg/L | 0.02924 | 28.49% |
| V 292.402† | 10399.4 | 0.09061 | mg/L | 0.001259 | 0.9061 mg/L | 0.01259 | 1.39% |
| Zn 206.200† | 1198.3 | 1.764 | mg/L | 0.0117 | 17.64 mg/L | 0.117 | 0.66% |

Sequence No.: 5
 Sample ID: RG84 H SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 324
 Date Collected: 8/6/2010 2:14:11 PM
 Data Type: Original

Nebulizer Parameters: RG84 H SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 H SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------|----------|--------|
| ScA 357.253 | 1990795.1 | 104.7 | % | 0.88 | | | 0.84% |
| ScR 361.383 | 312321.2 | 106.7 | % | 1.12 | | | 1.05% |
| Ag 328.068† | 189.1 | 0.00054 | mg/L | 0.000077 | 0.00108 mg/L | 0.000154 | 14.29% |
| Al 308.215† | 147405.6 | 116.3 | mg/L | 0.23 | 232.6 mg/L | 0.46 | 0.20% |
| As 188.979† | -83.4 | 0.04413 | mg/L | 0.003692 | 0.08826 mg/L | 0.007383 | 8.37% |
| B 249.677† | 324.7 | 0.09342 | mg/L | 0.001229 | 0.1868 mg/L | 0.00246 | 1.32% |
| Ba 233.527† | 6369.6 | 1.890 | mg/L | 0.0276 | 3.781 mg/L | 0.0551 | 1.46% |
| Be 313.042† | 1199.1 | 0.00177 | mg/L | 0.000065 | 0.00355 mg/L | 0.000130 | 3.66% |
| Ca 317.933† | 1461639.3 | 100.7 | mg/L | 0.74 | 201.3 mg/L | 1.47 | 0.73% |
| Cd 228.802† | 641.9 | 0.03048 | mg/L | 0.000216 | 0.06096 mg/L | 0.000432 | 0.71% |
| Co 228.616† | 3313.5 | 0.09721 | mg/L | 0.000552 | 0.1944 mg/L | 0.00110 | 0.57% |
| Cr 267.716† | 3406.9 | 0.6652 | mg/L | 0.00924 | 1.330 mg/L | 0.0185 | 1.39% |
| Cu 324.752† | 531280.8 | 1.917 | mg/L | 0.0080 | 3.835 mg/L | 0.0161 | 0.42% |
| Fe 273.955† | 240520.0 | 210.3 | mg/L | 1.96 | 420.7 mg/L | 3.92 | 0.93% |
| K 766.490† | 13990.6 | 9.628 | mg/L | 0.1381 | 19.26 mg/L | 0.276 | 1.43% |
| Mg 279.077† | 41007.3 | 43.58 | mg/L | 0.249 | 87.15 mg/L | 0.497 | 0.57% |
| Mn 257.610† | 132511.1 | 4.206 | mg/L | 0.0273 | 8.411 mg/L | 0.0547 | 0.65% |
| Mo 202.031† | 995.4 | 0.05616 | mg/L | 0.000546 | 0.1123 mg/L | 0.00109 | 0.97% |
| Na 589.592† | 71067.0 | 5.961 | mg/L | 0.0301 | 11.92 mg/L | 0.060 | 0.50% |
| Na 330.237† | 270.7 | 6.603 | mg/L | 0.7186 | 13.21 mg/L | 1.437 | 10.88% |
| Ni 231.604† | 556.9 | 0.3271 | mg/L | 0.00549 | 0.6541 mg/L | 0.01097 | 1.68% |
| Pb 220.353† | 13826.4 | 1.880 | mg/L | 0.0137 | 3.760 mg/L | 0.0273 | 0.73% |
| Sb 206.836† | 71.9 | 0.02906 | mg/L | 0.002712 | 0.05812 mg/L | 0.005424 | 9.33% |
| Se 196.026† | 51.5 | 0.03371 | mg/L | 0.002904 | 0.06741 mg/L | 0.005808 | 8.61% |
| Si 288.158† | 1979.0 | 1.340 | mg/L | 0.0189 | 2.680 mg/L | 0.0378 | 1.41% |
| Sn 189.927† | 112.9 | 0.03801 | mg/L | 0.001496 | 0.07603 mg/L | 0.002993 | 3.94% |
| Sr 421.552† | 393357.0 | 0.5872 | mg/L | 0.00699 | 1.174 mg/L | 0.0140 | 1.19% |
| Ti 334.903† | 126791.6 | 5.767 | mg/L | 0.0547 | 11.53 mg/L | 0.109 | 0.95% |
| Tl 190.801† | -30.8 | 0.01769 | mg/L | 0.004308 | 0.03537 mg/L | 0.008615 | 24.36% |
| V 292.402† | 45057.7 | 0.4357 | mg/L | 0.00412 | 0.8715 mg/L | 0.00823 | 0.94% |
| Zn 206.200† | 13929.9 | 20.52 | mg/L | 0.067 | 41.04 mg/L | 0.133 | 0.33% |

Sequence No.: 6
 Sample ID: RG84 I SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 325
 Date Collected: 8/6/2010 2:18:09 PM
 Data Type: Original

Nebulizer Parameters: RG84 I SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 I SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1987787.4 | 104.5 | % | 1.00 | | | 0.95% |
| ScR 361.383 | 307877.2 | 105.2 | % | 1.04 | | | 0.99% |
| Ag 328.068† | -93.7 | -0.00064 | mg/L | 0.000068 | -0.00128 mg/L | 0.000136 | 10.64% |
| Al 308.215† | 199239.1 | 157.2 | mg/L | 1.52 | 314.3 mg/L | 3.04 | 0.97% |
| As 188.979† | -175.6 | 0.04443 | mg/L | 0.002831 | 0.08887 mg/L | 0.005662 | 6.37% |
| B 249.677† | 50.8 | 0.01442 | mg/L | 0.000711 | 0.02884 mg/L | 0.001421 | 4.93% |
| Ba 233.527† | 1822.5 | 0.5247 | mg/L | 0.00448 | 1.049 mg/L | 0.0090 | 0.85% |
| Be 313.042† | 1666.1 | 0.00248 | mg/L | 0.000055 | 0.00496 mg/L | 0.000110 | 2.23% |
| Ca 317.933† | 943294.0 | 64.96 | mg/L | 0.720 | 129.9 mg/L | 1.44 | 1.11% |
| Cd 228.802† | 125.1 | 0.00638 | mg/L | 0.000326 | 0.01276 mg/L | 0.000652 | 5.11% |
| Co 228.616† | 2982.3 | 0.08053 | mg/L | 0.001328 | 0.1611 mg/L | 0.00266 | 1.65% |
| Cr 267.716† | 1065.2 | 0.2094 | mg/L | 0.00406 | 0.4188 mg/L | 0.00811 | 1.94% |
| Cu 324.752† | 86729.4 | 0.3229 | mg/L | 0.00285 | 0.6458 mg/L | 0.00570 | 0.88% |
| Fe 273.955† | 263567.0 | 230.5 | mg/L | 2.51 | 461.0 mg/L | 5.01 | 1.09% |
| K 766.490† | 15291.3 | 10.52 | mg/L | 0.070 | 21.05 mg/L | 0.141 | 0.67% |
| Mg 279.077† | 52927.4 | 56.27 | mg/L | 0.520 | 112.5 mg/L | 1.04 | 0.92% |
| Mn 257.610† | 90590.0 | 2.875 | mg/L | 0.0295 | 5.750 mg/L | 0.0591 | 1.03% |
| Mo 202.031† | 110.0 | 0.00527 | mg/L | 0.000561 | 0.01054 mg/L | 0.001122 | 10.64% |
| Na 589.592† | 74164.1 | 6.221 | mg/L | 0.0642 | 12.44 mg/L | 0.128 | 1.03% |
| Na 330.237† | 126.2 | 6.537 | mg/L | 0.2577 | 13.07 mg/L | 0.515 | 3.94% |
| Ni 231.604† | 324.8 | 0.1908 | mg/L | 0.00215 | 0.3815 mg/L | 0.00430 | 1.13% |
| Pb 220.353† | 455.9 | 0.07237 | mg/L | 0.002045 | 0.1447 mg/L | 0.00409 | 2.83% |
| Sb 206.836† | 29.5 | 0.02232 | mg/L | 0.001036 | 0.04463 mg/L | 0.002072 | 4.64% |
| Se 196.026† | 49.9 | 0.03488 | mg/L | 0.003580 | 0.06977 mg/L | 0.007161 | 10.26% |
| Si 288.158† | 1816.0 | 1.230 | mg/L | 0.0062 | 2.460 mg/L | 0.0124 | 0.50% |
| Sn 189.927† | -39.0 | -0.00341 | mg/L | 0.001574 | -0.00683 mg/L | 0.003149 | 46.10% |
| Sr 421.552† | 297476.6 | 0.4441 | mg/L | 0.00480 | 0.8881 mg/L | 0.00961 | 1.08% |
| Ti 334.903† | 201050.3 | 9.151 | mg/L | 0.0903 | 18.30 mg/L | 0.181 | 0.99% |
| Tl 190.801† | -45.4 | 0.01118 | mg/L | 0.002425 | 0.02235 mg/L | 0.004849 | 21.70% |
| V 292.402† | 57105.8 | 0.5520 | mg/L | 0.00801 | 1.104 mg/L | 0.0160 | 1.45% |
| Zn 206.200† | 2035.0 | 2.993 | mg/L | 0.0304 | 5.987 mg/L | 0.0608 | 1.02% |

Sequence No.: 7
 Sample ID: RG84 J SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 326
 Date Collected: 8/6/2010 2:21:51 PM
 Data Type: Original

Nebulizer Parameters: RG84 J SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 J SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 2015892.8 | 106.0 | % | 1.21 | | | 1.14% |
| ScR 361.383 | 312578.4 | 106.8 | % | 1.43 | | | 1.34% |
| Ag 328.068† | 19.5 | 0.00005 | mg/L | 0.000256 | 0.00010 mg/L | 0.000513 | 499.05% |
| Al 308.215† | 164244.4 | 129.6 | mg/L | 1.76 | 259.1 mg/L | 3.52 | 1.36% |
| As 188.979† | -197.8 | 0.02886 | mg/L | 0.005178 | 0.05772 mg/L | 0.010357 | 17.94% |
| B 249.677† | 48.8 | 0.01386 | mg/L | 0.000323 | 0.02773 mg/L | 0.000646 | 2.33% |
| Ba 233.527† | 1724.2 | 0.4976 | mg/L | 0.00758 | 0.9953 mg/L | 0.01516 | 1.52% |
| Be 313.042† | 1242.3 | 0.00180 | mg/L | 0.000055 | 0.00360 mg/L | 0.000110 | 3.04% |
| Ca 317.933† | 913311.0 | 62.90 | mg/L | 0.966 | 125.8 mg/L | 1.93 | 1.54% |
| Cd 228.802† | 144.3 | 0.00737 | mg/L | 0.000117 | 0.01474 mg/L | 0.000235 | 1.59% |
| Co 228.616† | 2611.0 | 0.06857 | mg/L | 0.001113 | 0.1371 mg/L | 0.00223 | 1.62% |
| Cr 267.716† | 1503.4 | 0.2944 | mg/L | 0.00335 | 0.5888 mg/L | 0.00669 | 1.14% |
| Cu 324.752† | 127241.8 | 0.4665 | mg/L | 0.00528 | 0.9330 mg/L | 0.01056 | 1.13% |
| Fe 273.955† | 233665.2 | 204.4 | mg/L | 3.39 | 408.7 mg/L | 6.78 | 1.66% |
| K 766.490† | 11729.1 | 8.071 | mg/L | 0.1497 | 16.14 mg/L | 0.299 | 1.85% |
| Mg 279.077† | 46620.8 | 49.56 | mg/L | 0.756 | 99.13 mg/L | 1.511 | 1.52% |
| Mn 257.610† | 77765.8 | 2.468 | mg/L | 0.0476 | 4.936 mg/L | 0.0952 | 1.93% |
| Mo 202.031† | 230.6 | 0.01232 | mg/L | 0.000548 | 0.02465 mg/L | 0.001096 | 4.45% |
| Na 589.592† | 74094.9 | 6.215 | mg/L | 0.1070 | 12.43 mg/L | 0.214 | 1.72% |
| Na 330.237† | 250.6 | 6.451 | mg/L | 0.3825 | 12.90 mg/L | 0.765 | 5.93% |
| Ni 231.604† | 419.9 | 0.2466 | mg/L | 0.00528 | 0.4931 mg/L | 0.01056 | 2.14% |
| Pb 220.353† | 5378.3 | 0.7375 | mg/L | 0.00767 | 1.475 mg/L | 0.0153 | 1.04% |
| Sb 206.836† | 25.7 | 0.01975 | mg/L | 0.001902 | 0.03949 mg/L | 0.003804 | 9.63% |
| Se 196.026† | 52.5 | 0.03705 | mg/L | 0.001350 | 0.07411 mg/L | 0.002700 | 3.64% |
| Si 288.158† | 2307.8 | 1.563 | mg/L | 0.0228 | 3.125 mg/L | 0.0457 | 1.46% |
| Sn 189.927† | -13.4 | 0.00344 | mg/L | 0.001932 | 0.00689 mg/L | 0.003863 | 56.11% |
| Sr 421.552† | 185424.3 | 0.2768 | mg/L | 0.00432 | 0.5536 mg/L | 0.00864 | 1.56% |
| Ti 334.903† | 200500.1 | 9.127 | mg/L | 0.1518 | 18.25 mg/L | 0.304 | 1.66% |
| Tl 190.801† | -35.3 | 0.01261 | mg/L | 0.001028 | 0.02521 mg/L | 0.002057 | 8.16% |
| V 292.402† | 46833.7 | 0.4506 | mg/L | 0.00753 | 0.9013 mg/L | 0.01505 | 1.67% |
| Zn 206.200† | 14391.9 | 21.20 | mg/L | 0.357 | 42.40 mg/L | 0.714 | 1.68% |

Sequence No.: 8
 Sample ID: RG84 K SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 327
 Date Collected: 8/6/2010 2:25:34 PM
 Data Type: Original

Nebulizer Parameters: RG84 K SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 K SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 2020191.1 | 106.2 | % | 0.22 | | | 0.21% |
| ScR 361.383 | 313527.2 | 107.1 | % | 1.36 | | | 1.27% |
| Ag 328.068+ | 5.2 | -0.00004 | mg/L | 0.000090 | -0.00007 mg/L | 0.000180 | 246.25% |
| Al 308.215+ | 139218.2 | 109.8 | mg/L | 1.21 | 219.6 mg/L | 2.42 | 1.10% |
| As 188.979+ | -150.0 | 0.03529 | mg/L | 0.000687 | 0.07058 mg/L | 0.001374 | 1.95% |
| B 249.677+ | 227.5 | 0.06539 | mg/L | 0.002254 | 0.1308 mg/L | 0.00451 | 3.45% |
| Ba 233.527+ | 2208.6 | 0.6456 | mg/L | 0.00947 | 1.291 mg/L | 0.0189 | 1.47% |
| Be 313.042+ | 1199.7 | 0.00174 | mg/L | 0.000077 | 0.00348 mg/L | 0.000154 | 4.43% |
| Ca 317.933+ | 879984.9 | 60.60 | mg/L | 0.653 | 121.2 mg/L | 1.31 | 1.08% |
| Cd 228.802+ | 172.8 | 0.00858 | mg/L | 0.000018 | 0.01715 mg/L | 0.000036 | 0.21% |
| Co 228.616+ | 2844.0 | 0.07908 | mg/L | 0.000203 | 0.1582 mg/L | 0.00041 | 0.26% |
| Cr 267.716+ | 1363.2 | 0.2669 | mg/L | 0.00373 | 0.5338 mg/L | 0.00746 | 1.40% |
| Cu 324.752+ | 143267.6 | 0.5226 | mg/L | 0.00147 | 1.045 mg/L | 0.0029 | 0.28% |
| Fe 273.955+ | 200213.1 | 175.1 | mg/L | 1.76 | 350.2 mg/L | 3.51 | 1.00% |
| K 766.490+ | 10259.7 | 7.060 | mg/L | 0.0733 | 14.12 mg/L | 0.147 | 1.04% |
| Mg 279.077+ | 38464.9 | 40.89 | mg/L | 0.361 | 81.78 mg/L | 0.722 | 0.88% |
| Mn 257.610+ | 71283.8 | 2.262 | mg/L | 0.0207 | 4.525 mg/L | 0.0413 | 0.91% |
| Mo 202.031+ | 214.8 | 0.01145 | mg/L | 0.000114 | 0.02289 mg/L | 0.000227 | 0.99% |
| Na 589.592+ | 71599.4 | 6.006 | mg/L | 0.0659 | 12.01 mg/L | 0.132 | 1.10% |
| Na 330.237+ | 150.1 | 6.518 | mg/L | 0.1554 | 13.04 mg/L | 0.311 | 2.38% |
| Ni 231.604+ | 369.0 | 0.2167 | mg/L | 0.00299 | 0.4334 mg/L | 0.00598 | 1.38% |
| Pb 220.353+ | 3183.4 | 0.4382 | mg/L | 0.00217 | 0.8765 mg/L | 0.00434 | 0.50% |
| Sb 206.836+ | 23.5 | 0.01753 | mg/L | 0.000361 | 0.03506 mg/L | 0.000723 | 2.06% |
| Se 196.026+ | 44.0 | 0.03054 | mg/L | 0.007578 | 0.06108 mg/L | 0.015156 | 24.81% |
| Si 288.158+ | 2036.4 | 1.379 | mg/L | 0.0278 | 2.758 mg/L | 0.0556 | 2.02% |
| Sn 189.927+ | 28.3 | 0.01402 | mg/L | 0.001853 | 0.02804 mg/L | 0.003706 | 13.22% |
| Sr 421.552+ | 379096.0 | 0.5659 | mg/L | 0.00410 | 1.132 mg/L | 0.0082 | 0.73% |
| Ti 334.903+ | 168793.0 | 7.683 | mg/L | 0.0745 | 15.37 mg/L | 0.149 | 0.97% |
| Tl 190.801+ | -27.6 | 0.01225 | mg/L | 0.002912 | 0.02450 mg/L | 0.005825 | 23.77% |
| V 292.402+ | 47994.7 | 0.4663 | mg/L | 0.00360 | 0.9325 mg/L | 0.00719 | 0.77% |
| Zn 206.200+ | 3203.2 | 4.716 | mg/L | 0.0686 | 9.431 mg/L | 0.1371 | 1.45% |

Sequence No.: 9
 Sample ID: RG84 A SWC
 Analyst: ALA
 Dilution: 20X

Autosampler Location: 328
 Date Collected: 8/6/2010 2:29:31 PM
 Data Type: Original

Nebulizer Parameters: RG84 A SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG84 A SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1981049.3 | 104.2 | % | 2.84 | | | 2.72% |
| ScR 361.383 | 305188.7 | 104.3 | % | 2.00 | | | 1.91% |
| Ag 328.068† | 146.5 | 0.00074 | mg/L | 0.000346 | 0.01479 mg/L | 0.006924 | 46.83% |
| Al 308.215† | 18501.9 | 14.59 | mg/L | 0.436 | 291.9 mg/L | 8.71 | 2.99% |
| As 188.979† | 21.9 | 0.02737 | mg/L | 0.003377 | 0.5474 mg/L | 0.06755 | 12.34% |
| B 249.677† | 36.1 | 0.01039 | mg/L | 0.000910 | 0.2078 mg/L | 0.01820 | 8.76% |
| Ba 233.527† | 489.5 | 0.1414 | mg/L | 0.00211 | 2.827 mg/L | 0.0423 | 1.50% |
| Be 313.042† | 148.9 | 0.00022 | mg/L | 0.000061 | 0.00444 mg/L | 0.001212 | 27.32% |
| Ca 317.933† | 142246.2 | 9.796 | mg/L | 0.3042 | 195.9 mg/L | 6.08 | 3.11% |
| Cd 228.802† | 697.0 | 0.03279 | mg/L | 0.001065 | 0.6558 mg/L | 0.02131 | 3.25% |
| Co 228.616† | 689.6 | 0.02085 | mg/L | 0.000772 | 0.4170 mg/L | 0.01543 | 3.70% |
| Cr 267.716† | 2288.2 | 0.4472 | mg/L | 0.00727 | 8.945 mg/L | 0.1453 | 1.62% |
| Cu 324.752† | 94589.6 | 0.3430 | mg/L | 0.00837 | 6.860 mg/L | 0.1674 | 2.44% |
| Fe 273.955† | 66539.0 | 58.19 | mg/L | 1.828 | 1164 mg/L | 36.6 | 3.14% |
| K 766.490† | 1239.5 | 0.8530 | mg/L | 0.01497 | 17.06 mg/L | 0.299 | 1.75% |
| Mg 279.077† | 4420.0 | 4.680 | mg/L | 0.0832 | 93.59 mg/L | 1.664 | 1.78% |
| Mn 257.610† | 19327.9 | 0.6136 | mg/L | 0.01675 | 12.27 mg/L | 0.335 | 2.73% |
| Mo 202.031† | 564.7 | 0.03268 | mg/L | 0.001120 | 0.6536 mg/L | 0.02239 | 3.43% |
| Na 589.592† | 5671.0 | 0.4757 | mg/L | 0.01407 | 9.513 mg/L | 0.2815 | 2.96% |
| Na 330.237† | 28.3 | 0.6264 | mg/L | 0.16588 | 12.53 mg/L | 3.318 | 26.48% |
| Ni 231.604† | 444.5 | 0.2610 | mg/L | 0.00568 | 5.221 mg/L | 0.1135 | 2.17% |
| Pb 220.353† | 1268.0 | 0.1709 | mg/L | 0.00535 | 3.419 mg/L | 0.1069 | 3.13% |
| Sb 206.836† | 33.8 | 0.00936 | mg/L | 0.000946 | 0.1872 mg/L | 0.01892 | 10.11% |
| Se 196.026† | 14.2 | 0.01052 | mg/L | 0.006814 | 0.2105 mg/L | 0.13628 | 64.75% |
| Si 288.158† | 149.7 | 0.1015 | mg/L | 0.00015 | 2.029 mg/L | 0.0030 | 0.15% |
| Sn 189.927† | 91.4 | 0.02567 | mg/L | 0.000615 | 0.5134 mg/L | 0.01231 | 2.40% |
| Sr 421.552† | 35310.5 | 0.05271 | mg/L | 0.001574 | 1.054 mg/L | 0.0315 | 2.99% |
| Ti 334.903† | 16196.8 | 0.7369 | mg/L | 0.02023 | 14.74 mg/L | 0.405 | 2.75% |
| Tl 190.801† | -5.7 | 0.00602 | mg/L | 0.002610 | 0.1205 mg/L | 0.05220 | 43.33% |
| V 292.402† | 5227.5 | 0.04847 | mg/L | 0.001314 | 0.9693 mg/L | 0.02629 | 2.71% |
| Zn 206.200† | 1730.8 | 2.549 | mg/L | 0.0401 | 50.98 mg/L | 0.802 | 1.57% |

Sequence No.: 10
 Sample ID: RG84 ASPK SWC
 Analyst: ALA
 Dilution: 20X

Autosampler Location: 329
 Date Collected: 8/6/2010 2:33:27 PM
 Data Type: Original

Nebulizer Parameters: RG84 ASPK SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 ASPK SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. | Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------|-------|----------|--------|
| ScA 357.253 | 1989623.1 | 104.6 | % | 2.11 | | | | 2.02% |
| ScR 361.383 | 310811.4 | 106.2 | % | 2.41 | | | | 2.27% |
| Ag 328.068† | 9029.3 | 0.05082 | mg/L | 0.000944 | 1.016 | mg/L | 0.0189 | 1.86% |
| Al 308.215† | 20595.3 | 16.25 | mg/L | 0.331 | 324.9 | mg/L | 6.62 | 2.04% |
| As 188.979† | 300.3 | 0.2167 | mg/L | 0.00302 | 4.334 | mg/L | 0.0604 | 1.39% |
| B 249.677† | 34.3 | 0.00973 | mg/L | 0.000682 | 0.1946 | mg/L | 0.01363 | 7.01% |
| Ba 233.527† | 1219.4 | 0.3599 | mg/L | 0.01039 | 7.199 | mg/L | 0.2079 | 2.89% |
| Be 313.042† | 25897.2 | 0.04476 | mg/L | 0.000993 | 0.8953 | mg/L | 0.01986 | 2.22% |
| Ca 317.933† | 158651.3 | 10.93 | mg/L | 0.243 | 218.5 | mg/L | 4.85 | 2.22% |
| Cd 228.802† | 1844.7 | 0.08599 | mg/L | 0.001927 | 1.720 | mg/L | 0.0385 | 2.24% |
| Co 228.616† | 2352.2 | 0.07588 | mg/L | 0.001991 | 1.518 | mg/L | 0.0398 | 2.62% |
| Cr 267.716† | 2695.3 | 0.5265 | mg/L | 0.01546 | 10.53 | mg/L | 0.309 | 2.94% |
| Cu 324.752† | 129988.4 | 0.4702 | mg/L | 0.00874 | 9.404 | mg/L | 0.1748 | 1.86% |
| Fe 273.955† | 70611.7 | 61.75 | mg/L | 1.311 | 1235 | mg/L | 26.2 | 2.12% |
| K 766.490† | 2669.0 | 1.837 | mg/L | 0.0378 | 36.73 | mg/L | 0.756 | 2.06% |
| Mg 279.077† | 5646.5 | 5.985 | mg/L | 0.1626 | 119.7 | mg/L | 3.25 | 2.72% |
| Mn 257.610† | 24543.4 | 0.7791 | mg/L | 0.01784 | 15.58 | mg/L | 0.357 | 2.29% |
| Mo 202.031† | 688.5 | 0.03986 | mg/L | 0.000758 | 0.7973 | mg/L | 0.01516 | 1.90% |
| Na 589.592† | 17086.8 | 1.433 | mg/L | 0.0362 | 28.66 | mg/L | 0.724 | 2.52% |
| Na 330.237† | 62.8 | 1.754 | mg/L | 0.1186 | 35.07 | mg/L | 2.372 | 6.76% |
| Ni 231.604† | 569.1 | 0.3342 | mg/L | 0.00933 | 6.683 | mg/L | 0.1866 | 2.79% |
| Pb 220.353† | 2881.6 | 0.3899 | mg/L | 0.00809 | 7.799 | mg/L | 0.1618 | 2.07% |
| Sb 206.836† | 38.0 | 0.01024 | mg/L | 0.001733 | 0.2047 | mg/L | 0.03465 | 16.93% |
| Se 196.026† | 252.0 | 0.1977 | mg/L | 0.00289 | 3.954 | mg/L | 0.0577 | 1.46% |
| Si 288.158† | 169.6 | 0.1151 | mg/L | 0.00547 | 2.303 | mg/L | 0.1094 | 4.75% |
| Sn 189.927† | 67.5 | 0.01922 | mg/L | 0.000564 | 0.3844 | mg/L | 0.01128 | 2.93% |
| Sr 421.552† | 68570.5 | 0.1024 | mg/L | 0.00246 | 2.047 | mg/L | 0.0492 | 2.40% |
| Ti 334.903† | 16868.5 | 0.7673 | mg/L | 0.01822 | 15.35 | mg/L | 0.364 | 2.37% |
| Tl 190.801† | 334.8 | 0.1947 | mg/L | 0.00414 | 3.893 | mg/L | 0.0828 | 2.13% |
| V 292.402† | 10223.7 | 0.09923 | mg/L | 0.001847 | 1.985 | mg/L | 0.0369 | 1.86% |
| Zn 206.200† | 1943.6 | 2.863 | mg/L | 0.0750 | 57.25 | mg/L | 1.500 | 2.62% |

Sequence No.: 11
 Sample ID: RG84 ADUP SWC
 Analyst: ALA
 Dilution: 20X

Autosampler Location: 330
 Date Collected: 8/6/2010 2:37:23 PM
 Data Type: Original

Nebulizer Parameters: RG84 ADUP SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG84 ADUP SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2018469.4 | 106.1 | % | 0.70 | | | 0.66% |
| ScR 361.383 | 309773.5 | 105.8 | % | 0.41 | | | 0.39% |
| Ag 328.068† | 665.6 | 0.00366 | mg/L | 0.000167 | 0.07325 mg/L | 0.003340 | 4.56% |
| Al 308.215† | 21659.8 | 17.09 | mg/L | 0.036 | 341.7 mg/L | 0.72 | 0.21% |
| As 188.979† | 28.0 | 0.03212 | mg/L | 0.002228 | 0.6424 mg/L | 0.04455 | 6.94% |
| B 249.677† | 30.9 | 0.00886 | mg/L | 0.000687 | 0.1772 mg/L | 0.01375 | 7.76% |
| Ba 233.527† | 518.2 | 0.1496 | mg/L | 0.00095 | 2.993 mg/L | 0.0190 | 0.64% |
| Be 313.042† | 180.7 | 0.00028 | mg/L | 0.000019 | 0.00553 mg/L | 0.000375 | 6.78% |
| Ca 317.933† | 141351.5 | 9.735 | mg/L | 0.0424 | 194.7 mg/L | 0.85 | 0.44% |
| Cd 228.802† | 694.1 | 0.03264 | mg/L | 0.000245 | 0.6529 mg/L | 0.00490 | 0.75% |
| Co 228.616† | 807.4 | 0.02466 | mg/L | 0.000130 | 0.4933 mg/L | 0.00260 | 0.53% |
| Cr 267.716† | 2282.1 | 0.4462 | mg/L | 0.00269 | 8.925 mg/L | 0.0537 | 0.60% |
| Cu 324.752† | 8744525.0 | 31.36 | mg/L | 0.249 | 627.3 mg/L | 4.97 | 0.79% |
| Fe 273.955† | 70537.9 | 61.69 | mg/L | 0.254 | 1234 mg/L | 5.1 | 0.41% |
| K 766.490† | 1224.2 | 0.8424 | mg/L | 0.01840 | 16.85 mg/L | 0.368 | 2.18% |
| Mg 279.077† | 4467.0 | 4.728 | mg/L | 0.0261 | 94.56 mg/L | 0.522 | 0.55% |
| Mn 257.610† | 20223.4 | 0.6420 | mg/L | 0.00439 | 12.84 mg/L | 0.088 | 0.68% |
| Mo 202.031† | 574.2 | 0.03323 | mg/L | 0.000112 | 0.6647 mg/L | 0.00223 | 0.34% |
| Na 589.592† | 5797.8 | 0.4863 | mg/L | 0.00570 | 9.726 mg/L | 0.1139 | 1.17% |
| Na 330.237† | 27.4 | 0.5319 | mg/L | 0.18082 | 10.64 mg/L | 3.616 | 34.00% |
| Ni 231.604† | 447.8 | 0.2630 | mg/L | 0.00403 | 5.260 mg/L | 0.0806 | 1.53% |
| Pb 220.353† | 1578.1 | 0.1737 | mg/L | 0.00018 | 3.474 mg/L | 0.0037 | 0.11% |
| Sb 206.836† | 31.6 | 0.00847 | mg/L | 0.000822 | 0.1695 mg/L | 0.01644 | 9.70% |
| Se 196.026† | 13.2 | 0.00975 | mg/L | 0.002061 | 0.1951 mg/L | 0.04122 | 21.13% |
| Si 288.158† | 158.9 | 0.1077 | mg/L | 0.00387 | 2.154 mg/L | 0.0775 | 3.60% |
| Sn 189.927† | 54.0 | 0.01550 | mg/L | 0.000306 | 0.3100 mg/L | 0.00612 | 1.97% |
| Sr 421.552† | 36078.9 | 0.05386 | mg/L | 0.000158 | 1.077 mg/L | 0.0032 | 0.29% |
| Ti 334.903† | 16855.0 | 0.7668 | mg/L | 0.00389 | 15.34 mg/L | 0.078 | 0.51% |
| Tl 190.801† | -6.9 | 0.00588 | mg/L | 0.001100 | 0.1176 mg/L | 0.02199 | 18.71% |
| V 292.402† | 5230.6 | 0.04811 | mg/L | 0.000178 | 0.9621 mg/L | 0.00355 | 0.37% |
| Zn 206.200† | 1934.6 | 2.849 | mg/L | 0.0129 | 56.99 mg/L | 0.258 | 0.45% |

Sequence No.: 12
 Sample ID: DIL
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 331
 Date Collected: 8/6/2010 2:41:36 PM
 Data Type: Original

Nebulizer Parameters: DIL

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 202.0 kPa | 0.75 L/min |

Mean Data: DIL

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1980086.0 | 104.1 % | % | 0.75 | | | 0.72% |
| ScR 361.383 | 304228.1 | 103.9 % | % | 0.32 | | | 0.31% |
| Ag 328.068† | -15.7 | -0.00009 | mg/L | 0.000054 | -0.00009 mg/L | 0.000054 | 61.57% |
| Al 308.215† | 5.4 | 0.00427 | mg/L | 0.006088 | 0.00427 mg/L | 0.006088 | 142.49% |
| As 188.979† | 0.7 | 0.00046 | mg/L | 0.001246 | 0.00046 mg/L | 0.001246 | 269.05% |
| B 249.677† | -10.8 | -0.00311 | mg/L | 0.001037 | -0.00311 mg/L | 0.001037 | 33.39% |
| Ba 233.527† | 1.4 | 0.00043 | mg/L | 0.000872 | 0.00043 mg/L | 0.000872 | 201.23% |
| Be 313.042† | -2.1 | 0.00000 | mg/L | 0.000036 | 0.00000 mg/L | 0.000036 | 992.20% |
| Ca 317.933† | 27.0 | 0.00186 | mg/L | 0.001011 | 0.00186 mg/L | 0.001011 | 54.47% |
| Cd 228.802† | -5.5 | -0.00026 | mg/L | 0.000183 | -0.00026 mg/L | 0.000183 | 71.04% |
| Co 228.616† | 3.3 | 0.00011 | mg/L | 0.000137 | 0.00011 mg/L | 0.000137 | 124.77% |
| Cr 267.716† | 4.4 | 0.00085 | mg/L | 0.000448 | 0.00085 mg/L | 0.000448 | 52.98% |
| Cu 324.752† | 461.2 | 0.00165 | mg/L | 0.000460 | 0.00165 mg/L | 0.000460 | 27.83% |
| Fe 273.955† | 1.4 | 0.00127 | mg/L | 0.000675 | 0.00127 mg/L | 0.000675 | 53.23% |
| K 766.490† | 30.5 | 0.02101 | mg/L | 0.009747 | 0.02101 mg/L | 0.009747 | 46.40% |
| Mg 279.077† | 7.0 | 0.00748 | mg/L | 0.002745 | 0.00748 mg/L | 0.002745 | 36.68% |
| Mn 257.610† | -2.5 | -0.00008 | mg/L | 0.000023 | -0.00008 mg/L | 0.000023 | 28.20% |
| Mo 202.031† | -4.9 | -0.00029 | mg/L | 0.000212 | -0.00029 mg/L | 0.000212 | 73.65% |
| Na 589.592† | 28.9 | 0.00242 | mg/L | 0.001097 | 0.00242 mg/L | 0.001097 | 45.29% |
| Na 330.237† | 12.8 | 0.4411 | mg/L | 0.18330 | 0.4411 mg/L | 0.18330 | 41.56% |
| Ni 231.604† | 4.8 | 0.00281 | mg/L | 0.001455 | 0.00281 mg/L | 0.001455 | 51.80% |
| Pb 220.353† | -14.7 | -0.00200 | mg/L | 0.000219 | -0.00200 mg/L | 0.000219 | 10.93% |
| Sb 206.836† | -0.8 | -0.00031 | mg/L | 0.001598 | -0.00031 mg/L | 0.001598 | 519.70% |
| Se 196.026† | 8.1 | 0.00641 | mg/L | 0.003691 | 0.00641 mg/L | 0.003691 | 57.60% |
| Si 288.158† | 6.4 | 0.00430 | mg/L | 0.001678 | 0.00430 mg/L | 0.001678 | 38.99% |
| Sn 189.927† | 2.1 | 0.00057 | mg/L | 0.000653 | 0.00057 mg/L | 0.000653 | 115.14% |
| Sr 421.552† | -29.3 | -0.00004 | mg/L | 0.000012 | -0.00004 mg/L | 0.000012 | 27.38% |
| Ti 334.903† | 2.4 | 0.00011 | mg/L | 0.000552 | 0.00011 mg/L | 0.000552 | 511.15% |
| Tl 190.801† | 1.5 | 0.00082 | mg/L | 0.001805 | 0.00082 mg/L | 0.001805 | 220.35% |
| V 292.402† | 4.9 | 0.00005 | mg/L | 0.000061 | 0.00005 mg/L | 0.000061 | 114.37% |
| Zn 206.200† | -0.0 | -0.00007 | mg/L | 0.001615 | -0.00007 mg/L | 0.001615 | >999.9% |

Sequence No.: 13
Sample ID: CV⁹
Analyst: ALA
Dilution: 1X

Autosampler Location: 7
Date Collected: 8/6/2010 2:45:47 PM
Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------|----------|--------------------|----------|-------|
| ScA 357.253 | 1971878.5 | 103.7 | % | 0.27 | | | 0.26% |
| ScR 361.383 | 301536.4 | 103.0 | % | 0.29 | | | 0.28% |
| Ag 328.068† | 184124.7 | 1.038 | mg/L | 0.0121 | 1.038 mg/L | 0.0121 | 1.17% |
| Al 308.215† | 2773.6 | 2.155 | mg/L | 0.0084 | 2.155 mg/L | 0.0084 | 0.39% |
| As 188.979† | 2983.3 | 2.041 | mg/L | 0.0118 | 2.041 mg/L | 0.0118 | 0.58% |
| B 249.677† | 3452.7 | 0.9939 | mg/L | 0.00582 | 0.9939 mg/L | 0.00582 | 0.59% |
| Ba 233.527† | 3368.1 | 1.010 | mg/L | 0.0027 | 1.010 mg/L | 0.0027 | 0.27% |
| Be 313.042† | 566087.1 | 0.9793 | mg/L | 0.00687 | 0.9793 mg/L | 0.00687 | 0.70% |
| Ca 317.933† | 31807.6 | 2.191 | mg/L | 0.0160 | 2.191 mg/L | 0.0160 | 0.73% |
| Cd 228.802† | 23068.2 | 1.075 | mg/L | 0.0063 | 1.075 mg/L | 0.0063 | 0.58% |
| Co 228.616† | 31900.5 | 1.057 | mg/L | 0.0073 | 1.057 mg/L | 0.0073 | 0.69% |
| Cr 267.716† | 5283.5 | 1.028 | mg/L | 0.0054 | 1.028 mg/L | 0.0054 | 0.52% |
| Cu 324.752† | 294444.0 | 1.055 | mg/L | 0.0067 | 1.055 mg/L | 0.0067 | 0.63% |
| Fe 273.955† | 2447.3 | 2.135 | mg/L | 0.0140 | 2.135 mg/L | 0.0140 | 0.66% |
| K 766.490† | 31641.4 | 21.77 | mg/L | 0.073 | 21.77 mg/L | 0.073 | 0.34% |
| Mg 279.077† | 2031.6 | 2.170 | mg/L | 0.0024 | 2.170 mg/L | 0.0024 | 0.11% |
| Mn 257.610† | 30588.5 | 0.9712 | mg/L | 0.00433 | 0.9712 mg/L | 0.00433 | 0.45% |
| Mo 202.031† | 17785.4 | 1.035 | mg/L | 0.0101 | 1.035 mg/L | 0.0101 | 0.97% |
| Na 589.592† | 592774.3 | 49.72 | mg/L | 0.400 | 49.72 mg/L | 0.400 | 0.80% |
| Na 330.237† | 1576.5 | 54.26 | mg/L | 0.216 | 54.26 mg/L | 0.216 | 0.40% |
| Ni 231.604† | 1722.9 | 1.013 | mg/L | 0.0055 | 1.013 mg/L | 0.0055 | 0.54% |
| Pb 220.353† | 14936.6 | 2.028 | mg/L | 0.0105 | 2.028 mg/L | 0.0105 | 0.52% |
| Sb 206.836† | 5891.6 | 2.201 | mg/L | 0.0107 | 2.201 mg/L | 0.0107 | 0.49% |
| Se 196.026† | 2606.6 | 2.053 | mg/L | 0.0030 | 2.053 mg/L | 0.0030 | 0.15% |
| Si 288.158† | 3287.4 | 2.230 | mg/L | 0.0010 | 2.230 mg/L | 0.0010 | 0.05% |
| Sn 189.927† | 3961.9 | 1.080 | mg/L | 0.0045 | 1.080 mg/L | 0.0045 | 0.41% |
| Sr 421.552† | 674063.3 | 1.006 | mg/L | 0.0038 | 1.006 mg/L | 0.0038 | 0.38% |
| Ti 334.903† | 23097.5 | 1.050 | mg/L | 0.0037 | 1.050 mg/L | 0.0037 | 0.35% |
| Tl 190.801† | 3674.0 | 2.031 | mg/L | 0.0116 | 2.031 mg/L | 0.0116 | 0.57% |
| V 292.402† | 103218.4 | 1.054 | mg/L | 0.0050 | 1.054 mg/L | 0.0050 | 0.47% |
| Zn 206.200† | 675.3 | 0.9943 | mg/L | 0.00264 | 0.9943 mg/L | 0.00264 | 0.27% |

Sequence No.: 14
 Sample ID: CB⁹
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 2:50:00 PM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Conc. Units | Sample Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|-------------|-----------------|---------|
| ScA 357.253 | 1978470.0 | 104.0 | % | 0.71 | | | 0.68% |
| ScR 361.383 | 282408.8 | 96.49 | % | 0.962 | | | 1.00% |
| Ag 328.068† | -4.3 | -0.00002 | mg/L | 0.000329 | -0.00002 | 0.000329 | >999.9% |
| Al 308.215† | 5.3 | 0.00418 | mg/L | 0.005184 | 0.00418 | 0.005184 | 124.17% |
| As 188.979† | 0.7 | 0.00049 | mg/L | 0.002532 | 0.00049 | 0.002532 | 517.86% |
| B 249.677† | -0.8 | -0.00024 | mg/L | 0.001277 | -0.00024 | 0.001277 | 530.43% |
| Ba 233.527† | 4.4 | 0.00132 | mg/L | 0.000605 | 0.00132 | 0.000605 | 45.71% |
| Be 313.042† | 128.4 | 0.00022 | mg/L | 0.000092 | 0.00022 | 0.000092 | 41.41% |
| Ca 317.933† | 16.4 | 0.00113 | mg/L | 0.002392 | 0.00113 | 0.002392 | 212.33% |
| Cd 228.802† | 0.1 | 0.00000 | mg/L | 0.000081 | 0.00000 | 0.000081 | >999.9% |
| Co 228.616† | -2.2 | -0.00007 | mg/L | 0.000101 | -0.00007 | 0.000101 | 139.08% |
| Cr 267.716† | -2.2 | -0.00043 | mg/L | 0.000510 | -0.00043 | 0.000510 | 117.23% |
| Cu 324.752† | 420.9 | 0.00151 | mg/L | 0.000507 | 0.00151 | 0.000507 | 33.57% |
| Fe 273.955† | -0.0 | -0.00001 | mg/L | 0.003091 | -0.00001 | 0.003091 | >999.9% |
| K 766.490† | 70.9 | 0.04880 | mg/L | 0.010472 | 0.04880 | 0.010472 | 21.46% |
| Mg 279.077† | 4.3 | 0.00462 | mg/L | 0.007658 | 0.00462 | 0.007658 | 165.82% |
| Mn 257.610† | 2.6 | 0.00008 | mg/L | 0.000124 | 0.00008 | 0.000124 | 148.63% |
| Mo 202.031† | -0.2 | -0.00001 | mg/L | 0.000060 | -0.00001 | 0.000060 | 674.06% |
| Na 589.592† | 140.7 | 0.01180 | mg/L | 0.005553 | 0.01180 | 0.005553 | 47.06% |
| Na 330.237† | -8.2 | -0.2805 | mg/L | 0.11358 | -0.2805 | 0.11358 | 40.48% |
| Ni 231.604† | 6.1 | 0.00361 | mg/L | 0.000664 | 0.00361 | 0.000664 | 18.42% |
| Pb 220.353† | -5.7 | -0.00078 | mg/L | 0.001239 | -0.00078 | 0.001239 | 159.05% |
| Sb 206.836† | 6.3 | 0.00238 | mg/L | 0.001776 | 0.00238 | 0.001776 | 74.77% |
| Se 196.026† | 12.7 | 0.00997 | mg/L | 0.000907 | 0.00997 | 0.000907 | 9.10% |
| Si 288.158† | 11.4 | 0.00772 | mg/L | 0.001969 | 0.00772 | 0.001969 | 25.51% |
| Sn 189.927† | 5.2 | 0.00142 | mg/L | 0.000461 | 0.00142 | 0.000461 | 32.34% |
| Sr 421.552† | 96.3 | 0.00014 | mg/L | 0.000101 | 0.00014 | 0.000101 | 70.61% |
| Ti 334.903† | -17.4 | -0.00079 | mg/L | 0.000477 | -0.00079 | 0.000477 | 60.11% |
| Tl 190.801† | 3.8 | 0.00211 | mg/L | 0.002711 | 0.00211 | 0.002711 | 128.61% |
| V 292.402† | -0.7 | -0.00001 | mg/L | 0.000116 | -0.00001 | 0.000116 | >999.9% |
| Zn 206.200† | -0.7 | -0.00103 | mg/L | 0.002633 | -0.00103 | 0.002633 | 255.04% |

Sequence No.: 15
 Sample ID: RG51 MB1 SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 301
 Date Collected: 8/6/2010 2:53:56 PM
 Data Type: Original

Nebulizer Parameters: RG51 MB1 SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 MB1 SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1978311.8 | 104.0 | % | 1.11 | | | 1.07% |
| ScR 361.383 | 283519.6 | 96.87 | % | 0.995 | | | 1.03% |
| Ag 328.068† | -0.5 | 0.00000 | mg/L | 0.000095 | -0.00001 mg/L | 0.000191 | >999.9% |
| Al 308.215† | 16.1 | 0.01270 | mg/L | 0.010482 | 0.02541 mg/L | 0.020964 | 82.52% |
| As 188.979† | 3.7 | 0.00252 | mg/L | 0.002541 | 0.00503 mg/L | 0.005081 | 101.00% |
| B 249.677† | -6.2 | -0.00178 | mg/L | 0.001449 | -0.00355 mg/L | 0.002898 | 81.59% |
| Ba 233.527† | 7.0 | 0.00211 | mg/L | 0.000572 | 0.00423 mg/L | 0.001144 | 27.07% |
| Be 313.042† | 70.0 | 0.00012 | mg/L | 0.000026 | 0.00024 mg/L | 0.000053 | 21.77% |
| Ca 317.933† | 198.2 | 0.01365 | mg/L | 0.002204 | 0.02731 mg/L | 0.004408 | 16.14% |
| Cd 228.802† | 0.4 | 0.00001 | mg/L | 0.000106 | 0.00002 mg/L | 0.000212 | >999.9% |
| Co 228.616† | 0.4 | 0.00001 | mg/L | 0.000063 | 0.00002 mg/L | 0.000126 | 584.70% |
| Cr 267.716† | 0.3 | 0.00006 | mg/L | 0.001009 | 0.00012 mg/L | 0.002017 | >999.9% |
| Cu 324.752† | 480.9 | 0.00172 | mg/L | 0.000295 | 0.00345 mg/L | 0.000591 | 17.13% |
| Fe 273.955† | 6.1 | 0.00537 | mg/L | 0.001383 | 0.01074 mg/L | 0.002766 | 25.75% |
| K 766.490† | 125.8 | 0.08654 | mg/L | 0.032761 | 0.1731 mg/L | 0.06552 | 37.86% |
| Mg 279.077† | 5.6 | 0.00593 | mg/L | 0.006942 | 0.01185 mg/L | 0.013885 | 117.14% |
| Mn 257.610† | 3.0 | 0.00010 | mg/L | 0.000069 | 0.00019 mg/L | 0.000139 | 72.70% |
| Mo 202.031† | -4.0 | -0.00023 | mg/L | 0.000351 | -0.00046 mg/L | 0.000702 | 151.61% |
| Na 589.592† | 71.8 | 0.00602 | mg/L | 0.006815 | 0.01205 mg/L | 0.013630 | 113.14% |
| Na 330.237† | -3.7 | -0.1265 | mg/L | 0.25823 | -0.2529 mg/L | 0.51646 | 204.19% |
| Ni 231.604† | 4.2 | 0.00244 | mg/L | 0.001143 | 0.00489 mg/L | 0.002285 | 46.76% |
| Pb 220.353† | -2.7 | -0.00036 | mg/L | 0.000471 | -0.00073 mg/L | 0.000942 | 129.32% |
| Sb 206.836† | -2.3 | -0.00084 | mg/L | 0.002372 | -0.00169 mg/L | 0.004745 | 281.01% |
| Se 196.026† | 4.3 | 0.00342 | mg/L | 0.006854 | 0.00685 mg/L | 0.013709 | 200.22% |
| Si 288.158† | 24.8 | 0.01676 | mg/L | 0.000786 | 0.03353 mg/L | 0.001571 | 4.69% |
| Sn 189.927† | 1.4 | 0.00038 | mg/L | 0.000949 | 0.00075 mg/L | 0.001898 | 252.55% |
| Sr 421.552† | 49.5 | 0.00007 | mg/L | 0.000039 | 0.00015 mg/L | 0.000078 | 52.52% |
| Ti 334.903† | -1.0 | -0.00005 | mg/L | 0.000777 | -0.00010 mg/L | 0.001553 | >999.9% |
| Tl 190.801† | 1.6 | 0.00089 | mg/L | 0.001961 | 0.00178 mg/L | 0.003921 | 219.87% |
| V 292.402† | 7.9 | 0.00008 | mg/L | 0.000223 | 0.00016 mg/L | 0.000447 | 277.97% |
| Zn 206.200† | 1.3 | 0.00195 | mg/L | 0.002276 | 0.00390 mg/L | 0.004551 | 116.85% |

Sequence No.: 16
 Sample ID: RG51 B SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 302
 Date Collected: 8/6/2010 2:57:52 PM
 Data Type: Original

Nebulizer Parameters: RG51 B SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 B SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2006581.5 | 105.5 | % | 1.24 | | | 1.17% |
| ScR 361.383 | 313364.6 | 107.1 | % | 0.53 | | | 0.49% |
| Ag 328.068† | -43.2 | -0.00050 | mg/L | 0.000294 | -0.00100 mg/L | 0.000587 | 58.87% |
| Al 308.215† | 195527.3 | 154.2 | mg/L | 0.43 | 308.5 mg/L | 0.86 | 0.28% |
| As 188.979† | -162.5 | 0.02643 | mg/L | 0.001151 | 0.05285 mg/L | 0.002302 | 4.36% |
| B 249.677† | 47.1 | 0.01336 | mg/L | 0.000925 | 0.02672 mg/L | 0.001851 | 6.93% |
| Ba 233.527† | 2222.8 | 0.6502 | mg/L | 0.00690 | 1.300 mg/L | 0.0138 | 1.06% |
| Be 313.042† | 1315.6 | 0.00197 | mg/L | 0.000020 | 0.00395 mg/L | 0.000040 | 1.02% |
| Ca 317.933† | 576920.1 | 39.73 | mg/L | 0.215 | 79.46 mg/L | 0.430 | 0.54% |
| Cd 228.802† | 84.1 | 0.00453 | mg/L | 0.000221 | 0.00906 mg/L | 0.000441 | 4.87% |
| Co 228.616† | 2599.3 | 0.07104 | mg/L | 0.000969 | 0.1421 mg/L | 0.00194 | 1.36% |
| Cr 267.716† | 1682.4 | 0.3269 | mg/L | 0.00260 | 0.6537 mg/L | 0.00520 | 0.79% |
| Cu 324.752† | 42152.7 | 0.1595 | mg/L | 0.00156 | 0.3189 mg/L | 0.00312 | 0.98% |
| Fe 273.955† | 198906.6 | 174.0 | mg/L | 0.80 | 347.9 mg/L | 1.60 | 0.46% |
| K 766.490† | 7920.7 | 5.451 | mg/L | 0.0250 | 10.90 mg/L | 0.050 | 0.46% |
| Mg 279.077† | 56773.0 | 60.40 | mg/L | 0.189 | 120.8 mg/L | 0.38 | 0.31% |
| Mn 257.610† | 99063.0 | 3.143 | mg/L | 0.0212 | 6.287 mg/L | 0.0424 | 0.68% |
| Mo 202.031† | 113.2 | 0.00589 | mg/L | 0.000122 | 0.01179 mg/L | 0.000244 | 2.07% |
| Na 589.592† | 19661.6 | 1.649 | mg/L | 0.0114 | 3.298 mg/L | 0.0229 | 0.69% |
| Na 330.237† | -9.8 | 1.904 | mg/L | 0.1902 | 3.808 mg/L | 0.3805 | 9.99% |
| Ni 231.604† | 586.2 | 0.3442 | mg/L | 0.00277 | 0.6884 mg/L | 0.00555 | 0.81% |
| Pb 220.353† | 579.2 | 0.09301 | mg/L | 0.001166 | 0.1860 mg/L | 0.00233 | 1.25% |
| Sb 206.836† | 21.5 | 0.01570 | mg/L | 0.000548 | 0.03140 mg/L | 0.001095 | 3.49% |
| Se 196.026† | 52.0 | 0.03828 | mg/L | 0.008238 | 0.07655 mg/L | 0.016476 | 21.52% |
| Si 288.158† | 4648.8 | 3.148 | mg/L | 0.0159 | 6.296 mg/L | 0.0319 | 0.51% |
| Sn 189.927† | -26.6 | -0.00190 | mg/L | 0.000996 | -0.00380 mg/L | 0.001993 | 52.46% |
| Sr 421.552† | 117101.8 | 0.1748 | mg/L | 0.00061 | 0.3496 mg/L | 0.00122 | 0.35% |
| Ti 334.903† | 167665.0 | 7.633 | mg/L | 0.0353 | 15.27 mg/L | 0.071 | 0.46% |
| Tl 190.801† | -35.1 | 0.00886 | mg/L | 0.005409 | 0.01772 mg/L | 0.010818 | 61.07% |
| V 292.402† | 41392.9 | 0.3997 | mg/L | 0.00202 | 0.7994 mg/L | 0.00404 | 0.51% |
| Zn 206.200† | 290.4 | 0.4235 | mg/L | 0.00722 | 0.8469 mg/L | 0.01445 | 1.71% |

Sequence No.: 17
 Sample ID: RG51 C SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 303
 Date Collected: 8/6/2010 3:01:34 PM
 Data Type: Original

Nebulizer Parameters: RG51 C SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 C SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2007295.4 | 105.6 | % | 0.12 | | | 0.12% |
| ScR 361.383 | 309718.8 | 105.8 | % | 2.88 | | | 2.72% |
| Ag 328.068† | -7.7 | -0.00037 | mg/L | 0.000155 | -0.00074 mg/L | 0.000310 | 41.75% |
| Al 308.215† | 191584.9 | 151.1 | mg/L | 4.64 | 302.3 mg/L | 9.28 | 3.07% |
| As 188.979† | -119.0 | 0.04698 | mg/L | 0.001669 | 0.09395 mg/L | 0.003338 | 3.55% |
| B 249.677† | 30.2 | 0.00852 | mg/L | 0.000273 | 0.01703 mg/L | 0.000546 | 3.20% |
| Ba 233.527† | 2459.5 | 0.7222 | mg/L | 0.01638 | 1.444 mg/L | 0.0328 | 2.27% |
| Be 313.042† | 1388.3 | 0.00213 | mg/L | 0.000123 | 0.00425 mg/L | 0.000246 | 5.79% |
| Ca 317.933† | 521959.7 | 35.95 | mg/L | 1.130 | 71.89 mg/L | 2.260 | 3.14% |
| Cd 228.802† | 109.8 | 0.00563 | mg/L | 0.000123 | 0.01127 mg/L | 0.000245 | 2.18% |
| Co 228.616† | 2502.0 | 0.06877 | mg/L | 0.000583 | 0.1375 mg/L | 0.00117 | 0.85% |
| Cr 267.716† | 1366.2 | 0.2662 | mg/L | 0.00464 | 0.5324 mg/L | 0.00928 | 1.74% |
| Cu 324.752† | 47731.9 | 0.1792 | mg/L | 0.00081 | 0.3583 mg/L | 0.00163 | 0.45% |
| Fe 273.955† | 187495.5 | 164.0 | mg/L | 4.78 | 327.9 mg/L | 9.56 | 2.92% |
| K 766.490† | 7144.0 | 4.916 | mg/L | 0.1427 | 9.832 mg/L | 0.2854 | 2.90% |
| Mg 279.077† | 47717.0 | 50.76 | mg/L | 1.454 | 101.5 mg/L | 2.91 | 2.87% |
| Mn 257.610† | 106434.0 | 3.377 | mg/L | 0.1015 | 6.755 mg/L | 0.2030 | 3.01% |
| Mo 202.031† | 98.4 | 0.00510 | mg/L | 0.000495 | 0.01020 mg/L | 0.000991 | 9.71% |
| Na 589.592† | 17076.3 | 1.432 | mg/L | 0.0442 | 2.865 mg/L | 0.0884 | 3.09% |
| Na 330.237† | -17.9 | 1.454 | mg/L | 0.0577 | 2.909 mg/L | 0.1155 | 3.97% |
| Ni 231.604† | 577.9 | 0.3393 | mg/L | 0.00813 | 0.6787 mg/L | 0.01626 | 2.40% |
| Pb 220.353† | 2098.9 | 0.2993 | mg/L | 0.00248 | 0.5985 mg/L | 0.00495 | 0.83% |
| Sb 206.836† | 29.7 | 0.01866 | mg/L | 0.001808 | 0.03732 mg/L | 0.003616 | 9.69% |
| Se 196.026† | 46.9 | 0.03448 | mg/L | 0.001796 | 0.06897 mg/L | 0.003592 | 5.21% |
| Si 288.158† | 3428.9 | 2.322 | mg/L | 0.0621 | 4.644 mg/L | 0.1242 | 2.67% |
| Sn 189.927† | -22.4 | -0.00116 | mg/L | 0.000853 | -0.00233 mg/L | 0.001706 | 73.31% |
| Sr 421.552† | 112071.6 | 0.1673 | mg/L | 0.00489 | 0.3346 mg/L | 0.00978 | 2.92% |
| Ti 334.903† | 156607.6 | 7.129 | mg/L | 0.2127 | 14.26 mg/L | 0.425 | 2.98% |
| Tl 190.801† | -35.6 | 0.00738 | mg/L | 0.004725 | 0.01475 mg/L | 0.009451 | 64.06% |
| V 292.402† | 37279.6 | 0.3590 | mg/L | 0.00092 | 0.7180 mg/L | 0.00184 | 0.26% |
| Zn 206.200† | 325.0 | 0.4744 | mg/L | 0.00767 | 0.9489 mg/L | 0.01534 | 1.62% |

Sequence No.: 18
 Sample ID: RG51 D SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 304
 Date Collected: 8/6/2010 3:05:30 PM
 Data Type: Original

Nebulizer Parameters: RG51 D SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 D SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2014653.5 | 105.9 | % | 0.78 | | | 0.74% |
| ScR 361.383 | 310329.4 | 106.0 | % | 1.67 | | | 1.57% |
| Ag 328.068† | -40.0 | -0.00031 | mg/L | 0.000090 | -0.00061 mg/L | 0.000180 | 29.47% |
| Al 308.215† | 193084.3 | 152.3 | mg/L | 2.29 | 304.6 mg/L | 4.59 | 1.51% |
| As 188.979† | -189.5 | 0.02749 | mg/L | 0.001778 | 0.05498 mg/L | 0.003555 | 6.47% |
| B 249.677† | 21.7 | 0.00603 | mg/L | 0.001423 | 0.01207 mg/L | 0.002847 | 23.59% |
| Ba 233.527† | 2011.9 | 0.5869 | mg/L | 0.00959 | 1.174 mg/L | 0.0192 | 1.63% |
| Be 313.042† | 1276.6 | 0.00190 | mg/L | 0.000050 | 0.00380 mg/L | 0.000099 | 2.61% |
| Ca 317.933† | 556404.7 | 38.32 | mg/L | 0.489 | 76.64 mg/L | 0.978 | 1.28% |
| Cd 228.802† | 50.2 | 0.00300 | mg/L | 0.000151 | 0.00601 mg/L | 0.000302 | 5.02% |
| Co 228.616† | 2602.1 | 0.06934 | mg/L | 0.000250 | 0.1387 mg/L | 0.00050 | 0.36% |
| Cr 267.716† | 1314.2 | 0.2558 | mg/L | 0.00490 | 0.5116 mg/L | 0.00979 | 1.91% |
| Cu 324.752† | 40142.1 | 0.1520 | mg/L | 0.00152 | 0.3040 mg/L | 0.00303 | 1.00% |
| Fe 273.955† | 199487.1 | 174.5 | mg/L | 2.41 | 348.9 mg/L | 4.83 | 1.38% |
| K 766.490† | 8602.5 | 5.920 | mg/L | 0.0977 | 11.84 mg/L | 0.195 | 1.65% |
| Mg 279.077† | 52816.7 | 56.18 | mg/L | 0.916 | 112.4 mg/L | 1.83 | 1.63% |
| Mn 257.610† | 76580.9 | 2.430 | mg/L | 0.0353 | 4.860 mg/L | 0.0706 | 1.45% |
| Mo 202.031† | 85.9 | 0.00433 | mg/L | 0.000309 | 0.00867 mg/L | 0.000619 | 7.13% |
| Na 589.592† | 17846.0 | 1.497 | mg/L | 0.0288 | 2.994 mg/L | 0.0575 | 1.92% |
| Na 330.237† | -28.4 | 1.579 | mg/L | 0.1676 | 3.158 mg/L | 0.3352 | 10.61% |
| Ni 231.604† | 588.8 | 0.3457 | mg/L | 0.00672 | 0.6915 mg/L | 0.01345 | 1.94% |
| Pb 220.353† | 172.7 | 0.03734 | mg/L | 0.000159 | 0.07468 mg/L | 0.000318 | 0.43% |
| Sb 206.836† | 20.3 | 0.01732 | mg/L | 0.002506 | 0.03463 mg/L | 0.005012 | 14.47% |
| Se 196.026† | 42.3 | 0.03068 | mg/L | 0.008167 | 0.06136 mg/L | 0.016333 | 26.62% |
| Si 288.158† | 3235.9 | 2.191 | mg/L | 0.0410 | 4.382 mg/L | 0.0821 | 1.87% |
| Sn 189.927† | -38.0 | -0.00457 | mg/L | 0.001109 | -0.00914 mg/L | 0.002218 | 24.27% |
| Sr 421.552† | 131477.1 | 0.1963 | mg/L | 0.00297 | 0.3925 mg/L | 0.00594 | 1.51% |
| Ti 334.903† | 191039.9 | 8.697 | mg/L | 0.1362 | 17.39 mg/L | 0.272 | 1.57% |
| Tl 190.801† | -33.0 | 0.00943 | mg/L | 0.003362 | 0.01886 mg/L | 0.006724 | 35.66% |
| V 292.402† | 40418.0 | 0.3887 | mg/L | 0.00524 | 0.7774 mg/L | 0.01048 | 1.35% |
| Zn 206.200† | 208.7 | 0.3031 | mg/L | 0.00578 | 0.6063 mg/L | 0.01156 | 1.91% |

Sequence No.: 19
 Sample ID: RG51 ADUP SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 305
 Date Collected: 8/6/2010 3:09:12 PM
 Data Type: Original

Nebulizer Parameters: RG51 ADUP SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 ADUP SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1993267.8 | 104.8 | % | 0.61 | | | 0.58% |
| ScR 361.383 | 313933.0 | 107.3 | % | 1.35 | | | 1.26% |
| Ag 328.068† | -101.8 | -0.00079 | mg/L | 0.000023 | -0.00157 mg/L | 0.000045 | 2.89% |
| Al 308.215† | 211380.3 | 166.7 | mg/L | 1.89 | 333.5 mg/L | 3.77 | 1.13% |
| As 188.979† | -201.3 | 0.02132 | mg/L | 0.003331 | 0.04264 mg/L | 0.006661 | 15.62% |
| B 249.677† | 25.4 | 0.00705 | mg/L | 0.002270 | 0.01410 mg/L | 0.004540 | 32.20% |
| Ba 233.527† | 2012.7 | 0.5838 | mg/L | 0.00540 | 1.168 mg/L | 0.0108 | 0.93% |
| Be 313.042† | 1405.8 | 0.00205 | mg/L | 0.000058 | 0.00410 mg/L | 0.000117 | 2.84% |
| Ca 317.933† | 793367.7 | 54.64 | mg/L | 0.810 | 109.3 mg/L | 1.62 | 1.48% |
| Cd 228.802† | 61.9 | 0.00355 | mg/L | 0.000169 | 0.00711 mg/L | 0.000338 | 4.75% |
| Co 228.616† | 3233.4 | 0.08965 | mg/L | 0.000375 | 0.1793 mg/L | 0.00075 | 0.42% |
| Cr 267.716† | 1412.4 | 0.2756 | mg/L | 0.00298 | 0.5512 mg/L | 0.00595 | 1.08% |
| Cu 324.752† | 84520.1 | 0.3135 | mg/L | 0.00239 | 0.6270 mg/L | 0.00478 | 0.76% |
| Fe 273.955† | 239073.0 | 209.1 | mg/L | 2.53 | 418.2 mg/L | 5.06 | 1.21% |
| K 766.490† | 9258.3 | 6.371 | mg/L | 0.0842 | 12.74 mg/L | 0.168 | 1.32% |
| Mg 279.077† | 56925.2 | 60.54 | mg/L | 0.454 | 121.1 mg/L | 0.91 | 0.75% |
| Mn 257.610† | 103528.7 | 3.285 | mg/L | 0.0222 | 6.571 mg/L | 0.0445 | 0.68% |
| Mo 202.031† | 119.4 | 0.00600 | mg/L | 0.000226 | 0.01200 mg/L | 0.000453 | 3.77% |
| Na 589.592† | 41346.2 | 3.468 | mg/L | 0.0412 | 6.936 mg/L | 0.0825 | 1.19% |
| Na 330.237† | 31.2 | 3.735 | mg/L | 0.1902 | 7.469 mg/L | 0.3805 | 5.09% |
| Ni 231.604† | 531.1 | 0.3119 | mg/L | 0.00357 | 0.6237 mg/L | 0.00715 | 1.15% |
| Pb 220.353† | 743.7 | 0.1147 | mg/L | 0.00036 | 0.2294 mg/L | 0.00073 | 0.32% |
| Sb 206.836† | 31.6 | 0.02192 | mg/L | 0.001509 | 0.04383 mg/L | 0.003017 | 6.88% |
| Se 196.026† | 45.1 | 0.03178 | mg/L | 0.006478 | 0.06357 mg/L | 0.012955 | 20.38% |
| Si 288.158† | 4763.3 | 3.225 | mg/L | 0.0488 | 6.451 mg/L | 0.0976 | 1.51% |
| Sn 189.927† | -37.4 | -0.00360 | mg/L | 0.002094 | -0.00720 mg/L | 0.004188 | 58.17% |
| Sr 421.552† | 238661.6 | 0.3563 | mg/L | 0.00416 | 0.7125 mg/L | 0.00832 | 1.17% |
| Ti 334.903† | 193826.5 | 8.823 | mg/L | 0.0996 | 17.65 mg/L | 0.199 | 1.13% |
| Tl 190.801† | -40.0 | 0.01134 | mg/L | 0.005702 | 0.02269 mg/L | 0.011403 | 50.26% |
| V 292.402† | 54214.6 | 0.5254 | mg/L | 0.00212 | 1.051 mg/L | 0.0042 | 0.40% |
| Zn 206.200† | 290.1 | 0.4226 | mg/L | 0.00431 | 0.8452 mg/L | 0.00862 | 1.02% |

Sequence No.: 20
 Sample ID: RG51 A SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 306
 Date Collected: 8/6/2010 3:13:09 PM
 Data Type: Original

Nebulizer Parameters: RG51 A SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 A SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2006678.2 | 105.5 | % | 2.09 | | | 1.98% |
| ScR 361.383 | 313637.7 | 107.2 | % | 1.39 | | | 1.29% |
| Ag 328.068† | -116.4 | -0.00087 | mg/L | 0.000079 | -0.00173 mg/L | 0.000158 | 9.14% |
| Al 308.215† | 216395.5 | 170.7 | mg/L | 1.48 | 341.4 mg/L | 2.97 | 0.87% |
| As 188.979† | -235.3 | 0.02311 | mg/L | 0.004671 | 0.04621 mg/L | 0.009343 | 20.22% |
| B 249.677† | 25.1 | 0.00696 | mg/L | 0.001254 | 0.01393 mg/L | 0.002509 | 18.01% |
| Ba 233.527† | 1931.3 | 0.5574 | mg/L | 0.00628 | 1.115 mg/L | 0.0126 | 1.13% |
| Be 313.042† | 1431.1 | 0.00205 | mg/L | 0.000091 | 0.00409 mg/L | 0.000182 | 4.44% |
| Ca 317.933† | 873699.0 | 60.17 | mg/L | 0.551 | 120.3 mg/L | 1.10 | 0.92% |
| Cd 228.802† | 66.7 | 0.00386 | mg/L | 0.000150 | 0.00773 mg/L | 0.000300 | 3.88% |
| Co 228.616† | 3464.0 | 0.09472 | mg/L | 0.002462 | 0.1894 mg/L | 0.00492 | 2.60% |
| Cr 267.716† | 1468.4 | 0.2866 | mg/L | 0.00363 | 0.5732 mg/L | 0.00727 | 1.27% |
| Cu 324.752† | 93917.3 | 0.3480 | mg/L | 0.00749 | 0.6960 mg/L | 0.01498 | 2.15% |
| Fe 273.955† | 262342.2 | 229.4 | mg/L | 1.94 | 458.9 mg/L | 3.89 | 0.85% |
| K 766.490† | 9283.0 | 6.388 | mg/L | 0.1079 | 12.78 mg/L | 0.216 | 1.69% |
| Mg 279.077† | 62227.0 | 66.18 | mg/L | 1.175 | 132.4 mg/L | 2.35 | 1.78% |
| Mn 257.610† | 113050.3 | 3.588 | mg/L | 0.0772 | 7.175 mg/L | 0.1543 | 2.15% |
| Mo 202.031† | 128.6 | 0.00644 | mg/L | 0.000273 | 0.01288 mg/L | 0.000546 | 4.24% |
| Na 589.592† | 50513.1 | 4.237 | mg/L | 0.0447 | 8.474 mg/L | 0.0894 | 1.06% |
| Na 330.237† | 39.7 | 4.438 | mg/L | 0.4505 | 8.875 mg/L | 0.9010 | 10.15% |
| Ni 231.604† | 542.7 | 0.3187 | mg/L | 0.00188 | 0.6374 mg/L | 0.00375 | 0.59% |
| Pb 220.353† | 675.7 | 0.1047 | mg/L | 0.00032 | 0.2094 mg/L | 0.00065 | 0.31% |
| Sb 206.836† | 26.0 | 0.02167 | mg/L | 0.000645 | 0.04334 mg/L | 0.001290 | 2.98% |
| Se 196.026† | 45.2 | 0.03153 | mg/L | 0.006081 | 0.06305 mg/L | 0.012162 | 19.29% |
| Si 288.158† | 3737.7 | 2.531 | mg/L | 0.0302 | 5.062 mg/L | 0.0604 | 1.19% |
| Sn 189.927† | -42.1 | -0.00399 | mg/L | 0.002375 | -0.00799 mg/L | 0.004750 | 59.46% |
| Sr 421.552† | 254192.2 | 0.3794 | mg/L | 0.00456 | 0.7589 mg/L | 0.00912 | 1.20% |
| Ti 334.903† | 224254.7 | 10.21 | mg/L | 0.099 | 20.42 mg/L | 0.197 | 0.97% |
| Tl 190.801† | -42.0 | 0.01344 | mg/L | 0.002279 | 0.02688 mg/L | 0.004559 | 16.96% |
| V 292.402† | 60304.0 | 0.5844 | mg/L | 0.01399 | 1.169 mg/L | 0.0280 | 2.39% |
| Zn 206.200† | 298.8 | 0.4353 | mg/L | 0.00455 | 0.8707 mg/L | 0.00910 | 1.04% |

Sequence No.: 21
 Sample ID: RG51 ASPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 307
 Date Collected: 8/6/2010 3:17:07 PM
 Data Type: Original

Nebulizer Parameters: RG51 ASPK SWC

Analyte Back Pressure Flow
 All 202.0 kPa 0.75 L/min

Mean Data: RG51 ASPK SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------|----------|--------------------|----------|--------|
| ScA 357.253 | 2036782.0 | 107.1 | % | 0.90 | | | 0.84% |
| ScR 361.383 | 317622.4 | 108.5 | % | 2.31 | | | 2.13% |
| Ag 328.068† | 84828.9 | 0.4782 | mg/L | 0.00045 | 0.9564 mg/L | 0.00091 | 0.09% |
| Al 308.215† | 222568.0 | 175.6 | mg/L | 3.96 | 351.1 mg/L | 7.92 | 2.25% |
| As 188.979† | 2642.7 | 1.955 | mg/L | 0.0108 | 3.910 mg/L | 0.0215 | 0.55% |
| B 249.677† | 28.7 | 0.00675 | mg/L | 0.000748 | 0.01349 mg/L | 0.001496 | 11.09% |
| Ba 233.527† | 8356.7 | 2.486 | mg/L | 0.0540 | 4.973 mg/L | 0.1081 | 2.17% |
| Be 313.042† | 279380.5 | 0.4829 | mg/L | 0.01300 | 0.9659 mg/L | 0.02599 | 2.69% |
| Ca 317.933† | 1008921.0 | 69.48 | mg/L | 1.879 | 139.0 mg/L | 3.76 | 2.70% |
| Cd 228.802† | 11339.9 | 0.5259 | mg/L | 0.00756 | 1.052 mg/L | 0.0151 | 1.44% |
| Co 228.616† | 18243.6 | 0.5869 | mg/L | 0.00857 | 1.174 mg/L | 0.0171 | 1.46% |
| Cr 267.716† | 3768.4 | 0.7331 | mg/L | 0.01514 | 1.466 mg/L | 0.0303 | 2.06% |
| Cu 324.752† | 218812.1 | 0.7951 | mg/L | 0.00184 | 1.590 mg/L | 0.0037 | 0.23% |
| Fe 273.955† | 239946.6 | 209.8 | mg/L | 4.98 | 419.7 mg/L | 9.96 | 2.37% |
| K 766.490† | 24276.4 | 16.71 | mg/L | 0.416 | 33.41 mg/L | 0.833 | 2.49% |
| Mg 279.077† | 62192.8 | 66.15 | mg/L | 1.360 | 132.3 mg/L | 2.72 | 2.06% |
| Mn 257.610† | 120699.9 | 3.831 | mg/L | 0.0950 | 7.661 mg/L | 0.1901 | 2.48% |
| Mo 202.031† | 120.6 | 0.00581 | mg/L | 0.000282 | 0.01163 mg/L | 0.000564 | 4.85% |
| Na 589.592† | 166589.5 | 13.97 | mg/L | 0.342 | 27.95 mg/L | 0.683 | 2.45% |
| Na 330.237† | 359.3 | 15.07 | mg/L | 0.062 | 30.14 mg/L | 0.125 | 0.41% |
| Ni 231.604† | 1273.8 | 0.7480 | mg/L | 0.01580 | 1.496 mg/L | 0.0316 | 2.11% |
| Pb 220.353† | 14560.9 | 1.992 | mg/L | 0.0230 | 3.983 mg/L | 0.0459 | 1.15% |
| Sb 206.836† | 39.1 | 0.02185 | mg/L | 0.001653 | 0.04370 mg/L | 0.003306 | 7.57% |
| Se 196.026† | 2546.4 | 2.000 | mg/L | 0.0244 | 4.001 mg/L | 0.0487 | 1.22% |
| Si 288.158† | 2197.4 | 1.490 | mg/L | 0.0364 | 2.980 mg/L | 0.0727 | 2.44% |
| Sn 189.927† | -41.7 | -0.00394 | mg/L | 0.002013 | -0.00788 mg/L | 0.004026 | 51.06% |
| Sr 421.552† | 578830.6 | 0.8641 | mg/L | 0.01908 | 1.728 mg/L | 0.0382 | 2.21% |
| Ti 334.903† | 199893.7 | 9.098 | mg/L | 0.2025 | 18.20 mg/L | 0.405 | 2.23% |
| Tl 190.801† | 3356.1 | 1.887 | mg/L | 0.0118 | 3.773 mg/L | 0.0235 | 0.62% |
| V 292.402† | 100632.7 | 0.9992 | mg/L | 0.00258 | 1.998 mg/L | 0.0052 | 0.26% |
| Zn 206.200† | 593.0 | 0.8686 | mg/L | 0.01417 | 1.737 mg/L | 0.0283 | 1.63% |

Sequence No.: 22

Autosampler Location: 308

Sample ID: ~~RF71 APOST SWC~~ 222222

Date Collected: 8/6/2010 3:20:50 PM

Analyst: ALA

Data Type: Original

Dilution: 2X

#8910

Nebulizer Parameters: RF71 APOST SWC

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 203.0 kPa | 0.75 L/min |

Mean Data: RF71 APOST SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1980734.8 | 104.2 | % | 1.85 | | | 1.78% |
| ScR 361.383 | 309824.0 | 105.9 | % | 1.19 | | | 1.12% |
| Ag 328.068† | 85574.6 | 0.4826 | mg/L | 0.01143 | 0.9651 mg/L | 0.02286 | 2.37% |
| Al 308.215† | 157477.6 | 124.2 | mg/L | 0.91 | 248.4 mg/L | 1.82 | 0.73% |
| As 188.979† | 2830.7 | 2.028 | mg/L | 0.0354 | 4.055 mg/L | 0.0708 | 1.75% |
| B 249.677† | 266.8 | 0.07550 | mg/L | 0.000932 | 0.1510 mg/L | 0.00186 | 1.23% |
| Ba 233.527† | 7426.7 | 2.210 | mg/L | 0.0276 | 4.420 mg/L | 0.0552 | 1.25% |
| Be 313.042† | 274289.8 | 0.4742 | mg/L | 0.00431 | 0.9485 mg/L | 0.00862 | 0.91% |
| Ca 317.933† | 630581.6 | 43.43 | mg/L | 0.375 | 86.86 mg/L | 0.750 | 0.86% |
| Cd 228.802† | 11279.2 | 0.5226 | mg/L | 0.01021 | 1.045 mg/L | 0.0204 | 1.95% |
| Co 228.616† | 17450.8 | 0.5661 | mg/L | 0.01146 | 1.132 mg/L | 0.0229 | 2.02% |
| Cr 267.716† | 3956.8 | 0.7681 | mg/L | 0.01066 | 1.536 mg/L | 0.0213 | 1.39% |
| Cu 324.752† | 229078.5 | 0.8311 | mg/L | 0.01735 | 1.662 mg/L | 0.0347 | 2.09% |
| Fe 273.955† | 212039.5 | 185.4 | mg/L | 1.45 | 370.9 mg/L | 2.90 | 0.78% |
| K 766.490† | 30559.4 | 21.03 | mg/L | 0.241 | 42.06 mg/L | 0.482 | 1.15% |
| Mg 279.077† | 69637.7 | 74.10 | mg/L | 0.552 | 148.2 mg/L | 1.10 | 0.75% |
| Mn 257.610† | 76763.8 | 2.437 | mg/L | 0.0265 | 4.873 mg/L | 0.0530 | 1.09% |
| Mo 202.031† | 217.7 | 0.01191 | mg/L | 0.000517 | 0.02382 mg/L | 0.001034 | 4.34% |
| Na 589.592† | 312889.6 | 26.24 | mg/L | 0.273 | 52.49 mg/L | 0.547 | 1.04% |
| Na 330.237† | 773.6 | 28.27 | mg/L | 0.475 | 56.53 mg/L | 0.949 | 1.68% |
| Ni 231.604† | 1264.1 | 0.7438 | mg/L | 0.00723 | 1.488 mg/L | 0.0145 | 0.97% |
| Pb 220.353† | 14899.1 | 2.030 | mg/L | 0.0362 | 4.061 mg/L | 0.0723 | 1.78% |
| Sb 206.836† | 5714.4 | 2.131 | mg/L | 0.0389 | 4.262 mg/L | 0.0778 | 1.82% |
| Se 196.026† | 2600.2 | 2.045 | mg/L | 0.0449 | 4.089 mg/L | 0.0898 | 2.19% |
| Si 288.158† | 12698.7 | 8.601 | mg/L | 0.1241 | 17.20 mg/L | 0.248 | 1.44% |
| Sn 189.927† | 5.3 | 0.00758 | mg/L | 0.001287 | 0.01515 mg/L | 0.002574 | 16.99% |
| Sr 421.552† | 491104.9 | 0.7331 | mg/L | 0.00672 | 1.466 mg/L | 0.0134 | 0.92% |
| Ti 334.903† | 132559.4 | 6.034 | mg/L | 0.0535 | 12.07 mg/L | 0.107 | 0.89% |
| Tl 190.801† | 3368.9 | 1.889 | mg/L | 0.0329 | 3.778 mg/L | 0.0658 | 1.74% |
| V 292.402† | 86154.5 | 0.8563 | mg/L | 0.01534 | 1.713 mg/L | 0.0307 | 1.79% |
| Zn 206.200† | 723.2 | 1.062 | mg/L | 0.0141 | 2.124 mg/L | 0.0281 | 1.32% |

Sequence No.: 23
 Sample ID: RG51 REF1 SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 309
 Date Collected: 8/6/2010 3:24:33 PM
 Data Type: Original

Nebulizer Parameters: RG51 REF1 SWC

Analyte Back Pressure Flow
 All 193.0 kPa 0.75 L/min

Mean Data: RG51 REF1 SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------|--------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1980165.0 | 104.1 | % | 1.42 | | | 1.37% |
| ScR 361.383 | 297894.2 | 101.8 | % | 6.42 | | | 6.31% |
| Ag 328.068† | 186046.5 | 1.049 | mg/L | 0.0142 | 2.097 mg/L | 0.0284 | 1.35% |
| Al 308.215† | 127166.8 | 100.3 | mg/L | 6.40 | 200.6 mg/L | 12.79 | 6.38% |
| As 188.979† | 1979.4 | 1.384 | mg/L | 0.0187 | 2.767 mg/L | 0.0374 | 1.35% |
| B 249.677† | 4033.7 | 1.162 | mg/L | 0.0674 | 2.323 mg/L | 0.1348 | 5.80% |
| Ba 233.527† | 11106.0 | 3.316 | mg/L | 0.2097 | 6.633 mg/L | 0.4194 | 6.32% |
| Be 313.042† | 535362.4 | 0.9262 | mg/L | 0.05707 | 1.852 mg/L | 0.1141 | 6.16% |
| Ca 317.933† | 629311.6 | 43.34 | mg/L | 2.790 | 86.68 mg/L | 5.579 | 6.44% |
| Cd 228.802† | 16039.2 | 0.7476 | mg/L | 0.00953 | 1.495 mg/L | 0.0191 | 1.27% |
| Co 228.616† | 24520.8 | 0.8072 | mg/L | 0.00984 | 1.614 mg/L | 0.0197 | 1.22% |
| Cr 267.716† | 3911.1 | 0.7634 | mg/L | 0.04715 | 1.527 mg/L | 0.0943 | 6.18% |
| Cu 324.752† | 194355.7 | 0.7065 | mg/L | 0.01035 | 1.413 mg/L | 0.0207 | 1.46% |
| Fe 273.955† | 178540.7 | 156.1 | mg/L | 10.19 | 312.3 mg/L | 20.38 | 6.53% |
| K 766.490† | 58771.2 | 40.44 | mg/L | 2.367 | 80.89 mg/L | 4.733 | 5.85% |
| Mg 279.077† | 29175.4 | 31.01 | mg/L | 1.982 | 62.01 mg/L | 3.963 | 6.39% |
| Mn 257.610† | 143132.5 | 4.543 | mg/L | 0.2921 | 9.085 mg/L | 0.5841 | 6.43% |
| Mo 202.031† | 8442.7 | 0.4904 | mg/L | 0.00659 | 0.9808 mg/L | 0.01318 | 1.34% |
| Na 589.592† | 68897.0 | 5.779 | mg/L | 0.3566 | 11.56 mg/L | 0.713 | 6.17% |
| Na 330.237† | 153.3 | 5.753 | mg/L | 0.4739 | 11.51 mg/L | 0.948 | 8.24% |
| Ni 231.604† | 989.6 | 0.5814 | mg/L | 0.03671 | 1.163 mg/L | 0.0734 | 6.31% |
| Pb 220.353† | 9559.6 | 1.304 | mg/L | 0.0178 | 2.608 mg/L | 0.0356 | 1.36% |
| Sb 206.836† | 1352.4 | 0.5229 | mg/L | 0.00788 | 1.046 mg/L | 0.0158 | 1.51% |
| Se 196.026† | 2252.8 | 1.771 | mg/L | 0.0316 | 3.542 mg/L | 0.0633 | 1.79% |
| Si 288.158† | 4274.1 | 2.897 | mg/L | 0.1901 | 5.794 mg/L | 0.3802 | 6.56% |
| Sn 189.927† | 6666.9 | 1.817 | mg/L | 0.0228 | 3.633 mg/L | 0.0456 | 1.25% |
| Sr 421.552† | 388980.5 | 0.5807 | mg/L | 0.03655 | 1.161 mg/L | 0.0731 | 6.29% |
| Ti 334.903† | 52254.8 | 2.376 | mg/L | 0.1517 | 4.752 mg/L | 0.3035 | 6.39% |
| Tl 190.801† | 2448.6 | 1.379 | mg/L | 0.0137 | 2.758 mg/L | 0.0275 | 1.00% |
| V 292.402† | 86403.7 | 0.8647 | mg/L | 0.01102 | 1.729 mg/L | 0.0220 | 1.27% |
| Zn 206.200† | 1229.9 | 1.809 | mg/L | 0.1172 | 3.618 mg/L | 0.2345 | 6.48% |

Sequence No.: 24
Sample ID: RG51 MBSPK SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 310
Date Collected: 8/6/2010 3:28:16 PM
Data Type: Original

Nebulizer Parameters: RG51 MBSPK SWC
Analyte Back Pressure Flow
All 199.0 kPa 0.75 L/min

Mean Data: RG51 MBSPK SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1953076.9 | 102.7 % | 1.99 | | | 1.94% |
| ScR 361.383 | 298759.2 | 102.1 % | 3.69 | | | 3.61% |
| Ag 328.068† | 95514.2 | 0.5387 mg/L | 0.01163 | 1.077 mg/L | 0.0233 | 2.16% |
| Al 308.215† | 2766.7 | 2.173 mg/L | 0.0830 | 4.345 mg/L | 0.1660 | 3.82% |
| As 188.979† | 3076.7 | 2.087 mg/L | 0.0380 | 4.173 mg/L | 0.0759 | 1.82% |
| B 249.677† | 3.5 | -0.00034 mg/L | 0.002231 | -0.00067 mg/L | 0.004462 | 661.53% |
| Ba 233.527† | 6821.7 | 2.046 mg/L | 0.0724 | 4.092 mg/L | 0.1448 | 3.54% |
| Be 313.042† | 288635.7 | 0.4993 mg/L | 0.02146 | 0.9986 mg/L | 0.04292 | 4.30% |
| Ca 317.933† | 155369.6 | 10.70 mg/L | 0.476 | 21.40 mg/L | 0.953 | 4.45% |
| Cd 228.802† | 11691.1 | 0.5412 mg/L | 0.00664 | 1.082 mg/L | 0.0133 | 1.23% |
| Co 228.616† | 16063.3 | 0.5326 mg/L | 0.00836 | 1.065 mg/L | 0.0167 | 1.57% |
| Cr 267.716† | 2671.0 | 0.5182 mg/L | 0.01922 | 1.036 mg/L | 0.0384 | 3.71% |
| Cu 324.752† | 141020.8 | 0.5058 mg/L | 0.01230 | 1.012 mg/L | 0.0246 | 2.43% |
| Fe 273.955† | 2587.5 | 2.260 mg/L | 0.0877 | 4.520 mg/L | 0.1754 | 3.88% |
| K 766.490† | 15990.7 | 11.00 mg/L | 0.456 | 22.01 mg/L | 0.912 | 4.14% |
| Mg 279.077† | 10066.2 | 10.72 mg/L | 0.394 | 21.45 mg/L | 0.788 | 3.68% |
| Mn 257.610† | 15375.5 | 0.4884 mg/L | 0.01951 | 0.9768 mg/L | 0.03902 | 3.99% |
| Mo 202.031† | 27.5 | 0.00142 mg/L | 0.000439 | 0.00283 mg/L | 0.000878 | 30.99% |
| Na 589.592† | 117966.5 | 9.895 mg/L | 0.3984 | 19.79 mg/L | 0.797 | 4.03% |
| Na 330.237† | 316.3 | 10.82 mg/L | 0.286 | 21.64 mg/L | 0.572 | 2.64% |
| Ni 231.604† | 867.9 | 0.5096 mg/L | 0.01790 | 1.019 mg/L | 0.0358 | 3.51% |
| Pb 220.353† | 14970.9 | 2.032 mg/L | 0.0423 | 4.065 mg/L | 0.0846 | 2.08% |
| Sb 206.836† | 19.5 | 0.00361 mg/L | 0.002076 | 0.00721 mg/L | 0.004153 | 57.56% |
| Se 196.026† | 2669.7 | 2.102 mg/L | 0.0401 | 4.203 mg/L | 0.0803 | 1.91% |
| Si 288.158† | 12.3 | 0.01027 mg/L | 0.002540 | 0.02054 mg/L | 0.005080 | 24.73% |
| Sn 189.927† | -5.3 | -0.00095 mg/L | 0.000717 | -0.00191 mg/L | 0.001435 | 75.21% |
| Sr 421.552† | 335925.7 | 0.5015 mg/L | 0.01877 | 1.003 mg/L | 0.0375 | 3.74% |
| Ti 334.903† | 49.2 | 0.00148 mg/L | 0.000224 | 0.00296 mg/L | 0.000448 | 15.14% |
| Tl 190.801† | 3745.6 | 2.069 mg/L | 0.0429 | 4.137 mg/L | 0.0858 | 2.07% |
| V 292.402† | 53379.5 | 0.5448 mg/L | 0.00893 | 1.090 mg/L | 0.0179 | 1.64% |
| Zn 206.200† | 339.5 | 0.5001 mg/L | 0.01864 | 1.000 mg/L | 0.0373 | 3.73% |

Sequence No.: 25
 Sample ID: CV 10
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 7
 Date Collected: 8/6/2010 3:32:27 PM
 Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1940284.8 | 102.0 % | 0.13 | | | 0.13% |
| ScR 361.383 | 291911.3 | 99.74 % | 1.733 | | | 1.74% |
| Ag 328.068† | 187908.8 | 1.060 mg/L | 0.0071 | 1.060 mg/L | 0.0071 | 0.67% |
| Al 308.215† | 2829.1 | 2.198 mg/L | 0.0407 | 2.198 mg/L | 0.0407 | 1.85% |
| As 188.979† | 3074.8 | 2.103 mg/L | 0.0034 | 2.103 mg/L | 0.0034 | 0.16% |
| B 249.677† | 3533.0 | 1.017 mg/L | 0.0168 | 1.017 mg/L | 0.0168 | 1.65% |
| Ba 233.527† | 3485.9 | 1.045 mg/L | 0.0190 | 1.045 mg/L | 0.0190 | 1.81% |
| Be 313.042† | 587222.3 | 1.016 mg/L | 0.0178 | 1.016 mg/L | 0.0178 | 1.75% |
| Ca 317.933† | 33248.5 | 2.290 mg/L | 0.0420 | 2.290 mg/L | 0.0420 | 1.83% |
| Cd 228.802† | 23710.5 | 1.105 mg/L | 0.0082 | 1.105 mg/L | 0.0082 | 0.74% |
| Co 228.616† | 32723.5 | 1.084 mg/L | 0.0105 | 1.084 mg/L | 0.0105 | 0.97% |
| Cr 267.716† | 5457.4 | 1.062 mg/L | 0.0169 | 1.062 mg/L | 0.0169 | 1.59% |
| Cu 324.752† | 298958.9 | 1.071 mg/L | 0.0084 | 1.071 mg/L | 0.0084 | 0.78% |
| Fe 273.955† | 2529.2 | 2.206 mg/L | 0.0435 | 2.206 mg/L | 0.0435 | 1.97% |
| K 766.490† | 32712.2 | 22.51 mg/L | 0.492 | 22.51 mg/L | 0.492 | 2.19% |
| Mg 279.077† | 2087.2 | 2.229 mg/L | 0.0424 | 2.229 mg/L | 0.0424 | 1.90% |
| Mn 257.610† | 31601.9 | 1.003 mg/L | 0.0213 | 1.003 mg/L | 0.0213 | 2.12% |
| Mo 202.031† | 18225.9 | 1.060 mg/L | 0.0079 | 1.060 mg/L | 0.0079 | 0.75% |
| Na 589.592† | 603221.0 | 50.60 mg/L | 0.727 | 50.60 mg/L | 0.727 | 1.44% |
| Na 330.237† | 1607.0 | 55.31 mg/L | 1.257 | 55.31 mg/L | 1.257 | 2.27% |
| Ni 231.604† | 1796.5 | 1.057 mg/L | 0.0190 | 1.057 mg/L | 0.0190 | 1.80% |
| Pb 220.353† | 15062.2 | 2.045 mg/L | 0.0137 | 2.045 mg/L | 0.0137 | 0.67% |
| Sb 206.836† | 6014.7 | 2.247 mg/L | 0.0016 | 2.247 mg/L | 0.0016 | 0.07% |
| Se 196.026† | 2672.2 | 2.104 mg/L | 0.0070 | 2.104 mg/L | 0.0070 | 0.33% |
| Si 288.158† | 3377.2 | 2.291 mg/L | 0.0481 | 2.291 mg/L | 0.0481 | 2.10% |
| Sn 189.927† | 4074.7 | 1.110 mg/L | 0.0030 | 1.110 mg/L | 0.0030 | 0.27% |
| Sr 421.552† | 688427.1 | 1.028 mg/L | 0.0141 | 1.028 mg/L | 0.0141 | 1.37% |
| Ti 334.903† | 23704.2 | 1.078 mg/L | 0.0216 | 1.078 mg/L | 0.0216 | 2.01% |
| Tl 190.801† | 3761.4 | 2.079 mg/L | 0.0016 | 2.079 mg/L | 0.0016 | 0.08% |
| V 292.402† | 106180.7 | 1.084 mg/L | 0.0112 | 1.084 mg/L | 0.0112 | 1.03% |
| Zn 206.200† | 707.8 | 1.042 mg/L | 0.0173 | 1.042 mg/L | 0.0173 | 1.66% |

Sequence No.: 26
 Sample ID: CB (0)
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 3:36:41 PM
 Data Type: Original

Nebulizer Parameters: CB

Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1956052.5 | 102.9 % | % | 0.69 | | | 0.67% |
| ScR 361.383 | 278421.1 | 95.13 % | % | 0.412 | | | 0.43% |
| Ag 328.068† | -5.7 | -0.00003 mg/L | mg/L | 0.000035 | -0.00003 mg/L | 0.000035 | 108.65% |
| Al 308.215† | 1.1 | 0.00085 mg/L | mg/L | 0.011272 | 0.00085 mg/L | 0.011272 | >999.9% |
| As 188.979† | -0.5 | -0.00034 mg/L | mg/L | 0.001480 | -0.00034 mg/L | 0.001480 | 438.71% |
| B 249.677† | -9.2 | -0.00266 mg/L | mg/L | 0.001086 | -0.00266 mg/L | 0.001086 | 40.90% |
| Ba 233.527† | 8.5 | 0.00254 mg/L | mg/L | 0.000350 | 0.00254 mg/L | 0.000350 | 13.80% |
| Be 313.042† | 189.9 | 0.00033 mg/L | mg/L | 0.000086 | 0.00033 mg/L | 0.000086 | 26.07% |
| Ca 317.933† | 1.3 | 0.00009 mg/L | mg/L | 0.000799 | 0.00009 mg/L | 0.000799 | 893.21% |
| Cd 228.802† | -4.8 | -0.00022 mg/L | mg/L | 0.000268 | -0.00022 mg/L | 0.000268 | 122.09% |
| Co 228.616† | 7.9 | 0.00026 mg/L | mg/L | 0.000254 | 0.00026 mg/L | 0.000254 | 96.75% |
| Cr 267.716† | -2.3 | -0.00044 mg/L | mg/L | 0.001280 | -0.00044 mg/L | 0.001280 | 288.48% |
| Cu 324.752† | 536.9 | 0.00193 mg/L | mg/L | 0.000307 | 0.00193 mg/L | 0.000307 | 15.93% |
| Fe 273.955† | -0.9 | -0.00077 mg/L | mg/L | 0.002210 | -0.00077 mg/L | 0.002210 | 288.61% |
| K 766.490† | 92.0 | 0.06330 mg/L | mg/L | 0.026816 | 0.06330 mg/L | 0.026816 | 42.36% |
| Mg 279.077† | -5.5 | -0.00587 mg/L | mg/L | 0.010659 | -0.00587 mg/L | 0.010659 | 181.58% |
| Mn 257.610† | 7.6 | 0.00024 mg/L | mg/L | 0.000063 | 0.00024 mg/L | 0.000063 | 26.09% |
| Mo 202.031† | 4.5 | 0.00026 mg/L | mg/L | 0.000257 | 0.00026 mg/L | 0.000257 | 97.79% |
| Na 589.592† | 110.9 | 0.00930 mg/L | mg/L | 0.001181 | 0.00930 mg/L | 0.001181 | 12.70% |
| Na 330.237† | 7.1 | 0.2444 mg/L | mg/L | 0.35917 | 0.2444 mg/L | 0.35917 | 146.95% |
| Ni 231.604† | 5.7 | 0.00337 mg/L | mg/L | 0.000654 | 0.00337 mg/L | 0.000654 | 19.42% |
| Pb 220.353† | -2.6 | -0.00035 mg/L | mg/L | 0.001035 | -0.00035 mg/L | 0.001035 | 293.37% |
| Sb 206.836† | 12.0 | 0.00449 mg/L | mg/L | 0.001456 | 0.00449 mg/L | 0.001456 | 32.45% |
| Se 196.026† | 7.4 | 0.00586 mg/L | mg/L | 0.006703 | 0.00586 mg/L | 0.006703 | 114.41% |
| Si 288.158† | 16.2 | 0.01094 mg/L | mg/L | 0.002193 | 0.01094 mg/L | 0.002193 | 20.05% |
| Sn 189.927† | 2.2 | 0.00061 mg/L | mg/L | 0.001000 | 0.00061 mg/L | 0.001000 | 163.14% |
| Sr 421.552† | 121.6 | 0.00018 mg/L | mg/L | 0.000074 | 0.00018 mg/L | 0.000074 | 40.86% |
| Ti 334.903† | -11.4 | -0.00052 mg/L | mg/L | 0.000365 | -0.00052 mg/L | 0.000365 | 70.21% |
| Tl 190.801† | 3.6 | 0.00200 mg/L | mg/L | 0.001393 | 0.00200 mg/L | 0.001393 | 69.51% |
| V 292.402† | 16.0 | 0.00016 mg/L | mg/L | 0.000202 | 0.00016 mg/L | 0.000202 | 124.49% |
| Zn 206.200† | 0.2 | 0.00026 mg/L | mg/L | 0.002670 | 0.00026 mg/L | 0.002670 | >999.9% |

Sequence No.: 27
 Sample ID: RG51 F SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 311
 Date Collected: 8/6/2010 3:40:37 PM
 Data Type: Original

Nebulizer Parameters: RG51 F SWC
 Analyte Back Pressure Flow
 All 199.0 kPa 0.75 L/min

Mean Data: RG51 F SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2006157.7 | 105.5 | % | 1.45 | | | 1.37% |
| ScR 361.383 | 307636.9 | 105.1 | % | 2.02 | | | 1.93% |
| Ag 328.068† | -71.0 | -0.00058 | mg/L | 0.000368 | -0.00116 mg/L | 0.000735 | 63.31% |
| Al 308.215† | 207523.2 | 163.7 | mg/L | 3.05 | 327.4 mg/L | 6.09 | 1.86% |
| As 188.979† | -214.9 | 0.03017 | mg/L | 0.002200 | 0.06034 mg/L | 0.004399 | 7.29% |
| B 249.677† | 30.3 | 0.00849 | mg/L | 0.003149 | 0.01698 mg/L | 0.006298 | 37.10% |
| Ba 233.527† | 2033.5 | 0.5894 | mg/L | 0.01329 | 1.179 mg/L | 0.0266 | 2.25% |
| Be 313.042† | 1375.5 | 0.00203 | mg/L | 0.000080 | 0.00405 mg/L | 0.000161 | 3.96% |
| Ca 317.933† | 707891.4 | 48.75 | mg/L | 0.864 | 97.50 mg/L | 1.729 | 1.77% |
| Cd 228.802† | 59.6 | 0.00348 | mg/L | 0.000199 | 0.00697 mg/L | 0.000398 | 5.71% |
| Co 228.616† | 3067.2 | 0.08235 | mg/L | 0.001195 | 0.1647 mg/L | 0.00239 | 1.45% |
| Cr 267.716† | 1911.0 | 0.3722 | mg/L | 0.00835 | 0.7445 mg/L | 0.01669 | 2.24% |
| Cu 324.752† | 47889.3 | 0.1822 | mg/L | 0.00284 | 0.3643 mg/L | 0.00568 | 1.56% |
| Fe 273.955† | 248155.4 | 217.0 | mg/L | 4.03 | 434.0 mg/L | 8.07 | 1.86% |
| K 766.490† | 9671.4 | 6.655 | mg/L | 0.1308 | 13.31 mg/L | 0.262 | 1.96% |
| Mg 279.077† | 63544.0 | 67.59 | mg/L | 1.171 | 135.2 mg/L | 2.34 | 1.73% |
| Mn 257.610† | 101066.8 | 3.207 | mg/L | 0.0618 | 6.414 mg/L | 0.1236 | 1.93% |
| Mo 202.031† | 189.7 | 0.01019 | mg/L | 0.000267 | 0.02038 mg/L | 0.000535 | 2.62% |
| Na 589.592† | 25673.7 | 2.153 | mg/L | 0.0426 | 4.307 mg/L | 0.0853 | 1.98% |
| Na 330.237† | -22.7 | 2.137 | mg/L | 0.4260 | 4.273 mg/L | 0.8521 | 19.94% |
| Ni 231.604† | 539.4 | 0.3168 | mg/L | 0.00831 | 0.6335 mg/L | 0.01663 | 2.62% |
| Pb 220.353† | 132.7 | 0.03107 | mg/L | 0.002040 | 0.06213 mg/L | 0.004080 | 6.57% |
| Sb 206.836† | 40.1 | 0.02507 | mg/L | 0.002930 | 0.05015 mg/L | 0.005860 | 11.69% |
| Se 196.026† | 48.3 | 0.03476 | mg/L | 0.003380 | 0.06952 mg/L | 0.006760 | 9.72% |
| Si 288.158† | 3537.9 | 2.396 | mg/L | 0.0515 | 4.791 mg/L | 0.1031 | 2.15% |
| Sn 189.927† | -38.4 | -0.00368 | mg/L | 0.000420 | -0.00735 mg/L | 0.000839 | 11.42% |
| Sr 421.552† | 186620.1 | 0.2786 | mg/L | 0.00505 | 0.5572 mg/L | 0.01009 | 1.81% |
| Ti 334.903† | 215725.9 | 9.821 | mg/L | 0.1820 | 19.64 mg/L | 0.364 | 1.85% |
| Tl 190.801† | -45.0 | 0.00983 | mg/L | 0.007001 | 0.01965 mg/L | 0.014002 | 71.25% |
| V 292.402† | 46382.2 | 0.4447 | mg/L | 0.00693 | 0.8895 mg/L | 0.01386 | 1.56% |
| Zn 206.200† | 241.6 | 0.3512 | mg/L | 0.00675 | 0.7024 mg/L | 0.01349 | 1.92% |

Sequence No.: 28
 Sample ID: RG51 G SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 312
 Date Collected: 8/6/2010 3:44:23 PM
 Data Type: Original

Nebulizer Parameters: RG51 G SWC

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 200.0 kPa | 0.75 L/min |

Mean Data: RG51 G SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1991592.1 | 104.7 | % | 0.39 | | | 0.37% |
| ScR 361.383 | 307583.3 | 105.1 | % | 2.15 | | | 2.05% |
| Ag 328.068† | -83.1 | -0.00079 | mg/L | 0.000300 | -0.00159 mg/L | 0.000601 | 37.81% |
| Al 308.215† | 195179.6 | 154.0 | mg/L | 3.14 | 307.9 mg/L | 6.27 | 2.04% |
| As 188.979† | -134.5 | 0.04073 | mg/L | 0.002811 | 0.08146 mg/L | 0.005622 | 6.90% |
| B 249.677† | 28.3 | 0.00796 | mg/L | 0.000933 | 0.01592 mg/L | 0.001867 | 11.72% |
| Ba 233.527† | 2632.3 | 0.7729 | mg/L | 0.01685 | 1.546 mg/L | 0.0337 | 2.18% |
| Be 313.042† | 1419.5 | 0.00216 | mg/L | 0.000168 | 0.00433 mg/L | 0.000337 | 7.78% |
| Ca 317.933† | 526800.3 | 36.28 | mg/L | 0.886 | 72.56 mg/L | 1.771 | 2.44% |
| Cd 228.802† | 102.6 | 0.00532 | mg/L | 0.000032 | 0.01065 mg/L | 0.000065 | 0.61% |
| Co 228.616† | 2570.6 | 0.07048 | mg/L | 0.000516 | 0.1410 mg/L | 0.00103 | 0.73% |
| Cr 267.716† | 1486.3 | 0.2901 | mg/L | 0.00784 | 0.5803 mg/L | 0.01569 | 2.70% |
| Cu 324.752† | 47179.0 | 0.1780 | mg/L | 0.00038 | 0.3560 mg/L | 0.00076 | 0.21% |
| Fe 273.955† | 201895.8 | 176.6 | mg/L | 3.81 | 353.1 mg/L | 7.63 | 2.16% |
| K 766.490† | 8110.7 | 5.581 | mg/L | 0.1642 | 11.16 mg/L | 0.328 | 2.94% |
| Mg 279.077† | 47657.8 | 50.69 | mg/L | 1.165 | 101.4 mg/L | 2.33 | 2.30% |
| Mn 257.610† | 107996.7 | 3.427 | mg/L | 0.0843 | 6.854 mg/L | 0.1686 | 2.46% |
| Mo 202.031† | 403.2 | 0.02283 | mg/L | 0.000208 | 0.04565 mg/L | 0.000417 | 0.91% |
| Na 589.592† | 19770.6 | 1.658 | mg/L | 0.0423 | 3.317 mg/L | 0.0847 | 2.55% |
| Na 330.237† | -14.9 | 1.614 | mg/L | 0.1117 | 3.228 mg/L | 0.2234 | 6.92% |
| Ni 231.604† | 560.2 | 0.3290 | mg/L | 0.01078 | 0.6580 mg/L | 0.02156 | 3.28% |
| Pb 220.353† | 3185.8 | 0.4464 | mg/L | 0.00115 | 0.8929 mg/L | 0.00231 | 0.26% |
| Sb 206.836† | 35.1 | 0.02217 | mg/L | 0.000307 | 0.04434 mg/L | 0.000615 | 1.39% |
| Se 196.026† | 39.8 | 0.02885 | mg/L | 0.002572 | 0.05770 mg/L | 0.005144 | 8.91% |
| Si 288.158† | 3830.0 | 2.594 | mg/L | 0.0632 | 5.187 mg/L | 0.1264 | 2.44% |
| Sn 189.927† | 404.6 | 0.1151 | mg/L | 0.00140 | 0.2302 mg/L | 0.00280 | 1.22% |
| Sr 421.552† | 133376.0 | 0.1991 | mg/L | 0.00441 | 0.3982 mg/L | 0.00881 | 2.21% |
| Ti 334.903† | 161860.5 | 7.369 | mg/L | 0.1733 | 14.74 mg/L | 0.347 | 2.35% |
| Tl 190.801† | -37.7 | 0.00818 | mg/L | 0.003199 | 0.01637 mg/L | 0.006397 | 39.09% |
| V 292.402† | 39971.3 | 0.3850 | mg/L | 0.00134 | 0.7700 mg/L | 0.00268 | 0.35% |
| Zn 206.200† | 356.8 | 0.5212 | mg/L | 0.00853 | 1.042 mg/L | 0.0171 | 1.64% |

Sequence No.: 29
 Sample ID: RG54 A SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 313
 Date Collected: 8/6/2010 3:48:05 PM
 Data Type: Original

Nebulizer Parameters: RG54 A SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 A SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1988683.8 | 104.6 | % | 0.77 | | | 0.73% |
| ScR 361.383 | 307028.0 | 104.9 | % | 0.61 | | | 0.58% |
| Ag 328.068† | -99.9 | -0.00079 | mg/L | 0.000159 | -0.00158 mg/L | 0.000319 | 20.11% |
| Al 308.215† | 220179.3 | 173.7 | mg/L | 1.43 | 347.4 mg/L | 2.85 | 0.82% |
| As 188.979† | -192.3 | 0.03136 | mg/L | 0.000252 | 0.06272 mg/L | 0.000503 | 0.80% |
| B 249.677† | 33.7 | 0.00949 | mg/L | 0.000629 | 0.01898 mg/L | 0.001259 | 6.63% |
| Ba 233.527† | 2280.4 | 0.6652 | mg/L | 0.00260 | 1.330 mg/L | 0.0052 | 0.39% |
| Be 313.042† | 1585.8 | 0.00238 | mg/L | 0.000012 | 0.00477 mg/L | 0.000024 | 0.50% |
| Ca 317.933† | 837921.5 | 57.71 | mg/L | 0.283 | 115.4 mg/L | 0.57 | 0.49% |
| Cd 228.802† | 74.2 | 0.00411 | mg/L | 0.000190 | 0.00821 mg/L | 0.000381 | 4.63% |
| Co 228.616† | 2979.0 | 0.08097 | mg/L | 0.000768 | 0.1619 mg/L | 0.00154 | 0.95% |
| Cr 267.716† | 1723.3 | 0.3365 | mg/L | 0.00299 | 0.6730 mg/L | 0.00598 | 0.89% |
| Cu 324.752† | 61913.4 | 0.2316 | mg/L | 0.00257 | 0.4632 mg/L | 0.00515 | 1.11% |
| Fe 273.955† | 224739.5 | 196.5 | mg/L | 1.45 | 393.1 mg/L | 2.90 | 0.74% |
| K 766.490† | 10601.5 | 7.295 | mg/L | 0.0506 | 14.59 mg/L | 0.101 | 0.69% |
| Mg 279.077† | 49577.0 | 52.72 | mg/L | 0.394 | 105.4 mg/L | 0.79 | 0.75% |
| Mn 257.610† | 105368.5 | 3.344 | mg/L | 0.0176 | 6.687 mg/L | 0.0351 | 0.53% |
| Mo 202.031† | 365.7 | 0.02027 | mg/L | 0.000708 | 0.04054 mg/L | 0.001417 | 3.49% |
| Na 589.592† | 37420.9 | 3.139 | mg/L | 0.0195 | 6.277 mg/L | 0.0389 | 0.62% |
| Na 330.237† | 14.6 | 3.227 | mg/L | 0.1896 | 6.455 mg/L | 0.3792 | 5.87% |
| Ni 231.604† | 520.5 | 0.3057 | mg/L | 0.00301 | 0.6114 mg/L | 0.00602 | 0.98% |
| Pb 220.353† | 1094.5 | 0.1646 | mg/L | 0.00023 | 0.3292 mg/L | 0.00046 | 0.14% |
| Sb 206.836† | 36.9 | 0.02337 | mg/L | 0.001738 | 0.04675 mg/L | 0.003476 | 7.44% |
| Se 196.026† | 51.7 | 0.03682 | mg/L | 0.009624 | 0.07364 mg/L | 0.019249 | 26.14% |
| Si 288.158† | 3307.2 | 2.239 | mg/L | 0.0182 | 4.479 mg/L | 0.0363 | 0.81% |
| Sn 189.927† | -36.2 | -0.00301 | mg/L | 0.001200 | -0.00603 mg/L | 0.002399 | 39.79% |
| Sr 421.552† | 205851.4 | 0.3073 | mg/L | 0.00252 | 0.6146 mg/L | 0.00503 | 0.82% |
| Ti 334.903† | 198841.3 | 9.051 | mg/L | 0.0490 | 18.10 mg/L | 0.098 | 0.54% |
| Tl 190.801† | -39.3 | 0.01000 | mg/L | 0.004244 | 0.01999 mg/L | 0.008488 | 42.46% |
| V 292.402† | 49211.8 | 0.4760 | mg/L | 0.00577 | 0.9520 mg/L | 0.01155 | 1.21% |
| Zn 206.200† | 334.8 | 0.4883 | mg/L | 0.00173 | 0.9765 mg/L | 0.00347 | 0.35% |

Sequence No.: 30
 Sample ID: RG54 B SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 314
 Date Collected: 8/6/2010 3:52:02 PM
 Data Type: Original

Nebulizer Parameters: RG54 B SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 B SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|--------|----------|--------------------|----------|--------|
| ScA 357.253 | 1985693.9 | 104.4 % | | 1.09 | | | 1.04% |
| ScR 361.383 | 308106.6 | 105.3 % | | 0.86 | | | 0.82% |
| Ag 328.068† | -44.4 | -0.00045 mg/L | | 0.000124 | -0.00090 mg/L | 0.000247 | 27.41% |
| Al 308.215† | 183083.0 | 144.4 mg/L | | 1.73 | 288.9 mg/L | 3.45 | 1.20% |
| As 188.979† | -169.2 | 0.01483 mg/L | | 0.002473 | 0.02965 mg/L | 0.004946 | 16.68% |
| B 249.677† | 18.8 | 0.00518 mg/L | | 0.000161 | 0.01037 mg/L | 0.000323 | 3.11% |
| Ba 233.527† | 1816.1 | 0.5291 mg/L | | 0.00498 | 1.058 mg/L | 0.0100 | 0.94% |
| Be 313.042† | 1208.4 | 0.00181 mg/L | | 0.000052 | 0.00361 mg/L | 0.000105 | 2.90% |
| Ca 317.933† | 534529.5 | 36.81 mg/L | | 0.423 | 73.63 mg/L | 0.846 | 1.15% |
| Cd 228.802† | 45.5 | 0.00276 mg/L | | 0.000207 | 0.00552 mg/L | 0.000414 | 7.50% |
| Co 228.616† | 2768.0 | 0.07743 mg/L | | 0.000756 | 0.1549 mg/L | 0.00151 | 0.98% |
| Cr 267.716† | 1618.9 | 0.3153 mg/L | | 0.00289 | 0.6305 mg/L | 0.00579 | 0.92% |
| Cu 324.752† | 40084.1 | 0.1518 mg/L | | 0.00212 | 0.3035 mg/L | 0.00424 | 1.40% |
| Fe 273.955† | 188932.4 | 165.2 mg/L | | 1.73 | 330.5 mg/L | 3.46 | 1.05% |
| K 766.490† | 7614.2 | 5.240 mg/L | | 0.0506 | 10.48 mg/L | 0.101 | 0.97% |
| Mg 279.077† | 48734.7 | 51.84 mg/L | | 0.626 | 103.7 mg/L | 1.25 | 1.21% |
| Mn 257.610† | 87161.6 | 2.766 mg/L | | 0.0276 | 5.532 mg/L | 0.0552 | 1.00% |
| Mo 202.031† | 82.3 | 0.00415 mg/L | | 0.000299 | 0.00830 mg/L | 0.000598 | 7.21% |
| Na 589.592† | 15768.5 | 1.323 mg/L | | 0.0142 | 2.645 mg/L | 0.0284 | 1.07% |
| Na 330.237† | -20.0 | 1.447 mg/L | | 0.1258 | 2.894 mg/L | 0.2516 | 8.69% |
| Ni 231.604† | 658.5 | 0.3867 mg/L | | 0.00393 | 0.7733 mg/L | 0.00787 | 1.02% |
| Pb 220.353† | 110.9 | 0.02839 mg/L | | 0.001101 | 0.05678 mg/L | 0.002202 | 3.88% |
| Sb 206.836† | 25.5 | 0.01674 mg/L | | 0.002859 | 0.03348 mg/L | 0.005718 | 17.08% |
| Se 196.026† | 46.0 | 0.03375 mg/L | | 0.004675 | 0.06751 mg/L | 0.009350 | 13.85% |
| Si 288.158† | 8156.3 | 5.523 mg/L | | 0.0760 | 11.05 mg/L | 0.152 | 1.38% |
| Sn 189.927† | -30.1 | -0.00316 mg/L | | 0.002167 | -0.00632 mg/L | 0.004333 | 68.58% |
| Sr 421.552† | 149010.0 | 0.2224 mg/L | | 0.00228 | 0.4449 mg/L | 0.00456 | 1.02% |
| Ti 334.903† | 158925.4 | 7.235 mg/L | | 0.0822 | 14.47 mg/L | 0.164 | 1.14% |
| Tl 190.801† | -28.1 | 0.01109 mg/L | | 0.001630 | 0.02217 mg/L | 0.003260 | 14.70% |
| V 292.402† | 38881.6 | 0.3752 mg/L | | 0.00738 | 0.7504 mg/L | 0.01475 | 1.97% |
| Zn 206.200† | 237.4 | 0.3455 mg/L | | 0.00378 | 0.6911 mg/L | 0.00756 | 1.09% |

Sequence No.: 31
 Sample ID: RG54 C SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 315
 Date Collected: 8/6/2010 3:55:44 PM
 Data Type: Original

Nebulizer Parameters: RG54 C SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 C SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|--------|----------|--------------------|----------|--------|
| ScA 357.253 | 1999786.3 | 105.2 % | | 0.21 | | | 0.20% |
| ScR 361.383 | 310226.7 | 106.0 % | | 1.42 | | | 1.34% |
| Ag 328.068† | -91.2 | -0.00072 mg/L | | 0.000427 | -0.00143 mg/L | 0.000855 | 59.60% |
| Al 308.215† | 188173.6 | 148.4 mg/L | | 0.48 | 296.9 mg/L | 0.95 | 0.32% |
| As 188.979† | -161.1 | 0.02450 mg/L | | 0.002343 | 0.04900 mg/L | 0.004685 | 9.56% |
| B 249.677† | 34.9 | 0.00985 mg/L | | 0.001734 | 0.01970 mg/L | 0.003468 | 17.60% |
| Ba 233.527† | 1982.5 | 0.5792 mg/L | | 0.00710 | 1.158 mg/L | 0.0142 | 1.23% |
| Be 313.042† | 1317.8 | 0.00199 mg/L | | 0.000051 | 0.00398 mg/L | 0.000102 | 2.56% |
| Ca 317.933† | 590469.4 | 40.67 mg/L | | 0.130 | 81.33 mg/L | 0.261 | 0.32% |
| Cd 228.802† | 55.8 | 0.00322 mg/L | | 0.000096 | 0.00643 mg/L | 0.000193 | 3.00% |
| Co 228.616† | 2664.1 | 0.07360 mg/L | | 0.000173 | 0.1472 mg/L | 0.00035 | 0.24% |
| Cr 267.716† | 1487.3 | 0.2896 mg/L | | 0.00482 | 0.5793 mg/L | 0.00964 | 1.66% |
| Cu 324.752† | 62641.6 | 0.2324 mg/L | | 0.00073 | 0.4649 mg/L | 0.00145 | 0.31% |
| Fe 273.955† | 186345.7 | 163.0 mg/L | | 0.64 | 325.9 mg/L | 1.29 | 0.39% |
| K 766.490† | 7931.2 | 5.458 mg/L | | 0.0116 | 10.92 mg/L | 0.023 | 0.21% |
| Mg 279.077† | 47478.8 | 50.50 mg/L | | 0.126 | 101.0 mg/L | 0.25 | 0.25% |
| Mn 257.610† | 88988.8 | 2.824 mg/L | | 0.0150 | 5.648 mg/L | 0.0300 | 0.53% |
| Mo 202.031† | 81.2 | 0.00402 mg/L | | 0.000135 | 0.00803 mg/L | 0.000269 | 3.35% |
| Na 589.592† | 18127.1 | 1.520 mg/L | | 0.0105 | 3.041 mg/L | 0.0209 | 0.69% |
| Na 330.237† | -18.1 | 1.583 mg/L | | 0.2425 | 3.165 mg/L | 0.4850 | 15.32% |
| Ni 231.604† | 629.7 | 0.3698 mg/L | | 0.00682 | 0.7395 mg/L | 0.01364 | 1.84% |
| Pb 220.353† | 673.4 | 0.1054 mg/L | | 0.00069 | 0.2108 mg/L | 0.00138 | 0.66% |
| Sb 206.836† | 25.6 | 0.01736 mg/L | | 0.001970 | 0.03471 mg/L | 0.003940 | 11.35% |
| Se 196.026† | 45.2 | 0.03280 mg/L | | 0.005519 | 0.06560 mg/L | 0.011038 | 16.83% |
| Si 288.158† | 7673.0 | 5.196 mg/L | | 0.0216 | 10.39 mg/L | 0.043 | 0.42% |
| Sn 189.927† | -30.2 | -0.00289 mg/L | | 0.001024 | -0.00578 mg/L | 0.002047 | 35.41% |
| Sr 421.552† | 161122.0 | 0.2405 mg/L | | 0.00060 | 0.4810 mg/L | 0.00120 | 0.25% |
| Ti 334.903† | 164165.2 | 7.473 mg/L | | 0.0326 | 14.95 mg/L | 0.065 | 0.44% |
| Tl 190.801† | -34.6 | 0.00722 mg/L | | 0.001855 | 0.01444 mg/L | 0.003710 | 25.70% |
| V 292.402† | 39319.1 | 0.3797 mg/L | | 0.00127 | 0.7593 mg/L | 0.00255 | 0.34% |
| Zn 206.200† | 290.5 | 0.4238 mg/L | | 0.00672 | 0.8476 mg/L | 0.01345 | 1.59% |

Sequence No.: 32
 Sample ID: RG54 E SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 316
 Date Collected: 8/6/2010 3:59:26 PM
 Data Type: Original

Nebulizer Parameters: RG54 E SWC
 Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 E SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. | Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------|-------|----------|--------|
| ScA 357.253 | 1992198.7 | 104.8 | % | 0.63 | | | | 0.60% |
| ScR 361.383 | 304370.4 | 104.0 | % | 2.16 | | | | 2.08% |
| Ag 328.068† | -31.4 | -0.00036 | mg/L | 0.000261 | -0.00072 | mg/L | 0.000521 | 72.79% |
| Al 308.215† | 202103.6 | 159.4 | mg/L | 2.34 | 318.9 | mg/L | 4.67 | 1.47% |
| As 188.979† | -150.2 | 0.04286 | mg/L | 0.002809 | 0.08572 | mg/L | 0.005618 | 6.55% |
| B 249.677† | 40.2 | 0.01140 | mg/L | 0.001365 | 0.02280 | mg/L | 0.002730 | 11.97% |
| Ba 233.527† | 2273.9 | 0.6662 | mg/L | 0.01360 | 1.332 | mg/L | 0.0272 | 2.04% |
| Be 313.042† | 1703.9 | 0.00266 | mg/L | 0.000066 | 0.00533 | mg/L | 0.000133 | 2.49% |
| Ca 317.933† | 565916.5 | 38.97 | mg/L | 0.645 | 77.95 | mg/L | 1.290 | 1.66% |
| Cd 228.802† | 80.2 | 0.00430 | mg/L | 0.000114 | 0.00859 | mg/L | 0.000227 | 2.64% |
| Co 228.616† | 2260.5 | 0.05913 | mg/L | 0.000802 | 0.1183 | mg/L | 0.00160 | 1.36% |
| Cr 267.716† | 1740.9 | 0.3401 | mg/L | 0.00753 | 0.6802 | mg/L | 0.01506 | 2.21% |
| Cu 324.752† | 34232.8 | 0.1308 | mg/L | 0.00059 | 0.2615 | mg/L | 0.00118 | 0.45% |
| Fe 273.955† | 190865.1 | 166.9 | mg/L | 2.91 | 333.8 | mg/L | 5.82 | 1.74% |
| K 766.490† | 7133.1 | 4.909 | mg/L | 0.0418 | 9.817 | mg/L | 0.0835 | 0.85% |
| Mg 279.077† | 41165.4 | 43.77 | mg/L | 0.689 | 87.55 | mg/L | 1.377 | 1.57% |
| Mn 257.610† | 87978.9 | 2.792 | mg/L | 0.0542 | 5.583 | mg/L | 0.1083 | 1.94% |
| Mo 202.031† | 160.6 | 0.00867 | mg/L | 0.000361 | 0.01733 | mg/L | 0.000722 | 4.16% |
| Na 589.592† | 18073.1 | 1.516 | mg/L | 0.0307 | 3.032 | mg/L | 0.0613 | 2.02% |
| Na 330.237† | -30.6 | 1.309 | mg/L | 0.1729 | 2.619 | mg/L | 0.3458 | 13.21% |
| Ni 231.604† | 528.7 | 0.3105 | mg/L | 0.00898 | 0.6209 | mg/L | 0.01795 | 2.89% |
| Pb 220.353† | 998.3 | 0.1513 | mg/L | 0.00262 | 0.3026 | mg/L | 0.00524 | 1.73% |
| Sb 206.836† | 11.6 | 0.01884 | mg/L | 0.001282 | 0.03769 | mg/L | 0.002564 | 6.80% |
| Se 196.026† | 41.7 | 0.03016 | mg/L | 0.007757 | 0.06033 | mg/L | 0.015515 | 25.72% |
| Si 288.158† | 7305.8 | 4.947 | mg/L | 0.0930 | 9.894 | mg/L | 0.1860 | 1.88% |
| Sn 189.927† | 2024.5 | 0.5561 | mg/L | 0.00562 | 1.112 | mg/L | 0.0112 | 1.01% |
| Sr 421.552† | 151436.7 | 0.2261 | mg/L | 0.00323 | 0.4521 | mg/L | 0.00647 | 1.43% |
| Ti 334.903† | 177506.8 | 8.081 | mg/L | 0.1396 | 16.16 | mg/L | 0.279 | 1.73% |
| Tl 190.801† | -27.9 | 0.01153 | mg/L | 0.001816 | 0.02306 | mg/L | 0.003633 | 15.75% |
| V 292.402† | 37096.3 | 0.3565 | mg/L | 0.00196 | 0.7130 | mg/L | 0.00391 | 0.55% |
| Zn 206.200† | 294.3 | 0.4290 | mg/L | 0.01230 | 0.8580 | mg/L | 0.02461 | 2.87% |

Sequence No.: 33
 Sample ID: RG54 F SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 317
 Date Collected: 8/6/2010 4:03:08 PM
 Data Type: Original

Nebulizer Parameters: RG54 F SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 F SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2005302.4 | 105.4 | % | 0.59 | | | 0.56% |
| ScR 361.383 | 313633.1 | 107.2 | % | 1.84 | | | 1.72% |
| Ag 328.068† | -118.5 | -0.00076 | mg/L | 0.000032 | -0.00151 mg/L | 0.000064 | 4.25% |
| Al 308.215† | 205698.4 | 162.3 | mg/L | 1.62 | 324.5 mg/L | 3.24 | 1.00% |
| As 188.979† | -175.9 | 0.02662 | mg/L | 0.005195 | 0.05325 mg/L | 0.010389 | 19.51% |
| B 249.677† | 31.7 | 0.00893 | mg/L | 0.001874 | 0.01786 mg/L | 0.003748 | 20.98% |
| Ba 233.527† | 1930.7 | 0.5619 | mg/L | 0.01081 | 1.124 mg/L | 0.0216 | 1.92% |
| Be 313.042† | 1396.6 | 0.00210 | mg/L | 0.000039 | 0.00419 mg/L | 0.000077 | 1.84% |
| Ca 317.933† | 647565.9 | 44.60 | mg/L | 0.442 | 89.20 mg/L | 0.884 | 0.99% |
| Cd 228.802† | 45.7 | 0.00276 | mg/L | 0.000213 | 0.00551 mg/L | 0.000425 | 7.71% |
| Co 228.616† | 2689.9 | 0.07308 | mg/L | 0.000893 | 0.1462 mg/L | 0.00179 | 1.22% |
| Cr 267.716† | 1966.8 | 0.3826 | mg/L | 0.00572 | 0.7651 mg/L | 0.01143 | 1.49% |
| Cu 324.752† | 38184.9 | 0.1456 | mg/L | 0.00013 | 0.2912 mg/L | 0.00027 | 0.09% |
| Fe 273.955† | 207411.7 | 181.4 | mg/L | 1.77 | 362.8 mg/L | 3.54 | 0.98% |
| K 766.490† | 10070.9 | 6.930 | mg/L | 0.0644 | 13.86 mg/L | 0.129 | 0.93% |
| Mg 279.077† | 55930.3 | 59.50 | mg/L | 0.574 | 119.0 mg/L | 1.15 | 0.97% |
| Mn 257.610† | 75881.8 | 2.408 | mg/L | 0.0255 | 4.816 mg/L | 0.0511 | 1.06% |
| Mo 202.031† | 84.0 | 0.00411 | mg/L | 0.000342 | 0.00822 mg/L | 0.000683 | 8.31% |
| Na 589.592† | 15850.0 | 1.329 | mg/L | 0.0155 | 2.659 mg/L | 0.0310 | 1.17% |
| Na 330.237† | -30.4 | 1.405 | mg/L | 0.1341 | 2.809 mg/L | 0.2682 | 9.55% |
| Ni 231.604† | 578.5 | 0.3397 | mg/L | 0.00651 | 0.6794 mg/L | 0.01302 | 1.92% |
| Pb 220.353† | 9.8 | 0.01671 | mg/L | 0.000654 | 0.03341 mg/L | 0.001308 | 3.92% |
| Sb 206.836† | 34.0 | 0.02045 | mg/L | 0.003593 | 0.04091 mg/L | 0.007185 | 17.56% |
| Se 196.026† | 45.5 | 0.03283 | mg/L | 0.006535 | 0.06565 mg/L | 0.013070 | 19.91% |
| Si 288.158† | 2192.7 | 1.485 | mg/L | 0.0273 | 2.970 mg/L | 0.0546 | 1.84% |
| Sn 189.927† | -46.8 | -0.00692 | mg/L | 0.001056 | -0.01383 mg/L | 0.002113 | 15.27% |
| Sr 421.552† | 129145.8 | 0.1928 | mg/L | 0.00174 | 0.3856 mg/L | 0.00347 | 0.90% |
| Ti 334.903† | 179174.9 | 8.157 | mg/L | 0.0784 | 16.31 mg/L | 0.157 | 0.96% |
| Tl 190.801† | -34.2 | 0.00968 | mg/L | 0.002715 | 0.01937 mg/L | 0.005431 | 28.04% |
| V 292.402† | 43442.2 | 0.4195 | mg/L | 0.00109 | 0.8391 mg/L | 0.00218 | 0.26% |
| Zn 206.200† | 195.1 | 0.2828 | mg/L | 0.00585 | 0.5656 mg/L | 0.01170 | 2.07% |

Sequence No.: 34
Sample ID: RG54 H SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 318
Date Collected: 8/6/2010 4:06:50 PM
Data Type: Original

Nebulizer Parameters: RG54 H SWC

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: RG54 H SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|--------|----------|--------------------|----------|--------|
| ScA 357.253 | 2032843.1 | 106.9 % | | 1.04 | | | 0.97% |
| ScR 361.383 | 314617.8 | 107.5 % | | 0.99 | | | 0.92% |
| Ag 328.068† | -106.5 | -0.00079 mg/L | | 0.000061 | -0.00158 mg/L | 0.000122 | 7.70% |
| Al 308.215† | 207711.5 | 163.9 mg/L | | 0.29 | 327.7 mg/L | 0.58 | 0.18% |
| As 188.979† | -208.5 | 0.02583 mg/L | | 0.000610 | 0.05166 mg/L | 0.001221 | 2.36% |
| B 249.677† | 23.8 | 0.00663 mg/L | | 0.000601 | 0.01326 mg/L | 0.001201 | 9.06% |
| Ba 233.527† | 2064.6 | 0.6010 mg/L | | 0.00594 | 1.202 mg/L | 0.0119 | 0.99% |
| Be 313.042† | 1398.3 | 0.00206 mg/L | | 0.000061 | 0.00412 mg/L | 0.000122 | 2.97% |
| Ca 317.933† | 725714.4 | 49.98 mg/L | | 0.168 | 99.96 mg/L | 0.337 | 0.34% |
| Cd 228.802† | 59.4 | 0.00348 mg/L | | 0.000309 | 0.00696 mg/L | 0.000618 | 8.89% |
| Co 228.616† | 2980.1 | 0.08059 mg/L | | 0.000694 | 0.1612 mg/L | 0.00139 | 0.86% |
| Cr 267.716† | 1786.3 | 0.3480 mg/L | | 0.00456 | 0.6960 mg/L | 0.00912 | 1.31% |
| Cu 324.752† | 47205.9 | 0.1783 mg/L | | 0.00174 | 0.3565 mg/L | 0.00348 | 0.98% |
| Fe 273.955† | 218828.7 | 191.4 mg/L | | 0.38 | 382.8 mg/L | 0.75 | 0.20% |
| K 766.490† | 10922.1 | 7.516 mg/L | | 0.0763 | 15.03 mg/L | 0.153 | 1.02% |
| Mg 279.077† | 54515.9 | 57.98 mg/L | | 0.891 | 116.0 mg/L | 1.78 | 1.54% |
| Mn 257.610† | 100669.0 | 3.194 mg/L | | 0.0380 | 6.389 mg/L | 0.0761 | 1.19% |
| Mo 202.031† | 240.4 | 0.01312 mg/L | | 0.000078 | 0.02623 mg/L | 0.000156 | 0.59% |
| Na 589.592† | 31248.8 | 2.621 mg/L | | 0.0328 | 5.242 mg/L | 0.0655 | 1.25% |
| Na 330.237† | -4.7 | 2.626 mg/L | | 0.0581 | 5.252 mg/L | 0.1162 | 2.21% |
| Ni 231.604† | 590.9 | 0.3470 mg/L | | 0.00308 | 0.6940 mg/L | 0.00615 | 0.89% |
| Pb 220.353† | 412.5 | 0.07081 mg/L | | 0.001851 | 0.1416 mg/L | 0.00370 | 2.61% |
| Sb 206.836† | 30.5 | 0.02125 mg/L | | 0.002007 | 0.04250 mg/L | 0.004014 | 9.45% |
| Se 196.026† | 46.5 | 0.03321 mg/L | | 0.005790 | 0.06643 mg/L | 0.011579 | 17.43% |
| Si 288.158† | 3315.8 | 2.245 mg/L | | 0.0179 | 4.491 mg/L | 0.0358 | 0.80% |
| Sn 189.927† | -33.3 | -0.00247 mg/L | | 0.000348 | -0.00493 mg/L | 0.000696 | 14.11% |
| Sr 421.552† | 204065.2 | 0.3046 mg/L | | 0.00081 | 0.6092 mg/L | 0.00161 | 0.26% |
| Ti 334.903† | 205173.2 | 9.340 mg/L | | 0.0277 | 18.68 mg/L | 0.055 | 0.30% |
| Tl 190.801† | -30.1 | 0.01414 mg/L | | 0.002206 | 0.02829 mg/L | 0.004413 | 15.60% |
| V 292.402† | 48464.7 | 0.4688 mg/L | | 0.00468 | 0.9377 mg/L | 0.00935 | 1.00% |
| Zn 206.200† | 250.6 | 0.3645 mg/L | | 0.00463 | 0.7290 mg/L | 0.00926 | 1.27% |

Sequence No.: 35
 Sample ID: RG54 I SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 319
 Date Collected: 8/6/2010 4:10:48 PM
 Data Type: Original

Nebulizer Parameters: RG54 I SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG54 I SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1999089.7 | 105.1 | % | 0.79 | | | 0.75% |
| ScR 361.383 | 311999.0 | 106.6 | % | 0.72 | | | 0.68% |
| Ag 328.068† | -96.8 | -0.00067 | mg/L | 0.000102 | -0.00134 mg/L | 0.000203 | 15.22% |
| Al 308.215† | 206399.5 | 162.8 | mg/L | 1.90 | 325.6 mg/L | 3.79 | 1.16% |
| As 188.979† | -191.7 | 0.01555 | mg/L | 0.000527 | 0.03110 mg/L | 0.001054 | 3.39% |
| B 249.677† | 28.9 | 0.00812 | mg/L | 0.001332 | 0.01624 mg/L | 0.002664 | 16.40% |
| Ba 233.527† | 2515.4 | 0.7391 | mg/L | 0.00528 | 1.478 mg/L | 0.0106 | 0.71% |
| Be 313.042† | 1287.9 | 0.00194 | mg/L | 0.000083 | 0.00387 mg/L | 0.000165 | 4.27% |
| Ca 317.933† | 515652.9 | 35.51 | mg/L | 0.435 | 71.03 mg/L | 0.869 | 1.22% |
| Cd 228.802† | 43.4 | 0.00268 | mg/L | 0.000127 | 0.00535 mg/L | 0.000253 | 4.73% |
| Co 228.616† | 2591.1 | 0.07009 | mg/L | 0.000791 | 0.1402 mg/L | 0.00158 | 1.13% |
| Cr 267.716† | 1330.7 | 0.2591 | mg/L | 0.00076 | 0.5181 mg/L | 0.00152 | 0.29% |
| Cu 324.752† | 33599.4 | 0.1280 | mg/L | 0.00121 | 0.2559 mg/L | 0.00241 | 0.94% |
| Fe 273.955† | 185435.3 | 162.2 | mg/L | 1.77 | 324.3 mg/L | 3.53 | 1.09% |
| K 766.490† | 9457.4 | 6.508 | mg/L | 0.0766 | 13.02 mg/L | 0.153 | 1.18% |
| Mg 279.077† | 48679.3 | 51.78 | mg/L | 0.597 | 103.6 mg/L | 1.19 | 1.15% |
| Mn 257.610† | 79437.8 | 2.521 | mg/L | 0.0280 | 5.041 mg/L | 0.0561 | 1.11% |
| Mo 202.031† | 74.9 | 0.00374 | mg/L | 0.000808 | 0.00748 mg/L | 0.001616 | 21.60% |
| Na 589.592† | 15278.4 | 1.281 | mg/L | 0.0114 | 2.563 mg/L | 0.0228 | 0.89% |
| Na 330.237† | -38.4 | 1.064 | mg/L | 0.0928 | 2.128 mg/L | 0.1855 | 8.72% |
| Ni 231.604† | 553.9 | 0.3253 | mg/L | 0.00246 | 0.6505 mg/L | 0.00491 | 0.76% |
| Pb 220.353† | 344.0 | 0.06327 | mg/L | 0.001280 | 0.1265 mg/L | 0.00256 | 2.02% |
| Sb 206.836† | 25.2 | 0.01833 | mg/L | 0.003214 | 0.03665 mg/L | 0.006428 | 17.54% |
| Se 196.026† | 43.7 | 0.03204 | mg/L | 0.005386 | 0.06408 mg/L | 0.010773 | 16.81% |
| Si 288.158† | 3519.9 | 2.384 | mg/L | 0.0233 | 4.767 mg/L | 0.0466 | 0.98% |
| Sn 189.927† | -30.6 | -0.00296 | mg/L | 0.001044 | -0.00592 mg/L | 0.002089 | 35.28% |
| Sr 421.552† | 161102.5 | 0.2405 | mg/L | 0.00259 | 0.4810 mg/L | 0.00518 | 1.08% |
| Ti 334.903† | 178241.4 | 8.115 | mg/L | 0.0966 | 16.23 mg/L | 0.193 | 1.19% |
| Tl 190.801† | -28.7 | 0.01008 | mg/L | 0.002498 | 0.02017 mg/L | 0.004996 | 24.77% |
| V 292.402† | 38419.7 | 0.3700 | mg/L | 0.00260 | 0.7401 mg/L | 0.00520 | 0.70% |
| Zn 206.200† | 192.5 | 0.2790 | mg/L | 0.00293 | 0.5579 mg/L | 0.00585 | 1.05% |

Sequence No.: 36
Sample ID: RG54 J SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 320
Date Collected: 8/6/2010 4:14:30 PM
Data Type: Original

Nebulizer Parameters: RG54 J SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG54 J SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Conc. Units | Sample | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|-------------|--------|----------|--------|
| ScA 357.253 | 2006313.9 | 105.5 | % | 0.46 | | | | 0.44% |
| ScR 361.383 | 313088.8 | 107.0 | % | 0.40 | | | | 0.37% |
| Ag 328.068† | -85.2 | -0.00054 | mg/L | 0.000033 | -0.00109 | mg/L | 0.000065 | 6.01% |
| Al 308.215† | 224313.4 | 177.0 | mg/L | 0.75 | 353.9 | mg/L | 1.49 | 0.42% |
| As 188.979† | -210.0 | 0.01560 | mg/L | 0.005562 | 0.03121 | mg/L | 0.011124 | 35.64% |
| B 249.677† | 22.4 | 0.00625 | mg/L | 0.001362 | 0.01250 | mg/L | 0.002725 | 21.80% |
| Ba 233.527† | 2397.3 | 0.7023 | mg/L | 0.00222 | 1.405 | mg/L | 0.0044 | 0.32% |
| Be 313.042† | 1414.3 | 0.00213 | mg/L | 0.000013 | 0.00425 | mg/L | 0.000025 | 0.60% |
| Ca 317.933† | 498554.3 | 34.34 | mg/L | 0.279 | 68.67 | mg/L | 0.558 | 0.81% |
| Cd 228.802† | 41.6 | 0.00262 | mg/L | 0.000175 | 0.00524 | mg/L | 0.000349 | 6.67% |
| Co 228.616† | 2681.8 | 0.07175 | mg/L | 0.000292 | 0.1435 | mg/L | 0.00058 | 0.41% |
| Cr 267.716† | 1319.7 | 0.2573 | mg/L | 0.00124 | 0.5146 | mg/L | 0.00247 | 0.48% |
| Cu 324.752† | 40076.4 | 0.1520 | mg/L | 0.00064 | 0.3039 | mg/L | 0.00128 | 0.42% |
| Fe 273.955† | 203032.1 | 177.6 | mg/L | 0.98 | 355.1 | mg/L | 1.96 | 0.55% |
| K 766.490† | 13667.1 | 9.405 | mg/L | 0.0522 | 18.81 | mg/L | 0.104 | 0.56% |
| Mg 279.077† | 51394.5 | 54.67 | mg/L | 0.237 | 109.3 | mg/L | 0.47 | 0.43% |
| Mn 257.610† | 75120.3 | 2.384 | mg/L | 0.0197 | 4.767 | mg/L | 0.0394 | 0.83% |
| Mo 202.031† | 91.9 | 0.00475 | mg/L | 0.000089 | 0.00950 | mg/L | 0.000177 | 1.87% |
| Na 589.592† | 15058.1 | 1.263 | mg/L | 0.0051 | 2.526 | mg/L | 0.0102 | 0.40% |
| Na 330.237† | -42.5 | 1.102 | mg/L | 0.1421 | 2.205 | mg/L | 0.2842 | 12.89% |
| Ni 231.604† | 522.7 | 0.3069 | mg/L | 0.00176 | 0.6139 | mg/L | 0.00353 | 0.57% |
| Pb 220.353† | 17.7 | 0.02028 | mg/L | 0.001172 | 0.04055 | mg/L | 0.002343 | 5.78% |
| Sb 206.836† | 25.1 | 0.01931 | mg/L | 0.001002 | 0.03862 | mg/L | 0.002003 | 5.19% |
| Se 196.026† | 38.3 | 0.02782 | mg/L | 0.009135 | 0.05564 | mg/L | 0.018269 | 32.83% |
| Si 288.158† | 5152.0 | 3.489 | mg/L | 0.0144 | 6.977 | mg/L | 0.0288 | 0.41% |
| Sn 189.927† | -32.1 | -0.00312 | mg/L | 0.000839 | -0.00623 | mg/L | 0.001679 | 26.94% |
| Sr 421.552† | 162281.7 | 0.2422 | mg/L | 0.00155 | 0.4845 | mg/L | 0.00310 | 0.64% |
| Ti 334.903† | 193336.6 | 8.802 | mg/L | 0.0486 | 17.60 | mg/L | 0.097 | 0.55% |
| Tl 190.801† | -34.9 | 0.00880 | mg/L | 0.001845 | 0.01760 | mg/L | 0.003690 | 20.97% |
| V 292.402† | 42591.9 | 0.4104 | mg/L | 0.00254 | 0.8208 | mg/L | 0.00508 | 0.62% |
| Zn 206.200† | 199.5 | 0.2889 | mg/L | 0.00225 | 0.5779 | mg/L | 0.00450 | 0.78% |

Sequence No.: 37
Sample ID: CV 11
Analyst: ALA
Dilution: 1X

Autosampler Location: 7
Date Collected: 8/6/2010 4:18:12 PM
Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
All 201.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1961836.6 | 103.2 % | 0.42 | | | 0.41% |
| ScR 361.383 | 298838.7 | 102.1 % | 0.27 | | | 0.27% |
| Ag 328.068† | 188696.0 | 1.064 mg/L | 0.0017 | 1.064 mg/L | 0.0017 | 0.16% |
| Al 308.215† | 2820.7 | 2.192 mg/L | 0.0136 | 2.192 mg/L | 0.0136 | 0.62% |
| As 188.979† | 3069.3 | 2.099 mg/L | 0.0081 | 2.099 mg/L | 0.0081 | 0.38% |
| B 249.677† | 3508.0 | 1.010 mg/L | 0.0012 | 1.010 mg/L | 0.0012 | 0.12% |
| Ba 233.527† | 3463.5 | 1.038 mg/L | 0.0021 | 1.038 mg/L | 0.0021 | 0.20% |
| Be 313.042† | 586226.9 | 1.014 mg/L | 0.0039 | 1.014 mg/L | 0.0039 | 0.39% |
| Ca 317.933† | 32882.5 | 2.265 mg/L | 0.0169 | 2.265 mg/L | 0.0169 | 0.75% |
| Cd 228.802† | 23941.5 | 1.116 mg/L | 0.0031 | 1.116 mg/L | 0.0031 | 0.28% |
| Co 228.616† | 33058.6 | 1.095 mg/L | 0.0011 | 1.095 mg/L | 0.0011 | 0.10% |
| Cr 267.716† | 5426.4 | 1.055 mg/L | 0.0018 | 1.055 mg/L | 0.0018 | 0.18% |
| Cu 324.752† | 299059.8 | 1.072 mg/L | 0.0026 | 1.072 mg/L | 0.0026 | 0.24% |
| Fe 273.955† | 2525.5 | 2.203 mg/L | 0.0067 | 2.203 mg/L | 0.0067 | 0.30% |
| K 766.490† | 32760.1 | 22.54 mg/L | 0.108 | 22.54 mg/L | 0.108 | 0.48% |
| Mg 279.077† | 2081.6 | 2.223 mg/L | 0.0093 | 2.223 mg/L | 0.0093 | 0.42% |
| Mn 257.610† | 31236.0 | 0.9917 mg/L | 0.00365 | 0.9917 mg/L | 0.00365 | 0.37% |
| Mo 202.031† | 18276.8 | 1.063 mg/L | 0.0029 | 1.063 mg/L | 0.0029 | 0.27% |
| Na 589.592† | 597315.7 | 50.10 mg/L | 0.091 | 50.10 mg/L | 0.091 | 0.18% |
| Na 330.237† | 1596.5 | 54.95 mg/L | 0.222 | 54.95 mg/L | 0.222 | 0.40% |
| Ni 231.604† | 1780.8 | 1.047 mg/L | 0.0050 | 1.047 mg/L | 0.0050 | 0.48% |
| Pb 220.353† | 15111.3 | 2.052 mg/L | 0.0017 | 2.052 mg/L | 0.0017 | 0.08% |
| Sb 206.836† | 6008.2 | 2.245 mg/L | 0.0120 | 2.245 mg/L | 0.0120 | 0.53% |
| Se 196.026† | 2673.5 | 2.105 mg/L | 0.0079 | 2.105 mg/L | 0.0079 | 0.37% |
| Si 288.158† | 3351.6 | 2.273 mg/L | 0.0057 | 2.273 mg/L | 0.0057 | 0.25% |
| Sn 189.927† | 4075.2 | 1.110 mg/L | 0.0071 | 1.110 mg/L | 0.0071 | 0.64% |
| Sr 421.552† | 689602.8 | 1.029 mg/L | 0.0018 | 1.029 mg/L | 0.0018 | 0.17% |
| Ti 334.903† | 23573.0 | 1.072 mg/L | 0.0051 | 1.072 mg/L | 0.0051 | 0.48% |
| Tl 190.801† | 3754.2 | 2.075 mg/L | 0.0119 | 2.075 mg/L | 0.0119 | 0.58% |
| V 292.402† | 106117.4 | 1.084 mg/L | 0.0055 | 1.084 mg/L | 0.0055 | 0.51% |
| Zn 206.200† | 701.0 | 1.032 mg/L | 0.0050 | 1.032 mg/L | 0.0050 | 0.49% |

Sequence No.: 38
 Sample ID: CB 11
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 1
 Date Collected: 8/6/2010 4:22:21 PM
 Data Type: Original

Nebulizer Parameters: CB

| | | |
|---------|---------------|------------|
| Analyte | Back Pressure | Flow |
| All | 200.0 kPa | 0.75 L/min |

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1977349.4 | 104.0 | % | 1.36 | | | 1.31% |
| ScR 361.383 | 304676.0 | 104.1 | % | 1.66 | | | 1.60% |
| Ag 328.068† | 15.3 | 0.00009 | mg/L | 0.000164 | 0.00009 mg/L | 0.000164 | 188.89% |
| Al 308.215† | 10.4 | 0.00818 | mg/L | 0.019798 | 0.00818 mg/L | 0.019798 | 242.02% |
| As 188.979† | 2.5 | 0.00173 | mg/L | 0.002885 | 0.00173 mg/L | 0.002885 | 166.85% |
| B 249.677† | -0.7 | -0.00021 | mg/L | 0.001786 | -0.00021 mg/L | 0.001786 | 850.37% |
| Ba 233.527† | 5.8 | 0.00174 | mg/L | 0.000618 | 0.00174 mg/L | 0.000618 | 35.59% |
| Be 313.042† | 49.2 | 0.00009 | mg/L | 0.000103 | 0.00009 mg/L | 0.000103 | 120.86% |
| Ca 317.933† | 17.1 | 0.00118 | mg/L | 0.000316 | 0.00118 mg/L | 0.000316 | 26.84% |
| Cd 228.802† | -5.0 | -0.00024 | mg/L | 0.000014 | -0.00024 mg/L | 0.000014 | 5.68% |
| Co 228.616† | -0.8 | -0.00003 | mg/L | 0.000215 | -0.00003 mg/L | 0.000215 | 750.95% |
| Cr 267.716† | -3.9 | -0.00076 | mg/L | 0.001610 | -0.00076 mg/L | 0.001610 | 210.90% |
| Cu 324.752† | 439.9 | 0.00158 | mg/L | 0.000112 | 0.00158 mg/L | 0.000112 | 7.13% |
| Fe 273.955† | -0.3 | -0.00026 | mg/L | 0.002003 | -0.00026 mg/L | 0.002003 | 773.53% |
| K 766.490† | 14.5 | 0.01001 | mg/L | 0.012952 | 0.01001 mg/L | 0.012952 | 129.39% |
| Mg 279.077† | 3.1 | 0.00328 | mg/L | 0.005067 | 0.00328 mg/L | 0.005067 | 154.55% |
| Mn 257.610† | 0.0 | 0.00000 | mg/L | 0.000055 | 0.00000 mg/L | 0.000055 | >999.9% |
| Mo 202.031† | -2.9 | -0.00017 | mg/L | 0.000219 | -0.00017 mg/L | 0.000219 | 131.18% |
| Na 589.592† | 15.1 | 0.00126 | mg/L | 0.003789 | 0.00126 mg/L | 0.003789 | 299.83% |
| Na 330.237† | -1.0 | -0.03445 | mg/L | 0.148507 | -0.03445 mg/L | 0.148507 | 431.10% |
| Ni 231.604† | 5.0 | 0.00294 | mg/L | 0.001692 | 0.00294 mg/L | 0.001692 | 57.60% |
| Pb 220.353† | 0.3 | 0.00004 | mg/L | 0.000329 | 0.00004 mg/L | 0.000329 | 895.93% |
| Sb 206.836† | 5.8 | 0.00218 | mg/L | 0.001739 | 0.00218 mg/L | 0.001739 | 79.88% |
| Se 196.026† | 6.8 | 0.00539 | mg/L | 0.006418 | 0.00539 mg/L | 0.006418 | 119.06% |
| Si 288.158† | 10.7 | 0.00728 | mg/L | 0.004181 | 0.00728 mg/L | 0.004181 | 57.45% |
| Sn 189.927† | 3.4 | 0.00092 | mg/L | 0.000500 | 0.00092 mg/L | 0.000500 | 54.53% |
| Sr 421.552† | 25.0 | 0.00004 | mg/L | 0.000044 | 0.00004 mg/L | 0.000044 | 118.48% |
| Ti 334.903† | 11.2 | 0.00051 | mg/L | 0.000357 | 0.00051 mg/L | 0.000357 | 70.19% |
| Tl 190.801† | 1.5 | 0.00080 | mg/L | 0.000913 | 0.00080 mg/L | 0.000913 | 113.72% |
| V 292.402† | 28.7 | 0.00029 | mg/L | 0.000138 | 0.00029 mg/L | 0.000138 | 47.80% |
| Zn 206.200† | -1.0 | -0.00140 | mg/L | 0.000520 | -0.00140 mg/L | 0.000520 | 37.00% |

Handwritten signature
 8-9-10

Sequence No.: 39
 Sample ID: RG42 MB SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 321
 Date Collected: 8/6/2010 4:26:32 PM
 Data Type: Original

 Nebulizer Parameters: RG42 MB SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

 Mean Data: RG42 MB SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|----------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 1974990.7 | 103.9 | % | 0.57 | | | 0.55% |
| ScR 361.383 | 284087.0 | 97.06 | % | 0.597 | | | 0.62% |
| Ag 328.068† | 17.6 | 0.00010 | mg/L | 0.000122 | 0.00020 mg/L | 0.000243 | 122.45% |
| Al 308.215† | 9.2 | 0.00726 | mg/L | 0.007438 | 0.01452 mg/L | 0.014877 | 102.46% |
| As 188.979† | 3.7 | 0.00251 | mg/L | 0.002886 | 0.00503 mg/L | 0.005772 | 114.78% |
| B 249.677† | -8.1 | -0.00233 | mg/L | 0.001297 | -0.00467 mg/L | 0.002595 | 55.58% |
| Ba 233.527† | 15.5 | 0.00466 | mg/L | 0.000476 | 0.00932 mg/L | 0.000951 | 10.21% |
| Be 313.042† | 88.6 | 0.00015 | mg/L | 0.000018 | 0.00031 mg/L | 0.000036 | 11.86% |
| Ca 317.933† | 144.5 | 0.00995 | mg/L | 0.001270 | 0.01991 mg/L | 0.002540 | 12.76% |
| Cd 228.802† | -3.9 | -0.00019 | mg/L | 0.000173 | -0.00038 mg/L | 0.000347 | 90.71% |
| Co 228.616† | 5.5 | 0.00018 | mg/L | 0.000111 | 0.00036 mg/L | 0.000223 | 61.67% |
| Cr 267.716† | -6.4 | -0.00125 | mg/L | 0.002089 | -0.00250 mg/L | 0.004178 | 167.28% |
| Cu 324.752† | 487.1 | 0.00175 | mg/L | 0.000170 | 0.00350 mg/L | 0.000339 | 9.70% |
| Fe 273.955† | 5.8 | 0.00505 | mg/L | 0.000625 | 0.01010 mg/L | 0.001250 | 12.38% |
| K 766.490† | 102.6 | 0.07061 | mg/L | 0.026483 | 0.1412 mg/L | 0.05297 | 37.51% |
| Mg 279.077† | -0.3 | -0.00030 | mg/L | 0.003039 | -0.00060 mg/L | 0.006077 | >999.9% |
| Mn 257.610† | 3.0 | 0.00010 | mg/L | 0.000060 | 0.00019 mg/L | 0.000121 | 62.92% |
| Mo 202.031† | -6.4 | -0.00038 | mg/L | 0.000264 | -0.00075 mg/L | 0.000528 | 70.29% |
| Na 589.592† | 7.3 | 0.00061 | mg/L | 0.002300 | 0.00122 mg/L | 0.004600 | 377.90% |
| Na 330.237† | 10.7 | 0.3685 | mg/L | 0.44962 | 0.7369 mg/L | 0.89924 | 122.03% |
| Ni 231.604† | 4.0 | 0.00234 | mg/L | 0.001336 | 0.00469 mg/L | 0.002672 | 56.97% |
| Pb 220.353† | 0.2 | 0.00002 | mg/L | 0.000192 | 0.00004 mg/L | 0.000383 | 875.61% |
| Sb 206.836† | -2.9 | -0.00105 | mg/L | 0.002042 | -0.00210 mg/L | 0.004084 | 194.05% |
| Se 196.026† | 5.1 | 0.00398 | mg/L | 0.003027 | 0.00796 mg/L | 0.006053 | 76.00% |
| Si 288.158† | 18.6 | 0.01260 | mg/L | 0.003879 | 0.02519 mg/L | 0.007758 | 30.79% |
| Sn 189.927† | 5.4 | 0.00147 | mg/L | 0.000334 | 0.00295 mg/L | 0.000669 | 22.70% |
| Sr 421.552† | 93.5 | 0.00014 | mg/L | 0.000035 | 0.00028 mg/L | 0.000071 | 25.41% |
| Ti 334.903† | -6.0 | -0.00028 | mg/L | 0.000539 | -0.00055 mg/L | 0.001077 | 195.59% |
| Tl 190.801† | 1.4 | 0.00075 | mg/L | 0.002261 | 0.00150 mg/L | 0.004522 | 302.15% |
| V 292.402† | -8.8 | -0.00010 | mg/L | 0.000172 | -0.00019 mg/L | 0.000343 | 180.58% |
| Zn 206.200† | 0.8 | 0.00111 | mg/L | 0.002739 | 0.00222 mg/L | 0.005478 | 247.27% |

Sequence No.: 40
 Sample ID: RG51 E SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 322
 Date Collected: 8/6/2010 4:30:29 PM
 Data Type: Original

Nebulizer Parameters: RG51 E SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG51 E SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1981555.1 | 104.2 | % | 0.86 | | | 0.83% |
| ScR 361.383 | 310111.7 | 106.0 | % | 0.69 | | | 0.65% |
| Ag 328.068† | -71.3 | -0.00050 | mg/L | 0.000281 | -0.00101 mg/L | 0.000563 | 55.80% |
| Al 308.215† | 173404.4 | 136.8 | mg/L | 0.90 | 273.6 mg/L | 1.81 | 0.66% |
| As 188.979† | -170.7 | 0.01924 | mg/L | 0.003320 | 0.03848 mg/L | 0.006640 | 17.26% |
| B 249.677† | 29.3 | 0.00826 | mg/L | 0.001004 | 0.01652 mg/L | 0.002009 | 12.16% |
| Ba 233.527† | 1822.6 | 0.5319 | mg/L | 0.00501 | 1.064 mg/L | 0.0100 | 0.94% |
| Be 313.042† | 1219.5 | 0.00183 | mg/L | 0.000046 | 0.00366 mg/L | 0.000091 | 2.49% |
| Ca 317.933† | 492071.2 | 33.89 | mg/L | 0.277 | 67.78 mg/L | 0.554 | 0.82% |
| Cd 228.802† | 45.6 | 0.00273 | mg/L | 0.000083 | 0.00545 mg/L | 0.000166 | 3.04% |
| Co 228.616† | 2461.8 | 0.06691 | mg/L | 0.000768 | 0.1338 mg/L | 0.00154 | 1.15% |
| Cr 267.716† | 1245.9 | 0.2423 | mg/L | 0.00123 | 0.4846 mg/L | 0.00247 | 0.51% |
| Cu 324.752† | 34685.6 | 0.1316 | mg/L | 0.00185 | 0.2632 mg/L | 0.00370 | 1.41% |
| Fe 273.955† | 177917.5 | 155.6 | mg/L | 1.00 | 311.2 mg/L | 2.00 | 0.64% |
| K 766.490† | 7737.0 | 5.324 | mg/L | 0.0057 | 10.65 mg/L | 0.011 | 0.11% |
| Mg 279.077† | 48381.6 | 51.47 | mg/L | 0.283 | 102.9 mg/L | 0.57 | 0.55% |
| Mn 257.610† | 72264.3 | 2.293 | mg/L | 0.0137 | 4.586 mg/L | 0.0274 | 0.60% |
| Mo 202.031† | 79.3 | 0.00403 | mg/L | 0.000469 | 0.00805 mg/L | 0.000937 | 11.64% |
| Na 589.592† | 13245.1 | 1.111 | mg/L | 0.0049 | 2.222 mg/L | 0.0098 | 0.44% |
| Na 330.237† | -42.1 | 0.7687 | mg/L | 0.09422 | 1.537 mg/L | 0.1884 | 12.26% |
| Ni 231.604† | 534.5 | 0.3139 | mg/L | 0.00126 | 0.6278 mg/L | 0.00253 | 0.40% |
| Pb 220.353† | 138.1 | 0.03135 | mg/L | 0.001217 | 0.06269 mg/L | 0.002434 | 3.88% |
| Sb 206.836† | 23.9 | 0.01718 | mg/L | 0.001197 | 0.03436 mg/L | 0.002395 | 6.97% |
| Se 196.026† | 42.5 | 0.03119 | mg/L | 0.003470 | 0.06239 mg/L | 0.006939 | 11.12% |
| Si 288.158† | 4670.8 | 3.163 | mg/L | 0.0275 | 6.326 mg/L | 0.0549 | 0.87% |
| Sn 189.927† | -36.6 | -0.00493 | mg/L | 0.001351 | -0.00986 mg/L | 0.002703 | 27.42% |
| Sr 421.552† | 120834.5 | 0.1804 | mg/L | 0.00135 | 0.3608 mg/L | 0.00270 | 0.75% |
| Ti 334.903† | 165343.4 | 7.527 | mg/L | 0.0456 | 15.05 mg/L | 0.091 | 0.61% |
| Tl 190.801† | -28.4 | 0.00908 | mg/L | 0.003414 | 0.01816 mg/L | 0.006828 | 37.60% |
| V 292.402† | 37003.1 | 0.3566 | mg/L | 0.00248 | 0.7132 mg/L | 0.00495 | 0.69% |
| Zn 206.200† | 183.3 | 0.2662 | mg/L | 0.00434 | 0.5324 mg/L | 0.00869 | 1.63% |

Sequence No.: 41
 Sample ID: RG42 A SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 323
 Date Collected: 8/6/2010 4:34:25 PM
 Data Type: Original

 Nebulizer Parameters: RG42 A SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

 Mean Data: RG42 A SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------|--------|----------|--------------------|----------|--------|
| ScA 357.253 | 1969472.9 | 103.6 % | | 1.47 | | | 1.42% |
| ScR 361.383 | 298750.5 | 102.1 % | | 1.39 | | | 1.36% |
| Ag 328.068† | 39.0 | 0.00023 mg/L | | 0.000161 | 0.00045 mg/L | 0.000322 | 71.28% |
| Al 308.215† | 38628.7 | 30.47 mg/L | | 0.471 | 60.94 mg/L | 0.942 | 1.55% |
| As 188.979† | -22.6 | 0.01997 mg/L | | 0.003323 | 0.03993 mg/L | 0.006647 | 16.65% |
| B 249.677† | 768.4 | 0.2216 mg/L | | 0.00096 | 0.4431 mg/L | 0.00191 | 0.43% |
| Ba 233.527† | 619.7 | 0.1802 mg/L | | 0.00208 | 0.3604 mg/L | 0.00416 | 1.15% |
| Be 313.042† | 402.0 | 0.00060 mg/L | | 0.000018 | 0.00120 mg/L | 0.000036 | 2.95% |
| Ca 317.933† | 311887.1 | 21.48 mg/L | | 0.267 | 42.96 mg/L | 0.533 | 1.24% |
| Cd 228.802† | 79.3 | 0.00382 mg/L | | 0.000153 | 0.00764 mg/L | 0.000305 | 4.00% |
| Co 228.616† | 786.8 | 0.02197 mg/L | | 0.000515 | 0.04394 mg/L | 0.001030 | 2.34% |
| Cr 267.716† | 561.9 | 0.1086 mg/L | | 0.00159 | 0.2172 mg/L | 0.00317 | 1.46% |
| Cu 324.752† | 67807.3 | 0.2461 mg/L | | 0.00422 | 0.4923 mg/L | 0.00845 | 1.72% |
| Fe 273.955† | 67477.4 | 59.01 mg/L | | 0.714 | 118.0 mg/L | 1.43 | 1.21% |
| K 766.490† | 8135.8 | 5.599 mg/L | | 0.0770 | 11.20 mg/L | 0.154 | 1.38% |
| Mg 279.077† | 22054.2 | 23.47 mg/L | | 0.280 | 46.93 mg/L | 0.559 | 1.19% |
| Mn 257.610† | 14971.3 | 0.4752 mg/L | | 0.00671 | 0.9504 mg/L | 0.01342 | 1.41% |
| Mo 202.031† | 306.6 | 0.01746 mg/L | | 0.000159 | 0.03493 mg/L | 0.000318 | 0.91% |
| Na 589.592† | 699695.1 | 58.69 mg/L | | 0.629 | 117.4 mg/L | 1.26 | 1.07% |
| Na 330.237† | 1808.5 | 62.48 mg/L | | 0.936 | 125.0 mg/L | 1.87 | 1.50% |
| Ni 231.604† | 142.6 | 0.08373 mg/L | | 0.001232 | 0.1675 mg/L | 0.00246 | 1.47% |
| Pb 220.353† | 1867.1 | 0.2543 mg/L | | 0.00110 | 0.5087 mg/L | 0.00220 | 0.43% |
| Sb 206.836† | 21.6 | 0.01008 mg/L | | 0.000664 | 0.02017 mg/L | 0.001329 | 6.59% |
| Se 196.026† | 22.3 | 0.01607 mg/L | | 0.006301 | 0.03214 mg/L | 0.012602 | 39.21% |
| Si 288.158† | 2867.4 | 1.942 mg/L | | 0.0159 | 3.883 mg/L | 0.0318 | 0.82% |
| Sn 189.927† | 57.9 | 0.01765 mg/L | | 0.001554 | 0.03531 mg/L | 0.003107 | 8.80% |
| Sr 421.552† | 136266.6 | 0.2034 mg/L | | 0.00166 | 0.4068 mg/L | 0.00332 | 0.82% |
| Ti 334.903† | 43762.9 | 1.992 mg/L | | 0.0247 | 3.983 mg/L | 0.0494 | 1.24% |
| Tl 190.801† | -4.8 | 0.00646 mg/L | | 0.001650 | 0.01291 mg/L | 0.003299 | 25.55% |
| V 292.402† | 13583.0 | 0.1312 mg/L | | 0.00155 | 0.2624 mg/L | 0.00310 | 1.18% |
| Zn 206.200† | 1047.5 | 1.542 mg/L | | 0.0169 | 3.084 mg/L | 0.0338 | 1.10% |

Sequence No.: 42
Sample ID: RG42 B SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 324
Date Collected: 8/6/2010 4:38:37 PM
Data Type: Original

DEL

Nebulizer Parameters: RG42 B SWC
Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG42 B SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|--------|
| ScA 357.253 | 1959222.9 | 103.0 | % | 0.84 | | | 0.81% |
| ScR 361.383 | 304150.4 | 103.9 | % | 0.37 | | | 0.35% |
| Ag 328.068† | 70.7 | 0.00032 | mg/L | 0.000096 | 0.00063 mg/L | 0.000192 | 30.40% |
| Al 308.215† | 93083.1 | 73.42 | mg/L | 0.298 | 146.8 mg/L | 0.60 | 0.41% |
| As 188.979† | -16.6 | 0.07788 | mg/L | 0.000687 | 0.1558 mg/L | 0.00137 | 0.88% |
| B 249.677† | 397.4 | 0.1145 | mg/L | 0.00075 | 0.2289 mg/L | 0.00151 | 0.66% |
| Ba 233.527† | 943.4 | 0.2679 | mg/L | 0.00122 | 0.5359 mg/L | 0.00243 | 0.45% |
| Be 313.042† | 807.9 | 0.00117 | mg/L | 0.000020 | 0.00234 mg/L | 0.000039 | 1.68% |
| Ca 317.933† | 455978.1 | 31.40 | mg/L | 0.134 | 62.81 mg/L | 0.269 | 0.43% |
| Cd 228.802† | 828.5 | 0.03902 | mg/L | 0.000364 | 0.07805 mg/L | 0.000729 | 0.93% |
| Co 228.616† | 1824.2 | 0.05004 | mg/L | 0.000669 | 0.1001 mg/L | 0.00134 | 1.34% |
| Cr 267.716† | 1757.9 | 0.3440 | mg/L | 0.00076 | 0.6880 mg/L | 0.00153 | 0.22% |
| Cu 324.752† | 149507.5 | 0.5449 | mg/L | 0.00472 | 1.090 mg/L | 0.0094 | 0.87% |
| Fe 273.955† | 181942.7 | 159.1 | mg/L | 0.93 | 318.2 mg/L | 1.86 | 0.58% |
| K 766.490† | 12795.3 | 8.805 | mg/L | 0.0738 | 17.61 mg/L | 0.148 | 0.84% |
| Mg 279.077† | 35391.0 | 37.63 | mg/L | 0.163 | 75.25 mg/L | 0.327 | 0.43% |
| Mn 257.610† | 52848.2 | 1.678 | mg/L | 0.0175 | 3.355 mg/L | 0.0349 | 1.04% |
| Mo 202.031† | 570.0 | 0.03261 | mg/L | 0.000567 | 0.06523 mg/L | 0.001135 | 1.74% |
| Na 589.592† | 522323.5 | 43.81 | mg/L | 0.365 | 87.62 mg/L | 0.729 | 0.83% |
| Na 330.237† | 1398.5 | 48.12 | mg/L | 0.186 | 96.24 mg/L | 0.372 | 0.39% |
| Ni 231.604† | 401.5 | 0.2358 | mg/L | 0.00225 | 0.4717 mg/L | 0.00450 | 0.96% |
| Pb 220.353† | 5677.1 | 0.7717 | mg/L | 0.00704 | 1.543 mg/L | 0.0141 | 0.91% |
| Sb 206.836† | 341.4 | 0.1316 | mg/L | 0.00089 | 0.2632 mg/L | 0.00178 | 0.68% |
| Se 196.026† | 37.0 | 0.02698 | mg/L | 0.003895 | 0.05396 mg/L | 0.007790 | 14.44% |
| Si 288.158† | 2371.4 | 1.606 | mg/L | 0.0139 | 3.212 mg/L | 0.0278 | 0.86% |
| Sn 189.927† | 155.9 | 0.04622 | mg/L | 0.001384 | 0.09244 mg/L | 0.002768 | 2.99% |
| Sr 421.552† | 213527.1 | 0.3187 | mg/L | 0.00195 | 0.6375 mg/L | 0.00391 | 0.61% |
| Ti 334.903† | 109792.6 | 4.998 | mg/L | 0.0340 | 9.995 mg/L | 0.0680 | 0.68% |
| Tl 190.801† | -27.4 | 0.00973 | mg/L | 0.002364 | 0.01946 mg/L | 0.004728 | 24.29% |
| V 292.402† | 32667.9 | 0.3139 | mg/L | 0.00404 | 0.6279 mg/L | 0.00808 | 1.29% |
| Zn 206.200† | 4339.3 | 6.390 | mg/L | 0.0125 | 12.78 mg/L | 0.025 | 0.20% |

Sequence No.: 43
Sample ID: RG42 C SWC
Analyst: ALA
Dilution: 2X

DEL

Autosampler Location: 325
Date Collected: 8/6/2010 4:42:34 PM
Data Type: Original

Nebulizer Parameters: RG42 C SWC

Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RG42 C SWC

| Analyte | Mean Corrected Intensity | Conc. | Calib. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------|--------------|----------|--------------------|----------|---------|
| ScA 357.253 | 2007583.3 | 105.6 | % | 0.28 | | | 0.26% |
| ScR 361.383 | 308912.1 | 105.5 | % | 0.21 | | | 0.20% |
| Ag 328.068† | 21.5 | 0.00011 | mg/L | 0.000216 | 0.00022 mg/L | 0.000433 | 195.85% |
| Al 308.215† | 91212.6 | 71.95 | mg/L | 0.256 | 143.9 mg/L | 0.51 | 0.36% |
| As 188.979† | -104.4 | 0.01644 | mg/L | 0.002108 | 0.03288 mg/L | 0.004216 | 12.82% |
| B 249.677† | 56.1 | 0.01604 | mg/L | 0.002118 | 0.03207 mg/L | 0.004236 | 13.21% |
| Ba 233.527† | 1244.5 | 0.3624 | mg/L | 0.00161 | 0.7248 mg/L | 0.00321 | 0.44% |
| Be 313.042† | 759.0 | 0.00111 | mg/L | 0.000013 | 0.00222 mg/L | 0.000027 | 1.20% |
| Ca 317.933† | 549693.7 | 37.86 | mg/L | 0.241 | 75.71 mg/L | 0.481 | 0.64% |
| Cd 228.802† | 114.8 | 0.00572 | mg/L | 0.000064 | 0.01143 mg/L | 0.000128 | 1.12% |
| Co 228.616† | 1721.4 | 0.04735 | mg/L | 0.000327 | 0.09470 mg/L | 0.000655 | 0.69% |
| Cr 267.716† | 1204.6 | 0.2354 | mg/L | 0.00068 | 0.4708 mg/L | 0.00136 | 0.29% |
| Cu 324.752† | 90342.0 | 0.3297 | mg/L | 0.00331 | 0.6594 mg/L | 0.00663 | 1.00% |
| Fe 273.955† | 130211.0 | 113.9 | mg/L | 0.45 | 227.8 mg/L | 0.90 | 0.39% |
| K 766.490† | 6053.6 | 4.166 | mg/L | 0.0207 | 8.332 mg/L | 0.0415 | 0.50% |
| Mg 279.077† | 25834.4 | 27.46 | mg/L | 0.141 | 54.93 mg/L | 0.282 | 0.51% |
| Mn 257.610† | 39496.5 | 1.253 | mg/L | 0.0077 | 2.507 mg/L | 0.0154 | 0.61% |
| Mo 202.031† | 264.9 | 0.01475 | mg/L | 0.000439 | 0.02951 mg/L | 0.000878 | 2.98% |
| Na 589.592† | 37172.8 | 3.118 | mg/L | 0.0067 | 6.236 mg/L | 0.0134 | 0.22% |
| Na 330.237† | 64.7 | 3.272 | mg/L | 0.0645 | 6.544 mg/L | 0.1290 | 1.97% |
| Ni 231.604† | 261.4 | 0.1535 | mg/L | 0.00208 | 0.3071 mg/L | 0.00416 | 1.36% |
| Pb 220.353† | 2423.5 | 0.3332 | mg/L | 0.00290 | 0.6663 mg/L | 0.00580 | 0.87% |
| Sb 206.836† | 27.1 | 0.01499 | mg/L | 0.000393 | 0.02999 mg/L | 0.000787 | 2.62% |
| Se 196.026† | 31.1 | 0.02191 | mg/L | 0.005381 | 0.04382 mg/L | 0.010761 | 24.56% |
| Si 288.158† | 2694.2 | 1.824 | mg/L | 0.0106 | 3.649 mg/L | 0.0212 | 0.58% |
| Sn 189.927† | 39.4 | 0.01471 | mg/L | 0.001012 | 0.02942 mg/L | 0.002023 | 6.88% |
| Sr 421.552† | 149783.6 | 0.2236 | mg/L | 0.00095 | 0.4472 mg/L | 0.00191 | 0.43% |
| Ti 334.903† | 107596.9 | 4.897 | mg/L | 0.0254 | 9.795 mg/L | 0.0507 | 0.52% |
| Tl 190.801† | -15.8 | 0.00899 | mg/L | 0.003026 | 0.01798 mg/L | 0.006051 | 33.65% |
| V 292.402† | 28531.3 | 0.2763 | mg/L | 0.00038 | 0.5525 mg/L | 0.00077 | 0.14% |
| Zn 206.200† | 1510.9 | 2.224 | mg/L | 0.0067 | 4.448 mg/L | 0.0134 | 0.30% |

Sequence No.: 44
 Sample ID: RG42 D SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 326
 Date Collected: 8/6/2010 4:46:30 PM
 Data Type: Original

DEL

Nebulizer Parameters: RG42 D SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG42 D SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | Std.Dev. | RSD |
|-------------|----------------|----------|-----------------|----------|----------|-------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | | |
| ScA 357.253 | 1977799.3 | 104.0 | % | 0.58 | | | | 0.56% |
| ScR 361.383 | 303673.5 | 103.8 | % | 1.45 | | | | 1.39% |
| Ag 328.068† | -15.4 | -0.00008 | mg/L | 0.000259 | -0.00016 | mg/L | 0.000518 | 329.65% |
| Al 308.215† | 91364.1 | 72.07 | mg/L | 0.854 | 144.1 | mg/L | 1.71 | 1.18% |
| As 188.979† | -53.1 | 0.05299 | mg/L | 0.003479 | 0.1060 | mg/L | 0.00696 | 6.57% |
| B 249.677† | 296.7 | 0.08544 | mg/L | 0.002296 | 0.1709 | mg/L | 0.00459 | 2.69% |
| Ba 233.527† | 721.4 | 0.2044 | mg/L | 0.00288 | 0.4088 | mg/L | 0.00576 | 1.41% |
| Be 313.042† | 754.8 | 0.00109 | mg/L | 0.000044 | 0.00217 | mg/L | 0.000087 | 4.01% |
| Ca 317.933† | 1759129.3 | 121.2 | mg/L | 1.80 | 242.3 | mg/L | 3.60 | 1.49% |
| Cd 228.802† | 381.5 | 0.01808 | mg/L | 0.000275 | 0.03616 | mg/L | 0.000550 | 1.52% |
| Co 228.616† | 1427.7 | 0.03721 | mg/L | 0.000239 | 0.07441 | mg/L | 0.000477 | 0.64% |
| Cr 267.716† | 929.2 | 0.1791 | mg/L | 0.00108 | 0.3582 | mg/L | 0.00217 | 0.61% |
| Cu 324.752† | 71773.5 | 0.2631 | mg/L | 0.00116 | 0.5262 | mg/L | 0.00232 | 0.44% |
| Fe 273.955† | 134190.9 | 117.4 | mg/L | 1.53 | 234.7 | mg/L | 3.05 | 1.30% |
| K 766.490† | 11080.2 | 7.625 | mg/L | 0.1045 | 15.25 | mg/L | 0.209 | 1.37% |
| Mg 279.077† | 34688.6 | 36.89 | mg/L | 0.452 | 73.77 | mg/L | 0.904 | 1.22% |
| Mn 257.610† | 38760.6 | 1.230 | mg/L | 0.0168 | 2.460 | mg/L | 0.0335 | 1.36% |
| Mo 202.031† | 233.5 | 0.01148 | mg/L | 0.000546 | 0.02297 | mg/L | 0.001091 | 4.75% |
| Na 589.592† | 429359.0 | 36.01 | mg/L | 0.517 | 72.03 | mg/L | 1.033 | 1.43% |
| Na 330.237† | 1104.7 | 39.45 | mg/L | 0.295 | 78.91 | mg/L | 0.589 | 0.75% |
| Ni 231.604† | 207.0 | 0.1216 | mg/L | 0.00536 | 0.2431 | mg/L | 0.01072 | 4.41% |
| Pb 220.353† | 1602.3 | 0.2215 | mg/L | 0.00166 | 0.4430 | mg/L | 0.00332 | 0.75% |
| Sb 206.836† | 153.2 | 0.06292 | mg/L | 0.001745 | 0.1258 | mg/L | 0.00349 | 2.77% |
| Se 196.026† | 63.0 | 0.04136 | mg/L | 0.002112 | 0.08271 | mg/L | 0.004224 | 5.11% |
| Si 288.158† | 3275.1 | 2.218 | mg/L | 0.0384 | 4.436 | mg/L | 0.0767 | 1.73% |
| Sn 189.927† | 46.4 | 0.02060 | mg/L | 0.001707 | 0.04121 | mg/L | 0.003414 | 8.29% |
| Sr 421.552† | 328813.7 | 0.4908 | mg/L | 0.00674 | 0.9817 | mg/L | 0.01349 | 1.37% |
| Ti 334.903† | 112670.3 | 5.123 | mg/L | 0.0725 | 10.25 | mg/L | 0.145 | 1.41% |
| Tl 190.801† | -4.9 | 0.01552 | mg/L | 0.001842 | 0.03104 | mg/L | 0.003684 | 11.87% |
| V 292.402† | 31112.4 | 0.3018 | mg/L | 0.00141 | 0.6035 | mg/L | 0.00282 | 0.47% |
| Zn 206.200† | 1894.5 | 2.789 | mg/L | 0.0394 | 5.578 | mg/L | 0.0789 | 1.41% |

Sequence No.: 45
 Sample ID: RG42 E SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 327
 Date Collected: 8/6/2010 4:50:42 PM
 Data Type: Original

Nebulizer Parameters: RG42 E SWC

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RG42 E SWC

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|--------------------|----------|--------------------|----------|--------|
| ScA 357.253 | 2010438.6 | 105.7 % | 1.20 | | | 1.13% |
| ScR 361.383 | 310067.5 | 105.9 % | 1.06 | | | 1.00% |
| Ag 328.068† | 94.9 | 0.00050 mg/L | 0.000088 | 0.00100 mg/L | 0.000176 | 17.67% |
| Al 308.215† | 118223.5 | 93.26 mg/L | 1.335 | 186.5 mg/L | 2.67 | 1.43% |
| As 188.979† | -92.7 | 0.03211 mg/L | 0.002690 | 0.06421 mg/L | 0.005379 | 8.38% |
| B 249.677† | 117.4 | 0.03368 mg/L | 0.001898 | 0.06736 mg/L | 0.003795 | 5.63% |
| Ba 233.527† | 1490.0 | 0.4326 mg/L | 0.00500 | 0.8653 mg/L | 0.00999 | 1.15% |
| Be 313.042† | 1090.1 | 0.00164 mg/L | 0.000041 | 0.00328 mg/L | 0.000082 | 2.49% |
| Ca 317.933† | 1317966.9 | 90.77 mg/L | 1.478 | 181.5 mg/L | 2.96 | 1.63% |
| Cd 228.802† | 143.4 | 0.00707 mg/L | 0.000211 | 0.01413 mg/L | 0.000423 | 2.99% |
| Co 228.616† | 2373.4 | 0.06771 mg/L | 0.001022 | 0.1354 mg/L | 0.00204 | 1.51% |
| Cr 267.716† | 1410.3 | 0.2744 mg/L | 0.00321 | 0.5488 mg/L | 0.00642 | 1.17% |
| Cu 324.752† | 135739.4 | 0.4943 mg/L | 0.00498 | 0.9887 mg/L | 0.00995 | 1.01% |
| Fe 273.955† | 166080.9 | 145.2 mg/L | 2.08 | 290.5 mg/L | 4.15 | 1.43% |
| K 766.490† | 8276.1 | 5.695 mg/L | 0.0815 | 11.39 mg/L | 0.163 | 1.43% |
| Mg 279.077† | 36322.0 | 38.62 mg/L | 0.566 | 77.23 mg/L | 1.132 | 1.47% |
| Mn 257.610† | 49016.3 | 1.556 mg/L | 0.0251 | 3.111 mg/L | 0.0501 | 1.61% |
| Mo 202.031† | 361.8 | 0.01947 mg/L | 0.000861 | 0.03895 mg/L | 0.001721 | 4.42% |
| Na 589.592† | 40971.6 | 3.437 mg/L | 0.0533 | 6.873 mg/L | 0.1065 | 1.55% |
| Na 330.237† | 72.4 | 3.865 mg/L | 0.2217 | 7.730 mg/L | 0.4434 | 5.74% |
| Ni 231.604† | 363.5 | 0.2135 mg/L | 0.00340 | 0.4269 mg/L | 0.00680 | 1.59% |
| Pb 220.353† | 3873.6 | 0.5312 mg/L | 0.00718 | 1.062 mg/L | 0.0144 | 1.35% |
| Sb 206.836† | 38.4 | 0.01973 mg/L | 0.001565 | 0.03946 mg/L | 0.003130 | 7.93% |
| Se 196.026† | 54.7 | 0.03692 mg/L | 0.002544 | 0.07384 mg/L | 0.005088 | 6.89% |
| Si 288.158† | 2707.4 | 1.833 mg/L | 0.0165 | 3.667 mg/L | 0.0330 | 0.90% |
| Sn 189.927† | 57.7 | 0.02239 mg/L | 0.001158 | 0.04479 mg/L | 0.002316 | 5.17% |
| Sr 421.552† | 254978.8 | 0.3806 mg/L | 0.00572 | 0.7612 mg/L | 0.01144 | 1.50% |
| Ti 334.903† | 118935.6 | 5.410 mg/L | 0.0823 | 10.82 mg/L | 0.165 | 1.52% |
| Tl 190.801† | -9.1 | 0.01759 mg/L | 0.000965 | 0.03517 mg/L | 0.001929 | 5.49% |
| V 292.402† | 35126.9 | 0.3399 mg/L | 0.00324 | 0.6798 mg/L | 0.00649 | 0.95% |
| Zn 206.200† | 1882.1 | 2.770 mg/L | 0.0289 | 5.540 mg/L | 0.0579 | 1.04% |

Sequence No.: 46
 Sample ID: RG47 A SWC
 Analyst: ALA
 Dilution: 5X

Autosampler Location: 328
 Date Collected: 8/6/2010 4:54:39 PM
 Data Type: Original

*AS-9
 Ret
 DEL*

Nebulizer Parameters: RG47 A SWC

Analyte Back Pressure Flow
 All 201.0 kPa 0.75 L/min

Mean Data: RG47 A SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|---------|-----------------|----------|---------|-------|--------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1995498.3 | 104.9 | % | 1.16 | | | 1.11% |
| ScR 361.383 | 308704.1 | 105.5 | % | 0.64 | | | 0.61% |
| Ag 328.068† | 123.2 | 0.00052 | mg/L | 0.000213 | 0.00258 | mg/L | 41.30% |
| Al 308.215† | 53347.3 | 42.08 | mg/L | 0.379 | 210.4 | mg/L | 0.90% |
| As 188.979† | -45.8 | 0.01655 | mg/L | 0.001239 | 0.08274 | mg/L | 7.49% |
| B 249.677† | 94.4 | 0.02714 | mg/L | 0.000853 | 0.1357 | mg/L | 3.14% |
| Ba 233.527† | 2358.5 | 0.6951 | mg/L | 0.00470 | 3.475 | mg/L | 0.68% |
| Be 313.042† | 355.6 | 0.00050 | mg/L | 0.000010 | 0.00249 | mg/L | 1.94% |
| Ca 317.933† | 584021.3 | 40.22 | mg/L | 0.307 | 201.1 | mg/L | 0.76% |
| Cd 228.802† | 468.4 | 0.02220 | mg/L | 0.000461 | 0.1110 | mg/L | 2.08% |
| Co 228.616† | 1232.2 | 0.03453 | mg/L | 0.000344 | 0.1726 | mg/L | 1.00% |
| Cr 267.716† | 1138.7 | 0.2241 | mg/L | 0.00038 | 1.120 | mg/L | 0.17% |
| Cu 324.752† | 123127.9 | 0.4494 | mg/L | 0.00629 | 2.247 | mg/L | 1.40% |
| Fe 273.955† | 149152.8 | 130.4 | mg/L | 1.09 | 652.2 | mg/L | 0.84% |
| K 766.490† | 3902.9 | 2.686 | mg/L | 0.0517 | 13.43 | mg/L | 1.92% |
| Mg 279.077† | 20673.1 | 21.96 | mg/L | 0.136 | 109.8 | mg/L | 0.62% |
| Mn 257.610† | 49682.2 | 1.577 | mg/L | 0.0108 | 7.885 | mg/L | 0.68% |
| Mo 202.031† | 264.1 | 0.01467 | mg/L | 0.000334 | 0.07333 | mg/L | 2.28% |
| Na 589.592† | 13976.5 | 1.172 | mg/L | 0.0109 | 5.862 | mg/L | 0.93% |
| Na 330.237† | 13.9 | 1.170 | mg/L | 0.1815 | 5.848 | mg/L | 15.52% |
| Ni 231.604† | 357.5 | 0.2099 | mg/L | 0.00075 | 1.050 | mg/L | 0.35% |
| Pb 220.353† | 863.8 | 0.1151 | mg/L | 0.00161 | 0.5755 | mg/L | 1.40% |
| Sb 206.836† | 30.5 | 0.01320 | mg/L | 0.000681 | 0.06600 | mg/L | 5.16% |
| Se 196.026† | 26.4 | 0.01808 | mg/L | 0.003666 | 0.09040 | mg/L | 20.27% |
| Si 288.158† | 2632.5 | 1.783 | mg/L | 0.0042 | 8.913 | mg/L | 0.23% |
| Sn 189.927† | 34.8 | 0.01258 | mg/L | 0.001261 | 0.06288 | mg/L | 10.03% |
| Sr 421.552† | 84660.0 | 0.1264 | mg/L | 0.00104 | 0.6319 | mg/L | 0.83% |
| Ti 334.903† | 59569.3 | 2.710 | mg/L | 0.0216 | 13.55 | mg/L | 0.80% |
| Tl 190.801† | -11.8 | 0.01423 | mg/L | 0.002077 | 0.07116 | mg/L | 14.59% |
| V 292.402† | 16744.9 | 0.1559 | mg/L | 0.00231 | 0.7795 | mg/L | 1.48% |
| Zn 206.200† | 843.2 | 1.241 | mg/L | 0.0104 | 6.205 | mg/L | 0.84% |

Sequence No.: 47
 Sample ID: RF47 MBSPK SWC
 Analyst: ALA
 Dilution: 2X

Autosampler Location: 329
 Date Collected: 8/6/2010 4:58:35 PM
 Data Type: Original

Nebulizer Parameters: RF47 MBSPK SWC
 Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: RF47 MBSPK SWC

| Analyte | Mean Corrected | | Calib. Units | Std.Dev. | Sample | | RSD |
|-------------|----------------|---------------|--------------|----------|---------------|----------|---------|
| | Intensity | Conc. | | | Conc. | Units | |
| ScA 357.253 | 1984923.2 | 104.4 % | % | 0.99 | | | 0.95% |
| ScR 361.383 | 304798.6 | 104.1 % | % | 0.44 | | | 0.42% |
| Ag 328.068† | 92642.3 | 0.5225 mg/L | mg/L | 0.00286 | 1.045 mg/L | 0.0057 | 0.55% |
| Al 308.215† | 2730.0 | 2.144 mg/L | mg/L | 0.0152 | 4.288 mg/L | 0.0304 | 0.71% |
| As 188.979† | 3055.1 | 2.072 mg/L | mg/L | 0.0211 | 4.144 mg/L | 0.0423 | 1.02% |
| B 249.677† | -8.5 | -0.00377 mg/L | mg/L | 0.001173 | -0.00753 mg/L | 0.002346 | 31.14% |
| Ba 233.527† | 6711.9 | 2.013 mg/L | mg/L | 0.0147 | 4.026 mg/L | 0.0294 | 0.73% |
| Be 313.042† | 284287.1 | 0.4918 mg/L | mg/L | 0.00266 | 0.9836 mg/L | 0.00533 | 0.54% |
| Ca 317.933† | 153191.3 | 10.55 mg/L | mg/L | 0.050 | 21.10 mg/L | 0.101 | 0.48% |
| Cd 228.802† | 11526.2 | 0.5336 mg/L | mg/L | 0.00417 | 1.067 mg/L | 0.0083 | 0.78% |
| Co 228.616† | 15778.4 | 0.5232 mg/L | mg/L | 0.00497 | 1.046 mg/L | 0.0099 | 0.95% |
| Cr 267.716† | 2625.5 | 0.5094 mg/L | mg/L | 0.00264 | 1.019 mg/L | 0.0053 | 0.52% |
| Cu 324.752† | 143015.4 | 0.5130 mg/L | mg/L | 0.00335 | 1.026 mg/L | 0.0067 | 0.65% |
| Fe 273.955† | 2575.4 | 2.250 mg/L | mg/L | 0.0192 | 4.499 mg/L | 0.0384 | 0.85% |
| K 766.490† | 15972.0 | 10.99 mg/L | mg/L | 0.100 | 21.98 mg/L | 0.201 | 0.91% |
| Mg 279.077† | 9986.2 | 10.64 mg/L | mg/L | 0.029 | 21.28 mg/L | 0.057 | 0.27% |
| Mn 257.610† | 15123.5 | 0.4804 mg/L | mg/L | 0.00109 | 0.9608 mg/L | 0.00219 | 0.23% |
| Mo 202.031† | 19.5 | 0.00095 mg/L | mg/L | 0.000107 | 0.00190 mg/L | 0.000215 | 11.31% |
| Na 589.592† | 114748.2 | 9.625 mg/L | mg/L | 0.0384 | 19.25 mg/L | 0.077 | 0.40% |
| Na 330.237† | 311.3 | 10.65 mg/L | mg/L | 0.213 | 21.30 mg/L | 0.426 | 2.00% |
| Ni 231.604† | 862.2 | 0.5063 mg/L | mg/L | 0.00133 | 1.013 mg/L | 0.0027 | 0.26% |
| Pb 220.353† | 15051.6 | 2.043 mg/L | mg/L | 0.0216 | 4.086 mg/L | 0.0433 | 1.06% |
| Sb 206.836† | 6.0 | -0.00140 mg/L | mg/L | 0.002093 | -0.00280 mg/L | 0.004186 | 149.37% |
| Se 196.026† | 2669.4 | 2.101 mg/L | mg/L | 0.0224 | 4.203 mg/L | 0.0447 | 1.06% |
| Si 288.158† | 7.2 | 0.00674 mg/L | mg/L | 0.003368 | 0.01349 mg/L | 0.006735 | 49.93% |
| Sn 189.927† | -10.8 | -0.00245 mg/L | mg/L | 0.000114 | -0.00490 mg/L | 0.000228 | 4.65% |
| Sr 421.552† | 331782.2 | 0.4953 mg/L | mg/L | 0.00372 | 0.9905 mg/L | 0.00743 | 0.75% |
| Ti 334.903† | 66.2 | 0.00226 mg/L | mg/L | 0.000386 | 0.00452 mg/L | 0.000772 | 17.08% |
| Tl 190.801† | 3713.8 | 2.051 mg/L | mg/L | 0.0222 | 4.102 mg/L | 0.0444 | 1.08% |
| V 292.402† | 51639.7 | 0.5271 mg/L | mg/L | 0.00474 | 1.054 mg/L | 0.0095 | 0.90% |
| Zn 206.200† | 337.8 | 0.4976 mg/L | mg/L | 0.00517 | 0.9951 mg/L | 0.01035 | 1.04% |

Sequence No.: 48
Sample ID: RF42 MBSPK SWC
Analyst: ALA
Dilution: 2X

Autosampler Location: 330
Date Collected: 8/6/2010 5:02:46 PM
Data Type: Original

Nebulizer Parameters: RF42 MBSPK SWC
Analyte Back Pressure Flow
All 200.0 kPa 0.75 L/min

Mean Data: RF42 MBSPK SWC

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|---------------|-----------------|--------------------|----------|---------|
| ScA 357.253 | 1956929.7 | 102.9 % | 0.98 | | | 0.95% |
| ScR 361.383 | 302902.5 | 103.5 % | 1.13 | | | 1.09% |
| Ag 328.068† | 93339.4 | 0.5264 mg/L | 0.00310 | 1.053 mg/L | 0.0062 | 0.59% |
| Al 308.215† | 2692.1 | 2.114 mg/L | 0.0257 | 4.228 mg/L | 0.0513 | 1.21% |
| As 188.979† | 3064.7 | 2.078 mg/L | 0.0233 | 4.157 mg/L | 0.0466 | 1.12% |
| B 249.677† | -11.3 | -0.00460 mg/L | 0.000168 | -0.00919 mg/L | 0.000336 | 3.66% |
| Ba 233.527† | 6751.7 | 2.025 mg/L | 0.0255 | 4.050 mg/L | 0.0510 | 1.26% |
| Be 313.042† | 286479.6 | 0.4956 mg/L | 0.00326 | 0.9912 mg/L | 0.00652 | 0.66% |
| Ca 317.933† | 154447.4 | 10.64 mg/L | 0.087 | 21.27 mg/L | 0.173 | 0.81% |
| Cd 228.802† | 11604.6 | 0.5372 mg/L | 0.00357 | 1.074 mg/L | 0.0071 | 0.66% |
| Co 228.616† | 15966.4 | 0.5294 mg/L | 0.00188 | 1.059 mg/L | 0.0038 | 0.36% |
| Cr 267.716† | 2639.2 | 0.5121 mg/L | 0.00371 | 1.024 mg/L | 0.0074 | 0.73% |
| Cu 324.752† | 139231.5 | 0.4994 mg/L | 0.00374 | 0.9988 mg/L | 0.00748 | 0.75% |
| Fe 273.955† | 2526.1 | 2.206 mg/L | 0.0277 | 4.413 mg/L | 0.0554 | 1.25% |
| K 766.490† | 15916.7 | 10.95 mg/L | 0.121 | 21.91 mg/L | 0.243 | 1.11% |
| Mg 279.077† | 9888.0 | 10.53 mg/L | 0.154 | 21.07 mg/L | 0.307 | 1.46% |
| Mn 257.610† | 15019.1 | 0.4771 mg/L | 0.00617 | 0.9541 mg/L | 0.01235 | 1.29% |
| Mo 202.031† | 25.0 | 0.00127 mg/L | 0.000132 | 0.00254 mg/L | 0.000265 | 10.43% |
| Na 589.592† | 115587.6 | 9.695 mg/L | 0.0817 | 19.39 mg/L | 0.163 | 0.84% |
| Na 330.237† | 313.2 | 10.71 mg/L | 0.034 | 21.42 mg/L | 0.068 | 0.32% |
| Ni 231.604† | 863.5 | 0.5070 mg/L | 0.00567 | 1.014 mg/L | 0.0113 | 1.12% |
| Pb 220.353† | 14798.6 | 2.009 mg/L | 0.0080 | 4.018 mg/L | 0.0161 | 0.40% |
| Sb 206.836† | 17.6 | 0.00297 mg/L | 0.000527 | 0.00593 mg/L | 0.001053 | 17.75% |
| Se 196.026† | 2659.0 | 2.093 mg/L | 0.0294 | 4.186 mg/L | 0.0589 | 1.41% |
| Si 288.158† | 7.2 | 0.00679 mg/L | 0.004702 | 0.01357 mg/L | 0.009403 | 69.27% |
| Sn 189.927† | -7.3 | -0.00148 mg/L | 0.000808 | -0.00297 mg/L | 0.001616 | 54.43% |
| Sr 421.552† | 335010.8 | 0.5001 mg/L | 0.00353 | 1.000 mg/L | 0.0071 | 0.71% |
| Ti 334.903† | 15.5 | -0.00005 mg/L | 0.000390 | -0.00011 mg/L | 0.000779 | 716.29% |
| Tl 190.801† | 3729.0 | 2.059 mg/L | 0.0271 | 4.119 mg/L | 0.0542 | 1.32% |
| V 292.402† | 52754.4 | 0.5384 mg/L | 0.00401 | 1.077 mg/L | 0.0080 | 0.74% |
| Zn 206.200† | 338.6 | 0.4987 mg/L | 0.00474 | 0.9973 mg/L | 0.00948 | 0.95% |

Sequence No.: 49
 Sample ID: CV 12
 Analyst: ALA
 Dilution: 1X

Autosampler Location: 7
 Date Collected: 8/6/2010 5:06:57 PM
 Data Type: Original

Nebulizer Parameters: CV

Analyte Back Pressure Flow
 All 200.0 kPa 0.75 L/min

Mean Data: CV

| Analyte | Mean Corrected Intensity | Calib. Conc. Units | Std.Dev. | Sample Conc. Units | Std.Dev. | RSD |
|-------------|--------------------------|-----------------------|----------|--------------------|----------|-------|
| ScA 357.253 | 1973028.1 | 103.8 % | 0.01 | | | 0.01% |
| ScR 361.383 | 299585.7 | 102.4 % | 1.48 | | | 1.45% |
| Ag 328.068† | 187271.5 | 1.056 mg/L | 0.0071 | 1.056 mg/L | 0.0071 | 0.67% |
| Al 308.215† | 2824.0 | 2.194 mg/L | 0.0310 | 2.194 mg/L | 0.0310 | 1.41% |
| As 188.979† | 3096.5 | 2.118 mg/L | 0.0045 | 2.118 mg/L | 0.0045 | 0.21% |
| B 249.677† | 3516.9 | 1.012 mg/L | 0.0140 | 1.012 mg/L | 0.0140 | 1.39% |
| Ba 233.527† | 3481.6 | 1.044 mg/L | 0.0154 | 1.044 mg/L | 0.0154 | 1.48% |
| Be 313.042† | 585035.3 | 1.012 mg/L | 0.0138 | 1.012 mg/L | 0.0138 | 1.36% |
| Ca 317.933† | 33207.0 | 2.287 mg/L | 0.0438 | 2.287 mg/L | 0.0438 | 1.92% |
| Cd 228.802† | 23773.2 | 1.108 mg/L | 0.0075 | 1.108 mg/L | 0.0075 | 0.68% |
| Co 228.616† | 32835.1 | 1.088 mg/L | 0.0070 | 1.088 mg/L | 0.0070 | 0.64% |
| Cr 267.716† | 5463.0 | 1.063 mg/L | 0.0128 | 1.063 mg/L | 0.0128 | 1.20% |
| Cu 324.752† | 298655.8 | 1.070 mg/L | 0.0069 | 1.070 mg/L | 0.0069 | 0.65% |
| Fe 273.955† | 2537.5 | 2.213 mg/L | 0.0347 | 2.213 mg/L | 0.0347 | 1.57% |
| K 766.490† | 33085.4 | 22.77 mg/L | 0.290 | 22.77 mg/L | 0.290 | 1.27% |
| Mg 279.077† | 2094.6 | 2.237 mg/L | 0.0337 | 2.237 mg/L | 0.0337 | 1.51% |
| Mn 257.610† | 31644.2 | 1.005 mg/L | 0.0170 | 1.005 mg/L | 0.0170 | 1.69% |
| Mo 202.031† | 18248.2 | 1.062 mg/L | 0.0089 | 1.062 mg/L | 0.0089 | 0.84% |
| Na 589.592† | 594786.2 | 49.89 mg/L | 0.734 | 49.89 mg/L | 0.734 | 1.47% |
| Na 330.237† | 1601.4 | 55.12 mg/L | 0.718 | 55.12 mg/L | 0.718 | 1.30% |
| Ni 231.604† | 1798.7 | 1.058 mg/L | 0.0181 | 1.058 mg/L | 0.0181 | 1.72% |
| Pb 220.353† | 15078.7 | 2.048 mg/L | 0.0175 | 2.048 mg/L | 0.0175 | 0.85% |
| Sb 206.836† | 6049.6 | 2.260 mg/L | 0.0047 | 2.260 mg/L | 0.0047 | 0.21% |
| Se 196.026† | 2704.5 | 2.130 mg/L | 0.0070 | 2.130 mg/L | 0.0070 | 0.33% |
| Si 288.158† | 3365.9 | 2.283 mg/L | 0.0399 | 2.283 mg/L | 0.0399 | 1.75% |
| Sn 189.927† | 4104.9 | 1.119 mg/L | 0.0020 | 1.119 mg/L | 0.0020 | 0.18% |
| Sr 421.552† | 688633.0 | 1.028 mg/L | 0.0127 | 1.028 mg/L | 0.0127 | 1.23% |
| Ti 334.903† | 23735.7 | 1.079 mg/L | 0.0201 | 1.079 mg/L | 0.0201 | 1.86% |
| Tl 190.801† | 3782.0 | 2.090 mg/L | 0.0063 | 2.090 mg/L | 0.0063 | 0.30% |
| V 292.402† | 106463.2 | 1.087 mg/L | 0.0105 | 1.087 mg/L | 0.0105 | 0.96% |
| Zn 206.200† | 706.5 | 1.040 mg/L | 0.0155 | 1.040 mg/L | 0.0155 | 1.49% |

Sequence No.: 50

Sample ID: CB *17*

Analyst: ALA

Dilution: 1X

Autosampler Location: 1

Date Collected: 8/6/2010 5:11:10 PM

Data Type: Original

Nebulizer Parameters: CB

| Analyte | Back Pressure | Flow |
|---------|---------------|------------|
| All | 200.0 kPa | 0.75 L/min |

Mean Data: CB

| Analyte | Mean Corrected Intensity | Conc. Units | Calib. Units | Std.Dev. | Conc. Units | Sample Units | Std.Dev. | RSD |
|-------------|--------------------------|-------------|--------------|----------|-------------|--------------|----------|---------|
| ScA 357.253 | 1970974.8 | 103.6 | % | 0.58 | | | | 0.56% |
| ScR 361.383 | 304668.5 | 104.1 | % | 0.65 | | | | 0.63% |
| Ag 328.068† | -3.9 | -0.00002 | mg/L | 0.000146 | -0.00002 | mg/L | 0.000146 | 671.69% |
| Al 308.215† | 5.8 | 0.00459 | mg/L | 0.004992 | 0.00459 | mg/L | 0.004992 | 108.78% |
| As 188.979† | 0.2 | 0.00011 | mg/L | 0.002684 | 0.00011 | mg/L | 0.002684 | >999.9% |
| B 249.677† | -3.4 | -0.00097 | mg/L | 0.000934 | -0.00097 | mg/L | 0.000934 | 96.36% |
| Ba 233.527† | 5.1 | 0.00152 | mg/L | 0.000884 | 0.00152 | mg/L | 0.000884 | 58.00% |
| Be 313.042† | 72.8 | 0.00013 | mg/L | 0.000051 | 0.00013 | mg/L | 0.000051 | 40.14% |
| Ca 317.933† | 34.6 | 0.00238 | mg/L | 0.000423 | 0.00238 | mg/L | 0.000423 | 17.76% |
| Cd 228.802† | -5.8 | -0.00027 | mg/L | 0.000153 | -0.00027 | mg/L | 0.000153 | 56.36% |
| Co 228.616† | 1.0 | 0.00003 | mg/L | 0.000388 | 0.00003 | mg/L | 0.000388 | >999.9% |
| Cr 267.716† | -3.2 | -0.00062 | mg/L | 0.001126 | -0.00062 | mg/L | 0.001126 | 181.14% |
| Cu 324.752† | 554.6 | 0.00199 | mg/L | 0.000138 | 0.00199 | mg/L | 0.000138 | 6.96% |
| Fe 273.955† | 0.8 | 0.00069 | mg/L | 0.001419 | 0.00069 | mg/L | 0.001419 | 204.23% |
| K 766.490† | 17.4 | 0.01194 | mg/L | 0.010964 | 0.01194 | mg/L | 0.010964 | 91.79% |
| Mg 279.077† | -6.8 | -0.00729 | mg/L | 0.001874 | -0.00729 | mg/L | 0.001874 | 25.70% |
| Mn 257.610† | 3.1 | 0.00010 | mg/L | 0.000150 | 0.00010 | mg/L | 0.000150 | 154.15% |
| Mo 202.031† | -1.7 | -0.00010 | mg/L | 0.000139 | -0.00010 | mg/L | 0.000139 | 138.39% |
| Na 589.592† | 97.9 | 0.00821 | mg/L | 0.001834 | 0.00821 | mg/L | 0.001834 | 22.34% |
| Na 330.237† | -3.8 | -0.1320 | mg/L | 0.04319 | -0.1320 | mg/L | 0.04319 | 32.72% |
| Ni 231.604† | 3.9 | 0.00231 | mg/L | 0.002109 | 0.00231 | mg/L | 0.002109 | 91.14% |
| Pb 220.353† | 0.7 | 0.00009 | mg/L | 0.000376 | 0.00009 | mg/L | 0.000376 | 406.01% |
| Sb 206.836† | 12.1 | 0.00451 | mg/L | 0.000679 | 0.00451 | mg/L | 0.000679 | 15.07% |
| Se 196.026† | 4.4 | 0.00347 | mg/L | 0.002407 | 0.00347 | mg/L | 0.002407 | 69.45% |
| Si 288.158† | 10.1 | 0.00685 | mg/L | 0.002824 | 0.00685 | mg/L | 0.002824 | 41.23% |
| Sn 189.927† | 2.9 | 0.00078 | mg/L | 0.000349 | 0.00078 | mg/L | 0.000349 | 44.85% |
| Sr 421.552† | 48.3 | 0.00007 | mg/L | 0.000076 | 0.00007 | mg/L | 0.000076 | 105.47% |
| Ti 334.903† | -12.0 | -0.00055 | mg/L | 0.000700 | -0.00055 | mg/L | 0.000700 | 128.01% |
| Tl 190.801† | 4.1 | 0.00226 | mg/L | 0.001091 | 0.00226 | mg/L | 0.001091 | 48.25% |
| V 292.402† | -0.1 | 0.00000 | mg/L | 0.000131 | 0.00000 | mg/L | 0.000131 | >999.9% |
| Zn 206.200† | -0.6 | -0.00091 | mg/L | 0.001005 | -0.00091 | mg/L | 0.001005 | 110.54% |

end play

**General Chemistry Raw Data
Analyst Notes and Raw Data**

ARI Job ID: RG51

8-2-10

TOTAL SOLIDS/VOLATILE SOLIDS (TS / TVS) BENCHSHEET

SOLIDS (dry at 104 (12-24 hr) then combust at 550 (30 min)) DATE: 7/30/2010 ANALYST: KE / CDE / RR 19:10
Instrumentation Drying Ovens: 12 Muffle Furnace: N/A Analytical Balance: 1123230597

Batch drying time
 record times as mm/dd/yy hh:mm
 7/30/2010 19:10 KE
 7/31/2010 14:30 RR
 elapsed hrs = 19.3

| SAMPLE ID | DISH # | SAMPLE (grams) | TARE WT (grams) | DRY WT 104C (grams) | | dry wt (g) | TS (%) | ASH WT 550C (grams) | | Ash Wt (g) | TVS (mg/kg) (%) |
|-------------|--------|----------------|-----------------|---------------------|--------|------------|--------|---------------------|---|------------|-----------------|
| | | | | CV-02 | CV-02 | | | 1 | 2 | | |
| Blank | | | 1.1129 | 1.1129 | 1.1129 | 0.00 | | | | | |
| RG51 D3 | | 6.1385 | 1.1033 | 5.8990 | 4.80 | 95.2% | | | | | |
| RG51 E1 | | 6.2249 | 1.1038 | 5.9965 | 4.89 | 95.5% | | | | | |
| RG51 F6 | | 6.2874 | 1.1480 | 5.9022 | 4.75 | 92.5% | | | | | |
| RG51 F6 dup | | 6.2747 | 1.0995 | 5.8516 | 4.75 | 91.8% | | | | | |

TS (%) calculated as:
 Final dry wt (g) = (Dry Wt - Tare Wt)
 TS = (Final Dry Wt) / (grams Sample-Tare) (A)
 TVS (mg/kg dry wt) calculated as:
 Final ash wt (g) = (min ash wt - tare wt)
 TVS (mg/kg) = [(Dry wt-Ash wt) / (dry weight)] * 1,000,000
 if ash wt > dry wt, "Chk for Err"
 if dry wt-ash wt < 0.001 g, "< (1/dry wt) * 1,000,000"

| SAMPLE ID | DISH # | SAMPLE (grams) | TARE WT (grams) | DRY WT 104C (grams) | | dry wt (g) | TS (%) | ASH WT 550C (grams) | | Ash Wt (g) | TVS (mg/kg) (%) |
|-------------|--------|----------------|-----------------|---------------------|-------|------------|--------|---------------------|---|------------|-----------------|
| | | | | CV-02 | CV-02 | | | 1 | 2 | | |
| RG51 F6 trp | | 6.1652 | 1.1451 | 5.7450 | 4.60 | 91.6% | | | | | |
| RG54 E6 | | 6.3388 | 1.1551 | 5.7556 | 4.60 | 88.7% | | | | | |
| RG54 F6 | | 6.9543 | 1.0916 | 6.3131 | 5.22 | 89.1% | | | | | |
| RG54 K6 | | 6.4966 | 1.1538 | 5.3935 | 4.24 | 79.4% | | | | | |
| RG58 E8 | | 6.1694 | 1.1331 | 5.4653 | 4.33 | 86.0% | | | | | |
| RG58 F8 | | 6.2314 | 1.0902 | 5.3668 | 4.28 | 83.2% | | | | | |
| RG58 K8 | | 6.7517 | 1.1191 | 6.1708 | 5.05 | 89.7% | | | | | |
| RG58 L8 | | 6.2854 | 1.1000 | 5.6066 | 4.51 | 86.9% | | | | | |
| RG58 R8 | | 6.4034 | 1.1513 | 5.9219 | 4.77 | 90.8% | | | | | |
| RG58 S8 | | 6.8870 | 1.1213 | 6.3245 | 5.20 | 90.2% | | | | | |
| RG60 E8 | | 6.4681 | 1.1254 | 6.0312 | 4.91 | 91.8% | | | | | |
| RG60 F8 | | 6.7541 | 1.1268 | 6.2698 | 5.14 | 91.4% | | | | | |
| RG43 A1 | | 5.5283 | 1.1292 | 4.8556 | 3.73 | 84.7% | | | | | |
| RG43 A1 dup | | 5.1486 | 1.1108 | 4.2117 | 3.10 | 76.8% | | | | | |

TOTAL SOLIDS/VOLATILE SOLIDS (TS / TVS) BENCHSHEET

SOLIDS (dry at 104 (12-24 hr), then combust at 550 (30 min)) **DATE:** 7/30/2010
Instrumentation **Drying Ovens:** 12 **Muffle Furnace:** N/A **ANALYST:** KE / CDE / RR 19:10
Analytical Balance: 1123230597

| Batch drying time | | TS (%) calculated as: | | | | TVS (mg/kg dry wt) calculated as: | | | |
|----------------------------------|--------|---------------------------------------|------------------|---------------------|------------|---|---------------------|------------|-----------------|
| record times as mm/dd/yyyy hh:mm | | Final dry wt (g) = (Dry Wt - Tare Wt) | | | | Final ash wt (g) = (min ash wt - tare wt) | | | |
| 7/30/2010 19:10 | KE | CV-02 | CV-02 | CV-02 | | | | | |
| 7/31/2010 14:30 | RR | 7/30/10 17:46 KE | 7/30/10 17:10 KE | 7/31/10 14:30 RR | | | | | |
| elapsed hrs = 19.3 | | 10.0000 | 10.0000 | 10.0000 | | | | | |
| Cal Wt (g) | | Cal/OK! | Cal/OK! | Cal/OK! | | | | | |
| | | record weights to 4 places | | | | | | | |
| SAMPLE ID | DISH # | SAMPLE (grams) | TARE WT (grams) | DRY WT 104C (grams) | dry Wt (g) | TS (%) | ASH WT 550C (grams) | Ash Wt (g) | TVS (mg/kg) (%) |
| RG43 A1 trp | | 5.5697 | 1.1196 | 4.7123 | 3.59 | 80.7% | 1 | 2 | |
| | | | | | | | | | |

| | | | | | | | | | |
|---------|--------|--------|--------|--|------|-------|--|--|----|
| RG43 B1 | 6.5779 | 1.1286 | 5.4363 | | | 4.90% | | | NA |
| | | | | | 4.31 | 79.1% | | | |



Analytical Resources, Incorporated
Analytical Chemists and Consultants

TOTAL / VOLATILE SOLIDS (TS/TVS) BENCHSHEET

| Analyst: <u>CDZ</u> Date: <u>7-30-70</u> Oven ID: <u>012</u> Balance ID: <u>1123230597</u> | | Time in Oven: <u>17:10</u> Time Out of Oven: <u>14:15</u> Elapsed Time (> 12 Hrs): <u>(A)</u> | |
|--|--------|---|-------|
| Sample ID | Dish # | Cal Weight ID | CV-02 |
| BLANK | 1 | CV-02 | CV-02 |
| ASST | 2 | CV-02 | CV-02 |
| ES | 3 | CV-02 | CV-02 |
| FL | 4 | CV-02 | CV-02 |
| MPF6 | 5 | CV-02 | CV-02 |
| MPF6 | 6 | CV-02 | CV-02 |
| RGSS4 | 7 | CV-02 | CV-02 |
| FL | 8 | CV-02 | CV-02 |
| K6 | 9 | CV-02 | CV-02 |
| RGSS8 | 10 | CV-02 | CV-02 |
| FL | 11 | CV-02 | CV-02 |
| K8 | 12 | CV-02 | CV-02 |
| L8 | 13 | CV-02 | CV-02 |
| R8 | 14 | CV-02 | CV-02 |
| S6 | 15 | CV-02 | CV-02 |
| RG60 | 16 | CV-02 | CV-02 |
| FL | 17 | CV-02 | CV-02 |
| RG43 | 18 | CV-02 | CV-02 |
| MPA1 | 19 | CV-02 | CV-02 |
| MPA1 | 20 | CV-02 | CV-02 |
| B1 | 21 | CV-02 | CV-02 |

TS (mg/kg dry weight) calculated as:
Final Dry Weight (g) = (Dry Weight - Tare Weight)
TS = (Final Dry Weight) / (Grams Sample - Tare Weight)

TVS (mg/kg dry weight) calculated as:
Final Ash Weight (g) = (Minimum Ash Weight - Tare Weight)
TVS (mg/kg) = [(Dry Weight - Ash Weight) / (Dry Weight) * 1,000,000
If Ash Weight > Dry Weight then "Check for Error"
If Dry Weight - Ash Weight < 0.001 < (1/Dry Weight) * 1,000,000

Revision 002
12/28/09

Page 00449

6053F

② 6.3388
③ ~~6.3388~~ 6.9543
④ 6.4966
⑤ 6.1150

7-30-70 (A)

7051 : 81100

W
8-4-10

| TOC Solids Prep Log | | | | | | DATE: | 7/30/2010 |
|---|--------|------------------|--------------------------|---------|-------------|---|--|
| acid purging to remove IC and drying at 70°C for TOC analysis General notes regarding prep method and samples (identify the acid used) | | | | | | ANALYST: | KE 19:30 (A) |
| | | | | | | <i>make no entry to shaded cells, they are calculated</i> | |
| Sample ID | | IC Test + / - | Gravimetric Data (grams) | | | % Solids | Sample description & notes (homogeneity and exclusions) |
| ARI # | Client | | Tare Wt. | Wet wt. | 70°C dry wt | | |
| Blank | | | 13.1088 | | 13.1088 | 0 mg | |
| RG51 D3 | | - | 13.2258 | 18.0648 | 17.9648 | 97.93% | |
| RG51 E3 | | - | 13.1478 | 18.5727 | 18.4813 | 98.32% | |
| RG51 F3 | | - | 13.2387 | 18.4485 | 18.1578 | 94.42% | |
| RG51 F3 DUP | | - | 13.2621 | 18.6455 | 18.3746 | 94.97% | |
| RG51 F3 TRIP | | - | 13.1517 | 18.8582 | 18.5545 | 94.68% | |
| RG54 E6 | | - | 12.8131 | 18.0133 | 17.7049 | 94.07% | |
| RG54 F6 | | - | 13.0790 | 18.3047 | 17.8947 | 92.15% | |
| RG54 K6 | | - | 13.2288 | 18.2421 | 17.2378 | 79.97% | |
| RG58 E8 | | - | 13.1709 | 18.5807 | 17.9854 | 89.00% | |
| RG58 F8 | | - | 13.1603 | 18.9466 | 18.0800 | 85.02% | |
| RG58 K8 | | - | 13.2105 | 18.4043 | 17.9875 | 91.98% | |
| RG58 L8 | | - | 13.0982 | 18.7507 | 18.1468 | 89.32% | |
| RG58 R8 | | - | 12.9965 | 18.9213 | 18.4918 | 92.75% | |
| RG58 S8 | | - | 13.0830 | 18.3251 | 17.7781 | 89.57% | |
| RG60 E8 | | - | 13.1423 | 18.5458 | 18.2656 | 94.81% | |
| RG60 F8 | | - | 13.1331 | 18.1632 | 17.8433 | 93.64% | |
| RG43 B1 | | +++ | 13.1604 | 18.7234 | 17.8416 | 84.15% | |



TOC Solids Preparation Log

Acid purge to remove IC and drying 70 °C for TOC analysis
Add general notes regarding samples and preparation and identify the acid used

Analyst 7-30-10 (W) / CAC Date 7-30-10 19:32(A)

| Sample Identification | | IC Test | Gravimetric Data | | | % Solids | Sample description & notes |
|-----------------------|-----------|---------|------------------|---------|---------|----------|----------------------------|
| ARI # | Client ID | | Tare | Wet | 70 °C | | |
| Blank | | | 13.1088 | Ø | 13.1088 | | |
| RG51 D3 | | - | 13.2288 | 18.0648 | 17.9648 | | Sand & Rocks |
| E1 | | - | 13.1478 | 18.5727 | 18.4813 | | |
| F6 | | - | 13.2387 | 18.4485 | 18.1578 | | |
| OPF6 | | - | 13.2621 | 18.6455 | 18.3746 | | |
| PPF6 | | - | 13.1517 | 18.8582 | 18.5545 | | |
| RG54 E6 | | - | 12.8131 | 18.0133 | 17.9854 | 17.7049 | |
| F6 | | - | 13.0790 | 18.3047 | 17.8947 | | |
| K6 | | - | 13.2288 | 18.2421 | 17.2378 | | |
| RG58 E8 | | - | 13.1709 | 18.5807 | 17.9854 | | |
| F8 | | - | 13.1603 | 18.9466 | 18.0800 | | |
| K8 | | - | 13.2105 | 18.4043 | 17.9875 | | Mud Sand & Rock |
| L8 | | - | 13.0982 | 18.7507 | 18.1468 | | |
| R8 | | - | 12.9965 | 18.9213 | 18.4918 | | |
| S8 | | - | 13.0830 | 18.3251 | 17.781 | | |
| RG60 E8 | | - | 13.1423 | 18.5458 | 18.2650 | | Remain unAged (no Acid) |
| F8 | | - | 13.1331 | 18.1632 | 17.8433 | | |
| RG43 A1 | | +++ | 13.2487 | 18.3062 | | | |
| OP A1 | | +++ | 13.1282 | 18.8937 | | | |
| PP A1 | | +++ | 13.1972 | 18.678 | | | |
| Ø B1 | | +++ | 13.1604 | 18.7234 | | | |

7-30-10
(W)

RG43
Ø B1 +++ - 131604-187234 - 17.8416 8-3-10 (W)

W
8-9-10

TOC, Solids Data Analysis DATE: 8/9/2010
 Instrument: Apollo 2 ANALYST: CR 10:05
 Mode: NPOC Inlet: Boat
 Spike Std = 2,500 ppm C

Calibration Data
 Cal Curve ID: CAL 072210 Conc: 5,000 ppm
 Calibration Curve Standard: ARI # 00103 - 1 Curve Date: 07/22/10
 CalFact: 2.599E+05 intercept: -120606 r2: 0.99983
 Curve Range (µgC): 8 to 100

Verification Standard Source: ERA# 0513 - 10 - 06 Conc: 5,000 ppm
 dilution: 10 mL to 50 1,000 ppm

Standard Reference Material Source: NIST 8704 Conc: 33,510 ppm

Silica Blanks

| Replicate determinations | | | | | Mean | RSD | condition |
|--------------------------|--|--|--|--|------|-----|-----------|
| | | | | | | | |

Sample Data
 "C corr" (with dilution) = ("C obs" - (Mean silica Blank * %Silica)) * Dilution Factor

| Sample ID | Dilution Data | | | | Spike (µL Std) | Combustion Data | | | comments |
|---|-----------------|----------------|------------|-----------------|----------------|-----------------|---------------|----------------|-----------|
| | Sample wt. (mg) | Final wt. (mg) | Silica (%) | Dilution Factor | | Burn wt. (mg) | C obs (ppm C) | C corr (ppm C) | |
| ICV | | | | 1.00 | | 40.0 | 949 | 949 | 94.90% |
| Blank | | | | 1.00 | | 40.0 | 29.73 | 30 | Blank OK |
| NIST 8704 | | | | 1.00 | | 2.5 | 33212 | 33,212 | 99.11% |
| RG51 D3 | | | | 1.00 | | 3.2 | 4018 | 4,018 | Range OK! |
| RG51 E1 | | | | 1.00 | | 3.6 | 3660 | 3,660 | Range OK! |
| RG51 F6 | | | | 1.00 | | 3.6 | 2746 | 2,746 | Range OK! |
| RG51 F6 dup | | | | 1.00 | | 3.7 | 3048 | 3,048 | RPD=10.4% |
| RG51 F6 trp | | | | 1.00 | | 3.6 | 3325 | 3,325 | RSD=9.5% |
| RG51 F6 ms | | | | 1.00 | 10 | 3.0 | 10415 | 10,415 | Range OK! |
| Spike = 0.025 mg C to 3.0 mg samp = 8,333 ppm 92% | | | | | | | | | |
| CCV | | | | 1.00 | | 40.0 | 892 | 892 | 89.20% |
| CCV | | | | 1.00 | | 40.0 | 919 | 919 | 91.90% |
| Blank | | | | 1.00 | | 40.0 | 47.47 | 47 | Blank OK |
| NIST 8704 | | | | 1.00 | | 2.1 | 33696 | 33,696 | 100.56% |



du
8-9-10
10F1

**TOC Solids Sample Run Log
Apollo 9000**

| | | |
|---|-----------------------|-----------------------------|
| Set-Up Parameters MODE: <i>NPDC BOM</i> | | INLET: <i>BOM SAMPLE</i> |
| Standards: | Source | Conc (ppm) |
| Calibration: | <i>API 00103-01</i> | <i>5000</i> |
| Verification: | <i>EPA 1513-10-06</i> | <i>5000 TO 1000 FOR CVS</i> |
| SRM: | <i>NBS 8704</i> | <i>33570</i> |

Sample Sequence:

| Sample ID | Dilution Data (mg) | | Burn Wt mg | Matrix Spike Data | | Comments |
|---------------------|--------------------|--------------|---------------|-------------------|-----------|----------|
| | Sample | + Silica Gel | | mg/L | µL added | |
| <i>ICV</i> | | | <i>40</i> | | | |
| <i>ICB</i> | | | <i>40</i> | | | |
| <i>NBS 8704</i> | | | <i>2.5</i> | | | |
| <i>RG51 D3</i> | | | <i>3.2</i> | | | |
| <i>E1</i> | | | <i>3.6</i> | | | |
| <i>F6</i> | | | <i>3.6</i> | | | |
| <i>F6000</i> | | | <i>3.7</i> | | | |
| <i>F6000</i> | | | <i>3.6</i> | | | |
| <i>F6MS</i> | | | <i>3.0</i> | <i>2500</i> | <i>10</i> | |
| <i>CEV</i> | | | <i>40</i> | | | |
| <i>CEV</i> | | | <i>40</i> | | | |
| <i>BWL</i> | | | <i>40</i> | | | |
| <i>NBS 8704</i> | | | <i>2.1</i> | | | |
| <i>du</i> 8-9-10 | | | | | | |


```

=====
Sample ID:  CVS BOAT 1000          Mode:      TOC
Method:      Boat Sampler          Filename:   08091005
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:09
Operator ID: CARLOS                Sample Type: Cal. Verification
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|----------|---------|----------|--------------------|-----------------|------------------|
| 1 | 949.3958 | 37.9758 | 9734089 | 19.200 | 20.193 | 130 |

```

=====
Sample ID:  ICB BOAT              Mode:      TOC
Method:      Boat Sampler          Filename:   08091013
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:15
Operator ID: CARLOS                Sample Type: Cal. Verification
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|---------|--------|----------|--------------------|-----------------|------------------|
| 1 | 29.7277 | 1.1891 | 65605 | 18.904 | 19.896 | 51 |

```

=====
Sample ID:  NBS 8704              Mode:      TOC
Method:      Boat Sampler          Filename:   08091020
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:25
Operator ID: CARLOS                Sample Type: Cal. Verification
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|------------|---------|----------|--------------------|-----------------|------------------|
| 1 | 33211.7500 | 83.0294 | 21575300 | 18.752 | 19.751 | 242 |

```

=====
Sample ID:  RG51 D3               Mode:      TOC
Method:      Boat Sampler          Filename:   08091029
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:32
Operator ID: CARLOS                Sample Type: Sample
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|-----------|---------|----------|--------------------|-----------------|------------------|
| 1 | 4018.1853 | 12.8582 | 3379459 | 18.636 | 19.636 | 113 |

```

=====
Sample ID:  RG51 E1               Mode:      TOC
Method:      Boat Sampler          Filename:   08091037
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:40
Operator ID: CARLOS                Sample Type: Sample
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|-----------|---------|----------|--------------------|-----------------|------------------|
| 1 | 3659.5400 | 13.1743 | 3462551 | 18.662 | 19.658 | 123 |

```

=====
Sample ID:  RG51 F6               Mode:      TOC
Method:      Boat Sampler          Filename:   08091042
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:45
Operator ID: CARLOS                Sample Type: Sample
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|-----------|--------|----------|--------------------|-----------------|------------------|
| 1 | 2745.8174 | 9.8849 | 2598013 | 18.816 | 19.811 | 109 |

```

=====
Sample ID:  RG51 F6 DUP           Mode:      TOC
Method:      Boat Sampler          Filename:   08091048
Cal. Curve:  BOAT CAL 07232010    Timestamp: 2010/08/09 10:52
Operator ID: CARLOS                Sample Type: Sample
    
```

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|-----------|---------|----------|--------------------|-----------------|------------------|
| 1 | 3048.1897 | 11.2783 | 2964224 | 18.882 | 19.881 | 116 |

Sample ID: RG51 F6 TRP Mode: TOC
Method: Boat Sampler Filename: 08091057
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 11:00
Operator ID: CARLOS Sample Type: Sample

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|-----------|---------|----------|-----------------------|--------------------|---------------------|
| 1 | 3325.4363 | 11.9716 | 3146432 | 19.141 | 20.140 | 110 |

Sample ID: RG51 F6 MS Mode: TOC
Method: Boat Sampler Filename: 08091128
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 11:31
Operator ID: CARLOS Sample Type: Sample

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|------------|---------|----------|-----------------------|--------------------|---------------------|
| 1 | 10415.2441 | 31.2457 | 8212171 | 19.152 | 20.144 | 125 |

Sample ID: CVS BOAT 1000 Mode: TOC
Method: Boat Sampler Filename: 08091357
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 14:01
Operator ID: CARLOS Sample Type: Cal. Verification

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|----------|---------|----------|-----------------------|--------------------|---------------------|
| 1 | 892.1044 | 35.6842 | 9131783 | 18.260 | 19.260 | 146 |

Last Message: Out of Calibration

Sample ID: CVS BOAT 1000 Mode: TOC
Method: Boat Sampler Filename: 08091405
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 14:08
Operator ID: CARLOS Sample Type: Cal. Verification

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|----------|---------|----------|-----------------------|--------------------|---------------------|
| 1 | 918.8392 | 36.7536 | 9412846 | 18.523 | 19.522 | 130 |

Sample ID: ICB BOAT Mode: TOC
Method: Boat Sampler Filename: 08091412
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 14:15
Operator ID: CARLOS Sample Type: Cal. Verification

| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|---------|--------|----------|-----------------------|--------------------|---------------------|
| 1 | 47.4670 | 1.8987 | 252099 | 18.436 | 19.432 | 69 |

Sample ID: NBS 8704 Mode: TOC
Method: Boat Sampler Filename: 08091443
Cal. Curve: BOAT CAL 07232010 Timestamp: 2010/08/09 14:48
Operator ID: CARLOS Sample Type: Cal. Verification


| Rep # | ppm C | ug C | Raw Data | Beginning Baseline | Ending Baseline | Integration Time |
|-------|------------|---------|----------|-----------------------|--------------------|---------------------|
| 1 | 33696.0547 | 70.7617 | 18351048 | 18.902 | 19.900 | 225 |

Table of Contents: ARI Job RG58

Client: Floyd/Snider

Project: POS-LLA Lora Lake RI

| | Page From: | Page To: |
|---|------------|------------|
| Inventory Sheet | | |
| Cover Letter | <u>1</u> | <u>1</u> |
| Chain of Custody Documentation | <u>2</u> | <u>7</u> |
| Case Narrative, Data Qualifiers, Control Limits | <u>8</u> | <u>25</u> |
| Volatile Analysis | | |
| Report and Summary QC Forms | <u>26</u> | <u>69</u> |
| Semivolatile PAH Analysis | | |
| Report and Summary QC Forms | <u>70</u> | <u>113</u> |
| PCP/Chlorophenols Analysis | | |
| Report and Summary QC Forms | <u>114</u> | <u>162</u> |
| TPHD Analysis | | |
| Report and Summary QC Forms | <u>163</u> | <u>192</u> |
| TPHG/BETX Analysis | | |
| Report and Summary QC Forms | <u>193</u> | <u>250</u> |
| Metals Analysis | | |
| Report and Summary QC Forms | <u>251</u> | <u>291</u> |
| General Chemistry Analysis | | |
| Report and Summary QC Forms | <u>292</u> | <u>303</u> |
| Total Solids | | |
| Report and Summary QC Forms | <u>304</u> | <u>312</u> |
| Subcontracted Analysis | | |
| Report and Summary QC Forms | <u>NA</u> | <u>NA</u> |
| Volatile Raw Data | | |
| Preparation Log | <u>313</u> | <u>315</u> |
| Initial Calibration | <u>316</u> | <u>409</u> |
| Run Logs, Continuing Calibrations, and Raw Data | <u>410</u> | <u>562</u> |


Signature


²⁶
August-13-2010
Date

Table of Contents: ARI Job RG58

Client: Floyd/Snyder

Project: POS-LLA Lora Lake RI

| | Page From: | Page To: |
|---|-------------|-------------|
| Semivolatile PAH Raw Data | | |
| Extractions Bench Sheets and Notes | <u>563</u> | <u>565</u> |
| Initial Calibration | <u>566</u> | <u>679</u> |
| Run Logs, Continuing Calibrations, and Raw Data | <u>680</u> | <u>855</u> |
| PCP/Chlorophenols Raw Data | | |
| Extractions Bench Sheets and Notes | <u>856</u> | <u>858</u> |
| Initial Calibration | <u>859</u> | <u>914</u> |
| Run Logs, Continuing Calibrations, and Raw Data | <u>915</u> | <u>1030</u> |
| TPHD Raw Data | | |
| Extractions Bench Sheets and Notes | <u>1031</u> | <u>1035</u> |
| Initial Calibration | <u>1036</u> | <u>1109</u> |
| Run Logs, Continuing Calibrations, and Raw Data | <u>1110</u> | <u>1246</u> |
| TPHG/BETX Raw Data | | |
| Preparation Log | <u>1247</u> | <u>1249</u> |
| Initial Calibration | <u>1250</u> | <u>1392</u> |
| Run Logs, Continuing Calibrations, and Raw Data | <u>1393</u> | <u>1489</u> |
| Metals Raw Data | | |
| Preparation Bench Sheets and Notes | <u>1490</u> | <u>1492</u> |
| Run Logs, Calibrations, and Raw Data | <u>1493</u> | <u>1612</u> |
| General Chemistry Raw Data | | |
| Analyst Notes and Raw Data | <u>1613</u> | <u>1626</u> |



 Signature

26
August-13-2010
 Date



Analytical Resources, Incorporated
Analytical Chemists and Consultants

August 26, 2010

Jessi Massingale
Floyd-Snyder Inc.
601 Union Street, Suite 600
Seattle, WA 98101-2341

RE: Client Project: Lora Lake RI
ARI Job No: RG58

Dear Ms. Massingale:

Please find enclosed the original Chain-of-Custody (COC) record, sample receipt documentation, and the final data package for samples from the project referenced above.

Sample receipt and detail of these analyses are discussed in the Case Narrative.

An electronic copy of this package will remain on file with ARI. Should you have any questions or problems, please feel free to contact me at your convenience.

Sincerely,

ANALYTICAL RESOURCES, INC.

A handwritten signature in black ink, appearing to read "Susan D. Dunning".

Susan D. Dunning
Director, Client Services
sue@arilabs.com
206-695-6207

Enclosures

cc: eFile RG58

SD/sdrd

Chain of Custody Documentation

ARI Job ID: RG58

Chain of Custody Record & Laboratory Analysis Request

ARI Assigned Number: _____ of _____
 Turn-around Requested: _____
 Date: 7/29/10
 Ice Present? YES
 No. of Coolers: _____
 Cooler Temps: 3.6 °C

Analytical Resources, Incorporated
 Analytical Chemists and Consultants
 4611 South 134th Place, Suite 100
 Tukwila, WA 98168
 206-695-6200 206-695-6201 (fax)



ARI Client Company: Floyd Snider Phone: 206-292-2578
 Client Contact: M.M. Callaghan / J. Marrison
 Client Project Name: Love Lake RI
 Client Project #: POS-LVA Samplers: MM

| Sample ID | Date | Time | Matrix | No. Containers | Analysis Requested | | | | | | Notes/Comments | | | |
|--|---------|-------|--------|----------------|---|------------|----------|------------------------|----------------|---|----------------|------------|---------------|----------------|
| | | | | | PAHs (8270) | PCP (8041) | NMTPH-DX | NMTPH-6X + BETX (8021) | As + Pb (6010) | LOCS (8200C) | | TOL (Pbms) | Dioxin (1413) | Azoline (Diox) |
| PSB22-0-05-072910 | 7/29/10 | 09:05 | S | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-1-5-2-072910 | | 09:10 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-2-4-072910 | | 09:07 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-4-6-072910 | | 08:56 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-17-19-072910 | | 08:44 | | 8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-19-20-072910 | | 08:37 | ↓ | 8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| PSB22-TB | | 15:25 | W | 2 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | |
| Comments/Special Instructions <u>See project list for notes</u> | | | | | Relinquished by: (Signature) <u>[Signature]</u> Printed Name: <u>Susan Domingo</u> Company: <u>ARI</u> | | | | | Received by: (Signature) <u>[Signature]</u> Printed Name: _____ Company: _____ | | | | |
| Date & Time: <u>7/29/10 18:25</u> | | | | | Date & Time: <u>7/29/10 18:25</u> | | | | | Date & Time: _____ | | | | |

Limits of Liability: ARI will perform all requested services in accordance with appropriate methodology following ARI Standard Operating Procedures and the ARI Quality Assurance Program. This program meets standards for the industry. The total liability of ARI, its officers, agents, employees, or successors, arising out of or in connection with the requested services, shall not exceed the invoiced amount for said services. The acceptance by the client of a proposal for services by ARI release ARI from any liability in excess thereof, not withstanding any provision to the contrary in any contract, purchase order or co-signed agreement between ARI and the Client.

Sample Retention Policy: All samples submitted to ARI will be appropriately discarded no sooner than 90 days after receipt or 60 days after submission of hardcopy data, whichever is longer, unless alternate retention schedules have been established by work-order or contract.

Chain of Custody Record & Laboratory Analysis Request

ARI Assigned Number: Standard Turn-around Requested: Standard

ARI Client Company: Floyd Sinden Phone: 206-292-2078

Client Contact: M. McCalllogh (J. Massingale)

Client Project Name: Lum Lake RI

Client Project #: Pos-LUA Samplers: MM

Analytical Resources, Incorporated
Analytical Chemists and Consultants
4611 South 134th Place, Suite 100
Tukwila, WA 98168
206-695-6200 206-695-6201 (fax)



Page: 1 of 1

Date: 7/29/10 Ice Present? YES

No. of Coolers: 7.3° Cooler Temps:

| Sample ID | Date | Time | Matrix | No. Containers | Analysis Requested | | | | | | Notes/Comments | | | |
|-------------------------------|-------------------------------|-------|--------|----------------|--|------------|--|----------------------|--|------------------|-----------------------------------|------------|-----------------------------------|---------------------|
| | | | | | 7AH5 (5270) | PCP (5041) | MM-TPH-DX | NNTPH-GX + BTR (522) | As + Pb (6010) | VOCs - SC (8260) | | TOC (Plus) | Dioxin (MS) | ARCHIVE (for DOKUM) |
| PSB23-0-0.5-072910 | 7/29/10 | 12:10 | S | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| PSB23-1.5-2-072910 | | 12:05 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| PSB23-2-A-072910 | | 12:15 | | 1415 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | MM MS/MS |
| PSB23-4-6-072910 | | 12:20 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| PSB23-14-16.5-072910 | | 12:30 | | 8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| PSB23-16.5-19-072910 | | 12:25 | | 8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| PSB23-TB | | 17:15 | W | 2 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | |
| Comments/Special Instructions | see project specific voc list | | | | Relinquished by: <u>[Signature]</u> (Signature) Printed Name: <u>Susan D Downard</u> Company: <u>ARI</u> | | Relinquished by: <u>[Signature]</u> (Signature) Printed Name: <u>Susan D Downard</u> Company: <u>ARI</u> | | Received by: <u>[Signature]</u> (Signature) Printed Name: <u>Susan D Downard</u> Company: <u>ARI</u> | | Date & Time: <u>7/29/10 18:25</u> | | Date & Time: <u>07/29/10 1825</u> | |

Limits of Liability: ARI will perform all requested services in accordance with appropriate methodology following ARI Standard Operating Procedures and the ARI Quality Assurance Program. This program meets standards for the industry. The total liability of ARI, its officers, agents, employees, or successors, arising out of or in connection with the requested services, shall not exceed the invoiced amount for said services. The acceptance by the client of a proposal for services by ARI release ARI from any liability in excess thereof, not withstanding any provision to the contrary in any contract, purchase order or co-signed agreement between ARI and the Client.

Sample Retention Policy: All samples submitted to ARI will be appropriately discarded no sooner than 90 days after receipt or 60 days after submission of hardcopy data, whichever is longer, unless alternate retention schedules have been established by work-order or contract.

Chain of Custody Record & Laboratory Analysis Request

ARI Assigned Number: Standard Turn-around Requested: _____ of 1 Page: 1

ARI Client Company: Floyd Snider Phone: 206-292-2078 Date: 7/29/10 Ice Present? YES

Client Contact: M. McCullough - J. Massingale No. of Coolers: _____ Cooler Temps: 0.0

Client Project Name: Low Lake RI Samplers: MM

Client Project #: POS-LUA

Analytical Resources, Incorporated
Analytical Chemists and Consultants
4611 South 134th Place, Suite 100
Tukwila, WA 98168
206-695-6200 206-695-6201 (fax)



| Sample ID | Date | Time | Matrix | No. Containers | Analysis Requested | | | | | | Notes/Comments | | | | | | | |
|---|---|-------|--------|-----------------------------------|---|-----------|----------|-----------------------------------|---|---------------------|----------------|-----------------------------------|---|------------------|--|--|--|--|
| | | | | | PAHs (82p) | PCP (804) | NMTPH-IX | NMTPH-IX + BTEX (821) | As + Pb (60p) | VOCs - Sulf (82600) | | TRC (Pikab) | Dioxin (1615) | Azthine (Dioxin) | | | | |
| PSB-24-0-05-072910 | 7/29/10 | 10:33 | S | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-15-2-072910 | | 10:58 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-2-A-072910 | | 10:43 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-2-A-072910-D | | 10:45 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-4-0-072910 | | 11:01 | | 6 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-14-16-072910 | | 11:00 | | #8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-16-17-072910 | | 11:15 | ↓ | 8 | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | | | | | | | | |
| PSB-24-TB | | 17:35 | W | 2 | | | | | | | | | | | | | | |
| Comments/Special Instructions <u>See project list for VOCs</u> | Relinquished by: (Signature) <u>[Signature]</u> Printed Name: <u>Sean D. Dunne</u> Company: <u>ARI</u> | | | | Received by: (Signature) <u>[Signature]</u> Printed Name: <u>Sean D. Dunne</u> Company: <u>ARI</u> | | | | Relinquished by: (Signature) <u>[Signature]</u> Printed Name: <u>Sean D. Dunne</u> Company: <u>ARI</u> | | | | Received by: (Signature) <u>[Signature]</u> Printed Name: <u>Sean D. Dunne</u> Company: <u>ARI</u> | | | | | |
| Date & Time: <u>7/29/10 18:26</u> | | | | Date & Time: <u>7/29/10 18:26</u> | | | | Date & Time: <u>7/29/10 18:26</u> | | | | Date & Time: <u>7/29/10 18:26</u> | | | | | | |

Limits of Liability: ARI will perform all requested services in accordance with appropriate methodology following ARI Standard Operating Procedures and the ARI Quality Assurance Program. This program meets standards for the industry. The total liability of ARI, its officers, agents, employees, or successors, arising out of or in connection with the requested services, shall not exceed the invoiced amount for said services. The acceptance by the client of a proposal for services by ARI release ARI from any liability in excess thereof, not withstanding any provision to the contrary in any contract, purchase order or co-signed agreement between ARI and the Client.

Sample Retention Policy: All samples submitted to ARI will be appropriately discarded no sooner than 90 days after receipt or 60 days after submission of hardcopy data, whichever is longer, unless alternate retention schedules have been established by work-order or contract.

2658:00005



Cooler Receipt Form

ARI Client: Floyd Snider
 COC No(s): _____
 Assigned ARI Job No: RG58 ^{NA}

Project Name: Lora Lake RI
 Delivered by: Fed-Ex UPS Courier Hand Delivered Other
 Tracking No: _____ ^{NA}

Preliminary Examination Phase:

Were intact, properly signed and dated custody seals attached to the outside of to cooler? YES NO
 Were custody papers included with the cooler? YES NO
 Were custody papers properly filled out (ink, signed, etc.) YES NO
 Temperature of Cooler(s) (°C) (recommended 2.0-6.0 °C for chemistry)..... 43 5.6 0.0 5.6 13
 If cooler temperature is out of compliance fill out form 00070F Temp Gun ID#: _____
 Cooler Accepted by: [Signature] Date: 07/29/10 Time: 18:30

Complete custody forms and attach all shipping documents

Log-In Phase:

Was a temperature blank included in the cooler? YES NO
 What kind of packing material was used? ... Bubble Wrap Wet Ice Gel Packs Baggies Foam Block Paper Other: _____
 Was sufficient ice used (if appropriate)? NA YES NO
 Were all bottles sealed in individual plastic bags? YES NO
 Did all bottles arrive in good condition (unbroken)? YES NO
 Were all bottle labels complete and legible? YES NO
 Did the number of containers listed on COC match with the number of containers received? YES NO
 Did all bottle labels and tags agree with custody papers? YES NO
 Were all bottles used correct for the requested analyses? YES NO
 Do any of the analyses (bottles) require preservation? (attach preservation sheet, excluding VOCs)... NA YES NO
 Were all VOC vials free of air bubbles? NA YES NO
 Was sufficient amount of sample sent in each bottle? YES NO
 Date VOC Trip Blank was made at ARI..... NA
 Was Sample Split by ARI: NA YES Date/Time: _____ Equipment: _____ Split by: _____
 Samples Logged by: [Signature] Date: 7/30/10 Time: 1400

**** Notify Project Manager of discrepancies or concerns ****

| Sample ID on Bottle | Sample ID on COC | Sample ID on Bottle | Sample ID on COC |
|---------------------|------------------|---------------------|------------------|
| | | | |
| | | | |
| | | | |

Additional Notes, Discrepancies, & Resolutions:

By: _____ Date: _____

| | | | |
|--|--|--|-------------------|
| | | | Small → "sm" |
| | | | Peabubbles → "pb" |
| | | | Large → "lg" |
| | | | Headspace → "hs" |



Cooler Temperature Compliance Form

| Cooler#: | | Temperature(°C): 7.3 | |
|-------------------|--------------|----------------------|--|
| Sample ID | Bottle Count | Bottle Type | |
| PSB23-0-05-072910 | 6 | | |
| -1.5-2-072910 | 6 | | |
| -2-4-072910 | 15 | | |
| -4-6-072910 | 6 | | |
| -14-16.5-072910 | 8 | | |
| -16.5-19-072910 | 8 | | |
| -TB | 2 | | |

| Cooler#: | | Temperature(°C): | |
|-----------|--------------|------------------|--|
| Sample ID | Bottle Count | Bottle Type | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |

| Cooler#: | | Temperature(°C): | |
|-----------|--------------|------------------|--|
| Sample ID | Bottle Count | Bottle Type | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |

| Cooler#: | | Temperature(°C): | |
|-----------|--------------|------------------|--|
| Sample ID | Bottle Count | Bottle Type | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |

Completed by: _____ Date: _____ Time: _____

Case Narrative, Data Qualifiers, Control Limits

ARI Job ID: RG58



Case Narrative

Client: Floyd Snider
Project: Lora Lake RI
ARI Job No.: RG58

Sample receipt

Analytical Resources, Inc. (ARI) accepted nineteen soil samples and three trip blanks on July 29, 2010 under ARI job RG58. The cooler temperatures measured by IR thermometer following ARI SOP were 0.0, 3.6 and 7.3°C. For details regarding sample receipt, please refer to the enclosed Cooler Receipt Form.

Dioxin/Furan analyses were subcontracted to Frontier Analytical Laboratory in El Dorado Hills, CA. The dioxin data on CD as generated by Frontier is forwarded with this package.

Volatiles by SW8260C

The samples and associated laboratory QC were analyzed within method recommended holding times.

Initial and continuing calibrations were within method requirements for target compounds. Internal standards were within limits.

The surrogate percent recoveries were within control limits.

The method blank was clean at the reporting limits. The LCS and LCSD percent recoveries and RPD were within control limits.

No additional volume was received for matrix QC.

PAHs by SW8270D

The samples were initially screened to determine if a response was present that would require modifications in the extraction process. No modifications were required. The samples and associated laboratory QC were extracted and analyzed within the method recommended holding times.

Initial and continuing calibrations were within method requirements. Internal standards were within limits.

The surrogate percent recoveries were within control limits.



The method blank was clean at the reporting limit. The LCS percent recoveries were within control limits.

The matrix spike and matrix spike duplicate percent recoveries of the benzofluoranthenes was high of advisory control limits. No action is required for matrix QC.

In response to comments from NELAP and DOD auditors, ARI will now report the 'total' benzofluoranthenes rather than the individual compounds. This total will include the response of the b, k and j isomers.

Pentachlorophenol by SW8041

The samples and associated laboratory QC were extracted and analyzed within the method recommended holding times.

Initial and continuing calibrations were within method requirements.

The surrogate percent recoveries were within control limits.

The method blank was clean at the reporting limit. The LCS percent recovery was within control limits.

The matrix spike and matrix spike duplicate percent recoveries were within advisory control limits.

Acid/Silica Cleaned NWTPH-Dx

The samples and associated laboratory QC were extracted 08/06/10 and analyzed within the method recommended holding times. Sample **PSB24-14-16-072910** was lost during the extraction process and re-extracted within holding time on 08/10/10.

Initial and continuing calibrations were within method requirements.

The surrogate percent recoveries were within control limits, with exceptions. Sample **PSB24-2-4-072910** was adjusted for a suspected double surrogate spike. As the sample was clean, no further action was taken.

The method blanks were clean at the reporting limits. The LCS/LSCD percent recoveries and RPDs were within control limits.

The matrix spike and matrix spike duplicate percent recoveries were within advisory control limits.



BETX by SW8021B Mod and NWTPH-Gx

The samples and associated laboratory QC were analyzed within the method recommended holding times.

Initial and continuing calibrations were within method requirements, with allowed outliers outside of 15% for the BETX calibration on PID2 on 08/06/10. As the samples analyzed were only trip blanks and no vials remained for reanalysis, no action was taken.

The surrogate percent recoveries were within control limits.

The method blanks were clean at the reporting limits. The LCS and LCSD percent recoveries were within control limits.

No additional volume was received for matrix QC.

Total Arsenic and Lead by SW846 6010B

The samples and associated laboratory QC were digested and analyzed within the method recommended holding time.

The method blank was clean at the reporting limits. The LCS percent recoveries were within control limits.

The SRM results were within advisory ranges.

The matrix spike percent recoveries were within limits.

Duplicate RPDs were within control limits.

General Chemistry (TOC/TS)

The samples and associated laboratory QC were prepared and analyzed within the method recommended holding time.

The method blanks were clean at the reporting limits. The LCS percent recovery was within control limits.

The SRM percent recovery was within limits.

The batch matrix spike percent recovery and replicate RSDs were within control limit. Copies of the summary form have been included in this report.



Data Reporting Qualifiers

Effective 7/10/2009

Inorganic Data

- U Indicates that the target analyte was not detected at the reported concentration
- * Duplicate RPD is not within established control limits
- B Reported value is less than the CRDL but \geq the Reporting Limit
- N Matrix Spike recovery not within established control limits
- NA Not Applicable, analyte not spiked
- H The natural concentration of the spiked element is so much greater than the concentration spiked that an accurate determination of spike recovery is not possible
- L Analyte concentration is ≤ 5 times the Reporting Limit and the replicate control limit defaults to ± 1 RL instead of the normal 20% RPD

Organic Data

- U Indicates that the target analyte was not detected at the reported concentration
- * Flagged value is not within established control limits
- B Analyte detected in an associated Method Blank at a concentration greater than one-half of ARI's Reporting Limit or 5% of the regulatory limit or 5% of the analyte concentration in the sample.
- J Estimated concentration when the value is less than ARI's established reporting limits
- D The spiked compound was not detected due to sample extract dilution
- E Estimated concentration calculated for an analyte response above the valid instrument calibration range. A dilution is required to obtain an accurate quantification of the analyte.
- Q Indicates a detected analyte with an initial or continuing calibration that does not meet established acceptance criteria ($< 20\%$ RSD, $< 20\%$ Drift or minimum RRF).
- S Indicates an analyte response that has saturated the detector. The calculated concentration is not valid; a dilution is required to obtain valid quantification of the analyte



- NA The flagged analyte was not analyzed for
- NR Spiked compound recovery is not reported due to chromatographic interference
- NS The flagged analyte was not spiked into the sample
- M Estimated value for an analyte detected and confirmed by an analyst but with low spectral match parameters. This flag is used only for GC-MS analyses
- M2 The sample contains PCB congeners that do not match any standard Aroclor pattern. The PCBs are identified and quantified as the Aroclor whose pattern most closely matches that of the sample. The reported value is an estimate.
- N The analysis indicates the presence of an analyte for which there is presumptive evidence to make a "tentative identification"
- Y The analyte is not detected at or above the reported concentration. The reporting limit is raised due to chromatographic interference. The Y flag is equivalent to the U flag with a raised reporting limit.
- C The analyte was positively identified on only one of two chromatographic columns. Chromatographic interference prevented a positive identification on the second column
- P The analyte was detected on both chromatographic columns but the quantified values differ by $\geq 40\%$ RPD with no obvious chromatographic interference

Geotechnical Data

- A The total of all fines fractions. This flag is used to report total fines when only sieve analysis is requested and balances total grain size with sample weight.
- F Samples were frozen prior to particle size determination
- SM Sample matrix was not appropriate for the requested analysis. This normally refers to samples contaminated with an organic product that interferes with the sieving process and/or moisture content, porosity and saturation calculations
- SS Sample did not contain the proportion of "fines" required to perform the pipette portion of the grain size analysis
- W Weight of sample in some pipette aliquots was below the level required for accurate weighting

SURRE SOLUTIONS

| LABEL | SOLN ID | TEST | CONC. UG/ML | SOLVENT | EXP. |
|-------|----------------------|------------|-------------|---------|----------|
| A | 1752-2 | ABN | 100/150 | MEOH | 01/22/11 |
| B | 1747-2 | SIM PNA | 15/75 | MEOH | 10/07/10 |
| C | 1705-4 | SIM ABN | 25/37.5 | MEOH | 03/08/11 |
| D | 1751-1 | LOW PCB | 0.2 | HEXANE | 12/29/10 |
| E | 1661-2 | HERB | 62.5 | MEOH | 10/02/10 |
| F | 1683-3 | PCP | 12.5 | ACETONE | 12/09/10 |
| G | 1707-2 | 1,4DIOXANE | 100 | MEOH | 03/19/11 |
| H | 1723-2 | OP-PEST | 25 | MEOH | 04/02/11 |
| I | 1747-1 | LOW S. PNA | 1.5 | MEOH | 10/07/10 |
| J | 1681-2 | TBT-PORE | 0.125 | MECL2 | 12/01/10 |
| K | 1689-1 | MED PCB | 20 | ACETONE | 12/29/10 |
| L | 1681-1 | TBT | 2.5 | MECL2 | 12/01/10 |
| M | 1682-1 | EPH | 1500 | MECL2 | 09/17/10 |
| N | 1689-3 | PCB | 2 | ACETONE | 12/29/10 |
| O | 1755-1 | TPH | 450 | MECL2 | 06/02/11 |
| P | 1742-2 | HCID | 2250 | MECL2 | 05/13/11 |
| Q | 1620-2 | EDB | 1 | MEOH | 06/22/10 |
| R | 1615-1 | RESIN ACID | 250 | ACETONE | 06/17/10 |
| S* | 1568-5 | PBDE | .25 | MEOH | 01/13/11 |
| T | 1674-2 | ALKYL PNA | 10 | MEOH | 07/30/10 |
| U | 1633-1 | CONGENER | 2.5 | ACETONE | 08/11/10 |
| V | | | | | |
| | *reverified solution | | | | |
| | | | | | |
| | | | | | |
| | | | | | |
| | | | | | |
| | | | | | |
| | | | | | |
| | | | | | |

LCS SOLUTIONS

8/12/2010

| LABL SOLN ID | | TEST | CONC. UG/ML | SOLVENT | EXP. |
|--------------|--------|--------------|-------------|---------|----------|
| 1 | 1754-4 | PCB 1660 | 20 | ACETONE | 03/30/11 |
| 2# | | BCOC PEST | 10 | ACETONE | NA |
| 3 | 1705-3 | PEST | 02/04/20 | ACETONE | 03/08/11 |
| 4 | 1744-3 | LOW PEST | 0.2/0.4/2 | ACETONE | 03/08/11 |
| 5 | 1677-1 | EPH | 1500 | MECL2 | 11/12/10 |
| 6 | 1702-2 | PCP | 12.5/125 | ACETONE | 02/18/11 |
| 7 | 1750-1 | ABN | 100 | ACETONE | 01/31/11 |
| 8 | 1681-4 | TBT | 2.5 | MECL2 | 12/01/10 |
| 9 | 1682-2 | PORE TBT | .125/.25 | MECL2 | 12/01/10 |
| 10 | 1749-1 | ABN ACID | 100/200 | MECL2 | 01/28/11 |
| 11 | 1730-2 | TPHD | 15000 | ACETONE | 04/26/11 |
| 12 | 1749-2 | ABN BASE | 200 | MEOH | 01/29/11 |
| 13 | 1716-2 | LOW PCB | 2 | ACETONE | 03/30/11 |
| 14 | 1753-3 | LOW ABN ACID | 10/20 | MEOH | 01/28/11 |
| 15 | 1726-3 | SIM PNA | 15/75 | MEOH | 10/07/10 |
| 16 | 1707-1 | DIOXANE | 100 | MEOH | 11/05/10 |
| 17 | 1644-1 | 1248 PCB | 10 | ACETONE | 09/10/10 |
| 18 | 1726-4 | LOW SIM PNA | 1.5 | ACETONE | 10/07/10 |
| 19 | 1746-3 | AK103 | 7500 | ACETONE | 12/01/10 |
| 20 | 1682-4 | PNA | 100 | ACETONE | 12/04/10 |
| 21 | 1725-1 | SKY/BHT | 100 | MEOH | 03/18/11 |
| 22 | 1728-1 | HERB | 12.5/12500 | MEOH | 10/20/10 |
| 23 | 1753-4 | LW ABN BASE | 20 | MEOH | 01/29/11 |
| 24 | 1696-1 | LOW ABN | 10 | ACETONE | 01/13/11 |
| 25# | | DIPHENYL | 100 | MEOH | NA |
| 26 | 1723-3 | OP-PEST | 25 | MEOH | 11/20/10 |
| 27 | 1668-3 | STEROLS | 200 | MEOH | 10/30/10 |
| 28# | 1750-2 | ADD. PEST | 4 | ACETONE | 09/03/10 |
| 29# | | DECANES | 100 | MEOH | NA |
| 30 | 1620-1 | EDB/DBCP | 0.2 | MEOH | 06/22/10 |

LCS SOLUTIONS

8/12/2010

| | | | | | |
|----|-----------------------------|-------------|--------|---------|----------|
| 31 | 1707-3 | TERPINEOL | 100 | MEOH | 03/19/11 |
| 32 | 1619-3 | GUAIACOL | 50-200 | ACETONE | 04/30/10 |
| 33 | 1639-3 | RETENE | 100 | MEOH | 09/03/10 |
| 34 | 1633-1 | CONGENERS | 2.5 | ACETONE | 08/11/10 |
| 35 | 1674-3 | ALKYL PNA A | 10 | MEOH | 10/28/10 |
| 36 | 1601-3 | ALKYL PNA B | 10 | MEOH | 05/13/10 |
| 50 | 1617-1 | FULL RESIN | 250 | ACETONE | 06/17/10 |
| 51 | 1696-3 | DDTS | 2.5 | ACETONE | 06/03/10 |
| 52 | 1613-5 | 1232 PCB | 20 | ACETONE | 06/16/10 |
| 53 | 1703-3 | DALAPON | 50 | MEOH | 09/11/10 |
| 53 | 1701-2 | PBDE | 0.5 | ACETONE | 02/10/11 |
| 54 | 1753-1 | T-CHLORDANE | 10 | ACETONE | 07/21/11 |
| 55 | 1753-2 | TOXAPHENE | 50 | ACETONE | 07/21/11 |
| | #=PROJECT SPECIFIC SOLUTION | | | | |
| | *=REVERIFIED SOLUTION | | | | |
| | | | | | |
| | | | | | |
| | | | | | |
| | | | | | |



**Spike Recovery Control Limits for Analysis of Solid Samples
Volatile Organic Compounds (VOA) EPA SW-846 Methods 8260C
5 mL Purge Volume ⁽⁷⁾
Effective:5/18/09**

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| | Low Level ⁽¹⁾ | Low Level ME Limits ⁽³⁾ | Medium Level ⁽²⁾ | Medium Level ME Limits ⁽³⁾ |
|--|--------------------------|---------------------------------------|-----------------------------|--|
| LCS Spike Recovery ⁽⁸⁾ | | | | |
| Dichlorodifluoromethane | 53 - 148 | 37 - 164 | 25 - 128 | 10 - 145 |
| Chloromethane | 64 - 125 | 54 - 135 | 55 - 121 | 44 - 132 |
| Vinyl Chloride | 63 - 137 | 51 - 149 | 66 - 123 | 57 - 133 |
| Bromomethane | 57 - 136 | 44 - 149 | 40 - 154 | 21 - 173 |
| Chloroethane | 64 - 131 | 53 - 142 | 72 - 128 | 63 - 137 |
| Trichlorofluoromethane | 69 - 132 | 59 - 143 | 69 - 135 | 58 - 146 |
| Acrolein | 54 - 137 | 40 - 151 | 39 - 135 | 23 - 151 |
| 1,1,2-Trichloro-1,2,2-trifluoroethane | 74 - 130 | 65 - 139 | 65 - 139 | 53 - 151 |
| Acetone | 60 - 131 | 48 - 143 | 55 - 130 | 43 - 143 |
| 1,1-Dichloroethene | 75 - 126 | 67 - 135 | 73 - 133 | 63 - 143 |
| Bromoethane | 76 - 126 | 68 - 134 | 74 - 133 | 64 - 143 |
| Methyl Iodide | 65 - 139 | 53 - 151 | 47 - 155 | 29 - 173 |
| Methylene Chloride | 70 - 123 | 61 - 132 | 80 - 120 | 75 - 122 |
| Acrylonitrile | 67 - 125 | 57 - 135 | 62 - 129 | 51 - 140 |
| Methyl tert-Butyl Ether | 70 - 120 | 62 - 128 | 69 - 128 | 59 - 138 |
| Carbon Disulfide | 71 - 129 | 61 - 139 | 64 - 135 | 52 - 147 |
| trans-1,2-Dichloroethene | 80 - 120 | 74 - 126 | 78 - 125 | 70 - 133 |
| Vinyl Acetate | 60 - 136 | 47 - 149 | 66 - 132 | 55 - 143 |
| 1,1-Dichloroethane | 80 - 120 | 75 - 124 | 77 - 124 | 69 - 132 |
| 2-Butanone | 70 - 120 | 62 - 127 | 65 - 126 | 55 - 136 |
| 2,2-Dichloropropane | 74 - 123 | 66 - 131 | 75 - 127 | 66 - 136 |
| cis-1,2-Dichloroethene | 80 - 120 | 76 - 123 | 80 - 125 | 74 - 132 |
| Chloroform | 80 - 120 | 74 - 123 | 80 - 124 | 73 - 131 |
| Bromodichloromethane | 77 - 121 | 70 - 128 | 78 - 130 | 69 - 139 |
| 1,1,1-Trichloroethane | 77 - 121 | 70 - 128 | 76 - 130 | 67 - 139 |
| 1,1-Dichloropropene | 80 - 120 | 77 - 123 | 77 - 131 | 68 - 140 |
| Carbon Tetrachloride | 77 - 122 | 70 - 130 | 74 - 129 | 65 - 138 |
| 1,2-Dichloroethane | 76 - 120 | 69 - 123 | 73 - 123 | 65 - 131 |
| Benzene | 80 - 120 | 80 - 126 | 80 - 120 | 75 - 130 |
| Trichloroethene | 80 - 120 | 77 - 123 | 80 - 125 | 75 - 132 |
| 1,2-Dichloropropane | 80 - 120 | 76 - 120 | 80 - 122 | 74 - 129 |
| Bromochloromethane | 80 - 120 | 73 - 127 | 80 - 127 | 73 - 135 |
| Dibromomethane | 80 - 120 | 74 - 121 | 80 - 121 | 76 - 128 |
| 2-Chloroethylvinylether | 10 - 191 | 10 - 222 | 61 - 128 | 50 - 139 |



**Spike Recovery Control Limits for Analysis of Solid Samples
Volatile Organic Compounds (VOA) EPA SW-846 Methods 8260C
5 mL Purge Volume ⁽⁷⁾
Effective:5/18/09**

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| | Low Level ⁽¹⁾ | Low Level ME Limits ⁽³⁾ | Medium Level ⁽²⁾ | Medium Level ME Limits ⁽³⁾ |
|-----------------------------|---------------------------------|---|------------------------------------|--|
| 4-Methyl-2-Pentanone | 67 - 120 | 59 - 125 | 80 - 123 | 73 - 130 |
| cis-1,3-Dichloropropene | 74 - 120 | 67 - 125 | 80 - 122 | 73 - 129 |
| Toluene | 80 - 120 | 79 - 120 | 80 - 122 | 80 - 127 |
| trans-1,3-Dichloropropene | 65 - 120 | 57 - 125 | 80 - 123 | 79 - 129 |
| 2-Hexanone | 65 - 130 | 54 - 141 | 58 - 129 | 46 - 141 |
| 1,1,2-Trichloroethane | 80 - 120 | 75 - 122 | 80 - 120 | 77 - 126 |
| 1,3-Dichloropropane | 80 - 120 | 74 - 122 | 80 - 120 | 76 - 126 |
| Tetrachloroethene | 80 - 121 | 79 - 127 | 80 - 130 | 73 - 138 |
| Dibromochloromethane | 64 - 120 | 55 - 128 | 77 - 120 | 70 - 127 |
| Ethylene Dibromide | 75 - 120 | 68 - 124 | 80 - 120 | 80 - 120 |
| Chlorobenzene | 80 - 120 | 82 - 120 | 80 - 121 | 80 - 127 |
| Ethylbenzene | 80 - 127 | 80 - 134 | 80 - 126 | 80 - 132 |
| 1,1,2,2-Tetrachloroethane | 74 - 120 | 66 - 128 | 79 - 120 | 73 - 123 |
| m,p-Xylene | 80 - 125 | 80 - 131 | 80 - 130 | 80 - 137 |
| o-Xylene | 78 - 120 | 71 - 126 | 80 - 124 | 80 - 130 |
| Styrene | 80 - 123 | 78 - 130 | 80 - 132 | 77 - 140 |
| Isopropylbenzene | 80 - 127 | 84 - 133 | 80 - 130 | 80 - 137 |
| Bromoform | 60 - 120 | 50 - 128 | 68 - 129 | 58 - 139 |
| 1,1,1,2-Tetrachloroethane | 69 - 121 | 60 - 130 | 80 - 126 | 76 - 133 |
| 1,2,3-Trichloropropane | 72 - 121 | 64 - 129 | 77 - 120 | 71 - 121 |
| trans-1,4-Dichloro-2-butene | 65 - 126 | 55 - 136 | 66 - 127 | 56 - 137 |
| n-Propylbenzene | 80 - 132 | 80 - 139 | 80 - 132 | 77 - 140 |
| Bromobenzene | 80 - 120 | 78 - 122 | 80 - 121 | 80 - 127 |
| 1,3,5-Trimethylbenzene | 80 - 125 | 80 - 131 | 78 - 137 | 68 - 147 |
| 2-Chlorotoluene | 80 - 125 | 77 - 132 | 80 - 123 | 80 - 129 |
| 4-Chlorotoluene | 80 - 127 | 77 - 134 | 80 - 130 | 74 - 138 |
| tert-Butylbenzene | 87 - 122 | 80 - 128 | 80 - 133 | 78 - 141 |
| 1,2,4-Trimethylbenzene | 80 - 126 | 80 - 132 | 80 - 131 | 79 - 139 |
| sec-Butylbenzene | 80 - 134 | 80 - 142 | 80 - 136 | 76 - 146 |
| 4-Isopropyltoluene | 80 - 131 | 80 - 138 | 80 - 141 | 71 - 151 |
| 1,3-Dichlorobenzene | 80 - 120 | 80 - 126 | 80 - 126 | 77 - 133 |
| 1,4-Dichlorobenzene | 80 - 120 | 79 - 126 | 80 - 121 | 77 - 127 |
| n-Butylbenzene | 80 - 138 | 80 - 146 | 80 - 138 | 77 - 147 |
| 1,2-Dichlorobenzene | 80 - 120 | 78 - 122 | 80 - 120 | 80 - 121 |
| 1,2-Dibromo-3-chloropropane | 59 - 120 | 49 - 130 | 67 - 121 | 58 - 130 |
| 1,2,4-Trichlorobenzene | 78 - 130 | 69 - 139 | 80 - 133 | 72 - 142 |



**Spike Recovery Control Limits for Analysis of Solid Samples
Volatile Organic Compounds (VOA) EPA SW-846 Methods 8260C
5 mL Purge Volume ⁽⁷⁾
Effective:5/18/09**

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| | Low Level ⁽¹⁾ | Low Level ME Limits ⁽³⁾ | Medium Level ⁽²⁾ | Medium Level ME Limits ⁽³⁾ |
|----------------------------------|--------------------------|------------------------------------|-----------------------------|---------------------------------------|
| Hexachloro-1,3-butadiene | 76 - 129 | 67 - 138 | 62 - 148 | 48 - 162 |
| Naphthalene | 66 - 120 | 58 - 126 | 74 - 133 | 64 - 143 |
| 1,2,3-Trichlorobenzene | 73 - 123 | 65 - 131 | 80 - 126 | 72 - 134 |
| MB/LCS Surrogate Recovery | | | | |
| Dibromofluoromethane | 80 - 120 | (4) | 80 - 120 | (4) |
| d4-1,2-Dichloroethane | 79 - 121 | (4) | 76 - 120 | (4) |
| d8-Toluene | 80 - 120 | (4) | 80 - 120 | (4) |
| 4-Bromofluorobenzene | 80 - 120 | (4) | 80 - 120 | (4) |
| d4-1,2-Dichlorobenzene | 80 - 120 | (4) | 80 - 120 | (4) |
| Sample Surrogate Recovery | | | | |
| Dibromofluoromethane | 30 - 160 ⁽⁶⁾ | (4) | 30 - 160 ⁽⁶⁾ | (4) |
| d4-1,2-Dichloroethane | 75 - 152 | (4) | 69 - 120 | (4) |
| d8-Toluene | 82 - 115 | (4) | 80 - 120 | (4) |
| 4-Bromofluorobenzene | 64 - 120 | (4) | 76 - 128 | (4) |
| d4-1,2-Dichlorobenzene | 80 - 120 | (4) | 80 - 120 | (4) |

(1) Control Limits calculated using all data generated 1/1/08 through 12/31/08.

(2) Control Limits calculated using all data generated 3/1/07 through 11/15/07.

(3) **ME** = A **marginal exceedance** defined in the NELAC Standard⁽⁵⁾ as beyond the LCS-CL but still within the ME limits. ME limits are between 3 and 4 standard deviations around the mean. A maximum of four marginal exceedances are acceptable. Five or more marginal exceedances require corrective action.

(4) Marginal Exceedances not allowed for surrogate standards

(5) **2003 NELAC Standard (EPA/600/R-04/003), July 2003**, Chapter 5, pages 251-252.

(6) 30 – 160 are default, advisory control limits used when there is insufficient data to calculate historic control limits. **DO NOT** use these limits as the sole reason to reject the data from a batch of analyses

(7) Highlighted control limits (**bold font**) are adjusted from the calculated values as follows:

a) ARI does not use control limits < 10

b) Control limits for analyzes with no separate preparation procedure are adjusted to reflect the minimum uncertainty in the calibration of the instrument allowed by the referenced analytical method.

(8) Laboratory Control Sample (LCS) spike recovery control limits also used as advisory control limits for sample matrix spike (MS) analyzes. MS recovery values are advisory and not used to assess the acceptability of an analytical batch.



**Spike Recovery Control Limits for Polycyclic Aromatic Hydrocarbons
EPA Method SW-846-8270D ^(1,2)
Effective 5/1/09**

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| Sample Matrix | Water | | Soil | |
|------------------------------------|-------------------------|--------------------------|-------------------------|--------------------------|
| | 500 mL to 0.5 mL | | 7.5 g / 0.5 mL | |
| Sample Volume / Final Volume | | | | |
| LCS Spike Recovery ⁽⁶⁾ | Control Limits | ME Limits ⁽³⁾ | Control Limits | ME Limits ⁽³⁾ |
| Napthalene | 30 - 100 | 21 - 100 | 37 - 100 | 31 - 100 |
| 2-Methylnapthalene | 33 - 108 | 21 - 121 | 43 - 101 | 33 - 111 |
| 1-Methylnapthalene | 34 - 100 | 26 - 100 | 39 - 100 | 32 - 100 |
| Acenaphthylene | 45 - 100 | 38 - 100 | 44 - 100 | 37 - 100 |
| Acenaphthene | 40 - 100 | 32 - 100 | 41 - 100 | 35 - 100 |
| Dibenzofuran | 45 - 100 | 37 - 100 | 44 - 100 | 37 - 100 |
| Fluorene | 45 - 100 | 37 - 105 | 49 - 100 | 43 - 100 |
| Phenanthrene | 47 - 101 | 38 - 110 | 48 - 100 | 42 - 100 |
| Anthracene | 47 - 100 | 38 - 108 | 50 - 100 | 44 - 100 |
| Fluoranthene | 48 - 110 | 38 - 120 | 54 - 100 | 47 - 107 |
| Pyrene | 48 - 109 | 38 - 119 | 41 - 105 | 30 - 116 |
| Benz(a)anthracene | 44 - 105 | 34 - 115 | 49 - 100 | 42 - 102 |
| Chrysene | 50 - 103 | 41 - 112 | 50 - 100 | 43 - 101 |
| Benzofluoranthene(s) (Total) | 30 - 160 ⁽⁷⁾ | 30 - 160 ⁽⁷⁾ | 30 - 160 ⁽⁷⁾ | 30 - 160 ⁽⁷⁾ |
| Benzo(a)pyrene | 44 - 107 | 34 - 118 | 50 - 100 | 42 - 105 |
| Indeno(1,2,3-cd)pyrene | 30 - 106 | 17 - 119 | 33 - 101 | 22 - 112 |
| Dibenzo(a,h)anthracene | 42 - 103 | 32 - 113 | 37 - 104 | 26 - 115 |
| Benzo(g,h,i)Perylene | 42 - 102 | 32 - 112 | 33 - 107 | 21 - 119 |
| MB / LCS Surrogate Recovery | | - | | |
| d14-p-Terphenyl | 52 - 110 | (5) | 47 - 112 | (5) |
| 2-Fluorobiphenyl | 36 - 100 | (5) | 40 - 100 | (5) |
| Sample Surrogate Recovery | | | | |
| d14-p-Terphenyl | 23 - 120 | (5) | 35 - 112 | (5) |
| 2-Fluorobiphenyl | 38 - 100 | (5) | 34 - 100 | (5) |

- (1) Control limits calculated using all available spike recovery data from 7/1/07 through 2/27/09.
- (2) Highlighted control limits (**bold font**) adjusted to demonstrate that ARI does not use control limits < 10 for the lower limit or < 100 for the upper limit.
- (3) **ME** = A marginal exceedance defined in the NELAC Standard (4) as beyond the LCS-CL but still within the ME limits. ME limits are between 3 and 4 standard deviations around the mean. A maximum of one marginal exceedance is acceptable. Two or more marginal exceedances require corrective action.
- (4) **2003 NELAC Standard (EPA/600/R-04/003), July 2003**, Chapter 5, pages 251-252.
- (5) Marginal Exceedances are not allowed for surrogate standards.
- (6) Laboratory Control Sample (LCS) spike recovery control limits also used as advisory control limits for sample matrix spike (MS) analyzes. MS recovery values are advisory and not used to assess the acceptability of an analytical batch.
- (7) Default limits pending generation of historic limits for total benzofluoranthrenes (7/29/10)



Spike Recovery Control Limits for Chlorinated Phenols
EPA Method SW-846-8041^(1,2)

Effective 5/1/09

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| Sample Matrix: | ARI's Calculated Control Limits | |
|--|---------------------------------|-----------------|
| | Water | Soil / Sediment |
| Sample Amount / Final Volume: | 500 / 50 mL | 10 g / 25 mL |
| LCS Spike Recovery⁽³⁾ | | |
| Pentachlorophenol | 27 - 115 | 10 - 162 |
| | | |
| Method Blank/LCS Surrogate Recovery | | |
| 2,4,6-Tribromophenol | 40 - 130 | 50 - 115 |
| | | |
| Sample Surrogate Recovery | | |
| 2,4,6-Tribromophenol | 11 - 156 | 10 - 146 |
| | | |

(1) ARI's Control limits calculated using all available spike recovery data from 1/1/08 through 12/1/08.

(2) Highlighted control limits (**bold font**) adjusted to demonstrate that ARI does not use control limits < 10.

(3) Laboratory Control Sample (LCS) spike recovery control limits also used as advisory control limits for sample matrix spike (MS) analyzes. MS recovery values are advisory and not used to assess the acceptability of an analytical batch.



**Spike Recovery Control Limits Hydrocarbon Identification (NWTPH-HCID)
and Diesel Range Petroleum Hydrocarbons (NWTPH-D & AK-102) ⁽¹⁾**
Effective 5/1/09

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| Method: | NWTPH-HCID ⁽²⁾ | NWTPH-D | | AK102 ⁽²⁾ |
|--|---------------------------|-------------|-------------|----------------------------|
| Sample Matrix: | Water & Soil | Water | Soil | Water & Soil |
| Preparation: | 500 to 1 mL | 500 to 1 mL | 10g to 1 mL | 500 to 1 mL or 10g to 1 mL |
| LCS Spike Recovery ⁽³⁾ | | | | |
| Diesel | -- - -- | 56 - 103 | 55 - 104 | 75 - 125 |
| Diesel with Acid & Silica Clean-up | -- - -- | 43 - 100 | 54 - 96 | (4) |
| Diesel with Silica Clean-up | -- -- | 43 - 100 | 54 - 96 | 75 - 125 |
| Method Blank/LCS Surrogate Recovery | | | | |
| o-Terphenyl | -- - -- | 57 - 120 | 58 - 121 | 60 - 120 |
| o-Terphenyl with Acid & Silica Clean-up | -- - -- | 51 - 120 | 63 - 115 | (4) |
| o-Terphenyl Silica Clean-up | | 51 - 120 | 63 - 115 | 60 - 120 |
| Sample Surrogate Recovery | | | | |
| o-Terphenyl | 50 - 150 | 35 - 131 | 53 - 118 | 50 - 150 |
| o-Terphenyl with Acid & Silica Clean-up | -- - -- | 41 - 121 | 49 - 120 | (4) |
| o-Terphenyl with Silica Clean-up | | 41 - 121 | 49 - 120 | 50 - 150 |

1. Control Limits calculated using all data generated 1/1/08 through 12/31/08
2. Method specified, non-prescriptive limits. The NWTPH-HCID Method does not include LCS or MS analyses.
3. Laboratory Control Sample (LCS) spike recovery control limits also used as advisory control limits for sample matrix spike (MS) analyzes. MS recovery values are advisory and not used to assess the acceptability of an analytical batch.
4. Alaska State UST Methods do not allow acid cleanup of sample extracts.



**Spike Recovery Control Limits BTEX – EPA Method 8021 &
Gasoline – Methods NWTPH-G and AK101^(1,2)**

Effective 5/1/09

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| Sample Matrix: | Aqueous Samples | | Soil / Sediment Samples | |
|--|-----------------|-------------------|-------------------------|-------------------|
| Analytical Method: | Method 8021B | NWTPH-G AK-101 | Method 8021B | NWTPH-G AK-101 |
| LCS Spike Recovery ⁽³⁾ | | | | |
| Benzene | 73 - 120 | | 72 - 120 | |
| Toluene | 73 - 120 | | 72 - 120 | |
| Ethyl benzene | 69 - 120 | | 71 - 120 | |
| <i>m,p</i> -Xylenes | 72 - 120 | | 72 - 120 | |
| <i>o</i> -Xlyene | 73 - 120 | | 72 - 120 | |
| MTBE | 30 - 182 | | 40 - 163 | |
| Gasoline | | 75 - 124 | | 74 - 124 |
| | | | | |
| Method Blank/LCS Surrogate Recovery | | | | |
| Trifluorotoluene (TFT) | 79 - 120 | 80 - 120 | 80 - 120 | 80 - 120 |
| Bromobenzene | 79 - 120 | 80 - 120 | 77 - 120 | 80 - 120 |
| | | | | |
| Sample Surrogate Recovery | | | | |
| Trifluorotoluene (TFT) | 80 - 120 | 80 - 120 | 68 - 124 | 66 - 123 |
| Bromobenzene | 80 - 120 | 80 - 120 | 62 - 134 | 62 - 130 |

(1) Control Limits calculated using all data generated 1/1/08 through 12/31/08.

(2) Highlighted control limits (bold font) are adjusted from the calculated values as follows:

a) Highlighted control limits (**bold font**) adjusted to demonstrate that ARI does not use control limits < 10 for the lower limit or < 100 for the upper limit.

b) Control limits for analytes with no separate preparation procedure are adjusted to reflect the minimum uncertainty in the calibration of the instrument allowed by the referenced analytical method.

(3) Laboratory Control Sample (LCS) spike recovery control limits also used as advisory control limits for sample matrix spike (MS) analytes. MS recovery values are advisory and not used to assess the acceptability of an analytical batch.



Summary of Laboratory Control Limits Metals Analyses (All Methods & Sample Matrices)

Effective 5/1/09

Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. <http://www.arilabs.com/portal/downloads/ARI-CLs.zip>

| Element | Matrix Spike Recovery | LCS Recovery | Replicate RPD |
|-----------|-----------------------|--------------|---------------|
| Aluminum | 75 - 125 | 80 - 120 | ≤ 20% |
| Antimony | 75 - 125 | 80 - 120 | ≤ 20% |
| Arsenic | 75 - 125 | 80 - 120 | ≤ 20% |
| Barium | 75 - 125 | 80 - 120 | ≤ 20% |
| Beryllium | 75 - 125 | 80 - 120 | ≤ 20% |
| Boron | 75 - 125 | 80 - 120 | ≤ 20% |
| Cadmium | 75 - 125 | 80 - 120 | ≤ 20% |
| Calcium | 75 - 125 | 80 - 120 | ≤ 20% |
| Chromium | 75 - 125 | 80 - 120 | ≤ 20% |
| Cobalt | 75 - 125 | 80 - 120 | ≤ 20% |
| Copper | 75 - 125 | 80 - 120 | ≤ 20% |
| Iron | 75 - 125 | 80 - 120 | ≤ 20% |
| Lead | 75 - 125 | 80 - 120 | ≤ 20% |
| Magnesium | 75 - 125 | 80 - 120 | ≤ 20% |
| Manganese | 75 - 125 | 80 - 120 | ≤ 20% |
| Mercury | 75 - 125 | 80 - 120 | ≤ 20% |
| Nickel | 75 - 125 | 80 - 120 | ≤ 20% |
| Potassium | 75 - 125 | 80 - 120 | ≤ 20% |
| Selenium | 75 - 125 | 80 - 120 | ≤ 20% |
| Silica | 75 - 125 | 80 - 120 | ≤ 20% |
| Silver | 75 - 125 | 80 - 120 | ≤ 20% |
| Sodium | 75 - 125 | 80 - 120 | ≤ 20% |
| Strontium | 75 - 125 | 80 - 120 | ≤ 20% |
| Thallium | 75 - 125 | 80 - 120 | ≤ 20% |
| Vanadium | 75 - 125 | 80 - 120 | ≤ 20% |
| Zinc | 75 - 125 | 80 - 120 | ≤ 20% |



| Spike Recovery Control Limits for Conventional Wet Chemistry Effective 5/1/09 | | |
|---|----------------------|-----------------|
| Control limits are updated periodically. Assure that you have ARI's current control limits by downloading the files at the time of use. http://www.arilabs.com/portal/downloads/ARI-CLs.zip | | |
| Sample Matrix: | ARI's Control Limits | |
| | Water | Soil / Sediment |
| Matrix Spike Recoveries | % Recovery | % Recovery |
| Ammonia | 75 - 125 | 75 - 125 |
| Bromide | 75 - 125 | 75 - 125 |
| Chloride | 75 - 125 | 75 - 125 |
| Cyanide | 75 - 125 | 75 - 125 |
| Ferrous Iron | 75 - 125 | 75 - 125 |
| Fluoride | 75 - 125 | 75 - 125 |
| Formaldehyde | 75 - 125 | 75 - 125 |
| Hexane Extractable Material | -- - -- | 78 - 114 |
| Hexavalent Chromium | 75 - 125 | 75 - 125 |
| Nitrate/Nitrite | 75 - 125 | 75 - 125 |
| Oil and Grease | 75 - 125 | 75 - 125 |
| Phenol | 75 - 125 | 75 - 125 |
| Phosphorous | 75 - 125 | 75 - 125 |
| Sulfate | 75 - 125 | 75 - 125 |
| Sulfide | 75 - 125 | 75 - 125 |
| Total Kjeldahl Nitrogen | 75 - 125 | 75 - 125 |
| Total Organic Carbon | 75 - 125 | 75 - 125 |
| Duplicate RPDs | | |
| Acidity | ±20% | ±20% |
| Alkalinity | ±20% | ±20% |
| BOD | ±20% | ±20% |
| Cation Exchange | ±20% | ±20% |
| COD | ±20% | ±20% |
| Conductivity | ±20% | ±20% |
| Salinity | ±20% | ±20% |
| Solids | ±20% | ±20% |
| Turbidity | ±20% | ±20% |

**Volatile Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB22-0-0.5-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58A


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18236

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 8.84 g-dry-wt

Date Analyzed: 08/09/10 16:11

Purge Volume: 5.0 mL

Moisture: 5.1%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)


Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 112% |
| d8-Toluene | 98.1% |
| Bromofluorobenzene | 93.2% |
| d4-1,2-Dichlorobenzene | 100% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C
Page 1 of 1

Sample ID: PSB22-1.5-2-072910
SAMPLE

Lab Sample ID: RG58B
LIMS ID: 10-18237
Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB
Date Analyzed: 08/09/10 16:38

Sample Amount: 7.55 g-dry-wt
Purge Volume: 5.0 mL
Moisture: 7.2%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.7 | < 0.7 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.7 | < 0.7 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.7 | < 0.7 | U |
| 79-01-6 | Trichloroethene | 0.7 | < 0.7 | U |
| 127-18-4 | Tetrachloroethene | 0.7 | < 0.7 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 120% |
| d8-Toluene | 99.8% |
| Bromofluorobenzene | 94.5% |
| d4-1,2-Dichlorobenzene | 104% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB22-2-4-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58C


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18238

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 8.41 g-dry-wt

Date Analyzed: 08/09/10 17:04

Purge Volume: 5.0 mL

Moisture: 9.2%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 122% |
| d8-Toluene | 102% |
| Bromofluorobenzene | 96.7% |
| d4-1,2-Dichlorobenzene | 102% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB22-4-6-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58D


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18239

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 8.25 g-dry-wt

Date Analyzed: 08/09/10 17:31

Purge Volume: 5.0 mL

Moisture: 8.7%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 127% |
| d8-Toluene | 104% |
| Bromofluorobenzene | 94.6% |
| d4-1,2-Dichlorobenzene | 103% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB22-17-19-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58E


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18240

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 8.12 g-dry-wt

Date Analyzed: 08/09/10 17:57

Purge Volume: 5.0 mL

Moisture: 12.9%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 136% |
| d8-Toluene | 108% |
| Bromofluorobenzene | 97.3% |
| d4-1,2-Dichlorobenzene | 103% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C
Page 1 of 1

Sample ID: PSB22-19-20-072910
SAMPLE

Lab Sample ID: RG58F
LIMS ID: 10-18241
Matrix: Soil
Data Release Authorized: *AB*
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB
Date Analyzed: 08/09/10 18:24

Sample Amount: 8.74 g-dry-wt
Purge Volume: 5.0 mL
Moisture: 16.8%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)


Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 134% |
| d8-Toluene | 104% |
| Bromofluorobenzene | 99.8% |
| d4-1,2-Dichlorobenzene | 102% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C
Page 1 of 1

Sample ID: PSB23-14-16.5-072910
SAMPLE

Lab Sample ID: RG58K
LIMS ID: 10-18246
Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB
Date Analyzed: 08/09/10 18:50

Sample Amount: 11.1 g-dry-wt
Purge Volume: 5.0 mL
Moisture: 10.4%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.4 | < 0.4 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.4 | < 0.4 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.4 | < 0.4 | U |
| 79-01-6 | Trichloroethene | 0.4 | < 0.4 | U |
| 127-18-4 | Tetrachloroethene | 0.4 | < 0.4 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 134% |
| d8-Toluene | 105% |
| Bromofluorobenzene | 96.9% |
| d4-1,2-Dichlorobenzene | 104% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C
Page 1 of 1

Sample ID: PSB23-16.5-19-072910
SAMPLE

Lab Sample ID: RG58L
LIMS ID: 10-18247
Matrix: Soil
Data Release Authorized: *AS*
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB
Date Analyzed: 08/09/10 19:16

Sample Amount: 8.55 g-dry-wt
Purge Volume: 5.0 mL
Moisture: 13.8%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.6 | < 0.6 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.6 | < 0.6 | U |
| 79-01-6 | Trichloroethene | 0.6 | < 0.6 | U |
| 127-18-4 | Tetrachloroethene | 0.6 | < 0.6 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|------|
| d4-1,2-Dichloroethane | 139% |
| d8-Toluene | 105% |
| Bromofluorobenzene | 100% |
| d4-1,2-Dichlorobenzene | 106% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB24-14-16-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58R


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18253

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 9.72 g-dry-wt

Date Analyzed: 08/09/10 21:02

Purge Volume: 5.0 mL

Moisture: 10.8%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.5 | < 0.5 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.5 | < 0.5 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.5 | < 0.5 | U |
| 79-01-6 | Trichloroethene | 0.5 | < 0.5 | U |
| 127-18-4 | Tetrachloroethene | 0.5 | < 0.5 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 140% |
| d8-Toluene | 105% |
| Bromofluorobenzene | 99.3% |
| d4-1,2-Dichlorobenzene | 106% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB24-16-17-072910

Page 1 of 1

SAMPLE

Lab Sample ID: RG58S


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18254

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 9.95 g-dry-wt

Date Analyzed: 08/10/10 12:35

Purge Volume: 5.0 mL

Moisture: 12.7%

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 0.5 | < 0.5 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 0.5 | < 0.5 | U |
| 107-06-2 | 1,2-Dichloroethane | 0.5 | < 0.5 | U |
| 79-01-6 | Trichloroethene | 0.5 | < 0.5 | U |
| 127-18-4 | Tetrachloroethene | 0.5 | < 0.5 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 122% |
| d8-Toluene | 105% |
| Bromofluorobenzene | 98.2% |
| d4-1,2-Dichlorobenzene | 104% |

VOA SURROGATE RECOVERY SUMMARY



Matrix: Soil

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 POS-LLA

| ARI ID | Client ID | Level | DCE | TOL | BFB | DCB | TOT OUT |
|-------------|----------------------|-------|-------|-------|-------|-------|---------|
| MB-080910 | Method Blank | Low | 118% | 104% | 96.7% | 101% | 0 |
| LCS-080910 | Lab Control | Low | 92.0% | 103% | 101% | 98.2% | 0 |
| LCSD-080910 | Lab Control Dup | Low | 110% | 105% | 101% | 99.7% | 0 |
| RG58A | PSB22-0-0.5-072910 | Low | 112% | 98.1% | 93.2% | 100% | 0 |
| RG58B | PSB22-1.5-2-072910 | Low | 120% | 99.8% | 94.5% | 104% | 0 |
| RG58C | PSB22-2-4-072910 | Low | 122% | 102% | 96.7% | 102% | 0 |
| RG58D | PSB22-4-6-072910 | Low | 127% | 104% | 94.6% | 103% | 0 |
| RG58E | PSB22-17-19-072910 | Low | 136% | 108% | 97.3% | 103% | 0 |
| RG58F | PSB22-19-20-072910 | Low | 134% | 104% | 99.8% | 102% | 0 |
| RG58K | PSB23-14-16.5-072910 | Low | 134% | 105% | 96.9% | 104% | 0 |
| RG58L | PSB23-16.5-19-072910 | Low | 139% | 105% | 100% | 106% | 0 |
| RG58R | PSB24-14-16-072910 | Low | 140% | 105% | 99.3% | 106% | 0 |
| MB-081010 | Method Blank | Low | 105% | 102% | 93.1% | 100% | 0 |
| LCS-081010 | Lab Control | Low | 107% | 102% | 98.5% | 101% | 0 |
| LCSD-081010 | Lab Control Dup | Low | 107% | 102% | 99.2% | 102% | 0 |
| RG58S | PSB24-16-17-072910 | Low | 122% | 105% | 98.2% | 104% | 0 |

LCS/MB LIMITS

QC LIMITS

| | Low | Med | Low | Med |
|--------------------------------|--------|--------|--------|--------|
| SW8260C | | | | |
| (DCE) = d4-1,2-Dichloroethane | 79-121 | 76-120 | 75-152 | 69-120 |
| (TOL) = d8-Toluene | 80-120 | 80-120 | 82-115 | 80-120 |
| (BFB) = Bromofluorobenzene | 80-120 | 80-120 | 64-120 | 76-128 |
| (DCB) = d4-1,2-Dichlorobenzene | 80-120 | 80-120 | 80-120 | 80-120 |

Log Number Range: 10-18236 to 10-18254

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB22-TB

Page 1 of 1

TRIP BLANK

Lab Sample ID: RG58T


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18255

Project: Lora Lake RI

Matrix: Water

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 5.00 mL

Date Analyzed: 08/09/10 19:43

Purge Volume: 5.0 mL

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 107-06-2 | 1,2-Dichloroethane | 1.0 | < 1.0 | U |
| 79-01-6 | Trichloroethene | 1.0 | < 1.0 | U |
| 127-18-4 | Tetrachloroethene | 1.0 | < 1.0 | U |

Reported in µg/L (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 123% |
| d8-Toluene | 105% |
| Bromofluorobenzene | 95.4% |
| d4-1,2-Dichlorobenzene | 104% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: PSB23-TB

Page 1 of 1

TRIP BLANK

Lab Sample ID: RG58U

QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18256

Project: Lora Lake RI

Matrix: Water

POS-LLA

Data Release Authorized: *AS*

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB

Sample Amount: 5.00 mL

Date Analyzed: 08/09/10 20:09

Purge Volume: 5.0 mL

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 107-06-2 | 1,2-Dichloroethane | 1.0 | < 1.0 | U |
| 79-01-6 | Trichloroethene | 1.0 | < 1.0 | U |
| 127-18-4 | Tetrachloroethene | 1.0 | < 1.0 | U |

Reported in µg/L (ppb)


Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 127% |
| d8-Toluene | 106% |
| Bromofluorobenzene | 94.9% |
| d4-1,2-Dichlorobenzene | 103% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C
Page 1 of 1

Sample ID: PSB24-TB
TRIP BLANK

Lab Sample ID: RG58V
LIMS ID: 10-18257
Matrix: Water
Data Release Authorized: 
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Instrument/Analyst: FINN5/PAB
Date Analyzed: 08/09/10 20:35

Sample Amount: 5.00 mL
Purge Volume: 5.0 mL

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 107-06-2 | 1,2-Dichloroethane | 1.0 | < 1.0 | U |
| 79-01-6 | Trichloroethene | 1.0 | < 1.0 | U |
| 127-18-4 | Tetrachloroethene | 1.0 | < 1.0 | U |

Reported in µg/L (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 126% |
| d8-Toluene | 104% |
| Bromofluorobenzene | 97.1% |
| d4-1,2-Dichlorobenzene | 102% |

VOA SURROGATE RECOVERY SUMMARY



Matrix: Water

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 POS-LLA

| ARI ID | Client ID | PV | DCE | TOL | BFB | DCB | TOT OUT |
|--------|-----------|----|-------|------|-------|------|---------|
| RG58T | PSB22-TB | 5 | 123% | 105% | 95.4% | 104% | 0 |
| RG58U | PSB23-TB | 5 | 127%* | 106% | 94.9% | 103% | 1 |
| RG58V | PSB24-TB | 5 | 126%* | 104% | 97.1% | 102% | 1 |

LCS/MB LIMITS

QC LIMITS

SW8260C

(DCE) = d4-1,2-Dichloroethane
 (TOL) = d8-Toluene
 (BFB) = Bromofluorobenzene
 (DCB) = d4-1,2-Dichlorobenzene

80-122
 80-120
 80-120
 80-120

80-125
 80-120
 80-120
 80-120

Prep Method: SW5030B
 Log Number Range: 10-18255 to 10-18257

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: LCS-080910

Page 1 of 1

LAB CONTROL SAMPLE

Lab Sample ID: LCS-080910

QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18236

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: *[Signature]*

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

Instrument/Analyst LCS: FINN5/PAB

Sample Amount LCS: 5.00 g-dry-wt

LCS: FINN5/PAB

LCS: 5.00 g-dry-wt

Date Analyzed LCS: 08/09/10 11:22

Purge Volume LCS: 5.0 mL

LCS: 08/09/10 11:49

LCS: 5.0 mL

Moisture: NA

| Analyte | LCS | Spike | LCS | LCS | Spike | LCS | RPD |
|--------------------------|------|-----------|----------|------|------------|----------|------|
| | | Added-LCS | Recovery | | Added-LCSD | Recovery | |
| trans-1,2-Dichloroethene | 46.9 | 50.0 | 93.8% | 48.1 | 50.0 | 96.2% | 2.5% |
| cis-1,2-Dichloroethene | 48.1 | 50.0 | 96.2% | 49.3 | 50.0 | 98.6% | 2.5% |
| 1,2-Dichloroethane | 50.6 | 50.0 | 101% | 50.2 | 50.0 | 100% | 0.8% |
| Trichloroethene | 47.4 | 50.0 | 94.8% | 46.8 | 50.0 | 93.6% | 1.3% |
| Tetrachloroethene | 46.2 | 50.0 | 92.4% | 43.3 | 50.0 | 86.6% | 6.5% |

Reported in µg/kg (ppb)

RPD calculated using sample concentrations per SW846.

Volatile Surrogate Recovery

| | LCS | LCS |
|------------------------|-------|-------|
| d4-1,2-Dichloroethane | 92.0% | 110% |
| d8-Toluene | 103% | 105% |
| Bromofluorobenzene | 101% | 101% |
| d4-1,2-Dichlorobenzene | 98.2% | 99.7% |

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: LCS-081010

Page 1 of 1

LAB CONTROL SAMPLE

Lab Sample ID: LCS-081010


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18254

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

Instrument/Analyst LCS: FINN5/PAB

Sample Amount LCS: 5.00 g-dry-wt

LCS: FINN5/PAB

LCS: 5.00 g-dry-wt

Date Analyzed LCS: 08/10/10 11:12

Purge Volume LCS: 5.0 mL

LCS: 08/10/10 11:37

LCS: 5.0 mL

Moisture: NA

| Analyte | LCS | Spike | LCS | LCS | Spike | LCS | RPD |
|--------------------------|------|-----------|----------|------|-----------|----------|-------|
| | | Added-LCS | Recovery | | Added-LCS | Recovery | |
| trans-1,2-Dichloroethene | 51.1 | 50.0 | 102% | 45.9 | 50.0 | 91.8% | 10.7% |
| cis-1,2-Dichloroethene | 52.4 | 50.0 | 105% | 47.7 | 50.0 | 95.4% | 9.4% |
| 1,2-Dichloroethane | 49.3 | 50.0 | 98.6% | 48.2 | 50.0 | 96.4% | 2.3% |
| Trichloroethene | 48.4 | 50.0 | 96.8% | 43.5 | 50.0 | 87.0% | 10.7% |
| Tetrachloroethene | 43.3 | 50.0 | 86.6% | 41.2 | 50.0 | 82.4% | 5.0% |

Reported in µg/kg (ppb)

RPD calculated using sample concentrations per SW846.

Volatile Surrogate Recovery

| | LCS | LCS |
|------------------------|-------|-------|
| d4-1,2-Dichloroethane | 107% | 107% |
| d8-Toluene | 102% | 102% |
| Bromofluorobenzene | 98.5% | 99.2% |
| d4-1,2-Dichlorobenzene | 101% | 102% |

4A
VOLATILE METHOD BLANK SUMMARY

Method Blank ID.

MB0809

Lab Name: ANALYTICAL RESOURCES, INC
 ARI Job No: RG58
 Lab File ID: MB0809
 Date Analyzed: 08/09/10
 Instrument ID: FINN5

Client: FLOYD SNIDER
 Project: LORA LAKE RI
 Lab Sample ID: MB0809
 Time Analyzed: 1216
 Heated Purge: (Y/N) Y

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS and MSD:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | TIME ANALYZED |
|----|-------------------|------------------|----------------|------------------|
| | ===== | ===== | ===== | ===== |
| 01 | LCS0809 | LCS0809 | LCS0809 | 1122 |
| 02 | LCS0809 | LCS0809 | LCS0809A | 1149 |
| 03 | PSB22-0-0.5- | RG58A | RG58A | 1611 |
| 04 | PSB22-1.5-2- | RG58B | RG58B | 1638 |
| 05 | PSB22-2-4-07 | RG58C | RG58C | 1704 |
| 06 | PSB22-4-6-07 | RG58D | RG58D | 1731 |
| 07 | PSB22-17-19- | RG58E | RG58E | 1757 |
| 08 | PSB22-19-20- | RG58F | RG58F | 1824 |
| 09 | PSB23-14-16. | RG58K | RG58K | 1850 |
| 10 | PSB23-16.5-1 | RG58L | RG58L | 1916 |
| 11 | PSB22-TB | RG58T | RG58T | 1943 |
| 12 | PSB23-TB | RG58U | RG58U | 2009 |
| 13 | PSB24-TB | RG58V | RG58V | 2035 |
| 14 | PSB24-14-16- | RG58R | RG58R | 2102 |
| 15 | | | | |
| 16 | | | | |
| 17 | | | | |
| 18 | | | | |
| 19 | | | | |
| 20 | | | | |
| 21 | | | | |
| 22 | | | | |
| 23 | | | | |
| 24 | | | | |
| 25 | | | | |
| 26 | | | | |
| 27 | | | | |
| 28 | | | | |
| 29 | | | | |
| 30 | | | | |

COMMENTS:

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: MB-080910

Page 1 of 1

METHOD BLANK

Lab Sample ID: MB-080910

QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18236

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: *AS*

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

Instrument/Analyst: FINN5/PAB

Sample Amount: 5.00 g-dry-wt

Date Analyzed: 08/09/10 12:16

Purge Volume: 5.0 mL

Moisture: NA

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 107-06-2 | 1,2-Dichloroethane | 1.0 | < 1.0 | U |
| 79-01-6 | Trichloroethene | 1.0 | < 1.0 | U |
| 127-18-4 | Tetrachloroethene | 1.0 | < 1.0 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 118% |
| d8-Toluene | 104% |
| Bromofluorobenzene | 96.7% |
| d4-1,2-Dichlorobenzene | 101% |

4A
VOLATILE METHOD BLANK SUMMARY

Method Blank ID.

MB0810

Lab Name: ANALYTICAL RESOURCES, INC
 ARI Job No: RG58
 Lab File ID: MB0810
 Date Analyzed: 08/10/10
 Instrument ID: FINN5

Client: FLOYD SNIDER
 Project: LORA LAKE RI
 Lab Sample ID: MB0810
 Time Analyzed: 1206
 Heated Purge: (Y/N) Y

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS and MSD:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | TIME ANALYZED |
|----|-------------------|------------------|----------------|------------------|
| | ===== | ===== | ===== | ===== |
| 01 | LCS0810 | LCS0810 | LCS0810 | 1112 |
| 02 | LCS0810 | LCS0810 | LCS0810A | 1137 |
| 03 | PSB24-16-17- | RG58S | RG58S2 | 1235 |
| 04 | | | | |
| 05 | | | | |
| 06 | | | | |
| 07 | | | | |
| 08 | | | | |
| 09 | | | | |
| 10 | | | | |
| 11 | | | | |
| 12 | | | | |
| 13 | | | | |
| 14 | | | | |
| 15 | | | | |
| 16 | | | | |
| 17 | | | | |
| 18 | | | | |
| 19 | | | | |
| 20 | | | | |
| 21 | | | | |
| 22 | | | | |
| 23 | | | | |
| 24 | | | | |
| 25 | | | | |
| 26 | | | | |
| 27 | | | | |
| 28 | | | | |
| 29 | | | | |
| 30 | | | | |

COMMENTS:

ORGANICS ANALYSIS DATA SHEET

Volatiles by Purge & Trap GC/MS-Method SW8260C

Sample ID: MB-081010

Page 1 of 1

METHOD BLANK

Lab Sample ID: MB-081010


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18254

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

Instrument/Analyst: FINN5/PAB

Sample Amount: 5.00 g-dry-wt

Date Analyzed: 08/10/10 12:06

Purge Volume: 5.0 mL

Moisture: NA

| CAS Number | Analyte | RL | Result | Q |
|------------|--------------------------|-----|--------|---|
| 156-60-5 | trans-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 156-59-2 | cis-1,2-Dichloroethene | 1.0 | < 1.0 | U |
| 107-06-2 | 1,2-Dichloroethane | 1.0 | < 1.0 | U |
| 79-01-6 | Trichloroethene | 1.0 | < 1.0 | U |
| 127-18-4 | Tetrachloroethene | 1.0 | < 1.0 | U |

Reported in µg/kg (ppb)

Volatile Surrogate Recovery

| | |
|------------------------|-------|
| d4-1,2-Dichloroethane | 105% |
| d8-Toluene | 102% |
| Bromofluorobenzene | 93.1% |
| d4-1,2-Dichlorobenzene | 100% |

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: ANALYTICAL RESOURCES, INC Contract: FLOYD SNIDER

Lab Code: ARI Case No.: LORA LAKE RI SDG No.: RG58

Lab File ID: BFB07231

BFB Injection Date: 07/23/10

Instrument ID: FINN5

BFB Injection Time: 1648

GC Column: RTX502.2 ID: 0.18 (mm)

Heated Purge: (Y/N) N

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 50 | 8.0 - 40.0% of mass 95 | 24.7 |
| 75 | 30.0 - 66.0% of mass 95 | 49.1 |
| 95 | Base Peak, 100% relative abundance | 100.0 |
| 96 | 5.0 - 9.0% of mass 95 | 7.1 |
| 173 | Less than 2.0% of mass 174 | 0.2 (0.2)1 |
| 174 | 50.0 - 101.0% of mass 95 | 77.4 |
| 175 | 4.0 - 9.0% of mass 174 | 5.7 (7.4)1 |
| 176 | 93.0 - 101.0% of mass 174 | 76.4 (98.8)1 |
| 177 | 5.0 - 9.0% of mass 176 | 5.5 (7.2)2 |

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------|---------------|-------------|---------------|---------------|
| 01 | VSTD200 | IC0723 | 2000723 | 07/23/10 | 1718 |
| 02 | VSTD150 | IC0723 | 1500723 | 07/23/10 | 1749 |
| 03 | VSTD100 | IC0723 | 1000723 | 07/23/10 | 1816 |
| 04 | VSTD050 | IC0723 | 0500723 | 07/23/10 | 1842 |
| 05 | VSTD010 | IC0723 | 0100723 | 07/23/10 | 1909 |
| 06 | VSTD005 | IC0723 | 0050723 | 07/23/10 | 1935 |
| 07 | VSTD002 | IC0723 | 0020723 | 07/23/10 | 2002 |
| 08 | VSTD001 | IC0723 | 0010723 | 07/23/10 | 2028 |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: ANALYTICAL RESOURCES, INC Contract: FLOYD SNIDER

Lab Code: ARI Case No.: LORA LAKE RI SDG No.: RG58

Lab File ID: BFB0809 BFB Injection Date: 08/09/10

Instrument ID: FINN5 BFB Injection Time: 0918

GC Column: RTX502.2 ID: 0.18 (mm) Heated Purge: (Y/N) N

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 50 | 8.0 - 40.0% of mass 95 | 26.4 |
| 75 | 30.0 - 66.0% of mass 95 | 50.4 |
| 95 | Base Peak, 100% relative abundance | 100.0 |
| 96 | 5.0 - 9.0% of mass 95 | 6.8 |
| 173 | Less than 2.0% of mass 174 | 0.1 (0.2)1 |
| 174 | 50.0 - 101.0% of mass 95 | 69.1 |
| 175 | 4.0 - 9.0% of mass 174 | 5.1 (7.4)1 |
| 176 | 93.0 - 101.0% of mass 174 | 69.5 (100.5)1 |
| 177 | 5.0 - 9.0% of mass 176 | 4.4 (6.3)2 |

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|-------------------|------------------|----------------|------------------|------------------|
| 01 | VSTD050 | CC0809 | 0500809 | 08/09/10 | 1035 |
| 02 | LCS0809 | LCS0809 | LCS0809 | 08/09/10 | 1122 |
| 03 | LCS0809 | LCS0809 | LCS0809A | 08/09/10 | 1149 |
| 04 | MB0809 | MB0809 | MB0809 | 08/09/10 | 1216 |
| 05 | PSB22-0-0.5-0729 | RG58A | RG58A | 08/09/10 | 1611 |
| 06 | PSB22-1.5-2-0729 | RG58B | RG58B | 08/09/10 | 1638 |
| 07 | PSB22-2-4-072910 | RG58C | RG58C | 08/09/10 | 1704 |
| 08 | PSB22-4-6-072910 | RG58D | RG58D | 08/09/10 | 1731 |
| 09 | PSB22-17-19-0729 | RG58E | RG58E | 08/09/10 | 1757 |
| 10 | PSB22-19-20-0729 | RG58F | RG58F | 08/09/10 | 1824 |
| 11 | PSB23-14-16.5-07 | RG58K | RG58K | 08/09/10 | 1850 |
| 12 | PSB23-16.5-19-07 | RG58L | RG58L | 08/09/10 | 1916 |
| 13 | PSB22-TB | RG58T | RG58T | 08/09/10 | 1943 |
| 14 | PSB23-TB | RG58U | RG58U | 08/09/10 | 2009 |
| 15 | PSB24-TB | RG58V | RG58V | 08/09/10 | 2035 |
| 16 | PSB24-14-16-0729 | RG58R | RG58R | 08/09/10 | 2102 |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: ANALYTICAL RESOURCES, INC Contract: FLOYD SNIDER

Lab Code: ARI Case No.: LORA LAKE RI SDG No.: RG58

Lab File ID: BFB0810 BFB Injection Date: 08/10/10

Instrument ID: FINN5 BFB Injection Time: 0846

GC Column: RTX502.2 ID: 0.18 (mm) Heated Purge: (Y/N) N

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 50 | 8.0 - 40.0% of mass 95 | 26.7 |
| 75 | 30.0 - 66.0% of mass 95 | 49.8 |
| 95 | Base Peak, 100% relative abundance | 100.0 |
| 96 | 5.0 - 9.0% of mass 95 | 6.9 |
| 173 | Less than 2.0% of mass 174 | 0.2 (0.2)1 |
| 174 | 50.0 - 101.0% of mass 95 | 70.4 |
| 175 | 4.0 - 9.0% of mass 174 | 5.1 (7.3)1 |
| 176 | 93.0 - 101.0% of mass 174 | 68.3 (97.0)1 |
| 177 | 5.0 - 9.0% of mass 176 | 4.5 (6.6)2 |

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|------------------|---------------|-------------|---------------|---------------|
| 01 | VSTD050 | CC0810 | 0500810A | 08/10/10 | 1038 |
| 02 | LCS0810 | LCS0810 | LCS0810 | 08/10/10 | 1112 |
| 03 | LCS0810 | LCS0810 | LCS0810A | 08/10/10 | 1137 |
| 04 | MB0810 | MB0810 | MB0810 | 08/10/10 | 1206 |
| 05 | PSB24-16-17-0729 | RG58S | RG58S2 | 08/10/10 | 1235 |
| 06 | | | | | |
| 07 | | | | | |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF1: 0010723

RF2: 0020723

RF5: 0050723

RF10: 0100723

RF50: 0500723

| COMPOUND | RF1 | RF2 | RF5 | RF10 | RF50 |
|------------------------------|-------|-------|-------|-------|-------|
| Chloromethane | 2.155 | 1.962 | 1.917 | 2.009 | 1.652 |
| Vinyl Chloride | 1.519 | 1.452 | 1.513 | 1.597 | 1.363 |
| Bromomethane | 0.934 | 0.851 | 0.777 | 0.625 | 0.810 |
| Chloroethane | 1.071 | 1.093 | 0.988 | 0.871 | 0.876 |
| Trichlorofluoromethane | 1.476 | 1.559 | 1.505 | 1.410 | 1.426 |
| Acrolein | 0.205 | 0.197 | 0.177 | 0.164 | 0.157 |
| 112Trichloro122Trifluoroetha | 1.274 | 1.182 | 1.204 | 1.123 | 1.014 |
| Acetone | 0.308 | 0.320 | 0.314 | 0.301 | 0.268 |
| 1,1-Dichloroethene | 1.036 | 1.019 | 1.041 | 1.032 | 0.979 |
| Bromoethane | 0.707 | 0.744 | 0.729 | 0.753 | 0.727 |
| Iodomethane | 1.011 | 1.066 | 1.142 | 1.140 | 1.253 |
| Methylene Chloride | | 1.396 | 1.190 | 1.128 | 0.935 |
| Acrylonitrile | 0.196 | 0.243 | 0.283 | 0.285 | 0.261 |
| Carbon Disulfide | 3.372 | 3.310 | 3.395 | 3.282 | 3.176 |
| Trans-1,2-Dichloroethene | 0.815 | 0.825 | 0.806 | 0.895 | 0.794 |
| Vinyl Acetate | 1.378 | 1.475 | 1.529 | 1.560 | 1.561 |
| 1,1-Dichloroethane | 1.593 | 1.577 | 1.616 | 1.674 | 1.534 |
| 2-Butanone | 0.326 | 0.330 | 0.344 | 0.353 | 0.328 |
| 2,2-Dichloropropane | 0.887 | 0.897 | 0.933 | 0.951 | 0.913 |
| Cis-1,2-Dichloroethene | 0.703 | 0.702 | 0.718 | 0.759 | 0.692 |
| Chloroform | 1.249 | 1.296 | 1.316 | 1.320 | 1.203 |
| Bromochloromethane | 0.301 | 0.323 | 0.367 | 0.357 | 0.335 |
| 1,1,1-Trichloroethane | 0.977 | 0.934 | 0.973 | 0.985 | 0.933 |
| 1,1-Dichloropropene | 0.670 | 0.690 | 0.712 | 0.765 | 0.673 |
| Carbon Tetrachloride | 0.581 | 0.624 | 0.604 | 0.630 | 0.570 |
| 1,2-Dichloroethane | 0.571 | 0.629 | 0.633 | 0.678 | 0.586 |
| Benzene | 1.759 | 1.768 | 1.800 | 1.965 | 1.656 |
| Trichloroethene | 0.436 | 0.500 | 0.510 | 0.540 | 0.468 |
| 1,2-Dichloropropane | 0.524 | 0.521 | 0.548 | 0.582 | 0.501 |
| Bromodichloromethane | 0.521 | 0.592 | 0.582 | 0.604 | 0.542 |
| Dibromomethane | 0.253 | 0.259 | 0.260 | 0.288 | 0.249 |
| 2-Chloroethyl Vinyl Ether | | 0.142 | 0.173 | 0.190 | 0.185 |
| 4-Methyl-2-Pentanone | 0.141 | 0.137 | 0.132 | 0.143 | 0.133 |
| Cis 1,3-dichloropropene | 0.503 | 0.566 | 0.600 | 0.660 | 0.638 |
| Toluene | 1.257 | 1.104 | 1.022 | 1.052 | 0.921 |
| Trans 1,3-Dichloropropene | 0.446 | 0.472 | 0.491 | 0.540 | 0.521 |
| 2-Hexanone | 0.489 | 0.418 | 0.404 | 0.438 | 0.381 |

FORM VI VOA

RG58 : 00051

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF1: 0010723

RF2: 0020723

RF5: 0050723

RF10: 0100723

RF50: 0500723

| COMPOUND | RF1 | RF2 | RF5 | RF10 | RF50 |
|-----------------------------|-------|-------|-------|-------|-------|
| 1,1,2-Trichloroethane | 0.269 | 0.295 | 0.323 | 0.339 | 0.296 |
| 1,3-Dichloropropane | 0.683 | 0.714 | 0.715 | 0.756 | 0.678 |
| Tetrachloroethene | 0.617 | 0.527 | 0.565 | 0.567 | 0.490 |
| Chlorodibromomethane | 0.427 | 0.440 | 0.465 | 0.502 | 0.453 |
| 1,2-Dibromoethane | 0.301 | 0.328 | 0.338 | 0.349 | 0.322 |
| Chlorobenzene | 1.449 | 1.256 | 1.215 | 1.285 | 1.093 |
| Ethyl Benzene | 2.203 | 2.176 | 2.088 | 2.268 | 2.021 |
| 1,1,1,2-Tetrachloroethane | 0.488 | 0.463 | 0.438 | 0.454 | 0.389 |
| m,p-xylene | 0.686 | 0.701 | 0.756 | 0.820 | 0.768 |
| o-Xylene | 0.597 | 0.672 | 0.700 | 0.773 | 0.750 |
| Styrene | 1.013 | 1.042 | 1.151 | 1.321 | 1.228 |
| Bromoform | 0.588 | 0.562 | 0.563 | 0.584 | 0.521 |
| 1,1,2,2-Tetrachloroethane | 1.199 | 1.124 | 1.036 | 1.126 | 0.917 |
| 1,2,3-Trichloropropane | | 0.226 | 0.221 | 0.226 | 0.186 |
| Trans-1,4-Dichloro 2-Butene | | 0.322 | 0.326 | 0.349 | 0.301 |
| N-Propyl Benzene | 4.356 | 4.362 | 4.593 | 5.132 | 4.292 |
| Bromobenzene | 0.977 | 0.937 | 0.972 | 1.058 | 0.917 |
| Isopropyl Benzene | 3.581 | 3.464 | 3.670 | 4.080 | 3.636 |
| 2-Chloro Toluene | 3.123 | 2.806 | 3.073 | 3.372 | 2.810 |
| 4-Chloro Toluene | 2.626 | 2.911 | 2.880 | 3.298 | 2.959 |
| T-Butyl Benzene | 2.255 | 2.386 | 2.573 | 2.864 | 2.638 |
| 1,3,5-Trimethyl Benzene | 2.663 | 2.667 | 2.918 | 3.226 | 2.998 |
| 1,2,4-Trimethylbenzene | 2.438 | 2.545 | 2.851 | 3.260 | 2.948 |
| S-Butyl Benzene | 3.651 | 3.689 | 3.984 | 4.454 | 4.031 |
| 4-Isopropyl Toluene | 2.226 | 2.542 | 2.823 | 3.180 | 2.946 |
| 1,3-Dichlorobenzene | 1.562 | 1.533 | 1.674 | 1.912 | 1.646 |
| 1,4-Dichlorobenzene | 1.655 | 1.573 | 1.702 | 1.839 | 1.597 |
| N-Butyl Benzene | 2.810 | 2.765 | 3.045 | 3.430 | 3.102 |
| 1,2-Dichlorobenzene | 1.537 | 1.602 | 1.638 | 1.750 | 1.517 |
| 1,2-Dibromo 3-Chloropropane | 0.152 | 0.209 | 0.190 | 0.200 | 0.171 |
| 1,2,4-Trichlorobenzene | 0.965 | 1.017 | 0.971 | 1.126 | 0.860 |
| Hexachloro 1,3-Butadiene | 0.585 | 0.688 | 0.689 | 0.751 | 0.589 |
| Naphthalene | 1.716 | 1.756 | 1.742 | 2.094 | 1.618 |
| 1,2,3-Trichlorobenzene | 0.961 | 1.020 | 0.960 | 1.136 | 0.809 |
| Dichlorodifluoromethane | 0.618 | 0.692 | 0.660 | 0.633 | 0.675 |
| Methyl tert-Butyl Ether | 1.392 | 1.482 | 1.616 | 1.631 | 1.525 |

FORM VI VOA

RG58 : 00052

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF1: 0010723

RF2: 0020723

RF5: 0050723

RF10: 0100723

RF50: 0500723

| COMPOUND | RF1 | RF2 | RF5 | RF10 | RF50 |
|------------------------|-------|-------|-------|-------|-------|
| d4-1,2-Dichloroethane | 0.718 | 0.705 | 0.687 | 0.646 | 0.643 |
| d8-Toluene | 1.123 | 1.149 | 1.122 | 1.106 | 1.114 |
| 4-Bromofluorobenzene | 0.550 | 0.557 | 0.558 | 0.551 | 0.566 |
| d4-1,2-Dichlorobenzene | 0.929 | 0.920 | 0.920 | 0.926 | 0.925 |
| Dibromofluoromethane | 0.649 | 0.629 | 0.614 | 0.586 | 0.599 |

FORM VI VOA

RG58: 00053

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF100: 1000723

RF150: 1500723

RF200: 2000723

| COMPOUND | RF100 | RF150 | RF200 |
|-------------------------------------|-------|-------|-------|
| Chloromethane | 1.566 | 1.388 | 1.306 |
| Vinyl Chloride | 1.358 | 1.171 | 1.061 |
| Bromomethane | 0.769 | 0.647 | 0.579 |
| Chloroethane | 0.778 | 0.629 | |
| Trichlorofluoromethane | 1.280 | 1.042 | 0.967 |
| Acrolein | 0.146 | 0.119 | |
| 1,1,2-Trichloro-2,2-Trifluoroethane | 0.976 | 0.818 | 0.758 |
| Acetone | 0.244 | 0.204 | |
| 1,1-Dichloroethene | 0.934 | 0.797 | 0.739 |
| Bromoethane | 0.727 | 0.633 | 0.591 |
| Iodomethane | 1.256 | 1.066 | 1.025 |
| Methylene Chloride | 0.929 | 0.821 | |
| Acrylonitrile | 0.258 | 0.230 | 0.220 |
| Carbon Disulfide | 2.867 | 2.186 | 1.913 |
| Trans-1,2-Dichloroethene | 0.835 | 0.766 | 0.722 |
| Vinyl Acetate | 1.554 | 1.197 | 1.056 |
| 1,1-Dichloroethane | 1.561 | 1.255 | 1.069 |
| 2-Butanone | 0.323 | 0.268 | 0.247 |
| 2,2-Dichloropropane | 0.956 | 0.876 | 0.855 |
| Cis-1,2-Dichloroethene | 0.742 | 0.687 | 0.690 |
| Chloroform | 1.234 | 1.073 | 0.959 |
| Bromochloromethane | 0.351 | 0.332 | 0.335 |
| 1,1,1-Trichloroethane | 0.962 | 0.878 | 0.863 |
| 1,1-Dichloropropene | 0.695 | 0.631 | 0.596 |
| Carbon Tetrachloride | 0.592 | 0.551 | 0.570 |
| 1,2-Dichloroethane | 0.598 | 0.544 | 0.529 |
| Benzene | 1.455 | 1.088 | |
| Trichloroethene | 0.485 | 0.448 | 0.461 |
| 1,2-Dichloropropane | 0.518 | 0.470 | 0.475 |
| Bromodichloromethane | 0.555 | 0.516 | 0.514 |
| Dibromomethane | 0.260 | 0.237 | 0.249 |
| 2-Chloroethyl Vinyl Ether | 0.194 | 0.187 | 0.198 |
| 4-Methyl-2-Pentanone | 0.132 | 0.122 | 0.117 |
| Cis 1,3-dichloropropene | 0.676 | 0.620 | 0.570 |
| Toluene | 0.946 | 0.783 | 0.707 |
| Trans 1,3-Dichloropropene | 0.559 | 0.524 | 0.508 |
| 2-Hexanone | 0.322 | | |

FORM VI VOA

RG58 : 00054

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF100: 1000723

RF150: 1500723

RF200: 2000723

| COMPOUND | RF100 | RF150 | RF200 |
|-----------------------------|-------|-------|-------|
| 1,1,2-Trichloroethane | 0.308 | 0.291 | 0.306 |
| 1,3-Dichloropropane | 0.724 | 0.676 | 0.684 |
| Tetrachloroethene | 0.546 | 0.543 | 0.590 |
| Chlorodibromomethane | 0.493 | 0.479 | 0.528 |
| 1,2-Dibromoethane | 0.328 | 0.309 | 0.324 |
| Chlorobenzene | 1.173 | 0.982 | 0.930 |
| Ethyl Benzene | 1.784 | 1.342 | |
| 1,1,1,2-Tetrachloroethane | 0.428 | 0.439 | 0.492 |
| m,p-xylene | 0.804 | 0.647 | 0.616 |
| o-Xylene | 0.840 | 0.828 | 0.865 |
| Styrene | 1.342 | 1.127 | 1.094 |
| Bromoform | 0.539 | 0.500 | 0.474 |
| 1,1,2,2-Tetrachloroethane | 0.890 | 0.780 | 0.707 |
| 1,2,3-Trichloropropane | 0.183 | 0.160 | 0.146 |
| Trans-1,4-Dichloro 2-Butene | 0.299 | 0.258 | 0.237 |
| N-Propyl Benzene | 3.334 | | |
| Bromobenzene | 0.956 | 0.872 | 0.817 |
| Isopropyl Benzene | 3.053 | 2.076 | |
| 2-Chloro Toluene | 2.821 | 1.980 | |
| 4-Chloro Toluene | 2.626 | 1.857 | |
| T-Butyl Benzene | 2.560 | 1.958 | 1.463 |
| 1,3,5-Trimethyl Benzene | 2.733 | 1.921 | |
| 1,2,4-Trimethylbenzene | 2.800 | 1.985 | |
| S-Butyl Benzene | 3.263 | | |
| 4-Isopropyl Toluene | 2.747 | 2.006 | |
| 1,3-Dichlorobenzene | 1.804 | 1.479 | 1.214 |
| 1,4-Dichlorobenzene | 1.775 | 1.484 | 1.208 |
| N-Butyl Benzene | 2.846 | 1.945 | |
| 1,2-Dichlorobenzene | 1.586 | 1.401 | 1.156 |
| 1,2-Dibromo 3-Chloropropane | 0.158 | 0.137 | 0.128 |
| 1,2,4-Trichlorobenzene | 0.913 | 0.825 | 0.739 |
| Hexachloro 1,3-Butadiene | 0.597 | 0.554 | 0.542 |
| Naphthalene | 1.558 | 1.287 | |
| 1,2,3-Trichlorobenzene | 0.822 | 0.736 | 0.646 |
| Dichlorodifluoromethane | 0.674 | 0.632 | 0.601 |
| Methyl tert-Butyl Ether | 1.542 | 1.313 | 1.151 |

FORM VI VOA

RG58 : 00055

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

LAB FILE ID: RF100: 1000723

RF150: 1500723

RF200: 2000723

| COMPOUND | RF100 | RF150 | RF200 |
|------------------------|-------|-------|-------|
| d4-1,2-Dichloroethane | 0.641 | 0.617 | 0.560 |
| d8-Toluene | 1.080 | 1.048 | 1.047 |
| 4-Bromofluorobenzene | 0.592 | 0.613 | 0.695 |
| d4-1,2-Dichlorobenzene | 0.902 | 0.880 | 0.873 |
| Dibromofluoromethane | 0.586 | 0.572 | 0.533 |

FORM VI VOA

RG58 : 00056

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

| COMPOUND | CURVE TYPE | AVE RF | %RSD OR R ² |
|---------------------------------------|------------|--------|------------------------|
| Chloromethane | AVRG | 1.744 | 17.8 |
| Vinyl Chloride | AVRG | 1.379 | 13.3 |
| Bromomethane | AVRG | 0.749 | 16.3 |
| Chloroethane | AVRG | 0.901 | 18.3 |
| Trichlorofluoromethane | AVRG | 1.333 | 16.4 |
| Acrolein | AVRG | 0.166 | 17.8 |
| 1,1,2-Trichloro-1,2,2-Trifluoroethane | AVRG | 1.044 | 17.8 |
| Acetone | AVRG | 0.280 | 15.4 |
| 1,1-Dichloroethene | AVRG | 0.947 | 12.4 |
| Bromoethane | AVRG | 0.701 | 8.2 |
| Iodomethane | AVRG | 1.120 | 8.5 |
| Methylene Chloride | AVRG | 1.066 | 19.9 |
| Acrylonitrile | AVRG | 0.247 | 12.5 |
| Carbon Disulfide | AVRG | 2.938 | 19.6 |
| Trans-1,2-Dichloroethene | AVRG | 0.807 | 6.3 |
| Vinyl Acetate | AVRG | 1.414 | 13.5 |
| 1,1-Dichloroethane | AVRG | 1.485 | 14.1 |
| 2-Butanone | AVRG | 0.315 | 11.8 |
| 2,2-Dichloropropane | AVRG | 0.909 | 4.0 |
| Cis-1,2-Dichloroethene | AVRG | 0.711 | 3.7 |
| Chloroform | AVRG | 1.206 | 10.6 |
| Bromochloromethane | AVRG | 0.338 | 6.1 |
| 1,1,1-Trichloroethane | AVRG | 0.938 | 4.9 |
| 1,1-Dichloropropene | AVRG | 0.679 | 7.5 |
| Carbon Tetrachloride | AVRG | 0.590 | 4.7 |
| 1,2-Dichloroethane | AVRG | 0.596 | 8.3 |
| Benzene | AVRG | 1.642 | 17.6 |
| Trichloroethene | AVRG | 0.481 | 7.2 |
| 1,2-Dichloropropane | AVRG | 0.518 | 7.1 |
| Bromodichloromethane | AVRG | 0.553 | 6.5 |
| Dibromomethane | AVRG | 0.257 | 5.7 |
| 2-Chloroethyl Vinyl Ether | AVRG | 0.181 | 10.5 |
| 4-Methyl-2-Pentanone | AVRG | 0.132 | 6.7 |
| Cis 1,3-dichloropropene | AVRG | 0.604 | 9.4 |
| Toluene | AVRG | 0.974 | 18.0 |
| Trans 1,3-Dichloropropene | AVRG | 0.508 | 7.2 |
| 2-Hexanone | AVRG | 0.409 | 13.6 |

<- Indicates value outside QC limits:
(%RSD < 20% or R² > 0.990)

FORM VI VOA

RG58 : 00057

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC
ARI Job No: RG58
Instrument ID: FINN5

Client: FLOYD SNIDER
Project: LORA LAKE RI
Calibration Date: 07/23/10

| COMPOUND | CURVE TYPE | AVE RF | %RSD OR R ² |
|-----------------------------|------------|--------|------------------------|
| ===== | ===== | ===== | ===== |
| 1,1,2-Trichloroethane | AVRG | 0.303 | 7.0 |
| 1,3-Dichloropropane | AVRG | 0.704 | 4.0 |
| Tetrachloroethene | AVRG | 0.556 | 7.0 |
| Chlorodibromomethane | AVRG | 0.473 | 7.2 |
| 1,2-Dibromoethane | AVRG | 0.325 | 4.7 |
| Chlorobenzene | AVRG | 1.173 | 14.4 |
| Ethyl Benzene | AVRG | 1.983 | 16.3 |
| 1,1,1,2-Tetrachloroethane | AVRG | 0.449 | 7.4 |
| m,p-xylene | AVRG | 0.725 | 10.2 |
| o-Xylene | AVRG | 0.753 | 12.3 |
| Styrene | AVRG | 1.165 | 10.5 |
| Bromoform | AVRG | 0.541 | 7.5 |
| 1,1,2,2-Tetrachloroethane | AVRG | 0.972 | 18.2 |
| 1,2,3-Trichloropropane | AVRG | 0.193 | 17.0 |
| Trans-1,4-Dichloro 2-Butene | AVRG | 0.299 | 13.1 |
| N-Propyl Benzene | AVRG | 4.345 | 13.4 |
| Bromobenzene | AVRG | 0.938 | 7.7 |
| Isopropyl Benzene | AVRG | 3.366 | 19.2 |
| 2-Chloro Toluene | AVRG | 2.855 | 15.4 |
| 4-Chloro Toluene | AVRG | 2.736 | 16.4 |
| T-Butyl Benzene | AVRG | 2.337 | 19.1 |
| 1,3,5-Trimethyl Benzene | AVRG | 2.732 | 15.0 |
| 1,2,4-Trimethylbenzene | AVRG | 2.690 | 15.2 |
| S-Butyl Benzene | AVRG | 3.845 | 10.6 |
| 4-Isopropyl Toluene | AVRG | 2.638 | 15.6 |
| 1,3-Dichlorobenzene | AVRG | 1.603 | 13.2 |
| 1,4-Dichlorobenzene | AVRG | 1.604 | 12.2 |
| N-Butyl Benzene | AVRG | 2.849 | 16.1 |
| 1,2-Dichlorobenzene | AVRG | 1.523 | 11.8 |
| 1,2-Dibromo 3-Chloropropane | AVRG | 0.168 | 17.6 |
| 1,2,4-Trichlorobenzene | AVRG | 0.927 | 13.0 |
| Hexachloro 1,3-Butadiene | AVRG | 0.624 | 12.0 |
| Naphthalene | AVRG | 1.682 | 14.5 |
| 1,2,3-Trichlorobenzene | AVRG | 0.886 | 18.2 |
| Dichlorodifluoromethane | AVRG | 0.648 | 4.8 |
| Methyl tert-Butyl Ether | AVRG | 1.456 | 11.2 |
| ===== | ===== | ===== | ===== |

<- Indicates value outside QC limits:
(%RSD < 20% or R² > 0.990)

FORM 6
VOLATILE INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Calibration Date: 07/23/10

| COMPOUND | CURVE TYPE | AVE RF | %RSD OR R ² |
|------------------------|------------|--------|------------------------|
| d4-1,2-Dichloroethane | AVRG | 0.652 | 7.8 |
| d8-Toluene | AVRG | 1.099 | 3.4 |
| 4-Bromofluorobenzene | AVRG | 0.585 | 8.5 |
| d4-1,2-Dichlorobenzene | AVRG | 0.909 | 2.4 |
| Dibromofluoromethane | AVRG | 0.596 | 6.0 |

<- Indicates value outside QC limits:
(%RSD < 20% or R² > 0.990)

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/09/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1035

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|---------------------------------------|------------------|-----------------|------------|---------------|----------------|
| Chloromethane | 1.744 | 1.269 | 0.100 | AVRG | -27.2 |
| Vinyl Chloride | 1.379 | 1.147 | 0.010 | AVRG | -16.8 |
| Bromomethane | 0.749 | 0.862 | 0.010 | AVRG | 15.1 |
| Chloroethane | 0.901 | 0.771 | 0.010 | AVRG | -14.4 |
| Trichlorofluoromethane | 1.333 | 1.222 | 0.010 | AVRG | -8.3 |
| Acrolein | 0.166 | 0.136 | 0.010 | AVRG | -18.1 |
| 1,1,2-Trichloro-1,2,2-Trifluoroethane | 1.044 | 0.917 | 0.010 | AVRG | -12.2 |
| Acetone | 0.280 | 0.244 | 0.010 | AVRG | -12.8 |
| 1,1-Dichloroethene | 0.947 | 0.818 | 0.010 | AVRG | -13.6 |
| Bromoethane | 0.701 | 0.607 | 0.010 | AVRG | -13.4 |
| Iodomethane | 1.120 | 1.167 | 0.010 | AVRG | 4.2 |
| Methylene Chloride | 1.066 | 0.784 | 0.010 | AVRG | -26.4 |
| Acrylonitrile | 0.247 | 0.227 | 0.010 | AVRG | -8.1 |
| Carbon Disulfide | 2.938 | 2.736 | 0.010 | AVRG | -6.9 |
| Trans-1,2-Dichloroethene | 0.807 | 0.686 | 0.010 | AVRG | -15.0 |
| Vinyl Acetate | 1.414 | 1.374 | 0.010 | AVRG | -2.8 |
| 1,1-Dichloroethane | 1.485 | 1.330 | 0.100 | AVRG | -10.4 |
| 2-Butanone | 0.315 | 0.287 | 0.010 | AVRG | -8.9 |
| 2,2-Dichloropropane | 0.908 | 0.820 | 0.010 | AVRG | -9.7 |
| Cis-1,2-Dichloroethene | 0.712 | 0.624 | 0.010 | AVRG | -12.4 |
| Chloroform | 1.206 | 1.048 | 0.010 | AVRG | -13.1 |
| Bromochloromethane | 0.338 | 0.290 | 0.010 | AVRG | -14.2 |
| 1,1,1-Trichloroethane | 0.938 | 0.802 | 0.010 | AVRG | -14.5 |
| 1,1-Dichloropropene | 0.679 | 0.620 | 0.010 | AVRG | -8.7 |
| Carbon Tetrachloride | 0.590 | 0.505 | 0.010 | AVRG | -14.4 |
| 1,2-Dichloroethane | 0.596 | 0.533 | 0.010 | AVRG | -10.6 |
| Benzene | 1.642 | 1.487 | 0.010 | AVRG | -9.4 |
| Trichloroethene | 0.481 | 0.423 | 0.010 | AVRG | -12.0 |
| 1,2-Dichloropropane | 0.517 | 0.438 | 0.010 | AVRG | -15.3 |
| Bromodichloromethane | 0.553 | 0.494 | 0.010 | AVRG | -10.7 |
| Dibromomethane | 0.257 | 0.229 | 0.010 | AVRG | -10.9 |
| 2-Chloroethyl Vinyl Ether | 0.181 | 0.180 | 0.010 | AVRG | -0.6 |
| 4-Methyl-2-Pentanone | 0.132 | 0.116 | 0.010 | AVRG | -12.1 |
| Cis 1,3-dichloropropene | 0.604 | 0.572 | 0.010 | AVRG | -5.3 |
| Toluene | 0.974 | 0.835 | 0.010 | AVRG | -14.3 |
| Trans 1,3-Dichloropropene | 0.508 | 0.474 | 0.010 | AVRG | -6.7 |
| 2-Hexanone | 0.409 | 0.332 | 0.010 | AVRG | -18.8 |

<- Exceeds QC limit of 20% D
* RF less than minimum RF

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/09/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1035

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|-----------------------------|------------------|-----------------|------------|---------------|----------------|
| ===== | ===== | ===== | ===== | ===== | ===== |
| 1,1,2-Trichloroethane | 0.303 | 0.263 | 0.010 | AVRG | -13.2 |
| 1,3-Dichloropropane | 0.704 | 0.605 | 0.010 | AVRG | -14.1 |
| Tetrachloroethene | 0.556 | 0.465 | 0.010 | AVRG | -16.4 |
| Chlorodibromomethane | 0.473 | 0.392 | 0.010 | AVRG | -17.1 |
| 1,2-Dibromoethane | 0.325 | 0.290 | 0.010 | AVRG | -10.8 |
| Chlorobenzene | 1.173 | 1.005 | 0.300 | AVRG | -14.3 |
| Ethyl Benzene | 1.983 | 1.868 | 0.010 | AVRG | -5.8 |
| 1,1,1,2-Tetrachloroethane | 0.449 | 0.343 | 0.010 | AVRG | -23.6 |
| m,p-xylene | 0.725 | 0.711 | 0.010 | AVRG | -1.9 |
| o-Xylene | 0.753 | 0.690 | 0.010 | AVRG | -8.4 |
| Styrene | 1.165 | 1.130 | 0.010 | AVRG | -3.0 |
| Bromoform | 0.541 | 0.459 | 0.100 | AVRG | -15.2 |
| 1,1,2,2-Tetrachloroethane | 0.972 | 0.803 | 0.300 | AVRG | -17.4 |
| 1,2,3-Trichloropropane | 0.192 | 0.166 | 0.010 | AVRG | -13.5 |
| Trans-1,4-Dichloro 2-Butene | 0.299 | 0.291 | 0.010 | AVRG | -2.7 |
| N-Propyl Benzene | 4.345 | 4.340 | 0.010 | AVRG | -0.1 |
| Bromobenzene | 0.938 | 0.827 | 0.010 | AVRG | -11.8 |
| Isopropyl Benzene | 3.366 | 3.479 | 0.010 | AVRG | 3.4 |
| 2-Chloro Toluene | 2.855 | 2.799 | 0.010 | AVRG | -2.0 |
| 4-Chloro Toluene | 2.737 | 2.778 | 0.010 | AVRG | 1.5 |
| T-Butyl Benzene | 2.337 | 2.546 | 0.010 | AVRG | 8.9 |
| 1,3,5-Trimethyl Benzene | 2.732 | 2.900 | 0.010 | AVRG | 6.1 |
| 1,2,4-Trimethylbenzene | 2.690 | 2.912 | 0.010 | AVRG | 8.2 |
| S-Butyl Benzene | 3.845 | 3.919 | 0.010 | AVRG | 1.9 |
| 4-Isopropyl Toluene | 2.638 | 3.007 | 0.010 | AVRG | 14.0 |
| 1,3-Dichlorobenzene | 1.603 | 1.620 | 0.010 | AVRG | 1.1 |
| 1,4-Dichlorobenzene | 1.604 | 1.612 | 0.010 | AVRG | 0.5 |
| N-Butyl Benzene | 2.849 | 3.323 | 0.010 | AVRG | 16.6 |
| 1,2-Dichlorobenzene | 1.523 | 1.436 | 0.010 | AVRG | -5.7 |
| 1,2-Dibromo 3-Chloropropane | 0.168 | 0.147 | 0.010 | AVRG | -12.5 |
| 1,2,4-Trichlorobenzene | 0.927 | 0.941 | 0.010 | AVRG | 1.5 |
| Hexachloro 1,3-Butadiene | 0.624 | 0.607 | 0.010 | AVRG | -2.7 |
| Naphthalene | 1.682 | 1.525 | 0.010 | AVRG | -9.3 |
| 1,2,3-Trichlorobenzene | 0.886 | 0.787 | 0.010 | AVRG | -11.2 |
| Dichlorodifluoromethane | 0.648 | 0.548 | 0.010 | AVRG | -15.4 |
| Methyl tert-Butyl Ether | 1.456 | 1.302 | 0.010 | AVRG | -10.6 |
| ===== | ===== | ===== | ===== | ===== | ===== |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/09/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1035

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|------------------------|------------------|-----------------|------------|---------------|----------------|
| ===== | ===== | ===== | ===== | ===== | ===== |
| d4-1,2-Dichloroethane | 0.652 | 0.616 | 0.010 | AVRG | -5.5 |
| d8-Toluene | 1.099 | 1.167 | 0.010 | AVRG | 6.2 |
| 4-Bromofluorobenzene | 0.585 | 0.571 | 0.010 | AVRG | -2.4 |
| d4-1,2-Dichlorobenzene | 0.909 | 0.867 | 0.010 | AVRG | -4.6 |
| Dibromofluoromethane | 0.596 | 0.568 | 0.010 | AVRG | -4.7 |

<- Exceeds QC limit of 20% D
* RF less than minimum RF

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/10/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1038

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|------------------------------|------------------|-----------------|------------|---------------|----------------|
| Chloromethane | 1.744 | 1.422 | 0.100 | AVRG | -18.5 |
| Vinyl Chloride | 1.379 | 1.345 | 0.010 | AVRG | -2.5 |
| Bromomethane | 0.749 | 1.041 | 0.010 | AVRG | 39.0 <- |
| Chloroethane | 0.901 | 0.899 | 0.010 | AVRG | -0.2 |
| Trichlorofluoromethane | 1.333 | 1.246 | 0.010 | AVRG | -6.5 |
| Acrolein | 0.166 | 0.158 | 0.010 | AVRG | -4.8 |
| 112Trichloro122Trifluoroetha | 1.044 | 1.036 | 0.010 | AVRG | -0.8 |
| Acetone | 0.280 | 0.265 | 0.010 | AVRG | -5.4 |
| 1,1-Dichloroethene | 0.947 | 0.853 | 0.010 | AVRG | -9.9 |
| Bromoethane | 0.701 | 0.568 | 0.010 | AVRG | -19.0 |
| Iodomethane | 1.120 | 0.800 | 0.010 | AVRG | -28.6 <- |
| Methylene Chloride | 1.066 | 0.920 | 0.010 | AVRG | -13.7 |
| Acrylonitrile | 0.247 | 0.255 | 0.010 | AVRG | 3.2 |
| Carbon Disulfide | 2.938 | 2.398 | 0.010 | AVRG | -18.4 |
| Trans-1,2-Dichloroethene | 0.807 | 0.780 | 0.010 | AVRG | -3.3 |
| Vinyl Acetate | 1.414 | 1.507 | 0.010 | AVRG | 6.6 |
| 1,1-Dichloroethane | 1.485 | 1.479 | 0.100 | AVRG | -0.4 |
| 2-Butanone | 0.315 | 0.330 | 0.010 | AVRG | 4.8 |
| 2,2-Dichloropropane | 0.908 | 0.809 | 0.010 | AVRG | -10.9 |
| Cis-1,2-Dichloroethene | 0.712 | 0.696 | 0.010 | AVRG | -2.2 |
| Chloroform | 1.206 | 1.170 | 0.010 | AVRG | -3.0 |
| Bromochloromethane | 0.338 | 0.309 | 0.010 | AVRG | -8.6 |
| 1,1,1-Trichloroethane | 0.938 | 0.838 | 0.010 | AVRG | -10.7 |
| 1,1-Dichloropropene | 0.679 | 0.671 | 0.010 | AVRG | -1.2 |
| Carbon Tetrachloride | 0.590 | 0.537 | 0.010 | AVRG | -9.0 |
| 1,2-Dichloroethane | 0.596 | 0.585 | 0.010 | AVRG | -1.8 |
| Benzene | 1.642 | 1.652 | 0.010 | AVRG | 0.6 |
| Trichloroethene | 0.481 | 0.470 | 0.010 | AVRG | -2.3 |
| 1,2-Dichloropropane | 0.517 | 0.491 | 0.010 | AVRG | -5.0 |
| Bromodichloromethane | 0.553 | 0.538 | 0.010 | AVRG | -2.7 |
| Dibromomethane | 0.257 | 0.256 | 0.010 | AVRG | -0.4 |
| 2-Chloroethyl Vinyl Ether | 0.181 | 0.202 | 0.010 | AVRG | 11.6 |
| 4-Methyl-2-Pentanone | 0.132 | 0.128 | 0.010 | AVRG | -3.0 |
| Cis 1,3-dichloropropene | 0.604 | 0.623 | 0.010 | AVRG | 3.1 |
| Toluene | 0.974 | 0.932 | 0.010 | AVRG | -4.3 |
| Trans 1,3-Dichloropropene | 0.508 | 0.497 | 0.010 | AVRG | -2.2 |
| 2-Hexanone | 0.409 | 0.385 | 0.010 | AVRG | -5.9 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/10/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1038

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|-----------------------------|------------------|-----------------|------------|---------------|----------------|
| 1,1,2-Trichloroethane | 0.303 | 0.303 | 0.010 | AVRG | 0.0 |
| 1,3-Dichloropropane | 0.704 | 0.710 | 0.010 | AVRG | 0.8 |
| Tetrachloroethene | 0.556 | 0.530 | 0.010 | AVRG | -4.7 |
| Chlorodibromomethane | 0.473 | 0.458 | 0.010 | AVRG | -3.2 |
| 1,2-Dibromoethane | 0.325 | 0.320 | 0.010 | AVRG | -1.5 |
| Chlorobenzene | 1.173 | 1.148 | 0.300 | AVRG | -2.1 |
| Ethyl Benzene | 1.983 | 2.121 | 0.010 | AVRG | 7.0 |
| 1,1,1,2-Tetrachloroethane | 0.449 | 0.381 | 0.010 | AVRG | -15.1 |
| m,p-xylene | 0.725 | 0.816 | 0.010 | AVRG | 12.6 |
| o-Xylene | 0.753 | 0.783 | 0.010 | AVRG | 4.0 |
| Styrene | 1.165 | 1.305 | 0.010 | AVRG | 12.0 |
| Bromoform | 0.541 | 0.515 | 0.100 | AVRG | -4.8 |
| 1,1,2,2-Tetrachloroethane | 0.972 | 0.931 | 0.300 | AVRG | -4.2 |
| 1,2,3-Trichloropropane | 0.192 | 0.186 | 0.010 | AVRG | -3.1 |
| Trans-1,4-Dichloro 2-Butene | 0.299 | 0.344 | 0.010 | AVRG | 15.0 |
| N-Propyl Benzene | 4.345 | 4.795 | 0.010 | AVRG | 10.4 |
| Bromobenzene | 0.938 | 0.943 | 0.010 | AVRG | 0.5 |
| Isopropyl Benzene | 3.366 | 3.805 | 0.010 | AVRG | 13.0 |
| 2-Chloro Toluene | 2.855 | 2.994 | 0.010 | AVRG | 4.9 |
| 4-Chloro Toluene | 2.737 | 3.342 | 0.010 | AVRG | 22.1 <- |
| T-Butyl Benzene | 2.337 | 2.752 | 0.010 | AVRG | 17.8 |
| 1,3,5-Trimethyl Benzene | 2.732 | 3.234 | 0.010 | AVRG | 18.4 |
| 1,2,4-Trimethylbenzene | 2.690 | 3.218 | 0.010 | AVRG | 19.6 |
| S-Butyl Benzene | 3.845 | 4.393 | 0.010 | AVRG | 14.2 |
| 4-Isopropyl Toluene | 2.638 | 3.319 | 0.010 | AVRG | 25.8 <- |
| 1,3-Dichlorobenzene | 1.603 | 1.849 | 0.010 | AVRG | 15.3 |
| 1,4-Dichlorobenzene | 1.604 | 1.830 | 0.010 | AVRG | 14.1 |
| N-Butyl Benzene | 2.849 | 3.714 | 0.010 | AVRG | 30.4 <- |
| 1,2-Dichlorobenzene | 1.523 | 1.652 | 0.010 | AVRG | 8.5 |
| 1,2-Dibromo 3-Chloropropane | 0.168 | 0.162 | 0.010 | AVRG | -3.6 |
| 1,2,4-Trichlorobenzene | 0.927 | 1.076 | 0.010 | AVRG | 16.1 |
| Hexachloro 1,3-Butadiene | 0.624 | 0.669 | 0.010 | AVRG | 7.2 |
| Naphthalene | 1.682 | 1.754 | 0.010 | AVRG | 4.3 |
| 1,2,3-Trichlorobenzene | 0.886 | 0.927 | 0.010 | AVRG | 4.6 |
| Dichlorodifluoromethane | 0.648 | 0.592 | 0.010 | AVRG | -8.6 |
| Methyl tert-Butyl Ether | 1.456 | 1.268 | 0.010 | AVRG | -12.9 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Instrument ID: FINN5

Cont. Calib. Date: 08/10/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1038

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|------------------------|------------------|-----------------|------------|---------------|----------------|
| ===== | ===== | ===== | ===== | ===== | ===== |
| d4-1,2-Dichloroethane | 0.652 | 0.593 | 0.010 | AVRG | -9.0 |
| d8-Toluene | 1.099 | 1.125 | 0.010 | AVRG | 2.4 |
| 4-Bromofluorobenzene | 0.585 | 0.580 | 0.010 | AVRG | -0.8 |
| d4-1,2-Dichlorobenzene | 0.909 | 0.904 | 0.010 | AVRG | -0.6 |
| Dibromofluoromethane | 0.596 | 0.546 | 0.010 | AVRG | -8.4 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

8A
VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Ical Midpoint ID: 0500723

Ical Date: 07/23/10

Instrument ID: FINN5

Project Run Date: 08/09/10

| | IS1 (PFB) AREA # | RT # | IS2 (DFB) AREA # | RT # | IS3 (CLB) AREA # | RT # |
|-----------------|---------------------|------|---------------------|------|---------------------|-------|
| ICAL MIDPT | 131115 | 6.62 | 191559 | 7.63 | 161199 | 10.78 |
| UPPER LIMIT | 262230 | 7.12 | 383118 | 8.13 | 322398 | 11.28 |
| LOWER LIMIT | 65558 | 6.12 | 95780 | 7.13 | 80600 | 10.28 |
| Sample ID | | | | | | |
| 01 LCS0809 | 103776 | 6.62 | 147372 | 7.64 | 120524 | 10.78 |
| 02 LCS0809 | 106566 | 6.63 | 157864 | 7.64 | 135479 | 10.79 |
| 03 MB0809 | 95082 | 6.61 | 136899 | 7.63 | 118413 | 10.77 |
| 04 PSB22-0-0.5- | 163926 | 6.62 | 239062 | 7.63 | 194173 | 10.78 |
| 05 PSB22-1.5-2- | 141403 | 6.63 | 209666 | 7.65 | 174438 | 10.79 |
| 06 PSB22-2-4-07 | 123053 | 6.62 | 179902 | 7.64 | 151011 | 10.78 |
| 07 PSB22-4-6-07 | 114044 | 6.62 | 169449 | 7.64 | 144305 | 10.78 |
| 08 PSB22-17-19- | 110155 | 6.63 | 166411 | 7.65 | 149317 | 10.79 |
| 09 PSB22-19-20- | 103536 | 6.63 | 156457 | 7.65 | 137444 | 10.79 |
| 10 PSB23-14-16. | 104622 | 6.62 | 159024 | 7.64 | 137738 | 10.78 |
| 11 PSB23-16.5-1 | 100728 | 6.62 | 154377 | 7.63 | 139039 | 10.78 |
| 12 PSB22-TB | 97416 | 6.61 | 148990 | 7.63 | 126813 | 10.77 |
| 13 PSB23-TB | 100027 | 6.62 | 154248 | 7.64 | 136628 | 10.78 |
| 14 PSB24-TB | 100981 | 6.62 | 154524 | 7.64 | 131451 | 10.78 |
| 15 PSB24-14-16- | 101772 | 6.63 | 157962 | 7.64 | 139242 | 10.79 |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |

IS1 (PFB) = Pentafluorobenzene
 IS2 (DFB) = 1,4-Difluorobenzene
 IS3 (CLB) = d5-Chlorobenzene

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Ical midpoint
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Ical midpoint

* Values outside of QC limits.

8A
VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Ical Midpoint ID: 0500723

Ical Date: 07/23/10

Instrument ID: FINN5

Project Run Date: 08/09/10

| | IS4 (DCB) AREA # | RT # | AREA # | RT # | AREA # | RT # |
|-----------------|---------------------|-------|--------|-------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 88279 | 13.47 | | | | |
| UPPER LIMIT | 176558 | 13.97 | | | | |
| LOWER LIMIT | 44140 | 12.97 | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Sample ID | | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| 01 LCS0809 | 65104 | 13.47 | | | | |
| 02 LCS0809 | 75648 | 13.47 | | | | |
| 03 MB0809 | 58588 | 13.46 | | | | |
| 04 PSB22-0-0.5- | 95238 | 13.46 | | | | |
| 05 PSB22-1.5-2- | 83991 | 13.48 | | | | |
| 06 PSB22-2-4-07 | 75393 | 13.47 | | | | |
| 07 PSB22-4-6-07 | 70759 | 13.47 | | | | |
| 08 PSB22-17-19- | 78068 | 13.48 | | | | |
| 09 PSB22-19-20- | 73064 | 13.48 | | | | |
| 10 PSB23-14-16. | 67417 | 13.47 | | | | |
| 11 PSB23-16.5-1 | 72259 | 13.46 | | | | |
| 12 PSB22-TB | 61537 | 13.46 | | | | |
| 13 PSB23-TB | 65693 | 13.47 | | | | |
| 14 PSB24-TB | 64680 | 13.47 | | | | |
| 15 PSB24-14-16- | 70424 | 13.47 | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |

IS4 (DCB) = d4-1,4-Dichlorobenzene

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint

AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint

RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Ical midpoint

RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Ical midpoint

* Values outside of QC limits.

8A
VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Ical Midpoint ID: 0500723

Ical Date: 07/23/10

Instrument ID: FINN5

Project Run Date: 08/10/10

| | IS1 (PFB) AREA # | RT # | IS2 (DFB) AREA # | RT # | IS3 (CLB) AREA # | RT # |
|-----------------|---------------------|-------|---------------------|-------|---------------------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 131115 | 6.62 | 191559 | 7.63 | 161199 | 10.78 |
| UPPER LIMIT | 262230 | 7.12 | 383118 | 8.13 | 322398 | 11.28 |
| LOWER LIMIT | 65558 | 6.12 | 95780 | 7.13 | 80600 | 10.28 |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Sample ID | | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| 01 LCS0810 | 113963 | 6.63 | 170822 | 7.65 | 146772 | 10.79 |
| 02 LCS0810 | 120686 | 6.63 | 178947 | 7.64 | 146633 | 10.79 |
| 03 MB0810 | 114844 | 6.62 | 162120 | 7.64 | 136524 | 10.78 |
| 04 PSB24-16-17- | 109057 | 6.62 | 158794 | 7.63 | 136121 | 10.78 |
| 05 | | | | | | |
| 06 | | | | | | |
| 07 | | | | | | |
| 08 | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |

IS1 (PFB) = Pentafluorobenzene
 IS2 (DFB) = 1,4-Difluorobenzene
 IS3 (CLB) = d5-Chlorobenzene

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Ical midpoint
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Ical midpoint

* Values outside of QC limits.

8A
VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD SNIDER

ARI Job No: RG58

Project: LORA LAKE RI

Ical Midpoint ID: 0500723

Ical Date: 07/23/10

Instrument ID: FINN5

Project Run Date: 08/10/10

| | IS4 (DCB) AREA # | RT # | AREA # | RT # | AREA # | RT # |
|-----------------|---------------------|-------|--------|-------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 88279 | 13.47 | | | | |
| UPPER LIMIT | 176558 | 13.97 | | | | |
| LOWER LIMIT | 44140 | 12.97 | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Sample ID | | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| 01 LCS0810 | 80742 | 13.48 | | | | |
| 02 LCS0810 | 78163 | 13.47 | | | | |
| 03 MB0810 | 66691 | 13.47 | | | | |
| 04 PSB24-16-17- | 67577 | 13.46 | | | | |
| 05 | | | | | | |
| 06 | | | | | | |
| 07 | | | | | | |
| 08 | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |

IS4 (DCB) = d4-1,4-Dichlorobenzene

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Ical midpoint
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Ical midpoint

* Values outside of QC limits.

**Semivolatile PAH Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB22-0-0.5-072910

SAMPLE

Lab Sample ID: RG58A

LIMS ID: 10-18236

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 20:11

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.4 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 5.1%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 89.2% |
| 2-Fluorobiphenyl | 75.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB22-1.5-2-072910

SAMPLE

Lab Sample ID: RG58B

LIMS ID: 10-18237

Matrix: Soil

Data Release Authorized: *B*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 20:44

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.2 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.2%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 81.2% |
| 2-Fluorobiphenyl | 68.8% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB22-2-4-072910

SAMPLE

Lab Sample ID: RG58C

LIMS ID: 10-18238

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 21:16

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.7 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 9.2%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 88.4% |
| 2-Fluorobiphenyl | 74.4% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB22-4-6-072910

SAMPLE

Lab Sample ID: RG58D

LIMS ID: 10-18239

Matrix: Soil

Data Release Authorized: *AS*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 21:49

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.6 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 8.7%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 96.0% |
| 2-Fluorobiphenyl | 80.4% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB22-17-19-072910

SAMPLE

Lab Sample ID: RG58E

LIMS ID: 10-18240

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 22:22

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.4 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 12.9%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 90.0% |
| 2-Fluorobiphenyl | 71.6% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB22-19-20-072910

SAMPLE

Lab Sample ID: RG58F

LIMS ID: 10-18241

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 22:55

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.9 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 16.8%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 88.4% |
| 2-Fluorobiphenyl | 74.0% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-0-0.5-072910

SAMPLE

Lab Sample ID: RG58G

LIMS ID: 10-18242

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 12:19

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.1 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 6.5%

| CAS Number | Analyte | RL | Result |
|-----------------|---------------------------------|-----------|-------------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | 12 J |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | 18 J |

Reported in µg/kg (ppb)

Semivolatle Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 51.2% |
| 2-Fluorobiphenyl | 62.4% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB23-1.5-2-072910

SAMPLE

Lab Sample ID: RG58H

LIMS ID: 10-18243

Matrix: Soil

Data Release Authorized: *B*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 21:06

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.2 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.2%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 81.2% |
| 2-Fluorobiphenyl | 73.6% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1




Sample ID: PSB23-2-4-072910

SAMPLE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/17/10 19:33

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.4 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 80.0% |
| 2-Fluorobiphenyl | 77.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB23-4-6-072910

SAMPLE

Lab Sample ID: RG58J

LIMS ID: 10-18245

Matrix: Soil

Data Release Authorized: *AB*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 17:16

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.1 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 3.5%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 65.6% |
| 2-Fluorobiphenyl | 73.6% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-14-16.5-072910

SAMPLE

Lab Sample ID: RG58K

LIMS ID: 10-18246

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 17:49

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.2 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 10.4%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo (a) anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo (a) pyrene | 20 | < 20 U |
| 193-39-5 | Indeno (1,2,3-cd) pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz (a,h) anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 83.6% |
| 2-Fluorobiphenyl | 68.4% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-16.5-19-072910

SAMPLE

Lab Sample ID: RG58L

LIMS ID: 10-18247

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 18:22

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.1 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 13.8%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 82.8% |
| 2-Fluorobiphenyl | 66.8% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB24-0-0.5-072910

SAMPLE

Lab Sample ID: RG58M

LIMS ID: 10-18248

Matrix: Soil

Data Release Authorized: *AB*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 18:55

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.1 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 4.8%

| CAS Number | Analyte | RL | Result |
|---------------|---------------------------------|-----------|-------------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | 12 J |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 59.2% |
| 2-Fluorobiphenyl | 66.4% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB24-1.5-2-072910

SAMPLE

Lab Sample ID: RG58N

LIMS ID: 10-18249

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 19:28

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.5 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 6.3%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 78.4% |
| 2-Fluorobiphenyl | 69.2% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB24-2-4-072910

SAMPLE

Lab Sample ID: RG580

LIMS ID: 10-18250

Matrix: Soil

Data Release Authorized: *AS*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 20:00

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.2 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.4%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatiles Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 84.0% |
| 2-Fluorobiphenyl | 72.0% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB24-2-4-072910-D

SAMPLE

Lab Sample ID: RG58P

LIMS ID: 10-18251

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 20:33

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.4 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.6%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 78.8% |
| 2-Fluorobiphenyl | 65.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1



Sample ID: PSB24-4-6-072910

SAMPLE

Lab Sample ID: RG58Q

LIMS ID: 10-18252

Matrix: Soil

Data Release Authorized: *B*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 12:52

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 26.4 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.5%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 82.4% |
| 2-Fluorobiphenyl | 66.0% |

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1

Sample ID: PSB24-14-16-072910

SAMPLE

Lab Sample ID: RG58R

LIMS ID: 10-18253

Matrix: Soil

Data Release Authorized: *[Signature]*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 21:38

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.9 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 10.8%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 79.6% |
| 2-Fluorobiphenyl | 65.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB24-16-17-072910

SAMPLE

Lab Sample ID: RG58S

LIMS ID: 10-18254

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 22:11

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.8 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 12.7%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | < 19 U |
| 218-01-9 | Chrysene | 19 | < 19 U |
| 50-32-8 | Benzo(a)pyrene | 19 | < 19 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | < 19 U |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | < 19 U |
| TOTBFA | Total Benzofluoranthenes | 19 | < 19 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 79.6% |
| 2-Fluorobiphenyl | 65.2% |

SW8270 PNA SURROGATE RECOVERY SUMMARY

Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

| <u>Client ID</u> | <u>TER</u> | <u>FBP</u> | <u>TOT OUT</u> |
|----------------------|------------|------------|----------------|
| PSB22-0-0.5-072910 | 89.2% | 75.6% | 0 |
| PSB22-1.5-2-072910 | 81.2% | 68.8% | 0 |
| PSB22-2-4-072910 | 88.4% | 74.4% | 0 |
| PSB22-4-6-072910 | 96.0% | 80.4% | 0 |
| PSB22-17-19-072910 | 90.0% | 71.6% | 0 |
| PSB22-19-20-072910 | 88.4% | 74.0% | 0 |
| PSB23-0-0.5-072910 | 51.2% | 62.4% | 0 |
| PSB23-1.5-2-072910 | 81.2% | 73.6% | 0 |
| MB-081110 | 88.0% | 71.2% | 0 |
| LCS-081110 | 98.0% | 70.4% | 0 |
| PSB23-2-4-072910 | 80.0% | 77.6% | 0 |
| PSB23-2-4-072910 MS | 85.2% | 73.6% | 0 |
| PSB23-2-4-072910 MSD | 83.2% | 71.6% | 0 |
| PSB23-4-6-072910 | 65.6% | 73.6% | 0 |
| PSB23-14-16.5-072910 | 83.6% | 68.4% | 0 |
| PSB23-16.5-19-072910 | 82.8% | 66.8% | 0 |
| PSB24-0-0.5-072910 | 59.2% | 66.4% | 0 |
| PSB24-1.5-2-072910 | 78.4% | 69.2% | 0 |
| PSB24-2-4-072910 | 84.0% | 72.0% | 0 |
| PSB24-2-4-072910-D | 78.8% | 65.6% | 0 |
| PSB24-4-6-072910 | 82.4% | 66.0% | 0 |
| PSB24-14-16-072910 | 79.6% | 65.6% | 0 |
| PSB24-16-17-072910 | 79.6% | 65.2% | 0 |

LCS/MB LIMITS QC LIMITS

(TER) = d14-p-Terphenyl (47-112) (35-112)
(FBP) = 2-Fluorobiphenyl (40-100) (34-100)

Prep Method: SW3550C
Log Number Range: 10-18236 to 10-18254

ORGANICS ANALYSIS DATA SHEET

PNA's by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-2-4-072910

MS/MSD

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted MS/MSD: 08/11/10

Sample Amount MS: 25.5 g-dry-wt

MSD: 25.8 g-dry-wt

Date Analyzed MS: 08/14/10 15:37

Final Extract Volume MS: 0.5 mL

MSD: 08/14/10 16:10

MSD: 0.5 mL

Instrument/Analyst MS: NT6/JZ

Dilution Factor MS: 1.00

MSD: NT6/JZ

MSD: 1.00

GPC Cleanup: No

Alumina Cleanup: No

Silica Gel Cleanup: Yes

| Analyte | Sample | MS | Spike Added-MS | MS Recovery | MSD | Spike Added-MSD | MSD Recovery | RPD |
|--------------------------|--------|-----|-------------------|----------------|-----|--------------------|-----------------|------|
| Benzo(a)anthracene | < 19.7 | 354 | 490 | 72.2% | 355 | 484 | 73.3% | 0.3% |
| Chrysene | < 19.7 | 351 | 490 | 71.6% | 344 | 484 | 71.1% | 2.0% |
| Benzo(a)pyrene | < 19.7 | 298 | 490 | 60.8% | 292 | 484 | 60.3% | 2.0% |
| Indeno(1,2,3-cd)pyrene | < 19.7 | 320 | 490 | 65.3% | 312 | 484 | 64.5% | 2.5% |
| Dibenz(a,h)anthracene | < 19.7 | 327 | 490 | 66.7% | 318 | 484 | 65.7% | 2.8% |
| Total Benzofluoranthenes | < 19.7 | 664 | 490 | 136% | 655 | 484 | 135% | 1.4% |

Results reported in µg/kg

RPD calculated using sample concentrations per SW846.

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-2-4-072910

MATRIX SPIKE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 15:37

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.5 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | --- |
| 218-01-9 | Chrysene | 20 | --- |
| 50-32-8 | Benzo(a)pyrene | 20 | --- |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | --- |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | --- |
| TOTBFA | Total Benzofluoranthenes | 20 | --- |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 85.2% |
| 2-Fluorobiphenyl | 73.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: PSB23-2-4-072910

MATRIX SPIKE DUPLICATE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/14/10 16:10

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.8 g-dry-wt

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 19 | --- |
| 218-01-9 | Chrysene | 19 | --- |
| 50-32-8 | Benzo(a)pyrene | 19 | --- |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 19 | --- |
| 53-70-3 | Dibenz(a,h)anthracene | 19 | --- |
| TOTBFA | Total Benzofluoranthenes | 19 | --- |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 83.2% |
| 2-Fluorobiphenyl | 71.6% |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1


Sample ID: LCS-081110

LAB CONTROL

Lab Sample ID: LCS-081110

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: NA

Date Received: 07/29/10

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 19:38

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Silica Gel Cleanup: Yes

Sample Amount: 25.0 g-dry-wt

Final Extract Volume: 0.50 mL

Dilution Factor: 1.00

Alumina Cleanup: No

| Analyte | Lab Control | Spike Added | Recovery |
|--------------------------|-------------|-------------|----------|
| Benzo(a)anthracene | 381 | 500 | 76.2% |
| Chrysene | 377 | 500 | 75.4% |
| Benzo(a)pyrene | 324 | 500 | 64.8% |
| Indeno(1,2,3-cd)pyrene | 216 | 500 | 43.2% |
| Dibenz(a,h)anthracene | 228 | 500 | 45.6% |
| Total Benzofluoranthenes | 943 U | 1000 | 94.3% |

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| dl4-p-Terphenyl | 98.0% |
| 2-Fluorobiphenyl | 70.4% |

Results reported in µg/kg

4B
SEMIVOLATILE METHOD BLANK SUMMARY

BLANK NO.

RG58MBS1

Lab Name: ANALYTICAL RESOURCES, INC
 ARI Job No: RG58
 Lab File ID: 08131005
 Instrument ID: NT6
 Matrix: SOLID

Client: FLOYD/SNIDER
 Project: LORA LAKE RI
 Date Extracted: 08/11/10
 Date Analyzed: 08/13/10
 Time Analyzed: 1336

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS and MSD:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED |
|----|----------------------|------------------|----------------|------------------|
| | ===== | ===== | ===== | ===== |
| 01 | RG58LCSS1 | RG58LCSS1 | 08131016 | 08/13/10 |
| 02 | PSB22-0-0.5-0729 | RG58A | 08131017 | 08/13/10 |
| 03 | PSB22-1.5-2-0729 | RG58B | 08131018 | 08/13/10 |
| 04 | PSB22-2-4-072910 | RG58C | 08131019 | 08/13/10 |
| 05 | PSB22-4-6-072910 | RG58D | 08131020 | 08/13/10 |
| 06 | PSB22-17-19-0729 | RG58E | 08131021 | 08/13/10 |
| 07 | PSB22-19-20-0729 | RG58F | 08131022 | 08/13/10 |
| 08 | PSB23-0-0.5-0729 | RG58G | 08141002 | 08/14/10 |
| 09 | PSB24-4-6-072910 | RG58Q | 08141003 | 08/14/10 |
| 10 | PSB23-2-4-07291 | RG58IMS | 08141006 | 08/14/10 |
| 11 | PSB23-2-4-07291 | RG58IMSD | 08141007 | 08/14/10 |
| 12 | PSB23-4-6-072910 | RG58J | 08141009 | 08/14/10 |
| 13 | PSB23-14-16.5-07 | RG58K | 08141010 | 08/14/10 |
| 14 | PSB23-16.5-19-07 | RG58L | 08141011 | 08/14/10 |
| 15 | PSB24-0-0.5-0729 | RG58M | 08141012 | 08/14/10 |
| 16 | PSB24-1.5-2-0729 | RG58N | 08141013 | 08/14/10 |
| 17 | PSB24-2-4-072910 | RG58O | 08141014 | 08/14/10 |
| 18 | PSB24-2-4-072910 | RG58P | 08141015 | 08/14/10 |
| 19 | PSB23-1.5-2-0729 | RG58H | 08141016 | 08/14/10 |
| 20 | PSB24-14-16-0729 | RG58R | 08141017 | 08/14/10 |
| 21 | PSB24-16-17-0729 | RG58S | 08141018 | 08/14/10 |
| 22 | PSB23-2-4-072910 | RG58I | 08171018 | 08/17/10 |
| 23 | _____ | _____ | _____ | _____ |
| 24 | _____ | _____ | _____ | _____ |
| 25 | _____ | _____ | _____ | _____ |
| 26 | _____ | _____ | _____ | _____ |
| 27 | _____ | _____ | _____ | _____ |
| 28 | _____ | _____ | _____ | _____ |
| 29 | _____ | _____ | _____ | _____ |
| 30 | _____ | _____ | _____ | _____ |

ORGANICS ANALYSIS DATA SHEET

PNAs by SW8270D GC/MS

Page 1 of 1

Sample ID: MB-081110

METHOD BLANK

Lab Sample ID: MB-081110

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: *AB*

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: NA

Date Received: NA

Date Extracted: 08/11/10

Date Analyzed: 08/13/10 13:36

Instrument/Analyst: NT6/JZ

GPC Cleanup: No

Alumina: No

Silica Gel: Yes

Sample Amount: 25.0 g

Final Extract Volume: 0.5 mL

Dilution Factor: 1.00

Percent Moisture: NA

| CAS Number | Analyte | RL | Result |
|------------|--------------------------|----|--------|
| 56-55-3 | Benzo(a)anthracene | 20 | < 20 U |
| 218-01-9 | Chrysene | 20 | < 20 U |
| 50-32-8 | Benzo(a)pyrene | 20 | < 20 U |
| 193-39-5 | Indeno(1,2,3-cd)pyrene | 20 | < 20 U |
| 53-70-3 | Dibenz(a,h)anthracene | 20 | < 20 U |
| TOTBFA | Total Benzofluoranthenes | 20 | < 20 U |

Reported in µg/kg (ppb)

Semivolatile Surrogate Recovery

| | |
|------------------|-------|
| d14-p-Terphenyl | 88.0% |
| 2-Fluorobiphenyl | 71.2% |

5B
 SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
 DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

Instrument ID: NT6

Project: LORA LAKE RI

DFTPP Injection Date: 07/23/10

DFTPP Injection Time: 1501

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 51 | 10.0 - 80.0% of mass 198 | 32.8 |
| 68 | Less than 2.0% of mass 69 | 0.0 (0.0)1 |
| 69 | Mass 69 relative abundance | 39.4 |
| 70 | Less than 2.0% of mass 69 | 0.1 (0.3)1 |
| 127 | 10.0 - 80.0% of mass 198 | 50.5 |
| 197 | Less than 2.0% of mass 198 | 0.0 |
| 198 | Base Peak, 100% relative abundance | 100.0 |
| 199 | 5.0 to 9.0% of mass 198 | 7.4 |
| 275 | 10.0 - 60.0% of mass 198 | 26.8 |
| 365 | Greater than 1.0% of mass 198 | 3.26 |
| 441 | 0.0 - 24.0% of mass 442 | 10.5 (15.1)2 |
| 442 | 50.0 - 200.0% of mass 198 | 69.5 |
| 443 | 15.0 - 24.0% of mass 442 | 14.4 (20.7)2 |

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------------|------------------|----------------|------------------|------------------|
| 01 | IC250723 | IC250723 | 07231001 | 07/23/10 | 1501 |
| 02 | IC010723 | IC010723 | 07231002 | 07/23/10 | 1538 |
| 03 | IC050723 | IC050723 | 07231003 | 07/23/10 | 1616 |
| 04 | IC100723 | IC100723 | 07231004 | 07/23/10 | 1652 |
| 05 | IC400723 | IC400723 | 07231005 | 07/23/10 | 1729 |
| 06 | IC600723 | IC600723 | 07231006 | 07/23/10 | 1801 |
| 07 | IC800723 | IC800723 | 07231007 | 07/23/10 | 1838 |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

5B
SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

Instrument ID: NT6

Project: LORA LAKE RI

DFTPP Injection Date: 08/13/10

DFTPP Injection Time: 1124

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 51 | 10.0 - 80.0% of mass 198 | 31.3 |
| 68 | Less than 2.0% of mass 69 | 0.0 (0.0)1 |
| 69 | Mass 69 relative abundance | 37.6 |
| 70 | Less than 2.0% of mass 69 | 0.3 (0.9)1 |
| 127 | 10.0 - 80.0% of mass 198 | 49.6 |
| 197 | Less than 2.0% of mass 198 | 0.0 |
| 198 | Base Peak, 100% relative abundance | 100.0 |
| 199 | 5.0 to 9.0% of mass 198 | 7.1 |
| 275 | 10.0 - 60.0% of mass 198 | 26.9 |
| 365 | Greater than 1.0% of mass 198 | 2.89 |
| 441 | 0.0 - 24.0% of mass 442 | 11.2 (14.5)2 |
| 442 | 50.0 - 200.0% of mass 198 | 77.1 |
| 443 | 15.0 - 24.0% of mass 442 | 15.6 (20.2)2 |

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------------|------------------|----------------|------------------|------------------|
| 01 | CC0813 | CC0813 | 08131001 | 08/13/10 | 1124 |
| 02 | RG58MBS1 | RG58MBS1 | 08131005 | 08/13/10 | 1336 |
| 03 | RG58LCSS1 | RG58LCSS1 | 08131016 | 08/13/10 | 1938 |
| 04 | PSB22-0-0.5-0729 | RG58A | 08131017 | 08/13/10 | 2011 |
| 05 | PSB22-1.5-2-0729 | RG58B | 08131018 | 08/13/10 | 2044 |
| 06 | PSB22-2-4-072910 | RG58C | 08131019 | 08/13/10 | 2116 |
| 07 | PSB22-4-6-072910 | RG58D | 08131020 | 08/13/10 | 2149 |
| 08 | PSB22-17-19-0729 | RG58E | 08131021 | 08/13/10 | 2222 |
| 09 | PSB22-19-20-0729 | RG58F | 08131022 | 08/13/10 | 2255 |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

5B
SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

Instrument ID: NT6

Project: LORA LAKE RI

DFTPP Injection Date: 08/14/10

DFTPP Injection Time: 1145

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 51 | 10.0 - 80.0% of mass 198 | 30.7 |
| 68 | Less than 2.0% of mass 69 | 0.0 (0.0)1 |
| 69 | Mass 69 relative abundance | 38.4 |
| 70 | Less than 2.0% of mass 69 | 0.3 (0.7)1 |
| 127 | 10.0 - 80.0% of mass 198 | 48.3 |
| 197 | Less than 2.0% of mass 198 | 0.0 |
| 198 | Base Peak, 100% relative abundance | 100.0 |
| 199 | 5.0 to 9.0% of mass 198 | 7.1 |
| 275 | 10.0 - 60.0% of mass 198 | 27.5 |
| 365 | Greater than 1.0% of mass 198 | 3.25 |
| 441 | 0.0 - 24.0% of mass 442 | 11.5 (14.4)2 |
| 442 | 50.0 - 200.0% of mass 198 | 80.4 |
| 443 | 15.0 - 24.0% of mass 442 | 15.9 (19.7)2 |

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------------|------------------|----------------|------------------|------------------|
| 01 | CC0814 | CC0814 | 08141001 | 08/14/10 | 1145 |
| 02 | PSB23-0-0.5-0729 | RG58G | 08141002 | 08/14/10 | 1219 |
| 03 | PSB24-4-6-072910 | RG58Q | 08141003 | 08/14/10 | 1252 |
| 04 | PSB23-2-4-07291 | RG58IMS | 08141006 | 08/14/10 | 1537 |
| 05 | PSB23-2-4-07291 | RG58IMSD | 08141007 | 08/14/10 | 1610 |
| 06 | PSB23-4-6-072910 | RG58J | 08141009 | 08/14/10 | 1716 |
| 07 | PSB23-14-16.5-07 | RG58K | 08141010 | 08/14/10 | 1749 |
| 08 | PSB23-16.5-19-07 | RG58L | 08141011 | 08/14/10 | 1822 |
| 09 | PSB24-0-0.5-0729 | RG58M | 08141012 | 08/14/10 | 1855 |
| 10 | PSB24-1.5-2-0729 | RG58N | 08141013 | 08/14/10 | 1928 |
| 11 | PSB24-2-4-072910 | RG58O | 08141014 | 08/14/10 | 2000 |
| 12 | PSB24-2-4-072910 | RG58P | 08141015 | 08/14/10 | 2033 |
| 13 | PSB23-1.5-2-0729 | RG58H | 08141016 | 08/14/10 | 2106 |
| 14 | PSB24-14-16-0729 | RG58R | 08141017 | 08/14/10 | 2138 |
| 15 | PSB24-16-17-0729 | RG58S | 08141018 | 08/14/10 | 2211 |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

5B
SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

Instrument ID: NT6

Project: LORA LAKE RI

DFTPP Injection Date: 08/17/10

DFTPP Injection Time: 1003

| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 51 | 10.0 - 80.0% of mass 198 | 31.9 |
| 68 | Less than 2.0% of mass 69 | 0.0 (0.0)1 |
| 69 | Mass 69 relative abundance | 38.4 |
| 70 | Less than 2.0% of mass 69 | 0.1 (0.3)1 |
| 127 | 10.0 - 80.0% of mass 198 | 48.6 |
| 197 | Less than 2.0% of mass 198 | 0.0 |
| 198 | Base Peak, 100% relative abundance | 100.0 |
| 199 | 5.0 to 9.0% of mass 198 | 7.1 |
| 275 | 10.0 - 60.0% of mass 198 | 27.7 |
| 365 | Greater than 1.0% of mass 198 | 3.17 |
| 441 | 0.0 - 24.0% of mass 442 | 11.2 (14.3)2 |
| 442 | 50.0 - 200.0% of mass 198 | 78.3 |
| 443 | 15.0 - 24.0% of mass 442 | 15.9 (20.3)2 |

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------------|------------------|----------------|------------------|------------------|
| 01 | CC0817 | CC0817 | 08171001 | 08/17/10 | 1003 |
| 02 | PSB23-2-4-072910 | RG58I | 08171018 | 08/17/10 | 1933 |
| 03 | | | | | |
| 04 | | | | | |
| 05 | | | | | |
| 06 | | | | | |
| 07 | | | | | |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

SEMIVOLATILE 8270-D INITIAL CALIBRATION DATA

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Instrument ID: NT6

Calibration Date: 07/23/10

| COMPOUND | RRF | RRF | RRF | RRF | RRF | RRF | RRF | RRF | %RSD |
|---------------------------|-------|-------|-------|-------|-------|-------|-------|-------|------|
| | 1 | 5 | 10 | 25 | 40 | 60 | 80 | | |
| Naphthalene | 1.344 | 1.200 | 1.234 | 1.150 | 1.086 | 0.978 | 0.921 | 1.130 | 13.0 |
| 2-Methylnaphthalene | 0.728 | 0.638 | 0.666 | 0.617 | 0.598 | 0.559 | 0.536 | 0.620 | 10.5 |
| Acenaphthylene | 2.388 | 2.206 | 2.262 | 2.117 | 1.979 | 1.779 | 1.677 | 2.058 | 12.6 |
| Acenaphthene | 1.449 | 1.311 | 1.358 | 1.306 | 1.260 | 1.174 | 1.140 | 1.285 | 8.3 |
| Dibenzofuran | 1.971 | 1.742 | 1.824 | 1.716 | 1.655 | 1.552 | 1.492 | 1.707 | 9.5 |
| Fluorene | 1.725 | 1.509 | 1.552 | 1.465 | 1.398 | 1.296 | 1.238 | 1.455 | 11.3 |
| Phenanthrene | 1.456 | 1.294 | 1.343 | 1.256 | 1.196 | 1.102 | 1.049 | 1.242 | 11.3 |
| Anthracene | 1.476 | 1.349 | 1.393 | 1.324 | 1.242 | 1.132 | 1.067 | 1.283 | 11.3 |
| Fluoranthene | 1.469 | 1.440 | 1.474 | 1.407 | 1.319 | 1.196 | 1.117 | 1.346 | 10.5 |
| Pyrene | 1.491 | 1.147 | 1.199 | 1.298 | 1.134 | 1.109 | 1.052 | 1.204 | 12.3 |
| Benzo (a) anthracene | 1.391 | 1.067 | 1.108 | 1.258 | 1.104 | 1.098 | 1.067 | 1.156 | 10.6 |
| Chrysene | 1.340 | 1.001 | 1.042 | 1.160 | 1.031 | 1.015 | 0.986 | 1.082 | 11.7 |
| Benzo (a) pyrene | 1.398 | 1.287 | 1.363 | 1.282 | 1.246 | 1.150 | 1.101 | 1.261 | 8.5 |
| Indeno (1,2,3-cd) pyrene | 1.859 | 1.700 | 1.761 | 1.708 | 1.672 | 1.582 | 1.529 | 1.687 | 6.5 |
| Dibenzo (a, h) anthracene | 1.371 | 1.330 | 1.381 | 1.333 | 1.299 | 1.220 | 1.142 | 1.296 | 6.7 |
| Benzo (g, h, i) perylene | 1.721 | 1.540 | 1.579 | 1.535 | 1.502 | 1.415 | 1.360 | 1.522 | 7.7 |
| 1-methylnaphthalene | 0.741 | 0.665 | 0.679 | 0.642 | 0.620 | 0.581 | 0.557 | 0.641 | 9.7 |
| Total Benzofluoranthenes | 1.545 | 1.350 | 1.369 | 1.319 | 1.237 | 1.131 | 1.063 | 1.288 | 12.5 |
| Terphenyl-d14 | 0.848 | 0.620 | 0.666 | 0.760 | 0.675 | 0.682 | | 0.708 | 11.6 |
| 2-Fluorobiphenyl | 1.655 | 1.418 | 1.444 | 1.370 | 1.295 | 1.218 | | 1.400 | 10.7 |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |
| | | | | | | | | | |

<- Outside QC limits: %RSD <20% or R² > 0.990

SEMIVOLATILE 8270-D CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Instrument ID: NT6

Cont. Calib. Date: 08/13/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1124

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|--------------------------|------------------|-----------------|------------|---------------|----------------|
| Naphthalene | 1.130 | 1.148 | 0.700 | AVRG | 1.6 |
| 2-Methylnaphthalene | 0.620 | 0.630 | 0.400 | AVRG | 1.6 |
| Acenaphthylene | 2.058 | 2.075 | 0.900 | AVRG | 0.8 |
| Acenaphthene | 1.285 | 1.260 | 0.900 | AVRG | -1.9 |
| Dibenzofuran | 1.707 | 1.727 | 0.800 | AVRG | 1.2 |
| Fluorene | 1.455 | 1.471 | 0.900 | AVRG | 1.1 |
| Phenanthrene | 1.242 | 1.268 | 0.700 | AVRG | 2.1 |
| Anthracene | 1.283 | 1.336 | 0.700 | AVRG | 4.1 |
| Fluoranthene | 1.346 | 1.474 | 0.600 | AVRG | 9.5 |
| Pyrene | 1.204 | 1.232 | 0.600 | AVRG | 2.3 |
| Benzo (a) anthracene | 1.156 | 1.243 | 0.800 | AVRG | 7.5 |
| Chrysene | 1.082 | 1.132 | 0.700 | AVRG | 4.6 |
| Benzo (a) pyrene | 1.261 | 1.264 | 0.700 | AVRG | 0.2 |
| Indeno (1,2,3-cd) pyrene | 1.687 | 1.659 | 0.500 | AVRG | -1.6 |
| Dibenzo (a,h) anthracene | 1.296 | 1.311 | 0.400 | AVRG | 1.2 |
| Benzo (g,h,i) perylene | 1.522 | 1.479 | 0.500 | AVRG | -2.8 |
| 1-methylnaphthalene | 0.641 | 0.656 | 0.010 | AVRG | 2.3 |
| Total Benzofluoranthenes | 1.288 | 1.281 | 0.010 | AVRG | -0.5 |
| Terphenyl-d14 | 0.708 | 0.758 | 0.010 | AVRG | 7.1 |
| 2-Fluorobiphenyl | 1.400 | 1.351 | 0.010 | AVRG | -3.5 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

SEMIVOLATILE 8270-D CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Instrument ID: NT6

Cont. Calib. Date: 08/14/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1145

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|--------------------------|------------------|-----------------|------------|---------------|----------------|
| Naphthalene | 1.130 | 1.146 | 0.700 | AVRG | 1.4 |
| 2-Methylnaphthalene | 0.620 | 0.625 | 0.400 | AVRG | 0.8 |
| Acenaphthylene | 2.058 | 2.062 | 0.900 | AVRG | 0.2 |
| Acenaphthene | 1.285 | 1.279 | 0.900 | AVRG | -0.5 |
| Dibenzofuran | 1.707 | 1.715 | 0.800 | AVRG | 0.5 |
| Fluorene | 1.455 | 1.491 | 0.900 | AVRG | 2.5 |
| Phenanthrene | 1.242 | 1.262 | 0.700 | AVRG | 1.6 |
| Anthracene | 1.283 | 1.320 | 0.700 | AVRG | 2.9 |
| Fluoranthene | 1.346 | 1.443 | 0.600 | AVRG | 7.2 |
| Pyrene | 1.204 | 1.242 | 0.600 | AVRG | 3.2 |
| Benzo (a) anthracene | 1.156 | 1.232 | 0.800 | AVRG | 6.6 |
| Chrysene | 1.082 | 1.119 | 0.700 | AVRG | 3.4 |
| Benzo (a) pyrene | 1.261 | 1.267 | 0.700 | AVRG | 0.5 |
| Indeno (1,2,3-cd) pyrene | 1.687 | 1.622 | 0.500 | AVRG | -3.8 |
| Dibenzo (a,h) anthracene | 1.296 | 1.286 | 0.400 | AVRG | -0.8 |
| Benzo (g,h,i) perylene | 1.522 | 1.432 | 0.500 | AVRG | -5.9 |
| 1-methylnaphthalene | 0.641 | 0.656 | 0.010 | AVRG | 2.3 |
| Total Benzofluoranthenes | 1.288 | 1.291 | 0.010 | AVRG | 0.2 |
| Terphenyl-d14 | 0.708 | 0.756 | 0.010 | AVRG | 6.8 |
| 2-Fluorobiphenyl | 1.400 | 1.334 | 0.010 | AVRG | -4.7 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

SEMIVOLATILE 8270-D CONTINUING CALIBRATION CHECK

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Instrument ID: NT6

Cont. Calib. Date: 08/17/10

Init. Calib. Date: 07/23/10

Cont. Calib. Time: 1003

| COMPOUND | CalAmt or ARF | CC Amt or RF | MIN RRF | CURVE TYPE | %D or Drift |
|--------------------------|------------------|-----------------|------------|---------------|----------------|
| ===== | ===== | ===== | ===== | ===== | ===== |
| Naphthalene | 1.130 | 1.160 | 0.700 | AVRG | 2.6 |
| 2-Methylnaphthalene | 0.620 | 0.627 | 0.400 | AVRG | 1.1 |
| Acenaphthylene | 2.058 | 2.088 | 0.900 | AVRG | 1.4 |
| Acenaphthene | 1.285 | 1.262 | 0.900 | AVRG | -1.8 |
| Dibenzofuran | 1.707 | 1.669 | 0.800 | AVRG | -2.2 |
| Fluorene | 1.455 | 1.473 | 0.900 | AVRG | 1.2 |
| Phenanthrene | 1.242 | 1.230 | 0.700 | AVRG | -1.0 |
| Anthracene | 1.283 | 1.297 | 0.700 | AVRG | 1.1 |
| Fluoranthene | 1.346 | 1.439 | 0.600 | AVRG | 6.9 |
| Pyrene | 1.204 | 1.248 | 0.600 | AVRG | 3.6 |
| Benzo (a) anthracene | 1.156 | 1.239 | 0.800 | AVRG | 7.2 |
| Chrysene | 1.082 | 1.122 | 0.700 | AVRG | 3.7 |
| Benzo (a) pyrene | 1.261 | 1.266 | 0.700 | AVRG | 0.4 |
| Indeno (1,2,3-cd) pyrene | 1.687 | 1.712 | 0.500 | AVRG | 1.5 |
| Dibenzo (a,h) anthracene | 1.296 | 1.350 | 0.400 | AVRG | 4.2 |
| Benzo (g,h,i) perylene | 1.522 | 1.488 | 0.500 | AVRG | -2.2 |
| 1-methylnaphthalene | 0.641 | 0.653 | 0.010 | AVRG | 1.9 |
| Total Benzofluoranthenes | 1.288 | 1.288 | 0.010 | AVRG | 0.0 |
| ===== | ===== | ===== | ===== | ===== | ===== |
| Terphenyl-d14 | 0.708 | 0.749 | 0.010 | AVRG | 5.8 |
| 2-Fluorobiphenyl | 1.400 | 1.347 | 0.010 | AVRG | -3.8 |

<- Exceeds QC limit of 20% D

* RF less than minimum RF

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/13/10

| | IS1 (DCB) | | IS2 (NPT) | | IS3 (ANT) | |
|-------------|--------------|-------|-----------|-------|-----------|-------|
| | AREA # | RT # | AREA # | RT # | AREA # | RT # |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 182786 | 7.59 | 584137 | 9.64 | 320442 | 12.50 |
| UPPER LIMIT | 365572 | | 1168274 | | 640884 | |
| LOWER LIMIT | 91393 | | 292068 | | 160221 | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 166565 | 7.19 | 550174 | 9.25 | 321882 | 12.09 |
| UPPER LIMIT | | 7.69 | | 9.75 | | 12.59 |
| LOWER LIMIT | | 6.69 | | 8.75 | | 11.59 |
| 01 | RG58MBS1 | | 643814 | 9.24 | 381227 | 12.09 |
| 02 | RG58LCSS1 | | 644270 | 9.25 | 383454 | 12.09 |
| 03 | PSB22-0-0.5- | | 638478 | 9.25 | 383943 | 12.09 |
| 04 | PSB22-1.5-2- | | 656447 | 9.25 | 398652 | 12.09 |
| 05 | PSB22-2-4-07 | | 637885 | 9.24 | 387188 | 12.09 |
| 06 | PSB22-4-6-07 | | 597978 | 9.24 | 360487 | 12.09 |
| 07 | PSB22-17-19- | | 642738 | 9.25 | 386938 | 12.09 |
| 08 | PSB22-19-20- | | 648070 | 9.25 | 387488 | 12.09 |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS1 = 1,4-Dichlorobenzene-d4
 IS2 = Naphthalene-d8
 IS3 = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/13/10

| | IS4 (PHN) AREA # | RT # | IS5 (CRY) AREA # | RT # | IS6 (PRY) AREA # | RT # |
|-----------------|---------------------|-------|---------------------|-------|---------------------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 503793 | 14.86 | 532343 | 19.16 | 517269 | 21.31 |
| UPPER LIMIT | 1007586 | | 1064686 | | 1034538 | |
| LOWER LIMIT | 251896 | | 266172 | | 258634 | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 505369 | 14.44 | 591540 | 18.72 | 590209 | 20.85 |
| UPPER LIMIT | | 14.94 | | 19.22 | | 21.35 |
| LOWER LIMIT | | 13.94 | | 18.22 | | 20.35 |
| 01 RG58MBS1 | 617258 | 14.43 | 707196 | 18.71 | 696194 | 20.85 |
| 02 RG58LCSS1 | 683157 | 14.44 | 756612 | 18.73 | 350289 | 20.86 |
| 03 PSB22-0-0.5- | 661888 | 14.44 | 755662 | 18.72 | 342124 | 20.86 |
| 04 PSB22-1.5-2- | 689410 | 14.44 | 788440 | 18.72 | 345872 | 20.86 |
| 05 PSB22-2-4-07 | 668956 | 14.44 | 779291 | 18.72 | 339241 | 20.86 |
| 06 PSB22-4-6-07 | 627772 | 14.44 | 730678 | 18.72 | 323824 | 20.86 |
| 07 PSB22-17-19- | 671130 | 14.44 | 790351 | 18.72 | 351433 | 20.86 |
| 08 PSB22-19-20- | 662734 | 14.44 | 789619 | 18.72 | 391639 | 20.85 |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS4 = Phenanthrene-d10

IS5 = Chrysene-d12

IS6 = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint

AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint

RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal

RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/13/10

| | IS7 AREA # | RT # | AREA # | RT # | AREA # | RT # |
|-----------------|---------------|-------|--------|-------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 719428 | 20.35 | | | | |
| UPPER LIMIT | 1438856 | | | | | |
| LOWER LIMIT | 359714 | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 731396 | 19.94 | | | | |
| UPPER LIMIT | | 20.44 | | | | |
| LOWER LIMIT | | 19.44 | | | | |
| 01 RG58MBS1 | | | | | | |
| 02 RG58LCSS1 | | | | | | |
| 03 PSB22-0-0.5- | | | | | | |
| 04 PSB22-1.5-2- | | | | | | |
| 05 PSB22-2-4-07 | | | | | | |
| 06 PSB22-4-6-07 | | | | | | |
| 07 PSB22-17-19- | | | | | | |
| 08 PSB22-19-20- | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS7 = Di-n-octylphthalate-d4

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/14/10

| | IS1 (DCB) | | IS2 (NPT) | | IS3 (ANT) | |
|-------------|--------------|-------|-----------|-------|-----------|-------|
| | AREA # | RT # | AREA # | RT # | AREA # | RT # |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 182786 | 7.59 | 584137 | 9.64 | 320442 | 12.50 |
| UPPER LIMIT | 365572 | | 1168274 | | 640884 | |
| LOWER LIMIT | 91393 | | 292068 | | 160221 | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 161123 | 7.14 | 534987 | 9.20 | 314167 | 12.04 |
| UPPER LIMIT | | 7.64 | | 9.70 | | 12.54 |
| LOWER LIMIT | | 6.64 | | 8.70 | | 11.54 |
| 01 | PSB23-0-0.5- | | 609707 | 9.19 | 357717 | 12.03 |
| 02 | PSB24-4-6-07 | | 651377 | 9.19 | 384687 | 12.03 |
| 03 | PSB23-2-4-07 | | 631717 | 9.19 | 367554 | 12.03 |
| 04 | PSB23-2-4-07 | | 625717 | 9.19 | 362448 | 12.03 |
| 05 | PSB23-4-6-07 | | 583051 | 9.18 | 338386 | 12.03 |
| 06 | PSB23-14-16. | | 646661 | 9.19 | 379763 | 12.03 |
| 07 | PSB23-16.5-1 | | 647714 | 9.19 | 377082 | 12.03 |
| 08 | PSB24-0-0.5- | | 646535 | 9.18 | 379257 | 12.03 |
| 09 | PSB24-1.5-2- | | 657121 | 9.19 | 383701 | 12.03 |
| 10 | PSB24-2-4-07 | | 661841 | 9.19 | 391994 | 12.03 |
| 11 | PSB24-2-4-07 | | 648336 | 9.19 | 382557 | 12.03 |
| 12 | PSB23-1.5-2- | | 641761 | 9.19 | 377490 | 12.03 |
| 13 | PSB24-14-16- | | 650786 | 9.19 | 385258 | 12.03 |
| 14 | PSB24-16-17- | | 672532 | 9.19 | 397533 | 12.03 |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS1 = 1,4-Dichlorobenzene-d4

IS2 = Naphthalene-d8

IS3 = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint

AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint

RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal

RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/14/10

| | IS4 (PHN) AREA # | RT # | IS5 (CRY) AREA # | RT # | IS6 (PRY) AREA # | RT # | |
|-------------|---------------------|--------|---------------------|--------|---------------------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== | |
| ICAL MIDPT | 503793 | 14.86 | 532343 | 19.16 | 517269 | 21.31 | |
| UPPER LIMIT | 1007586 | | 1064686 | | 1034538 | | |
| LOWER LIMIT | 251896 | | 266172 | | 258634 | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== | |
| CCAL | 507730 | 14.38 | 579626 | 18.66 | 556861 | 20.79 | |
| UPPER LIMIT | | 14.88 | | 19.16 | | 21.29 | |
| LOWER LIMIT | | 13.88 | | 18.16 | | 20.29 | |
| 01 | PSB23-0-0.5- | 581514 | 14.38 | 683358 | 18.65 | 697178 | 20.79 |
| 02 | PSB24-4-6-07 | 620079 | 14.38 | 705221 | 18.65 | 669507 | 20.79 |
| 03 | PSB23-2-4-07 | 610711 | 14.38 | 695593 | 18.66 | 709373 | 20.79 |
| 04 | PSB23-2-4-07 | 600899 | 14.38 | 673123 | 18.66 | 686443 | 20.79 |
| 05 | PSB23-4-6-07 | 552970 | 14.38 | 627739 | 18.65 | 618942 | 20.79 |
| 06 | PSB23-14-16. | 619065 | 14.38 | 697558 | 18.65 | 671572 | 20.78 |
| 07 | PSB23-16.5-1 | 610030 | 14.38 | 701040 | 18.65 | 668043 | 20.79 |
| 08 | PSB24-0-0.5- | 615667 | 14.38 | 709038 | 18.65 | 734362 | 20.79 |
| 09 | PSB24-1.5-2- | 628125 | 14.38 | 712465 | 18.65 | 697629 | 20.78 |
| 10 | PSB24-2-4-07 | 644324 | 14.38 | 729013 | 18.65 | 707146 | 20.79 |
| 11 | PSB24-2-4-07 | 619258 | 14.37 | 690647 | 18.65 | 688671 | 20.79 |
| 12 | PSB23-1.5-2- | 618870 | 14.37 | 720723 | 18.65 | 720130 | 20.79 |
| 13 | PSB24-14-16- | 619734 | 14.38 | 709277 | 18.65 | 691371 | 20.79 |
| 14 | PSB24-16-17- | 647131 | 14.37 | 746474 | 18.65 | 716161 | 20.78 |
| 15 | | | | | | | |
| 16 | | | | | | | |
| 17 | | | | | | | |
| 18 | | | | | | | |
| 19 | | | | | | | |
| 20 | | | | | | | |
| 21 | | | | | | | |
| 22 | | | | | | | |
| 23 | | | | | | | |
| 24 | | | | | | | |
| 25 | | | | | | | |

IS4 = Phenanthrene-d10

IS5 = Chrysene-d12

IS6 = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/14/10

| | IS7 AREA # | RT # | AREA # | RT # | AREA # | RT # |
|-----------------|---------------|-------|--------|-------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 719428 | 20.35 | | | | |
| UPPER LIMIT | 1438856 | | | | | |
| LOWER LIMIT | 359714 | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 696743 | 19.88 | | | | |
| UPPER LIMIT | | 20.38 | | | | |
| LOWER LIMIT | | 19.38 | | | | |
| 01 PSB23-0-0.5- | | | | | | |
| 02 PSB24-4-6-07 | | | | | | |
| 03 PSB23-2-4-07 | | | | | | |
| 04 PSB23-2-4-07 | | | | | | |
| 05 PSB23-4-6-07 | | | | | | |
| 06 PSB23-14-16. | | | | | | |
| 07 PSB23-16.5-1 | | | | | | |
| 08 PSB24-0-0.5- | | | | | | |
| 09 PSB24-1.5-2- | | | | | | |
| 10 PSB24-2-4-07 | | | | | | |
| 11 PSB24-2-4-07 | | | | | | |
| 12 PSB23-1.5-2- | | | | | | |
| 13 PSB24-14-16- | | | | | | |
| 14 PSB24-16-17- | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS7 = Di-n-octylphthalate-d4

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/17/10

| | IS1 (DCB) AREA # | RT # | IS2 (NPT) AREA # | RT # | IS3 (ANT) AREA # | RT # |
|-----------------|---------------------|-------|---------------------|-------|---------------------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 182786 | 7.59 | 584137 | 9.64 | 320442 | 12.50 |
| UPPER LIMIT | 365572 | | 1168274 | | 640884 | |
| LOWER LIMIT | 91393 | | 292068 | | 160221 | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 146831 | 6.95 | 471677 | 9.01 | 271376 | 11.85 |
| UPPER LIMIT | | 7.45 | | 9.51 | | 12.35 |
| LOWER LIMIT | | 6.45 | | 8.51 | | 11.35 |
| 01 PSB23-2-4-07 | | | 544376 | 9.01 | 309944 | 11.85 |
| 02 | | | | | | |
| 03 | | | | | | |
| 04 | | | | | | |
| 05 | | | | | | |
| 06 | | | | | | |
| 07 | | | | | | |
| 08 | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS1 = 1,4-Dichlorobenzene-d4

IS2 = Naphthalene-d8

IS3 = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint

AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint

RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal

RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No: RI24

Project: LORA LAKE RI

Ical Midpoint ID: 07231001

Ical Date: 07/23/10

Instrument ID: NT6

Cont. Cal Date: 08/17/10

| | IS4 (PHN) AREA # | RT # | IS5 (CRY) AREA # | RT # | IS6 (PRY) AREA # | RT # |
|-----------------|---------------------|-------|---------------------|-------|---------------------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 503793 | 14.86 | 532343 | 19.16 | 517269 | 21.31 |
| UPPER LIMIT | 1007586 | | 1064686 | | 1034538 | |
| LOWER LIMIT | 251896 | | 266172 | | 258634 | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 437424 | 14.19 | 496791 | 18.46 | 491254 | 20.59 |
| UPPER LIMIT | | 14.69 | | 18.96 | | 21.09 |
| LOWER LIMIT | | 13.69 | | 17.96 | | 20.09 |
| 01 PSB23-2-4-07 | 496087 | 14.19 | 620437 | 18.46 | 645398 | 20.59 |
| 02 | | | | | | |
| 03 | | | | | | |
| 04 | | | | | | |
| 05 | | | | | | |
| 06 | | | | | | |
| 07 | | | | | | |
| 08 | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS4 = Phenanthrene-d10

IS5 = Chrysene-d12

IS6 = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

8B
SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC
ARI Job No: RI24
Ical Midpoint ID: 07231001
Instrument ID: NT6

Client: FLOYD/SNIDER
Project: LORA LAKE RI
Ical Date: 07/23/10
Cont. Cal Date: 08/17/10

| | IS7 AREA # | RT # | AREA # | RT # | AREA # | RT # |
|-----------------|---------------|-------|--------|-------|--------|-------|
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| ICAL MIDPT | 719428 | 20.35 | | | | |
| UPPER LIMIT | 1438856 | | | | | |
| LOWER LIMIT | 359714 | | | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| CCAL | 591733 | 19.71 | | | | |
| UPPER LIMIT | | 20.21 | | | | |
| LOWER LIMIT | | 19.21 | | | | |
| 01 PSB23-2-4-07 | | | | | | |
| 02 | | | | | | |
| 03 | | | | | | |
| 04 | | | | | | |
| 05 | | | | | | |
| 06 | | | | | | |
| 07 | | | | | | |
| 08 | | | | | | |
| 09 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

IS7 = Di-n-octylphthalate-d4

AREA UPPER LIMIT = +100% of internal standard area from Ical midpoint
 AREA LOWER LIMIT = - 50% of internal standard area from Ical midpoint
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT from Cont. Cal
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT from Cont. Cal

* Values outside of QC limits.

**PCP/Chlorophenols Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-0-0.5-072910
SAMPLE

Lab Sample ID: RG58A
LIMS ID: 10-18236
Matrix: Soil
Data Release Authorized: *mw*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 11:43
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.61 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 5.1%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.5 | < 6.5 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 46.0% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-1.5-2-072910
SAMPLE

Lab Sample ID: RG58B
LIMS ID: 10-18237
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 12:03
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.53 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.2%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.6 | < 6.6 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 36.4% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-2-4-072910
SAMPLE

Lab Sample ID: RG58C
LIMS ID: 10-18238
Matrix: Soil
Data Release Authorized: *MM*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 12:23
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.14 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 9.2%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.8 | < 6.8 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 54.0% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-4-6-072910
SAMPLE

Lab Sample ID: RG58D
LIMS ID: 10-18239
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 17:43
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.15 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 8.7%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.8 | < 6.8 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 42.0% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-17-19-072910
SAMPLE

Lab Sample ID: RG58E
LIMS ID: 10-18240
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 18:03
Instrument/Analyst: ECD1/AAR

Sample Amount: 8.81 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 12.9%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 7.1 | < 7.1 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 30.6% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB22-19-20-072910
SAMPLE

Lab Sample ID: RG58F
LIMS ID: 10-18241
Matrix: Soil
Data Release Authorized: *WVW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 18:23
Instrument/Analyst: ECD1/AAR

Sample Amount: 8.39 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 16.8%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 7.4 | < 7.4 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 38.4% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-0-0.5-072910
SAMPLE

Lab Sample ID: RG58G
LIMS ID: 10-18242
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 18:43
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.38 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 6.5%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|--------|
| 87-86-5 | Pentachlorophenol | 6.7 | 14 |

Reported in $\mu\text{g}/\text{kg}$ (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 43.2% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-1.5-2-072910
SAMPLE

Lab Sample ID: RG58H
LIMS ID: 10-18243
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 20:51
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.39 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.2%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.7 | < 6.7 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 63.6% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-2-4-072910
SAMPLE

Lab Sample ID: RG58I
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *MMW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 19:23
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.46 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.6 | < 6.6 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 45.2% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-4-6-072910
SAMPLE

Lab Sample ID: RG58J
LIMS ID: 10-18245
Matrix: Soil
Data Release Authorized: *WW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 13:03
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.74 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 3.5%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.4 | < 6.4 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 52.4% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-14-16.5-072910
SAMPLE

Lab Sample ID: RG58K
LIMS ID: 10-18246
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 13:23
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.31 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 10.4%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.7 | < 6.7 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 44.0% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-16.5-19-072910
SAMPLE

Lab Sample ID: RG58L
LIMS ID: 10-18247
Matrix: Soil
Data Release Authorized: *WWW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 13:44
Instrument/Analyst: ECD1/AAR

Sample Amount: 8.67 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 13.8%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 7.2 | < 7.2 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 41.2% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB24-0-0.5-072910
SAMPLE

Lab Sample ID: RG58M
LIMS ID: 10-18248
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 14:04
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.52 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 4.8%

| CAS Number | Analyte | RL | Result |
|---------------------------------|----------------------|-------|--------|
| 87-86-5 | Pentachlorophenol | 6.6 | 14 |
| Reported in µg/kg (ppb) | | | |
| Chlorophenol Surrogate Recovery | | | |
| | 2,4,6-Tribromophenol | 52.4% | |

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB24-1.5-2-072910
SAMPLE

Lab Sample ID: RG58N
LIMS ID: 10-18249
Matrix: Soil
Data Release Authorized: *MMW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 14:24
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.54 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 6.3%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.6 | < 6.6 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 46.4% |
|----------------------|-------|

Sample ID: PSB24-2-4-072910
SAMPLE

Lab Sample ID: RG580
LIMS ID: 10-18250
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 21:11
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.31 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.4%

| CAS Number | Analyte | RL | Result |
|---------------------------------|----------------------|-------|---------|
| 87-86-5 | Pentachlorophenol | 6.7 | < 6.7 U |
| Reported in µg/kg (ppb) | | | |
| Chlorophenol Surrogate Recovery | | | |
| | 2,4,6-Tribromophenol | 61.6% | |

Sample ID: PSB24-2-4-072910-D
SAMPLE

Lab Sample ID: RG58P
LIMS ID: 10-18251
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 21:31
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.56 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.6%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.5 | < 6.5 U |

Reported in $\mu\text{g}/\text{kg}$ (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 66.8% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB24-4-6-072910
SAMPLE

Lab Sample ID: RG58Q
LIMS ID: 10-18252
Matrix: Soil
Data Release Authorized: *mm*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 21:51
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.34 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.5%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.7 | < 6.7 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 44.8% |
|----------------------|-------|

Sample ID: PSB24-14-16-072910
SAMPLE

Lab Sample ID: RG58R
LIMS ID: 10-18253
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 16:24
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.06 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 10.8%

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.9 | < 6.9 U |

Reported in $\mu\text{g}/\text{kg}$ (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 51.6% |
|----------------------|-------|

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB24-16-17-072910
SAMPLE

Lab Sample ID: RG58S
LIMS ID: 10-18254
Matrix: Soil
Data Release Authorized: *MMW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/13/10 16:44
Instrument/Analyst: ECD1/AAR

Sample Amount: 8.99 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 12.7%

| CAS Number | Analyte | RL | Result |
|--|----------------------|-------|---------|
| 87-86-5 | Pentachlorophenol | 7.0 | < 7.0 U |
| Reported in µg/kg (ppb) | | | |
| <u>Chlorophenol Surrogate Recovery</u> | | | |
| | 2,4,6-Tribromophenol | 53.6% | |

SW8041 CHLOROPHENOLICS SURROGATE RECOVERY SUMMARY

Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

| <u>Client ID</u> | <u>TBP</u> | <u>TOT OUT</u> |
|----------------------|------------|----------------|
| PSB22-0-0.5-072910 | 46.0% | 0 |
| PSB22-1.5-2-072910 | 36.4% | 0 |
| PSB22-2-4-072910 | 54.0% | 0 |
| PSB22-4-6-072910 | 42.0% | 0 |
| PSB22-17-19-072910 | 30.6% | 0 |
| PSB22-19-20-072910 | 38.4% | 0 |
| PSB23-0-0.5-072910 | 43.2% | 0 |
| PSB23-1.5-2-072910 | 63.6% | 0 |
| MB-081010 | 59.6% | 0 |
| LCS-081010 | 61.4% | 0 |
| PSB23-2-4-072910 | 45.2% | 0 |
| PSB23-2-4-072910 MS | 56.4% | 0 |
| PSB23-2-4-072910 MSD | 81.8% | 0 |
| PSB23-4-6-072910 | 52.4% | 0 |
| PSB23-14-16.5-072910 | 44.0% | 0 |
| PSB23-16.5-19-072910 | 41.2% | 0 |
| PSB24-0-0.5-072910 | 52.4% | 0 |
| PSB24-1.5-2-072910 | 46.4% | 0 |
| PSB24-2-4-072910 | 61.6% | 0 |
| PSB24-2-4-072910-D | 66.8% | 0 |
| PSB24-4-6-072910 | 44.8% | 0 |
| PSB24-14-16-072910 | 51.6% | 0 |
| PSB24-16-17-072910 | 53.6% | 0 |

LCS/MB LIMITS QC LIMITS

(TBP) = 2,4,6-Tribromophenol

(50-115)

(10-146)

Prep Method: SW3550B
Log Number Range: 10-18236 to 10-18254

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-2-4-072910
MS/MSD

Lab Sample ID: RG58I
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *MWJ*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted MS/MSD: 08/10/10
Date Analyzed MS: 08/16/10 19:43
MSD: 08/20/10 20:31
Instrument/Analyst MS: ECD1/AAR
MSD: ECD1/AAR
Percent Moisture: 7.0%

Sample Amount MS: 9.47 g-dry-wt
MSD: 9.47 g-dry-wt
Final Extract Volume MS: 25 mL
MSD: 25 mL
Dilution Factor MS: 1.00
MSD: 1.00

| Analyte | Sample | MS | Spike Added-MS | MS Recovery | MSD | Spike Added-MSD | MSD Recovery | RPD |
|-------------------|--------|------|----------------|-------------|------|-----------------|--------------|-------|
| Pentachlorophenol | < 6.61 | 47.8 | 66.0 | 72.4% | 58.9 | 66.0 | 89.2% | 20.8% |

Results reported in µg/kg
RPD calculated using sample concentrations per SW846.

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-2-4-072910
MATRIX SPIKE

Lab Sample ID: RG58I
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *WJW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/16/10 19:43
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.47 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|--|----------------------|-----|--------|
| 87-86-5 | Pentachlorophenol | 6.6 | --- |
| Reported in µg/kg (ppb) | | | |
| Chlorophenol Surrogate Recovery | | | |
| | 2,4,6-Tribromophenol | | 56.4% |

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: PSB23-2-4-072910
MATRIX SPIKE DUP

Lab Sample ID: RG58I
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *WWW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 20:31
Instrument/Analyst: ECD1/AAR

Sample Amount: 9.47 g-dry-wt
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: 7.0%

| CAS Number | Analyte | RL | Result |
|--|----------------------|-------|--------|
| 87-86-5 | Pentachlorophenol | 6.6 | --- |
| Reported in µg/kg (ppb) | | | |
| Chlorophenol Surrogate Recovery | | | |
| | 2,4,6-Tribromophenol | 81.8% | |

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: LCS-081010
LAB CONTROL

Lab Sample ID: LCS-081010
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *MW*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 20:11
Instrument/Analyst: ECD1/AAR

Sample Amount: 10.0 g
Final Extract Volume: 25 mL
Dilution Factor: 1.00

| Analyte | Lab Control | Spike Added | Recovery |
|-------------------|-------------|-------------|----------|
| Pentachlorophenol | 48.3 | 62.5 | 77.3% |

Chlorophenols Surrogate Recovery

2,4,6-Tribromophenol 61.4%

Results reported in µg/kg

4
 CHLOROPHENOL METHOD BLANK SUMMARY

SAMPLE NO.

| |
|----------|
| RG58MBS1 |
|----------|

Lab Name: ANALYTICAL RESOURCES, INC
 ARI Job No.: RG58
 Lab Sample ID: RG58MBS1
 Matrix (soil/water) SOLID
 Sulfur Cleanup (Y/N) Y
 Date Analyzed (1): 08/20/10
 Time Analyzed (1): 1951
 Instrument ID (1): ECD1
 GC Column (1): ZB5 ID: 0.53 (mm)

Client: FLOYD/SNIDER
 Project: LORA LAKE RI
 Lab File ID: 0820A019
 Extraction: (SepF/Cont/Sonc) SW3550C
 Date Extracted: 08/10/10
 Date Analyzed (2): 08/20/10
 Time Analyzed (2): 1951
 Instrument ID (2): ECD1
 GC Column (2): ZB35 ID: 0.53 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS and MSD:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED 1 | DATE ANALYZED 2 |
|----|----------------------|------------------|--------------------|--------------------|
| | ===== | ===== | ===== | ===== |
| 01 | PSB22-0-0.5- | RG58A | 08/13/10 | 08/13/10 |
| 02 | PSB22-1.5-2- | RG58B | 08/13/10 | 08/13/10 |
| 03 | PSB22-2-4-07 | RG58C | 08/13/10 | 08/13/10 |
| 04 | PSB23-4-6-07 | RG58J | 08/13/10 | 08/13/10 |
| 05 | PSB23-14-16. | RG58K | 08/13/10 | 08/13/10 |
| 06 | PSB23-16.5-1 | RG58L | 08/13/10 | 08/13/10 |
| 07 | PSB24-0-0.5- | RG58M | 08/13/10 | 08/13/10 |
| 08 | PSB24-1.5-2- | RG58N | 08/13/10 | 08/13/10 |
| 09 | PSB24-14-16- | RG58R | 08/13/10 | 08/13/10 |
| 10 | PSB24-16-17- | RG58S | 08/13/10 | 08/13/10 |
| 11 | PSB22-4-6-07 | RG58D | 08/16/10 | 08/16/10 |
| 12 | PSB22-17-19- | RG58E | 08/16/10 | 08/16/10 |
| 13 | PSB22-19-20- | RG58F | 08/16/10 | 08/16/10 |
| 14 | PSB23-0-0.5- | RG58G | 08/16/10 | 08/16/10 |
| 15 | PSB23-2-4-07 | RG58I | 08/16/10 | 08/16/10 |
| 16 | PSB23-2-4-07 | RG58IMS | 08/16/10 | 08/16/10 |
| 17 | RG58LCSS1 | RG58LCSS1 | 08/20/10 | 08/20/10 |
| 18 | PSB23-2-4-07 | RG58IMSD | 08/20/10 | 08/20/10 |
| 19 | PSB23-1.5-2- | RG58H | 08/20/10 | 08/20/10 |
| 20 | PSB24-2-4-07 | RG58O | 08/20/10 | 08/20/10 |
| 21 | PSB24-2-4-07 | RG58P | 08/20/10 | 08/20/10 |
| 22 | PSB24-4-6-07 | RG58Q | 08/20/10 | 08/20/10 |

ORGANICS ANALYSIS DATA SHEET
PCP by GC/ECD Method SW8041
Page 1 of 1

Sample ID: MB-081010
METHOD BLANK

Lab Sample ID: MB-081010
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized: *W*
Reported: 08/23/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: NA
Date Received: NA

Date Extracted: 08/10/10
Date Analyzed: 08/20/10 19:51
Instrument/Analyst: ECD1/AAR

Sample Amount: 10.0 g
Final Extract Volume: 25 mL
Dilution Factor: 1.00
Percent Moisture: NA

| CAS Number | Analyte | RL | Result |
|------------|-------------------|-----|---------|
| 87-86-5 | Pentachlorophenol | 6.2 | < 6.2 U |

Reported in µg/kg (ppb)

Chlorophenol Surrogate Recovery

| | |
|----------------------|-------|
| 2,4,6-Tribromophenol | 59.6% |
|----------------------|-------|

6D
 CHLOROPHENOL INITIAL CALIBRATION
 RETENTION TIME WINDOWS

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Instrument ID: ECD1

Calibration Date: 08/09/10

| COMPOUND | RT OF STANDARDS | | | | | MEAN RT | RT WINDOW | |
|----------------------|-----------------|-------|-------|-------|-------|------------|-----------|-------|
| | LVL 1 | LVL 2 | LVL 3 | LVL 4 | LVL 5 | | FROM | TO |
| Pentachlorophenol | 11.22 | 11.22 | 11.22 | 11.21 | 11.21 | 11.21 | 11.15 | 11.29 |
| 2,4,6-Trichloropheno | 7.26 | 7.26 | 7.26 | 7.26 | 7.26 | 7.26 | 7.19 | 7.33 |
| 2,3,6-Trichloropheno | 7.62 | 7.62 | 7.62 | 7.61 | 7.61 | 7.62 | 7.55 | 7.69 |
| 2,4,5-Trichloropheno | 8.25 | 8.24 | 8.23 | 8.22 | 8.21 | 8.23 | 8.17 | 8.31 |
| 2,3,4-Trichloropheno | 8.81 | 8.79 | 8.78 | 8.77 | 8.76 | 8.78 | 8.72 | 8.86 |
| 2,3,5,6-Tetrachlorop | 9.01 | 9.01 | 9.00 | 9.00 | 8.99 | 9.00 | 8.94 | 9.08 |
| 2,3,4,5-Tetrachlorop | 10.42 | 10.41 | 10.41 | 10.40 | 10.39 | 10.40 | 10.34 | 10.48 |
| 2,4-Dichlorophenol | 6.90 | 6.89 | 6.89 | 6.89 | 6.88 | 6.89 | 6.82 | 6.96 |
| 2,4,6-Tribromophenol | 10.01 | 10.00 | 10.00 | 9.99 | 9.98 | 10.00 | 9.93 | 10.07 |

6D
 CHLOROPHENOL INITIAL CALIBRATION
 RETENTION TIME WINDOWS

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Instrument ID: ECD1

Calibration Date: 08/09/10

| COMPOUND | RT OF STANDARDS | | | | | MEAN RT | RT WINDOW | |
|----------------------|-----------------|-------|-------|-------|-------|------------|-----------|-------|
| | LVL 1 | LVL 2 | LVL 3 | LVL 4 | LVL 5 | | FROM | TO |
| Pentachlorophenol | 11.66 | 11.65 | 11.65 | 11.65 | 11.65 | 11.65 | 11.59 | 11.73 |
| 2,4,6-Trichloropheno | 7.33 | 7.33 | 7.33 | 7.33 | 7.33 | 7.33 | 7.26 | 7.40 |
| 2,3,6-Trichloropheno | 7.86 | 7.86 | 7.86 | 7.86 | 7.85 | 7.86 | 7.79 | 7.93 |
| 2,4,5-Trichloropheno | 8.62 | 8.61 | 8.60 | 8.59 | 8.59 | 8.60 | 8.54 | 8.69 |
| 2,3,4-Trichloropheno | 9.38 | 9.37 | 9.36 | 9.36 | 9.35 | 9.36 | 9.31 | 9.45 |
| 2,3,5,6-Tetrachlorop | 9.28 | 9.27 | 9.27 | 9.26 | 9.26 | 9.27 | 9.21 | 9.35 |
| 2,3,4,5-Tetrachlorop | 11.13 | 11.12 | 11.11 | 11.11 | 11.10 | 11.11 | 11.06 | 11.20 |
| 2,4-Dichlorophenol | 7.17 | 7.16 | 7.16 | 7.16 | 7.15 | 7.16 | 7.10 | 7.24 |
| 2,4,6-Tribromophenol | 10.65 | 10.64 | 10.64 | 10.63 | 10.63 | 10.64 | 10.58 | 10.72 |

6E
 CHLOROPHENOL INITIAL CALIBRATION
 CALIBRATION FACTORS

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Instrument ID: ECD1

Calibration Date: 08/09/10

| COMPOUND | CALIBRATION FACTORS | | | | | | R ² / %RSD | CT |
|-----------------------|---------------------|-------|-------|-------|-------|-------|--------------------------|----|
| | LVL 1 | LVL 2 | LVL 3 | LVL 4 | LVL 5 | LVL 6 | | |
| Pentachlorophenol | 24528 | 19824 | 17830 | 15337 | 13686 | 11965 | 0.9996 | Q |
| 2,4,6-Trichlorophenol | 13540 | 10473 | 9560 | 8413 | 7539 | 6660 | 0.9997 | Q |
| 2,3,6-Trichlorophenol | 12902 | 10500 | 9607 | 8801 | 8025 | 7161 | 0.9998 | Q |
| 2,4,5-Trichlorophenol | 6404 | 5362 | 5688 | 4915 | 4290 | 3627 | 19.7 | A |
| 2,3,4-Trichlorophenol | 8393 | 7068 | 7135 | 7922 | 5474 | 5053 | 19.4 | A |
| 2,3,5,6-Tetrachloroph | 17905 | 15060 | 14996 | 14233 | 11882 | 10558 | 18.4 | A |
| 2,3,4,5-Tetrachloroph | 16324 | 13459 | 12294 | 10216 | 8895 | 7628 | 0.9995 | Q |
| 2,4-Dichlorophenol | 721 | 627 | 611 | 486 | 409 | 342 | 0.9993 | Q |
| 2,4,6-Tribromophenol | 18561 | 14998 | 13969 | 12135 | 11200 | 9940 | 0.9997 | Q |
| AVE RSD | | | | | | | 23.3 | |

CT stands for Curve Types:

- A Indicates an Average Response Factor Curve
- L Indicates a Linear Curve
- Q Indicates a Quadratic Curve

CALIBRATION FILES

- LVL 1: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A006.d/0809A006.cdf
- LVL 2: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A007.d/0809A007.cdf
- LVL 3: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A008.d
- LVL 4: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A005.d/0809A005.cdf
- LVL 5: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A009.d
- LVL 6: /chem2/ecd1.i/FPCP20100809.b/ical-1.b/0809A010.d

6E
 CHLOROPHENOL INITIAL CALIBRATION
 CALIBRATION FACTORS

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Instrument ID: ECD1

Calibration Date: 08/09/10

| COMPOUND | CALIBRATION FACTORS | | | | | | R ² / %RSD | CT |
|-----------------------|---------------------|-------|-------|-------|-------|-------|--------------------------|----|
| | LVL 1 | LVL 2 | LVL 3 | LVL 4 | LVL 5 | LVL 6 | | |
| Pentachlorophenol | 28790 | 24995 | 23903 | 21206 | 20507 | 18368 | 16.2 | A |
| 2,4,6-Trichlorophenol | 14811 | 12542 | 14020 | 12241 | 11222 | 10070 | 14.0 | A |
| 2,3,6-Trichlorophenol | 15358 | 13183 | 12610 | 12054 | 11138 | 10108 | 14.6 | A |
| 2,4,5-Trichlorophenol | 9451 | 7724 | 7152 | 6203 | 5568 | 4896 | 0.9997 | Q |
| 2,3,4-Trichlorophenol | 13138 | 11714 | 9430 | 8408 | 7532 | 6669 | 0.9995 | Q |
| 2,3,5,6-Tetrachloroph | 22710 | 20100 | 18581 | 17733 | 16666 | 15298 | 14.2 | A |
| 2,3,4,5-Tetrachloroph | 18414 | 16106 | 15136 | 13550 | 12798 | 11541 | 17.0 | A |
| 2,4-Dichlorophenol | 859 | 720 | 733 | 619 | 536 | 458 | 0.9997 | Q |
| 2,4,6-Tribromophenol | 22648 | 19438 | 18816 | 17793 | 17226 | 16083 | 12.2 | A |
| AVE RSD | | | | | | | 17.9 | |

CT stands for Curve Types:

- A Indicates an Average Response Factor Curve
- L Indicates a Linear Curve
- Q Indicates a Quadratic Curve

CALIBRATION FILES

- LVL 1: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A006.d/0809A006.cdf
- LVL 2: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A007.d/0809A007.cdf
- LVL 3: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A008.d
- LVL 4: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A005.d
- LVL 5: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A009.d
- LVL 6: /chem2/ecdl.i/FPCP20100809.b/ical-2.b/0809A010.d

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1043

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 22.2 | 25.0 | -11.2 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 24.0 | 25.0 | -4.0 |
| 2,3,6-Trichlorophenol | 7.62 | 7.55 | 7.69 | 21.8 | 25.0 | -12.8 |
| 2,4,5-Trichlorophenol | 8.22 | 8.17 | 8.31 | 23.0 | 25.0 | -8.0 |
| 2,3,4-Trichlorophenol | 8.77 | 8.72 | 8.86 | 22.8 | 25.0 | -8.8 |
| 2,3,5,6-Tetrachlorophenol | 9.00 | 8.94 | 9.08 | 23.2 | 25.0 | -7.2 |
| 2,3,4,5-Tetrachlorophenol | 10.40 | 10.34 | 10.48 | 22.3 | 25.0 | -10.8 |
| 2,4-Dichlorophenol | 6.89 | 6.82 | 6.96 | 216 | 250 | -13.6 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 22.4 | 25.0 | -10.4 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 9.6

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1043

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|----------------------------|-------|-----------|-------|----------------|---------------|-------|
| | | FROM | TO | | | |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 21.7 | 25.0 | -13.2 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 24.8 | 25.0 | -0.8 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 23.6 | 25.0 | -5.6 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 24.1 | 25.0 | -3.6 |
| 2,3,4-Trichlorophenol | 9.36 | 9.31 | 9.45 | 24.0 | 25.0 | -4.0 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 23.8 | 25.0 | -4.8 |
| 2,3,4,5-Tetrachlorophenol | 11.11 | 11.06 | 11.20 | 21.5 | 25.0 | -14.0 |
| 2,4-Dichlorophenol | 7.16 | 7.10 | 7.24 | 237 | 250 | -5.2 |
| 2,4,6-Tribromophenol (surr | 10.63 | 10.58 | 10.72 | 22.8 | 25.0 | -8.8 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 6.7

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1544

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| | | FROM | TO | | | |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 24.1 | 25.0 | -3.6 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 24.8 | 25.0 | -0.8 |
| 2,3,6-Trichlorophenol | 7.61 | 7.55 | 7.69 | 22.5 | 25.0 | -10.0 |
| 2,4,5-Trichlorophenol | 8.21 | 8.17 | 8.31 | 24.0 | 25.0 | -4.0 |
| 2,3,4-Trichlorophenol | 8.76 | 8.72 | 8.86 | 23.2 | 25.0 | -7.2 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 24.2 | 25.0 | -3.2 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 23.9 | 25.0 | -4.4 |
| 2,4-Dichlorophenol | 6.88 | 6.82 | 6.96 | 209 | 250 | -16.4 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 24.2 | 25.0 | -3.2 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 5.9

7E
CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1544

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 23.8 | 25.0 | -4.8 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 26.4 | 25.0 | 5.6 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 24.1 | 25.0 | -3.6 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 25.6 | 25.0 | 2.4 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 24.5 | 25.0 | -2.0 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 24.8 | 25.0 | -0.8 |
| 2,3,4,5-Tetrachlorophenol | 11.10 | 11.06 | 11.20 | 23.4 | 25.0 | -6.4 |
| 2,4-Dichlorophenol | 7.15 | 7.10 | 7.24 | 252 | 250 | 0.8 |
| 2,4,6-Tribromophenol (surr) | 10.63 | 10.58 | 10.72 | 24.5 | 25.0 | -2.0 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 3.2

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1724

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 24.7 | 25.0 | -1.2 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 25.4 | 25.0 | 1.6 |
| 2,3,6-Trichlorophenol | 7.61 | 7.55 | 7.69 | 23.1 | 25.0 | -7.6 |
| 2,4,5-Trichlorophenol | 8.21 | 8.17 | 8.31 | 24.7 | 25.0 | -1.2 |
| 2,3,4-Trichlorophenol | 8.76 | 8.72 | 8.86 | 23.5 | 25.0 | -6.0 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 24.1 | 25.0 | -3.6 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 24.6 | 25.0 | -1.6 |
| 2,4-Dichlorophenol | 6.88 | 6.82 | 6.96 | 227 | 250 | -9.2 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 24.8 | 25.0 | -0.8 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 3.6

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/13/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1724

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.64 | 11.59 | 11.73 | 23.9 | 25.0 | -4.4 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 26.2 | 25.0 | 4.8 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 24.2 | 25.0 | -3.2 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 25.8 | 25.0 | 3.2 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 24.9 | 25.0 | -0.4 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 25.1 | 25.0 | 0.4 |
| 2,3,4,5-Tetrachlorophenol | 11.10 | 11.06 | 11.20 | 23.5 | 25.0 | -6.0 |
| 2,4-Dichlorophenol | 7.15 | 7.10 | 7.24 | 252 | 250 | 0.8 |
| 2,4,6-Tribromophenol (surr) | 10.63 | 10.58 | 10.72 | 24.7 | 25.0 | -1.2 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 2.7

7E
CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/16/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1723

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|----------------------------|-------|-----------|-------|----------------|---------------|-------|
| | | FROM | TO | | | |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 22.3 | 25.0 | -10.8 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 24.5 | 25.0 | -2.0 |
| 2,3,6-Trichlorophenol | 7.62 | 7.55 | 7.69 | 22.3 | 25.0 | -10.8 |
| 2,4,5-Trichlorophenol | 8.22 | 8.17 | 8.31 | 23.1 | 25.0 | -7.6 |
| 2,3,4-Trichlorophenol | 8.76 | 8.72 | 8.86 | 27.1 | 25.0 | 8.4 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 22.8 | 25.0 | -8.8 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 23.2 | 25.0 | -7.2 |
| 2,4-Dichlorophenol | 6.89 | 6.82 | 6.96 | 211 | 250 | -15.6 |
| 2,4,6-Tribromophenol (surr | 9.99 | 9.93 | 10.07 | 23.3 | 25.0 | -6.8 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 8.7

7E
CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/16/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :1723

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 21.6 | 25.0 | -13.6 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 23.8 | 25.0 | -4.8 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 22.7 | 25.0 | -9.2 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 23.9 | 25.0 | -4.4 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 23.7 | 25.0 | -5.2 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 24.7 | 25.0 | -1.2 |
| 2,3,4,5-Tetrachlorophenol | 11.11 | 11.06 | 11.20 | 21.1 | 25.0 | -15.6 |
| 2,4-Dichlorophenol | 7.16 | 7.10 | 7.24 | 227 | 250 | -9.2 |
| 2,4,6-Tribromophenol (surr) | 10.63 | 10.58 | 10.72 | 22.5 | 25.0 | -10.0 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 8.1

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/16/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :2003

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 24.4 | 25.0 | -2.4 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 25.9 | 25.0 | 3.6 |
| 2,3,6-Trichlorophenol | 7.61 | 7.55 | 7.69 | 23.4 | 25.0 | -6.4 |
| 2,4,5-Trichlorophenol | 8.22 | 8.17 | 8.31 | 24.5 | 25.0 | -2.0 |
| 2,3,4-Trichlorophenol | 8.76 | 8.72 | 8.86 | 25.2 | 25.0 | 0.8 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 23.8 | 25.0 | -4.8 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 24.2 | 25.0 | -3.2 |
| 2,4-Dichlorophenol | 6.89 | 6.82 | 6.96 | 318 | 250 | 27.2 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 24.1 | 25.0 | -3.6 |
| | | | | | | |
| | | | | | | |

<-

AVERAGE %D = 6.0

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/16/10

Lab Sample ID (PCP): PCP CCAL

Time Analyzed :2003

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 22.6 | 25.0 | -9.6 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 26.4 | 25.0 | 5.6 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 24.7 | 25.0 | -1.2 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 25.7 | 25.0 | 2.8 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 24.4 | 25.0 | -2.4 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 25.2 | 25.0 | 0.8 |
| 2,3,4,5-Tetrachlorophenol | 11.11 | 11.06 | 11.20 | 25.5 | 25.0 | 2.0 |
| 2,4-Dichlorophenol | 7.16 | 7.10 | 7.24 | 259 | 250 | 3.6 |
| 2,4,6-Tribromophenol (surr | 10.63 | 10.58 | 10.72 | 24.1 | 25.0 | -3.6 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 3.5

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/20/10

Lab Sample ID (PCP): PCPCCAL

Time Analyzed :1931

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 21.6 | 25.0 | -13.6 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 23.9 | 25.0 | -4.4 |
| 2,3,6-Trichlorophenol | 7.62 | 7.55 | 7.69 | 21.9 | 25.0 | -12.4 |
| 2,4,5-Trichlorophenol | 8.22 | 8.17 | 8.31 | 23.2 | 25.0 | -7.2 |
| 2,3,4-Trichlorophenol | 8.77 | 8.72 | 8.86 | 22.0 | 25.0 | -12.0 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 22.4 | 25.0 | -10.4 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 22.2 | 25.0 | -11.2 |
| 2,4-Dichlorophenol | 6.89 | 6.82 | 6.96 | 227 | 250 | -9.2 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 22.6 | 25.0 | -9.6 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 10.0

7E
CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/20/10

Lab Sample ID (PCP): PCPCCAL

Time Analyzed :1931

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| | | FROM | TO | | | |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 21.6 | 25.0 | -13.6 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 22.6 | 25.0 | -9.6 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 21.7 | 25.0 | -13.2 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 23.8 | 25.0 | -4.8 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 22.3 | 25.0 | -10.8 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 22.7 | 25.0 | -9.2 |
| 2,3,4,5-Tetrachlorophenol | 11.11 | 11.06 | 11.20 | 21.6 | 25.0 | -13.6 |
| 2,4-Dichlorophenol | 7.16 | 7.10 | 7.24 | 218 | 250 | -12.8 |
| 2,4,6-Tribromophenol (surr) | 10.63 | 10.58 | 10.72 | 22.3 | 25.0 | -10.8 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 10.9

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB5 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/20/10

Lab Sample ID (PCP): PCPCCAL

Time Analyzed :2251

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| | | FROM | TO | | | |
| Pentachlorophenol | 11.21 | 11.15 | 11.29 | 22.2 | 25.0 | -11.2 |
| 2,4,6-Trichlorophenol | 7.26 | 7.19 | 7.33 | 25.2 | 25.0 | 0.8 |
| 2,3,6-Trichlorophenol | 7.62 | 7.55 | 7.69 | 23.7 | 25.0 | -5.2 |
| 2,4,5-Trichlorophenol | 8.22 | 8.17 | 8.31 | 23.8 | 25.0 | -4.8 |
| 2,3,4-Trichlorophenol | 8.77 | 8.72 | 8.86 | 24.6 | 25.0 | -1.6 |
| 2,3,5,6-Tetrachlorophenol | 8.99 | 8.94 | 9.08 | 23.1 | 25.0 | -7.6 |
| 2,3,4,5-Tetrachlorophenol | 10.39 | 10.34 | 10.48 | 23.1 | 25.0 | -7.6 |
| 2,4-Dichlorophenol | 6.89 | 6.82 | 6.96 | 225 | 250 | -10.0 |
| 2,4,6-Tribromophenol (surr) | 9.99 | 9.93 | 10.07 | 23.2 | 25.0 | -7.2 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 6.2

7E
 CHLOROPHENOL CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

ARI Job No.: RG58

Project: LORA LAKE RI

GC Column: ZB35 ID: 0.53 (mm)

Init. Calib. Date(s): 08/09/10 08/09/10

Client Sample No. (PCP):

Date Analyzed :08/20/10

Lab Sample ID (PCP): PCPCCAL

Time Analyzed :2251

| PCP MIX COMPOUND | RT | RT WINDOW | | CALC AMOUNT | NOM AMOUNT | %D |
|-----------------------------|-------|-----------|-------|----------------|---------------|-------|
| ===== | ===== | FROM | TO | ===== | ===== | ===== |
| Pentachlorophenol | 11.65 | 11.59 | 11.73 | 22.2 | 25.0 | -11.2 |
| 2,4,6-Trichlorophenol | 7.33 | 7.26 | 7.40 | 23.1 | 25.0 | -7.6 |
| 2,3,6-Trichlorophenol | 7.86 | 7.79 | 7.93 | 22.4 | 25.0 | -10.4 |
| 2,4,5-Trichlorophenol | 8.59 | 8.54 | 8.69 | 24.5 | 25.0 | -2.0 |
| 2,3,4-Trichlorophenol | 9.35 | 9.31 | 9.45 | 23.2 | 25.0 | -7.2 |
| 2,3,5,6-Tetrachlorophenol | 9.26 | 9.21 | 9.35 | 23.3 | 25.0 | -6.8 |
| 2,3,4,5-Tetrachlorophenol | 11.11 | 11.06 | 11.20 | 22.0 | 25.0 | -12.0 |
| 2,4-Dichlorophenol | 7.16 | 7.10 | 7.24 | 22.9 | 25.0 | -8.4 |
| 2,4,6-Tribromophenol (surr) | 10.63 | 10.58 | 10.72 | 22.9 | 25.0 | -8.4 |
| | | | | | | |
| | | | | | | |

AVERAGE %D = 8.2

8
CHLOROPHENOL ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER
 ARI Job No.: RG58 Project: LORA LAKE RI
 GC Column: ZB5 ID: 0.53 (mm) Instrument ID: ECD1
 Init. Calib. Date(s): 08/09/10 08/09/10

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS,
 SAMPLES, AND STANDARDS IS GIVEN BELOW:

| MEAN SURROGATE RT FROM INITIAL CALIBRATION S1 : 10.00 | | | | | |
|--|------------------|------------------|------------------|------------|-------|
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # | |
| ===== | ===== | ===== | ===== | ===== | |
| 01 | PCPD | 08/09/10 | 1223 | 9.99 | |
| 02 | PCPA | 08/09/10 | 1243 | 10.01 | |
| 03 | PCPB | 08/09/10 | 1303 | 10.00 | |
| 04 | PCPC | 08/09/10 | 1323 | 10.00 | |
| 05 | PCPE | 08/09/10 | 1343 | 9.98 | |
| 06 | PCPF | 08/09/10 | 1403 | 9.98 | |
| 07 | ZZZZZ | 08/09/10 | 1423 | 10.00 | |
| 08 | PCP CCAL | 08/13/10 | 1043 | 9.99 | |
| 09 | PSB22-0-0.5- | RG58A | 08/13/10 | 1143 | 9.99 |
| 10 | PSB22-1.5-2- | RG58B | 08/13/10 | 1203 | 9.99 |
| 11 | PSB22-2-4-07 | RG58C | 08/13/10 | 1223 | 9.99 |
| 12 | PSB23-4-6-07 | RG58J | 08/13/10 | 1303 | 9.99 |
| 13 | PSB23-14-16. | RG58K | 08/13/10 | 1323 | 9.99 |
| 14 | PSB23-16.5-1 | RG58L | 08/13/10 | 1344 | 9.99 |
| 15 | PSB24-0-0.5- | RG58M | 08/13/10 | 1404 | 9.98 |
| 16 | PSB24-1.5-2- | RG58N | 08/13/10 | 1424 | 9.99 |
| 17 | PCP CCAL | 08/13/10 | 1544 | 9.99 | |
| 18 | PSB24-14-16- | RG58R | 08/13/10 | 1624 | 10.00 |
| 19 | PSB24-16-17- | RG58S | 08/13/10 | 1644 | 10.00 |
| 20 | PCP CCAL | 08/13/10 | 1724 | 9.99 | |
| 21 | PCP CCAL | 08/16/10 | 1723 | 9.99 | |
| 22 | PSB22-4-6-07 | RG58D | 08/16/10 | 1743 | 9.99 |
| 23 | PSB22-17-19- | RG58E | 08/16/10 | 1803 | 9.99 |
| 24 | PSB22-19-20- | RG58F | 08/16/10 | 1823 | 9.99 |
| 25 | PSB23-0-0.5- | RG58G | 08/16/10 | 1843 | 9.99 |
| 26 | PSB23-2-4-07 | RG58I | 08/16/10 | 1923 | 9.99 |
| 27 | PSB23-2-4-07 | RG58IMS | 08/16/10 | 1943 | 9.99 |
| 28 | PCP CCAL | 08/16/10 | 2003 | 9.99 | |
| 29 | PCPCCAL | 08/20/10 | 1931 | 9.99 | |
| 30 | RG58MBS1 | RG58MBS1 | 08/20/10 | 1951 | 9.99 |
| 31 | RG58LCSS1 | RG58LCSS1 | 08/20/10 | 2011 | 9.98 |
| 32 | PSB23-2-4-07 | RG58IMSD | 08/20/10 | 2031 | 9.98 |

QC LIMITS
 S1 = 2,4,6-Tribromophenol (+/- 0.07 MINUTES)

* Values outside of QC limits.

8
CHLOROPHENOL ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER
 ARI Job No.: RG58 Project: LORA LAKE RI
 GC Column: ZB5 ID: 0.53 (mm) Instrument ID: ECD1
 Init. Calib. Date(s): 08/09/10 08/09/10

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS,
 SAMPLES, AND STANDARDS IS GIVEN BELOW:

| MEAN SURROGATE RT FROM INITIAL CALIBRATION | | | | | |
|--|----------------------|------------------|------------------|------------------|------------|
| S1 : 10.00 | | | | | |
| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # |
| | ===== | ===== | ===== | ===== | ===== |
| 01 | PSB23-1.5-2- | RG58H | 08/20/10 | 2051 | 9.99 |
| 02 | PSB24-2-4-07 | RG58O | 08/20/10 | 2111 | 9.99 |
| 03 | PSB24-2-4-07 | RG58P | 08/20/10 | 2131 | 9.99 |
| 04 | PSB24-4-6-07 | RG58Q | 08/20/10 | 2151 | 9.98 |
| 05 | ZZZZZ | ZZZZZ | 08/20/10 | 2211 | ---- |
| 06 | | PCPCCAL | 08/20/10 | 2251 | 9.99 |

QC LIMITS

S1 = 2,4,6-Tribromophenol (+/- 0.07 MINUTES)

* Values outside of QC limits.

8
CHLOROPHENOL ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER
 ARI Job No.: RG58 Project: LORA LAKE RI
 GC Column: ZB35 ID: 0.53 (mm) Instrument ID: ECD1
 Init. Calib. Date(s): 08/09/10 08/09/10

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS,
 SAMPLES, AND STANDARDS IS GIVEN BELOW:

| MEAN SURROGATE RT FROM INITIAL CALIBRATION | | | | |
|--|--------------|----------|----------|-------|
| S1 : 10.65 | | | | |
| CLIENT | LAB | DATE | TIME | S1 |
| SAMPLE NO. | SAMPLE ID | ANALYZED | ANALYZED | RT # |
| ===== | ===== | ===== | ===== | ===== |
| 01 | PCPD | 08/09/10 | 1223 | 10.63 |
| 02 | PCPA | 08/09/10 | 1243 | 10.65 |
| 03 | PCPB | 08/09/10 | 1303 | 10.64 |
| 04 | PCPC | 08/09/10 | 1323 | 10.64 |
| 05 | PCPE | 08/09/10 | 1343 | 10.63 |
| 06 | PCPF | 08/09/10 | 1403 | 10.63 |
| 07 | ZZZZZ | 08/09/10 | 1423 | 10.64 |
| 08 | PCP CCAL | 08/13/10 | 1043 | 10.63 |
| 09 | PSB22-0-0.5- | 08/13/10 | 1143 | 10.63 |
| 10 | PSB22-1.5-2- | 08/13/10 | 1203 | 10.63 |
| 11 | PSB22-2-4-07 | 08/13/10 | 1223 | 10.63 |
| 12 | PSB23-4-6-07 | 08/13/10 | 1303 | 10.63 |
| 13 | PSB23-14-16. | 08/13/10 | 1323 | 10.63 |
| 14 | PSB23-16.5-1 | 08/13/10 | 1344 | 10.63 |
| 15 | PSB24-0-0.5- | 08/13/10 | 1404 | 10.63 |
| 16 | PSB24-1.5-2- | 08/13/10 | 1424 | 10.63 |
| 17 | PCP CCAL | 08/13/10 | 1544 | 10.63 |
| 18 | PSB24-14-16- | 08/13/10 | 1624 | 10.63 |
| 19 | PSB24-16-17- | 08/13/10 | 1644 | 10.63 |
| 20 | PCP CCAL | 08/13/10 | 1724 | 10.63 |
| 21 | PCP CCAL | 08/16/10 | 1723 | 10.63 |
| 22 | PSB22-4-6-07 | 08/16/10 | 1743 | 10.63 |
| 23 | PSB22-17-19- | 08/16/10 | 1803 | 10.63 |
| 24 | PSB22-19-20- | 08/16/10 | 1823 | 10.63 |
| 25 | PSB23-0-0.5- | 08/16/10 | 1843 | 10.63 |
| 26 | PSB23-2-4-07 | 08/16/10 | 1923 | 10.63 |
| 27 | PSB23-2-4-07 | 08/16/10 | 1943 | 10.63 |
| 28 | PCP CCAL | 08/16/10 | 2003 | 10.63 |
| 29 | PCPCCAL | 08/20/10 | 1931 | 10.63 |
| 30 | RG58MBS1 | 08/20/10 | 1951 | 10.63 |
| 31 | RG58LCSS1 | 08/20/10 | 2011 | 10.63 |
| 32 | PSB23-2-4-07 | 08/20/10 | 2031 | 10.62 |

QC LIMITS
 S1 = 2,4,6-Tribromophenol (+/- 0.07 MINUTES)

* Values outside of QC limits.

8
CHLOROPHENOL ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER
 ARI Job No.: RG58 Project: LORA LAKE RI
 GC Column: ZB35 ID: 0.53 (mm) Instrument ID: ECD1
 Init. Calib. Date(s): 08/09/10 08/09/10

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS,
 SAMPLES, AND STANDARDS IS GIVEN BELOW:

| MEAN SURROGATE RT FROM INITIAL CALIBRATION | | | | | |
|--|----------------------|------------------|------------------|------------------|------------|
| S1 : 10.65 | | | | | |
| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # |
| | ===== | ===== | ===== | ===== | ===== |
| 01 | PSB23-1.5-2- | RG58H | 08/20/10 | 2051 | 10.63 |
| 02 | PSB24-2-4-07 | RG58O | 08/20/10 | 2111 | 10.63 |
| 03 | PSB24-2-4-07 | RG58P | 08/20/10 | 2131 | 10.63 |
| 04 | PSB24-4-6-07 | RG58Q | 08/20/10 | 2151 | 10.63 |
| 05 | ZZZZZ | ZZZZZ | 08/20/10 | 2211 | 10.63 |
| 06 | | PCPCCAL | 08/20/10 | 2251 | 10.63 |

QC LIMITS
 S1 = 2,4,6-Tribromophenol (+/- 0.07 MINUTES)

* Values outside of QC limits.

**TPHD Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

**ORGANICS ANALYSIS DATA SHEET
TOTAL DIESEL RANGE HYDROCARBONS**

NWTPHD by GC/FID-Silica and Acid Cleaned
Page 1 of 2
Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

Data Release Authorized:
Reported: 08/10/10

| ARI ID | Sample ID | Extraction Date | Analysis Date | EFV DL | Range | RL | Result |
|-----------------------|---|-----------------|-------------------|-------------|---|------------------|-------------------------------|
| RG58A 10-18236 | PSB22-0-0.5-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.2 10 | < 5.2 U < 10 U 78.9% |
| RG58B 10-18237 | PSB22-1.5-2-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.3 11 | < 5.3 U < 11 U 75.6% |
| RG58C 10-18238 | PSB22-2-4-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.5 11 | < 5.5 U < 11 U 80.0% |
| RG58D 10-18239 | PSB22-4-6-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 83.4% |
| RG58E 10-18240 | PSB22-17-19-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.7 11 | < 5.7 U < 11 U 78.7% |
| RG58F 10-18241 | PSB22-19-20-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.9 12 | < 5.9 U < 12 U 83.1% |
| RG58G 10-18242 | PSB23-0-0.5-072910 HC ID: RRO | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.3 11 | < 5.3 U 18 66.8% |
| RG58H 10-18243 | PSB23-1.5-2-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 70.4% |
| MB-080610 10-18244 | Method Blank HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.0 10 | < 5.0 U < 10 U 88.5% |
| RG58I 10-18244 | PSB23-2-4-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.3 10 | < 5.3 U < 10 U 79.8% |
| RG58J 10-18245 | PSB23-4-6-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.2 10 | < 5.2 U < 10 U 79.4% |


FORM I

RG58 : 00164

**ORGANICS ANALYSIS DATA SHEET
TOTAL DIESEL RANGE HYDROCARBONS**

NWTPHD by GC/FID-Silica and Acid Cleaned
Page 2 of 2
Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

Data Release Authorized: 
Reported: 08/10/10

| ARI ID | Sample ID | Extraction Date | Analysis Date | EFV DL | Range | RL | Result |
|-------------------|---|-----------------|-------------------|-------------|---|------------------|-------------------------------|
| RG58K 10-18246 | PSB23-14-16.5-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 89.0% |
| RG58L 10-18247 | PSB23-16.5-19-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.8 12 | < 5.8 U < 12 U 82.9% |
| RG58M 10-18248 | PSB24-0-0.5-072910 HC ID: RRO | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.2 10 | < 5.2 U 18 69.1% |
| RG58N 10-18249 | PSB24-1.5-2-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.2 10 | < 5.2 U < 10 U 77.9% |
| RG58O 10-18250 | PSB24-2-4-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 76.8% |
| RG58P 10-18251 | PSB24-2-4-072910-D HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 86.1% |
| RG58Q 10-18252 | PSB24-4-6-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.4 11 | < 5.4 U < 11 U 81.1% |
| RG58S 10-18254 | PSB24-16-17-072910 HC ID: --- | 08/06/10 | 08/08/10 FID3B | 1.00 1.0 | Diesel Motor Oil o-Terphenyl | 5.5 11 | < 5.5 U < 11 U 80.8% |

Reported in mg/kg (ppm)

EFV-Effective Final Volume in mL.
DL-Dilution of extract prior to analysis.
RL-Reporting limit.

Diesel quantitation on total peaks in the range from C12 to C24.
Motor Oil quantitation on total peaks in the range from C24 to C38.
HC ID: DRO/RRO indicate results of organics or additional hydrocarbons in ranges are not identifiable.

FORM I

RG58:00165

ORGANICS ANALYSIS DATA SHEET

TOTAL DIESEL RANGE HYDROCARBONS

NWTPHD by GC/FID-Silica and Acid Cleaned

Page 1 of 1


Matrix: Soil

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Data Release Authorized:

Reported: 08/13/10 

| ARI ID | Sample ID | Extraction Date | Analysis Date | EFV DL | Range | RL | Result |
|-----------|--------------------|-----------------|---------------|--------|--------------------------|-----|-----------------|
| MB-081010 | Method Blank | 08/10/10 | 08/11/10 | 1.00 | Diesel | 5.0 | < 5.0 U |
| 10-18253 | HC ID: --- | | FID3B | 1.0 | Motor Oil o-Terphenyl | 10 | < 10 U 89.2% |
| RG58R | PSB24-14-16-072910 | 08/10/10 | 08/11/10 | 1.00 | Diesel | 5.4 | < 5.4 U |
| 10-18253 | HC ID: --- | | FID3B | 1.0 | Motor Oil o-Terphenyl | 11 | < 11 U 74.4% |

Reported in mg/kg (ppm)

EFV-Effective Final Volume in mL.

DL-Dilution of extract prior to analysis.

RL-Reporting limit.

Diesel quantitation on total peaks in the range from C12 to C24.

Motor Oil quantitation on total peaks in the range from C24 to C38.

HC ID: DRO/RRO indicate results of organics or additional hydrocarbons in ranges are not identifiable.

CLEANED TPHD SURROGATE RECOVERY SUMMARY

Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

| <u>Client ID</u> | <u>OTER</u> | <u>TOT OUT</u> |
|----------------------|-------------|----------------|
| PSB22-0-0.5-072910 | 78.9% | 0 |
| PSB22-1.5-2-072910 | 75.6% | 0 |
| PSB22-2-4-072910 | 80.0% | 0 |
| PSB22-4-6-072910 | 83.4% | 0 |
| PSB22-17-19-072910 | 78.7% | 0 |
| PSB22-19-20-072910 | 83.1% | 0 |
| PSB23-0-0.5-072910 | 66.8% | 0 |
| PSB23-1.5-2-072910 | 70.4% | 0 |
| MB-080610 | 88.5% | 0 |
| LCS-080610 | 98.1% | 0 |
| PSB23-2-4-072910 | 79.8% | 0 |
| PSB23-2-4-072910 MS | 76.0% | 0 |
| PSB23-2-4-072910 MSD | 78.7% | 0 |
| PSB23-4-6-072910 | 79.4% | 0 |
| PSB23-14-16.5-0729 | 89.0% | 0 |
| PSB23-16.5-19-0729 | 82.9% | 0 |
| PSB24-0-0.5-072910 | 69.1% | 0 |
| PSB24-1.5-2-072910 | 77.9% | 0 |
| PSB24-2-4-072910 | 76.8% | 0 |
| PSB24-2-4-072910-D | 86.1% | 0 |
| PSB24-4-6-072910 | 81.1% | 0 |
| MB-081010 | 89.2% | 0 |
| LCS-081010 | 90.5% | 0 |
| LCSD-081010 | 89.7% | 0 |
| PSB24-14-16-072910 | 74.4% | 0 |
| PSB24-16-17-072910 | 80.8% | 0 |

LCS/MB LIMITS QC LIMITS

(OTER) = o-Terphenyl

(63-115)

(49-120)

Prep Method: SW3546
Log Number Range: 10-18236 to 10-18254

CLEANED TPHD SURROGATE RECOVERY SUMMARY

Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA

| <u>Client ID</u> | <u>OTER</u> | <u>TOT OUT</u> |
|--------------------|-------------|----------------|
| MB-081010 | 89.2% | 0 |
| LCS-081010 | 90.5% | 0 |
| LCSD-081010 | 89.7% | 0 |
| PSB24-14-16-072910 | 74.4% | 0 |

| | <u>LCS/MB LIMITS</u> | <u>QC LIMITS</u> |
|----------------------|----------------------|------------------|
| (OTER) = o-Terphenyl | (63-115) | (49-120) |

Prep Method: SW3546
Log Number Range: 10-18253 to 10-18253

ORGANICS ANALYSIS DATA SHEET
NWTPHD by GC/FID-Silica and Acid Cleaned
Page 1 of 1

Sample ID: PSB23-2-4-072910
MS/MSD

Lab Sample ID: RG58I
LIMS ID: 10-18244
Matrix: Soil
Data Release Authorized:
Reported: 08/10/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted MS/MSD: 08/06/10
Date Analyzed MS: 08/08/10 06:42
MSD: 08/08/10 07:01
Instrument/Analyst MS: FID/MS
MSD: FID/MS

Sample Amount MS: 9.35 g-dry-wt
MSD: 9.43 g-dry-wt
Final Extract Volume MS: 1.0 mL
MSD: 1.0 mL
Dilution Factor MS: 1.0
MSD: 1.0
Percent Moisture: 7.0%

| Range | Sample | MS | Spike Added-MS | MS Recovery | MSD | Spike Added-MSD | MSD Recovery | RPD |
|--------|--------|-----|----------------|-------------|-----|-----------------|--------------|------|
| Diesel | < 5.3 | 117 | 160 | 73.1% | 124 | 159 | 78.0% | 5.8% |

TPHD Surrogate Recovery

| | MS | MSD |
|-------------|-------|-------|
| o-Terphenyl | 76.0% | 78.7% |

Results reported in mg/kg
RPD calculated using sample concentrations per SW846.

ORGANICS ANALYSIS DATA SHEET

NWTPHD by GC/FID-Silica and Acid Cleaned

Sample ID: LCS-080610

Page 1 of 1

LAB CONTROL

Lab Sample ID: LCS-080610


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18244

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/18/10

Date Received: 07/29/10

Date Extracted: 08/06/10

Sample Amount: 10.0 g

Date Analyzed: 08/08/10 02:54

Final Extract Volume: 1.0 mL

Instrument/Analyst: FID/MS

Dilution Factor: 1.0

| Range | Lab Control | Spike Added | Recovery |
|--------|-------------|-------------|----------|
| Diesel | 138 | 150 | 92.0% |

TPHD Surrogate Recovery

| | |
|-------------|-------|
| o-Terphenyl | 98.1% |
|-------------|-------|


Results reported in mg/kg

ORGANICS ANALYSIS DATA SHEET

NWTPHD by GC/FID-Silica and Acid Cleaned

Sample ID: LCS-081010
LCS/LCSD

Page 1 of 1

Lab Sample ID: LCS-081010
LIMS ID: 10-18253
Matrix: Soil
Data Release Authorized: 
Reported: 08/13/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Date Extracted LCS/LCSD: 08/10/10
Date Analyzed LCS: 08/11/10 15:59
LCSD: 08/11/10 16:38
Instrument/Analyst LCS: FID/MS
LCSD: FID/MS

Sample Amount LCS: 10.0 g
LCSD: 10.0 g
Final Extract Volume LCS: 1.0 mL
LCSD: 1.0 mL
Dilution Factor LCS: 1.0
LCSD: 1.0

| Range | LCS | Spike Added-LCS | LCS Recovery | LCSD | Spike Added-LCSD | LCSD Recovery | RPD |
|--------|-----|-----------------|--------------|------|------------------|---------------|------|
| Diesel | 128 | 150 | 85.3% | 128 | 150 | 85.3% | 0.0% |

TPHD Surrogate Recovery

| | LCS | LCSD |
|-------------|-------|-------|
| o-Terphenyl | 90.5% | 89.7% |

Results reported in mg/kg
RPD calculated using sample concentrations per SW846.

TOTAL DIESEL RANGE HYDROCARBONS-EXTRACTION REPORT

Matrix: Soil
Date Received: 07/29/10

ARI Job: RG58
Project: Lora Lake RI
POS-LLA

| ARI ID | Client ID | Client Amt | Final Vol | Basis | Prep Date |
|---------------------|----------------------|------------|-----------|-------|-----------|
| 10-18236-RG58A | PSB22-0-0.5-072910 | 9.54 g | 1.00 mL | D | 08/06/10 |
| 10-18237-RG58B | PSB22-1.5-2-072910 | 9.46 g | 1.00 mL | D | 08/06/10 |
| 10-18238-RG58C | PSB22-2-4-072910 | 9.12 g | 1.00 mL | D | 08/06/10 |
| 10-18239-RG58D | PSB22-4-6-072910 | 9.17 g | 1.00 mL | D | 08/06/10 |
| 10-18240-RG58E | PSB22-17-19-072910 | 8.82 g | 1.00 mL | D | 08/06/10 |
| 10-18241-RG58F | PSB22-19-20-072910 | 8.44 g | 1.00 mL | D | 08/06/10 |
| 10-18242-RG58G | PSB23-0-0.5-072910 | 9.42 g | 1.00 mL | D | 08/06/10 |
| 10-18243-RG58H | PSB23-1.5-2-072910 | 9.31 g | 1.00 mL | D | 08/06/10 |
| 10-18244-080610MB1 | Method Blank | 10.0 g | 1.00 mL | - | 08/06/10 |
| 10-18244-080610LCS1 | Lab Control | 10.0 g | 1.00 mL | - | 08/06/10 |
| 10-18244-RG58I | PSB23-2-4-072910 | 9.48 g | 1.00 mL | D | 08/06/10 |
| 10-18244-RG58IMS | PSB23-2-4-072910 | 9.35 g | 1.00 mL | D | 08/06/10 |
| 10-18244-RG58IMSD | PSB23-2-4-072910 | 9.43 g | 1.00 mL | D | 08/06/10 |
| 10-18245-RG58J | PSB23-4-6-072910 | 9.70 g | 1.00 mL | D | 08/06/10 |
| 10-18246-RG58K | PSB23-14-16.5-072910 | 9.31 g | 1.00 mL | D | 08/06/10 |
| 10-18247-RG58L | PSB23-16.5-19-072910 | 18.64 g | 1.00 mL | D | 08/06/10 |
| 10-18248-RG58M | PSB24-0-0.5-072910 | 9.68 g | 1.00 mL | D | 08/06/10 |
| 10-18249-RG58N | PSB24-1.5-2-072910 | 9.56 g | 1.00 mL | D | 08/06/10 |
| 10-18250-RG58O | PSB24-2-4-072910 | 9.29 g | 1.00 mL | D | 08/06/10 |
| 10-18251-RG58P | PSB24-2-4-072910-D | 9.30 g | 1.00 mL | D | 08/06/10 |
| 10-18252-RG58Q | PSB24-4-6-072910 | 9.28 g | 1.00 mL | D | 08/06/10 |
| 10-18254-RG58S | PSB24-16-17-072910 | 9.03 g | 1.00 mL | D | 08/06/10 |

Basis: D=Dry Weight W=As Received
Diesel Extraction Report

TOTAL DIESEL RANGE HYDROCARBONS-EXTRACTION REPORT

Matrix: Soil
Date Received: 07/29/10

ARI Job: RG58
Project: Lora Lake RI
POS-LLA

| ARI ID | Client ID | Client Amt | Final Vol | Basis | Prep Date |
|----------------------|--------------------|------------|-----------|-------|-----------|
| 10-18253-081010MB1 | Method Blank | 10.0 g | 1.00 mL | - | 08/10/10 |
| 10-18253-081010LCS1 | Lab Control | 10.0 g | 1.00 mL | - | 08/10/10 |
| 10-18253-081010LCSD1 | Lab Control Dup | 10.0 g | 1.00 mL | - | 08/10/10 |
| 10-18253-RG58R | PSB24-14-16-072910 | 9.27 g | 1.00 mL | D | 08/10/10 |

Basis: D=Dry Weight W=As Received
Diesel Extraction Report

RG58 : 00173

4
TPH METHOD BLANK SUMMARY

BLANK NO.

RG58MBS1

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project No.: LORA LAKE APTS.

Date Extracted: 08/06/10

Matrix: SOLID

Date Analyzed : 08/08/10

Instrument ID : FID3B

Time Analyzed : 0235

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS, and MSD:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED |
|----|----------------------|------------------|------------------|
| | ===== | ===== | ===== |
| 01 | RG58LCSS1 | RG58LCSS1 | 08/08/10 |
| 02 | PSB22-0-0.5- | RG58A | 08/08/10 |
| 03 | PSB22-1.5-2- | RG58B | 08/08/10 |
| 04 | PSB22-2-4-07 | RG58C | 08/08/10 |
| 05 | PSB22-4-6-07 | RG58D | 08/08/10 |
| 06 | PSB22-17-19- | RG58E | 08/08/10 |
| 07 | PSB22-19-20- | RG58F | 08/08/10 |
| 08 | PSB23-0-0.5- | RG58G | 08/08/10 |
| 09 | PSB23-1.5-2- | RG58H | 08/08/10 |
| 10 | PSB23-2-4-07 | RG58I | 08/08/10 |
| 11 | PSB23-2-4-07 | RG58IMS | 08/08/10 |
| 12 | PSB23-2-4-07 | RG58IMSD | 08/08/10 |
| 13 | PSB23-4-6-07 | RG58J | 08/08/10 |
| 14 | PSB23-14-16. | RG58K | 08/08/10 |
| 15 | PSB23-16.5-1 | RG58L | 08/08/10 |
| 16 | PSB24-0-0.5- | RG58M | 08/08/10 |
| 17 | PSB24-1.5-2- | RG58N | 08/08/10 |
| 18 | PSB24-2-4-07 | RG58O | 08/08/10 |
| 19 | PSB24-2-4-07 | RG58P | 08/08/10 |
| 20 | PSB24-4-6-07 | RG58Q | 08/08/10 |
| 21 | PSB24-16-17- | RG58S | 08/08/10 |
| 22 | | | |
| 23 | | | |
| 24 | | | |
| 25 | | | |
| 26 | | | |
| 27 | | | |
| 28 | | | |
| 29 | | | |
| 30 | | | |

4
TPH METHOD BLANK SUMMARY

BLANK NO.

RH56MBS1

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project No.: LORA LAKE APTS.

Date Extracted: 08/10/10

Matrix: SOLID

Date Analyzed : 08/11/10

Instrument ID : FID3B

Time Analyzed : 1658

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS, and MSD:

| | CLIENT SAMPLE NO. ===== | LAB SAMPLE ID ===== | DATE ANALYZED ===== |
|----|-------------------------------|---------------------------|---------------------------|
| 01 | PSB24-14-16- | RG58R | 08/11/10 |
| 02 | RH56LCSS1 | RH56LCSS1 | 08/11/10 |
| 03 | RH56LCSDS1 | RH56LCSDS1 | 08/11/10 |

6a
NW DIESEL INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.
Instrument: FID3B.I
Calibration Date: 30-JUL-2010

Client: FLOYD/SNIDER
Project: LORA LAKE APTS.
SDG No.: RG58

| Diesel Range | RF1 50 | RF2 100 | RF3 250 | RF4 500 | RF5 1000 | RF6 2500 | Ave RF | %RSD |
|--------------|-----------|------------|------------|------------|-------------|-------------|--------|------|
| WA Diesel | 22218 | 21170 | 21958 | 21565 | 21008 | 20465 | 21398 | 3.0 |
| AK Diesel | 25279 | 23959 | 24625 | 24161 | 23624 | 22975 | 24104 | 3.3 |
| OR Diesel | 25497 | 24108 | 24785 | 24317 | 23782 | 23134 | 24271 | 3.4 |
| o-Terph | 19592 | 19395 | 20002 | 19771 | 20130 | 20713 | 19934 | 2.3 |

<- Indicates %RSD outside limits
Surrogate areas are not included in Diesel RF calculation.

Quant Ranges : WA Diesel C12-C24 (3.468-5.603)
 AK Diesel C10-C25 (2.858-5.764)
 OR Diesel C10-C28 (2.858-6.244)

Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0730b018.d | 30-JUL-2010 20:23 |
| 0730b019.d | 30-JUL-2010 20:42 |
| 0730b020.d | 30-JUL-2010 21:01 |
| 0730b021.d | 30-JUL-2010 21:20 |
| 0730b022.d | 30-JUL-2010 21:39 |
| 0730b023.d | 30-JUL-2010 21:58 |

6a
NW MOTOR OIL RANGE INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.
Instrument: FID3B.I
Calibration Date: 31-JUL-2010

Client: FLOYD/SNIDER
Project: LORA LAKE APTS.
SDG No.: RG58

| Product Range | RF1 100 | RF2 250 | RF3 500 | RF4 1000 | RF5 2500 | RF6 5000 | Ave RF | %RSD |
|---------------------|------------|------------|------------|-------------|-------------|-------------|--------|------|
| WA M.Oil C24-C38 | 12620 | 11767 | 11795 | 11887 | 11681 | 12739 | 12081 | 3.9 |
| Triac Surr | 14850 | 15844 | 16922 | 17487 | 16823 | 18431 | 16726 | 7.5 |

<- Indicates %RSD outside limits
Surrogate areas are not included in Motor Oil RF calculation.

Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0730b025.d | 30-JUL-2010 22:36 |
| 0730b026.d | 30-JUL-2010 22:55 |
| 0730b027.d | 30-JUL-2010 23:14 |
| 0730b028.d | 30-JUL-2010 23:32 |
| 0730b030.d | 31-JUL-2010 00:10 |
| 0730b032.d | 31-JUL-2010 00:47 |

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
 ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
 CCal Date: 11-AUG-2010 SDG No.: RG58
 Analysis Time: 14:09 Lab ID: DIESEL#1
 Instrument: FID3B.I Lab File Name: 0811b004.d

| Diesel Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|-----|
| WADies (C12-C24) | 5542845 | 259.0 | 250 | 3.6 |
| AK102 (C10-C25) | 6201528 | 257.3 | 250 | 2.9 |
| Terphenyl | 919032 | 46.1 | 45 | 2.5 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
 ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
 CCal Date: 11-AUG-2010 SDG No.: RG58
 Analysis Time: 14:29 Lab ID: MOIL#1
 Instrument: FID3B.I Lab File Name: 0811b005.d

| M.oil Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|------|
| WAMoil (C24-C38) | 5769580 | 477.6 | 500 | -4.5 |
| AK103 (C25-C36) | 5064949 | 567.0 | 500 | 13.4 |
| n-Triacontane | 775014 | 46.3 | 45 | 3.0 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
CCal Date: 11-AUG-2010 SDG No.: RG58
Analysis Time: 17:17 Lab ID: DIESEL#2
Instrument: FID3B.I Lab File Name: 0811b013.d

| Diesel Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|-----|
| WADies (C12-C24) | 5453138 | 254.8 | 250 | 1.9 |
| AK102 (C10-C25) | 6113567 | 253.6 | 250 | 1.5 |
| Terphenyl | 903826 | 45.3 | 45 | 0.8 |

* Surrogate areas are subtracted from range areas
<- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
 ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
 CCal Date: 11-AUG-2010 SDG No.: RG58
 Analysis Time: 17:37 Lab ID: MOIL#2
 Instrument: FID3B.I Lab File Name: 0811b014.d

| M.oil Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|------|
| WAMoil (C24-C38) | 5631299 | 466.1 | 500 | -6.8 |
| AK103 (C25-C36) | 4944998 | 553.6 | 500 | 10.7 |
| n-Triacontane | 772411 | 46.2 | 45 | 2.6 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 11-AUG-2010

SDG No.: RG58

Analysis Time: 22:24

Lab ID: DIESEL#3

Instrument: FID3B.I

Lab File Name: 0811b029.d

| Diesel Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|-----|
| WADies (C12-C24) | 5484226 | 256.3 | 250 | 2.5 |
| AK102 (C10-C25) | 6167821 | 255.9 | 250 | 2.4 |
| Terphenyl | 929664 | 46.6 | 45 | 3.6 |

* Surrogate areas are subtracted from range areas
<- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
 ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
 CCal Date: 11-AUG-2010 SDG No.: RG58
 Analysis Time: 22:43 Lab ID: MOIL#3
 Instrument: FID3B.I Lab File Name: 0811b030.d

| M.oil Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|------|
| WAMoil (C24-C38) | 5788545 | 479.1 | 500 | -4.2 |
| AK103 (C25-C36) | 5113570 | 572.5 | 500 | 14.5 |
| n-Triacontane | 778815 | 46.6 | 45 | 3.5 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 08-AUG-2010

SDG No.: RG58

Analysis Time: 01:57

Lab ID: DIESEL#5

Instrument: FID3B.I

Lab File Name: 0807b049.d

| Diesel Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|------|
| WADies (C12-C24) | 5018604 | 234.5 | 250 | -6.2 |
| AK102 (C10-C25) | 5625385 | 233.4 | 250 | -6.6 |
| Terphenyl | 826630 | 41.5 | 45 | -7.8 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC. Client: FLOYD/SNIDER
 ICal Date: 30-JUL-2010 Project: LORA LAKE APTS.
 CCal Date: 08-AUG-2010 SDG No.: RG58
 Analysis Time: 02:16 Lab ID: MOIL#5
 Instrument: FID3B.I Lab File Name: 0807b050.d

| M.oil Range | Area* | CalcAmt | NomAmt | % D |
|------------------|---------|---------|--------|-------|
| WAMoil (C24-C38) | 5293636 | 438.2 | 500 | -12.4 |
| AK103 (C25-C36) | 4645950 | 520.1 | 500 | 4.0 |
| n-Triacontane | 711967 | 42.6 | 45 | -5.4 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 08-AUG-2010

SDG No.: RG58

Analysis Time: 05:45

Lab ID: DIESEL#6

Instrument: FID3B.I

Lab File Name: 0807b061.d

| Diesel Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|------|
| WADies (C12-C24) | 5054270 | 236.2 | 250 | -5.5 |
| AK102 (C10-C25) | 5674046 | 235.4 | 250 | -5.8 |
| Terphenyl | 843760 | 42.3 | 45 | -5.9 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 08-AUG-2010

SDG No.: RG58

Analysis Time: 06:04

Lab ID: MOIL#6

Instrument: FID3B.I

Lab File Name: 0807b062.d

| M.oil Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|-------|
| WAMoil (C24-C38) | 5312867 | 439.8 | 500 | -12.0 |
| AK103 (C25-C36) | 4678648 | 523.8 | 500 | 4.8 |
| n-Triacontane | 731915 | 43.8 | 45 | -2.8 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

7a
DIESEL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 08-AUG-2010

SDG No.: RG58

Analysis Time: 10:12

Lab ID: DIESEL#7

Instrument: FID3B.I

Lab File Name: 0807b075.d

| Diesel Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|------|
| WADies (C12-C24) | 5211902 | 243.6 | 250 | -2.6 |
| AK102 (C10-C25) | 5853898 | 242.9 | 250 | -2.9 |
| Terphenyl | 865581 | 43.4 | 45 | -3.5 |

* Surrogate areas are subtracted from range areas
<- Indicates a %D outside QC limits

Quant Ranges : WA Diesel C12-C24
 AK Diesel C10-C25

7a
MOTOR OIL CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 30-JUL-2010

Project: LORA LAKE APTS.

CCal Date: 08-AUG-2010

SDG No.: RG58

Analysis Time: 10:31

Lab ID: MOIL#7

Instrument: FID3B.I

Lab File Name: 0807b076.d

| M.oil Range | Area* | CalcAmnt | NomAmnt | % D |
|------------------|---------|----------|---------|-------|
| WAMoil (C24-C38) | 5427679 | 449.3 | 500 | -10.1 |
| AK103 (C25-C36) | 4772155 | 534.2 | 500 | 6.8 |
| n-Triacontane | 748382 | 44.7 | 45 | -0.6 |

* Surrogate areas are subtracted from range areas
 <- Indicates a %D outside QC limits

Quant Ranges : WA M.Oil C24-C38
 AK M.Oil C25-C36

8
TPH ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project: LORA LAKE APTS.

Instrument ID: FID3B

GC Column: RTX-1

Run Date: 07/31/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| SURROGATE RT FROM DAILY STANDARD | | | | | |
|----------------------------------|------------------|------------------|------------------|---------------|---------------|
| | | TERPH: 4.76 | | TRIAC: 6.56 | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | TERPH RT # | TRIAC RT # |
| 01 | RT | 07/30/10 | 1944 | 4.76 | 6.56 |
| 02 | IB | 07/30/10 | 2004 | 4.76 | 6.56 |
| 03 | DIESEL 50 | 07/30/10 | 2023 | 4.76 | 6.56 |
| 04 | DIESEL 100 | 07/30/10 | 2042 | 4.76 | 6.56 |
| 05 | DIESEL 250 | 07/30/10 | 2101 | 4.76 | 6.55 |
| 06 | DIESEL 500 | 07/30/10 | 2120 | 4.77 | 6.56 |
| 07 | DIESEL 1000 | 07/30/10 | 2139 | 4.77 | 6.56 |
| 08 | DIESEL 2500 | 07/30/10 | 2158 | 4.79 | 6.56 |
| 09 | DIESEL ICV | 07/30/10 | 2217 | 4.76 | 6.56 |
| 10 | MOIL 100 | 07/30/10 | 2236 | 4.77 | 6.56 |
| 11 | MOIL 250 | 07/30/10 | 2255 | 4.76 | 6.56 |
| 12 | MOIL 500 | 07/30/10 | 2314 | 4.76 | 6.56 |
| 13 | MOIL 1000 | 07/30/10 | 2332 | 4.76 | 6.57 |
| 14 | RINSE | 07/30/10 | 2351 | 4.76 | 6.56 |
| 15 | MOIL 2500 | 07/31/10 | 0010 | 4.76 | 6.58 |
| 16 | RINSE | 07/31/10 | 0028 | 4.76 | 6.56 |
| 17 | MOIL 5000 | 07/31/10 | 0047 | 4.76 | 6.60 |
| 18 | RINSE | 07/31/10 | 0106 | 4.76 | 6.56 |
| 19 | MOIL ICV | 07/31/10 | 0125 | 4.76 | 6.56 |

TERPH = o-terph
TRIAC = Triacon Surr

QC LIMITS
(+/- 0.05 MINUTES)
(+/- 0.05 MINUTES)

* Values outside of QC limits.

8
TPH ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project: LORA LAKE APTS.

Instrument ID: FID3B

GC Column: RTX-1

Run Date: 08/11/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| SURROGATE RT FROM DAILY STANDARD | | | | | |
|----------------------------------|------------------|------------------|------------------|---------------|---------------|
| | | TERPH: 4.76 | TRIAC: 6.56 | | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | TERPH RT # | TRIAC RT # |
| 01 | RT | 08/11/10 | 1331 | 4.76 | 6.56 |
| 02 | IB | 08/11/10 | 1350 | 4.76 | 6.56 |
| 03 | DIESEL#1 | 08/11/10 | 1409 | 4.76 | 6.56 |
| 04 | MOIL#1 | 08/11/10 | 1429 | 4.76 | 6.56 |
| 05 | ZZZZZ | 08/11/10 | 1501 | 4.76 | 6.55 |
| 06 | ZZZZZ | 08/11/10 | 1520 | 4.76 | 6.56 |
| 07 | ZZZZZ | 08/11/10 | 1540 | 4.76 | 6.56 |
| 08 | RH56LCSS1 | 08/11/10 | 1559 | 4.76 | 6.56 |
| 09 | ZZZZZ | 08/11/10 | 1619 | 4.76 | 6.56 |
| 10 | RH56LCSDS1 | 08/11/10 | 1638 | 4.76 | 6.56 |
| 11 | RH56MBS1 | 08/11/10 | 1658 | 4.76 | 6.56 |
| 12 | DIESEL#2 | 08/11/10 | 1717 | 4.76 | 6.56 |
| 13 | DIESEL#2 | 08/11/10 | 1737 | 4.76 | 6.56 |
| 14 | ZZZZZ | 08/11/10 | 1756 | 4.76 | 6.56 |
| 15 | ZZZZZ | 08/11/10 | 1816 | 4.76 | 6.56 |
| 16 | ZZZZZ | 08/11/10 | 1835 | 4.76 | 6.56 |
| 17 | ZZZZZ | 08/11/10 | 1854 | 4.76 | 6.56 |
| 18 | ZZZZZ | 08/11/10 | 1913 | 4.76 | 6.56 |
| 19 | ZZZZZ | 08/11/10 | 1933 | 4.76 | 6.56 |
| 20 | ZZZZZ | 08/11/10 | 1952 | 4.76 | 6.56 |
| 21 | ZZZZZ | 08/11/10 | 2011 | 4.76 | 6.56 |
| 22 | ZZZZZ | 08/11/10 | 2030 | 4.76 | 6.56 |
| 23 | ZZZZZ | 08/11/10 | 2049 | 4.76 | 6.56 |
| 24 | ZZZZZ | 08/11/10 | 2108 | 4.76 | 6.56 |
| 25 | ZZZZZ | 08/11/10 | 2128 | 4.76 | 6.56 |
| 26 | ZZZZZ | 08/11/10 | 2147 | 4.76 | 6.56 |
| 27 | PSB24-14-16- | RG58R | 2206 | 4.76 | 6.56 |
| 28 | DIESEL#3 | DIESEL#3 | 2224 | 4.76 | 6.56 |
| 29 | MOIL#3 | MOIL#3 | 2243 | 4.76 | 6.56 |

TERPH = o-terph (+/- 0.05 MINUTES)
 TRIAC = Triacon Surr (+/- 0.05 MINUTES)

* Values outside of QC limits.

8
TPH ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project: LORA LAKE APTS.

Instrument ID: FID3B

GC Column: RTX-1

Run Date: 08/08/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| SURROGATE RT FROM DAILY STANDARD | | | | | |
|----------------------------------|------------------|------------------|------------------|---------------|----------------|
| | | TERPH: 4.76 | | TRIAIC: 6.56 | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | TERPH RT # | TRIAIC RT # |
| 01 | RT | 08/08/10 | 0120 | 4.76 | 6.56 |
| 02 | IB | 08/08/10 | 0138 | 4.76 | 6.56 |
| 03 | DIESEL#5 | 08/08/10 | 0157 | 4.76 | 6.56 |
| 04 | MOIL#5 | 08/08/10 | 0216 | 4.76 | 6.56 |
| 05 | RG58MBS1 | 08/08/10 | 0235 | 4.76 | 6.56 |
| 06 | RG58LCSS1 | 08/08/10 | 0254 | 4.77 | 6.56 |
| 07 | PSB22-0-0.5- | 08/08/10 | 0313 | 4.76 | 6.56 |
| 08 | PSB22-1.5-2- | 08/08/10 | 0332 | 4.76 | 6.56 |
| 09 | PSB22-2-4-07 | 08/08/10 | 0351 | 4.76 | 6.56 |
| 10 | PSB22-4-6-07 | 08/08/10 | 0410 | 4.76 | 6.56 |
| 11 | PSB22-17-19- | 08/08/10 | 0429 | 4.76 | 6.56 |
| 12 | PSB22-19-20- | 08/08/10 | 0448 | 4.76 | 6.56 |
| 13 | PSB23-0-0.5- | 08/08/10 | 0507 | 4.76 | 6.56 |
| 14 | PSB23-1.5-2- | 08/08/10 | 0526 | 4.76 | 6.56 |
| 15 | DIESEL#6 | 08/08/10 | 0545 | 4.76 | 6.57 |
| 16 | MOIL#6 | 08/08/10 | 0604 | 4.76 | 6.56 |
| 17 | PSB23-2-4-07 | 08/08/10 | 0623 | 4.76 | 6.56 |
| 18 | PSB23-2-4-07 | 08/08/10 | 0642 | 4.76 | 6.56 |
| 19 | PSB23-2-4-07 | 08/08/10 | 0701 | 4.76 | 6.56 |
| 20 | PSB23-4-6-07 | 08/08/10 | 0720 | 4.76 | 6.56 |
| 21 | PSB23-14-16. | 08/08/10 | 0739 | 4.76 | 6.56 |
| 22 | PSB23-16.5-1 | 08/08/10 | 0759 | 4.76 | 6.56 |
| 23 | PSB24-0-0.5- | 08/08/10 | 0818 | 4.76 | 6.56 |
| 24 | PSB24-1.5-2- | 08/08/10 | 0837 | 4.76 | 6.56 |
| 25 | PSB24-2-4-07 | 08/08/10 | 0856 | 4.76 | 6.56 |
| 26 | PSB24-2-4-07 | 08/08/10 | 0915 | 4.76 | 6.56 |
| 27 | PSB24-4-6-07 | 08/08/10 | 0934 | 4.76 | 6.56 |
| 28 | PSB24-16-17- | 08/08/10 | 0953 | 4.76 | 6.56 |
| 29 | DIESEL#7 | 08/08/10 | 1012 | 4.76 | 6.57 |
| 30 | MOIL#7 | 08/08/10 | 1031 | 4.76 | 6.56 |

TERPH = o-terph (+/- 0.05 MINUTES)
 TRIAC = Triacon Surr (+/- 0.05 MINUTES)

* Values outside of QC limits.

**TPHG/BETX Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB22-TB
 SAMPLE

Lab Sample ID: RG58T
 LIMS ID: 10-18255
 Matrix: Water
 Data Release Authorized: *WWW*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/06/10 08:50
 Instrument/Analyst: PID2/MH

Purge Volume: 5.0 mL
 Dilution Factor: 1.00

| CAS Number | Analyte | RL | Result |
|-------------|--------------|-----|---------|
| 71-43-2 | Benzene | 1.0 | < 1.0 U |
| 108-88-3 | Toluene | 1.0 | < 1.0 U |
| 100-41-4 | Ethylbenzene | 1.0 | < 1.0 U |
| 179601-23-1 | m,p-Xylene | 1.0 | < 1.0 U |
| 95-47-6 | o-Xylene | 1.0 | < 1.0 U |

| | | | |
|-----------------------------|------|----------|---------------|
| Gasoline Range Hydrocarbons | 0.25 | < 0.25 U | GAS ID --- |
|-----------------------------|------|----------|---------------|

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 96.9% |
| Bromobenzene | 97.0% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 95.1% |
| Bromobenzene | 95.7% |

BETX values reported in µg/L (ppb)
 Gasoline values reported in mg/L (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

ORGANICS ANALYSIS DATA SHEET

BETX by Method SW8021BMod

TPHG by Method NWTPHG

Page 1 of 1

Sample ID: PSB23-TB

SAMPLE

Lab Sample ID: RG58U

LIMS ID: 10-18256

Matrix: Water

Data Release Authorized: *MW*

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

Event: POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Analyzed: 08/06/10 09:32

Instrument/Analyst: PID2/MH

Purge Volume: 5.0 mL

Dilution Factor: 1.00

| CAS Number | Analyte | RL | Result | GAS ID |
|-------------|-----------------------------|------|----------|--------|
| 71-43-2 | Benzene | 1.0 | < 1.0 U | |
| 108-88-3 | Toluene | 1.0 | < 1.0 U | |
| 100-41-4 | Ethylbenzene | 1.0 | < 1.0 U | |
| 179601-23-1 | m,p-Xylene | 1.0 | < 1.0 U | |
| 95-47-6 | o-Xylene | 1.0 | < 1.0 U | |
| | Gasoline Range Hydrocarbons | 0.25 | < 0.25 U | --- |

BETX Surrogate Recovery

| | |
|------------------|------|
| Trifluorotoluene | 104% |
| Bromobenzene | 103% |

Gasoline Surrogate Recovery

| | |
|------------------|------|
| Trifluorotoluene | 101% |
| Bromobenzene | 103% |

BETX values reported in µg/L (ppb)
Gasoline values reported in mg/L (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.

GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.



ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB24-TB
 SAMPLE

Lab Sample ID: RG58V
 LIMS ID: 10-18257
 Matrix: Water
 Data Release Authorized: *MM*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/06/10 09:58
 Instrument/Analyst: PID2/MH

Purge Volume: 5.0 mL
 Dilution Factor: 1.00

| CAS Number | Analyte | RL | Result |
|-------------|--------------|-----|---------|
| 71-43-2 | Benzene | 1.0 | < 1.0 U |
| 108-88-3 | Toluene | 1.0 | < 1.0 U |
| 100-41-4 | Ethylbenzene | 1.0 | < 1.0 U |
| 179601-23-1 | m,p-Xylene | 1.0 | < 1.0 U |
| 95-47-6 | o-Xylene | 1.0 | < 1.0 U |

Gasoline Range Hydrocarbons 0.25 < 0.25 U GAS ID ---

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 98.7% |
| Bromobenzene | 97.8% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 96.8% |
| Bromobenzene | 98.0% |

BETX values reported in µg/L (ppb)
 Gasoline values reported in mg/L (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021EMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB22-17-19-072910
 SAMPLE

Lab Sample ID: RG58E
 LIMS ID: 10-18240
 Matrix: Soil
 Data Release Authorized: *mwj*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/09/10 12:58
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 110 mg-dry-wt
 Percent Moisture: 12.9%

| CAS Number | Analyte | RL | Result | GAS ID |
|-----------------------------|--------------|-----|---------|--------|
| 71-43-2 | Benzene | 11 | < 11 U | |
| 108-88-3 | Toluene | 11 | < 11 U | |
| 100-41-4 | Ethylbenzene | 11 | < 11 U | |
| 179601-23-1 | m,p-Xylene | 22 | < 22 U | |
| 95-47-6 | o-Xylene | 11 | < 11 U | |
| Gasoline Range Hydrocarbons | | 4.4 | < 4.4 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 92.8% |
| Bromobenzene | 94.3% |

Gasoline Surrogate Recovery

| | |
|------------------|------|
| Trifluorotoluene | 101% |
| Bromobenzene | 101% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.
 Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.
 Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB22-19-20-072910
 SAMPLE

Lab Sample ID: RG58F
 LIMS ID: 10-18241
 Matrix: Soil
 Data Release Authorized: *VW*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/09/10 13:22
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 130 mg-dry-wt
 Percent Moisture: 16.8%

| CAS Number | Analyte | RL | Result | GAS ID |
|-------------|-----------------------------|-----|---------|--------|
| 71-43-2 | Benzene | 9.8 | < 9.8 U | |
| 108-88-3 | Toluene | 9.8 | < 9.8 U | |
| 100-41-4 | Ethylbenzene | 9.8 | < 9.8 U | |
| 179601-23-1 | m,p-Xylene | 20 | < 20 U | |
| 95-47-6 | o-Xylene | 9.8 | < 9.8 U | |
| | Gasoline Range Hydrocarbons | 3.9 | < 3.9 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 91.2% |
| Bromobenzene | 92.2% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 98.9% |
| Bromobenzene | 99.8% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.
 Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.
 Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB23-14-16.5-072910
 SAMPLE

Lab Sample ID: RG58K
 LIMS ID: 10-18246
 Matrix: Soil
 Data Release Authorized: *WJ*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/09/10 13:47
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 160 mg-dry-wt
 Percent Moisture: 10.4%

| CAS Number | Analyte | RL | Result | GAS ID |
|-------------|-----------------------------|-----|---------|--------|
| 71-43-2 | Benzene | 7.6 | < 7.6 U | |
| 108-88-3 | Toluene | 7.6 | < 7.6 U | |
| 100-41-4 | Ethylbenzene | 7.6 | < 7.6 U | |
| 179601-23-1 | m,p-Xylene | 15 | < 15 U | |
| 95-47-6 | o-Xylene | 7.6 | < 7.6 U | |
| | Gasoline Range Hydrocarbons | 3.0 | < 3.0 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 93.8% |
| Bromobenzene | 92.7% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 101% |
| Bromobenzene | 99.9% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.

GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

ORGANICS ANALYSIS DATA SHEET

BETX by Method SW8021BMod

TPHG by Method NWTPHG

Page 1 of 1

Sample ID: PSB23-16.5-19-072910

SAMPLE

Lab Sample ID: RG58L

LIMS ID: 10-18247

Matrix: Soil

Data Release Authorized: *mw*

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

Event: POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Date Analyzed: 08/09/10 14:12

Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL

Sample Amount: 130 mg-dry-wt

Percent Moisture: 13.8%

| CAS Number | Analyte | RL | Result | GAS ID |
|-------------|-----------------------------|-----|---------|--------|
| 71-43-2 | Benzene | 9.7 | < 9.7 U | |
| 108-88-3 | Toluene | 9.7 | < 9.7 U | |
| 100-41-4 | Ethylbenzene | 9.7 | < 9.7 U | |
| 179601-23-1 | m,p-Xylene | 19 | < 19 U | |
| 95-47-6 | o-Xylene | 9.7 | < 9.7 U | |
| | Gasoline Range Hydrocarbons | 3.9 | < 3.9 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 86.6% |
| Bromobenzene | 89.5% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 94.6% |
| Bromobenzene | 95.6% |

BETX values reported in µg/kg (ppb)
Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.

GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB24-14-16-072910
 SAMPLE

Lab Sample ID: RG58R
 LIMS ID: 10-18253
 Matrix: Soil
 Data Release Authorized: *W*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/09/10 14:36
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 140 mg-dry-wt
 Percent Moisture: 10.8%

| CAS Number | Analyte | RL | Result | GAS ID |
|-----------------------------|--------------|-----|---------|--------|
| 71-43-2 | Benzene | 8.6 | < 8.6 U | |
| 108-88-3 | Toluene | 8.6 | < 8.6 U | |
| 100-41-4 | Ethylbenzene | 8.6 | < 8.6 U | |
| 179601-23-1 | m,p-Xylene | 17 | < 17 U | |
| 95-47-6 | o-Xylene | 8.6 | < 8.6 U | |
| Gasoline Range Hydrocarbons | | 3.4 | < 3.4 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 91.1% |
| Bromobenzene | 93.8% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 99.1% |
| Bromobenzene | 100% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.

GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: PSB24-16-17-072910
 SAMPLE

Lab Sample ID: RG58S
 LIMS ID: 10-18254
 Matrix: Soil
 Data Release Authorized: *WWW*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: 07/29/10
 Date Received: 07/29/10

Date Analyzed: 08/09/10 15:01
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 160 mg-dry-wt
 Percent Moisture: 12.7%

| CAS Number | Analyte | RL | Result | GAS ID |
|-----------------------------|--------------|-----|---------|--------|
| 71-43-2 | Benzene | 7.9 | < 7.9 U | |
| 108-88-3 | Toluene | 7.9 | < 7.9 U | |
| 100-41-4 | Ethylbenzene | 7.9 | < 7.9 U | |
| 179601-23-1 | m,p-Xylene | 16 | < 16 U | |
| 95-47-6 | o-Xylene | 7.9 | < 7.9 U | |
| Gasoline Range Hydrocarbons | | 3.2 | < 3.2 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 93.4% |
| Bromobenzene | 96.7% |

Gasoline Surrogate Recovery

| | |
|------------------|------|
| Trifluorotoluene | 102% |
| Bromobenzene | 104% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.
 Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.
 Results corrected for soil moisture content per Section 11.10.5 of EPA Method 8000C.

BETX WATER SURROGATE RECOVERY SUMMARY

ARI Job: RG58
Matrix: Water

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
Event: POS-LLA

| <u>Client ID</u> | <u>TFT</u> | <u>BBZ</u> | <u>TOT OUT</u> |
|------------------|------------|------------|----------------|
| MB-080610 | 89.6% | 91.8% | 0 |
| LCS-080610 | 95.9% | 96.9% | 0 |
| LCSD-080610 | 95.7% | 97.1% | 0 |
| PSB22-TB | 96.9% | 97.0% | 0 |
| PSB23-TB | 104% | 103% | 0 |
| PSB24-TB | 98.7% | 97.8% | 0 |

| | LCS/MB LIMITS | QC LIMITS |
|--------------------------|----------------------|------------------|
| (TFT) = Trifluorotoluene | (79-120) | (80-120) |
| (BBZ) = Bromobenzene | (79-120) | (80-120) |

Log Number Range: 10-18255 to 10-18257

TPHG WATER SURROGATE RECOVERY SUMMARY

ARI Job: RG58
Matrix: Water

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
Event: POS-LLA

| <u>Client ID</u> | <u>TFT</u> | <u>BBZ</u> | <u>TOT OUT</u> |
|------------------|------------|------------|----------------|
| MB-080610 | 89.9% | 92.7% | 0 |
| LCS-080610 | 96.7% | 97.5% | 0 |
| LCSD-080610 | 97.0% | 98.6% | 0 |
| PSB22-TB | 95.1% | 95.7% | 0 |
| PSB23-TB | 101% | 103% | 0 |
| PSB24-TB | 96.8% | 98.0% | 0 |

| | | |
|--------------------------|----------------------|------------------|
| | LCS/MB LIMITS | QC LIMITS |
| (TFT) = Trifluorotoluene | (80-120) | (80-120) |
| (BBZ) = Bromobenzene | (80-120) | (80-120) |

Log Number Range: 10-18255 to 10-18257

BETX SOIL SURROGATE RECOVERY SUMMARY

ARI Job: RG58
Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
Event: POS-LLA

| <u>Client ID</u> | <u>TFT</u> | <u>BBZ</u> | <u>TOT</u> | <u>OUT</u> |
|----------------------|------------|------------|------------|------------|
| MB-080910 | 90.4% | 93.4% | 0 | |
| LCS-080910 | 93.6% | 97.0% | 0 | |
| LCSD-080910 | 93.1% | 96.0% | 0 | |
| PSB22-17-19-072910 | 92.8% | 94.3% | 0 | |
| PSB22-19-20-072910 | 91.2% | 92.2% | 0 | |
| PSB23-14-16.5-072910 | 93.8% | 92.7% | 0 | |
| PSB23-16.5-19-072910 | 86.6% | 89.5% | 0 | |
| PSB24-14-16-072910 | 91.1% | 93.8% | 0 | |
| PSB24-16-17-072910 | 93.4% | 96.7% | 0 | |

| | LCS/MB LIMITS | QC LIMITS |
|--------------------------|----------------------|------------------|
| (TFT) = Trifluorotoluene | (80-120) | (68-124) |
| (BBZ) = Bromobenzene | (77-120) | (62-134) |

Log Number Range: 10-18240 to 10-18254

FORM II BETX

Page 1 for RG58

RG58 : 00205

TPHG SOIL SURROGATE RECOVERY SUMMARY

ARI Job: RG58
Matrix: Soil

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
Event: POS-LLA

| <u>Client ID</u> | <u>BFB</u> | <u>TFT</u> | <u>BBZ</u> | <u>TOT</u> | <u>OUT</u> |
|----------------------|------------|------------|------------|------------|------------|
| MB-080910 | NA | 98.9% | 101% | 0 | 0 |
| LCS-080910 | NA | 102% | 103% | 0 | 0 |
| LCSD-080910 | NA | 100% | 102% | 0 | 0 |
| PSB22-17-19-072910 | NA | 101% | 101% | 0 | 0 |
| PSB22-19-20-072910 | NA | 98.9% | 99.8% | 0 | 0 |
| PSB23-14-16.5-072910 | NA | 101% | 99.9% | 0 | 0 |
| PSB23-16.5-19-072910 | NA | 94.6% | 95.6% | 0 | 0 |
| PSB24-14-16-072910 | NA | 99.1% | 100% | 0 | 0 |
| PSB24-16-17-072910 | NA | 102% | 104% | 0 | 0 |

| | LCS/MB LIMITS | QC LIMITS |
|----------------------------|----------------------|------------------|
| (BFB) = Bromofluorobenzene | (70-130) | (70-130) |
| (TFT) = Trifluorotoluene | (80-120) | (66-123) |
| (BBZ) = Bromobenzene | (80-120) | (62-130) |

Log Number Range: 10-18240 to 10-18254

ORGANICS ANALYSIS DATA SHEET
BETX by Method SW8021BMod
Page 1 of 1

Sample ID: LCS-080610
LAB CONTROL SAMPLE

Lab Sample ID: LCS-080610
LIMS ID: 10-18255
Matrix: Water
Data Release Authorized: *MW*
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
Event: POS-LLA
Date Sampled: NA
Date Received: NA

Date Analyzed LCS: 08/06/10 07:17
LCSD: 08/06/10 07:43
Instrument/Analyst LCS: PID2/MH
LCSD: PID2/MH

Purge Volume: 5.0 mL
Dilution Factor LCS: 1.0
LCSD: 1.0

| Analyte | LCS | Spike Added-LCS | LCS Recovery | LCSD | Spike Added-LCSD | LCSD Recovery | RPD |
|--------------|------|-----------------|--------------|------|------------------|---------------|------|
| Benzene | 1.69 | 2.10 | 80.5% | 1.79 | 2.10 | 85.2% | 5.7% |
| Toluene | 26.2 | 28.7 | 91.3% | 27.0 | 28.7 | 94.1% | 3.0% |
| Ethylbenzene | 8.11 | 9.20 | 88.2% | 8.38 | 9.20 | 91.1% | 3.3% |
| m,p-Xylene | 30.1 | 33.8 | 89.1% | 30.9 | 33.8 | 91.4% | 2.6% |
| o-Xylene | 12.6 | 14.0 | 90.0% | 12.8 | 14.0 | 91.4% | 1.6% |

Reported in µg/L (ppb)

RPD calculated using sample concentrations per SW846.

BETX Surrogate Recovery

| | LCS | LCSD |
|------------------|-------|-------|
| Trifluorotoluene | 95.9% | 95.7% |
| Bromobenzene | 96.9% | 97.1% |

ORGANICS ANALYSIS DATA SHEET

TPHG by Method NWTPHG

Page 1 of 1

Sample ID: LCS-080610

LAB CONTROL SAMPLE

Lab Sample ID: LCS-080610

LIMS ID: 10-18255

Matrix: Water

Data Release Authorized: *MW*

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

Event: POS-LLA

Date Sampled: NA

Date Received: NA

Date Analyzed LCS: 08/06/10 07:17

Purge Volume: 5.0 mL

LCS D: 08/06/10 07:43

Instrument/Analyst LCS: PID2/MH

Dilution Factor LCS: 1.0

LCS D: PID2/MH

LCS D: 1.0

| Analyte | Spike | | LCS | | Spike | | LCS D | | RPD |
|-----------------------------|-------|-----------|----------|-------|-------------|----------|-------|--|-----|
| | LCS | Added-LCS | Recovery | LCS D | Added-LCS D | Recovery | LCS D | | |
| Gasoline Range Hydrocarbons | 0.93 | 1.00 | 93.0% | 0.95 | 1.00 | 95.0% | 2.1% | | |

Reported in mg/L (ppm)

RPD calculated using sample concentrations per SW846.

TPHG Surrogate Recovery

| | LCS | LCS D |
|------------------|-------|-------|
| Trifluorotoluene | 96.7% | 97.0% |
| Bromobenzene | 97.5% | 98.6% |

ORGANICS ANALYSIS DATA SHEET

BETX by Method SW8021BMod

Page 1 of 1


Sample ID: LCS-080910

LAB CONTROL SAMPLE

Lab Sample ID: LCS-080910

LIMS ID: 10-18240

Matrix: Soil

Data Release Authorized: 

Reported: 08/18/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

Event: POS-LLA

Date Sampled: NA

Date Received: NA

Date Analyzed LCS: 08/09/10 07:52

LCSD: 08/09/10 08:17

Purge Volume: 5.0 mL

Instrument/Analyst LCS: PID3/MH

LCSD: PID3/MH

Sample Amount LCS: 100 mg-dry-wt

LCSD: 100 mg-dry-wt

| Analyte | LCS | Spike | LCS | LCSD | Spike | LCS | RPD |
|--------------|------|-----------|----------|------|------------|----------|------|
| | | Added-LCS | Recovery | | Added-LCSD | Recovery | |
| Benzene | 99.0 | 105 | 94.3% | 98.5 | 105 | 93.8% | 0.5% |
| Toluene | 1320 | 1440 | 91.7% | 1320 | 1440 | 91.7% | 0.0% |
| Ethylbenzene | 398 | 460 | 86.5% | 406 | 460 | 88.3% | 2.0% |
| m,p-Xylene | 1440 | 1690 | 85.2% | 1430 | 1690 | 84.6% | 0.7% |
| o-Xylene | 625 | 700 | 89.3% | 628 | 700 | 89.7% | 0.5% |

Reported in µg/kg (ppb)


RPD calculated using sample concentrations per SW846.

BETX Surrogate Recovery

| | LCS | LCSD |
|------------------|-------|-------|
| Trifluorotoluene | 93.6% | 93.1% |
| Bromobenzene | 97.0% | 96.0% |

ORGANICS ANALYSIS DATA SHEET
TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: LCS-080910
LAB CONTROL SAMPLE

Lab Sample ID: LCS-080910
 LIMS ID: 10-18240
 Matrix: Soil
 Data Release Authorized: 
 Reported: 08/18/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: NA
 Date Received: NA

Date Analyzed LCS: 08/09/10 07:52
 LCSD: 08/09/10 08:17
 Instrument/Analyst LCS: PID3/MH
 LCSD: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount LCS: 100 mg-dry-wt
 LCSD: 100 mg-dry-wt

| Analyte | LCS | Spike | LCS | LCSD | Spike | LCS | RPD |
|-----------------------------|------|-----------|----------|------|------------|----------|------|
| | | Added-LCS | Recovery | | Added-LCSD | Recovery | |
| Gasoline Range Hydrocarbons | 46.6 | 50.0 | 93.2% | 46.1 | 50.0 | 92.2% | 1.1% |

Reported in mg/kg (ppm)

RPD calculated using sample concentrations per SW846.

TPHG Surrogate Recovery

| | LCS | LCSD |
|------------------|------|------|
| Trifluorotoluene | 102% | 100% |
| Bromobenzene | 103% | 102% |

4
BETX/GAS METHOD BLANK SUMMARY

BLANK NO.

MB0806S1

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Date Analyzed : 08/06/10

Matrix: WATER

Time Analyzed : 0809

Instrument ID : PID2

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS, and MSD:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED |
|----|----------------------|------------------|------------------|
| | ===== | ===== | ===== |
| 01 | LCS0806S1 | LCS0806 | 08/06/10 |
| 02 | LCSD0806S1 | LCSD0806 | 08/06/10 |
| 03 | PSB22-TB | RG58T | 08/06/10 |
| 04 | PSB23-TB | RG58U | 08/06/10 |
| 05 | PSB24-TB | RG58V | 08/06/10 |
| 06 | PSB9-TB | RG78M | 08/06/10 |
| 07 | PSB10-TB | RG78N | 08/06/10 |
| 08 | | | |
| 09 | | | |
| 10 | | | |
| 11 | | | |
| 12 | | | |
| 13 | | | |
| 14 | | | |
| 15 | | | |
| 16 | | | |
| 17 | | | |
| 18 | | | |
| 19 | | | |
| 20 | | | |
| 21 | | | |
| 22 | | | |
| 23 | | | |
| 24 | | | |
| 25 | | | |
| 26 | | | |
| 27 | | | |
| 28 | | | |
| 29 | | | |
| 30 | | | |

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: MB-080610
 METHOD BLANK

Lab Sample ID: MB-080610
 LIMS ID: 10-18255
 Matrix: Water
 Data Release Authorized: *mw*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: NA
 Date Received: NA

Date Analyzed: 08/06/10 08:09
 Instrument/Analyst: PID2/MH

Purge Volume: 5.0 mL
 Dilution Factor: 1.00

| CAS Number | Analyte | RL | Result |
|-------------|--------------|-----|---------|
| 71-43-2 | Benzene | 1.0 | < 1.0 U |
| 108-88-3 | Toluene | 1.0 | < 1.0 U |
| 100-41-4 | Ethylbenzene | 1.0 | < 1.0 U |
| 179601-23-1 | m,p-Xylene | 1.0 | < 1.0 U |
| 95-47-6 | o-Xylene | 1.0 | < 1.0 U |

Gasoline Range Hydrocarbons 0.25 < 0.25 U GAS ID ---

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 89.6% |
| Bromobenzene | 91.8% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 89.9% |
| Bromobenzene | 92.7% |

BETX values reported in µg/L (ppb)
 Gasoline values reported in mg/L (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.

Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

4
BETX/GAS METHOD BLANK SUMMARY

BLANK NO.

MB0809S1

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Date Analyzed : 08/09/10

Matrix: SOIL

Time Analyzed : 0841

Instrument ID : PID3

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS, and MSD:

| | CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED |
|----|----------------------|------------------|------------------|
| | ===== | ===== | ===== |
| 01 | LCS0809S1 | LCS0809 | 08/09/10 |
| 02 | LCSD0809S1 | LCSD0809 | 08/09/10 |
| 03 | PSB22-17-19- | RG58E | 08/09/10 |
| 04 | PSB22-19-20- | RG58F | 08/09/10 |
| 05 | PSB23-14-16. | RG58K | 08/09/10 |
| 06 | PSB23-16.5-1 | RG58L | 08/09/10 |
| 07 | PSB24-14-16- | RG58R | 08/09/10 |
| 08 | PSB24-16-17- | RG58S | 08/09/10 |
| 09 | PSB9A-11-13. | RG78A | 08/09/10 |
| 10 | PSB9A-1.5-2- | RG78B | 08/09/10 |
| 11 | PSB9A-4-6-07 | RG78D | 08/09/10 |
| 12 | PSB10-0-0.5- | RG78F | 08/09/10 |
| 13 | PSB10-2-4-07 | RG78H | 08/09/10 |
| 14 | PSB10-4-6-07 | RG78I | 08/09/10 |
| 15 | PSB10-8.5-10 | RG78J | 08/09/10 |
| 16 | PSB10-8.5-10 | RG78JMS | 08/09/10 |
| 17 | PSB10-8.5-10 | RG78JMSD | 08/09/10 |
| 18 | PSB10-14-15- | RG78K | 08/09/10 |
| 19 | PSB10-20-25- | RG78L | 08/09/10 |
| 20 | | | |
| 21 | | | |
| 22 | | | |
| 23 | | | |
| 24 | | | |
| 25 | | | |
| 26 | | | |
| 27 | | | |
| 28 | | | |
| 29 | | | |
| 30 | | | |

ORGANICS ANALYSIS DATA SHEET
 BETX by Method SW8021BMod
 TPHG by Method NWTPHG
 Page 1 of 1

Sample ID: MB-080910
 METHOD BLANK

Lab Sample ID: MB-080910
 LIMS ID: 10-18240
 Matrix: Soil
 Data Release Authorized: *WW*
 Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
 Project: Lora Lake RI
 Event: POS-LLA
 Date Sampled: NA
 Date Received: NA

Date Analyzed: 08/09/10 08:41
 Instrument/Analyst: PID3/MH

Purge Volume: 5.0 mL
 Sample Amount: 100 mg-dry-wt

| CAS Number | Analyte | RL | Result | GAS ID |
|-------------|-----------------------------|-----|---------|--------|
| 71-43-2 | Benzene | 12 | < 12 U | |
| 108-88-3 | Toluene | 12 | < 12 U | |
| 100-41-4 | Ethylbenzene | 12 | < 12 U | |
| 179601-23-1 | m,p-Xylene | 25 | < 25 U | |
| 95-47-6 | o-Xylene | 12 | < 12 U | |
| | Gasoline Range Hydrocarbons | 5.0 | < 5.0 U | --- |

BETX Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 90.4% |
| Bromobenzene | 93.4% |

Gasoline Surrogate Recovery

| | |
|------------------|-------|
| Trifluorotoluene | 98.9% |
| Bromobenzene | 101% |

BETX values reported in µg/kg (ppb)
 Gasoline values reported in mg/kg (ppm)

GAS: Indicates the presence of gasoline or weathered gasoline.
 GRO: Positive result that does not match an identifiable gasoline pattern.
 Quantitation on total peaks in the gasoline range from Toluene to Naphthalene.

6a
GAS INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

Instrument/Det: PID2.I/RTX 502-2 FID

Project: LORA LAKE

Calibration Date: 28-JUL-2010

SDG No.: RG58-RG78

| Gas Range | RF1 0.1 | RF2 0.25 | RF3 1.0 | RF4 2.5 | RF5 5.0 | RF6 20 | Ave RF | %RSD |
|-------------|----------------------|-------------|------------|------------|------------|-----------|----------|-------|
| WA Gas | 645285 | 580360 | 562860 | 559889 | 570101 | 542758 | 576875 | 6.2 |
| AK Gas | 1005780 | 915314 | 886524 | 857728 | 869699 | 800065 | 889185 | 7.7 |
| NW Gas | 689685 | 605684 | 586542 | 582439 | 591310 | 556137 | 601966 | 7.6 |
| 8015Gas | 1455915 | 1351382 | 1309436 | 1264474 | 1268273 | 1179446 | 1304821 | 7.2 |
| \$TFT(Surr) | 45.63636 39.29000 | 42.52273 | 41.85075 | 40.65000 | 40.39098 | 40.27528 | 41.51659 | 5.073 |
| \$BB(Surr) | 33.22727 28.20000 | 31.04545 | 30.40299 | 29.69000 | 29.64662 | 29.08989 | 30.18603 | 5.362 |

<- Indicates %RSD outside limits
Surrogate areas are not included in RF calculation.

Quant Ranges : WA Gas Toluene - nC12
 AK Gas nC6 - nC10
 NW Gas Toluene - Naphthalene
 8015 Gas 2-Methylpentane - 1,2,4-Trimethylbenzene

Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0728a014.d | 28-JUL-2010 13:24 |
| 0728a015.d | 28-JUL-2010 13:50 |
| 0728a016.d | 28-JUL-2010 14:16 |
| 0728a017.d | 28-JUL-2010 14:42 |
| 0728a018.d | 28-JUL-2010 15:08 |
| 0728a019.d | 28-JUL-2010 15:34 |

Surr Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0728a005.d | 28-JUL-2010 09:30 |
| 0728a006.d | 28-JUL-2010 09:56 |
| 0728a007.d | 28-JUL-2010 10:22 |
| 0728a008.d | 28-JUL-2010 10:48 |
| 0728a009.d | 28-JUL-2010 11:14 |
| 0728a010.d | 28-JUL-2010 11:40 |
| 0728a011.d | 28-JUL-2010 12:06 |

6
BETX INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: 072810-2

Project No.: LORA LAKE

Instrument/Det: PID2 /RTX 502-2 PID

Calibration Date: 07/28/10

| COMPOUND | CALIBRATION FACTORS | | | | | MEAN | %RSD |
|--------------|---------------------|-----|-----|-----|-----|------|------|
| | 0.25 | 0.5 | 5 | 25 | 50 | | |
| Benzene | 124 | 116 | 118 | 115 | 116 | | |
| Toluene | 120 | 96 | 102 | 102 | 101 | | |
| Ethylbenzene | 136 | 128 | 110 | 108 | 107 | | |
| M/P-Xylene | 84 | 95 | 101 | 99 | 98 | | |
| O-Xylene | 80 | 110 | 106 | 105 | 102 | | |
| MTBE | 44 | 44 | 42 | 42 | 41 | | |
| TFT(Surr) | 15 | 14 | 14 | 14 | 14 | | |
| BB(Surr) | 62 | 58 | 59 | 58 | 57 | | |

Calibration Files

```

/chem3/pid2.i/072810-2.b/0728a005.d
/chem3/pid2.i/072810-2.b/0728a006.d
/chem3/pid2.i/072810-2.b/0728a007.d
/chem3/pid2.i/072810-2.b/0728a008.d
/chem3/pid2.i/072810-2.b/0728a009.d
/chem3/pid2.i/072810-2.b/0728a010.d
/chem3/pid2.i/072810-2.b/0728a011.d

```

BETX INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: 072810-2

Project No.: LORA LAKE

Instrument/Det: PID2 /RTX 502-2 PID

Calibration Date: 07/28/10

| COMPOUND | CALIBRATION FACTORS | | | | | | |
|--------------|---------------------|-----|------|-------|--|--|--|
| | 100 | 200 | MEAN | %RSD | | | |
| Benzene | 111 | 115 | 116 | 3.40 | | | |
| Toluene | 100 | 106 | 104 | 7.49 | | | |
| Ethylbenzene | 105 | 109 | 115 | 10.66 | | | |
| M/P-Xylene | 98 | 104 | 97 | 6.53 | | | |
| O-Xylene | 102 | 106 | 102 | 9.74 | | | |
| MTBE | 40 | 41 | 42 | 3.83 | | | |
| TFT (Surr) | 14 | 14 | 14 | 2.94 | | | |
| BB (Surr) | 57 | 56 | 58 | 3.45 | | | |

6a
GAS INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

Instrument/Det: PID3.I/RTX 502-2 FID

Project: LORA LAKE

Calibration Date: 28-JUL-2010

SDG No.: RG58-RG78

| Gas Range | RF1 0.1 | RF2 0.25 | RF3 1.0 | RF4 2.5 | RF5 5.0 | RF6 20 | Ave RF | %RSD |
|--------------|----------------------|-------------|------------|------------|------------|-----------|----------|-------|
| WA Gas | 1009250 | 772696 | 761867 | 782843 | 800745 | 839442 | 827807 | 11.2 |
| AK Gas | 1342560 | 1066876 | 1050254 | 1042480 | 1063396 | 1225137 | 1131784 | 10.9 |
| NW Gas | 1102210 | 829838 | 811111 | 828987 | 844316 | 875713 | 882029 | 12.5 |
| 8015Gas | 1959390 | 1600162 | 1564234 | 1551602 | 1571254 | 1738000 | 1664107 | 9.6 |
| \$TFT (Surr) | 78.13636 70.30000 | 73.54545 | 71.97015 | 70.35000 | 70.48120 | 69.03933 | 71.97607 | 4.271 |
| \$BB (Surr) | 48.72727 42.23000 | 43.22727 | 42.49254 | 41.18000 | 42.06767 | 41.53933 | 43.06630 | 5.994 |

<- Indicates %RSD outside limits
Surrogate areas are not included in RF calculation.

Quant Ranges : WA Gas Toluene - nC12
 AK Gas nC6 - nC10
 NW Gas Toluene - Naphthalene
 8015 Gas 2-Methylpentane - 1,2,4-Trimethylbenzene

Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0728a012.d | 28-JUL-2010 11:42 |
| 0728a004.d | 28-JUL-2010 08:07 |
| 0728a005.d | 28-JUL-2010 08:31 |
| 0728a006.d | 28-JUL-2010 08:56 |
| 0728a007.d | 28-JUL-2010 09:20 |
| 0728a008.d | 28-JUL-2010 09:45 |

Surr Calibration Files Analysis Time

| | |
|------------|-------------------|
| 0629a005.d | 29-JUN-2010 07:59 |
| 0629a006.d | 29-JUN-2010 08:24 |
| 0629a007.d | 29-JUN-2010 08:48 |
| 0629a008.d | 29-JUN-2010 09:12 |
| 0629a009.d | 29-JUN-2010 09:37 |
| 0629a010.d | 29-JUN-2010 10:01 |
| 0629a011.d | 29-JUN-2010 10:26 |

6
BETX INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument/Det: PID3 /RTX 502-2 PID

Calibration Date: 06/29/10

| COMPOUND | CALIBRATION FACTORS | | | | | MEAN | %RSD |
|--------------|---------------------|------|------|------|------|------|------|
| | 0.25 | 0.5 | 5 | 25 | 50 | | |
| Benzene | 1564 | 1462 | 1257 | 1240 | 1256 | | |
| Toluene | 1608 | 1252 | 1288 | 1275 | 1275 | | |
| Ethylbenzene | 1404 | 1420 | 1164 | 1185 | 1190 | | |
| M/P-Xylene | 1614 | 1381 | 1314 | 1300 | 1302 | | |
| O-Xylene | 1352 | 1232 | 1295 | 1269 | 1282 | | |
| MTBE | 464 | 288 | 367 | 346 | 348 | | |
| TFT (Surr) | 243 | 220 | 213 | 214 | 217 | | |
| BB (Surr) | 496 | 451 | 434 | 440 | 456 | | |

Calibration Files

/chem3/pid3.i/20100629-1.b/0629a005.d
 /chem3/pid3.i/20100629-1.b/0629a006.d
 /chem3/pid3.i/20100629-1.b/0629a007.d
 /chem3/pid3.i/20100629-1.b/0629a008.d
 /chem3/pid3.i/20100629-1.b/0629a009.d
 /chem3/pid3.i/20100629-1.b/0629a010.d
 /chem3/pid3.i/20100629-1.b/0629a011.d

6
BETX INITIAL CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument/Det: PID3 /RTX 502-2 PID

Calibration Date: 06/29/10

| COMPOUND | CALIBRATION FACTORS | | | | | | |
|--------------|---------------------|-------|-------|-------|-------|-------|-------|
| | 100 | 200 | MEAN | %RSD | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 1220 | 1254 | 1322 | 10.16 | | | |
| Toluene | 1247 | 1294 | 1320 | 9.72 | | | |
| Ethylbenzene | 1152 | 1183 | 1242 | 9.38 | | | |
| M/P-Xylene | 1247 | 1268 | 1346 | 9.29 | | | |
| O-Xylene | 1256 | 1307 | 1285 | 3.02 | | | |
| MTBE | 334 | 343 | 356 | 15.04 | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| TFT(Surr) | 212 | 219 | 220 | 4.94 | | | |
| BB(Surr) | 450 | 463 | 456 | 4.41 | | | |

BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID2/RTX 502-2 PID

Calibration Date: 07/28/10

Init. Calib. Date(s): 07/28/10

Calib. File: 0728A012.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.48 | 7.43 | 7.53 | 23.80 | 25.00 | -4.8 |
| Toluene | 10.09 | 10.04 | 10.14 | 23.79 | 25.00 | -4.8 |
| Ethylbenzene | 12.65 | 12.61 | 12.71 | 22.67 | 25.00 | -9.3 |
| M/P-Xylene | 12.80 | 12.75 | 12.85 | 49.81 | 50.00 | -0.4 |
| O-Xylene | 13.60 | 13.58 | 13.64 | 24.60 | 25.00 | -1.6 |
| MTBE | 5.09 | 5.05 | 5.15 | 24.20 | 25.00 | -3.2 |
| TFT (Surr) | 8.22 | 8.18 | 8.28 | 95.96 | 100.0 | -4.0 |
| BB (Surr) | 14.82 | 14.77 | 14.87 | 97.16 | 100.0 | -2.8 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 28-JUL-2010

SDG No.: RG58-RG78

Lab File Name: 0728a021.d

Inst/Det: PID2.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmt | NomAmt | %D |
|-----------------|---------|---------|--------|-------|
| WAGas (Tol-C12) | 1722903 | 2.99 | 2.50 | 19.5 |
| AKGas (C6-C10) | 2201780 | 2.48 | 2.50 | -1.0 |
| NWGas (Tol-Nap) | 1751023 | 2.91 | 2.50 | 16.4 |
| 8015B (2MP-TMB) | 2869302 | 2.20 | 2.50 | -12.0 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 28-JUL-2010

SDG No.: RG58-RG78

Lab File Name: 0728a021.d

Inst/Det: PID2.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|------|
| Trifluorotol | 68079 | 98.4 | 100.0 | -1.6 |
| Bromoflrbenz | 26233 | 97.3 | 100.0 | -2.7 |

7
 BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID2/RTX 502-2 PID

Calibration Date: 08/06/10

Init. Calib. Date(s): 07/28/10

Calib. File: 0806A002.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.49 | 7.43 | 7.53 | 24.64 | 25.00 | -1.4 |
| Toluene | 10.10 | 10.04 | 10.14 | 24.20 | 25.00 | -3.2 |
| Ethylbenzene | 12.66 | 12.61 | 12.71 | 22.87 | 25.00 | -8.5 |
| M/P-Xylene | 12.80 | 12.75 | 12.85 | 48.19 | 50.00 | -3.6 |
| O-Xylene | 13.61 | 13.58 | 13.64 | 23.97 | 25.00 | -4.1 |
| MTBE | 5.11 | 5.05 | 5.15 | 23.70 | 25.00 | -5.2 |
| TFT (Surr) | 8.24 | 8.18 | 8.28 | 101.0 | 100.0 | 1.0 |
| BB (Surr) | 14.83 | 14.77 | 14.87 | 99.38 | 100.0 | -0.6 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 06-AUG-2010

SDG No.: RG58-~~RG78~~

Lab File Name: 0806a003.d

Inst/Det: PID2.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|------|
| WAGas (Tol-C12) | 1399696 | 2.43 | 2.50 | -2.9 |
| AKGas (C6-C10) | 2176873 | 2.45 | 2.50 | -2.1 |
| NWGas (Tol-Nap) | 1448524 | 2.41 | 2.50 | -3.7 |
| 8015B (2MP-TMB) | 3181324 | 2.44 | 2.50 | -2.5 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 06-AUG-2010

SDG No.: RG58-~~RG78~~

Lab File Name: 0806a003.d

Inst/Det: PID2.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|-----|
| Trifluorotol | 72060 | 102.1 | 100.0 | 2.1 |
| Bromoflrbenz | 29826 | 102.3 | 100.0 | 2.3 |

7
BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID2/RTX 502-2 PID

Calibration Date: 08/06/10

Init. Calib. Date(s): 07/28/10

Calib. File: 0806A014.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.49 | 7.43 | 7.53 | 22.90 | 25.00 | -8.4 |
| Toluene | 10.10 | 10.04 | 10.14 | 21.72 | 25.00 | -13.1 |
| Ethylbenzene | 12.66 | 12.61 | 12.71 | 20.54 | 25.00 | -17.8 |
| M/P-Xylene | 12.81 | 12.75 | 12.85 | 41.48 | 50.00 | -17.0 |
| O-Xylene | 13.61 | 13.58 | 13.64 | 21.02 | 25.00 | -15.9 |
| MTBE | 5.11 | 5.05 | 5.15 | 22.17 | 25.00 | -11.3 |
| TFT (Surr) | 8.24 | 8.18 | 8.28 | 90.81 | 100.0 | -9.2 |
| BB (Surr) | 14.83 | 14.77 | 14.87 | 92.19 | 100.0 | -7.8 |

↑
↑
↑

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 06-AUG-2010

SDG No.: RG58-R678

Lab File Name: 0806a015.d

Inst/Det: PID2.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|------|
| WAGas (Tol-C12) | 1323520 | 2.29 | 2.50 | -8.2 |
| AKGas (C6-C10) | 2081870 | 2.34 | 2.50 | -6.3 |
| NWGas (Tol-Nap) | 1362091 | 2.26 | 2.50 | -9.5 |
| 8015B (2MP-TMB) | 3034332 | 2.33 | 2.50 | -7.0 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 06-AUG-2010

SDG No.: RG58-R678

Lab File Name: 0806a015.d

Inst/Det: PID2.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|------|
| Trifluorotol | 70056 | 95.5 | 100.0 | -4.5 |
| Bromoflrbenz | 29684 | 97.8 | 100.0 | -2.2 |

BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID3/RTX 502-2 PID

Calibration Date: 08/09/10

Init. Calib. Date(s): 06/29/10

Calib. File: 0809A002.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.69 | 7.65 | 7.79 | 23.45 | 25.00 | -6.2 |
| Toluene | 10.27 | 10.24 | 10.38 | 22.92 | 25.00 | -8.3 |
| Ethylbenzene | 12.81 | 12.77 | 12.91 | 22.17 | 25.00 | -11.3 |
| M/P-Xylene | 12.94 | 12.91 | 13.05 | 44.92 | 50.00 | -10.2 |
| O-Xylene | 13.72 | 13.71 | 13.81 | 22.56 | 25.00 | -9.8 |
| MTBE | 5.29 | 5.24 | 5.38 | 24.98 | 25.00 | -0.1 |
| TFT (Surr) | 8.41 | 8.37 | 8.51 | 93.53 | 100.0 | -6.5 |
| BB (Surr) | 14.89 | 14.84 | 14.98 | 94.22 | 100.0 | -5.8 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a003.d

Inst/Det: PID3.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|-------|
| WAGas (Tol-C12) | 1840855 | 2.22 | 2.50 | -11.0 |
| AKGas (C6-C10) | 2410004 | 2.13 | 2.50 | -14.8 |
| NWGas (Tol-Nap) | 1964102 | 2.23 | 2.50 | -10.9 |
| 8015B (2MP-TMB) | 3571983 | 2.15 | 2.50 | -14.1 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a003.d

Inst/Det: PID3.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|-----|
| Trifluorotol | 88646 | 103.3 | 100.0 | 3.3 |
| Bromoflrbenz | 38121 | 103.4 | 100.0 | 3.4 |

BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID3/RTX 502-2 PID

Calibration Date: 08/09/10

Init. Calib. Date(s): 06/29/10

Calib. File: 0809A012.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.71 | 7.65 | 7.79 | 25.22 | 25.00 | 0.9 |
| Toluene | 10.31 | 10.24 | 10.38 | 24.37 | 25.00 | -2.5 |
| Ethylbenzene | 12.84 | 12.77 | 12.91 | 23.87 | 25.00 | -4.5 |
| M/P-Xylene | 12.98 | 12.91 | 13.05 | 47.30 | 50.00 | -5.4 |
| O-Xylene | 13.76 | 13.71 | 13.81 | 24.43 | 25.00 | -2.3 |
| MTBE | 5.30 | 5.24 | 5.38 | 26.13 | 25.00 | 4.5 |
| TFT (Surr) | 8.44 | 8.37 | 8.51 | 91.83 | 100.0 | -8.2 |
| BB (Surr) | 14.91 | 14.84 | 14.98 | 96.66 | 100.0 | -3.3 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a013.d

Inst/Det: PID3.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|------|
| WAGas (Tol-C12) | 2054503 | 2.48 | 2.50 | -0.7 |
| AKGas (C6-C10) | 2717390 | 2.40 | 2.50 | -4.0 |
| NWGas (Tol-Nap) | 2171923 | 2.46 | 2.50 | -1.5 |
| 8015B (2MP-TMB) | 4042380 | 2.43 | 2.50 | -2.8 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a013.d

Inst/Det: PID3.I/RTX 502-2 FID

| Surrogate | Area | CalcAmnt | NomAmnt | RPD |
|--------------|-------|----------|---------|------|
| Trifluorotol | 91799 | 106.5 | 100.0 | 6.5 |
| Bromoflrbenz | 37426 | 110.2 | 100.0 | 10.2 |

BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID3/RTX 502-2 PID

Calibration Date: 08/09/10

Init. Calib. Date(s): 06/29/10

Calib. File: 0809A024.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.72 | 7.65 | 7.79 | 5.163 | 5.326 | -3.0 |
| Toluene | 10.31 | 10.24 | 10.38 | 69.94 | 71.86 | -2.6 |
| Ethylbenzene | 12.84 | 12.77 | 12.91 | 21.37 | 22.91 | -6.7 |
| M/P-Xylene | 12.98 | 12.91 | 13.05 | 76.45 | 84.64 | -9.6 |
| O-Xylene | 13.76 | 13.71 | 13.81 | 33.48 | 35.03 | -4.4 |
| MTBE | 5.31 | 5.24 | 5.38 | 227.0 | 242.4 | -6.3 |
| TFT (Surr) | 8.44 | 8.37 | 8.51 | 93.88 | 100.0 | -6.1 |
| BB (Surr) | 14.91 | 14.84 | 14.98 | 96.29 | 100.0 | -3.7 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a024.d

Inst/Det: PID3.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|------|
| WAGas (Tol-C12) | 1944532 | 2.35 | 2.50 | -6.0 |
| AKGas (C6-C10) | 2595428 | 2.29 | 2.50 | -8.3 |
| NWGas (Tol-Nap) | 2053311 | 2.33 | 2.50 | -6.9 |
| 8015B (2MP-TMB) | 3873074 | 2.33 | 2.50 | -6.9 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a024.d

Inst/Det: PID3.I/RTX 502-2 FID

| Surrogate | Area | CalcAmnt | NomAmnt | RPD |
|--------------|-------|----------|---------|-----|
| Trifluorotol | 87843 | 102.7 | 100.0 | 2.7 |
| Bromoflrbenz | 38342 | 103.7 | 100.0 | 3.7 |

BETX CALIBRATION VERIFICATION SUMMARY

Lab Name: ANALYTICAL RESOURCES, INC Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project No.: LORA LAKE

Instrument/Det: PID3/RTX 502-2 PID

Calibration Date: 08/09/10

Init. Calib. Date(s): 06/29/10

Calib. File: 0809A035.D

| COMPOUND | RT | RT WINDOW | | CALC AMOUNT (ng/mL) | NOM AMOUNT (ng/mL) | %D |
|--------------|-------|-----------|-------|---------------------------|--------------------------|-------|
| | | FROM | TO | | | |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| Benzene | 7.72 | 7.65 | 7.79 | 5.173 | 5.326 | -2.9 |
| Toluene | 10.31 | 10.24 | 10.38 | 69.43 | 71.86 | -3.4 |
| Ethylbenzene | 12.84 | 12.77 | 12.91 | 21.25 | 22.91 | -7.2 |
| M/P-Xylene | 12.98 | 12.91 | 13.05 | 75.74 | 84.64 | -10.5 |
| O-Xylene | 13.76 | 13.71 | 13.81 | 32.76 | 35.03 | -6.5 |
| MTBE | 5.31 | 5.24 | 5.38 | 222.7 | 242.4 | -8.1 |
| TFT (Surr) | 8.44 | 8.37 | 8.51 | 90.00 | 100.0 | -10.0 |
| BB (Surr) | 14.91 | 14.84 | 14.98 | 93.36 | 100.0 | -6.6 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a035.d

Inst/Det: PID3.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|-------|
| WAGas (Tol-C12) | 1873948 | 2.26 | 2.50 | -9.5 |
| AKGas (C6-C10) | 2469808 | 2.18 | 2.50 | -12.7 |
| NWGas (Tol-Nap) | 1979464 | 2.24 | 2.50 | -10.2 |
| 8015B (2MP-TMB) | 3704465 | 2.23 | 2.50 | -11.0 |

* Surrogate areas are subtracted from Total Area
<- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 09-AUG-2010

SDG No.: RG58-RG78

Lab File Name: 0809a035.d

Inst/Det: PID3.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|------|
| Trifluorotol | 83511 | 96.9 | 100.0 | -3.1 |
| Bromoflrbenz | 36034 | 101.0 | 100.0 | 1.0 |

7a
GAS CONTINUING CALIBRATION VERIFICATION

Lab Name: ANALYTICAL RESOURCES, INC.

Client: FLOYD/SNIDER

ICal Date: 28-JUL-2010

Project: LORA LAKE

CCal Date: 28-JUL-2010

SDG No.: RG58-RG78

Lab File Name: 0728a010.d

Inst/Det: PID3.I/RTX 502-2 FID

| Gas Range | Area* | CalcAmnt | NomAmnt | %D |
|-----------------|---------|----------|---------|-------|
| WAGas (Tol-C12) | 2493506 | 3.01 | 2.50 | 20.5 |
| AKGas (C6-C10) | 2858408 | 2.53 | 2.50 | 1.0 |
| NWGas (Tol-Nap) | 2556570 | 2.90 | 2.50 | 15.9 |
| 8015B (2MP-TMB) | 3739886 | 2.25 | 2.50 | -10.1 |

<-

* Surrogate areas are subtracted from Total Area
 <- Indicates an RPD outside QC limits

7b
FID SURROGATE CONTINUING CALIBRATION

Lab Name: ANALYTICAL RESOURCES, INC.

ICal Date: 28-JUL-2010

CCal Date: 28-JUL-2010

Lab File Name: 0728a010.d

Client: ^{FLOYD/SNIDER} LANDAU ASSOCIATES

Project: ^{LOA LAKE} PROJECT STRIKER

SDG No.: ^{RG} ~~RG63~~ RG58 RG78

Inst/Det: PID3.I/RTX 502-2 FID

| Surrogate | Area | CalcAmt | NomAmt | RPD |
|--------------|-------|---------|--------|------|
| Trifluorotol | 85915 | 99.7 | 100.0 | -0.3 |
| Bromoflrbenz | 33856 | 101.1 | 100.0 | 1.1 |

8
BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument ID: PID2

GC Detector: RTX 502-2 FID

Run Date: 07/28/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | | | |
|----------------------|------------------|------------------|------------------|------------|------------|--|--|
| S1 : 8.18 | | S2 : 14.80 | | | | | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # | S2 RT # | | |
| 01 | RINSE | 07/28/10 | 0604 | 8.18 | 14.81 | | |
| 02 | RT+BCAL 1 | 07/28/10 | 0629 | 8.19 | 14.80 | | |
| 03 | GCAL 1 | 07/28/10 | 0655 | 8.19 | 14.80 | | |
| 04 | RINSE | 07/28/10 | 0904 | 8.20 | | | |
| 05 | BETX .25 | 07/28/10 | 0930 | 8.19 | 14.80 | | |
| 06 | BETX .5 | 07/28/10 | 0956 | 8.18 | 14.80 | | |
| 07 | BETX 5 | 07/28/10 | 1022 | 8.18 | 14.80 | | |
| 08 | BETX 25 | 07/28/10 | 1048 | 8.18 | 14.80 | | |
| 09 | BETX 50 | 07/28/10 | 1114 | 8.18 | 14.80 | | |
| 10 | BETX 100 | 07/28/10 | 1140 | 8.18 | 14.80 | | |
| 11 | BETX 200 | 07/28/10 | 1206 | 8.18 | 14.80 | | |
| 12 | BETX ICV | 07/28/10 | 1232 | 8.17 | 14.80 | | |
| 13 | RINSE | 07/28/10 | 1258 | | | | |
| 14 | GAS .1 | 07/28/10 | 1324 | 8.18 | 14.80 | | |
| 15 | GAS .25 | 07/28/10 | 1350 | 8.18 | 14.80 | | |
| 16 | GAS 1 | 07/28/10 | 1416 | 8.18 | 14.80 | | |
| 17 | GAS 2.5 | 07/28/10 | 1442 | 8.18 | 14.80 | | |
| 18 | GAS 5 | 07/28/10 | 1508 | 8.18 | 14.80 | | |
| 19 | GAS 20 | 07/28/10 | 1534 | 8.18 | 14.80 | | |
| 20 | RINSE | 07/28/10 | 1600 | | 14.86 | | |
| 21 | GAS ICV | 07/28/10 | 1626 | 8.18 | 14.80 | | |

QC LIMITS

S1 = TFT(Surr) (+/- 0.07 MINUTES)
S2 = BB(Surr) (+/- 0.07 MINUTES)

* Values outside of QC limits.

BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument ID: PID2

GC Detector: RTX 502-2 PID

Run Date: 08/06/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | | | |
|----------------------|------------------|------------------|------------------|------------|------------|------|-------|
| S1 : 8.23 | | S2 : 14.82 | | | | | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # | S2 RT # | | |
| ===== | ===== | ===== | ===== | ===== | ===== | | |
| 01 | ZZZZZ | ZZZZZ | 08/06/10 | | | | |
| 02 | RT+BCAL 1 | RT+BCAL 1 | 08/06/10 | 0625 | | 8.24 | 14.83 |
| 03 | GCAL 1 | GCAL 1 | 08/06/10 | 0651 | | 8.24 | 14.83 |
| 04 | LCS0806S1 | LCS0806 | 08/06/10 | 0717 | | 8.24 | 14.83 |
| 05 | LCSD0806S1 | LCSD0806 | 08/06/10 | 0743 | | 8.24 | 14.83 |
| 06 | MB0806S1 | MB0806 | 08/06/10 | 0809 | | 8.24 | 14.83 |
| 07 | PSB22-TB | RG58T | 08/06/10 | 0850 | | 8.24 | 14.83 |
| 08 | PSB23-TB | RG58U | 08/06/10 | 0932 | | 8.24 | 14.83 |
| 09 | PSB24-TB | RG58V | 08/06/10 | 0958 | | 8.24 | 14.83 |
| 10 | PSB9-TB | RG78M | 08/06/10 | 1023 | | 8.24 | 14.83 |
| 11 | PSB10-TB | RG78N | 08/06/10 | 1049 | | 8.24 | 14.83 |
| 12 | ZZZZZ | ZZZZZ | 08/06/10 | 1115 | | 8.24 | 14.83 |
| 13 | ZZZZZ | ZZZZZ | 08/06/10 | 1141 | | | |
| 14 | BCAL 2 | BCAL 2 | 08/06/10 | 1207 | | 8.24 | 14.83 |
| 15 | GCAL 2 | GCAL 2 | 08/06/10 | 1233 | | 8.24 | 14.83 |
| 16 | ZZZZZ | ZZZZZ | 08/06/10 | 1259 | | 8.24 | 14.83 |
| 17 | ZZZZZ | ZZZZZ | 08/06/10 | 1325 | | 8.24 | 14.83 |
| 18 | ZZZZZ | ZZZZZ | 08/06/10 | 1351 | | 8.24 | 14.83 |
| 19 | ZZZZZ | ZZZZZ | 08/06/10 | 1417 | | 8.24 | 14.83 |
| 20 | ZZZZZ | ZZZZZ | 08/06/10 | 1443 | | 8.24 | 14.83 |
| 21 | ZZZZZ | ZZZZZ | 08/06/10 | 1509 | | 8.24 | 14.83 |
| 22 | ZZZZZ | ZZZZZ | 08/06/10 | 1535 | | 8.24 | 14.83 |
| 23 | ZZZZZ | ZZZZZ | 08/06/10 | 1601 | | 8.24 | 14.83 |
| 24 | ZZZZZ | ZZZZZ | 08/06/10 | 1627 | | | |
| 25 | ZZZZZ | ZZZZZ | 08/06/10 | 1653 | | 8.24 | 14.83 |
| 26 | ZZZZZ | ZZZZZ | 08/06/10 | 1718 | | 8.25 | 14.83 |
| 27 | ZZZZZ | ZZZZZ | 08/06/10 | 1744 | | 8.24 | 14.83 |
| 28 | ZZZZZ | ZZZZZ | 08/06/10 | 1810 | | 8.24 | 14.83 |
| 29 | ZZZZZ | ZZZZZ | 08/06/10 | 1836 | | 8.24 | 14.83 |
| 30 | ZZZZZ | ZZZZZ | 08/06/10 | 1902 | | 8.24 | 14.83 |
| 31 | ZZZZZ | ZZZZZ | 08/06/10 | 1928 | | 8.24 | 14.83 |
| 32 | ZZZZZ | ZZZZZ | 08/06/10 | 1954 | | 8.24 | 14.83 |

QC LIMITS
S1 = TFT(Surr) (+/- 0.05 MINUTES)
S2 = BB(Surr) (+/- 0.05 MINUTES)

* Values outside of QC limits.

8
BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument ID: PID2

GC Detector: RTX 502-2 PID

Run Date: 08/06/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | | | |
|---------------------|-----------|----------|----------|-----------|-------|------------|-------|
| | | | | S1 : 8.23 | | S2 : 14.82 | |
| CLIENT | LAB | DATE | TIME | S1 | S2 | | |
| SAMPLE NO. | SAMPLE ID | ANALYZED | ANALYZED | RT | RT | # | # |
| ===== | ===== | ===== | ===== | ===== | ===== | ===== | ===== |
| 01 | ZZZZZ | 08/06/10 | 2020 | 8.24 | 14.83 | | |
| 02 | ZZZZZ | 08/06/10 | 2046 | 8.24 | 14.83 | | |
| 03 | ZZZZZ | 08/06/10 | 2112 | | | | |
| 04 | ZZZZZ | 08/06/10 | 2138 | 8.24 | 14.83 | | |
| 05 | ZZZZZ | 08/06/10 | 2204 | 8.24 | 14.82 | | |

QC LIMITS

S1 = TFT(Surr) (+/- 0.05 MINUTES)

S2 = BB(Surr) (+/- 0.05 MINUTES)

* Values outside of QC limits.

BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project: LORA LAKE

Instrument ID: PID3

GC Detector: RTX 502-2 PID

Run Date: 06/29/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | |
|----------------------|------------------|------------------|------------------|------------|------------|
| S1 : 8.44 | | S2 : 14.91 | | | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT # | S2 RT # |
| ===== | ===== | ===== | ===== | ===== | ===== |
| 01 | RINSE | 06/29/10 | 0548 | | |
| 02 | RT+BCAL 1 | 06/29/10 | 0613 | 8.42 | 14.90 |
| 03 | GCAL 1 | 06/29/10 | 0637 | 8.43 | 14.91 |
| 04 | RINSE | 06/29/10 | 0735 | | |
| 05 | BETX .25 | 06/29/10 | 0759 | 8.42 | 14.89 |
| 06 | BETX .5 | 06/29/10 | 0824 | 8.43 | 14.90 |
| 07 | BETX 5 | 06/29/10 | 0848 | 8.43 | 14.91 |
| 08 | BETX 25 | 06/29/10 | 0912 | 8.44 | 14.91 |
| 09 | BETX 50 | 06/29/10 | 0937 | 8.44 | 14.91 |
| 10 | BETX 100 | 06/29/10 | 1001 | 8.44 | 14.91 |
| 11 | BETX 200 | 06/29/10 | 1026 | 8.44 | 14.91 |
| 12 | BETX ICV | 06/29/10 | 1050 | 8.44 | 14.91 |
| 13 | GCAL 2 | 06/29/10 | 1145 | 8.37 | 14.87 |
| 14 | LCS0629 | 06/29/10 | 1210 | 8.42 | 14.89 |
| 15 | LCSD0629 | 06/29/10 | 1234 | 8.43 | 14.90 |
| 16 | MB0629 | 06/29/10 | 1259 | 8.43 | 14.91 |
| 17 | ZZZZZ | 06/29/10 | 1344 | 8.38 | 14.88 |
| 18 | ZZZZZ | 06/29/10 | 1408 | 8.42 | 14.90 |
| 19 | ZZZZZ | 06/29/10 | 1433 | 8.43 | 14.90 |
| 20 | ZZZZZ | 06/29/10 | 1458 | 8.43 | 14.91 |
| 21 | ZZZZZ | 06/29/10 | 1522 | 8.43 | 14.91 |
| 22 | ZZZZZ | 06/29/10 | 1547 | 8.44 | 14.91 |
| 23 | ZZZZZ | 06/29/10 | 1611 | 8.44 | 14.91 |
| 24 | RINSE | 06/29/10 | 1636 | | |
| 25 | BCAL 3 | 06/29/10 | 1700 | 8.44 | 14.91 |
| 26 | GCAL 2 | 06/29/10 | 1725 | 8.44 | 14.91 |

S1 = TFT (Surr) (+/- 0.07 MINUTES)
S2 = BB (Surr) (+/- 0.07 MINUTES)

QC LIMITS

* Values outside of QC limits.

BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58

Project: LORA LAKE

Instrument ID: PID3

GC Detector: RTX 502-2 FID

Run Date: 07/28/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | | | |
|----------------------|------------------|------------------|------------------|----------|---|----------|---|
| S1 : 8.44 | | S2 : 14.91 | | | | | |
| CLIENT SAMPLE NO. | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | S1 RT | # | S2 RT | # |
| 01 | ZZZZZ | 07/28/10 | 0653 | | | 14.86 | |
| 02 | RT+BCAL 1 | 07/28/10 | 0718 | 8.41 | | 14.89 | |
| 03 | ZZZZZ | 07/28/10 | 0742 | 8.43 | | 14.90 | |
| 04 | GAS .25 | 07/28/10 | 0807 | 8.43 | | 14.91 | |
| 05 | GAS 1 | 07/28/10 | 0831 | 8.44 | | 14.91 | |
| 06 | GAS 2.5 | 07/28/10 | 0856 | 8.44 | | 14.91 | |
| 07 | GAS 5 | 07/28/10 | 0920 | 8.44 | | 14.91 | |
| 08 | GAS 20 | 07/28/10 | 0945 | 8.44 | | 14.91 | |
| 09 | ZZZZZ | 07/28/10 | 1009 | | | 14.84 | |
| 10 | GAS ICV | 07/28/10 | 1034 | 8.44 | | 14.91 | |
| 11 | ZZZZZ | 07/28/10 | 1117 | | | 14.93 | |
| 12 | GAS .1 | 07/28/10 | 1142 | 8.43 | | 14.90 | |

QC LIMITS
S1 = TFT(Surr) (+/- 0.07 MINUTES)
S2 = BB(Surr) (+/- 0.07 MINUTES)

* Values outside of QC limits.

8
BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument ID: PID3

GC Detector: RTX 502-2 PID

Run Date: 08/09/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | |
|---------------------|--------------|-----------|---------------|------------|-------|
| | | S1 : 8.44 | | S2 : 14.91 | |
| CLIENT | LAB | DATE | TIME | S1 | S2 |
| SAMPLE NO. | SAMPLE ID | ANALYZED | ANALYZED | RT # | RT # |
| ===== | ===== | ===== | ===== | ===== | ===== |
| 01 | ZZZZZ | ZZZZZ | 08/09/10 0639 | | 14.86 |
| 02 | RT+BCAL 1 | RT+BCAL 1 | 08/09/10 0703 | 8.41 | 14.89 |
| 03 | GCAL 1 | GCAL 1 | 08/09/10 0728 | 8.43 | 14.90 |
| 04 | LCS0809S1 | LCS0809 | 08/09/10 0752 | 8.44 | 14.91 |
| 05 | LCSD0809S1 | LCSD0809 | 08/09/10 0817 | 8.44 | 14.91 |
| 06 | MB0809S1 | MB0809 | 08/09/10 0841 | 8.44 | 14.91 |
| 07 | ZZZZZ | ZZZZZ | 08/09/10 0940 | 8.37* | 14.87 |
| 08 | ZZZZZ | ZZZZZ | 08/09/10 1005 | 8.42 | 14.90 |
| 09 | ZZZZZ | ZZZZZ | 08/09/10 1030 | 8.43 | 14.90 |
| 10 | ZZZZZ | ZZZZZ | 08/09/10 1054 | 8.43 | 14.91 |
| 11 | ZZZZZ | ZZZZZ | 08/09/10 1119 | | |
| 12 | BCAL 2 | BCAL 2 | 08/09/10 1144 | 8.44 | 14.91 |
| 13 | GCAL 2 | GCAL 2 | 08/09/10 1208 | 8.44 | 14.91 |
| 14 | ZZZZZ | ZZZZZ | 08/09/10 1233 | 8.44 | 14.91 |
| 15 | PSB22-17-19- | RG58E | 08/09/10 1258 | 8.44 | 14.91 |
| 16 | PSB22-19-20- | RG58F | 08/09/10 1322 | 8.44 | 14.91 |
| 17 | PSB23-14-16. | RG58K | 08/09/10 1347 | 8.44 | 14.91 |
| 18 | PSB23-16.5-1 | RG58L | 08/09/10 1412 | 8.44 | 14.91 |
| 19 | PSB24-14-16- | RG58R | 08/09/10 1436 | 8.44 | 14.91 |
| 20 | PSB24-16-17- | RG58S | 08/09/10 1501 | 8.44 | 14.91 |
| 21 | PSB9A-11-13. | RG78A | 08/09/10 1525 | 8.44 | 14.91 |
| 22 | PSB9A-1.5-2- | RG78B | 08/09/10 1550 | 8.44 | 14.91 |
| 23 | ZZZZZ | ZZZZZ | 08/09/10 1615 | | |
| 24 | BCAL 3 | GCAL 3 | 08/09/10 1639 | 8.44 | 14.91 |
| 25 | PSB9A-4-6-07 | RG78D | 08/09/10 1704 | 8.44 | 14.91 |
| 26 | PSB10-0-0.5- | RG78F | 08/09/10 1728 | 8.44 | 14.91 |
| 27 | PSB10-2-4-07 | RG78H | 08/09/10 1753 | 8.44 | 14.91 |
| 28 | PSB10-4-6-07 | RG78I | 08/09/10 1817 | 8.44 | 14.91 |
| 29 | PSB10-8.5-10 | RG78J | 08/09/10 1842 | 8.44 | 14.91 |
| 30 | PSB10-8.5-10 | RG78JMS | 08/09/10 1907 | 8.44 | 14.91 |
| 31 | PSB10-8.5-10 | RG78JMSD | 08/09/10 1931 | 8.44 | 14.91 |
| 32 | PSB10-14-15- | RG78K | 08/09/10 1956 | 8.44 | 14.91 |

QC LIMITS

S1 = TFT(Surr) (+/- 0.07 MINUTES)
S2 = BB(Surr) (+/- 0.07 MINUTES)

* Values outside of QC limits.

8
BETX/GAS ANALYTICAL SEQUENCE

Lab Name: ANALYTICAL RESOURCES, INC

Client: FLOYD/SNIDER

SDG No.: RG58-RG78

Project: LORA LAKE

Instrument ID: PID3

GC Detector: RTX 502-2 PID

Run Date: 08/09/10

THE ANALYTICAL SEQUENCE OF BLANKS, SAMPLES, AND STANDARDS,
IS GIVEN BELOW:

| METHOD SURROGATE RT | | | | | |
|---------------------|-----------|------------|----------|-------|-------|
| S1 : 8.44 | | S2 : 14.91 | | | |
| CLIENT | LAB | DATE | TIME | S1 | S2 |
| SAMPLE NO. | SAMPLE ID | ANALYZED | ANALYZED | RT # | RT # |
| ===== | ===== | ===== | ===== | ===== | ===== |
| 01 PSB10-20-25- | RG78L | 08/09/10 | 2020 | 8.44 | 14.91 |
| 02 ZZZZZ | ZZZZZ | 08/09/10 | 2045 | | |
| 03 BCAL 4 | GCAL 4 | 08/09/10 | 2109 | 8.44 | 14.91 |

QC LIMITS

S1 = TFT(Surr) (+/- 0.07 MINUTES)

S2 = BB(Surr) (+/- 0.07 MINUTES)

* Values outside of QC limits.

**Metals Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

Cover Page

INORGANIC ANALYSIS DATA PACKAGE



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58

| CLIENT ID | ARI ID | ARI LIMS ID | REPREP |
|--------------------|------------|-------------|--------|
| PSB22-0-0.5-072910 | RG58A | 10-18236 | |
| PSB22-1.5-2-072910 | RG58B | 10-18237 | |
| PSB22-2-4-072910 | RG58C | 10-18238 | |
| PSB22-4-6-072910 | RG58D | 10-18239 | |
| PSB22-17-19-072910 | RG58E | 10-18240 | |
| PSB22-19-20-072910 | RG58F | 10-18241 | |
| PSB23-0-0.5-072910 | RG58G | 10-18242 | |
| PSB23-1.5-2-072910 | RG58H | 10-18243 | |
| PSB23-2-4-072910 | RG58I | 10-18244 | |
| PSB23-2-4-072910D | RG58IDUP | 10-18244 | |
| PSB23-2-4-072910S | RG58ISPK | 10-18244 | |
| PSB23-4-6-072910 | RG58J | 10-18245 | |
| PBS | RG58MB1 | 10-18245 | |
| LCSS | RG58MB1SPK | 10-18245 | |
| LCSS | RG58REF1 | 10-18245 | |
| PSB23-14-16.5-0729 | RG58K | 10-18246 | |
| PSB23-16.5-19-0729 | RG58L | 10-18247 | |
| PSB24-0-0.5-072910 | RG58M | 10-18248 | |
| PSB24-1.5-2-072910 | RG58N | 10-18249 | |
| PSB24-2-4-072910 | RG58O | 10-18250 | |
| PSB24-2-4-072910-D | RG58P | 10-18251 | |

Were ICP interelement corrections applied ? Yes/No YES

Were ICP background corrections applied ? Yes/No YES

If yes - were raw data generated before application of background corrections ? Yes/No NO

Comments: _____

THIS DATA PACKAGE HAS BEEN REVIEWED AND AUTHORIZED FOR RELEASE BY:

Signature: 

Name: Jay Kuhn

Date: 8/11/10

Title: Inorganic Manager

Cover Page

INORGANIC ANALYSIS DATA PACKAGE



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI


SDG: RG58

| CLIENT ID | ARI ID | ARI LIMS ID | REPREP |
|--------------------|--------|-------------|--------|
| PSB24-4-6-072910 | RG58Q | 10-18252 | |
| PSB24-14-16-072910 | RG58R | 10-18253 | |
| PSB24-16-17-072910 | RG58S | 10-18254 | |

Were ICP interelement corrections applied ? Yes/No YES
Were ICP background corrections applied ? Yes/No YES
If yes - were raw data generated before
application of background corrections ? Yes/No NO

Comments: _____

THIS DATA PACKAGE HAS BEEN REVIEWED AND AUTHORIZED FOR RELEASE BY:

Signature: 

Name: Jay Kuhn

Date: 01/11/10

Title: Inorganic Manager

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: PSB22-0-0.5-072910
SAMPLE

Lab Sample ID: RG58A


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18236

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Percent Total Solids: 93.9%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 7 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB22-1.5-2-072910
SAMPLE

Lab Sample ID: RG58B

LIMS ID: 10-18237

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 93.4%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 7 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB22-2-4-072910

SAMPLE

Lab Sample ID: RG58C

LIMS ID: 10-18238

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 89.3%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 7 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB22-4-6-072910

SAMPLE

Lab Sample ID: RG58D

LIMS ID: 10-18239

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 90.9%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 5 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB22-17-19-072910

SAMPLE

Lab Sample ID: RG58E

LIMS ID: 10-18240

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 86.8%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 6 | 6 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: PSB22-19-20-072910
SAMPLE

Lab Sample ID: RG58F


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18241

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Percent Total Solids: 82.6%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 6 | 6 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB23-0-0.5-072910
SAMPLE

Lab Sample ID: RG58G

LIMS ID: 10-18242

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 92.2%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 7 | |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 49 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB23-1.5-2-072910
SAMPLE

Lab Sample ID: RG58H

LIMS ID: 10-18243

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 92.1%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 8 | |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 25 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB23-2-4-072910

SAMPLE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 92.4%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 6 | |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 17 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB23-2-4-072910

DUPLICATE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

MATRIX DUPLICATE QUALITY CONTROL REPORT

| Analyte | Analysis Method | Sample | Duplicate | RPD | Control Limit | Q |
|---------|-----------------|--------|-----------|-------|---------------|---|
| Arsenic | 6010B | 6 | 7 | 15.4% | +/- 5 | L |
| Lead | 6010B | 17 | 19 | 11.1% | +/- 20% | |

Reported in mg/kg-dry

*-Control Limit Not Met

L-RPD Invalid, Limit = Detection Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB23-2-4-072910
MATRIX SPIKE

Lab Sample ID: RG58I

LIMS ID: 10-18244

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

MATRIX SPIKE QUALITY CONTROL REPORT

| Analyte | Analysis Method | Sample | Spike | Spike Added | % Recovery | Q |
|---------|-----------------|--------|-------|-------------|------------|---|
| Arsenic | 6010B | 6 | 196 | 213 | 89.2% | |
| Lead | 6010B | 17 | 204 | 213 | 87.8% | |

Reported in mg/kg-dry

N-Control Limit Not Met

H-% Recovery Not Applicable, Sample Concentration Too High

NA-Not Applicable, Analyte Not Spiked

Percent Recovery Limits: 75-125%

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB23-4-6-072910
SAMPLE

Lab Sample ID: RG58J

LIMS ID: 10-18245

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 90.8%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 13 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS


Page 1 of 1

Sample ID: PSB23-14-16.5-072910
SAMPLE

Lab Sample ID: RG58K

LIMS ID: 10-18246

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 87.2%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 6 | 6 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 3 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB23-16.5-19-072910

SAMPLE

Lab Sample ID: RG58L

LIMS ID: 10-18247

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 86.1%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 6 | 6 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB24-0-0.5-072910

SAMPLE

Lab Sample ID: RG58M

LIMS ID: 10-18248

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 94.2%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 9 | |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 32 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: PSB24-1.5-2-072910

SAMPLE

Lab Sample ID: RG58N


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18249

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Percent Total Solids: 92.7%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 7 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB24-2-4-072910

SAMPLE

Lab Sample ID: RG580

LIMS ID: 10-18250

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 91.5%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 4 | |

U-Analyte undetected at given RL


RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: PSB24-2-4-072910-D
SAMPLE

Lab Sample ID: RG58P
LIMS ID: 10-18251
Matrix: Soil
Data Release Authorized 
Reported: 08/11/10

QC Report No: RG58-Floyd/Snider
Project: Lora Lake RI
POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10

Percent Total Solids: 91.1%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------------|-------------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 4 | |

U-Analyte undetected at given RL
RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB24-4-6-072910

SAMPLE

Lab Sample ID: RG58Q

LIMS ID: 10-18252

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 92.3%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: PSB24-14-16-072910

SAMPLE

Lab Sample ID: RG58R


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18253

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: 07/29/10

Reported: 08/11/10

Date Received: 07/29/10

Percent Total Solids: 90.7%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 3 | |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: PSB24-16-17-072910

SAMPLE

Lab Sample ID: RG58S

LIMS ID: 10-18254

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: 07/29/10

Date Received: 07/29/10

Percent Total Solids: 86.7%

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1

Sample ID: LAB CONTROL

Lab Sample ID: RG58LCS


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18245

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

BLANK SPIKE QUALITY CONTROL REPORT

| Analyte | Analysis Method | Spike Found | Spike Added | % Recovery | Q |
|----------------|------------------------|--------------------|--------------------|-------------------|----------|
| Arsenic | 6010B | 192 | 200 | 96.0% | |
| Lead | 6010B | 191 | 200 | 95.5% | |

Reported in mg/kg-dry

N-Control limit not met

NA-Not Applicable, Analyte Not Spiked

Control Limits: 80-120%

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Page 1 of 1


Sample ID: STD REFERENCE

ERA D053540

Lab Sample ID: RG58SRM

LIMS ID: 10-18245

Matrix: Soil

Data Release Authorized: 

Reported: 08/11/10

QC Report No: RG58-Floyd/Snider

Project: Lora Lake RI

POS-LLA

Date Sampled: NA

Date Received: NA

| Analyte | Analysis Method | Analysis Date | mg/kg-dry | Certified Value | Advisory Range |
|---------|-----------------|---------------|-----------|-----------------|----------------|
| Arsenic | 6010B | 08/10/10 | 125 | 132 | 106-157 |
| Lead | 6010B | 08/10/10 | 122 | 130 | 106-154 |

INORGANICS ANALYSIS DATA SHEET

TOTAL METALS

Sample ID: METHOD BLANK

Page 1 of 1

Lab Sample ID: RG58MB


QC Report No: RG58-Floyd/Snider

LIMS ID: 10-18245

Project: Lora Lake RI

Matrix: Soil

POS-LLA

Data Release Authorized: 

Date Sampled: NA

Reported: 08/11/10

Date Received: NA

Percent Total Solids: NA

| Prep Meth | Prep Date | Analysis Method | Analysis Date | CAS Number | Analyte | RL | mg/kg-dry | Q |
|-----------|-----------|-----------------|---------------|------------|---------|----|-----------|---|
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7440-38-2 | Arsenic | 5 | 5 | U |
| 3050B | 08/09/10 | 6010B | 08/10/10 | 7439-92-1 | Lead | 2 | 2 | U |

U-Analyte undetected at given RL

RL-Reporting Limit

Calibration Verification

CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58



UNITS: ug/L

| ANALYTE | EL | M | RUN | ICVTV | ICV | %R | CCVTV | CCV1 | %R | CCV2 | %R | CCV3 | %R | CCV4 | %R | CCV5 | %R |
|---------|----|-----|----------|--------|---------|-------|--------|---------|-------|---------|------|---------|------|---------|------|---------|------|
| Arsenic | AS | ICP | IP081021 | 2000.0 | 2015.60 | 100.8 | 2000.0 | 2012.31 | 100.6 | 1979.92 | 99.0 | 1961.33 | 98.1 | 1957.20 | 97.9 | 1933.37 | 96.7 |
| Lead | PB | ICP | IP081021 | 2000.0 | 2008.61 | 100.4 | 2000.0 | 1999.97 | 100.0 | 1970.51 | 98.5 | 1952.89 | 97.6 | 1955.58 | 97.8 | 1927.00 | 96.4 |

Control Limits: Mercury 80-120; Other Metals 90-110

Calibration Verification



CLIENT: Floyd/Snider
 PROJECT: Lora Lake RI
 SDG: RG58

UNITS: ug/L

| ANALYTE | EL | M | RUN | CCVTV | CCV6 | CCV7 | CCV8 | CCV9 | CCV10 | CCV11 | %R | %R | %R | %R | %R |
|---------|----|-----|----------|--------|---------|------|---------|------|---------|-------|---------|------|----|----|----|
| Arsenic | AS | ICP | IP081021 | 2000.0 | 1935.53 | 96.8 | 1897.80 | 94.9 | 1880.79 | 94.0 | 1857.15 | 92.9 | | | |
| Lead | PB | ICP | IP081021 | 2000.0 | 1930.42 | 96.5 | 1909.36 | 95.5 | 1905.42 | 95.3 | 1869.32 | 93.5 | | | |

Control Limits: Mercury 80-120; Other Metals 90-110

CRDI Standard

CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58



UNITS:ug/L

ANALYTE EL M RUN CRA/I TV CR-1 %R CR-2 %R CR-3 %R CR-4 %R CR-5 %R CR-6 %R

| | | | | | | | | | | | | | | |
|---------|----|-----|----------|------|-------|-------|--|--|--|--|--|--|--|--|
| Arsenic | AS | ICP | IP081021 | 50.0 | 51.70 | 103.4 | | | | | | | | |
| Lead | PB | ICP | IP081021 | 20.0 | 19.54 | 97.7 | | | | | | | | |

Control Limits: no control limits have been established by the EPA at this time.

FORM II (2)

Calibration Blanks

CLIENT: Floyd/Snyder

PROJECT: Lora Lake RI

SDG: RG58



UNITS: ug/L

| ANALYTE | EL METH | RUN | CRDL | IDL | ICB | CCB1 | CCB2 | CCB3 | CCB4 | CCB5 | C |
|---------|---------|----------|------|------|------|------|------|------|------|------|---|
| Arsenic | AS ICP | IP081021 | 10.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | U |
| Lead | PB ICP | IP081021 | 3.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | U |

Calibration Blanks



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58

UNITS: ug/L

| ANALYTE | EL | METH | RUN | CRDL | IDL | CCB6 | CCB7 | CCB8 | CCB9 | CCB10 | CCB11 | C |
|---------|----|------|----------|------|------|------|------|------|------|-------|-------|---|
| Arsenic | AS | ICP | IP081021 | 10.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | 50.0 | U |
| Lead | PB | ICP | IP081021 | 3.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | 20.0 | U |

ICP Interference Check Sample



CLIENT: Floyd/Snider

ICS SOURCE: I.V.

PROJECT: Lora Lake RI

RUNID: IP081021

SDG: RG58

INSTRUMENT ID: OPTIMA ICP 1

UNITS: ug/L

| ANALYTE | ICSA TV | ICSAB TV | ICSA1 | ICSAB1 | %R | ICSA2 | ICSAB2 | %R | ICSA3 | ICSAB3 | %R |
|------------|---------|----------|----------|----------|-------|-------|--------|----|-------|--------|----|
| Aluminum | 200000 | 200000 | 205514.2 | 205794.4 | 102.9 | | | | | | |
| Antimony | 1000 | 1000 | -1.7 | 1078.9 | 107.9 | | | | | | |
| Arsenic | 1000 | 1000 | -3.7 | 1008.9 | 100.9 | | | | | | |
| Barium | 1000 | 1000 | 1.4 | 989.0 | 98.9 | | | | | | |
| Beryllium | 1000 | 1000 | -0.1 | 1019.9 | 102.0 | | | | | | |
| Boron | | | 17.8 | 16.7 | | | | | | | |
| Cadmium | 1000 | 1000 | 0.9 | 1018.4 | 101.8 | | | | | | |
| Calcium | 100000 | 100000 | 99640.6 | 100214.8 | 100.2 | | | | | | |
| Chromium | 1000 | 1000 | -0.2 | 1000.3 | 100.0 | | | | | | |
| Cobalt | 1000 | 1000 | 0.8 | 940.6 | 94.1 | | | | | | |
| Copper | 1000 | 1000 | 0.2 | 1089.7 | 109.0 | | | | | | |
| Iron | 200000 | 200000 | 199259.4 | 200028.9 | 100.0 | | | | | | |
| Lead | 1000 | 1000 | 4.1 | 957.0 | 95.7 | | | | | | |
| Magnesium | 100000 | 100000 | 102521.6 | 103533.6 | 103.5 | | | | | | |
| Manganese | 1000 | 1000 | -0.6 | 988.3 | 98.8 | | | | | | |
| Molybdenum | | | 2.4 | 2.5 | | | | | | | |
| Nickel | 1000 | 1000 | -1.1 | 967.7 | 96.8 | | | | | | |
| Potassium | | | -49.6 | -65.7 | | | | | | | |
| Selenium | 1000 | 1000 | -13.1 | 1012.3 | 101.2 | | | | | | |
| Silicon | | | 1.0 | -16.1 | | | | | | | |
| Silver | 1000 | 1000 | 0.3 | 1034.0 | 103.4 | | | | | | |
| Sodium | | | 2.9 | 25.9 | | | | | | | |
| Strontium | | | 3.9 | 4.3 | | | | | | | |
| Thallium | 1000 | 1000 | -29.3 | 941.7 | 94.2 | | | | | | |
| Tin | | | -6.2 | -6.7 | | | | | | | |
| Titanium | | | -1.2 | -2.0 | | | | | | | |
| Vanadium | 1000 | 1000 | 1.7 | 1023.0 | 102.3 | | | | | | |
| Zinc | 1000 | 1000 | -0.5 | 939.4 | 93.9 | | | | | | |

IDLs and ICP Linear Ranges



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58

UNITS: ug/L

| ANALYTE | EL | METH | INSTRUMENT | WAVELENGTH (nm) | GFA | | RL | RL DATE | ICP LINEAR RANGE (ug/L) | ICP LR DATE |
|---------|----|------|--------------|--------------------|-----------------|-------------|------|------------|----------------------------|----------------|
| | | | | | BACK- GROUND | CLP CRDL | | | | |
| Arsenic | AS | ICP | OPTIMA ICP 1 | 188.98 | | 10 | 50.0 | 4/1/2010 | 30000.0 | 1/5/2010 |
| Lead | PB | ICP | OPTIMA ICP 1 | 220.35 | | 3 | 20.0 | 4/1/2010 | 300000.0 | 1/5/2010 |

ICP Interelement Correction Factors



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58

IEC DATE: 7/6/2010

INSTRUMENT ID: OPTIMA ICP 1

| ANALYTE | WAVELENGTH | AL | AS | BA | BE | CA | CD | CO | CR | CU | FE |
|------------|------------|------------|-----------|-----------|----------|------------|----------|------------|------------|-----------|------------|
| Aluminum | 308.22 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Antimony | 206.84 | 0.2355440 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 17.0027000 | 0.000000 | 0.1572420 |
| Arsenic | 188.98 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -1.2352700 | 0.8180370 | 0.000000 | 0.000000 |
| Barium | 233.53 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.1428370 | 0.000000 | 0.000000 | 0.0470802 |
| Beryllium | 313.04 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Cadmium | 228.80 | 0.000000 | 1.8037800 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.0974417 | 0.000000 | 0.000000 | 0.000000 |
| Calcium | 317.93 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Chromium | 267.72 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.0177217 | 0.000000 | -0.1961840 | 0.000000 | 0.000000 | 0.000000 |
| Cobalt | 228.62 | 0.000000 | 0.000000 | 0.2779700 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.0353624 | 0.000000 | -0.0190915 |
| Copper | 324.75 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.3251790 | -0.0447468 | 0.000000 | 0.000000 |
| Iron | 273.96 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.7705580 | 0.000000 | 0.000000 |
| Lead | 220.35 | -0.2816010 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.1815720 | -2.2074600 | 0.7896340 | 0.0656631 |
| Magnesium | 279.08 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -1.1855000 | -0.9151660 | 0.000000 | 0.5909920 |
| Manganese | 257.61 | 0.0066850 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Molybdenum | 202.03 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.0905061 | 0.000000 | 0.000000 |
| Nickel | 231.60 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.3014560 | 0.000000 | 0.000000 | 0.000000 |
| Potassium | 766.49 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Selenium | 196.03 | -0.2017550 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Silicon | 288.16 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.9846030 | 0.000000 | 0.000000 |
| Silver | 328.07 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.0079591 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.0388957 |
| Sodium | 589.59 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 6.6097600 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Thallium | 190.80 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 7.4722900 | 0.3242200 | 0.000000 | 0.000000 |
| Tin | 189.93 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.0541080 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 |
| Titanium | 334.90 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.0390012 | 0.000000 | 0.000000 | 0.2355950 | 0.000000 | 0.000000 |
| Vanadium | 292.40 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -6.3540200 | 0.000000 | 0.1175110 |
| Zinc | 206.20 | 0.000000 | 0.000000 | 0.000000 | 0.000000 | -0.0274712 | 0.000000 | 0.000000 | 0.7506560 | 0.000000 | 0.000000 |

ICP Interelement Correction Factors



CLIENT: Floyd/Snider

PROJECT: Lora Lake RI

SDG: RG58

IEC DATE: 7/6/2010

INSTRUMENT ID: OPTIMA ICP 1

| ANALYTE | WAVELENGTH | MG | MN | MO | NI | PB | SB | TI | TL | V | ZN |
|------------|------------|------------|------------|------------|------------|------------|------------|------------|-----------|------------|-----------|
| Aluminum | 308.22 | 0.000000 | 0.000000 | 21.2545000 | 0.0000000 | 0.0000000 | 0.0000000 | 2.8125800 | 0.0000000 | 15.0921000 | 0.0000000 |
| Antimony | 206.84 | 0.000000 | 0.000000 | 1.0344800 | -0.3070020 | 0.0000000 | 0.0000000 | -1.4160400 | 0.0000000 | -3.8439000 | 0.0000000 |
| Arsenic | 188.98 | 0.000000 | 0.000000 | 2.5244400 | 0.0000000 | 0.0000000 | 0.0000000 | -2.0028700 | 0.0000000 | 0.2321020 | 0.0000000 |
| Barium | 233.53 | 0.000000 | 0.000000 | -0.0807140 | 0.1230910 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.4218910 | 0.0000000 |
| Beryllium | 313.04 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0147106 | 0.0000000 | 2.5747000 | 0.0000000 |
| Cadmium | 228.80 | 0.000000 | 0.000000 | 0.0000000 | -0.2903710 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Calcium | 317.93 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Chromium | 267.72 | 0.0253678 | 0.000000 | 0.1718520 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Cobalt | 228.62 | 0.000000 | 0.000000 | -0.2077620 | 0.1103830 | 0.0000000 | 0.0000000 | 1.7357300 | 0.0000000 | 0.0000000 | 0.0000000 |
| Copper | 324.75 | 0.000000 | 0.000000 | 0.2918050 | 0.0000000 | 0.0000000 | 0.0000000 | 0.2546650 | 0.0000000 | 0.0000000 | 0.0000000 |
| Iron | 273.96 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Lead | 220.35 | 0.000000 | 0.000000 | 0.0000000 | 0.2411010 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Magnesium | 279.08 | 0.000000 | 0.000000 | -2.3243600 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Manganese | 257.61 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | -0.2624450 | 0.0000000 | 0.0000000 | 0.0000000 | -0.0268726 | 0.0000000 |
| Molybdenum | 202.03 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0635115 |
| Nickel | 231.60 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | -0.7106400 | 0.0000000 | 0.5028230 | 0.0000000 | 0.0000000 |
| Potassium | 766.49 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Selenium | 196.03 | 0.000000 | 0.9733860 | 0.0000000 | 1.2234000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Silicon | 288.16 | -0.1332780 | 0.000000 | -1.6690100 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.5486720 | 0.0000000 |
| Silver | 328.07 | 0.000000 | 0.1753400 | 0.1445960 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Sodium | 589.59 | 0.000000 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | -0.2407240 | 0.0000000 |
| Thallium | 190.80 | 0.000000 | 1.3195900 | -1.8108400 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Tin | 189.93 | -0.0277709 | 0.000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 1.6792500 | 0.0000000 | 4.8373400 | 0.0000000 |
| Titanium | 334.90 | 0.000000 | 0.000000 | 0.9543820 | 0.0000000 | 0.0000000 | 0.0000000 | -0.3823320 | 0.0000000 | 0.0000000 | 0.0000000 |
| Vanadium | 292.40 | 0.000000 | -0.1453870 | -6.2931400 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |
| Zinc | 206.20 | -0.0223351 | 0.000000 | 0.2510450 | 0.0000000 | -0.0884182 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 | 0.0000000 |

Preparation Log



CLIENT: Floyd/Snider

ANALYSIS METHOD: ICP

PROJECT: Lora Lake RI

ARI PREP CODE: SWC

SDG: RG58

PREPDATE: 8/9/2010

| CLIENT ID | ARI ID | MASS (g) | INITIAL VOLUME (mL) | FINAL VOLUME (mL) |
|--------------------|------------|----------|---------------------|-------------------|
| PSB22-0-0.5-072910 | RG58A | 1.062 | 0.0 | 50.0 |
| PSB22-1.5-2-072910 | RG58B | 1.016 | 0.0 | 50.0 |
| PSB22-2-4-072910 | RG58C | 1.080 | 0.0 | 50.0 |
| PSB22-4-6-072910 | RG58D | 1.013 | 0.0 | 50.0 |
| PSB22-17-19-072910 | RG58E | 1.029 | 0.0 | 50.0 |
| PSB22-19-20-072910 | RG58F | 1.021 | 0.0 | 50.0 |
| PSB23-0-0.5-072910 | RG58G | 1.053 | 0.0 | 50.0 |
| PSB23-1.5-2-072910 | RG58H | 1.019 | 0.0 | 50.0 |
| PSB23-2-4-072910 | RG58I | 1.022 | 0.0 | 50.0 |
| PSB23-2-4-072910D | RG58IDUP | 1.019 | 0.0 | 50.0 |
| PSB23-2-4-072910S | RG58ISPK | 1.019 | 0.0 | 50.0 |
| PSB23-4-6-072910 | RG58J | 1.047 | 0.0 | 50.0 |
| PSB23-14-16.5-0729 | RG58K | 1.030 | 0.0 | 50.0 |
| PSB23-16.5-19-0729 | RG58L | 1.006 | 0.0 | 50.0 |
| PSB24-0-0.5-072910 | RG58M | 1.026 | 0.0 | 50.0 |
| PBS | RG58MB1 | 1.000 | 0.0 | 50.0 |
| LCSS | RG58MB1SPK | 1.000 | 0.0 | 50.0 |
| PSB24-1.5-2-072910 | RG58N | 1.068 | 0.0 | 50.0 |
| PSB24-2-4-072910 | RG58O | 1.075 | 0.0 | 50.0 |
| PSB24-2-4-072910-D | RG58P | 1.068 | 0.0 | 50.0 |
| PSB24-4-6-072910 | RG58Q | 1.025 | 0.0 | 50.0 |
| PSB24-14-16-072910 | RG58R | 1.031 | 0.0 | 50.0 |
| LCSS | RG58REF1 | 1.004 | 0.0 | 50.0 |
| PSB24-16-17-072910 | RG58S | 1.083 | 0.0 | 50.0 |

Analysis Run Log

CLIENT: Floyd/Snider
 PROJECT: Lora Lake RI
 SDG: RG58
 INSTRUMENT ID: OPTIMA ICP 1
 RUNID: IP081021
 METHOD: ICP
 START DATE: 8/10/2010
 END DATE: 8/10/2010

| CLIENT ID | ARI ID | DIL. | TIME | %R | AG | AL | AS | B | BA | BE | CA | CD | CO | CR | CU | FE | HG | K | MG | MN | MO | NA | NI | PB | SB | SE | SI | SN | TI | TL | U | V | ZN | | | | |
|-----------|------------|------|-------|----|----|----|----|---|----|----|----|----|----|----|----|----|----|---|----|----|----|----|----|----|----|----|----|----|----|----|---|---|----|---|---|---|---|
| S0 | S0 | 1.00 | 11073 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | | | |
| S2 | S2 | 1.00 | 11133 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | | |
| S3 | S3 | 1.00 | 11172 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | | |
| S4 | S4 | 1.00 | 11214 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| S5 | S5 | 1.00 | 11255 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| S0 | S0 | 1.00 | 11391 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ICV | ICV | 1.00 | 11434 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | | |
| ICB | ICB | 1.00 | 11494 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| CRI | CRII | 1.00 | 11554 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ICSA | ICSAI | 1.00 | 12014 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ICSAB | ICSABI | 1.00 | 12075 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | NEWICSA | 1.00 | 12134 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | NEWICSAB | 1.00 | 12200 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| CCV | CCV1 | 1.00 | 12270 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| CCB | CCB1 | 1.00 | 12330 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG62MB1 | 2.00 | 12390 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RH52MB | 5.00 | 12450 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RH52ADUP | 5.00 | 12512 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RH52A | 5.00 | 12574 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RH52ASEPK | 5.00 | 13040 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG60D | 5.00 | 13102 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG62BDUP | 2.00 | 13162 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG62B | 2.00 | 13222 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | ZZZZZZ | 2.00 | 13282 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG62MB1SPK | 2.00 | 13342 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| CCV | CCV2 | 1.00 | 13402 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| CCB | CCB2 | 1.00 | 13462 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X | |
| ZZZZZZ | RG63MB | 1.00 | 13522 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG63A | 1.00 | 13582 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG63B | 1.00 | 14042 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG49G | 1.00 | 14104 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG60B | 2.00 | 14164 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG76Q | 5.00 | 14224 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG76R | 2.00 | 14284 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| ZZZZZZ | RG76S | 2.00 | 14345 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |

Analysis Run Log

CLIENT: Floyd/Snider
 PROJECT: Lora Lake RI
 SDG: RG58
 INSTRUMENT ID: OPTIMA ICP 1
 RUNID: IP081021
 METHOD: ICP
 START DATE: 8/10/2010
 END DATE: 8/10/2010

| CLIENT ID | ARI ID | DIL. | TIME | %R | AG | AL | AS | B | BA | BE | CA | CD | CO | CR | CU | FE | HG | K | MG | MN | MO | NA | NI | PB | SB | SE | SI | SN | TI | TL | U | V | ZN | | | | |
|-----------|-----------|------|------|-------|----|----|----|---|----|----|----|----|----|----|----|----|----|---|----|----|----|----|----|----|----|----|----|----|----|----|---|---|----|--|--|--|--|
| ZZZZZZ | RG62BSPK | | 2.00 | 14405 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG76MBSPK | | 2.00 | 14464 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV3 | | 1.00 | 14524 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB3 | | 1.00 | 14584 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG76MB | | 2.00 | 15233 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82MB | | 1.00 | 15293 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG63C | | 1.00 | 15353 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG63D | | 1.00 | 15413 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG63E | | 1.00 | 15480 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82A | | 1.00 | 15540 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82B | | 1.00 | 16000 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82C | | 1.00 | 16060 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82D | | 1.00 | 16120 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG82MBSPK | | 1.00 | 16180 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | ZZZZZZ | | 1.00 | 16240 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV4 | | 1.00 | 16323 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB4 | | 1.00 | 16384 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62MB | | 2.00 | 16443 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RG76T | | 2.00 | 16503 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55B | | 2.00 | 16564 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55C | | 2.00 | 17024 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62A | | 2.00 | 17084 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62B | | 2.00 | 17143 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62C | | 2.00 | 17202 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62D | | 2.00 | 17261 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62E | | 2.00 | 17320 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH62MBSPK | | 2.00 | 17375 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV5 | | 1.00 | 17435 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB5 | | 1.00 | 17495 | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55MB | | 2.00 | 17543 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55D | | 2.00 | 18003 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55E | | 2.00 | 18064 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55F | | 2.00 | 18124 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55G | | 2.00 | 18184 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55H | | 2.00 | 18244 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Analysis Run Log

CLIENT: Floyd/Snider
 PROJECT: Lora Lake RI
 SDG: RG58
 INSTRUMENT ID: OPTIMA ICP 1
 RUNID: IP081021
 METHOD: ICP
 START DATE: 8/10/2010
 END DATE: 8/10/2010

| CLIENT ID | ARI ID | DIL. | TIME | %R | AG | AL | AS | B | BA | BE | CA | CD | CO | CR | CU | FE | HG | K | MG | MN | MO | NA | NI | PB | SB | SE | SI | SN | TI | TL | U | V | ZN | | | | |
|--------------------|------------|------|-------|----|----|----|----|---|----|----|----|----|----|----|----|----|----|---|----|----|----|----|----|----|----|----|----|----|----|----|---|---|----|--|--|--|--|
| ZZZZZZ | RH55ADUP | 2.00 | 18305 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55A | 2.00 | 18365 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55ASPX | 2.00 | 18425 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55MBSPK | 2.00 | 18484 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV6 | 1.00 | 18544 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB6 | 1.00 | 19004 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55I | 2.00 | 19064 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55J | 2.00 | 19123 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55K | 2.00 | 19182 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55L | 2.00 | 19240 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55M | 2.00 | 19301 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| ZZZZZZ | RH55N | 2.00 | 19361 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-0-0.5-072910 | RG58A | 2.00 | 19421 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-1.5-2-072910 | RG58B | 2.00 | 19482 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-2-4-072910 | RG58C | 2.00 | 19542 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-4-6-072910 | RG58D | 2.00 | 20002 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV7 | 1.00 | 20062 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB7 | 1.00 | 20123 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PBS | RG58MB1 | 2.00 | 20182 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-17-19-072910 | RG58E | 2.00 | 20242 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB22-19-20-072910 | RG58F | 2.00 | 20303 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-0-0.5-072910 | RG58G | 2.00 | 20363 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-1.5-2-072910 | RG58H | 2.00 | 20423 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-2-4-072910D | RG58IDUP | 2.00 | 20483 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-2-4-072910 | RG58I | 2.00 | 20544 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-2-4-072910S | RG58ISPK | 2.00 | 21004 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| LCSS | RG58REF1 | 2.00 | 21063 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| LCSS | RG58MB1SPK | 2.00 | 21122 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCV | CCV8 | 1.00 | 21183 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| CCB | CCB8 | 1.00 | 21243 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-4-6-072910 | RG58J | 2.00 | 21302 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-14-16.5-0729 | RG58K | 2.00 | 21363 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB23-16.5-19-0729 | RG58L | 2.00 | 21423 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB24-0-0.5-072910 | RG58M | 2.00 | 21483 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| PSB24-1.5-2-072910 | RG58N | 2.00 | 21544 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Analysis Run Log



CLIENT: Floyd/Snider
 PROJECT: Lora Lake RI
 SDG: RG58

INSTRUMENT ID: OPTIMA ICP 1
 RUNID: IP081021
 METHOD: ICP

START DATE: 8/10/2010
 END DATE: 8/10/2010


| CLIENT ID | ARI ID | DIL. | TIME | %R | AG | AL | AS | B | BA | BE | CA | CD | CO | CR | CU | FE | HG | K | MG | MN | MO | NA | NI | PB | SB | SE | SI | SN | TI | TL | U | V | ZN | | |
|--------------------|--------|------|-------|----|----|----|----|---|----|----|----|----|----|----|----|----|----|---|----|----|----|----|----|----|----|----|----|----|----|----|---|---|----|--|---|
| PSB24-2-4-072910 | RG580 | 2.00 | 22004 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| PSB24-2-4-072910-D | RG58P | 2.00 | 22064 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| PSB24-4-6-072910 | RG58Q | 2.00 | 22125 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| PSB24-14-16-072910 | RG58R | 2.00 | 22185 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| PSB24-16-17-072910 | RG58S | 2.00 | 22245 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| CCV | CCV9 | 1.00 | 22305 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |
| CCB | CCB9 | 1.00 | 22370 | | | | | X | | | | | | | | | | | | | | | | | | | | | | | | | | | X |

**General Chemistry Analysis
Report and Summary QC Forms**

ARI Job ID: RG58

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB22-17-19-072910
ARI ID: 10-18240 RG58E

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|-------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 86.00 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb, 1981 | Percent | 0.020 | 0.080 |

RL Analytical reporting limit
U Undetected at reported detection limit

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB22-19-20-072910
ARI ID: 10-18241 RG58F

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 83.20 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb,1981 | Percent | 0.020 | 0.078 |

RL Analytical reporting limit
U Undetected at reported detection limit

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB23-14-16.5-072910
ARI ID: 10-18246 RG58K

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|-------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 89.70 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb, 1981 | Percent | 0.020 | 0.290 |

RL Analytical reporting limit
U Undetected at reported detection limit

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB23-16.5-19-072910
ARI ID: 10-18247 RG58L

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 86.90 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb,1981 | Percent | 0.020 | 0.060 |

RL Analytical reporting limit
U Undetected at reported detection limit

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB24-14-16-072910
ARI ID: 10-18253 RG58R

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|-------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 90.80 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb, 1981 | Percent | 0.020 | 0.185 |

RL Analytical reporting limit
U Undetected at reported detection limit

SAMPLE RESULTS-CONVENTIONALS
RG58-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: 07/29/10
Date Received: 07/29/10


Client ID: PSB24-16-17-072910
ARI ID: 10-18254 RG58S

| Analyte | Date | Method | Units | RL | Sample |
|----------------------|----------------------|-------------|---------|-------|--------|
| Total Solids | 07/30/10 073010#1 | EPA 160.3 | Percent | 0.01 | 90.20 |
| Total Organic Carbon | 08/06/10 080610#1 | Plumb, 1981 | Percent | 0.020 | 0.065 |

RL Analytical reporting limit
U Undetected at reported detection limit

METHOD BLANK RESULTS-CONVENTIONALS
RG58-Floyd/Snider




Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: NA
Date Received: NA

| Analyte | Date | Units | Blank |
|----------------------|----------|---------|-----------|
| Total Solids | 07/30/10 | Percent | < 0.01 U |
| Total Organic Carbon | 08/06/10 | Percent | < 0.020 U |

LAB CONTROL RESULTS-CONVENTIONALS
RG58-Floyd/Snider




Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: NA
Date Received: NA

| Analyte/Method | QC ID | Date | Units | LCS | Spike Added | Recovery |
|-------------------------------------|-------|----------|---------|-------|-------------|----------|
| Total Organic Carbon Plumb, 1981 | ICVL | 08/06/10 | Percent | 0.096 | 0.100 | 96.0% |

STANDARD REFERENCE RESULTS-CONVENTIONALS
RG58-Floyd/Snider




Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lake RI
Event: POS-LLA
Date Sampled: NA
Date Received: NA

| Analyte/SRM ID | Date | Units | SRM | True Value | Recovery |
|------------------------------------|----------|---------|------|------------|----------|
| Total Organic Carbon NIST #8704 | 08/06/10 | Percent | 3.22 | 3.35 | 96.1% |

MS/MSD RESULTS-CONVENTIONALS
RG51-Floyd/Snider




Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lakes RI
Event: POS-LLA
Date Sampled: 07/28/10
Date Received: 07/28/10

| Analyte | Date | Units | Sample | Spike | Spike Added | Recovery |
|---|----------|---------|--------|-------|-------------|----------|
| ARI ID: RG51F Client ID: PSB12-14-17-072810 | | | | | | |
| Total Organic Carbon | 08/09/10 | Percent | 0.280 | 1.06 | 0.851 | 91.7% |

REPLICATE RESULTS-CONVENTIONALS
RG51-Floyd/Snider



Matrix: Soil
Data Release Authorized: 
Reported: 08/11/10

Project: Lora Lakes RI
Event: POS-LLA
Date Sampled: 07/28/10
Date Received: 07/28/10

| Analyte | Date | Units | Sample | Replicate(s) | RPD/RSD |
|---|----------|---------|--------|----------------|---------|
| ARI ID: RG51F Client ID: PSB12-14-17-072810 | | | | | |
| Total Solids | 07/30/10 | Percent | 92.50 | 91.80 91.60 | 0.5% |
| Total Organic Carbon | 08/09/10 | Percent | 0.280 | 0.311 0.339 | 9.5% |

Total Solids

ARI Job ID: RG58

Volatiles Total Solids-voats
Data By: Pat Basilio
Created: 8/10/10

Worklist: 1437
Analyst: PAB
Comments:

Oven ID: _____

Balance ID: _____

Samples In: Date: _____ Time: _____ Temp: _____ Analyst: _____

Samples Out: Date: _____ Time: _____ Temp: _____ Analyst: _____

| ARI ID | Tare Wt (g) | Wet Wt (g) | Dry Wt (g) | % Solids |
|-----------------------|----------------|---------------|---------------|----------|
| 1. RG58A 10-18236 | _____ | _____ | _____ | \$ 94.90 |
| 2. RG58B 10-18237 | _____ | _____ | _____ | \$ 92.80 |
| 3. RG58C 10-18238 | _____ | _____ | _____ | \$ 90.80 |
| 4. RG58D 10-18239 | _____ | _____ | _____ | \$ 91.30 |
| 5. RG58E 10-18240 | _____ | _____ | _____ | \$ 87.10 |
| 6. RG58F 10-18241 | _____ | _____ | _____ | \$ 83.20 |
| 7. RG58K 10-18246 | _____ | _____ | _____ | \$ 89.60 |
| 8. RG58L 10-18247 | _____ | _____ | _____ | \$ 86.20 |
| 9. RG58R 10-18253 | _____ | _____ | _____ | \$ 89.20 |
| 10. RG58S 10-18254 | _____ | _____ | _____ | \$ 87.30 |

Extractions Total Solids-exttts
Data By: Woo suk Chang
Created: 8/ 4/10

Worklist: 9610
Analyst: RVR
Comments:

Oven ID: _____

Balance ID: _____

Samples In: Date: _____ Time: _____ Temp: _____ Analyst: _____

Samples Out: Date: _____ Time: _____ Temp: _____ Analyst: _____

| | ARI ID CLIENT ID | Tare Wt (g) | Wet Wt (g) | Dry Wt (g) | % Solids | pH |
|-----|---|----------------|---------------|---------------|----------|----|
| 1. | RG58A 10-18236 PSB22-0-0.5-072910 | 1.18 | 11.96 | 11.41 | 94.9 | NR |
| 2. | RG58B 10-18237 PSB22-1.5-2-072910 | 1.16 | 14.70 | 13.72 | 92.8 | NR |
| 3. | RG58C 10-18238 PSB22-2-4-072910 | 1.18 | 13.75 | 12.59 | 90.8 | NR |
| 4. | RG58D 10-18239 PSB22-4-6-072910 | 1.19 | 11.61 | 10.70 | 91.3 | NR |
| 5. | RG58E 10-18240 PSB22-17-19-072910 | 1.19 | 11.55 | 10.21 | 87.1 | NR |
| 6. | RG58F 10-18241 PSB22-19-20-072910 | 1.16 | 12.01 | 10.19 | 83.2 | NR |
| 7. | RG58G 10-18242 PSB23-0-0.5-072910 | 1.19 | 11.81 | 11.12 | 93.5 | NR |
| 8. | RG58H 10-18243 PSB23-1.5-2-072910 | 1.17 | 13.17 | 12.30 | 92.8 | NR |
| 9. | RG58I 10-18244 PSB23-2-4-072910 | 1.19 | 12.62 | 11.82 | 93.0 | NR |
| 10. | RG58J 10-18245 PSB23-4-6-072910 | 29.13 | 42.60 | 42.13 | 96.5 | NR |
| 11. | RG58K 10-18246 PSB23-14-16.5-072910 | 1.19 | 14.61 | 13.22 | 89.6 | NR |
| 12. | RG58L 10-18247 PSB23-16.5-19-072910 | 1.17 | 12.05 | 10.55 | 86.2 | NR |
| 13. | RG58M 10-18248 PSB24-0-0.5-072910 | 1.18 | 14.41 | 13.77 | 95.2 | NR |

Extractions Total Solids-exttts
Data By: Woo suk Chang
Created: 8/ 4/10

Worklist: 9610
Analyst: RVR
Comments:

Oven ID: _____

Balance ID: _____

Samples In: Date: _____ Time: _____ Temp: _____ Analyst: _____

Samples Out: Date: _____ Time: _____ Temp: _____ Analyst: _____

| | ARI ID CLIENT ID | Tare Wt (g) | Wet Wt (g) | Dry Wt (g) | % Solids | pH |
|-----|---|----------------|---------------|---------------|----------|----|
| 14. | RG58N 10-18249 PSB24-1.5-2-072910 | 1.16 | 14.71 | 13.86 | 93.7 | NR |
| 15. | RG58O 10-18250 PSB24-2-4-072910 | 1.19 | 13.84 | 12.91 | 92.6 | NR |
| 16. | RG58P 10-18251 PSB24-2-4-072910-D | 1.17 | 14.00 | 13.02 | 92.4 | NR |
| 17. | RG58Q 10-18252 PSB24-4-6-072910 | 1.18 | 12.78 | 11.91 | 92.5 | NR |
| 18. | RG58R 10-18253 PSB24-14-16-072910 | 1.17 | 14.87 | 13.39 | 89.2 | NR |
| 19. | RG58S 10-18254 PSB24-16-17-072910 | 1.18 | 13.23 | 11.70 | 87.3 | NR |

Extractions Total Solids-exttts
 Data By: Woo suk Chang
 Created: 8/ 4/10

Worklist: 9610
 Analyst: WC
 Comments:

Oven ID: 015

Balance ID: 21754520

Samples In: Date: 8/4/10 Time: 19:20 Temp: 103 Analyst: WC

Samples Out: Date: 8/4/10 Time: 7:15 Temp: 1050 Analyst: RE

| ARI ID CLIENT ID | Tare Wt (g) | Wet Wt (g) | Dry Wt (g) | % Solids | pH |
|---|---------------------------|----------------------------|---------------------------|----------|----|
| 1. RG58A 10-18236 PSB22-0-0.5-072910 | 1.18 | 11.96 | 11.41 | | NR |
| 2. RG58B 10-18237 PSB22-1.5-2-072910 | 1.16 | 14.70 | 13.72 | | NR |
| 3. RG58C 10-18238 PSB22-2-4-072910 | 1.18 | 13.75 | 12.59 | | NR |
| 4. RG58D 10-18239 PSB22-4-6-072910 | 1.19g | 11.61g | 10.70 | | NR |
| 5. RG58E 10-18240 PSB22-17-19-072910 | 1.19g | 11.55g | 10.21 | | NR |
| 6. RG58F 10-18241 PSB22-19-20-072910 | 1.16g | 12.01g | 10.19 | | NR |
| 7. RG58G 10-18242 PSB23-0-0.5-072910 | 1.19g | 11.81g | 11.12 | | NR |
| 8. RG58H 10-18243 PSB23-1.5-2-072910 | 1.17g | 13.17g | 12.30 | | NR |
| 9. RG58I 10-18244 PSB23-2-4-072910 | 1.19g | 12.62g | 11.82 | | NR |
| 10. RG58J 10-18245 PSB23-4-6-072910 | 1.18g 29.13 | 12.13g 42.60 | 12.35 42.13 | | NR |
| 11. RG58K 10-18246 PSB23-14-16.5-072910 | 1.19 | 14.61 | 13.22 | | NR |
| 12. RG58L 10-18247 PSB23-16.5-19-072910 | 1.17g | 12.05g | 10.55 | | NR |
| 13. RG58M 10-18248 PSB24-0-0.5-072910 | 1.18 | 14.41 | 13.77 | | NR |

Extractions Total Solids-exttts
Data By: Woo suk Chang
Created: 8/ 4/10

Worklist: 9610
Analyst: WC
Comments:

Oven ID: _____

Balance ID: _____

Samples In: Date: _____ Time: _____ Temp: _____ Analyst: _____

Samples Out: Date: _____ Time: _____ Temp: _____ Analyst: _____

| ARI ID CLIENT ID | Tare Wt (g) | Wet Wt (g) | Dry Wt (g) | % Solids | pH |
|---|----------------|---------------|---------------|----------|----|
| 14. RG58N 10-18249 PSB24-1.5-2-072910 | 1.16 | 14.71 | 13.86 | | NR |
| 15. RG58O 10-18250 PSB24-2-4-072910 | 1.19 | 13.84 | 12.91 | | NR |
| 16. RG58P 10-18251 PSB24-2-4-072910-D | 1.17 | 14.00g | 13.02 | | NR |
| 17. RG58Q 10-18252 PSB24-4-6-072910 | 1.18 | 12.78 | 11.91 | | NR |
| 18. RG58R 10-18253 PSB24-14-16-072910 | 1.17 | 14.87 | 13.39 | | NR |
| 19. RG58S 10-18254 PSB24-16-17-072910 | 1.18 | 13.23 | 11.70 | | NR |

Solids Data Entry Report
Date: 08/10/10

Checked by: MH Date: 8/10/10
Data Analyst: KM

Solids Determination performed on 08/09/10 by KM

| JOB | SAMPLE | CLIENTID | TAREWEIGHT | SAMPDISH | DRYWEIGHT | SOLIDS |
|------|--------|--------------------|------------|----------|-----------|--------|
| RG58 | F | PSB22-19-20-072910 | 0.973 | 10.124 | 8.527 | 82.55 |

Solids Data Entry Report
Date: 08/10/10

Checked by: KM Date: 8/10/10
Data Analyst: MH

Solids Determination performed on 08/09/10 by KM

| JOB | SAMPLE | CLIENTID | TAREWEIGHT | SAMPDISH | DRYWEIGHT | SOLIDS |
|------|--------|---------------------|------------|----------|-----------|--------|
| RG58 | A | PSB22-0-0.5-072910 | 0.955 | 10.142 | 9.584 | 93.93 |
| RG58 | B | PSB22-1.5-2-072910 | 0.985 | 10.331 | 9.712 | 93.38 |
| RG58 | C | PSB22-2-4-072910 | 0.962 | 10.099 | 9.123 | 89.32 |
| RG58 | D | PSB22-4-6-072910 | 0.955 | 10.402 | 9.539 | 90.86 |
| RG58 | E | PSB22-17-19-072910 | 1.001 | 10.173 | 8.964 | 86.82 |
| RG58 | F | PSB22-19-20-072910 | 0.973 | 10.124 | 9.527 | 93.48 |
| RG58 | G | PSB23-0-0.5-072910 | 0.978 | 10.066 | 9.354 | 92.17 |
| RG58 | H | PSB23-1.5-2-072910 | 0.948 | 10.131 | 9.409 | 92.14 |
| RG58 | I | PSB23-2-4-072910 | 0.971 | 10.251 | 9.541 | 92.35 |
| RG58 | J | PSB23-4-6-072910 | 0.987 | 10.135 | 9.297 | 90.84 |
| RG58 | K | PSB23-14-16.5-07291 | 0.994 | 10.292 | 9.104 | 87.22 |
| RG58 | L | PSB23-16.5-19-07291 | 0.993 | 10.119 | 8.850 | 86.09 |
| RG58 | M | PSB24-0-0.5-072910 | 0.966 | 10.096 | 9.562 | 94.15 |
| RG58 | N | PSB24-1.5-2-072910 | 0.980 | 10.212 | 9.542 | 92.74 |
| RG58 | O | PSB24-2-4-072910 | 0.960 | 10.141 | 9.358 | 91.47 |
| RG58 | P | PSB24-2-4-072910-D | 0.959 | 10.162 | 9.343 | 91.10 |
| RG58 | Q | PSB24-4-6-072910 | 0.955 | 10.136 | 9.428 | 92.29 |
| RG58 | R | PSB24-14-16-072910 | 0.936 | 10.371 | 9.490 | 90.66 |
| RG58 | S | PSB24-16-17-072910 | 0.992 | 10.317 | 9.075 | 86.68 |



Analytical Resources, Incorporated
Analytical Chemists and Consultants

Total Solids Bench Sheet

Laboratory Section Metals

Oven Identification: 07 Balance ID: 068755
 Samples in Oven: Date: 8/09/10 Time: 1735 Temp: 103°C Analyst: KM
 Removed from Oven: Date: 8/10/10 Time: 0805 Temp: 102°C Analyst: MH
 Source of Total Solids Data If From A Different Lab: _____

| ARI Sample ID | Tare Weight (g) | Tare + Sample Wet (g) | Tare + Sample Dry (g) | Date & Time Last Weight | Final Weighting >12 hrs ¹ |
|---------------|-----------------|-----------------------|-----------------------|-------------------------|--------------------------------------|
| RG58 A | 0.955 | 10.142 | 9.584 | — | ✓ |
| " B | 0.985 | 10.331 | 9.712 | — | ✓ |
| " C | 0.962 | 10.099 | 9.123 | — | ✓ |
| " D | 0.955 | 10.402 | 9.539 | — | ✓ |
| " E | 1.001 | 10.173 | 8.964 | — | ✓ |
| " F | 0.973 | 10.124 | 8.527 | — | ✓ |
| " G | 0.978 | 10.066 | 9.354 | — | ✓ |
| " H | 0.948 | 10.131 | 9.409 | — | ✓ |
| " I | 0.971 | 10.251 | 9.541 | — | ✓ |
| " J | 0.987 | 10.135 | 9.297 | — | ✓ |
| " K | 0.994 | 10.292 | 9.104 | — | ✓ |
| " L | 0.993 | 10.119 | 8.850 | — | ✓ |
| " M | 0.966 | 10.096 | 9.562 | — | ✓ |
| " N | 0.980 | 10.212 | 9.542 | — | ✓ |
| " O | 0.960 | 10.141 | 9.358 | — | ✓ |
| " P | 0.959 | 10.162 | 9.343 | — | ✓ |
| " Q | 0.955 | 10.136 | 9.428 | — | ✓ |
| " R | 0.936 | 10.371 | 9.496 | — | ✓ |
| " S | 0.992 | 10.317 | 9.075 | — | ✓ |
| | | KM | | | |
| | | | | 8/09/10 | |
| <hr/> | | | | | |

1) Place a check mark in this column if samples have dried > 12 but < 24 hours. When samples have been at 104°C < 12 hours, constant weight must be verified as described in SOP 10023S. Use a 2nd bench sheet for additional weightings.

**Volatile Raw Data
Preparation Log**

ARI Job ID: RG58



Analytical Resources, Incorporated
Analytical Chemists and Consultants

Volatile Organics Extraction Bench Sheet

(8260B, 8260B-SIM, 8021, NWTPH-Gx, AK-101, TPH-G, VPH, TCLP-ZHE)

ARI Project No. RG58

Client ID/Project

Extraction Date

MeOH Lot No.

Analyst

1st Extraction:

2nd Extraction:

| Lab ID | Vial No. | Preservative | | Method 5035 Sample Weight | | | | Comments |
|--------------------|----------|--------------------|--------------------|---------------------------|------------------|---------------|----------------|----------|
| | | NaHSO ₃ | CH ₃ OH | Vial Weight | Tare (from vial) | Sample Weight | Extract Volume | |
| MB: | | | | | | | | |
| LCS: | | | | | | | | |
| LCS: | | | | | | | | |
| A | 1 | - | | 44.77 | 35.41 | 9.32 | | |
| B | 2 | - | | 43.56 | 35.42 | 8.14 | | |
| C | 3 | - | | 44.88 | 35.62 | 9.26 | | |
| D | 4 | - | | 44.21 | 35.17 | 9.04 | | |
| E | 5 | - | | 44.49 | 35.17 | 9.32 | | |
| F | 6 | - | | 45.79 | 35.30 | 10.49 | | |
| G | 7 | - | | 48.06 | 35.71 | 12.35 | | |
| H | 8 | - | | 45.19 | 35.27 | 9.92 | | |
| I | 9 | - | | 46.70 | 35.73 | 10.91 | | |
| J | 10 | - | | 47.00 | 35.26 | 11.74 | | |
| K | 11 | | | | | Spill | | |
| L | 12 | | | | | Spill | | |
| M | 13 | | | | | Spill | | |
| N | 14 | | | | | | | |
| | 15 | | | | | | | |
| | 16 | | | | | | | |
| | 17 | | | | | | | |
| | 18 | | | | | | | |
| | 19 | | | | | | | |
| | 20 | | | | | | | |
| Balance ID: | | | | | | | | |

Surrogate: _____

Spike: _____

Solution ID _____

Concentration _____

Amount Spiked _____

Analyst _____

Witness _____

RG58 : 00314



Analytical Resources, Incorporated
Analytical Chemists and Consultants

Volatile Organics Extraction Bench Sheet

8260B, 8260B-SIM, 8021, NWTPH-Gx, AK-101, TPH-G, VPH, TCLP-ZHE)

ARI Project No. PG58

Client ID/Project

Extraction Date

MeOH Lot No.

Analyst W

1st Extraction:

2nd Extraction:

| Lab ID | Vial No. | Preservative | | Method 5035 Sample Weight | | | | | Comments | |
|--------------------|----------|--------------------|--------------------|---------------------------|------------------|---------------|----------------|-------------------|----------|--|
| | | NaHSO ₃ | CH ₃ OH | Vial Weight | Tare (from vial) | Sample Weight | Extract Volume | MeOH Spilt Volume | | |
| MB: | | | | | | | | | | |
| LCS: | | | | | | | | | | |
| LCSD: | | | | | | | | | | |
| 1 | 7 | ✓ | | 47.45 | 35.70 | 11.45 | | | | |
| 2 | | | | | | | | | | |
| 3 | | | | | | | | | | |
| 4 | | | | | | | | | | |
| 5 | | | | | | | | | | |
| 6 | | | | | | | | | | |
| 7 | | | | | | | | | | |
| 8 | | | | | | | | | | |
| 9 | | | | | | | | | | |
| 10 | | | | | | | | | | |
| 11 | | | | | | | | | | |
| 12 | | | | | | | | | | |
| 13 | | | | | | | | | | |
| 14 | | | | | | | | | | |
| 15 | | | | | | | | | | |
| 16 | | | | | | | | | | |
| 17 | | | | | | | | | | |
| 18 | | | | | | | | | | |
| 19 | | | | | | | | | | |
| 20 | | | | | | | | | | |
| Balance ID: | | | | | | | | | | |

Surrogate: _____

Spike: _____

Solution ID

Concentration

Amount Spiked

Analyst

Witness

**Volatile Raw Data
Initial Calibration Notes and Raw Data**

ARI Job ID: RG58



VOA Analyst Notes / Corrective Action Log

ARI Project ID: F5 ical Client ID: _____

ARI SOP: **404S**(Gas) **410S**(BTEX) **430S**(VPH) **700S**(8260C) **703S**(SIM) **706S**(524.2) **710S**(RSK-175)

Parameter(s): _____

Instrument: NT-3 NT-5 NT-7 NT-9 NT-10 PID-1 PID-2 PID-3 FID-6 **FINN-5**

Purge Volume (mL) 5 Curve Date: 7/23/10 Analysis Start Date: 7/23/10

| | | | |
|-----------------------------------|----------------------|----------------------------------|---------------|
| pH ≤ 2.0 | YES / NO / NA | Method Blank In Control? | YES / NO |
| BFB Tune Meets Criteria? | YES / NO / NA | LCS / LCSD Recovery In Control? | YES / NO |
| Internal Standard Meets Criteria? | YES / NO / NA | Surrogate Recovery In Control? | YES / NO |
| ICal acceptable? | YES / NO | CCal acceptable? | YES / NO |
| Q flag applied? | YES / NO / NA | Q flag applied? | YES / NO / NA |
| Manual Integrations for ICal? | YES / NO | Manual Integrations for Samples? | Yes / NO |
| Special Analysis Criteria Met? | YES / NO / NA | | |

Bubbles/Headspace: None SM (≤ 2mm ●) PB (2-4mm) LG (> 4mm ●) Head Space

Detail problems, corrective actions and/or other pertinent information below (use reverse side when necessary):

ICV - brownstone 124.82R
 1,2,4 TCB 75.2R
 1,2,3 TCB 76.72R
 all analytes averaged

Additional Details on Reverse: Yes / **No**

Analyst: [Signature] Date: 7/29/10

Reviewer: [Signature] Date: 7/29/10

Analytical Resources Inc.: Organics Instrument Log

FINN5 Serial No.: 5500-000421A

Date: 7/23/10 Analysis: Staic Analyst: 19
 GC Program: F5 Column No: 82124 Column Type: MTK802L
 Instrument Tune (.U or .CT.): DEF 0723 EM Voltage: 1599
 Calibration File: 2008723 Curve Date: 7/23/10

| IS/SS | Ical/Ccal | LCS/ICV |
|----------------|----------------|----------------|
| <u>w 644-4</u> | <u>w 646-2</u> | <u>w 647-1</u> |
| | <u>w 646-3</u> | <u>w 645-1</u> |
| | | <u>16/rel</u> |
| | | |
| | | |
| | | |

INTERNAL STANDARD SUMMARY FOR DATABATCH - /chem1/finn5.i/23JUL10.b

| Time | Filename | LabID | ClientID | WT |
|---------|------------|---------|----------|--|
| 1 0837 | BFB0723.d | BFB0723 | BFB0723 | 0.00 |
| 2 1648 | BFB07231.d | BFB0723 | BFB0723 | 0.00 |
| 3 1718 | 2000723.d | IC0723 | VSTD200 | 5.00 6.62 159149 7.64 229095 10.79 171495 13.47 145587 |
| 4 1749 | 1500723.d | IC0723 | VSTD150 | 5.00 6.62 155784 7.64 228573 10.78 178614 13.47 122904 |
| 5 1816 | 1000723.d | IC0723 | VSTD100 | 5.00 6.62 135334 7.64 199732 10.78 160631 13.47 96340 |
| 6 1842 | 0500723.d | IC0723 | VSTD050 | 5.00 6.62 131115 7.63 191559 10.78 161199 13.47 88279 |
| 7 1909 | 0100723.d | IC0723 | VSTD010 | 5.00 6.62 118930 7.63 168271 10.78 140990 13.46 72150 |
| 8 1935 | 0050723.d | IC0723 | VSTD005 | 5.00 6.62 117041 7.63 170929 10.78 146260 13.46 75761 |
| 9 2002 | 0020723.d | IC0723 | VSTD002 | 5.00 6.62 125854 7.63 165926 10.78 143906 13.47 73251 |
| 10 2028 | 0010723.d | IC0723 | VSTD001 | 5.00 6.61 113813 7.63 168346 10.77 142296 13.46 71616 |
| 11 2214 | ICV0723.d | ICV0723 | ICV0723 | 5.00 6.62 130699 7.64 194200 10.78 160989 13.47 90026 |

[Handwritten signature]

Maintenance / Comments

Maintenance Verification (Identify ICal or CCal that demonstrates the instrument is in control):
 Every line must contain information or be lined out. Make all entries legible. Start a new page for each QC period.

MANUAL INTEGRATION SUMMARY FOR DATABATCH - /chem1/finn5.i/23JUL10.b

ARI Job No.: BFB0 Method: bfb8260.m Instrument: finn5.i Date: 23-JUL-2010

| Time | Filename | LabID | ClientID | DF | Manually Integrated Compounds |
|------|------------|---------|----------|----|---|
| 1648 | BFB07231.d | BFB0723 | BFB0723 | 1 | NO MANUAL INTEGRATION |
| 1718 | 2000723.d | IC0723 | VSTD200 | 1 | NO MANUAL INTEGRATION |
| 1749 | 1500723.d | IC0723 | VSTD150 | 1 | NO MANUAL INTEGRATION |
| 1816 | 1000723.d | IC0723 | VSTD100 | 1 | NO MANUAL INTEGRATION |
| 1842 | 0500723.d | IC0723 | VSTD050 | 1 | NO MANUAL INTEGRATION |
| 1909 | 0100723.d | IC0723 | VSTD010 | 1 | NO MANUAL INTEGRATION |
| 1935 | 0050723.d | IC0723 | VSTD005 | 1 | 2-Hexanone, Trans-1,4-Dichloro 2-Butene, |
| 2002 | 0020723.d | IC0723 | VSTD002 | 1 | Acetone, 2-Hexanone, 1,2,3-Trichloropropane, Trans-1,4-Dichloro 2-Butene, |
| 2028 | 0010723.d | IC0723 | VSTD001 | 1 | Acetone, 1,1,1-Trichloroethane, 2-Hexanone, 1,1,2,2-Tetrachloroethane, 1,2,3-Trichloropropane, Trans-1,4-Dichloro 2-Butene, |
| 2214 | ICV0723.d | ICV0723 | ICV0723 | 1 | NO MANUAL INTEGRATION |

Date : 23-JUL-2010 16:48

Client ID: BFB0723

Instrument: finn5.i

Sample Info: BFB0723,BFB0723,,1,23JUL10,,


Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

1 Bromofluorobenzene

Handwritten signature: j7/paho



| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 95 | Base Peak, 100% relative abundance | 100.00 |
| 50 | 8.00 - 40.00% of mass 95 | 24.73 |
| 75 | 30.00 - 66.00% of mass 95 | 49.06 |
| 96 | 5.00 - 9.00% of mass 95 | 7.07 |
| 173 | Less than 2.00% of mass 174 | 0.16 (0.21) |
| 174 | 50.00 - 101.00% of mass 95 | 77.38 |
| 175 | 4.00 - 9.00% of mass 174 | 5.70 (7.37) |
| 176 | 93.00 - 101.00% of mass 174 | 76.42 (98.77) |
| 177 | 5.00 - 9.00% of mass 176 | 5.51 (7.21) |

Date : 23-JUL-2010 16:48

Client ID: BFB0723

Instrument: finn5.i

Sample Info: BFB0723,BFB0723,,1,23JUL10,,

Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

Data File: BFB07231.d

Spectrum: Average Spectrum: 12.080 to 12.100 min. (SUB)

Location of Maximum: 95.00

Number of points: 55

| m/z | Y | m/z | Y | m/z | Y | m/z | Y |
|-------|------|-------|------|-------|------|--------|-------|
| 34.00 | 41 | 55.00 | 28 | 74.00 | 2174 | 95.00 | 12792 |
| 36.00 | 159 | 56.00 | 184 | 75.00 | 6276 | 96.00 | 905 |
| 37.00 | 938 | 57.00 | 440 | 76.00 | 565 | 117.00 | 17 |
| 38.00 | 936 | 60.00 | 91 | 77.00 | 77 | 119.00 | 25 |
| 39.00 | 400 | 61.00 | 624 | 78.00 | 18 | 141.00 | 28 |
| 40.00 | 260 | 62.00 | 625 | 79.00 | 363 | 143.00 | 45 |
| 44.00 | 96 | 63.00 | 460 | 80.00 | 109 | 145.00 | 24 |
| 45.00 | 144 | 64.00 | 38 | 81.00 | 331 | 172.00 | 26 |
| 47.00 | 178 | 65.00 | 22 | 82.00 | 62 | 173.00 | 21 |
| 48.00 | 81 | 68.00 | 1416 | 87.00 | 469 | 174.00 | 9898 |
| 49.00 | 708 | 69.00 | 1407 | 88.00 | 387 | 175.00 | 729 |
| 50.00 | 3164 | 70.00 | 64 | 92.00 | 317 | 176.00 | 9776 |
| 51.00 | 905 | 72.00 | 18 | 93.00 | 542 | 177.00 | 705 |
| 52.00 | 33 | 73.00 | 511 | 94.00 | 1387 | | |

Data File: /chem1/finn5.i/23JUL10.b/BFB07231.d

Date: 23-JUL-2010 16:48

Client ID: BFB0723

Sample Info: BFB0723,BFB0723,,1,23JUL10,,


Column phase: RTX502.2

Instrument: finn5.i

Operator: PB

Column diameter: 0.18

/chem1/finn5.i/23JUL10.b/BFB07231.d/BFB07231.LG



Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

Calibration File Names:
 Level 1: /chem1/finn5.i/23JUL10.b/0010723.d
 Level 2: /chem1/finn5.i/23JUL10.b/0020723.d
 Level 3: /chem1/finn5.i/23JUL10.b/0050723.d
 Level 4: /chem1/finn5.i/23JUL10.b/0100723.d
 Level 5: /chem1/finn5.i/23JUL10.b/0500723.d
 Level 6: /chem1/finn5.i/23JUL10.b/1000723.d
 Level 7: /chem1/finn5.i/23JUL10.b/1500723.d
 Level 8: /chem1/finn5.i/23JUL10.b/2000723.d

f 7/2010

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|---------------------------|---------|---------|---------|---------|---------|---------|---------|----------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 1 Dichlorodifluoromethane | 0.61856 | 0.69160 | 0.65985 | 0.63344 | 0.67493 | 0.67442 | | |
| | 0.63254 | 0.60144 | | | | | 0.64835 | 4.860 |
| 2 Chloromethane | 2.15529 | 1.96152 | 1.91728 | 2.00912 | 1.65244 | 1.56576 | | |
| | 1.38789 | 1.30591 | | | | | 1.74440 | 17.810 |
| 3 Vinyl Chloride | 1.51916 | 1.45247 | 1.51314 | 1.59745 | 1.36296 | 1.35754 | | |
| | 1.17136 | 1.06143 | | | | | 1.37944 | 13.295 |
| 4 Bromomethane | 0.93443 | 0.85086 | 0.77665 | 0.62524 | 0.81039 | 0.76904 | | |
| | 0.64701 | 0.57949 | | | | | 0.74914 | 16.282 |
| 181 Ethyl Ether | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | | |
| | +++++ | +++++ | | | | | +++++ | +++++ <- |
| 5 Chloroethane | 1.07062 | 1.09297 | 0.98777 | 0.87106 | 0.87644 | 0.77822 | | |
| | 0.62883 | +++++ | | | | | 0.90084 | 18.341 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|---|---------|---------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 6 Trichlorofluoromethane | 1.47611 | 1.55864 | 1.50469 | 1.41033 | 1.42641 | 1.27999 | | |
| | 1.04222 | 0.96730 | | | | | 1.33321 | 16.450 |
| 7 Acrolein | 0.20463 | 0.19693 | 0.17700 | 0.16354 | 0.15712 | 0.14591 | | |
| | 0.11901 | ++++ | | | | | 0.16631 | 17.814 |
| 8 1,1,2-Trichloro-1,2,2-Trifluoroethane | 1.27446 | 1.18209 | 1.20394 | 1.12348 | 1.01422 | 0.97608 | | |
| | 0.81784 | 0.75797 | | | | | 1.04376 | 17.834 |
| 9 Acetone | 0.30796 | 0.31971 | 0.31370 | 0.30116 | 0.26843 | 0.24372 | | |
| | 0.20402 | ++++ | | | | | 0.27982 | 15.417 |
| 10 1,1-Dichloroethene | 1.03591 | 1.01895 | 1.04143 | 1.03174 | 0.97906 | 0.93375 | | |
| | 0.79718 | 0.73915 | | | | | 0.94715 | 12.366 |
| 11 Bromoethane | 0.70730 | 0.74361 | 0.72880 | 0.75267 | 0.72730 | 0.72722 | | |
| | 0.63319 | 0.59114 | | | | | 0.70140 | 8.233 |
| 12 Iodomethane | 1.01087 | 1.06621 | 1.14259 | 1.14012 | 1.25306 | 1.25553 | | |
| | 1.06567 | 1.02480 | | | | | 1.11986 | 8.526 |
| 13 Methylene Chloride | ++++ | 1.39659 | 1.18975 | 1.12760 | 0.93514 | 0.92898 | | |
| | 0.82084 | ++++ | | | | | 1.06648 | 19.864 |
| 14 Acrylonitrile | 0.19594 | 0.24276 | 0.28315 | 0.28492 | 0.26101 | 0.25835 | | |
| | 0.23046 | 0.21983 | | | | | 0.24705 | 12.529 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|-----------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|---------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 16 Methyl tert-Butyl Ether | 1.39176 1.31326 | 1.48204 1.15084 | 1.61653 | 1.63134 | 1.52463 | 1.54183 | 1.45653 | 11.218 |
| 15 Carbon Disulfide | 3.37220 2.18562 | 3.30955 1.91323 | 3.39522 | 3.28180 | 3.17583 | 2.86693 | 2.93755 | 19.647 |
| 17 Trans-1,2-Dichloroethene | 0.81493 0.76581 | 0.82496 0.72223 | 0.80638 | 0.89481 | 0.79365 | 0.83461 | 0.80717 | 6.268 |
| 18 Vinyl Acetate | 1.37858 1.19699 | 1.47513 1.05617 | 1.52895 | 1.55974 | 1.56063 | 1.55351 | 1.41371 | 13.515 |
| 19 1,1-Dichloroethane | 1.59340 1.25502 | 1.57720 1.06889 | 1.61593 | 1.67405 | 1.53370 | 1.56119 | 1.48492 | 14.111 |
| 179 Hexane | ++++ ++++ | ++++ ++++ | ++++ | ++++ | ++++ | ++++ | ++++ | ++++ <- |
| 20 2-Butanone | 0.32659 0.26832 | 0.32955 0.24668 | 0.34359 | 0.35332 | 0.32770 | 0.32306 | 0.31485 | 11.826 |
| 21 2,2-Dichloropropane | 0.88742 0.87622 | 0.89660 0.85519 | 0.93309 | 0.95140 | 0.91310 | 0.95603 | 0.90863 | 3.989 |
| 22 Cis-1,2-Dichloroethene | 0.70291 0.68699 | 0.70218 0.68958 | 0.71753 | 0.75872 | 0.69175 | 0.74171 | 0.71142 | 3.685 |

Analytical Resources, Inc.
 INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|--------------------------|---------|---------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 24 Chloroform | 1.24898 | 1.29560 | 1.31578 | 1.31952 | 1.20276 | 1.23393 | | |
| | 1.07329 | 0.95949 | | | | | 1.20617 | 10.579 |
| 26 Bromochloromethane | 0.30137 | 0.32304 | 0.36688 | 0.35714 | 0.33542 | 0.35133 | | |
| | 0.33200 | 0.33497 | | | | | 0.33777 | 6.124 |
| 27 1,1,1-Trichloroethane | 0.97660 | 0.93458 | 0.97291 | 0.98520 | 0.93283 | 0.96160 | | |
| | 0.87853 | 0.86280 | | | | | 0.93813 | 4.889 |
| 182 1-Butanol | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ |
| 29 1,1-Dichloropropene | 0.66975 | 0.69007 | 0.71193 | 0.76499 | 0.67325 | 0.69499 | | |
| | 0.63130 | 0.59559 | | | | | 0.67899 | 7.511 |
| 30 Carbon Tetrachloride | 0.58124 | 0.62407 | 0.60370 | 0.63020 | 0.57050 | 0.59224 | | |
| | 0.55109 | 0.57045 | | | | | 0.59044 | 4.670 |
| 32 1,2-Dichloroethane | 0.57115 | 0.62874 | 0.63301 | 0.67822 | 0.58611 | 0.59776 | | |
| | 0.54427 | 0.52926 | | | | | 0.59607 | 8.280 |
| 33 Benzene | 1.75947 | 1.76841 | 1.80022 | 1.96537 | 1.65649 | 1.45472 | | |
| | 1.08835 | +++++ | | | | | 1.64186 | 17.603 |
| 180 Isooctane | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ |
| | +++++ | +++++ | | | | | +++++ | +++++ |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|---------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 35 Trichloroethene | 0.43601 0.44820 | 0.49962 0.46107 | 0.50986 | 0.54002 | 0.46846 | 0.48511 | 0.48104 | 7.173 |
| 36 1,2-Dichloropropane | 0.52451 0.47045 | 0.52147 0.47472 | 0.54818 | 0.58228 | 0.50133 | 0.51755 | 0.51756 | 7.121 |
| 38 1,4-Dioxane | ++++ ++++ | ++++ ++++ | ++++ | ++++ | ++++ | ++++ | ++++ | ++++ <- |
| 37 Bromodichloromethane | 0.52125 0.51592 | 0.59258 0.51411 | 0.58170 | 0.60376 | 0.54255 | 0.55496 | 0.55335 | 6.471 |
| 39 Dibromomethane | 0.25305 0.23699 | 0.25915 0.24918 | 0.25993 | 0.28772 | 0.24894 | 0.26038 | 0.25692 | 5.717 |
| 40 2-Chloroethyl Vinyl Ether | ++++ 0.18677 | 0.14178 0.19813 | 0.17329 | 0.18981 | 0.18519 | 0.19380 | 0.18125 | 10.524 |
| 41 4-Methyl-2-Pentanone | 0.14149 0.12187 | 0.13693 0.11715 | 0.13232 | 0.14268 | 0.13289 | 0.13206 | 0.13218 | 6.720 |
| 42 Cis 1,3-dichloropropene | 0.50313 0.61950 | 0.56652 0.56997 | 0.59990 | 0.66027 | 0.63768 | 0.67623 | 0.60415 | 9.387 |
| 28 Cyclohexane | ++++ ++++ | ++++ ++++ | ++++ | ++++ | ++++ | ++++ | ++++ | ++++ <- |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 44 Toluene | 1.25664 0.78347 | 1.10456 0.70675 | 1.02224 | 1.05184 | 0.92146 | 0.94617 | 0.97414 | 18.057 |
| 45 Trans 1,3-Dichloropropene | 0.44640 0.52387 | 0.47190 0.50804 | 0.49114 | 0.54059 | 0.52142 | 0.55921 | 0.50782 | 7.254 |
| 46 2-Hexanone | 0.48863 +++++ | 0.41802 +++++ | 0.40375 | 0.43814 | 0.38146 | 0.32234 | 0.40872 | 13.652 |
| 47 1,1,2-Trichloroethane | 0.26879 0.29114 | 0.29516 0.30558 | 0.32288 | 0.33895 | 0.29564 | 0.30800 | 0.30327 | 6.989 |
| 48 1,3-Dichloropropane | 0.68343 0.67642 | 0.71401 0.68404 | 0.71469 | 0.75583 | 0.67765 | 0.72373 | 0.70372 | 4.007 |
| 49 Tetrachloroethene | 0.61667 0.54309 | 0.52708 0.59035 | 0.56488 | 0.56674 | 0.48964 | 0.54556 | 0.55550 | 6.995 |
| 50 Chlorodibromomethane | 0.42693 0.47878 | 0.43952 0.52825 | 0.46540 | 0.50238 | 0.45273 | 0.49329 | 0.47341 | 7.173 |
| 51 1,2-Dibromoethane | 0.30087 0.30873 | 0.32786 0.32362 | 0.33839 | 0.34926 | 0.32203 | 0.32796 | 0.32484 | 4.715 |
| 53 Chlorobenzene | 1.44874 0.98203 | 1.25551 0.92990 | 1.21469 | 1.28463 | 1.09325 | 1.17322 | 1.17275 | 14.376 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|--------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 0.48807 0.43874 | 0.46350 0.49165 | 0.43819 | 0.45358 | 0.38926 | 0.42774 | 0.44884 | 7.446 |
| 54 Ethyl Benzene | 2.20280 1.34210 | 2.17625 +++++ | 2.08813 | 2.26814 | 2.02082 | 1.78412 | 1.98319 | 16.336 |
| 56 m,p-xylene | 0.68572 0.64714 | 0.70089 0.61656 | 0.75629 | 0.82054 | 0.76759 | 0.80414 | 0.72486 | 10.182 |
| 57 o-Xylene | 0.59735 0.82834 | 0.67179 0.86537 | 0.70053 | 0.77321 | 0.74982 | 0.84040 | 0.75335 | 12.283 |
| 58 Styrene | 1.01338 1.12721 | 1.04252 1.09402 | 1.15090 | 1.32066 | 1.22803 | 1.34186 | 1.16482 | 10.471 |
| 59 Isopropyl Benzene | 3.58090 2.07611 | 3.46378 +++++ | 3.66983 | 4.08053 | 3.63628 | 3.05286 | 3.36576 | 19.154 |
| 60 Bromoform | 0.58786 0.49959 | 0.56177 0.47363 | 0.56335 | 0.58351 | 0.52086 | 0.53868 | 0.54116 | 7.521 |
| 61 1,1,1,2,2-Tetrachloroethane | 1.19875 0.77962 | 1.12388 0.70704 | 1.03602 | 1.12613 | 0.91700 | 0.89056 | 0.97237 | 18.199 |
| 63 1,2,3-Trichloropropane | +++++ 0.16039 | 0.22594 0.14626 | 0.22109 | 0.22654 | 0.18550 | 0.18274 | 0.19264 | 16.965 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|--------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 65 Trans-1,4-Dichloro 2-Butene | ++++ 0.25759 | 0.32184 0.23740 | 0.32576 | 0.34893 | 0.30143 | 0.29907 | 0.29886 | 13.135 |
| 66 N-Propyl Benzene | 4.35587 ++++ | 4.36240 ++++ | 4.59339 | 5.13243 | 4.29164 | 3.33374 | 4.34491 | 13.450 |
| 67 Bromobenzene | 0.97674 0.87178 | 0.93719 0.81723 | 0.97174 | 1.05787 | 0.91718 | 0.95651 | 0.93828 | 7.723 |
| 68 1,3,5-Trimethyl Benzene | 2.66281 1.92105 | 2.66686 ++++ | 2.91760 | 3.22571 | 2.99783 | 2.73312 | 2.73214 | 15.058 |
| 69 2-Chloro Toluene | 3.12291 1.97970 | 2.80576 ++++ | 3.07335 | 3.37221 | 2.80971 | 2.82080 | 2.85492 | 15.393 |
| 70 4-Chloro Toluene | 2.62581 1.85746 | 2.91088 ++++ | 2.87998 | 3.29757 | 2.95871 | 2.62567 | 2.73658 | 16.426 |
| 71 T-Butyl Benzene | 2.25508 1.95835 | 2.38597 1.46344 | 2.57296 | 2.86417 | 2.63858 | 2.56035 | 2.33736 | 19.065 |
| 72 1,2,4-Trimethylbenzene | 2.43800 1.98513 | 2.54502 ++++ | 2.85134 | 3.25960 | 2.94781 | 2.80039 | 2.68961 | 15.258 |
| 73 S-Butyl Benzene | 3.65072 ++++ | 3.68903 ++++ | 3.98398 | 4.45398 | 4.03139 | 3.26306 | 3.84536 | 10.568 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|--------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|---------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 74 4-Isopropyl Toluene | 2.22576 2.00557 | 2.54160 ++++ | 2.82348 | 3.17997 | 2.94657 | 2.74678 | 2.63853 | 15.583 |
| 75 1,3-Dichlorobenzene | 1.56180 1.47885 | 1.53308 1.21428 | 1.67395 | 1.91240 | 1.64575 | 1.80399 | 1.60301 | 13.256 |
| 64 Cyclohexanone | ++++ ++++ | ++++ ++++ | ++++ | ++++ | ++++ | ++++ | ++++ | ++++ <- |
| 77 1,4-Dichlorobenzene | 1.65466 1.48449 | 1.57267 1.20781 | 1.70259 | 1.83867 | 1.59685 | 1.77492 | 1.60408 | 12.218 |
| 178 1,2,3-Trimethylbenzene | ++++ ++++ | ++++ ++++ | ++++ | ++++ | ++++ | ++++ | ++++ | ++++ <- |
| 78 N-Butyl Benzene | 2.81013 1.94473 | 2.76549 ++++ | 3.04510 | 3.43035 | 3.10253 | 2.84626 | 2.84923 | 16.127 |
| 80 1,2-Dichlorobenzene | 1.53737 1.40066 | 1.60237 1.15636 | 1.63752 | 1.74962 | 1.51750 | 1.58654 | 1.52349 | 11.753 |
| 81 1,2-Dibromo 3-Chloropropane | 0.15220 0.13717 | 0.20921 0.12795 | 0.18954 | 0.20055 | 0.17137 | 0.15806 | 0.16826 | 17.597 |
| 82 1,2,4-Trichlorobenzene | 0.96487 0.82523 | 1.01671 0.73938 | 0.97082 | 1.12640 | 0.86020 | 0.91319 | 0.92710 | 12.980 |

Analytical Resources, Inc.

INITIAL CALIBRATION DATA

Start Cal Date : 23-JUL-2010 17:18
 End Cal Date : 23-JUL-2010 20:28
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem1/finn5.i/23JUL10.b/s8260b.m
 Cal Date : 26-Jul-2010 09:12 patrickb
 Curve Type : Average

| Compound | 1.000 | 2.000 | 5.000 | 10.000 | 50.000 | 100.000 | RRF | % RSD |
|------------------------------|--------------------|--------------------|---------|---------|---------|---------|---------|--------|
| | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | | |
| | 150.000 | 200.000 | | | | | | |
| | Level 7 | Level 8 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 0.58506 0.55357 | 0.68805 0.54187 | 0.68940 | 0.75107 | 0.58913 | 0.59714 | 0.62441 | 12.059 |
| 84 Naphthalene | 1.71610 1.28695 | 1.75595 +++++ | 1.74219 | 2.09362 | 1.61770 | 1.55845 | 1.68157 | 14.468 |
| 85 1,2,3-Trichlorobenzene | 0.96068 0.73656 | 1.02012 0.64602 | 0.96026 | 1.13604 | 0.80895 | 0.82225 | 0.88636 | 18.168 |
| \$ 25 Dibromofluoromethane | 0.64899 0.57172 | 0.62877 0.53307 | 0.61356 | 0.58619 | 0.59870 | 0.58643 | 0.59593 | 5.995 |
| \$ 31 d4-1,2-Dichloroethane | 0.71761 0.61687 | 0.70471 0.55964 | 0.68731 | 0.64625 | 0.64321 | 0.64102 | 0.65208 | 7.847 |
| \$ 43 d8-Toluene | 1.12329 1.04839 | 1.14949 1.04692 | 1.12157 | 1.10618 | 1.11356 | 1.07971 | 1.09864 | 3.363 |
| \$ 62 4-Bromofluorobenzene | 0.54956 0.61336 | 0.55666 0.69489 | 0.55779 | 0.55088 | 0.56658 | 0.59164 | 0.58517 | 8.478 |
| \$ 79 d4-1,2-Dichlorobenzene | 0.92905 0.87965 | 0.92027 0.87290 | 0.92025 | 0.92575 | 0.92529 | 0.90255 | 0.90947 | 2.425 |

Analytical Resources, Inc.
RETENTION TIME SUMMARY REPORT

Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Batch File: /chem1/finn5.i/23JUL10.b
Inst ID: finn5.i

| Compound | RT01 | RT02 | RT03 | RT04 | RT05 | RT06 | RT07 | RT08 | EXPEC RT | RT WINDOW | AVG RT | STD DEV |
|---|-------|-------|-------|-------|-------|-------|-------|-------|----------|-------------|--------|---------|
| 1 Dichlorodifluoromethane | 3.015 | 3.015 | 3.005 | 3.005 | 3.005 | 3.005 | 3.005 | 2.995 | 3.015 | 2.750-3.280 | 3.006 | 0.006 |
| 2 Chloromethane | 3.316 | 3.316 | 3.306 | 3.306 | 3.306 | 3.296 | 3.306 | 3.296 | 3.316 | 3.051-3.581 | 3.306 | 0.008 |
| 3 Vinyl Chloride | 3.417 | 3.417 | 3.417 | 3.417 | 3.407 | 3.417 | 3.427 | 3.417 | 3.417 | 3.152-3.682 | 3.417 | 0.005 |
| 4 Bromomethane | 3.909 | 3.909 | 3.909 | 3.909 | 3.899 | 3.899 | 3.909 | 3.899 | 3.909 | 3.644-4.174 | 3.906 | 0.005 |
| 181 Ethyl Ether | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | 4.500 | 4.235-4.765 | +++++ | +++++ |
| 5 Chloroethane | 3.980 | 3.980 | 3.980 | 3.980 | 3.970 | 3.980 | 3.980 | 3.970 | 3.980 | 3.715-4.245 | 3.976 | 0.005 |
| 6 Trichlorofluoromethane | 4.241 | 4.241 | 4.241 | 4.241 | 4.231 | 4.231 | 4.241 | 4.231 | 4.241 | 3.976-4.506 | 4.237 | 0.005 |
| 7 Acrolein | 4.633 | 4.633 | 4.633 | 4.623 | 4.623 | 4.623 | 4.623 | 4.623 | 4.633 | 4.368-4.898 | 4.627 | 0.005 |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 4.643 | 4.643 | 4.643 | 4.633 | 4.633 | 4.643 | 4.643 | 4.633 | 4.643 | 4.378-4.908 | 4.638 | 0.005 |
| 9 Acetone | 4.693 | 4.683 | 4.683 | 4.673 | 4.673 | 4.673 | 4.673 | 4.673 | 4.693 | 4.428-4.958 | 4.678 | 0.008 |
| 10 1,1-Dichloroethane | 4.844 | 4.844 | 4.834 | 4.834 | 4.834 | 4.834 | 4.834 | 4.834 | 4.844 | 4.579-5.109 | 4.837 | 0.005 |
| 11 Bromoethane | 5.055 | 5.055 | 5.055 | 5.055 | 5.045 | 5.045 | 5.055 | 5.055 | 5.055 | 4.790-5.320 | 5.054 | 0.004 |
| 12 Iodomethane | 5.156 | 5.156 | 5.156 | 5.156 | 5.146 | 5.146 | 5.156 | 5.146 | 5.156 | 4.891-5.421 | 5.152 | 0.005 |
| 13 Methylene Chloride | 5.276 | 5.276 | 5.276 | 5.266 | 5.266 | 5.266 | 5.266 | 5.266 | 5.276 | 5.011-5.541 | 5.270 | 0.005 |
| 14 Acrylonitrile | 5.367 | 5.357 | 5.357 | 5.357 | 5.357 | 5.347 | 5.347 | 5.347 | 5.367 | 5.102-5.632 | 5.354 | 0.007 |
| 16 Methyl tert-Butyl Ether | 5.407 | 5.397 | 5.397 | 5.397 | 5.397 | 5.387 | 5.397 | 5.387 | 5.407 | 5.142-5.672 | 5.396 | 0.006 |
| 15 Carbon Disulfide | 5.377 | 5.377 | 5.377 | 5.377 | 5.367 | 5.367 | 5.377 | 5.367 | 5.377 | 5.112-5.642 | 5.373 | 0.005 |

Reviewer 1 Date: _____
Reviewer 2 Date: _____

T. Tran

Report Date : 29-Jul-2010 14:28

Analytical Resources, Inc.
RETENTION TIME SUMMARY REPORT

Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Batch File: /chem1/finn5.i/23JUL10.b
Inst ID: finn5.i

| Compound | RT01 | RT02 | RT03 | RT04 | RT05 | RT06 | RT07 | RT08 | EXPEC RT | RT WINDOW | AVG RT | STD DEV |
|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|----------|-------------|--------|---------|
| 17 Trans-1,2-Dichloroethane | 5.558 | 5.558 | 5.558 | 5.558 | 5.548 | 5.548 | 5.558 | 5.548 | 5.558 | 5.293-5.822 | 5.554 | 0.005 |
| 18 Vinyl Acetate | 5.879 | 5.879 | 5.879 | 5.879 | 5.869 | 5.869 | 5.879 | 5.869 | 5.879 | 5.614-6.144 | 5.875 | 0.005 |
| 19 1,1-Dichloroethane | 5.940 | 5.940 | 5.940 | 5.940 | 5.929 | 5.929 | 5.929 | 5.929 | 5.940 | 5.675-6.204 | 5.935 | 0.005 |
| 179 Hexane | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | 5.990 | 5.725-6.255 | +++++ | +++++ |
| 20 2-Butanone | 6.291 | 6.281 | 6.281 | 6.281 | 6.271 | 6.271 | 6.281 | 6.271 | 6.291 | 6.026-6.556 | 6.280 | 0.006 |
| 21 2,2-Dichloropropane | 6.462 | 6.462 | 6.462 | 6.452 | 6.452 | 6.452 | 6.452 | 6.442 | 6.462 | 6.197-6.727 | 6.455 | 0.007 |
| 22 Cis-1,2-Dichloroethane | 6.502 | 6.502 | 6.492 | 6.492 | 6.492 | 6.492 | 6.492 | 6.482 | 6.502 | 6.237-6.767 | 6.494 | 0.006 |
| * 23 Pentafluorobenzene | 6.623 | 6.623 | 6.623 | 6.623 | 6.623 | 6.623 | 6.623 | 6.613 | 6.623 | 6.358-6.888 | 6.622 | 0.004 |
| 24 Chloroform | 6.643 | 6.643 | 6.643 | 6.643 | 6.633 | 6.633 | 6.643 | 6.633 | 6.643 | 6.378-6.908 | 6.639 | 0.005 |
| 26 Bromochloromethane | 6.814 | 6.814 | 6.804 | 6.804 | 6.804 | 6.804 | 6.804 | 6.794 | 6.814 | 6.549-7.079 | 6.805 | 0.006 |
| \$ 25 Dibromofluoromethane | 6.844 | 6.844 | 6.844 | 6.844 | 6.834 | 6.834 | 6.834 | 6.834 | 6.844 | 6.579-7.109 | 6.839 | 0.005 |
| 27 1,1,1-Trichloroethane | 7.035 | 7.035 | 7.035 | 7.025 | 7.025 | 7.025 | 7.025 | 7.015 | 7.035 | 6.770-7.300 | 7.027 | 0.007 |
| 182 1-Butanol | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | 8.030 | 7.765-8.295 | +++++ | +++++ |
| 29 1,1-Dichloropropene | 7.176 | 7.176 | 7.176 | 7.176 | 7.166 | 7.166 | 7.176 | 7.166 | 7.176 | 6.870-7.481 | 7.172 | 0.005 |
| \$ 31 d4-1,2-Dichloroethane | 7.306 | 7.306 | 7.306 | 7.306 | 7.296 | 7.296 | 7.306 | 7.296 | 7.306 | 7.041-7.571 | 7.303 | 0.005 |
| 30 Carbon Tetrachloride | 7.296 | 7.296 | 7.286 | 7.286 | 7.286 | 7.286 | 7.286 | 7.286 | 7.296 | 6.991-7.602 | 7.289 | 0.005 |
| 32 1,2-Dichloroethane | 7.397 | 7.397 | 7.397 | 7.387 | 7.387 | 7.387 | 7.387 | 7.387 | 7.397 | 7.091-7.702 | 7.391 | 0.005 |
| 33 Benzene | 7.447 | 7.447 | 7.447 | 7.437 | 7.437 | 7.437 | 7.437 | 7.427 | 7.447 | 7.141-7.752 | 7.439 | 0.007 |
| 180 Isooctane | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | +++++ | 6.687 | 6.422-6.952 | +++++ | +++++ |
| * 34 1,4-Difluorobenzene | 7.638 | 7.638 | 7.638 | 7.628 | 7.628 | 7.628 | 7.628 | 7.628 | 7.638 | 7.332-7.944 | 7.632 | 0.005 |
| 35 Trichloroethene | 8.010 | 8.010 | 8.010 | 8.000 | 8.000 | 8.000 | 8.010 | 8.000 | 8.010 | 7.704-8.315 | 8.005 | 0.005 |
| 36 1,2-Dichloropropane | 8.171 | 8.171 | 8.171 | 8.171 | 8.161 | 8.161 | 8.161 | 8.161 | 8.171 | 7.865-8.476 | 8.166 | 0.005 |

f 7/28/10

Analytical Resources, Inc.
RETENTION TIME SUMMARY REPORT

Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Batch File: /chem1/finn5.i/23JUL10.b
Inst ID: finn5.i

| Compound | RT01 | RT02 | RT03 | RT04 | RT05 | RT06 | RT07 | RT08 | EXPEC RT | RT WINDOW | AVG RT | STD DEV |
|---------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|---------------|--------|---------|
| 38 1,4-Dioxane | 8.412 | 8.402 | 8.402 | 8.402 | 8.402 | 8.392 | 8.402 | 8.392 | 8.412 | 8.622-9.152 | 8.401 | 0.006 |
| 37 Bromodichloromethane | 8.472 | 8.472 | 8.472 | 8.472 | 8.472 | 8.462 | 8.472 | 8.462 | 8.472 | 8.167-8.778 | 8.470 | 0.005 |
| 39 Dibromomethane | 8.623 | 8.623 | 8.623 | 8.613 | 8.613 | 8.613 | 8.613 | 8.613 | 8.623 | 8.317-8.928 | 8.617 | 0.005 |
| 40 2-Chloroethyl Vinyl Et | 8.653 | 8.653 | 8.653 | 8.653 | 8.653 | 8.643 | 8.653 | 8.643 | 8.663 | 8.357-8.969 | 8.652 | 0.006 |
| 41 4-Methyl-2-Pentanone | 8.914 | 8.914 | 8.904 | 8.904 | 8.904 | 8.904 | 8.904 | 8.894 | 8.914 | 8.609-9.220 | 8.906 | 0.006 |
| 42 Cis 1,3-dichloropropen | 9.186 | 9.186 | 9.186 | 9.186 | 9.176 | 9.176 | 9.186 | 9.176 | 9.186 | 7.072-7.602 | 9.182 | 0.005 |
| 28 Cyclohexane | 9.276 | 9.266 | 9.266 | 9.266 | 9.266 | 9.256 | 9.266 | 9.256 | 9.276 | 8.880-9.491 | 9.265 | 0.006 |
| 43 d8-Toluene | 9.407 | 9.397 | 9.397 | 9.397 | 9.397 | 9.387 | 9.397 | 9.387 | 9.407 | 8.971-9.582 | 9.395 | 0.006 |
| 44 Toluene | 9.537 | 9.537 | 9.527 | 9.527 | 9.527 | 9.527 | 9.527 | 9.527 | 9.537 | 9.106-9.969 | 9.530 | 0.005 |
| 45 Trans 1,3-Dichloroprop | 9.588 | 9.578 | 9.578 | 9.578 | 9.578 | 9.578 | 9.578 | 9.568 | 9.588 | 9.282-9.893 | 9.578 | 0.005 |
| 46 2-Hexanone | 9.839 | 9.839 | 9.839 | 9.839 | 9.829 | 9.829 | 9.839 | 9.829 | 9.839 | 9.407-10.270 | 9.835 | 0.005 |
| 47 1,1,2-Trichloroethane | 9.960 | 9.960 | 9.960 | 9.960 | 9.949 | 9.949 | 9.960 | 9.949 | 9.960 | 9.528-10.391 | 9.956 | 0.005 |
| 48 1,3-Dichloropropane | 10.171 | 10.171 | 10.161 | 10.161 | 10.161 | 10.161 | 10.161 | 10.161 | 10.171 | 9.739-10.602 | 10.163 | 0.005 |
| 49 Tetrachloroethene | 10.392 | 10.392 | 10.392 | 10.392 | 10.382 | 10.382 | 10.382 | 10.382 | 10.392 | 10.086-10.697 | 10.387 | 0.005 |
| 50 Chlorodibromomethane | 10.794 | 10.784 | 10.784 | 10.784 | 10.784 | 10.784 | 10.784 | 10.774 | 10.794 | 10.362-11.225 | 10.784 | 0.005 |
| 51 1,2-Dibromoethane | 10.834 | 10.834 | 10.824 | 10.824 | 10.824 | 10.824 | 10.824 | 10.814 | 10.834 | 10.402-11.266 | 10.825 | 0.006 |
| 52 d5-Chlorobenzene | 10.854 | 10.854 | 10.854 | 10.854 | 10.844 | 10.844 | 10.854 | 10.844 | 10.854 | 10.432-11.296 | 10.851 | 0.007 |
| 53 Chlorobenzene | 10.864 | 10.864 | 10.864 | 10.864 | 10.854 | 10.854 | 10.854 | 10.854 | 10.864 | 10.432-11.296 | 10.858 | 0.005 |
| 55 1,1,1,2-Tetrachloroeth | 10.944 | 10.944 | 10.944 | 10.934 | 10.934 | 10.934 | 10.934 | 10.934 | 10.944 | 10.512-11.376 | 10.938 | 0.005 |
| 54 Ethyl Benzene | 11.437 | 11.437 | 11.427 | 11.427 | 11.427 | 11.427 | 11.427 | 11.417 | 11.437 | 11.005-11.869 | 11.428 | 0.006 |
| 56 m,p-xylene | 11.467 | 11.467 | 11.457 | 11.457 | 11.457 | 11.457 | 11.457 | 11.447 | 11.467 | 11.035-11.899 | 11.458 | 0.006 |
| 57 o-Xylene | 11.819 | 11.809 | 11.809 | 11.809 | 11.809 | 11.799 | 11.809 | 11.799 | 11.819 | 11.280-12.357 | 11.807 | 0.006 |
| 58 Styrene | | | | | | | | | | | | |
| 59 Isopropyl Benzene | | | | | | | | | | | | |

67/200

Report Date : 29-Jul-2010 14:28

Analytical Resources, Inc.
RETENTION TIME SUMMARY REPORT

Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Batch File: /chem1/finn5.i/23JUL10.b
Inst ID: finn5.i

| Compound | RT01 | RT02 | RT03 | RT04 | RT05 | RT06 | RT07 | RT08 | EXPEC RT | RT WINDOW | AVG RT | STD DEV |
|-----------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|---------------|--------|---------|
| 60 Bromoform | 11.879 | 11.869 | 11.869 | 11.869 | 11.869 | 11.859 | 11.869 | 11.859 | 11.879 | 11.340-12.418 | 11.868 | 0.006 |
| 61 1,1,2,2-Tetrachloroeth | 11.990 | 11.990 | 11.990 | 11.990 | 11.980 | 11.980 | 11.990 | 11.980 | 11.990 | 11.451-12.528 | 11.986 | 0.005 |
| 62 4-Bromofluorobenzene | 12.110 | 12.110 | 12.110 | 12.100 | 12.100 | 12.100 | 12.100 | 12.100 | 12.110 | 11.678-12.542 | 12.104 | 0.005 |
| 63 1,2,3-Trichloropropane | 12.160 | 12.160 | 12.160 | 12.150 | 12.150 | 12.150 | 12.150 | 12.150 | 12.160 | 11.622-12.699 | 12.154 | 0.005 |
| 65 Trans-1,4-Dichloro 2-B | 12.211 | 12.211 | 12.211 | 12.211 | 12.201 | 12.201 | 12.201 | 12.191 | 12.211 | 11.672-12.749 | 12.204 | 0.007 |
| 66 N-Propyl Benzene | 12.271 | 12.271 | 12.261 | 12.261 | 12.261 | 12.261 | 12.261 | 12.251 | 12.271 | 11.732-12.810 | 12.262 | 0.006 |
| 67 Bromobenzene | 12.361 | 12.351 | 12.351 | 12.351 | 12.351 | 12.341 | 12.351 | 12.341 | 12.361 | 11.823-12.900 | 12.350 | 0.006 |
| 68 1,3,5-Trimethyl Benzen | 12.442 | 12.442 | 12.432 | 12.432 | 12.432 | 12.432 | 12.432 | 12.422 | 12.442 | 11.903-12.980 | 12.433 | 0.006 |
| 69 2-Chloro Toluene | 12.502 | 12.502 | 12.492 | 12.492 | 12.492 | 12.492 | 12.492 | 12.482 | 12.502 | 11.963-13.041 | 12.493 | 0.006 |
| 70 4-Chloro Toluene | 12.552 | 12.542 | 12.542 | 12.532 | 12.532 | 12.532 | 12.532 | 12.532 | 12.552 | 12.014-13.091 | 12.537 | 0.008 |
| 71 T-Butyl Benzene | 12.854 | 12.854 | 12.844 | 12.844 | 12.844 | 12.844 | 12.844 | 12.834 | 12.854 | 12.315-13.392 | 12.845 | 0.006 |
| 72 1,2,4-Trimethylbenzene | 12.904 | 12.894 | 12.894 | 12.894 | 12.894 | 12.884 | 12.894 | 12.884 | 12.904 | 12.365-13.443 | 12.893 | 0.006 |
| 73 S-Butyl Benzene | 13.095 | 13.095 | 13.095 | 13.095 | 13.085 | 13.085 | 13.085 | 13.085 | 13.095 | 12.556-13.634 | 13.090 | 0.005 |
| 74 4-Isopropyl Toluene | 13.246 | 13.246 | 13.236 | 13.236 | 13.236 | 13.236 | 13.236 | 13.226 | 13.246 | 12.707-13.784 | 13.237 | 0.006 |
| 75 1,3-Dichlorobenzene | 13.397 | 13.387 | 13.387 | 13.387 | 13.387 | 13.377 | 13.387 | 13.377 | 13.397 | 12.858-13.935 | 13.385 | 0.006 |
| 64 Cyclohexanone | 13.467 | 13.467 | 13.467 | 13.467 | 13.457 | 13.457 | 13.467 | 13.457 | 13.467 | 13.336-14.200 | 13.463 | 0.005 |
| * 76 d4-1,4-Dichlorobenzene | 13.507 | 13.507 | 13.507 | 13.497 | 13.497 | 13.497 | 13.497 | 13.497 | 13.507 | 12.928-14.006 | 13.501 | 0.005 |
| 77 1,4-Dichlorobenzene | 13.507 | 13.507 | 13.507 | 13.497 | 13.497 | 13.497 | 13.497 | 13.497 | 13.507 | 12.968-14.046 | 13.501 | 0.005 |
| 178 1,2,3-Trimethylbenzene | 13.728 | 13.718 | 13.718 | 13.718 | 13.708 | 13.708 | 13.718 | 13.708 | 13.728 | 13.561-14.639 | 13.716 | 0.007 |
| 78 N-Butyl Benzene | 13.919 | 13.909 | 13.909 | 13.909 | 13.909 | 13.909 | 13.909 | 13.899 | 13.919 | 13.380-14.458 | 13.909 | 0.005 |
| 79 d4-1,2-Dichlorobenzene | 13.949 | 13.949 | 13.949 | 13.939 | 13.939 | 13.939 | 13.939 | 13.929 | 13.949 | 13.411-14.488 | 13.942 | 0.007 |
| 80 1,2-Dichlorobenzene | 14.854 | 14.854 | 14.844 | 14.844 | 14.844 | 14.844 | 14.844 | 14.834 | 14.854 | 14.315-15.393 | 14.845 | 0.006 |
| 81 1,2-Dibromo 3-Chloropr | | | | | | | | | | | | |

Handwritten signature/initials

Analytical Resources, Inc.
RETENTION TIME SUMMARY REPORT

Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Batch File: /chem1/finn5.i/23JUL10.b
Inst ID: finn5.i

Handwritten signature/initials

| Compound | RT01 | RT02 | RT03 | RT04 | RT05 | RT06 | RT07 | RT08 | EXPEC RT | RT WINDOW | AVG RT | STD DEV |
|---------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|---------------|--------|---------|
| 82 1,2,4-Trichlorobenzene | 15.899 | 15.899 | 15.899 | 15.889 | 15.889 | 15.889 | 15.889 | 15.889 | 15.899 | 15.360-16.438 | 15.893 | 0.005 |
| 83 Hexachloro 1,3-Butadie | 16.050 | 16.050 | 16.050 | 16.050 | 16.040 | 16.040 | 16.040 | 16.040 | 16.050 | 15.511-16.588 | 16.045 | 0.005 |
| 84 Naphthalene | 16.231 | 16.221 | 16.221 | 16.221 | 16.221 | 16.211 | 16.221 | 16.211 | 16.231 | 15.692-16.769 | 16.219 | 0.006 |
| 85 1,2,3-Trichlorobenzene | 16.512 | 16.512 | 16.512 | 16.512 | 16.502 | 16.502 | 16.502 | 16.492 | 16.512 | 15.973-17.051 | 16.506 | 0.007 |

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/0010723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD001
 Inj Date : 23-JUL-2010 20:28
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:28 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 20:28 Cal File: 0010723.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

patrickb

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|----------------------------------|-----------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 2.995 | 2.995 | (0.453) | 1408 | 1.00000 | 0.9540 |
| 2 Chloromethane | 50 | 3.296 | 3.296 | (0.498) | 4906 | 1.00000 | 1.236 |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 | (0.517) | 3458 | 1.00000 | 1.101 |
| 4 Bromomethane | 94 | 3.899 | 3.899 | (0.590) | 2127 | 1.00000 | 1.247 |
| 5 Chloroethane | 64 | 3.970 | 3.970 | (0.600) | 2437 | 1.00000 | 1.188 |
| 6 Trichlorofluoromethane | 101 | 4.231 | 4.231 | (0.640) | 3360 | 1.00000 | 1.107 |
| 7 Acrolein | 56 | 4.623 | 4.623 | (0.699) | 2329 | 5.00000 | 6.152 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.633 | 4.633 | (0.701) | 2901 | 1.00000 | 1.221 |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.707) | 3505 | 5.00000 | 5.503 (M) |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.834 | (0.731) | 2358 | 1.00000 | 1.094 |
| 11 Bromoethane | 108 | 5.055 | 5.055 | (0.764) | 1610 | 1.00000 | 1.008 |
| 12 Iodomethane | 142 | 5.146 | 5.146 | (0.778) | 2301 | 1.00000 | 0.9027 |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.796) | 3788 | 1.00000 | 1.560 |
| 14 Acrylonitrile | 53 | 5.347 | 5.347 | (0.808) | 446 | 1.00000 | 0.7931 (Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ----- | ---- | -- | ----- | ----- | ----- | ----- | ----- |
| 16 Methyl tert-Butyl Ether | 73 | 5.387 | 5.387 | (0.815) | 3168 | 1.00000 | 0.9555 (Q) |
| 15 Carbon Disulfide | 76 | 5.367 | 5.367 | (0.812) | 7676 | 1.00000 | 1.148 (Q) |
| 17 Trans-1,2-Dichloroethene | 96 | 5.548 | 5.548 | (0.839) | 1855 | 1.00000 | 1.010 |
| 18 Vinyl Acetate | 43 | 5.869 | 5.869 | (0.888) | 3138 | 1.00000 | 0.9751 |
| 19 1,1-Dichloroethane | 63 | 5.929 | 5.929 | (0.897) | 3627 | 1.00000 | 1.073 |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.948) | 3717 | 5.00000 | 5.186 (T) |
| 21 2,2-Dichloropropane | 77 | 6.442 | 6.442 | (0.974) | 2020 | 1.00000 | 0.9766 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.482 | 6.482 | (0.980) | 1600 | 1.00000 | 0.9880 |
| * 23 Pentafluorobenzene | 168 | 6.613 | 6.613 | (1.000) | 113813 | 50.00000 | |
| 24 Chloroform | 83 | 6.633 | 6.633 | (1.003) | 2843 | 1.00000 | 1.035 (Q) |
| 26 Bromochloromethane | 128 | 6.794 | 6.794 | (1.027) | 686 | 1.00000 | 0.8922 (Q) |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.033) | 73863 | 50.00000 | 54.452 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.015 | 7.015 | (1.061) | 2223 | 1.00000 | 1.041 (M) |
| 29 1,1-Dichloropropene | 75 | 7.166 | 7.166 | (0.939) | 2255 | 1.00000 | 0.9864 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 1957 | 1.00000 | 0.9844 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.103) | 81673 | 50.00000 | 55.025 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 1923 | 1.00000 | 0.9582 |
| 33 Benzene | 78 | 7.427 | 7.427 | (0.974) | 5924 | 1.00000 | 1.072 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 168346 | 50.00000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.049) | 1468 | 1.00000 | 0.9064 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.070) | 1766 | 1.00000 | 1.013 |
| 37 Bromodichloromethane | 83 | 8.392 | 8.392 | (1.100) | 1755 | 1.00000 | 0.9420 |
| 39 Dibromomethane | 93 | 8.462 | 8.462 | (1.109) | 852 | 1.00000 | 0.9849 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 404 | 1.00000 | 0.6620 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.643 | 8.643 | (1.133) | 2382 | 5.00000 | 5.352 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | 8.894 | 8.894 | (1.166) | 1694 | 1.00000 | 0.8328 |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 189101 | 50.00000 | 51.122 |
| 44 Toluene | 92 | 9.256 | 9.256 | (1.213) | 4231 | 1.00000 | 1.290 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.387 | 9.387 | (1.231) | 1503 | 1.00000 | 0.8790 (Q) |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 6953 | 5.00000 | 5.978 (M) |
| 47 1,1,2-Trichloroethane | 97 | 9.568 | 9.568 | (1.254) | 905 | 1.00000 | 0.8863 |
| 48 1,3-Dichloropropane | 76 | 9.829 | 9.829 | (0.912) | 1945 | 1.00000 | 0.9712 |
| 49 Tetrachloroethene | 166 | 9.949 | 9.949 | (0.924) | 1755 | 1.00000 | 1.110 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.943) | 1215 | 1.00000 | 0.9018 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.361) | 1013 | 1.00000 | 0.9262 (T) |
| * 52 d5-Chlorobenzene | 117 | 10.774 | 10.774 | (1.000) | 142296 | 50.00000 | |
| 53 Chlorobenzene | 112 | 10.814 | 10.814 | (1.004) | 4123 | 1.00000 | 1.235 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 6269 | 1.00000 | 1.111 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.844 | 10.844 | (1.007) | 1389 | 1.00000 | 1.087 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.015) | 3903 | 2.00000 | 1.892 (Q) |
| 57 o-Xylene | 106 | 11.417 | 11.417 | (1.060) | 1700 | 1.00000 | 0.7929 (Q) |
| 58 Styrene | 104 | 11.447 | 11.447 | (1.062) | 2884 | 1.00000 | 0.8700 |
| 59 Isopropyl Benzene | 105 | 11.799 | 11.799 | (0.877) | 5129 | 1.00000 | 1.064 |
| 60 Bromoform | 173 | 11.859 | 11.859 | (0.881) | 842 | 1.00000 | 1.086 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.980 | 11.980 | (0.890) | 1717 | 1.00000 | 1.233 (M) |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.123) | 78200 | 50.00000 | 46.957 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.903) | 282 | 1.00000 | 1.022 (QM) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | -- | ----- | ----- | ----- | ----- | ----- |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.191 | 12.191 | (0.906) | 407 | 1.00000 | 0.9508 (QM) |
| 66 N-Propyl Benzene | 91 | 12.251 | 12.251 | (0.910) | 6239 | 1.00000 | 1.002 |
| 67 Bromobenzene | 156 | 12.341 | 12.341 | (0.917) | 1399 | 1.00000 | 1.041 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.422 | 12.422 | (0.923) | 3814 | 1.00000 | 0.9746 |
| 69 2-Chloro Toluene | 91 | 12.482 | 12.482 | (0.928) | 4473 | 1.00000 | 1.094 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 3761 | 1.00000 | 0.9595 |
| 71 T-Butyl Benzene | 119 | 12.834 | 12.834 | (0.954) | 3230 | 1.00000 | 0.9648 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.884 | 12.884 | (0.957) | 3492 | 1.00000 | 0.9064 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 5229 | 1.00000 | 0.9494 |
| 74 4-Isopropyl Toluene | 119 | 13.226 | 13.226 | (0.983) | 3188 | 1.00000 | 0.8436 |
| 75 1,3-Dichlorobenzene | 146 | 13.377 | 13.377 | (0.994) | 2237 | 1.00000 | 0.9743 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 71616 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.003) | 2370 | 1.00000 | 1.032 (Q) |
| 78 N-Butyl Benzene | 91 | 13.708 | 13.708 | (1.019) | 4025 | 1.00000 | 0.9863 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.899 | 13.899 | (1.033) | 66535 | 50.0000 | 51.077 |
| 80 1,2-Dichlorobenzene | 146 | 13.929 | 13.929 | (1.035) | 2202 | 1.00000 | 1.009 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.834 | 14.834 | (1.102) | 218 | 1.00000 | 0.9046 (Q) |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.181) | 1382 | 1.00000 | 1.041 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.192) | 838 | 1.00000 | 0.9370 |
| 84 Naphthalene | 128 | 16.211 | 16.211 | (1.205) | 2458 | 1.00000 | 1.020 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.492 | 16.492 | (1.226) | 1376 | 1.00000 | 1.084 |

QC Flag Legend

- T - Target compound detected outside RT window.
- Q - Qualifier signal failed the ratio test.
- M - Compound response manually integrated.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 0010723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD001
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 113813 | -13.20 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 168346 | -12.12 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 142296 | -11.73 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 71616 | -18.88 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.61 | -0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.77 | -0.09 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.46 | -0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/firm5.i/23JUL10.b/0010723.d

Date: 23-JUL-2010 20:28

Client ID: VSTD001


Sample Info: IC0723,5,5,0

Column phase: Rtx502.2

Instrument: firm5.i

Operator: PB



Column diameter: 0.18



Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.LG
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.1
Client Sample ID: VSTD001


Handwritten signature

Compound: Acetone
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0010723.d

Acetone Amount: 5.50 Area: 3505



MANUAL INTEGRATION for Acetone

- ① Baseline correction
- ② Poor chromatography
- ③ Peak not found
- 4. Totals calculation

5. Other _____




Analyst: 

Date: 7/23/10

Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.LG
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.1
Client Sample ID: VSTD001


p 7/2ab

Compound: 1,1,1-Trichloroethane
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0010723.d

1,1,1-Trichloroethane Amount: 1.04 Area: 2223



MANUAL INTEGRATION for 1,1,1-Trichloroethane

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____




Analyst:

Date: 2/2/10

Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.LG
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.1
Client Sample ID: VSTD001


7/23/10

Compound: 2-Hexanone
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0010723.d

2-Hexanone Amount: 5.98 Area: 6953



MANUAL INTEGRATION for 2-Hexanone

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____




Analyst:

Date:


Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.LG
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.i
Client Sample ID: VSTD001

Compound: 1,1,2,2-Tetrachloroethane
CAS Number:

Handwritten signature



1,1,2,2-Tetrachloroethane Amount: 1.23 Area: 1717



MANUAL INTEGRATION for 1,1,2,2-Tetrachloroethane

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____




Analyst: n

Date: 2/2010

Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.L6
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.1
Client Sample ID: VSTD001


Handwritten signature

Compound: 1,2,3-Trichloropropane
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0010723.d


1,2,3-Trichloropropane Amount: 1.02 Area: 282



MANUAL INTEGRATION for 1,2,3-Trichloropropane

1. Baseline correction
2. Poor chromatography
- ③. Peak not found
4. Totals calculation

5. Other _____




Analyst: 

Date: 7/24/10

Data File: /chem1/finn5.1/23JUL10.b/0010723.d/0010723.LG
Injection Date: 23-JUL-2010 20:28
Instrument: finn5.1
Client Sample ID: VSTD001


Compound: Trans-1,4-Dichloro 2-Butene
CAS Number:

Handwritten: 7/rahs



IC0723, /chem1/finn5.i/23JUL10.b/0010723.d

Trans-1,4-Dichloro 2-Butene Amount: 0.95 Area: 407



MANUAL INTEGRATION for Trans-1,4-Dichloro 2-Butene

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____

Analyst: h

Date: 2/2/10

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/0020723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD002
 Inj Date : 23-JUL-2010 20:02
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:28 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 20:02 Cal File: 0020723.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature: J. Patrick

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | MASS | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|---|-----------|-------|---------------|--------|---------|------------|-----------------|----------------|
| | | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 3.005 (0.454) | 3205 | 2.00000 | 2.133 | | |
| 2 Chloromethane | 50 | 3.306 | 3.306 (0.499) | 9090 | 2.00000 | 2.249 | | |
| 3 Vinyl Chloride | 62 | 3.427 | 3.427 (0.517) | 6731 | 2.00000 | 2.106 (Q) | | |
| 4 Bromomethane | 94 | 3.909 | 3.909 (0.590) | 3943 | 2.00000 | 2.272 | | |
| 5 Chloroethane | 64 | 3.980 | 3.980 (0.601) | 5065 | 2.00000 | 2.426 | | |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.241 (0.640) | 7223 | 2.00000 | 2.338 | | |
| 7 Acrolein | 56 | 4.623 | 4.623 (0.698) | 4563 | 10.0000 | 11.841 | | |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | 4.643 | 4.643 (0.701) | 5478 | 2.00000 | 2.265 | | |
| 9 Acetone | 43 | 4.673 | 4.673 (0.706) | 7408 | 10.0000 | 11.426 (M) | | |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.834 (0.730) | 4722 | 2.00000 | 2.152 | | |
| 11 Bromoethane | 108 | 5.055 | 5.055 (0.763) | 3446 | 2.00000 | 2.120 | | |
| 12 Iodomethane | 142 | 5.156 | 5.156 (0.778) | 4941 | 2.00000 | 1.904 | | |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 (0.795) | 6472 | 2.00000 | 2.619 | | |
| 14 Acrylonitrile | 53 | 5.347 | 5.347 (0.807) | 1125 | 2.00000 | 1.965 (Q) | | |

| Compounds | QUANT SIG | | | | RESPONSE | AMOUNTS | |
|--------------------------------|-----------|--------|--------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.397 | (0.815) | 6868 | 2.00000 | 2.035 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.377 | (0.812) | 15337 | 2.00000 | 2.253 (Q) |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.558 | (0.839) | 3823 | 2.00000 | 2.044 |
| 18 Vinyl Acetate | 43 | 5.879 | 5.879 | (0.888) | 6836 | 2.00000 | 2.087 |
| 19 1,1-Dichloroethane | 63 | 5.929 | 5.929 | (0.895) | 7309 | 2.00000 | 2.124 |
| 20 2-Butanone | 43 | 6.281 | 6.281 | (0.948) | 7636 | 10.00000 | 10.467 |
| 21 2,2-Dichloropropane | 77 | 6.452 | 6.452 | (0.974) | 4155 | 2.00000 | 1.974 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.980) | 3254 | 2.00000 | 1.974 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 115854 | 50.00000 | |
| 24 Chloroform | 83 | 6.643 | 6.643 | (1.003) | 6004 | 2.00000 | 2.148 (Q) |
| 26 Bromochloromethane | 128 | 6.804 | 6.804 | (1.027) | 1497 | 2.00000 | 1.913 (Q) |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.032) | 72845 | 50.00000 | 52.755 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.061) | 4331 | 2.00000 | 1.992 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.176 | (0.941) | 4580 | 2.00000 | 2.033 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 4142 | 2.00000 | 2.114 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.306 | (1.103) | 81644 | 50.00000 | 54.036 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 4173 | 2.00000 | 2.110 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.975) | 11737 | 2.00000 | 2.154 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 165926 | 50.00000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.010 | (1.050) | 3316 | 2.00000 | 2.077 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.070) | 3461 | 2.00000 | 2.015 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.402 | (1.101) | 3933 | 2.00000 | 2.142 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.111) | 1720 | 2.00000 | 2.017 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 941 | 2.00000 | 1.564 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.653 | (1.134) | 4544 | 10.00000 | 10.360 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.167) | 3760 | 2.00000 | 1.875 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.186 | (1.204) | 190730 | 50.00000 | 52.314 |
| 44 Toluene | 92 | 9.266 | 9.266 | (1.215) | 7331 | 2.00000 | 2.268 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.397 | (1.232) | 3132 | 2.00000 | 1.858 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 12031 | 10.00000 | 10.227 (M) |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.578 | (1.256) | 1959 | 2.00000 | 1.946 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.839 | (0.912) | 4110 | 2.00000 | 2.029 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.960 | (0.924) | 3034 | 2.00000 | 1.898 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.942) | 2530 | 2.00000 | 1.857 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.361) | 2176 | 2.00000 | 2.018 (T) |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.784 | (1.000) | 143906 | 50.00000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.824 | (1.004) | 7227 | 2.00000 | 2.141 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 12527 | 2.00000 | 2.195 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.854 | (1.007) | 2668 | 2.00000 | 2.065 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.014) | 8069 | 4.00000 | 3.868 (Q) |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.060) | 3867 | 2.00000 | 1.783 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.062) | 6001 | 2.00000 | 1.790 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.809 | (0.877) | 10149 | 2.00000 | 2.058 |
| 60 Bromoform | 173 | 11.869 | 11.869 | (0.881) | 1646 | 2.00000 | 2.076 |
| 61 1,1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.990 | (0.890) | 3293 | 2.00000 | 2.312 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 80106 | 50.00000 | 47.564 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.902) | 662 | 2.00000 | 2.346 (QM) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.201 | 12.201 | (0.906) | 943 | 2.00000 | 2.154 (QM) |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.910) | 12782 | 2.00000 | 2.008 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.917) | 2746 | 2.00000 | 1.998 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.923) | 7814 | 2.00000 | 1.952 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 8221 | 2.00000 | 1.966 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 8529 | 2.00000 | 2.127 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 6991 | 2.00000 | 2.042 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.894 | (0.957) | 7457 | 2.00000 | 1.892 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 10809 | 2.00000 | 1.919 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.983) | 7447 | 2.00000 | 1.926 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.387 | (0.994) | 4492 | 2.00000 | 1.913 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 73251 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.002) | 4608 | 2.00000 | 1.961 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.718 | (1.019) | 8103 | 2.00000 | 1.941 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 67411 | 50.0000 | 50.594 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.035) | 4695 | 2.00000 | 2.104 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.102) | 613 | 2.00000 | 2.487 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.180) | 2979 | 2.00000 | 2.193 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.191) | 2016 | 2.00000 | 2.204 |
| 84 Naphthalene | 128 | 16.221 | 16.221 | (1.204) | 5145 | 2.00000 | 2.088 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.502 | 16.502 | (1.225) | 2989 | 2.00000 | 2.302 |

QC Flag Legend

- T - Target compound detected outside RT window.
- Q - Qualifier signal failed the ratio test.
- M - Compound response manually integrated.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: finn5.i
Lab File ID: 0020723.d
Lab Smp Id: IC0723
Analysis Type: VOA
Quant Type: ISTD
Operator: PB
Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
Misc Info: 10-

Calibration Date: 23-JUL-2010
Calibration Time: 18:42
Client Smp ID: VSTD002
Level: LOW
Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 115854 | -11.64 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 165926 | -13.38 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 143906 | -10.73 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 73251 | -17.02 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
AREA LOWER LIMIT = - 50% of internal standard area.
RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/finm5.i/23JUL10.b/0020723.d

Date: 23-JUL-2010 20:02

Client ID: VSTD002


Sample Info: IC0723,5,5,0

Column phase: Rtx502.2

Instrument: finm5.i

Operator: PB



Column diameter: 0.18




Data File: /chem1/finn5.1/23JUL10.b/0020723.d/0020723.LG
Injection Date: 23-JUL-2010 20:02
Instrument: finn5.1
Client Sample ID: VSTD002

p²/rals

Compound: Acetone
CAS Number:



Acetone Amount: 11.43 Area: 7408



MANUAL INTEGRATION for Acetone

- ① Baseline correction
- ② Poor chromatography
- ③ Peak not found
- ④ Totals calculation

5. Other _____




Analyst: *fl*

Date: *7/23/10*

Data File: /chem1/finn5.1/23JUL10.b/0020723.d/0020723.LG
Injection Date: 23-JUL-2010 20:02
Instrument: finn5.1
Client Sample ID: VSTD002


Handwritten signature

Compound: 2-Hexanone
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0020723.d

2-Hexanone Amount: 10.23 Area: 12031



MANUAL INTEGRATION for 2-Hexanone

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____




Analyst: *JK*

Date: 7/23/10

Data File: /chem1/finn5.1/23JUL10.b/0020723.d/0020723.LG
Injection Date: 23-JUL-2010 20:02
Instrument: finn5.i
Client Sample ID: VSTD002


U⁷/rabo

Compound: 1,2,3-Trichloropropane
CAS Number:



IC0723, /chem1/finn5.i/23JUL10.b/0020723.d

1,2,3-Trichloropropane Amount: 2.35 Area: 662



MANUAL INTEGRATION for 1,2,3-Trichloropropane

1. Baseline correction
2. Poor chromatography
- ③. Peak not found
4. Totals calculation

5. Other _____




Analyst: W

Date: 7/23/10


Data File: /chem1/finn5.i/23JUL10.b/0020723.d/0020723.LG
Injection Date: 23-JUL-2010 20:02
Instrument: finn5.1
Client Sample ID: VSTD002

U 7/20/10

Compound: Trans-1,4-Dichloro 2-Butene
CAS Number:



Trans-1,4-Dichloro 2-Butene Amount: 2.15 Area: 943



MANUAL INTEGRATION for Trans-1,4-Dichloro 2-Butene

- 1. Baseline correction
- 2. Poor chromatography
- 3. Peak not found
- 4. Totals calculation

5. Other _____

Analyst:

Date:

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/0050723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD005
 Inj Date : 23-JUL-2010 19:35
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:28 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 19:35 Cal File: 0050723.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $\text{Amt} * \text{DF} * \text{Pv} * 1 / (\text{Sa} * ((100 - \text{M}) / 100)) * \text{CpndVaria}$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|----------------------------------|-----------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 3.005 | (0.454) | 7723 | 5.00000 | 5.089 |
| 2 Chloromethane | 50 | 3.296 | 3.296 | (0.498) | 22440 | 5.00000 | 5.496 |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 | (0.516) | 17710 | 5.00000 | 5.485(Q) |
| 4 Bromomethane | 94 | 3.899 | 3.899 | (0.589) | 9090 | 5.00000 | 5.184 |
| 5 Chloroethane | 64 | 3.970 | 3.970 | (0.599) | 11561 | 5.00000 | 5.482 |
| 6 Trichlorofluoromethane | 101 | 4.231 | 4.231 | (0.639) | 17611 | 5.00000 | 5.643 |
| 7 Acrolein | 56 | 4.623 | 4.623 | (0.698) | 10358 | 25.0000 | 26.607 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.633 | 4.633 | (0.700) | 14091 | 5.00000 | 5.767 |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 18358 | 25.0000 | 28.028 |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.834 | (0.730) | 12189 | 5.00000 | 5.498 |
| 11 Bromoethane | 108 | 5.045 | 5.045 | (0.762) | 8530 | 5.00000 | 5.195 |
| 12 Iodomethane | 142 | 5.146 | 5.146 | (0.777) | 13373 | 5.00000 | 5.102 |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.795) | 13925 | 5.00000 | 5.578 |
| 14 Acrylonitrile | 53 | 5.347 | 5.347 | (0.807) | 3314 | 5.00000 | 5.730(Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.387 | 5.387 | (0.813) | 18920 | 5.00000 | 5.549 (Q) |
| 15 Carbon Disulfide | 76 | 5.367 | 5.367 | (0.810) | 39738 | 5.00000 | 5.779 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.548 | 5.548 | (0.838) | 9438 | 5.00000 | 4.995 |
| 18 Vinyl Acetate | 43 | 5.869 | 5.869 | (0.886) | 17895 | 5.00000 | 5.408 |
| 19 1,1-Dichloroethane | 63 | 5.929 | 5.929 | (0.895) | 18913 | 5.00000 | 5.441 |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.947) | 20107 | 25.0000 | 27.282 |
| 21 2,2-Dichloropropane | 77 | 6.452 | 6.452 | (0.974) | 10921 | 5.00000 | 5.134 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.980) | 8398 | 5.00000 | 5.043 (Q) |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 117041 | 50.0000 | |
| 24 Chloroform | 83 | 6.633 | 6.633 | (1.002) | 15400 | 5.00000 | 5.454 (Q) |
| 26 Bromochloromethane | 128 | 6.804 | 6.804 | (1.027) | 4294 | 5.00000 | 5.431 (Q) |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.032) | 71812 | 50.0000 | 51.480 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.061) | 11387 | 5.00000 | 5.185 |
| 29 1,1-Dichloropropene | 75 | 7.166 | 7.166 | (0.939) | 12169 | 5.00000 | 5.243 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 10319 | 5.00000 | 5.112 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.102) | 80444 | 50.0000 | 52.702 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 10820 | 5.00000 | 5.310 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.975) | 30771 | 5.00000 | 5.482 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 170929 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.049) | 8715 | 5.00000 | 5.300 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.070) | 9370 | 5.00000 | 5.296 |
| 37 Bromodichloromethane | 83 | 8.392 | 8.392 | (1.100) | 9943 | 5.00000 | 5.256 |
| 39 Dibromomethane | 93 | 8.462 | 8.462 | (1.109) | 4443 | 5.00000 | 5.059 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 2962 | 5.00000 | 4.780 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.643 | 8.643 | (1.133) | 11309 | 25.0000 | 25.028 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.167) | 10254 | 5.00000 | 4.965 |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 191709 | 50.0000 | 51.044 |
| 44 Toluene | 92 | 9.256 | 9.256 | (1.213) | 17473 | 5.00000 | 5.247 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.387 | 9.387 | (1.231) | 8395 | 5.00000 | 4.836 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 29526 | 25.0000 | 24.696 (M) |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.578 | (1.256) | 5519 | 5.00000 | 5.323 |
| 48 1,3-Dichloropropane | 76 | 9.829 | 9.829 | (0.911) | 10453 | 5.00000 | 5.078 |
| 49 Tetrachloroethene | 166 | 9.949 | 9.949 | (0.923) | 8262 | 5.00000 | 5.084 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.942) | 6807 | 5.00000 | 4.915 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.361) | 5784 | 5.00000 | 5.208 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.784 | (1.000) | 146260 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.824 | (1.004) | 17766 | 5.00000 | 5.179 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 30541 | 5.00000 | 5.264 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.844 | 10.844 | (1.006) | 6409 | 5.00000 | 4.881 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.014) | 22123 | 10.0000 | 10.434 (Q) |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.060) | 10246 | 5.00000 | 4.649 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.062) | 16833 | 5.00000 | 4.940 |
| 59 Isopropyl Benzene | 105 | 11.799 | 11.799 | (0.877) | 27803 | 5.00000 | 5.452 |
| 60 Bromoform | 173 | 11.859 | 11.859 | (0.881) | 4268 | 5.00000 | 5.205 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.980 | 11.980 | (0.890) | 7849 | 5.00000 | 5.327 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 81582 | 50.0000 | 47.660 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.903) | 1675 | 5.00000 | 5.738 |

| Compounds | QUANT SIG | | | | RESPONSE | AMOUNTS | |
|--------------------------------|-----------|--------|--------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.201 | 12.201 | (0.907) | 2468 | 5.00000 | 5.450 (QM) |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.911) | 34800 | 5.00000 | 5.286 |
| 67 Bromobenzene | 156 | 12.341 | 12.341 | (0.917) | 7362 | 5.00000 | 5.178 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.924) | 22104 | 5.00000 | 5.339 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 23284 | 5.00000 | 5.382 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 21819 | 5.00000 | 5.262 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 19493 | 5.00000 | 5.504 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.884 | 12.884 | (0.957) | 21602 | 5.00000 | 5.301 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 30183 | 5.00000 | 5.180 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.984) | 21391 | 5.00000 | 5.350 |
| 75 1,3-Dichlorobenzene | 146 | 13.377 | 13.377 | (0.994) | 12682 | 5.00000 | 5.221 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 75761 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.003) | 12899 | 5.00000 | 5.307 |
| 78 N-Butyl Benzene | 91 | 13.708 | 13.708 | (1.019) | 23070 | 5.00000 | 5.344 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.034) | 69719 | 50.0000 | 50.593 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.036) | 12406 | 5.00000 | 5.374 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.103) | 1436 | 5.00000 | 5.632 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.181) | 7355 | 5.00000 | 5.236 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.192) | 5223 | 5.00000 | 5.520 |
| 84 Naphthalene | 128 | 16.211 | 16.211 | (1.205) | 13199 | 5.00000 | 5.180 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.502 | 16.502 | (1.226) | 7275 | 5.00000 | 5.417 |

QC Flag Legend

- Q - Qualifier signal failed the ratio test.
- M - Compound response manually integrated.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 0050723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD005
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 117041 | -10.73 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 170929 | -10.77 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 146260 | -9.27 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 75761 | -14.18 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.46 | -0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/finn5.i/23JUL10.b/0050723.d

Date : 23-JUL-2010 19:36

Client ID: VSTD005


Sample Info: IC0723.5.5.0

Column Phase: RTX502.2

Instrument: finn5.i

Operator: PB




Column diameter: 0.18



Data File: /chem1/finn5.1/23JUL10.b/0050723.d/0050723.LG
Injection Date: 23-JUL-2010 19:35
Instrument: finn5.i
Client Sample ID: VSTD005

V 7/2010


Compound: 2-Hexanone
CAS Number:



RG58 : 00373

IC0723, /chem1/finn5.i/23JUL10.b/0050723.d

2-Hexanone Amount: 24.70 Area: 29526



MANUAL INTEGRATION for 2-Hexanone

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____




Analyst: U

Date: 7/10/10


Data File: /chem1/finn5.1/23JUL10.b/0050723.d/0050723.LG
Injection Date: 23-JUL-2010 19:35
Instrument: finn5.1
Client Sample ID: VSTD005

Compound: Trans-1,4-Dichloro 2-Butene
CAS Number:

10⁷/raw



Trans-1,4-Dichloro 2-Butene Amount: 5.45 Area: 2468



MANUAL INTEGRATION for Trans-1,4-Dichloro 2-Butene

1. Baseline correction
2. Poor chromatography
3. Peak not found
4. Totals calculation

5. Other _____

Analyst:

Date:

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/0100723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD010
 Inj Date : 23-JUL-2010 19:09
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 19:09 Cal File: 0100723.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

J. J. Walsh

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|----------------------------------|-----------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 3.005 | (0.454) | 15067 | 10.0000 | 9.770 |
| 2 Chloromethane | 50 | 3.306 | 3.306 | (0.499) | 47789 | 10.0000 | 11.518 |
| 3 Vinyl Chloride | 62 | 3.407 | 3.407 | (0.514) | 37997 | 10.0000 | 11.580(Q) |
| 4 Bromomethane | 94 | 3.899 | 3.899 | (0.589) | 14872 | 10.0000 | 8.346 |
| 5 Chloroethane | 64 | 3.970 | 3.970 | (0.599) | 20719 | 10.0000 | 9.669 |
| 6 Trichlorofluoromethane | 101 | 4.231 | 4.231 | (0.639) | 33546 | 10.0000 | 10.578 |
| 7 Acrolein | 56 | 4.623 | 4.623 | (0.698) | 19450 | 50.0000 | 49.169 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.633 | 4.633 | (0.700) | 26723 | 10.0000 | 10.764 |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 35817 | 50.0000 | 53.814 |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.834 | (0.730) | 24541 | 10.0000 | 10.893 |
| 11 Bromoethane | 108 | 5.055 | 5.055 | (0.763) | 17903 | 10.0000 | 10.731 |
| 12 Iodomethane | 142 | 5.146 | 5.146 | (0.777) | 27119 | 10.0000 | 10.181 |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.795) | 26821 | 10.0000 | 10.573 |
| 14 Acrylonitrile | 53 | 5.357 | 5.357 | (0.809) | 6777 | 10.0000 | 11.533(Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ----- | ---- | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.397 | (0.815) | 38803 | 10.0000 | 11.200 (Q) |
| 15 Carbon Disulfide | 76 | 5.367 | 5.367 | (0.810) | 78061 | 10.0000 | 11.172 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.548 | 5.548 | (0.838) | 21284 | 10.0000 | 11.086 |
| 18 Vinyl Acetate | 43 | 5.869 | 5.869 | (0.886) | 37100 | 10.0000 | 11.033 |
| 19 1,1-Dichloroethane | 63 | 5.929 | 5.929 | (0.895) | 39819 | 10.0000 | 11.274 |
| 20 2-Butanone | 43 | 6.281 | 6.281 | (0.948) | 42020 | 50.0000 | 56.109 |
| 21 2,2-Dichloropropane | 77 | 6.452 | 6.452 | (0.974) | 22630 | 10.0000 | 10.471 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.980) | 18047 | 10.0000 | 10.665 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 118930 | 50.0000 | |
| 24 Chloroform | 83 | 6.633 | 6.633 | (1.002) | 31386 | 10.0000 | 10.940 |
| 26 Bromochloromethane | 128 | 6.804 | 6.804 | (1.027) | 8495 | 10.0000 | 10.574 |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.032) | 69715 | 50.0000 | 49.182 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.061) | 23434 | 10.0000 | 10.502 |
| 29 1,1-Dichloropropene | 75 | 7.166 | 7.166 | (0.939) | 25745 | 10.0000 | 11.267 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 21209 | 10.0000 | 10.673 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.102) | 76858 | 50.0000 | 49.553 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 22825 | 10.0000 | 11.378 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.975) | 66143 | 10.0000 | 11.970 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 168271 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.049) | 18174 | 10.0000 | 11.226 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.070) | 19596 | 10.0000 | 11.250 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.402 | (1.101) | 20319 | 10.0000 | 10.911 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.111) | 9683 | 10.0000 | 11.199 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 6388 | 10.0000 | 10.472 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.653 | (1.134) | 24009 | 50.0000 | 53.974 |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.167) | 22221 | 10.0000 | 10.929 |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 186138 | 50.0000 | 50.343 |
| 44 Toluene | 92 | 9.266 | 9.266 | (1.215) | 35399 | 10.0000 | 10.798 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.397 | (1.232) | 18193 | 10.0000 | 10.645 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 61774 | 50.0000 | 53.599 |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.578 | (1.256) | 11407 | 10.0000 | 11.176 |
| 48 1,3-Dichloropropane | 76 | 9.829 | 9.829 | (0.911) | 21313 | 10.0000 | 10.740 |
| 49 Tetrachloroethene | 166 | 9.949 | 9.949 | (0.923) | 15981 | 10.0000 | 10.202 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.942) | 14166 | 10.0000 | 10.612 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.361) | 11754 | 10.0000 | 10.752 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.784 | (1.000) | 140990 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.824 | (1.004) | 36224 | 10.0000 | 10.954 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 63957 | 10.0000 | 11.437 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.844 | 10.844 | (1.006) | 12790 | 10.0000 | 10.106 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.014) | 46275 | 20.0000 | 22.640 (Q) |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.060) | 21803 | 10.0000 | 10.264 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.062) | 37240 | 10.0000 | 11.338 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.809 | (0.878) | 58882 | 10.0000 | 12.124 |
| 60 Bromoform | 173 | 11.869 | 11.869 | (0.882) | 8420 | 10.0000 | 10.783 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.980 | 11.980 | (0.890) | 16250 | 10.0000 | 11.581 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 77668 | 50.0000 | 47.070 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.903) | 3269 | 10.0000 | 11.760 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.201 | 12.201 | (0.907) | 5035 | 10.0000 | 11.675 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.911) | 74061 | 10.0000 | 11.812 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.918) | 15265 | 10.0000 | 11.274 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.924) | 46547 | 10.0000 | 11.806 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 48661 | 10.0000 | 11.812 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 47584 | 10.0000 | 12.050 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 41330 | 10.0000 | 12.254 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.894 | (0.958) | 47036 | 10.0000 | 12.119 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 64271 | 10.0000 | 11.583 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.984) | 45887 | 10.0000 | 12.052 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.387 | (0.995) | 27596 | 10.0000 | 11.930 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 72150 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.003) | 26532 | 10.0000 | 11.462 |
| 78 N-Butyl Benzene | 91 | 13.708 | 13.708 | (1.019) | 49500 | 10.0000 | 12.040 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.034) | 66793 | 50.0000 | 50.895 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.036) | 25247 | 10.0000 | 11.484 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.103) | 2894 | 10.0000 | 11.920 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.181) | 16254 | 10.0000 | 12.150 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.192) | 10838 | 10.0000 | 12.028 |
| 84 Naphthalene | 128 | 16.221 | 16.221 | (1.205) | 30211 | 10.0000 | 12.450 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.502 | 16.502 | (1.226) | 16393 | 10.0000 | 12.817 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 0100723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD010
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5


| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 118930 | -9.29 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 168271 | -12.16 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 140990 | -12.54 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 72150 | -18.27 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.46 | -0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/firm5.i/23JUL10.b/0100723.d
Date: 23-JUL-2010 19:09
Client ID: VSTD010
Sample Info: IC0723,5,5,0
Column phase: Rtx502.2

Instrument: firm5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/0500723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD050
 Inj Date : 23-JUL-2010 18:42
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 18:42 Cal File: 0500723.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature/initials

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | AMOUNTS | | | | | |
|---|-----------|---------|-------|---------|--------|----------|-----------------|
| | | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 3.005 | (0.454) | 88494 | 50.0000 | 52.050 |
| 2 Chloromethane | 50 | 3.306 | 3.306 | (0.499) | 216660 | 50.0000 | 47.364 |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 | (0.516) | 178705 | 50.0000 | 49.403 |
| 4 Bromomethane | 94 | 3.909 | 3.909 | (0.590) | 106254 | 50.0000 | 54.088 |
| 5 Chloroethane | 64 | 3.980 | 3.980 | (0.601) | 114914 | 50.0000 | 48.645 |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.241 | (0.640) | 187024 | 50.0000 | 53.495 |
| 7 Acrolein | 56 | 4.623 | 4.623 | (0.698) | 103002 | 250.000 | 236.19 |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | 4.633 | 4.633 | (0.700) | 132979 | 50.0000 | 48.585 |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 175977 | 250.000 | 239.83 |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.834 | (0.730) | 128370 | 50.0000 | 51.685 |
| 11 Bromoethane | 108 | 5.055 | 5.055 | (0.763) | 95360 | 50.0000 | 51.846 |
| 12 Iodomethane | 142 | 5.156 | 5.156 | (0.778) | 164295 | 50.0000 | 55.947 |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.795) | 122611 | 50.0000 | 43.842 |
| 14 Acrylonitrile | 53 | 5.357 | 5.357 | (0.809) | 34222 | 50.0000 | 52.824 |

| Compounds | QUANT SIG | | | | AMOUNTS | | |
|------------------------------|-----------|--------|--------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ---- | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.397 | (0.815) | 199902 | 50.0000 | 52.338 |
| 15 Carbon Disulfide | 76 | 5.377 | 5.377 | (0.812) | 416399 | 50.0000 | 54.056 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.558 | (0.839) | 104060 | 50.0000 | 49.162 |
| 18 Vinyl Acetate | 43 | 5.879 | 5.879 | (0.888) | 204622 | 50.0000 | 55.196 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.940 | (0.897) | 201091 | 50.0000 | 51.642 |
| 20 2-Butanone | 43 | 6.281 | 6.281 | (0.948) | 214832 | 250.0000 | 260.20 |
| 21 2,2-Dichloropropane | 77 | 6.452 | 6.452 | (0.974) | 119721 | 50.0000 | 50.246 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.980) | 90699 | 50.0000 | 48.618 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 131115 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.643 | (1.003) | 157700 | 50.0000 | 49.859 |
| 26 Bromochloromethane | 128 | 6.804 | 6.804 | (1.027) | 43978 | 50.0000 | 49.652 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.844 | (1.033) | 78499 | 50.0000 | 50.233 |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.061) | 122308 | 50.0000 | 49.717 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.176 | (0.941) | 128968 | 50.0000 | 49.578 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 109284 | 50.0000 | 48.311 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.306 | (1.103) | 84334 | 50.0000 | 49.320 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 112274 | 50.0000 | 49.165 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.975) | 317315 | 50.0000 | 50.445 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 191559 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.049) | 89737 | 50.0000 | 48.692 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.171 | (1.071) | 96034 | 50.0000 | 48.432 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.402 | (1.101) | 103931 | 50.0000 | 49.024 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.111) | 47687 | 50.0000 | 48.448 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 35475 | 50.0000 | 51.086 |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.653 | (1.134) | 127285 | 250.0000 | 251.36 |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.167) | 122153 | 50.0000 | 52.775 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.186 | (1.204) | 213313 | 50.0000 | 50.679 |
| 44 Toluene | 92 | 9.266 | 9.266 | (1.215) | 176514 | 50.0000 | 47.296 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.397 | (1.232) | 99882 | 50.0000 | 51.339 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 307458 | 250.0000 | 233.33 |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.578 | (1.256) | 56632 | 50.0000 | 48.742 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.839 | (0.912) | 109236 | 50.0000 | 48.147 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.960 | (0.924) | 78929 | 50.0000 | 44.072 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.942) | 72980 | 50.0000 | 47.816 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.392 | (1.362) | 61687 | 50.0000 | 49.567 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.784 | (1.000) | 161199 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.824 | (1.004) | 176231 | 50.0000 | 46.611 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 325754 | 50.0000 | 50.948 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.854 | (1.007) | 62748 | 50.0000 | 43.363 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.014) | 247468 | 100.0000 | 105.89 |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.060) | 120870 | 50.0000 | 49.766 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.062) | 197957 | 50.0000 | 52.713 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.809 | (0.877) | 321007 | 50.0000 | 54.019 |
| 60 Bromoform | 173 | 11.869 | 11.869 | (0.881) | 45981 | 50.0000 | 48.125 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.990 | (0.890) | 80952 | 50.0000 | 47.153 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 91332 | 50.0000 | 48.412 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.902) | 16376 | 50.0000 | 48.148 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.211 | (0.907) | 26610 | 50.0000 | 50.430 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.910) | 378862 | 50.0000 | 49.387 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.917) | 80968 | 50.0000 | 48.876 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.923) | 264645 | 50.0000 | 54.862 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 248038 | 50.0000 | 49.208 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 261192 | 50.0000 | 54.058 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 232931 | 50.0000 | 56.443 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.894 | (0.957) | 260230 | 50.0000 | 54.800 |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.095 | (0.972) | 355887 | 50.0000 | 52.419 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.983) | 260120 | 50.0000 | 55.837 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.387 | (0.994) | 145285 | 50.0000 | 51.333 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 88279 | 50.0000 | 50.0000 |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.002) | 140968 | 50.0000 | 49.774 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.718 | (1.019) | 273888 | 50.0000 | 54.445 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 81684 | 50.0000 | 50.870 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.035) | 133963 | 50.0000 | 49.803 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.102) | 15128 | 50.0000 | 50.924 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.180) | 75938 | 50.0000 | 46.392 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.050 | (1.192) | 52008 | 50.0000 | 47.175 |
| 84 Naphthalene | 128 | 16.221 | 16.221 | (1.204) | 142809 | 50.0000 | 48.101 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.512 | (1.226) | 71413 | 50.0000 | 45.633 |

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 0500723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD050
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 131115 | 0.00 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 191559 | 0.00 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 161199 | 0.00 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 88279 | 0.00 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/finn5.i/23JUL10.b/0500723.d

Date: 23-JUL-2010 18:42

Client ID: VST050

Sample Info: IC0723,5,5,0


Column phase: RtX502.2

Instrument: finn5.i

Operator: PB

Column diameter: 0.18

Page 5



/chem1/finn5.i/23JUL10.b/0500723.d/0500723.LC

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/1000723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD100
 Inj Date : 23-JUL-2010 18:16
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 18:16 Cal File: 1000723.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | MASS | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|---|-----------|------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | 3.005 | 3.005 | (0.454) | 182544 | 100.000 | 104.02 |
| 2 Chloromethane | 50 | | 3.306 | 3.306 | (0.499) | 423802 | 100.000 | 89.759 |
| 3 Vinyl Chloride | 62 | | 3.417 | 3.417 | (0.516) | 367442 | 100.000 | 98.412 |
| 4 Bromomethane | 94 | | 3.909 | 3.909 | (0.590) | 208154 | 100.000 | 102.66 |
| 5 Chloroethane | 64 | | 3.980 | 3.980 | (0.601) | 210640 | 100.000 | 86.388 |
| 6 Trichlorofluoromethane | 101 | | 4.241 | 4.241 | (0.640) | 346453 | 100.000 | 96.008 |
| 7 Acrolein | 56 | | 4.633 | 4.633 | (0.700) | 197468 | 500.000 | 438.68 |
| 8 1,1,2-Trichloro-1,2,2-Trifluoroethane | 101 | | 4.643 | 4.643 | (0.701) | 264194 | 100.000 | 93.516 |
| 9 Acetone | 43 | | 4.683 | 4.683 | (0.707) | 329833 | 500.000 | 435.50 |
| 10 1,1-Dichloroethene | 96 | | 4.834 | 4.834 | (0.730) | 252737 | 100.000 | 98.586 |
| 11 Bromoethane | 108 | | 5.055 | 5.055 | (0.763) | 196835 | 100.000 | 103.68 |
| 12 Iodomethane | 142 | | 5.156 | 5.156 | (0.778) | 339831 | 100.000 | 112.12 |
| 13 Methylene Chloride | 84 | | 5.276 | 5.276 | (0.797) | 251445 | 100.000 | 87.107 |
| 14 Acrylonitrile | 53 | | 5.357 | 5.357 | (0.809) | 69928 | 100.000 | 104.57(Q) |

| Compounds | QUANT SIG | | | | | | AMOUNTS | |
|------------------------------|-----------|------|--------|--------|---------|----------|--------------------|-------------------|
| | | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ---- | == | ===== | ===== | ===== | ===== | ===== | |
| 16 Methyl tert-Butyl Ether | 73 | | 5.397 | 5.397 | (0.815) | 417323 | 100.000 | 105.86 (Q) |
| 15 Carbon Disulfide | 76 | | 5.377 | 5.377 | (0.812) | 775986 | 100.000 | 97.596 |
| 17 Trans-1,2-Dichloroethene | 96 | | 5.558 | 5.558 | (0.839) | 225901 | 100.000 | 103.40 |
| 18 Vinyl Acetate | 43 | | 5.879 | 5.879 | (0.888) | 420486 | 100.000 | 109.89 |
| 19 1,1-Dichloroethane | 63 | | 5.940 | 5.940 | (0.897) | 422564 | 100.000 | 105.14 |
| 20 2-Butanone | 43 | | 6.281 | 6.281 | (0.948) | 437209 | 500.000 | 513.04 |
| 21 2,2-Dichloropropane | 77 | | 6.462 | 6.462 | (0.976) | 258768 | 100.000 | 105.22 |
| 22 Cis-1,2-Dichloroethene | 96 | | 6.492 | 6.492 | (0.980) | 200756 | 100.000 | 104.26 |
| * 23 Pentafluorobenzene | 168 | | 6.623 | 6.623 | (1.000) | 135334 | 50.0000 | |
| 24 Chloroform | 83 | | 6.643 | 6.643 | (1.003) | 333986 | 100.000 | 102.30 |
| 26 Bromochloromethane | 128 | | 6.804 | 6.804 | (1.027) | 95093 | 100.000 | 104.01 |
| \$ 25 Dibromofluoromethane | 111 | | 6.844 | 6.844 | (1.033) | 79364 | 50.0000 | 49.203 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | 7.035 | 7.035 | (1.062) | 260275 | 100.000 | 102.50 |
| 29 1,1-Dichloropropene | 75 | | 7.176 | 7.176 | (0.939) | 277625 | 100.000 | 102.36 |
| 30 Carbon Tetrachloride | 117 | | 7.286 | 7.286 | (0.954) | 236579 | 100.000 | 100.30 |
| \$ 31 d4-1,2-Dichloroethane | 65 | | 7.306 | 7.306 | (1.103) | 86752 | 50.0000 | 49.152 |
| 32 1,2-Dichloroethane | 62 | | 7.397 | 7.397 | (0.968) | 238783 | 100.000 | 100.28 |
| 33 Benzene | 78 | | 7.447 | 7.447 | (0.975) | 581109 | 100.000 | 88.602 |
| * 34 1,4-Difluorobenzene | 114 | | 7.638 | 7.638 | (1.000) | 199732 | 50.0000 | |
| 35 Trichloroethene | 95 | | 8.010 | 8.010 | (1.049) | 193783 | 100.000 | 100.84 |
| 36 1,2-Dichloropropane | 63 | | 8.171 | 8.171 | (1.070) | 206742 | 100.000 | 99.998 |
| 37 Bromodichloromethane | 83 | | 8.402 | 8.402 | (1.100) | 221686 | 100.000 | 100.29 |
| 39 Dibromomethane | 93 | | 8.472 | 8.472 | (1.109) | 104013 | 100.000 | 101.35 |
| 40 2-Chloroethyl Vinyl Ether | 63 | | 8.623 | 8.623 | (1.129) | 77415 | 100.000 | 106.92 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | | 8.653 | 8.653 | (1.133) | 263763 | 500.000 | 499.56 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | | 8.904 | 8.904 | (1.166) | 270130 | 100.000 | 111.93 |
| \$ 43 d8-Toluene | 98 | | 9.186 | 9.186 | (1.203) | 215653 | 50.0000 | 49.139 |
| 44 Toluene | 92 | | 9.266 | 9.266 | (1.213) | 377962 | 100.000 | 97.129 (Q) |
| 45 Trans 1,3-Dichloropropene | 75 | | 9.397 | 9.397 | (1.230) | 223383 | 100.000 | 110.12 |
| 46 2-Hexanone | 43 | | 9.527 | 9.527 | (0.884) | 517771 | 500.000 | 394.32 |
| 47 1,1,2-Trichloroethane | 97 | | 9.578 | 9.578 | (1.254) | 123034 | 100.000 | 101.56 |
| 48 1,3-Dichloropropane | 76 | | 9.839 | 9.839 | (0.912) | 232506 | 100.000 | 102.84 |
| 49 Tetrachloroethene | 166 | | 9.960 | 9.960 | (0.924) | 175269 | 100.000 | 98.211 |
| 50 Chlorodibromomethane | 129 | | 10.161 | 10.161 | (0.942) | 158474 | 100.000 | 104.20 |
| 51 1,2-Dibromoethane | 107 | | 10.392 | 10.392 | (1.361) | 131007 | 100.000 | 100.96 |
| * 52 d5-Chlorobenzene | 117 | | 10.784 | 10.784 | (1.000) | 160631 | 50.0000 | |
| 53 Chlorobenzene | 112 | | 10.824 | 10.824 | (1.004) | 376912 | 100.000 | 100.04 |
| 54 Ethyl Benzene | 91 | | 10.864 | 10.864 | (1.007) | 573170 | 100.000 | 89.962 |
| 55 1,1,1,2-Tetrachloroethane | 131 | | 10.854 | 10.854 | (1.007) | 137418 | 100.000 | 95.300 |
| 56 m,p-xylene | 106 | | 10.944 | 10.944 | (1.015) | 516678 | 200.000 | 221.87 (Q) |
| 57 o-Xylene | 106 | | 11.427 | 11.427 | (1.060) | 269989 | 100.000 | 111.56 (Q) |
| 58 Styrene | 104 | | 11.457 | 11.457 | (1.062) | 431090 | 100.000 | 115.20 |
| 59 Isopropyl Benzene | 105 | | 11.809 | 11.809 | (0.877) | 588226 | 100.000 | 90.704 |
| 60 Bromoform | 173 | | 11.869 | 11.869 | (0.881) | 103792 | 100.000 | 99.542 |
| 61 1,1,2,2-Tetrachloroethane | 83 | | 11.990 | 11.990 | (0.890) | 171593 | 100.000 | 91.586 |
| \$ 62 4-Bromofluorobenzene | 95 | | 12.110 | 12.110 | (1.123) | 95036 | 50.0000 | 50.553 |
| 63 1,2,3-Trichloropropane | 110 | | 12.160 | 12.160 | (0.903) | 35211 | 100.000 | 94.864 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.211 | (0.907) | 57625 | 100.000 | 100.07 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.910) | 642345 | 100.000 | 76.727 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.917) | 184300 | 100.000 | 101.94 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.923) | 526617 | 100.000 | 100.04 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 543512 | 100.000 | 98.805 |
| 70 4-Chloro Toluene | 91 | 12.542 | 12.542 | (0.931) | 505915 | 100.000 | 95.947 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 493329 | 100.000 | 109.54 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.894 | (0.957) | 539580 | 100.000 | 104.12 |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.095 | (0.972) | 628727 | 100.000 | 84.857 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.983) | 529249 | 100.000 | 104.10 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.387 | (0.994) | 347593 | 100.000 | 112.54 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 96340 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.507 | (1.003) | 341992 | 100.000 | 110.65 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.718 | (1.019) | 548418 | 100.000 | 99.896 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 86952 | 50.0000 | 49.620 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.949 | (1.036) | 305695 | 100.000 | 104.14 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.102) | 30455 | 100.000 | 93.940 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.899 | (1.181) | 175953 | 100.000 | 98.499 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.050 | (1.192) | 115056 | 100.000 | 95.632 |
| 84 Naphthalene | 128 | 16.221 | 16.221 | (1.204) | 300283 | 100.000 | 92.679 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.512 | (1.226) | 158431 | 100.000 | 92.767 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 1000723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD100
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 135334 | 3.22 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 199732 | 4.27 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 160631 | -0.35 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 96340 | 9.13 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |


AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/firm5.i/23JUL10.b/1000723.d
Date: 23-JUL-2010 18:16
Client ID: VSTD100
Sample Info: IC0723.5.5.0

Column phase: Rtx502.2

/chem1/firm5.i/23JUL10.b/1000723.d/1000723.LG

Instrument: firm5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/1500723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD150
 Inj Date : 23-JUL-2010 17:49
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:49 Cal File: 1500723.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

patrickb

Concentration Formula: Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|---|-----------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.015 | 3.015 | (0.455) | 295620 | 150.000 | 146.34 |
| 2 Chloromethane | 50 | 3.316 | 3.316 | (0.501) | 648632 | 150.000 | 119.34 |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 | (0.516) | 547438 | 150.000 | 127.37 |
| 4 Bromomethane | 94 | 3.909 | 3.909 | (0.590) | 302383 | 150.000 | 129.55 |
| 5 Chloroethane | 64 | 3.980 | 3.980 | (0.601) | 293885 | 150.000 | 104.71 |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.241 | (0.640) | 487082 | 150.000 | 117.26 |
| 7 Acrolein | 56 | 4.633 | 4.633 | (0.700) | 278099 | 750.000 | 536.71 |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | 4.643 | 4.643 | (0.701) | 382218 | 150.000 | 117.53 |
| 9 Acetone | 43 | 4.683 | 4.683 | (0.707) | 476748 | 750.000 | 546.84 |
| 10 1,1-Dichloroethene | 96 | 4.844 | 4.844 | (0.731) | 372564 | 150.000 | 126.25 |
| 11 Bromoethane | 108 | 5.055 | 5.055 | (0.763) | 295924 | 150.000 | 135.41 |
| 12 Iodomethane | 142 | 5.156 | 5.156 | (0.778) | 498041 | 150.000 | 142.74 |
| 13 Methylene Chloride | 84 | 5.276 | 5.276 | (0.797) | 383620 | 150.000 | 115.45 |
| 14 Acrylonitrile | 53 | 5.357 | 5.357 | (0.809) | 107704 | 150.000 | 139.92(Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|-----------------|----------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.397 | (0.815) | 613756 | 150.000 | 135.24 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.377 | (0.812) | 1021453 | 150.000 | 111.60 (Q) |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.558 | (0.839) | 357903 | 150.000 | 142.31 (Q) |
| 18 Vinyl Acetate | 43 | 5.879 | 5.879 | (0.888) | 559418 | 150.000 | 127.00 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.940 | (0.897) | 586536 | 150.000 | 126.78 |
| 20 2-Butanone | 43 | 6.281 | 6.281 | (0.948) | 627000 | 750.000 | 639.16 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.462 | (0.976) | 409501 | 150.000 | 144.65 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.502 | 6.502 | (0.982) | 321064 | 150.000 | 144.85 (Q) |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 155784 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.643 | (1.003) | 501605 | 150.000 | 133.48 |
| 26 Bromochloromethane | 128 | 6.814 | 6.814 | (1.029) | 155161 | 150.000 | 147.44 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.844 | (1.033) | 89065 | 50.0000 | 47.969 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.035 | (1.062) | 410583 | 150.000 | 140.47 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.176 | (0.939) | 432896 | 150.000 | 139.46 |
| 30 Carbon Tetrachloride | 117 | 7.296 | 7.296 | (0.955) | 377891 | 150.000 | 140.00 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.306 | (1.103) | 96098 | 50.0000 | 47.300 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.397 | (0.968) | 373218 | 150.000 | 136.97 |
| 33 Benzene | 78 | 7.447 | 7.447 | (0.975) | 746304 | 150.000 | 99.432 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.638 | (1.000) | 228573 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.010 | (1.049) | 307337 | 150.000 | 139.76 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.171 | (1.070) | 322596 | 150.000 | 136.35 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.402 | (1.100) | 353775 | 150.000 | 139.85 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.109) | 162509 | 150.000 | 138.36 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.623 | (1.129) | 128070 | 150.000 | 154.56 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.653 | (1.133) | 417853 | 750.000 | 691.54 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | 8.914 | 8.914 | (1.167) | 424803 | 150.000 | 153.81 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.186 | (1.203) | 239633 | 50.0000 | 47.713 |
| 44 Toluene | 92 | 9.266 | 9.266 | (1.213) | 537240 | 150.000 | 120.64 (Q) |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.397 | (1.230) | 359227 | 150.000 | 154.74 |
| 46 2-Hexanone | 43 | 9.537 | 9.537 | (0.884) | 658433 | 750.000 | 450.96 (Q) |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.578 | (1.254) | 199640 | 150.000 | 144.00 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.839 | (0.912) | 362456 | 150.000 | 144.18 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.960 | (0.924) | 291013 | 150.000 | 146.65 |
| 50 Chlorodibromomethane | 129 | 10.171 | 10.171 | (0.943) | 256549 | 150.000 | 151.70 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.392 | (1.361) | 211704 | 150.000 | 142.56 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.784 | (1.000) | 178614 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.834 | 10.834 | (1.005) | 526215 | 150.000 | 125.61 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.864 | (1.007) | 719154 | 150.000 | 101.51 (Q) |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.854 | (1.007) | 235095 | 150.000 | 146.62 |
| 56 m,p-xylene | 106 | 10.944 | 10.944 | (1.015) | 693534 | 300.000 | 267.84 (Q) |
| 57 o-Xylene | 106 | 11.437 | 11.437 | (1.061) | 443859 | 150.000 | 164.93 (Q) |
| 58 Styrene | 104 | 11.467 | 11.467 | (1.063) | 604009 | 150.000 | 145.16 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.809 | (0.877) | 765486 | 150.000 | 92.525 |
| 60 Bromoform | 173 | 11.869 | 11.869 | (0.881) | 184206 | 150.000 | 138.48 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.990 | (0.890) | 287454 | 150.000 | 120.26 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.110 | (1.123) | 109555 | 50.0000 | 52.409 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.160 | (0.903) | 59137 | 150.000 | 124.89 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.211 | (0.907) | 94977 | 150.000 | 129.29 |
| 66 N-Propyl Benzene | 91 | 12.271 | 12.271 | (0.911) | 798434 | 150.000 | 74.759 (Q) |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.917) | 321436 | 150.000 | 139.37 (Q) |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.442 | 12.442 | (0.924) | 708315 | 150.000 | 105.47 (Q) |
| 69 2-Chloro Toluene | 91 | 12.502 | 12.502 | (0.928) | 729939 | 150.000 | 104.02 |
| 70 4-Chloro Toluene | 91 | 12.542 | 12.542 | (0.931) | 684866 | 150.000 | 101.81 |
| 71 T-Butyl Benzene | 119 | 12.854 | 12.854 | (0.954) | 722068 | 150.000 | 125.68 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.894 | (0.957) | 731940 | 150.000 | 110.71 (Q) |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.095 | (0.972) | 812152 | 150.000 | 85.922 |
| 74 4-Isopropyl Toluene | 119 | 13.246 | 13.246 | (0.984) | 739478 | 150.000 | 114.02 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.387 | (0.994) | 545268 | 150.000 | 138.38 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 122904 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.507 | (1.003) | 547350 | 150.000 | 138.82 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.718 | (1.019) | 717047 | 150.000 | 102.38 (Q) |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 108113 | 50.0000 | 48.361 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.949 | (1.036) | 516441 | 150.000 | 137.91 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.854 | 14.854 | (1.103) | 50577 | 150.000 | 122.29 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.899 | (1.181) | 304271 | 150.000 | 133.52 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.050 | (1.192) | 204107 | 150.000 | 132.98 |
| 84 Naphthalene | 128 | 16.221 | 16.221 | (1.204) | 474513 | 150.000 | 114.80 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.512 | (1.226) | 271577 | 150.000 | 124.65 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 1500723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD150
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 155784 | 18.81 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 228573 | 19.32 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 178614 | 10.80 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 122904 | 39.22 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |


AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chemd/finm5.i/23JUL10.b/1500723.d
Date : 23-JUL-2010 17:49
Client ID: VSTD1150
Sample Info: IC0723,5,5,0

Column phase: Rtx502.2

Instrument: finm5.i
Operator: PB
Column diameter: 0.18

/chemd/finm5.i/23JUL10.b/1500723.d/1500723.LG

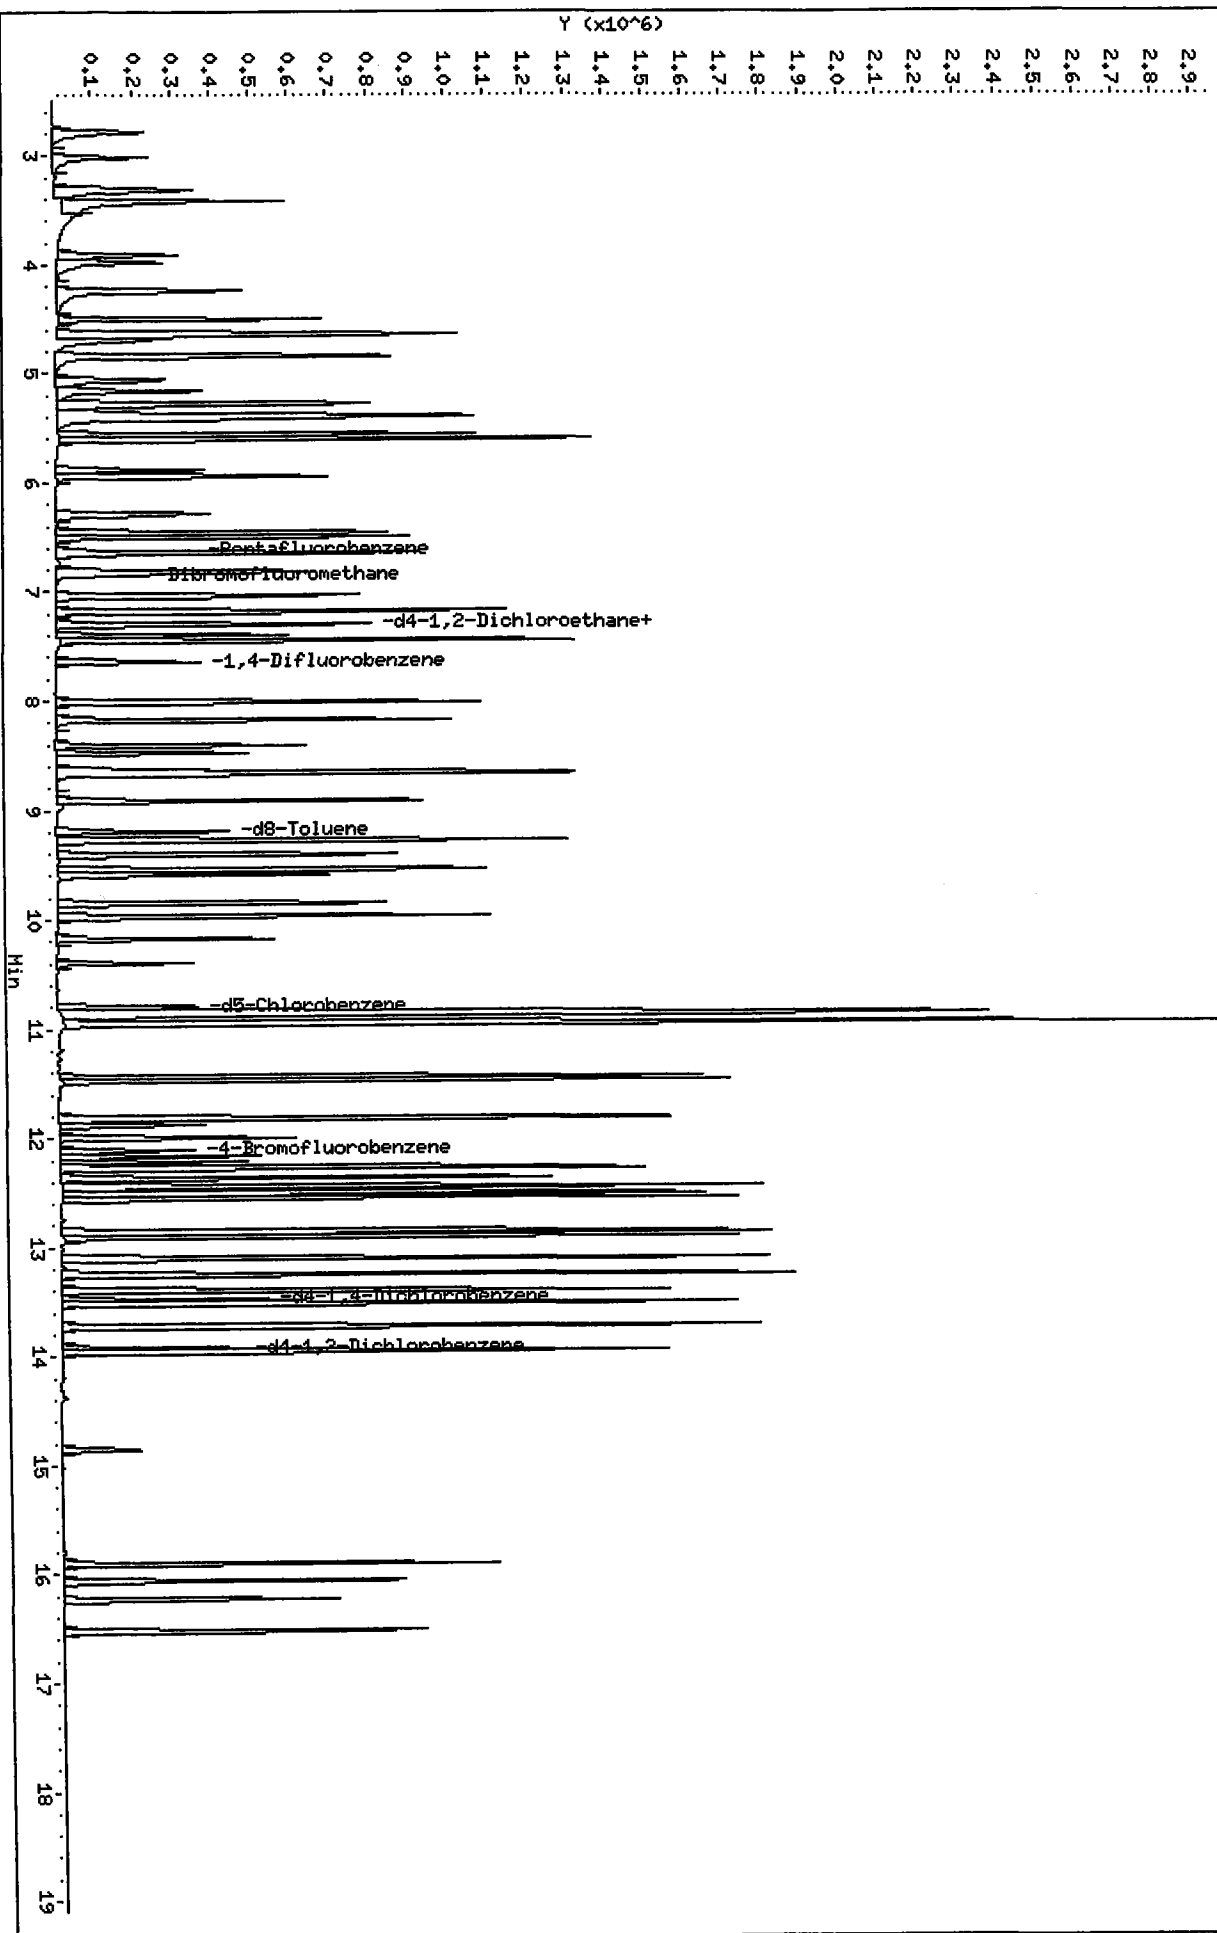

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/2000723.d
 Lab Smp Id: IC0723 Client Smp ID: VSTD200
 Inj Date : 23-JUL-2010 17:18
 Operator : PB Inst ID: finn5.i
 Smp Info : IC0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 Calibration Sample, Level: 8
 Dil Factor: 1.00000 Compound Sublist: voa.sub
 Integrator: HP RTE
 Target Version: 3.50
 Processing Host: cserv3

f 7/26/10

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | MASS | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|----------------------------------|-----------|-------|---------------|--------|---------|------------|-----------------|----------------|
| | | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.015 | 3.015 (0.455) | 382873 | 200.000 | 185.53 | | |
| 2 Chloromethane | 50 | 3.316 | 3.316 (0.501) | 831334 | 200.000 | 149.72 | | |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 (0.516) | 675701 | 200.000 | 153.89 | | |
| 4 Bromomethane | 94 | 3.909 | 3.909 (0.590) | 368903 | 200.000 | 154.71 | | |
| 5 Chloroethane | 64 | 3.980 | 3.980 (0.601) | 364783 | 200.000 | 127.22 | | |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.241 (0.640) | 615782 | 200.000 | 145.11 | | |
| 7 Acrolein | 56 | 4.633 | 4.633 (0.700) | 343518 | 1000.00 | 648.94 | | |
| 8 112Trichloro122Trifluoroethane | 101 | 4.643 | 4.643 (0.701) | 482521 | 200.000 | 145.24 | | |
| 9 Acetone | 43 | 4.693 | 4.693 (0.709) | 560993 | 1000.00 | 629.87 | | |
| 10 1,1-Dichloroethene | 96 | 4.844 | 4.844 (0.731) | 470540 | 200.000 | 156.08 (Q) | | |
| 11 Bromoethane | 108 | 5.055 | 5.055 (0.763) | 376320 | 200.000 | 168.56 | | |
| 12 Iodomethane | 142 | 5.156 | 5.156 (0.778) | 652382 | 200.000 | 183.02 | | |
| 13 Methylene Chloride | 84 | 5.276 | 5.276 (0.797) | 495091 | 200.000 | 145.85 (Q) | | |
| 14 Acrylonitrile | 53 | 5.367 | 5.367 (0.810) | 139945 | 200.000 | 177.96 (Q) | | |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ----- | ---- | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.407 | 5.407 | (0.816) | 732622 | 200.000 | 158.02 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.377 | (0.812) | 1217955 | 200.000 | 130.26 (Q) |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.558 | (0.839) | 459768 | 200.000 | 178.95 (Q) |
| 18 Vinyl Acetate | 43 | 5.879 | 5.879 | (0.888) | 672353 | 200.000 | 149.42 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.940 | (0.897) | 680449 | 200.000 | 143.96 |
| 20 2-Butanone | 43 | 6.291 | 6.291 | (0.950) | 785164 | 1000.00 | 783.47 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.462 | (0.976) | 544411 | 200.000 | 188.24 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.502 | 6.502 | (0.982) | 438984 | 200.000 | 193.86 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 159149 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.643 | (1.003) | 610807 | 200.000 | 159.10 |
| 26 Bromochloromethane | 128 | 6.814 | 6.814 | (1.029) | 213240 | 200.000 | 198.34 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.844 | (1.033) | 84837 | 50.0000 | 44.726 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.035 | (1.062) | 549252 | 200.000 | 183.94 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.176 | (0.939) | 545791 | 200.000 | 175.44 |
| 30 Carbon Tetrachloride | 117 | 7.296 | 7.296 | (0.955) | 522753 | 200.000 | 193.23 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.306 | (1.103) | 89066 | 50.0000 | 42.912 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.397 | (0.968) | 485007 | 200.000 | 177.58 |
| 33 Benzene | 78 | 7.447 | 7.447 | (0.975) | 870526 | 200.000 | 115.72 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.638 | (1.000) | 229095 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.010 | (1.049) | 422519 | 200.000 | 191.70 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.171 | (1.070) | 435024 | 200.000 | 183.44 |
| 37 Bromodichloromethane | 83 | 8.412 | 8.412 | (1.101) | 471123 | 200.000 | 185.82 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.109) | 228343 | 200.000 | 193.98 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.623 | (1.129) | 181565 | 200.000 | 218.62 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.663 | 8.663 | (1.134) | 536767 | 1000.00 | 886.32 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | 8.914 | 8.914 | (1.167) | 522307 | 200.000 | 188.68 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.186 | (1.203) | 239843 | 50.0000 | 47.646 |
| 44 Toluene | 92 | 9.276 | 9.276 | (1.214) | 647650 | 200.000 | 145.10 (Q) |
| 45 Trans 1,3-Dichloropropene | 75 | 9.407 | 9.407 | (1.232) | 465557 | 200.000 | 200.09 |
| 46 2-Hexanone | 43 | 9.537 | 9.537 | (0.884) | 763183 | 1000.00 | 544.40 (Q) |
| 47 1,1,2-Trichloroethane | 97 | 9.588 | 9.588 | (1.255) | 280030 | 200.000 | 201.53 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.839 | (0.912) | 469237 | 200.000 | 194.40 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.960 | (0.923) | 404966 | 200.000 | 212.54 |
| 50 Chlorodibromomethane | 129 | 10.171 | 10.171 | (0.942) | 362369 | 200.000 | 223.17 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.392 | (1.361) | 296560 | 200.000 | 199.25 |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.794 | (1.000) | 171495 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.834 | 10.834 | (1.004) | 637891 | 200.000 | 158.58 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.864 | (1.007) | 844494 | 200.000 | 124.15 (Q) |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.864 | 10.864 | (1.007) | 337259 | 200.000 | 219.07 |
| 56 m,p-xylene | 106 | 10.944 | 10.944 | (1.014) | 845893 | 400.000 | 340.24 (Q) |
| 57 o-Xylene | 106 | 11.437 | 11.437 | (1.060) | 593625 | 200.000 | 229.74 (Q) |
| 58 Styrene | 104 | 11.467 | 11.467 | (1.062) | 750474 | 200.000 | 187.84 (Q) |
| 59 Isopropyl Benzene | 105 | 11.819 | 11.819 | (0.878) | 880078 | 200.000 | 89.802 (Q) |
| 60 Bromoform | 173 | 11.879 | 11.879 | (0.882) | 275819 | 200.000 | 175.04 |
| 61 1,1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.990 | (0.890) | 411745 | 200.000 | 145.43 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.110 | (1.122) | 119170 | 50.0000 | 59.375 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.160 | (0.903) | 85172 | 200.000 | 151.85 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.211 | (0.907) | 138249 | 200.000 | 158.87 |
| 66 N-Propyl Benzene | 91 | 12.271 | 12.271 | (0.911) | 919942 | 200.000 | 72.715 (Q) |
| 67 Bromobenzene | 156 | 12.361 | 12.361 | (0.918) | 475914 | 200.000 | 174.20 (Q) |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.442 | 12.442 | (0.924) | 843459 | 200.000 | 106.02 (Q) |
| 69 2-Chloro Toluene | 91 | 12.502 | 12.502 | (0.928) | 835546 | 200.000 | 100.51 (Q) |
| 70 4-Chloro Toluene | 91 | 12.552 | 12.552 | (0.932) | 905693 | 200.000 | 113.66 (Q) |
| 71 T-Butyl Benzene | 119 | 12.854 | 12.854 | (0.954) | 852231 | 200.000 | 125.22 (Q) |
| 72 1,2,4-Trimethylbenzene | 105 | 12.904 | 12.904 | (0.958) | 866210 | 200.000 | 110.61 (Q) |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.095 | (0.972) | 959505 | 200.000 | 85.695 (Q) |
| 74 4-Isopropyl Toluene | 119 | 13.246 | 13.246 | (0.984) | 862152 | 200.000 | 112.22 (Q) |
| 75 1,3-Dichlorobenzene | 146 | 13.397 | 13.397 | (0.995) | 707131 | 200.000 | 151.50 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 145587 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.507 | (1.003) | 703363 | 200.000 | 150.59 |
| 78 N-Butyl Benzene | 91 | 13.728 | 13.728 | (1.019) | 866011 | 200.000 | 104.39 (Q) |
| § 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.919 | (1.034) | 127083 | 50.0000 | 47.990 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.949 | (1.036) | 673403 | 200.000 | 151.80 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.854 | 14.854 | (1.103) | 74509 | 200.000 | 152.08 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.899 | (1.181) | 430578 | 200.000 | 159.50 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.050 | (1.192) | 315558 | 200.000 | 173.56 |
| 84 Naphthalene | 128 | 16.231 | 16.231 | (1.205) | 551716 | 200.000 | 112.68 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.512 | (1.226) | 376206 | 200.000 | 145.77 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 2000723.d
 Lab Smp Id: IC0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: VSTD200
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 159149 | 21.38 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 229095 | 19.60 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 171495 | 6.39 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 145587 | 64.92 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.79 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Data File: /chem1/finm5.i/23JUL10.b/2000723.d

Date : 23-JUL-2010 17:18

Client ID: VSTD200

Sample Info: IC0723.5.5.0


Column phase: Rtx502.2

Instrument: finm5.i

Operator: PB

Column diameter: 0.18

/chem1/finm5.i/23JUL10.b/2000723.d/2000723.L6



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/23JUL10.b/ICV0723.d
 Lab Smp Id: ICV0723 Client Smp ID: ICV0723
 Inj Date : 23-JUL-2010 22:14
 Operator : PB Inst ID: finn5.i
 Smp Info : ICV0723,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/23JUL10.b/s8260b.m
 Meth Date : 29-Jul-2010 14:29 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

patrickb

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|---|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 3.015 | (0.454) | 88303 | 52.1032 | 52.103 |
| 2 Chloromethane | 50 | 3.306 | 3.316 | (0.499) | 217848 | 47.7755 | 47.775 |
| 3 Vinyl Chloride | 62 | 3.417 | 3.417 | (0.516) | 192357 | 53.3461 | 53.346 |
| 4 Bromomethane | 94 | 3.909 | 3.909 | (0.590) | 122206 | 62.4063 | 62.406 |
| 5 Chloroethane | 64 | 3.980 | 3.980 | (0.601) | 123869 | 52.6030 | 52.603 |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.241 | (0.640) | 196733 | 56.4516 | 56.452 |
| 7 Acrolein | 56 | 4.623 | 4.633 | (0.698) | 109928 | 252.871 | 252.87 |
| 8 1,1,2-Trichloro-2,2,2-Trifluoroethane | 101 | 4.643 | 4.643 | (0.701) | 142159 | 52.1041 | 52.104 |
| 9 Acetone | 43 | 4.683 | 4.693 | (0.707) | 183316 | 250.626 | 250.63 |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.844 | (0.730) | 130784 | 52.8244 | 52.824 |
| 11 Bromoethane | 108 | 5.055 | 5.055 | (0.763) | 98954 | 53.9712 | 53.971 |
| 12 Iodomethane | 142 | 5.156 | 5.156 | (0.778) | 164327 | 56.1364 | 56.136 |
| 13 Methylene Chloride | 84 | 5.276 | 5.276 | (0.797) | 130295 | 46.7382 | 46.738 |
| 14 Acrylonitrile | 53 | 5.357 | 5.367 | (0.809) | 36679 | 56.7973 | 56.797(Q) |

| Compounds | QUANT SIG | | CONCENTRATIONS | | | | |
|------------------------------|-----------|--------|----------------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.407 | (0.815) | 193967 | 50.9456 | 50.946 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.377 | (0.812) | 446067 | 58.0915 | 58.092 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.558 | (0.839) | 107789 | 51.0864 | 51.086 |
| 18 Vinyl Acetate | 43 | 5.879 | 5.879 | (0.888) | 205828 | 55.6982 | 55.698 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.940 | (0.897) | 207542 | 53.4687 | 53.469 |
| 20 2-Butanone | 43 | 6.281 | 6.291 | (0.948) | 220070 | 267.396 | 267.40 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.462 | (0.976) | 115299 | 48.5440 | 48.544 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.502 | (0.980) | 96880 | 52.0962 | 52.096 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.623 | (1.000) | 130699 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.643 | (1.003) | 163311 | 51.7971 | 51.797 |
| 26 Bromochloromethane | 128 | 6.804 | 6.814 | (1.027) | 45855 | 51.9357 | 51.936 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.844 | (1.033) | 79530 | 51.0546 | 51.055 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.035 | (1.062) | 121554 | 49.5682 | 49.568 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.176 | (0.939) | 128897 | 48.8768 | 48.877 |
| 30 Carbon Tetrachloride | 117 | 7.296 | 7.296 | (0.955) | 112147 | 48.9029 | 48.903 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.306 | (1.103) | 85607 | 50.2236 | 50.224 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.397 | (0.968) | 113558 | 49.0506 | 49.051 |
| 33 Benzene | 78 | 7.437 | 7.447 | (0.974) | 327392 | 51.3396 | 51.340 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.638 | (1.000) | 194200 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.010 | (1.049) | 89432 | 47.8663 | 47.866 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.171 | (1.070) | 96896 | 48.2020 | 48.202 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.412 | (1.100) | 105966 | 49.3042 | 49.304 |
| 39 Dibromomethane | 93 | 8.472 | 8.472 | (1.109) | 50061 | 50.1678 | 50.168 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.623 | (1.129) | 36400 | 51.7056 | 51.706 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.663 | (1.133) | 124957 | 243.406 | 243.40 |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.914 | (1.166) | 119381 | 50.8758 | 50.876 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.186 | (1.203) | 213419 | 50.0149 | 50.015 |
| 44 Toluene | 92 | 9.266 | 9.276 | (1.213) | 178106 | 47.0736 | 47.074 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.407 | (1.230) | 97312 | 49.3376 | 49.338 |
| 46 2-Hexanone | 43 | 9.527 | 9.537 | (0.884) | 302971 | 230.222 | 230.22 |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.588 | (1.254) | 58163 | 49.3789 | 49.379 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.839 | (0.912) | 111278 | 49.1112 | 49.111 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.960 | (0.924) | 77284 | 43.2093 | 43.209 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.171 | (0.942) | 74343 | 48.7727 | 48.773 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.392 | (1.361) | 60617 | 48.0450 | 48.045 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.794 | (1.000) | 160989 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.834 | (1.004) | 173699 | 46.0010 | 46.001 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.864 | (1.007) | 323591 | 50.6763 | 50.676 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.864 | (1.007) | 63372 | 43.8510 | 43.851 |
| 56 m,p-xylene | 106 | 10.944 | 10.944 | (1.015) | 245109 | 105.022 | 105.02 |
| 57 o-Xylene | 106 | 11.427 | 11.437 | (1.060) | 120691 | 49.7567 | 49.757 |
| 58 Styrene | 104 | 11.457 | 11.467 | (1.062) | 197449 | 52.6464 | 52.646 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.819 | (0.877) | 319484 | 52.7192 | 52.719 |
| 60 Bromoform | 173 | 11.869 | 11.879 | (0.881) | 46057 | 47.2689 | 47.269 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.990 | (0.890) | 81604 | 46.6101 | 46.610 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.110 | (1.123) | 92917 | 49.3160 | 49.316 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.160 | (0.903) | 16385 | 47.2399 | 47.240 |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------------------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.211 | (0.907) | 26774 | 49.7563 | 49.756 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.271 | (0.910) | 379504 | 48.5107 | 48.511 |
| 67 Bromobenzene | 156 | 12.351 | 12.361 | (0.917) | 77896 | 46.1089 | 46.109 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.442 | (0.923) | 260307 | 52.9158 | 52.916 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.502 | (0.928) | 265535 | 51.6571 | 51.657 |
| 70 4-Chloro Toluene | 91 | 12.542 | 12.552 | (0.931) | 238191 | 48.3413 | 48.341 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.854 | (0.954) | 232736 | 55.3018 | 55.302 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.904 | (0.957) | 256248 | 52.9143 | 52.914 |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.095 | (0.972) | 356050 | 51.4252 | 51.425 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.246 | (0.983) | 257043 | 54.1060 | 54.106 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.397 | (0.994) | 136992 | 47.4636 | 47.464 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.467 | (1.000) | 90026 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.507 | (1.003) | 134851 | 46.6906 | 46.691 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.728 | (1.019) | 266189 | 51.8878 | 51.888 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.919 | (1.033) | 82049 | 50.1059 | 50.106 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.949 | (1.036) | 130036 | 47.4052 | 47.405 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.854 | (1.102) | 14043 | 46.3542 | 46.354 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.899 | (1.181) | 62702 | 37.5627 | 37.563 (R) |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.050 | (1.192) | 47253 | 42.0301 | 42.030 |
| 84 Naphthalene | 128 | 16.221 | 16.231 | (1.204) | 125569 | 41.4735 | 41.473 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.512 | (1.226) | 61205 | 38.3513 | 38.351 |

QC Flag Legend

- Q - Qualifier signal failed the ratio test.
- R - Spike/Surrogate failed recovery limits.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: ICV0723.d
 Lab Smp Id: ICV0723
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 23-JUL-2010
 Calibration Time: 18:42
 Client Smp ID: ICV0723
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 130699 | -0.32 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 194200 | 1.38 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 160989 | -0.13 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 90026 | 1.98 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.62 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.78 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.47 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Client SDG: 23JUL10
 Sample Matrix: SOLID Fraction: VOA
 Lab Smp Id: ICV0723 Client Smp ID: ICV0723
 Level: LOW Operator: PB
 Data Type: MS DATA SampleType: LCS
 SpikeList File: all.spk Quant Type: ISTD
 Sublist File: voa.sub
 Method File: /chem1/finn5.i/23JUL10.b/s8260b.m
 Misc Info: 10-

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 1 Dichlorodifluorome | 50.000 | 52.103 | 104.21 | 53-148 |
| 2 Chloromethane | 50.000 | 47.775 | 95.55 | 64-125 |
| 3 Vinyl Chloride | 50.000 | 53.346 | 106.69 | 63-137 |
| 4 Bromomethane | 50.000 | 62.406 | 124.81 | 57-136 |
| 5 Chloroethane | 50.000 | 52.603 | 105.21 | 64-131 |
| 6 Trichlorofluoromet | 50.000 | 56.452 | 112.90 | 69-132 |
| 7 Acrolein | 250.00 | 252.87 | 101.15 | 54-137 |
| 8 112Trichloro122Tri | 50.000 | 52.104 | 104.21 | 74-130 |
| 9 Acetone | 250.00 | 250.63 | 100.25 | 60-131 |
| 10 1,1-Dichloroethene | 50.000 | 52.824 | 105.65 | 75-126 |
| 11 Bromoethane | 50.000 | 53.971 | 107.94 | 76-126 |
| 12 Iodomethane | 50.000 | 56.136 | 112.27 | 65-139 |
| 13 Methylene Chloride | 50.000 | 46.738 | 93.48 | 70-123 |
| 15 Carbon Disulfide | 50.000 | 58.092 | 116.18 | 71-129 |
| 14 Acrylonitrile | 50.000 | 56.797 | 113.59 | 67-125 |
| 16 Methyl tert-Butyl | 50.000 | 50.946 | 101.89 | 70-120 |
| 17 Trans-1,2-Dichloro | 50.000 | 51.086 | 102.17 | 80-120 |
| 18 Vinyl Acetate | 50.000 | 55.698 | 111.40 | 60-136 |
| 19 1,1-Dichloroethane | 50.000 | 53.469 | 106.94 | 80-120 |
| 20 2-Butanone | 250.00 | 267.40 | 106.96 | 70-120 |
| 21 2,2-Dichloropropan | 50.000 | 48.544 | 97.09 | 74-123 |
| 22 Cis-1,2-Dichloroet | 50.000 | 52.096 | 104.19 | 80-120 |
| 24 Chloroform | 50.000 | 51.797 | 103.59 | 80-120 |
| 26 Bromochloromethane | 50.000 | 51.936 | 103.87 | 80-120 |
| 27 1,1,1-Trichloroeth | 50.000 | 49.568 | 99.14 | 77-121 |
| 29 1,1-Dichloropropen | 50.000 | 48.877 | 97.75 | 80-120 |
| 30 Carbon Tetrachlori | 50.000 | 48.903 | 97.81 | 77-122 |
| 32 1,2-Dichloroethane | 50.000 | 49.051 | 98.10 | 76-120 |
| 33 Benzene | 50.000 | 51.340 | 102.68 | 80-120 |
| 35 Trichloroethene | 50.000 | 47.866 | 95.73 | 80-120 |
| 36 1,2-Dichloropropan | 50.000 | 48.202 | 96.40 | 80-120 |
| 37 Bromodichlorometha | 50.000 | 49.304 | 98.61 | 77-121 |
| 39 Dibromomethane | 50.000 | 50.168 | 100.34 | 80-120 |


| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 40 2-Chloroethyl Viny | 50.000 | 51.706 | 103.41 | 10-19I |
| 41 4-Methyl-2-Pentano | 250.00 | 243.40 | 97.36 | 67-120 |
| 42 Cis 1,3-dichloropr | 50.000 | 50.876 | 101.75 | 74-120 |
| 44 Toluene | 50.000 | 47.074 | 94.15 | 80-120 |
| 45 Trans 1,3-Dichloro | 50.000 | 49.338 | 98.68 | 65-120 |
| 46 2-Hexanone | 250.00 | 230.22 | 92.09 | 65-130 |
| 47 1,1,2-Trichloroeth | 50.000 | 49.379 | 98.76 | 80-120 |
| 48 1,3-Dichloropropan | 50.000 | 49.111 | 98.22 | 80-120 |
| 49 Tetrachloroethene | 50.000 | 43.209 | 86.42 | 80-121 |
| 50 Chlorodibromometha | 50.000 | 48.773 | 97.55 | 64-120 |
| 51 1,2-Dibromoethane | 50.000 | 48.045 | 96.09 | 75-120 |
| 53 Chlorobenzene | 50.000 | 46.001 | 92.00 | 80-120 |
| 55 1,1,1,2-Tetrachlor | 50.000 | 43.851 | 87.70 | 69-121 |
| 54 Ethyl Benzene | 50.000 | 50.676 | 101.35 | 80-127 |
| 56 m,p-xylene | 100.00 | 105.02 | 105.02 | 80-125 |
| 57 o-Xylene | 50.000 | 49.757 | 99.51 | 78-120 |
| 58 Styrene | 50.000 | 52.646 | 105.29 | 80-123 |
| 59 Isopropyl Benzene | 50.000 | 52.719 | 105.44 | 80-127 |
| 60 Bromoform | 50.000 | 47.269 | 94.54 | 60-120 |
| 61 1,1,2,2-Tetrachlor | 50.000 | 46.610 | 93.22 | 74-120 |
| 63 1,2,3-Trichloropro | 50.000 | 47.240 | 94.48 | 72-121 |
| 65 Trans-1,4-Dichloro | 50.000 | 49.756 | 99.51 | 65-126 |
| 66 N-Propyl Benzene | 50.000 | 48.511 | 97.02 | 80-132 |
| 67 Bromobenzene | 50.000 | 46.109 | 92.22 | 80-120 |
| 68 1,3,5-Trimethyl Be | 50.000 | 52.916 | 105.83 | 80-125 |
| 69 2-Chloro Toluene | 50.000 | 51.657 | 103.31 | 80-125 |
| 70 4-Chloro Toluene | 50.000 | 48.341 | 96.68 | 80-127 |
| 71 T-Butyl Benzene | 50.000 | 55.302 | 110.60 | 87-122 |
| 72 1,2,4-Trimethylben | 50.000 | 52.914 | 105.83 | 80-126 |
| 73 S-Butyl Benzene | 50.000 | 51.425 | 102.85 | 80-134 |
| 74 4-Isopropyl Toluen | 50.000 | 54.106 | 108.21 | 80-131 |
| 75 1,3-Dichlorobenzen | 50.000 | 47.464 | 94.93 | 80-120 |
| 77 1,4-Dichlorobenzen | 50.000 | 46.691 | 93.38 | 80-120 |
| 78 N-Butyl Benzene | 50.000 | 51.888 | 103.78 | 80-138 |
| 80 1,2-Dichlorobenzen | 50.000 | 47.405 | 94.81 | 80-120 |
| 81 1,2-Dibromo 3-Chlo | 50.000 | 46.354 | 92.71 | 59-120 |
| 82 1,2,4-Trichloroben | 50.000 | 37.563 | 75.13* | 78-130 |
| 83 Hexachloro 1,3-But | 50.000 | 42.030 | 84.06 | 76-129 |
| 84 Naphthalene | 50.000 | 41.473 | 82.95 | 66-120 |
| 85 1,2,3-Trichloroben | 50.000 | 38.351 | 76.70 | 73-123 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 51.055 | 102.11 | 30-160 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 50.224 | 100.45 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 50.015 | 100.03 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 49.316 | 98.63 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.106 | 100.21 | 80-120 |

Data File: /chem1/finm5.i/23JUL10.b/ICV0723.d
Date: 23-JUL-2010 22:14
Client ID: ICV0723
Sample Info: ICV0723.5.5.0
Column phase: Rtx502.2

Instrument: finm5.i
Operator: PB
Column diameter: 0.18



/chem1/finm5.i/23JUL10.b/ICV0723.d/ICV0723.LG

**Volatile Raw Data
Run Logs, Continuing Calibrations, and Raw Data**

ARI Job ID: RG58



VOA Analyst Notes / Corrective Action Log

ARI Project ID: RG58 Client ID: Floyd Sander

ARI SOP: **404S**(Gas) **410S**(BTEX) **430S**(VPH) **700S**(8260C) **703S**(SIM) **706S**(524.2) **710S**(RSK-175)

Parameter(s): _____

Instrument: NT-3 NT-5 NT-7 NT-9 NT-10 PID-1 PID-2 PID-3 FID-6 **FINN-5**

Purge Volume (mL) 5 Curve Date: 7/23/10 Analysis Start Date: 8/16/10

| | | | |
|-----------------------------------|-----------------------------|----------------------------------|-----------------------------|
| pH ≤ 2.0 | YES / NO / NA | Method Blank In Control? | YES / NO |
| BFB Tune Meets Criteria? | YES / NO / NA | LCS / LCSD Recovery In Control? | YES / NO |
| Internal Standard Meets Criteria? | YES / NO / NA | Surrogate Recovery In Control? | YES / NO |
| ICal acceptable? | YES / NO | CCal acceptable? | YES / NO |
| Q flag applied? | YES / NO / NA | Q flag applied? | YES / NO / NA |
| Manual Integrations for ICal? | YES / NO | Manual Integrations for Samples? | Yes / NO |
| Special Analysis Criteria Met? | YES / NO / NA | | |

Bubbles/Headspace: **None** SM (≤ 2mm ●) PB (2-4mm) LG (> 4mm ●) Head Space

Detail problems, corrective actions and/or other pertinent information below (use reverse side when necessary):

Additional Details on Reverse: Yes / **No**

Analyst: _____ Date: 8/16/10

Reviewer: _____ Date: 8/16/10

MANUAL INTEGRATION SUMMARY FOR DATABATCH - /chem1/finn5.i/09AUG10.b

ARI Job No.: BFB0 Method: bfb8260.m Instrument: finn5.i Date: 09-AUG-2010

Time Filename LabID ClientId DF Manually Integrated Compounds

0918 BFB0809.d BFB0809 BFB0809 1 NO MANUAL INTEGRATION

1035 0500809.d CC0809 VSTD050 1 NO MANUAL INTEGRATION

1122 LCS0809.d LCS0809 LCS0809 1 NO MANUAL INTEGRATION

1149 LCS0809A.d LCS0809 LCS0809 1 NO MANUAL INTEGRATION

1216 MB0809.d MB0809 MB0809 1 NO MANUAL INTEGRATION

1611 RG58A.d RG58A PSB22-0-0. 1 NO MANUAL INTEGRATION

1638 RG58B.d RG58B PSB22-1.5- 1 NO MANUAL INTEGRATION

1704 RG58C.d RG58C PSB22-2-4- 1 NO MANUAL INTEGRATION

1731 RG58D.d RG58D PSB22-4-6- 1 NO MANUAL INTEGRATION

1757 RG58E.d RG58E PSB22-17-1 1 NO MANUAL INTEGRATION

1824 RG58F.d RG58F PSB22-19-2 1 NO MANUAL INTEGRATION

1850 RG58K.d RG58K PSB23-14-1 1 NO MANUAL INTEGRATION

1916 RG58L.d RG58L PSB23-16.5 1 NO MANUAL INTEGRATION

1943 RG58T.d RG58T PSB22-TB 1 NO MANUAL INTEGRATION

2009 RG58U.d RG58U PSB23-TB 1 NO MANUAL INTEGRATION

2035 RG58V.d RG58V PSB24-TB 1 NO MANUAL INTEGRATION

2102 RG58R.d RG58R PSB24-14-1 1 NO MANUAL INTEGRATION

2128 RG58S.d RG58S PSB24-16-1 1 NO MANUAL INTEGRATION

2009 2035 2102 2128

Analytical Resources Inc.: Organics Instrument Log

FINN5 Serial No.: 5500-000421A

Date: 7/25/10 Analysis: Stanc Analyst: 17
 GC Program: PS Column No: 821729 Column Type: RX502-2
 Instrument Tune (.U or .CT.): BFB0809 EM Voltage: 1635
 Calibration File: 0500809 Curve Date: 7/25/10

IS/SS W644-L Ical/Ccal W644-L LCS/ICV W644-L

INTERNAL STANDARD SUMMARY FOR DATABATCH - /chem1/finn5.i/09AUG10.b

| Time | Filename | LabID | ClientID | WT |
|---------|------------|---------|---------------------|---|
| 1 0918 | BFB0809.d | BFB0809 | BFB0809 | 0.00 |
| 2 1035 | 0500809.d | CC0809 | VSTD050 | 5.00 6.61 112191 7.63 159474 10.77 135755 13.46 72226 |
| 3 1122 | LCS0809.d | LCS0809 | LCS0809 | 5.00 6.62 103776 7.64 147372 10.78 120524 13.47 65104 |
| 4 1149 | LCS0809A.d | LCS0809 | LCS0809 | 5.00 6.63 106566 7.64 157864 10.79 135479 13.47 75648 |
| 5 1216 | MB0809.d | MB0809 | MB0809 | 5.00 6.61 95082 7.63 136899 10.77 118413 13.46 58588 |
| 6 1258 | RH52A.d | RH52A | Baker Composit | 5.00 6.63 91323 7.64 133054 10.79 105354 13.47 43218 |
| 7 1332 | RH20A.d | RH20A | IT-ROB-CMP1-080410 | 5.00 6.62 92263 7.64 134744 10.78 102778 13.47 39784 |
| 8 1359 | RH20B.d | RH20B | IT-ROB-CMP2-080410 | 5.00 6.61 101332 7.63 146678 10.77 110534 13.46 40349 |
| 9 1425 | RG52C.d | RG52C | KSC-DP-7-S-3.5-4-10 | 5.00 6.62 105845 7.64 157020 10.78 136856 13.47 69288 |
| 10 1454 | RG52D.d | RG52D | KSC-DP-8-S-4.5-5-10 | 5.00 6.62 100289 7.64 151250 10.78 133181 13.47 70722 |
| 11 1518 | RG52E.d | RG52E | KSC-DP-9-S-5.5-6-10 | 5.00 6.62 112463 7.63 165613 10.78 139681 13.46 68152 |
| 12 1545 | RG52F.d | RG52F | KSC-DP-3-S-7-8-1007 | 5.00 6.63 99182 7.64 153470 10.79 141191 13.47 78283 |
| 13 1611 | RG58A.d | RG58A | PSB22-0-0.5-072910 | 5.00 6.62 163926 7.63 239062 10.78 194173 13.46 95238 |
| 14 1638 | RG58B.d | RG58B | PSB22-1.5-2-072910 | 5.00 6.63 141403 7.65 209666 10.79 174438 13.48 83991 |
| 15 1704 | RG58C.d | RG58C | PSB22-2-4-072910 | 5.00 6.62 123053 7.64 179902 10.78 151011 13.47 75393 |
| 16 1731 | RG58D.d | RG58D | PSB22-4-6-072910 | 5.00 6.62 114044 7.64 169449 10.78 144305 13.47 70759 |
| 17 1757 | RG58E.d | RG58E | PSB22-17-19-072910 | 5.00 6.63 110155 7.65 166411 10.79 149317 13.48 78068 |
| 18 1824 | RG58F.d | RG58F | PSB22-19-20-072910 | 5.00 6.63 103536 7.65 156457 10.79 137444 13.48 73064 |
| 19 1850 | RG58K.d | RG58K | PSB23-14-16.5-07291 | 5.00 6.62 104622 7.64 159024 10.78 137738 13.47 67417 |
| 20 1916 | RG58L.d | RG58L | PSB23-16.5-19-07291 | 5.00 6.62 100728 7.63 154377 10.78 139039 13.46 72259 |
| 21 1943 | RG58T.d | RG58T | PSB22-TB 2 LZ | 1 6.61 97416 7.63 148990 10.77 126813 13.46 61537 |
| 22 2009 | RG58U.d | RG58U | PSB23-TB 2 L | 1 6.62 100027 7.64 154248 10.78 136628 13.47 65693 |
| 23 2035 | RG58V.d | RG58V | PSB24-TB 1 LZ | 1 6.62 100981 7.64 154524 10.78 131451 13.47 64680 |
| 24 2102 | RG58R.d | RG58R | PSB24-14-16-072910 | 5.00 6.63 101772 7.64 157962 10.79 139242 13.47 70424 |
| 25 2128 | RG58S.d | RG58S | PSB24-16-17-072910 | 5.00 6.63 102459 7.64 160501 10.79 141767 13.47 71469 |

Mai

Mair
Every

Handwritten signature and scribbles over the bottom half of the table.

Q-FLAG SUMMARY FOR DATABATCH - /chem1/finn5.i/09AUG10.b

Instrument: finn5.i Date: 09-AUG-2010 Method: s8260b.m

INITIAL CAL: 23-JUL-2010

| Compound | %RSD or R ² |
|------------|------------------------|
| ----- | |
| NO Q-FLAGS | |
| ----- | |

CONTINUING CAL: 09-AUG-2010

| Compound | %D |
|---------------------------|-------|
| ----- | |
| Chloromethane | -27.2 |
| Methylene Chloride | -26.5 |
| 1,1,1,2-Tetrachloroethane | -23.5 |
| ----- | |

Date : 09-AUG-2010 09:18

Client ID: BFB0809

Instrument: finn5.i

Sample Info: BFB0809,BFB0809,,1,09AUG10,,


Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

1 Bromofluorobenzene

Handwritten signature



| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 95 | Base Peak, 100% relative abundance | 100.00 |
| 50 | 8.00 - 40.00% of mass 95 | 26.45 |
| 75 | 30.00 - 66.00% of mass 95 | 50.45 |
| 96 | 5.00 - 9.00% of mass 95 | 6.80 |
| 173 | Less than 2.00% of mass 174 | 0.13 (0.18) |
| 174 | 50.00 - 101.00% of mass 95 | 69.08 |
| 175 | 4.00 - 9.00% of mass 174 | 5.10 (7.38) |
| 176 | 93.00 - 101.00% of mass 174 | 69.46 (100.54) |
| 177 | 5.00 - 9.00% of mass 176 | 4.37 (6.29) |

Date : 09-AUG-2010 09:18

Client ID: BFB0809

Instrument: finn5.i

Sample Info: BFB0809,BFB0809,,1,09AUG10,,

Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

Data File: BFB0809.d

Spectrum: Average Spectrum: 12.090 to 12.110 min. (SUB)

Location of Maximum: 95.00

Number of points: 61

| m/z | Y | m/z | Y | m/z | Y | m/z | Y |
|-------|------|-------|-------|-------|-------|--------|-------|
| 34.00 | 5 | 57.00 | 557 | 76.00 | 938 | 104.00 | 38 |
| 36.00 | 276 | 58.00 | 20 | 77.00 | 57 | 117.00 | 79 |
| 37.00 | 1563 | 60.00 | 142 | 78.00 | 45 | 118.00 | 21 |
| 38.00 | 1481 | 61.00 | 930 | 79.00 | 418 | 128.00 | 34 |
| 39.00 | 549 | 62.00 | 1000 | 80.00 | 207 | 130.00 | 25 |
| 42.00 | 22 | 63.00 | 729 | 81.00 | 490 | 141.00 | 95 |
| 44.00 | 95 | 64.00 | 46 | 82.00 | 127 | 143.00 | 159 |
| 45.00 | 316 | 65.00 | 24 | 83.00 | 76 | 172.00 | 22 |
| 47.00 | 276 | 67.00 | 128 | 87.00 | 798 | 173.00 | 25 |
| 48.00 | 121 | 68.00 | 2362 | 88.00 | 717 | 174.00 | 13762 |
| 49.00 | 1083 | 69.00 | 2069 | 91.00 | 41 | 175.00 | 1016 |
| 50.00 | 5269 | 70.00 | 116 | 92.00 | 496 | 176.00 | 13837 |
| 51.00 | 1660 | 72.00 | 54 | 93.00 | 838 | 177.00 | 871 |
| 52.00 | 54 | 73.00 | 808 | 94.00 | 2091 | | |
| 53.00 | 85 | 74.00 | 3157 | 95.00 | 19920 | | |
| 56.00 | 279 | 75.00 | 10050 | 96.00 | 1354 | | |

Data File: /chem1/finn5.i/09AUG10.b/BFB0809.d

Date: 09-AUG-2010 09:18

Client ID: BFB0809

Sample Info: BFB0809, BFB0809, 1,09AUG10,,


Page 1

Instrument: finn5.i

Operator: PB

Column diameter: 0.18

Column phase: RTX502.2



RG58 : 00417

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/0500809.d
 Lab Smp Id: CC0809 Client Smp ID: VSTD050
 Inj Date : 09-AUG-2010 10:35
 Operator : PB Inst ID: finn5.i
 Smp Info : CC0809,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 09-Aug-2010 11:39 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | | AMOUNTS | | | | | |
|----------------------------------|-----------|-----|---------|--------|---------|----------|-----------------|----------------|
| | MASS | SIG | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | == | 2.995 | 2.995 | (0.453) | 61463 | 50.0000 | 42.249 |
| 2 Chloromethane | 50 | == | 3.296 | 3.296 | (0.498) | 142414 | 50.0000 | 36.384 |
| 3 Vinyl Chloride | 62 | == | 3.407 | 3.407 | (0.515) | 128656 | 50.0000 | 41.566 |
| 4 Bromomethane | 94 | == | 3.899 | 3.899 | (0.590) | 96693 | 50.0000 | 57.523 |
| 5 Chloroethane | 64 | == | 3.970 | 3.970 | (0.600) | 86529 | 50.0000 | 42.808 |
| 6 Trichlorofluoromethane | 101 | == | 4.231 | 4.231 | (0.640) | 137131 | 50.0000 | 45.840 |
| 7 Acrolein | 56 | == | 4.613 | 4.613 | (0.698) | 76413 | 250.000 | 204.77 |
| 8 112Trichloro122Trifluoroethane | 101 | == | 4.633 | 4.633 | (0.701) | 102926 | 50.0000 | 43.948 |
| 9 Acetone | 43 | == | 4.673 | 4.673 | (0.707) | 137058 | 250.000 | 218.30 |
| 10 1,1-Dichloroethene | 96 | == | 4.824 | 4.824 | (0.729) | 91771 | 50.0000 | 43.181 |
| 11 Bromoethane | 108 | == | 5.045 | 5.045 | (0.763) | 68137 | 50.0000 | 43.294 |
| 12 Iodomethane | 142 | == | 5.146 | 5.146 | (0.778) | 130904 | 50.0000 | 52.095 |
| 13 Methylene Chloride | 84 | == | 5.266 | 5.266 | (0.796) | 87957 | 50.0000 | 36.756 |
| 14 Acrylonitrile | 53 | == | 5.347 | 5.347 | (0.808) | 25510 | 50.0000 | 46.019 (Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.387 | 5.387 | (0.815) | 146056 | 50.0000 | 44.690 (Q) |
| 15 Carbon Disulfide | 76 | 5.367 | 5.367 | (0.812) | 307004 | 50.0000 | 46.577 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.548 | 5.548 | (0.839) | 76934 | 50.0000 | 42.478 |
| 18 Vinyl Acetate | 43 | 5.869 | 5.869 | (0.888) | 154106 | 50.0000 | 48.581 |
| 19 1,1-Dichloroethane | 63 | 5.929 | 5.929 | (0.897) | 149251 | 50.0000 | 44.794 |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.948) | 161034 | 250.0000 | 227.94 |
| 21 2,2-Dichloropropane | 77 | 6.452 | 6.452 | (0.976) | 91964 | 50.0000 | 45.107 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.982) | 69969 | 50.0000 | 43.832 |
| * 23 Pentafluorobenzene | 168 | 6.613 | 6.613 | (1.000) | 112191 | 50.0000 | |
| 24 Chloroform | 83 | 6.633 | 6.633 | (1.003) | 117524 | 50.0000 | 43.424 |
| 26 Bromochloromethane | 128 | 6.794 | 6.794 | (1.027) | 32527 | 50.0000 | 42.918 |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.033) | 63713 | 50.0000 | 47.648 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.062) | 89998 | 50.0000 | 42.754 |
| 29 1,1-Dichloropropene | 75 | 7.166 | 7.166 | (0.939) | 98963 | 50.0000 | 45.698 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.955) | 80551 | 50.0000 | 42.774 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.103) | 69074 | 50.0000 | 47.210 |
| 32 1,2-Dichloroethane | 62 | 7.387 | 7.387 | (0.968) | 85020 | 50.0000 | 44.721 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.975) | 237165 | 50.0000 | 45.289 |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 159474 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.049) | 67463 | 50.0000 | 43.971 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.070) | 69854 | 50.0000 | 42.317 |
| 37 Bromodichloromethane | 83 | 8.392 | 8.392 | (1.100) | 78743 | 50.0000 | 44.616 |
| 39 Dibromomethane | 93 | 8.462 | 8.462 | (1.109) | 36515 | 50.0000 | 44.561 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.129) | 28752 | 50.0000 | 49.736 |
| 41 4-Methyl-2-Pentanone | 58 | 8.643 | 8.643 | (1.133) | 92652 | 250.0000 | 219.78 |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.167) | 91241 | 50.0000 | 47.351 |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 186141 | 50.0000 | 53.121 |
| 44 Toluene | 92 | 9.256 | 9.256 | (1.213) | 133097 | 50.0000 | 42.838 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.387 | 9.387 | (1.231) | 75540 | 50.0000 | 46.639 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 225310 | 250.0000 | 203.03 |
| 47 1,1,2-Trichloroethane | 97 | 9.568 | 9.568 | (1.254) | 42002 | 50.0000 | 43.424 |
| 48 1,3-Dichloropropane | 76 | 9.829 | 9.829 | (0.912) | 82164 | 50.0000 | 43.002 |
| 49 Tetrachloroethene | 166 | 9.949 | 9.949 | (0.924) | 63144 | 50.0000 | 41.866 |
| 50 Chlorodibromomethane | 129 | 10.161 | 10.161 | (0.943) | 53188 | 50.0000 | 41.380 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.361) | 46239 | 50.0000 | 44.630 |
| * 52 d5-Chlorobenzene | 117 | 10.774 | 10.774 | (1.000) | 135755 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.824 | 10.824 | (1.005) | 136424 | 50.0000 | 42.845 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 253580 | 50.0000 | 47.094 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.844 | 10.844 | (1.007) | 46626 | 50.0000 | 38.261 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.015) | 193016 | 100.0000 | 98.074 |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.061) | 93660 | 50.0000 | 45.790 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.063) | 153410 | 50.0000 | 48.507 |
| 59 Isopropyl Benzene | 105 | 11.799 | 11.799 | (0.877) | 251279 | 50.0000 | 51.683 |
| 60 Bromoform | 173 | 11.859 | 11.859 | (0.881) | 33177 | 50.0000 | 42.442 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.980 | 11.980 | (0.890) | 58031 | 50.0000 | 41.315 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.123) | 77522 | 50.0000 | 48.793 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.903) | 11974 | 50.0000 | 43.032 |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|--------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.201 | 12.201 | (0.907) | 21053 | 50.0000 | 48.767 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.911) | 313485 | 50.0000 | 49.947 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.918) | 59704 | 50.0000 | 44.050 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.924) | 209424 | 50.0000 | 53.064 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 202179 | 50.0000 | 49.025 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 200645 | 50.0000 | 50.757 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 183864 | 50.0000 | 54.456 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.884 | 12.884 | (0.957) | 210320 | 50.0000 | 54.134 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 283027 | 50.0000 | 50.953 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.984) | 217185 | 50.0000 | 56.983 |
| 75 1,3-Dichlorobenzene | 146 | 13.377 | 13.377 | (0.994) | 116977 | 50.0000 | 50.517 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 72226 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.003) | 116434 | 50.0000 | 50.249 |
| 78 N-Butyl Benzene | 91 | 13.708 | 13.708 | (1.019) | 240025 | 50.0000 | 58.318 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.034) | 62606 | 50.0000 | 47.655 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.036) | 103734 | 50.0000 | 47.137 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.844 | 14.844 | (1.103) | 10641 | 50.0000 | 43.784 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.889 | 15.889 | (1.181) | 67997 | 50.0000 | 50.774 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.192) | 43843 | 50.0000 | 48.608 |
| 84 Naphthalene | 128 | 16.211 | 16.211 | (1.205) | 110168 | 50.0000 | 45.354 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.502 | 16.502 | (1.226) | 56822 | 50.0000 | 44.380 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: 0500809.d
 Lab Smp Id: CC0809
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-

Calibration Date: 09-AUG-2010
 Calibration Time: 09:48
 Client Smp ID: VSTD050
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 112191 | -14.43 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 159474 | -16.75 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 135755 | -15.78 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 72226 | -18.18 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.62 | 6.12 | 7.12 | 6.61 | -0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.77 | -0.09 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.46 | -0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: finn5.i Injection Date: 09-AUG-2010 10:35
 Lab File ID: 0500809.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
 Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
 Lab Sample ID: CC0809 Quant Type: ISTD
 Method: /chem1/finn5.i/09AUG10.b/s8260b.m

| COMPOUND | RRF / AMOUNT | RF50 | MIN | | MAX | | CURVE TYPE |
|-------------------------------|--------------|---------|-------|-------------|-------------|----------|------------|
| | | | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 1 Dichlorodifluoromethane | 0.64835 | 0.54785 | 0.010 | -15.50138 | 20.00000 | Averaged | |
| 2 Chloromethane | 1.74440 | 1.26938 | 0.100 | -27.23111 | 20.00000 | Averaged | <- wly |
| 3 Vinyl Chloride | 1.37944 | 1.14676 | 0.010 | -16.86795 | 20.00000 | Averaged | |
| 4 Bromomethane | 0.74914 | 0.86186 | 0.010 | 15.04666 | 20.00000 | Averaged | |
| 5 Chloroethane | 0.90084 | 0.77126 | 0.010 | -14.38446 | 20.00000 | Averaged | |
| 6 Trichlorofluoromethane | 1.33321 | 1.22229 | 0.010 | -8.31957 | 20.00000 | Averaged | |
| 7 Acrolein | 0.16631 | 0.13622 | 0.010 | -18.09118 | 20.00000 | Averaged | |
| 8 112Trichloro122Trifluoroeth | 1.04376 | 0.91742 | 0.010 | -12.10446 | 20.00000 | Averaged | |
| 9 Acetone | 0.27982 | 0.24433 | 0.010 | -12.68179 | 20.00000 | Averaged | |
| 10 1,1-Dichloroethene | 0.94715 | 0.81798 | 0.010 | -13.63705 | 20.00000 | Averaged | |
| 11 Bromoethane | 0.70140 | 0.60733 | 0.010 | -13.41190 | 20.00000 | Averaged | |
| 12 Iodomethane | 1.11986 | 1.16679 | 0.010 | 4.19095 | 20.00000 | Averaged | |
| 13 Methylene Chloride | 1.06648 | 0.78400 | 0.010 | -26.48774 | 20.00000 | Averaged | <- wly |
| 14 Acrylonitrile | 0.24705 | 0.22738 | 0.010 | -7.96124 | 20.00000 | Averaged | |
| 16 Methyl tert-Butyl Ether | 1.45653 | 1.30185 | 0.010 | -10.61963 | 20.00000 | Averaged | |
| 15 Carbon Disulfide | 2.93755 | 2.73642 | 0.010 | -6.84669 | 20.00000 | Averaged | |
| 17 Trans-1,2-Dichloroethene | 0.80717 | 0.68574 | 0.010 | -15.04433 | 20.00000 | Averaged | |
| 18 Vinyl Acetate | 1.41371 | 1.37360 | 0.010 | -2.83766 | 20.00000 | Averaged | |
| 19 1,1-Dichloroethane | 1.48492 | 1.33033 | 0.100 | -10.41113 | 20.00000 | Averaged | |
| 20 2-Butanone | 0.31485 | 0.28707 | 0.010 | -8.82350 | 20.00000 | Averaged | |
| 21 2,2-Dichloropropane | 0.90863 | 0.81971 | 0.010 | -9.78633 | 20.00000 | Averaged | |
| 22 Cis-1,2-Dichloroethene | 0.71142 | 0.62366 | 0.010 | -12.33561 | 20.00000 | Averaged | |
| 24 Chloroform | 1.20617 | 1.04753 | 0.010 | -13.15233 | 20.00000 | Averaged | |
| 26 Bromochloromethane | 0.33777 | 0.28992 | 0.010 | -14.16486 | 20.00000 | Averaged | |
| \$ 25 Dibromofluoromethane | 0.59593 | 0.56790 | 0.010 | -4.70337 | 20.00000 | Averaged | |
| 27 1,1,1-Trichloroethane | 0.93813 | 0.80218 | 0.010 | -14.49136 | 20.00000 | Averaged | |
| 29 1,1-Dichloropropene | 0.67899 | 0.62056 | 0.010 | -8.60439 | 20.00000 | Averaged | |
| 30 Carbon Tetrachloride | 0.59044 | 0.50510 | 0.010 | -14.45252 | 20.00000 | Averaged | |
| \$ 31 d4-1,2-Dichloroethane | 0.65208 | 0.61569 | 0.010 | -5.58084 | 20.00000 | Averaged | |
| 32 1,2-Dichloroethane | 0.59607 | 0.53313 | 0.010 | -10.55837 | 20.00000 | Averaged | |
| 33 Benzene | 1.64186 | 1.48717 | 0.010 | -9.42172 | 20.00000 | Averaged | |
| 35 Trichloroethene | 0.48104 | 0.42304 | 0.010 | -12.05819 | 20.00000 | Averaged | |
| 36 1,2-Dichloropropane | 0.51756 | 0.43803 | 0.010 | -15.36637 | 20.00000 | Averaged | |
| 37 Bromodichloromethane | 0.55335 | 0.49377 | 0.010 | -10.76813 | 20.00000 | Averaged | |
| 39 Dibromomethane | 0.25692 | 0.22897 | 0.010 | -10.87722 | 20.00000 | Averaged | |

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: finn5.i Injection Date: 09-AUG-2010 10:35
 Lab File ID: 0500809.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
 Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
 Lab Sample ID: CC0809 Quant Type: ISTD
 Method: /chem1/finn5.i/09AUG10.b/s8260b.m

| COMPOUND | RRF / AMOUNT | RF50 | MIN | | MAX | | CURVE TYPE |
|--------------------------------|--------------|---------|-------|-------------|-------------|----------|------------|
| | | | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 40 2-Chloroethyl Vinyl Ether | 0.18125 | 0.18029 | 0.001 | -0.52898 | 20.00000 | Averaged | |
| 41 4-Methyl-2-Pentanone | 0.13218 | 0.11620 | 0.010 | -12.08808 | 20.00000 | Averaged | |
| 42 Cis 1,3-dichloropropene | 0.60415 | 0.57214 | 0.010 | -5.29813 | 20.00000 | Averaged | |
| 43 d8-Toluene | 1.09864 | 1.16722 | 0.010 | 6.24234 | 20.00000 | Averaged | |
| 44 Toluene | 0.97414 | 0.83460 | 0.010 | -14.32415 | 20.00000 | Averaged | |
| 45 Trans 1,3-Dichloropropene | 0.50782 | 0.47368 | 0.010 | -6.72218 | 20.00000 | Averaged | |
| 46 2-Hexanone | 0.40872 | 0.33194 | 0.010 | -18.78708 | 20.00000 | Averaged | |
| 47 1,1,2-Trichloroethane | 0.30327 | 0.26338 | 0.010 | -13.15209 | 20.00000 | Averaged | |
| 48 1,3-Dichloropropane | 0.70372 | 0.60524 | 0.010 | -13.99485 | 20.00000 | Averaged | |
| 49 Tetrachloroethene | 0.55550 | 0.46513 | 0.010 | -16.26830 | 20.00000 | Averaged | |
| 50 Chlorodibromomethane | 0.47341 | 0.39180 | 0.010 | -17.23913 | 20.00000 | Averaged | |
| 51 1,2-Dibromoethane | 0.32484 | 0.28995 | 0.010 | -10.73963 | 20.00000 | Averaged | |
| 53 Chlorobenzene | 1.17275 | 1.00493 | 0.300 | -14.31002 | 20.00000 | Averaged | |
| 54 Ethyl Benzene | 1.98319 | 1.86792 | 0.010 | -5.81262 | 20.00000 | Averaged | |
| 55 1,1,1,2-Tetrachloroethane | 0.44884 | 0.34346 | 0.010 | -23.47787 | 20.00000 | Averaged | |
| 56 m,p-xylene | 0.72486 | 0.71090 | 0.010 | -1.92606 | 20.00000 | Averaged | |
| 57 o-Xylene | 0.75335 | 0.68992 | 0.010 | -8.41956 | 20.00000 | Averaged | |
| 58 Styrene | 1.16482 | 1.13005 | 0.010 | -2.98551 | 20.00000 | Averaged | |
| 59 Isopropyl Benzene | 3.36576 | 3.47907 | 0.010 | 3.36668 | 20.00000 | Averaged | |
| 60 Bromoform | 0.54116 | 0.45936 | 0.100 | -15.11529 | 20.00000 | Averaged | |
| 61 1,1,1,2-Tetrachloroethane | 0.97237 | 0.80347 | 0.300 | -17.37036 | 20.00000 | Averaged | |
| 62 4-Bromofluorobenzene | 0.58517 | 0.57105 | 0.010 | -2.41333 | 20.00000 | Averaged | |
| 63 1,2,3-Trichloropropane | 0.19264 | 0.16579 | 0.010 | -13.93648 | 20.00000 | Averaged | |
| 65 Trans-1,4-Dichloro 2-Butene | 0.29886 | 0.29149 | 0.010 | -2.46619 | 20.00000 | Averaged | |
| 66 N-Propyl Benzene | 4.34491 | 4.34033 | 0.010 | -0.10548 | 20.00000 | Averaged | |
| 67 Bromobenzene | 0.93828 | 0.82663 | 0.010 | -11.89947 | 20.00000 | Averaged | |
| 68 1,3,5-Trimethyl Benzene | 2.73214 | 2.89956 | 0.010 | 6.12800 | 20.00000 | Averaged | |
| 69 2-Chloro Toluene | 2.85492 | 2.79926 | 0.010 | -1.94967 | 20.00000 | Averaged | |
| 70 4-Chloro Toluene | 2.73658 | 2.77802 | 0.010 | 1.51427 | 20.00000 | Averaged | |
| 71 T-Butyl Benzene | 2.33736 | 2.54568 | 0.010 | 8.91263 | 20.00000 | Averaged | |
| 72 1,2,4-Trimethylbenzene | 2.68961 | 2.91197 | 0.010 | 8.26729 | 20.00000 | Averaged | |
| 73 S-Butyl Benzene | 3.84536 | 3.91862 | 0.010 | 1.90526 | 20.00000 | Averaged | |
| 74 4-Isopropyl Toluene | 2.63853 | 3.00702 | 0.010 | 13.96563 | 20.00000 | Averaged | |
| 75 1,3-Dichlorobenzene | 1.60301 | 1.61960 | 0.010 | 1.03454 | 20.00000 | Averaged | |
| 77 1,4-Dichlorobenzene | 1.60408 | 1.61208 | 0.010 | 0.49872 | 20.00000 | Averaged | |

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS


Instrument ID: finn5.i Injection Date: 09-AUG-2010 10:35
Lab File ID: 0500809.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
Lab Sample ID: CC0809 Quant Type: ISTD
Method: /chem1/finn5.i/09AUG10.b/s8260b.m

| COMPOUND | RRF / AMOUNT | RF50 | MIN | | MAX | | CURVE TYPE |
|--------------------------------|--------------|---------|-------|-------------|-------------|----------|------------|
| | | | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 78 N-Butyl Benzene | 2.84923 | 3.32325 | 0.010 | 16.63677 | 20.00000 | Averaged | |
| 79 d4-1,2-Dichlorobenzene | 0.90947 | 0.86681 | 0.010 | -4.69003 | 20.00000 | Averaged | |
| 80 1,2-Dichlorobenzene | 1.52349 | 1.43625 | 0.010 | -5.72648 | 20.00000 | Averaged | |
| 81 1,2-Dibromo 3-Chloropropane | 0.16826 | 0.14734 | 0.010 | -12.43192 | 20.00000 | Averaged | |
| 82 1,2,4-Trichlorobenzene | 0.92710 | 0.94146 | 0.010 | 1.54875 | 20.00000 | Averaged | |
| 83 Hexachloro 1,3-Butadiene | 0.62441 | 0.60703 | 0.010 | -2.78352 | 20.00000 | Averaged | |
| 84 Naphthalene | 1.68157 | 1.52533 | 0.010 | -9.29109 | 20.00000 | Averaged | |
| 85 1,2,3-Trichlorobenzene | 0.88636 | 0.78673 | 0.010 | -11.24008 | 20.00000 | Averaged | |

Data File: /chem1/finn5.i/09AUG10.b/0500809.d
Date : 09-AUG-2010 10:35
Client ID: VSTD050
Sample Info: CC0809,5,5,0

Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



/chem1/finn5.i/09AUG10.b/0500809.d/0500809.LC

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/LCS0809.d
 Lab Smp Id: LCS0809 Client Smp ID: LCS0809
 Inj Date : 09-AUG-2010 11:22
 Operator : PB Inst ID: finn5.i
 Smp Info : LCS0809,5,5,0
 Misc Info : 10-18236
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000 Compound Sublist: voa.sub
 Integrator: HP RTE
 Target Version: 3.50
 Processing Host: cserv3

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|-------|---------|--------|----------|-------------------|---------------|
| | | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.005 | 2.995 | (0.454) | 62464 | 46.4188 | 46.419 | |
| 2 Chloromethane | 50 | 3.306 | 3.296 | (0.499) | 148346 | 40.9735 | 40.973 | |
| 3 Vinyl Chloride | 62 | 3.417 | 3.407 | (0.516) | 131932 | 46.0808 | 46.081 | |
| 4 Bromomethane | 94 | 3.909 | 3.899 | (0.590) | 100202 | 64.4447 | 64.445 | |
| 5 Chloroethane | 64 | 3.980 | 3.970 | (0.601) | 90835 | 48.5821 | 48.582 | |
| 6 Trichlorofluoromethane | 101 | 4.241 | 4.231 | (0.640) | 136791 | 49.4347 | 49.435 | |
| 7 Acrolein | 56 | 4.623 | 4.613 | (0.698) | 83734 | 242.587 | 242.59 | |
| 8 112Trichloro122Trifluoroethane | 101 | 4.643 | 4.633 | (0.701) | 101727 | 46.9580 | 46.958 | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 144843 | 249.402 | 249.40 | |
| 10 1,1-Dichloroethene | 96 | 4.834 | 4.824 | (0.730) | 93428 | 47.5261 | 47.526 | |
| 11 Bromoethane | 108 | 5.055 | 5.045 | (0.763) | 70833 | 48.6564 | 48.656 | |
| 12 Iodomethane | 142 | 5.156 | 5.146 | (0.778) | 131309 | 56.4944 | 56.494 | |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.797) | 91484 | 41.3299 | 41.330 | |
| 14 Acrylonitrile | 53 | 5.357 | 5.347 | (0.809) | 27791 | 54.1988 | 54.199 (Q) | |

| Compounds | QUANT SIG | | CONCENTRATIONS | | | | |
|------------------------------|-----------|--------|----------------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.397 | 5.387 | (0.815) | 151278 | 50.0415 | 50.041 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.367 | (0.812) | 314532 | 51.5885 | 51.588 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.548 | (0.839) | 78507 | 46.8613 | 46.861 |
| 18 Vinyl Acetate | 43 | 5.879 | 5.869 | (0.888) | 165319 | 56.3423 | 56.342 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.929 | (0.897) | 152925 | 49.6190 | 49.619 |
| 20 2-Butanone | 43 | 6.281 | 6.271 | (0.948) | 176551 | 270.171 | 270.17 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.452 | (0.976) | 91720 | 48.6350 | 48.635 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.492 | 6.492 | (0.980) | 70985 | 48.0744 | 48.074 |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 103776 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.633 | (1.003) | 120699 | 48.2135 | 48.214 |
| 26 Bromochloromethane | 128 | 6.804 | 6.794 | (1.027) | 33873 | 48.3180 | 48.318 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 56662 | 45.8112 | 45.811 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.025 | (1.062) | 90481 | 46.4694 | 46.469 |
| 29 1,1-Dichloropropene | 75 | 7.176 | 7.166 | (0.939) | 99621 | 49.7789 | 49.779 |
| 30 Carbon Tetrachloride | 117 | 7.286 | 7.286 | (0.954) | 80765 | 46.4092 | 46.409 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 62283 | 46.0197 | 46.020 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.387 | (0.968) | 88868 | 50.5832 | 50.583 |
| 33 Benzene | 78 | 7.437 | 7.437 | (0.974) | 242443 | 50.0989 | 50.099 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 147372 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.000 | (1.049) | 67187 | 47.3867 | 47.387 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.161 | (1.070) | 73081 | 47.9069 | 47.907 |
| 37 Bromodichloromethane | 83 | 8.402 | 8.392 | (1.100) | 80306 | 49.2379 | 49.238 |
| 39 Dibromomethane | 93 | 8.472 | 8.462 | (1.109) | 38019 | 50.2065 | 50.206 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.613 | (1.129) | 29809 | 55.7979 | 55.798 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.653 | 8.643 | (1.133) | 100424 | 257.776 | 257.78 |
| 42 Cis 1,3-dichloropropene | 75 | 8.904 | 8.904 | (1.166) | 94251 | 52.9293 | 52.929 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 167179 | 51.6276 | 51.628 |
| 44 Toluene | 92 | 9.266 | 9.256 | (1.213) | 135157 | 47.0730 | 47.073 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.397 | 9.387 | (1.230) | 77632 | 51.8664 | 51.866 |
| 46 2-Hexanone | 43 | 9.527 | 9.527 | (0.884) | 244623 | 248.293 | 248.29 |
| 47 1,1,2-Trichloroethane | 97 | 9.578 | 9.568 | (1.254) | 44304 | 49.5646 | 49.565 |
| 48 1,3-Dichloropropane | 76 | 9.839 | 9.829 | (0.912) | 86755 | 51.1432 | 51.143 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.949 | (0.924) | 61827 | 46.1730 | 46.173 |
| 50 Chlorodibromomethane | 129 | 10.171 | 10.161 | (0.943) | 55717 | 48.8256 | 48.826 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.382 | (1.361) | 47958 | 50.0897 | 50.090 |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 120524 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.834 | 10.824 | (1.005) | 135941 | 48.0887 | 48.089 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.854 | (1.007) | 250730 | 52.4490 | 52.449 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.844 | (1.007) | 47023 | 43.4625 | 43.462 |
| 56 m,p-xylene | 106 | 10.944 | 10.934 | (1.015) | 191673 | 109.699 | 109.70 |
| 57 o-Xylene | 106 | 11.427 | 11.427 | (1.060) | 93101 | 51.2688 | 51.269 |
| 58 Styrene | 104 | 11.457 | 11.457 | (1.062) | 153251 | 54.5808 | 54.581 |
| 59 Isopropyl Benzene | 105 | 11.809 | 11.799 | (0.877) | 246157 | 56.1684 | 56.168 |
| 60 Bromoform | 173 | 11.869 | 11.859 | (0.881) | 34888 | 49.5127 | 49.513 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.980 | (0.890) | 60807 | 48.0266 | 48.027 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.123) | 70992 | 50.3298 | 50.330 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.150 | (0.903) | 12739 | 50.7877 | 50.788 |

| Compounds | QUANT SIG | | CONCENTRATIONS | | | | |
|--------------------------------|-----------|--------|----------------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.201 | (0.907) | 22186 | 57.0130 | 57.013 |
| 66 N-Propyl Benzene | 91 | 12.261 | 12.261 | (0.910) | 305467 | 53.9940 | 53.994 |
| 67 Bromobenzene | 156 | 12.351 | 12.351 | (0.917) | 59592 | 48.7773 | 48.777 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.432 | 12.432 | (0.923) | 204643 | 57.5250 | 57.525 |
| 69 2-Chloro Toluene | 91 | 12.492 | 12.492 | (0.928) | 204881 | 55.1150 | 55.115 |
| 70 4-Chloro Toluene | 91 | 12.542 | 12.532 | (0.931) | 190992 | 53.6005 | 53.600 |
| 71 T-Butyl Benzene | 119 | 12.844 | 12.844 | (0.954) | 176507 | 57.9960 | 57.996 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.894 | 12.884 | (0.957) | 201994 | 57.6781 | 57.678 |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.085 | (0.972) | 275174 | 54.9582 | 54.958 |
| 74 4-Isopropyl Toluene | 119 | 13.236 | 13.236 | (0.983) | 206312 | 60.0515 | 60.052 |
| 75 1,3-Dichlorobenzene | 146 | 13.387 | 13.377 | (0.994) | 111781 | 53.5542 | 53.554 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.457 | (1.000) | 65104 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.497 | (1.003) | 110382 | 52.8467 | 52.849 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.708 | (1.019) | 221398 | 59.6772 | 59.677 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 58117 | 49.0771 | 49.077 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.939 | (1.036) | 101428 | 51.1305 | 51.130 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.854 | 14.844 | (1.103) | 11125 | 50.7797 | 50.780 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.889 | (1.181) | 62105 | 51.4473 | 51.447 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.040 | (1.192) | 40802 | 50.1848 | 50.185 |
| 84 Naphthalene | 128 | 16.221 | 16.211 | (1.204) | 108716 | 49.6526 | 49.652 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.502 | (1.226) | 53776 | 46.5953 | 46.595 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: LCS0809.d
 Lab Smp Id: LCS0809
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18236

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: LCS0809
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 103776 | -20.85 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 147372 | -23.07 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 120524 | -25.23 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 65104 | -26.25 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Client SDG: 09AUG10
 Sample Matrix: SOLID Fraction: VOA
 Lab Smp Id: LCS0809 Client Smp ID: LCS0809
 Level: LOW Operator: PB
 Data Type: MS DATA SampleType: LCS
 SpikeList File: all.spk Quant Type: ISTD
 Sublist File: voa.sub
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18236

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 1 Dichlorodifluorome | 50.000 | 46.419 | 92.84 | 53-148 |
| 2 Chloromethane | 50.000 | 40.973 | 81.95 | 64-125 |
| 3 Vinyl Chloride | 50.000 | 46.081 | 92.16 | 63-137 |
| 4 Bromomethane | 50.000 | 64.445 | 128.89 | 57-136 |
| 5 Chloroethane | 50.000 | 48.582 | 97.16 | 64-131 |
| 6 Trichlorofluoromet | 50.000 | 49.435 | 98.87 | 69-132 |
| 7 Acrolein | 250.00 | 242.59 | 97.03 | 54-137 |
| 8 112Trichloro122Tri | 50.000 | 46.958 | 93.92 | 74-130 |
| 9 Acetone | 250.00 | 249.40 | 99.76 | 60-131 |
| 10 1,1-Dichloroethene | 50.000 | 47.526 | 95.05 | 75-126 |
| 11 Bromoethane | 50.000 | 48.656 | 97.31 | 76-126 |
| 12 Iodomethane | 50.000 | 56.494 | 112.99 | 65-139 |
| 13 Methylene Chloride | 50.000 | 41.330 | 82.66 | 70-123 |
| 15 Carbon Disulfide | 50.000 | 51.588 | 103.18 | 71-129 |
| 14 Acrylonitrile | 50.000 | 54.199 | 108.40 | 67-125 |
| 16 Methyl tert-Butyl | 50.000 | 50.041 | 100.08 | 70-120 |
| 17 Trans-1,2-Dichloro | 50.000 | 46.861 | 93.72 | 80-120 |
| 18 Vinyl Acetate | 50.000 | 56.342 | 112.68 | 60-136 |
| 19 1,1-Dichloroethane | 50.000 | 49.619 | 99.24 | 80-120 |
| 20 2-Butanone | 250.00 | 270.17 | 108.07 | 70-120 |
| 21 2,2-Dichloropropan | 50.000 | 48.635 | 97.27 | 74-123 |
| 22 Cis-1,2-Dichloroet | 50.000 | 48.074 | 96.15 | 80-120 |
| 24 Chloroform | 50.000 | 48.214 | 96.43 | 80-120 |
| 26 Bromochloromethane | 50.000 | 48.318 | 96.64 | 80-120 |
| 27 1,1,1-Trichloroeth | 50.000 | 46.469 | 92.94 | 77-121 |
| 29 1,1-Dichloropropen | 50.000 | 49.779 | 99.56 | 80-120 |
| 30 Carbon Tetrachlori | 50.000 | 46.409 | 92.82 | 77-122 |
| 32 1,2-Dichloroethane | 50.000 | 50.583 | 101.17 | 76-120 |
| 33 Benzene | 50.000 | 50.099 | 100.20 | 80-120 |
| 35 Trichloroethene | 50.000 | 47.387 | 94.77 | 80-120 |
| 36 1,2-Dichloropropan | 50.000 | 47.907 | 95.81 | 80-120 |
| 37 Bromodichlorometha | 50.000 | 49.238 | 98.48 | 77-121 |
| 39 Dibromomethane | 50.000 | 50.206 | 100.41 | 80-120 |

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 40 2-Chloroethyl Viny | 50.000 | 55.798 | 111.60 | 10-191 |
| 41 4-Methyl-2-Pentano | 250.00 | 257.78 | 103.11 | 67-120 |
| 42 Cis 1,3-dichloropr | 50.000 | 52.929 | 105.86 | 74-120 |
| 44 Toluene | 50.000 | 47.073 | 94.15 | 80-120 |
| 45 Trans 1,3-Dichloro | 50.000 | 51.866 | 103.73 | 65-120 |
| 46 2-Hexanone | 250.00 | 248.29 | 99.32 | 65-130 |
| 47 1,1,2-Trichloroeth | 50.000 | 49.565 | 99.13 | 80-120 |
| 48 1,3-Dichloropropan | 50.000 | 51.143 | 102.29 | 80-120 |
| 49 Tetrachloroethene | 50.000 | 46.173 | 92.35 | 80-121 |
| 50 Chlorodibromometha | 50.000 | 48.826 | 97.65 | 64-120 |
| 51 1,2-Dibromoethane | 50.000 | 50.090 | 100.18 | 75-120 |
| 53 Chlorobenzene | 50.000 | 48.089 | 96.18 | 80-120 |
| 55 1,1,1,2-Tetrachlor | 50.000 | 43.462 | 86.93 | 69-121 |
| 54 Ethyl Benzene | 50.000 | 52.449 | 104.90 | 80-127 |
| 56 m,p-xylene | 100.00 | 109.70 | 109.70 | 80-125 |
| 57 o-Xylene | 50.000 | 51.269 | 102.54 | 78-120 |
| 58 Styrene | 50.000 | 54.581 | 109.16 | 80-123 |
| 59 Isopropyl Benzene | 50.000 | 56.168 | 112.34 | 80-127 |
| 60 Bromoform | 50.000 | 49.513 | 99.03 | 60-120 |
| 61 1,1,2,2-Tetrachlor | 50.000 | 48.027 | 96.05 | 74-120 |
| 63 1,2,3-Trichloropro | 50.000 | 50.788 | 101.58 | 72-121 |
| 65 Trans-1,4-Dichloro | 50.000 | 57.013 | 114.03 | 65-126 |
| 66 N-Propyl Benzene | 50.000 | 53.994 | 107.99 | 80-132 |
| 67 Bromobenzene | 50.000 | 48.777 | 97.55 | 80-120 |
| 68 1,3,5-Trimethyl Be | 50.000 | 57.525 | 115.05 | 80-125 |
| 69 2-Chloro Toluene | 50.000 | 55.115 | 110.23 | 80-125 |
| 70 4-Chloro Toluene | 50.000 | 53.600 | 107.20 | 80-127 |
| 71 T-Butyl Benzene | 50.000 | 57.996 | 115.99 | 87-122 |
| 72 1,2,4-Trimethylben | 50.000 | 57.678 | 115.36 | 80-126 |
| 73 S-Butyl Benzene | 50.000 | 54.958 | 109.92 | 80-134 |
| 74 4-Isopropyl Toluen | 50.000 | 60.052 | 120.10 | 80-131 |
| 75 1,3-Dichlorobenzen | 50.000 | 53.554 | 107.11 | 80-120 |
| 77 1,4-Dichlorobenzen | 50.000 | 52.849 | 105.70 | 80-120 |
| 78 N-Butyl Benzene | 50.000 | 59.677 | 119.35 | 80-138 |
| 80 1,2-Dichlorobenzen | 50.000 | 51.130 | 102.26 | 80-120 |
| 81 1,2-Dibromo 3-Chlo | 50.000 | 50.780 | 101.56 | 59-120 |
| 82 1,2,4-Trichloroben | 50.000 | 51.447 | 102.89 | 78-130 |
| 83 Hexachloro 1,3-But | 50.000 | 50.185 | 100.37 | 76-129 |
| 84 Naphthalene | 50.000 | 49.652 | 99.31 | 66-120 |
| 85 1,2,3-Trichloroben | 50.000 | 46.595 | 93.19 | 73-123 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 45.811 | 91.62 | 30-160 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 46.020 | 92.04 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 51.628 | 103.26 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 50.330 | 100.66 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 49.077 | 98.15 | 80-120 |

Data File: /chem1/finn5.i/09AUG10.b/LCS0809.d

Date : 09-AUG-2010 11:22

Client ID: LCS0809

Sample Info: LCS0809,5,5,0


Column phase: Rtx502.2

Instrument: finn5.i

Operator: PB

Column diameter: 0.18

Page 8

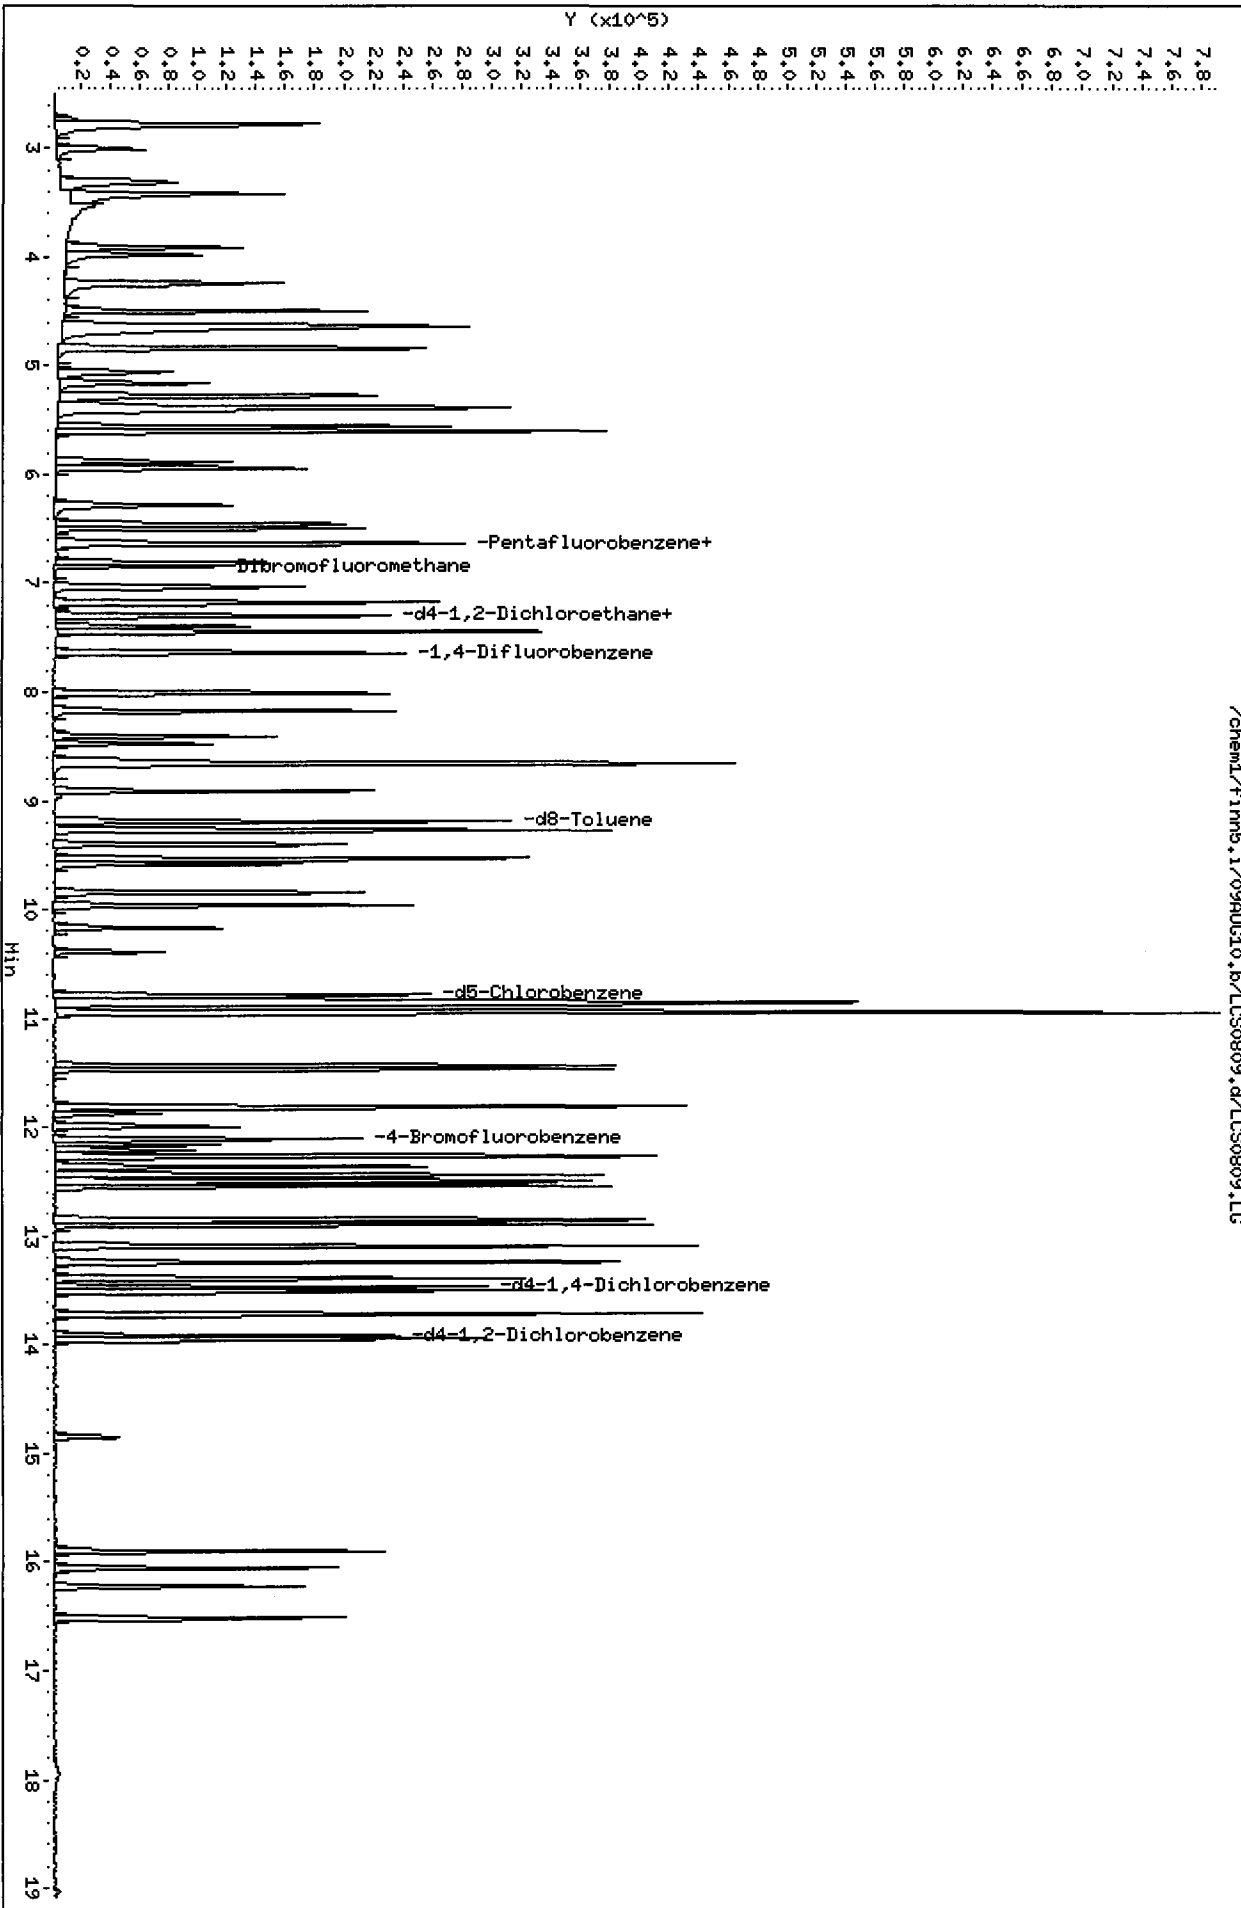


/chem1/finn5.i/09AUG10.b/LCS0809.d/LCS0809.LG

Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/LCS0809A.d
Lab Smp Id: LCS0809 Client Smp ID: LCS0809
Inj Date : 09-AUG-2010 11:49
Operator : PB Inst ID: finn5.i
Smp Info : LCS0809,5,5,0
Misc Info : 10-18236
Comment :
Method : /chem1/finn5.i/09AUG10.b/s8260b.m
Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
Als bottle: 1 QC Sample: LCSD
Dil Factor: 1.00000
Integrator: HP RTE Compound Sublist: voa.sub
Target Version: 3.50
Processing Host: cserv3



Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | | | | CONCENTRATIONS | | |
|----------------------------------|-----------|-------|--------|---------|----------------|-------------------|---------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.015 | 2.995 | (0.455) | 61495 | 44.5023 | 44.502 |
| 2 Chloromethane | 50 | 3.316 | 3.296 | (0.500) | 154826 | 41.6437 | 41.644 |
| 3 Vinyl Chloride | 62 | 3.427 | 3.407 | (0.517) | 133749 | 45.4924 | 45.492 |
| 4 Bromomethane | 94 | 3.919 | 3.899 | (0.591) | 101037 | 63.2805 | 63.280 |
| 5 Chloroethane | 64 | 3.980 | 3.970 | (0.600) | 92025 | 47.9300 | 47.930 |
| 6 Trichlorofluoromethane | 101 | 4.251 | 4.231 | (0.641) | 142143 | 50.0240 | 50.024 |
| 7 Acrolein | 56 | 4.633 | 4.613 | (0.698) | 85320 | 240.710 | 240.71 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.643 | 4.633 | (0.700) | 105782 | 47.5514 | 47.551 |
| 9 Acetone | 43 | 4.683 | 4.673 | (0.706) | 151519 | 254.066 | 254.07 |
| 10 1,1-Dichloroethene | 96 | 4.844 | 4.824 | (0.730) | 97179 | 48.1400 | 48.140 |
| 11 Bromoethane | 108 | 5.065 | 5.045 | (0.764) | 72555 | 48.5344 | 48.534 |
| 12 Iodomethane | 142 | 5.166 | 5.146 | (0.779) | 135401 | 56.7298 | 56.730 |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.795) | 96761 | 42.5695 | 42.569 |
| 14 Acrylonitrile | 53 | 5.357 | 5.347 | (0.808) | 28424 | 53.9820 | 53.982 (Q) |

| Compounds | QUANT SIG | | | | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | 5.407 | 5.387 | (0.815) | 160018 | 51.5468 | 51.547 (Q) |
| 15 Carbon Disulfide | 76 | 5.387 | 5.367 | (0.812) | 321911 | 51.4165 | 51.416 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.548 | (0.838) | 82681 | 48.0607 | 48.061 |
| 18 Vinyl Acetate | 43 | 5.879 | 5.869 | (0.886) | 170751 | 56.6700 | 56.670 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.929 | (0.895) | 158254 | 50.0037 | 50.004 |
| 20 2-Butanone | 43 | 6.281 | 6.271 | (0.947) | 182010 | 271.233 | 271.23 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.452 | (0.974) | 93506 | 48.2840 | 48.284 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.502 | 6.492 | (0.980) | 74686 | 49.2566 | 49.257 |
| * 23 Pentafluorobenzene | 168 | 6.633 | 6.613 | (1.000) | 106566 | 50.0000 | |
| 24 Chloroform | 83 | 6.653 | 6.633 | (1.003) | 125559 | 48.8418 | 48.842 |
| 26 Bromochloromethane | 128 | 6.814 | 6.794 | (1.027) | 36267 | 50.3784 | 50.378 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.032) | 65720 | 51.7435 | 51.743 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.025 | (1.061) | 93069 | 46.5471 | 46.547 |
| 29 1,1-Dichloropropene | 75 | 7.186 | 7.166 | (0.941) | 102201 | 47.6740 | 47.674 |
| 30 Carbon Tetrachloride | 117 | 7.296 | 7.286 | (0.955) | 84024 | 45.0730 | 45.073 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.101) | 76544 | 55.0762 | 55.076 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.387 | (0.968) | 94488 | 50.2076 | 50.208 |
| 33 Benzene | 78 | 7.447 | 7.437 | (0.975) | 252208 | 48.6529 | 48.653 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 157864 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.000 | (1.049) | 71094 | 46.8097 | 46.810 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.161 | (1.070) | 77768 | 47.5912 | 47.591 |
| 37 Bromodichloromethane | 83 | 8.412 | 8.392 | (1.101) | 86432 | 49.4718 | 49.472 |
| 39 Dibromomethane | 93 | 8.482 | 8.462 | (1.111) | 39857 | 49.1356 | 49.136 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.613 | (1.129) | 30760 | 53.7512 | 53.751 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.663 | 8.643 | (1.134) | 103793 | 248.717 | 248.72 |
| 42 Cis 1,3-dichloropropene | 75 | 8.914 | 8.904 | (1.167) | 100653 | 52.7678 | 52.768 |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 181921 | 52.4463 | 52.446 |
| 44 Toluene | 92 | 9.276 | 9.256 | (1.214) | 143365 | 46.6131 | 46.613 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.407 | 9.387 | (1.232) | 82835 | 51.6644 | 51.664 |
| 46 2-Hexanone | 43 | 9.537 | 9.527 | (0.884) | 255994 | 231.153 | 231.15 |
| 47 1,1,2-Trichloroethane | 97 | 9.588 | 9.568 | (1.255) | 47916 | 50.0428 | 50.043 |
| 48 1,3-Dichloropropane | 76 | 9.849 | 9.829 | (0.912) | 92389 | 48.4524 | 48.452 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.949 | (0.923) | 65149 | 43.2832 | 43.283 |
| 50 Chlorodibromomethane | 129 | 10.171 | 10.161 | (0.942) | 59744 | 46.5753 | 46.575 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.382 | (1.361) | 51001 | 49.7277 | 49.728 |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.774 | (1.000) | 135479 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.834 | 10.824 | (1.004) | 147015 | 46.2653 | 46.265 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.854 | (1.007) | 267806 | 49.8371 | 49.837 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.854 | 10.844 | (1.006) | 51300 | 42.1817 | 42.182 |
| 56 m,p-xylene | 106 | 10.944 | 10.934 | (1.014) | 203748 | 103.738 | 103.74 |
| 57 o-Xylene | 106 | 11.437 | 11.427 | (1.060) | 100490 | 49.2293 | 49.229 |
| 58 Styrene | 104 | 11.467 | 11.457 | (1.062) | 165452 | 52.4216 | 52.422 |
| 59 Isopropyl Benzene | 105 | 11.819 | 11.799 | (0.878) | 264063 | 51.8558 | 51.856 |
| 60 Bromoform | 173 | 11.879 | 11.859 | (0.882) | 36350 | 44.3971 | 44.397 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.980 | (0.890) | 65836 | 44.7510 | 44.751 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.122) | 80262 | 50.6206 | 50.620 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.150 | (0.903) | 13474 | 46.2306 | 46.231 |

| Compounds | QUANT SIG | | | | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.211 | 12.201 | (0.907) | 23605 | 52.2046 | 52.205 |
| 66 N-Propyl Benzene | 91 | 12.271 | 12.261 | (0.911) | 332331 | 50.5548 | 50.555 |
| 67 Bromobenzene | 156 | 12.361 | 12.351 | (0.918) | 66393 | 46.7695 | 46.769 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.442 | 12.432 | (0.924) | 225487 | 54.5496 | 54.550 |
| 69 2-Chloro Toluene | 91 | 12.502 | 12.492 | (0.928) | 211853 | 49.0471 | 49.047 |
| 70 4-Chloro Toluene | 91 | 12.542 | 12.532 | (0.931) | 220420 | 53.2372 | 53.237 |
| 71 T-Butyl Benzene | 119 | 12.854 | 12.844 | (0.954) | 194173 | 54.9079 | 54.908 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.904 | 12.884 | (0.958) | 223779 | 54.9923 | 54.992 |
| 73 S-Butyl Benzene | 105 | 13.095 | 13.085 | (0.972) | 300641 | 51.6754 | 51.675 |
| 74 4-Isopropyl Toluene | 119 | 13.246 | 13.236 | (0.984) | 228012 | 57.1173 | 57.117 |
| 75 1,3-Dichlorobenzene | 146 | 13.397 | 13.377 | (0.995) | 126798 | 52.2815 | 52.282 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.457 | (1.000) | 75648 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.507 | 13.497 | (1.003) | 123863 | 51.0373 | 51.037 |
| 78 N-Butyl Benzene | 91 | 13.718 | 13.708 | (1.019) | 249411 | 57.8577 | 57.858 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.909 | (1.034) | 68585 | 49.8443 | 49.844 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.939 | (1.036) | 115595 | 50.1501 | 50.150 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.854 | 14.844 | (1.103) | 12033 | 47.2687 | 47.269 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.889 | (1.181) | 74308 | 52.9763 | 52.976 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.050 | 16.040 | (1.192) | 46130 | 48.8298 | 48.830 |
| 84 Naphthalene | 128 | 16.221 | 16.211 | (1.204) | 129155 | 50.7656 | 50.766 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.512 | 16.502 | (1.226) | 67233 | 50.1356 | 50.136 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

| | |
|--|-------------------------------|
| Instrument ID: finn5.i | Calibration Date: 09-AUG-2010 |
| Lab File ID: LCS0809A.d | Calibration Time: 10:35 |
| Lab Smp Id: LCS0809 | Client Smp ID: LCS0809 |
| Analysis Type: VOA | Level: LOW |
| Quant Type: ISTD | Sample Type: SOIL |
| Operator: PB | |
| Method File: /chem1/finn5.i/09AUG10.b/s8260b.m | |
| Misc Info: 10-18236 | |

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 106566 | -18.72 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 157864 | -17.59 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 135479 | -15.96 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 75648 | -14.31 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Client SDG: 09AUG10
 Sample Matrix: SOLID Fraction: VOA
 Lab Smp Id: LCS0809 Client Smp ID: LCS0809
 Level: LOW Operator: PB
 Data Type: MS DATA SampleType: LCSD
 SpikeList File: all.spk Quant Type: ISTD
 Sublist File: voa.sub
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18236

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 1 Dichlorodifluorome | 50.000 | 44.502 | 89.00 | 53-148 |
| 2 Chloromethane | 50.000 | 41.644 | 83.29 | 64-125 |
| 3 Vinyl Chloride | 50.000 | 45.492 | 90.98 | 63-137 |
| 4 Bromomethane | 50.000 | 63.280 | 126.56 | 57-136 |
| 5 Chloroethane | 50.000 | 47.930 | 95.86 | 64-131 |
| 6 Trichlorofluoromet | 50.000 | 50.024 | 100.05 | 69-132 |
| 7 Acrolein | 250.00 | 240.71 | 96.28 | 54-137 |
| 8 112Trichloro122Tri | 50.000 | 47.551 | 95.10 | 74-130 |
| 9 Acetone | 250.00 | 254.07 | 101.63 | 60-131 |
| 10 1,1-Dichloroethene | 50.000 | 48.140 | 96.28 | 75-126 |
| 11 Bromoethane | 50.000 | 48.534 | 97.07 | 76-126 |
| 12 Iodomethane | 50.000 | 56.730 | 113.46 | 65-139 |
| 13 Methylene Chloride | 50.000 | 42.569 | 85.14 | 70-123 |
| 15 Carbon Disulfide | 50.000 | 51.416 | 102.83 | 71-129 |
| 14 Acrylonitrile | 50.000 | 53.982 | 107.96 | 67-125 |
| 16 Methyl tert-Butyl | 50.000 | 51.547 | 103.09 | 70-120 |
| 17 Trans-1,2-Dichloro | 50.000 | 48.061 | 96.12 | 80-120 |
| 18 Vinyl Acetate | 50.000 | 56.670 | 113.34 | 60-136 |
| 19 1,1-Dichloroethane | 50.000 | 50.004 | 100.01 | 80-120 |
| 20 2-Butanone | 250.00 | 271.23 | 108.49 | 70-120 |
| 21 2,2-Dichloropropan | 50.000 | 48.284 | 96.57 | 74-123 |
| 22 Cis-1,2-Dichloroet | 50.000 | 49.257 | 98.51 | 80-120 |
| 24 Chloroform | 50.000 | 48.842 | 97.68 | 80-120 |
| 26 Bromochloromethane | 50.000 | 50.378 | 100.76 | 80-120 |
| 27 1,1,1-Trichloroeth | 50.000 | 46.547 | 93.09 | 77-121 |
| 29 1,1-Dichloropropen | 50.000 | 47.674 | 95.35 | 80-120 |
| 30 Carbon Tetrachlori | 50.000 | 45.073 | 90.15 | 77-122 |
| 32 1,2-Dichloroethane | 50.000 | 50.208 | 100.42 | 76-120 |
| 33 Benzene | 50.000 | 48.653 | 97.31 | 80-120 |
| 35 Trichloroethene | 50.000 | 46.810 | 93.62 | 80-120 |
| 36 1,2-Dichloropropan | 50.000 | 47.591 | 95.18 | 80-120 |
| 37 Bromodichlorometha | 50.000 | 49.472 | 98.94 | 77-121 |
| 39 Dibromomethane | 50.000 | 49.136 | 98.27 | 80-120 |

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 40 2-Chloroethyl Viny | 50.000 | 53.751 | 107.50 | 10-191 |
| 41 4-Methyl-2-Pentano | 250.00 | 248.72 | 99.49 | 67-120 |
| 42 Cis 1,3-dichloropr | 50.000 | 52.768 | 105.54 | 74-120 |
| 44 Toluene | 50.000 | 46.613 | 93.23 | 80-120 |
| 45 Trans 1,3-Dichloro | 50.000 | 51.664 | 103.33 | 65-120 |
| 46 2-Hexanone | 250.00 | 231.15 | 92.46 | 65-130 |
| 47 1,1,2-Trichloroeth | 50.000 | 50.043 | 100.09 | 80-120 |
| 48 1,3-Dichloropropan | 50.000 | 48.452 | 96.90 | 80-120 |
| 49 Tetrachloroethene | 50.000 | 43.283 | 86.57 | 80-121 |
| 50 Chlorodibromometha | 50.000 | 46.575 | 93.15 | 64-120 |
| 51 1,2-Dibromoethane | 50.000 | 49.728 | 99.46 | 75-120 |
| 53 Chlorobenzene | 50.000 | 46.265 | 92.53 | 80-120 |
| 55 1,1,1,2-Tetrachlor | 50.000 | 42.182 | 84.36 | 69-121 |
| 54 Ethyl Benzene | 50.000 | 49.837 | 99.67 | 80-127 |
| 56 m,p-xylene | 100.00 | 103.74 | 103.74 | 80-125 |
| 57 o-Xylene | 50.000 | 49.229 | 98.46 | 78-120 |
| 58 Styrene | 50.000 | 52.422 | 104.84 | 80-123 |
| 59 Isopropyl Benzene | 50.000 | 51.856 | 103.71 | 80-127 |
| 60 Bromoform | 50.000 | 44.397 | 88.79 | 60-120 |
| 61 1,1,2,2-Tetrachlor | 50.000 | 44.751 | 89.50 | 74-120 |
| 63 1,2,3-Trichloropro | 50.000 | 46.231 | 92.46 | 72-121 |
| 65 Trans-1,4-Dichloro | 50.000 | 52.205 | 104.41 | 65-126 |
| 66 N-Propyl Benzene | 50.000 | 50.555 | 101.11 | 80-132 |
| 67 Bromobenzene | 50.000 | 46.769 | 93.54 | 80-120 |
| 68 1,3,5-Trimethyl Be | 50.000 | 54.550 | 109.10 | 80-125 |
| 69 2-Chloro Toluene | 50.000 | 49.047 | 98.09 | 80-125 |
| 70 4-Chloro Toluene | 50.000 | 53.237 | 106.47 | 80-127 |
| 71 T-Butyl Benzene | 50.000 | 54.908 | 109.82 | 87-122 |
| 72 1,2,4-Trimethylben | 50.000 | 54.992 | 109.98 | 80-126 |
| 73 S-Butyl Benzene | 50.000 | 51.675 | 103.35 | 80-134 |
| 74 4-Isopropyl Toluen | 50.000 | 57.117 | 114.23 | 80-131 |
| 75 1,3-Dichlorobenzen | 50.000 | 52.282 | 104.56 | 80-120 |
| 77 1,4-Dichlorobenzen | 50.000 | 51.037 | 102.07 | 80-120 |
| 78 N-Butyl Benzene | 50.000 | 57.858 | 115.72 | 80-138 |
| 80 1,2-Dichlorobenzen | 50.000 | 50.150 | 100.30 | 80-120 |
| 81 1,2-Dibromo 3-Chlo | 50.000 | 47.269 | 94.54 | 59-120 |
| 82 1,2,4-Trichloroben | 50.000 | 52.976 | 105.95 | 78-130 |
| 83 Hexachloro 1,3-But | 50.000 | 48.830 | 97.66 | 76-129 |
| 84 Naphthalene | 50.000 | 50.766 | 101.53 | 66-120 |
| 85 1,2,3-Trichloroben | 50.000 | 50.136 | 100.27 | 73-123 |


| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 51.743 | 103.49 | 30-160 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 55.076 | 110.15 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.446 | 104.89 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 50.620 | 101.24 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 49.844 | 99.69 | 80-120 |

Data File: /chem1/finn5.i/09AUG10.b/LCS0809A.d
Date : 09-AUG-2010 11:49
Client ID: LCS0809
Sample Info: LCS0809,5,5,0
Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18


/chem1/finn5.i/09AUG10.b/LCS0809A.d/LCS0809A.LG



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/MB0809.d
Lab Smp Id: MB0809 Client Smp ID: MB0809
Inj Date : 09-AUG-2010 12:16
Operator : PB Inst ID: finn5.i
Smp Info : MB0809,5,5,0
Misc Info : 10-18236
Comment :
Method : /chem1/finn5.i/09AUG10.b/s8260b.m
Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
Als bottle: 1 QC Sample: BLANK
Dil Factor: 1.00000
Integrator: HP RTE Compound Sublist: voa.sub
Target Version: 3.50
Processing Host: cserv3



Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.707) | 2278 | 4.28109 | |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | | | | | | |
| 14 Acrylonitrile | 53 | | | | | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-------------------|--------|--------|---------|------------------------|----------------------|----------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.948) | 1605 | 2.68067 | 2.691 |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.613 | 6.613 | (1.000) | 95082 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.033) | 59307 | 52.3340 | 52.334 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.103) | 72988 | 58.8605 | 58.860 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 136899 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | 8.643 | 8.643 | (1.133) | 1075 | 2.97049 | 2.970 (Q) |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 157014 | 52.1980 | 52.198 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.774 | 10.774 | (1.000) | 118413 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.123) | 66975 | 48.3284 | 48.328 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 58588 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.899 | 13.909 | (1.033) | 53785 | 50.4703 | 50.470 |
| 80 1,2-Dichlorobenzene | 146 | 13.939 | 13.939 | (1.036) | 915 | 0.51256 | 0.5126 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: MB0809.d
 Lab Smp Id: MB0809
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18236

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: MB0809
 Level: LOW
 Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 95082 | -27.48 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 136899 | -28.53 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 118413 | -26.54 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 58588 | -33.63 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.61 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.77 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.46 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Client SDG: 09AUG10
Sample Matrix: SOLID Fraction: VOA
Lab Smp Id: MB0809 Client Smp ID: MB0809
Level: LOW Operator: PB
Data Type: MS DATA SampleType: BLANK
SpikeList File: all.spk Quant Type: ISTD
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18236

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 52.334 | 104.67 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 58.860 | 117.72 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.198 | 104.40 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 48.328 | 96.66 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.470 | 100.94 | 80-120 |

Data File: /chem1/finn5.i/09AUG10.b/HB0809.d

Date : 09-AUG-2010 12:16

Client ID: HB0809


Sample Info: HB0809,5,5,0

Column phase: Rtx502.2

Instrument: finn5.i

Operator: PB

Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58A.d
 Lab Smp Id: RG58A Client Smp ID: PSB22-0-0.5-072910
 Inj Date : 09-AUG-2010 16:11
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58A,5,9.32,0
 Misc Info : 10-18236
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 9.32000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|----------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 110555 | 120.512 | 64.652(Q) <i>nlq</i> |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.795) | 9256 | 2.64723 | 1.420 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten initials

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.947) | 6880 | 6.66510 | 3.576 <i>nl</i> |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 163926 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.032) | 102677 | 52.5535 | 28.194 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.102) | 119875 | 56.0728 | 30.082 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 239062 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.203) | 257701 | 49.0593 | 26.319 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 194173 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 105877 | 46.5910 | 24.995 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 95238 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.034) | 87028 | 50.2380 | 26.952 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58A.d
 Lab Smp Id: RG58A
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18236

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB22-0-0.5-072910
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 163926 | 25.02 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 239062 | 24.80 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 194173 | 20.46 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 95238 | 7.88 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.46 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58A
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18236


Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-0-0.5-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 52.554 | 105.11 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 56.073 | 112.15 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 49.059 | 98.12 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 46.591 | 93.18 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.238 | 100.48 | 80-120 |

Data File: /chem1/finn5.1/09AUG10.b/R058A.d
Date: 09-AUG-2010 16:11
Client ID: PS822-0-0.5-072910
Sample Info: R058A,5,9,32,0

Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58B.d
 Lab Smp Id: RG58B Client Smp ID: PSB22-1.5-2-072910
 Inj Date : 09-AUG-2010 16:38
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58B,5,8.14,0
 Misc Info : 10-18237
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 8.14000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.683 | 4.673 | (0.706) | 118970 | 150.341 | 92.347 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.286 | 5.266 | (0.797) | 8859 | 2.93726 | 1.804 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten mark

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|----------------------|--------|--------|---------|----------|----------------------|-------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |
| 15 Carbon Disulfide | 76 | | | | | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | | |
| 18 Vinyl Acetate | 43 | | | | | | |
| 19 1,1-Dichloroethane | 63 | | | | | | |
| 20 2-Butanone | 43 | 6.291 | 6.271 | (0.948) | 5644 | 6.33861 | 3.893 <i>alg</i> |
| 21 2,2-Dichloropropane | 77 | | | | | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | | |
| * 23 Pentafluorobenzene | 168 | 6.633 | 6.613 | (1.000) | 141403 | 50.0000 | |
| 24 Chloroform | 83 | | | | | | |
| 26 Bromochloromethane | 128 | | | | | | |
| \$ 25 Dibromofluoromethane | 111 | 6.854 | 6.834 | (1.033) | 91257 | 54.1482 | 33.260 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | | |
| 29 1,1-Dichloropropene | 75 | | | | | | |
| 30 Carbon Tetrachloride | 117 | | | | | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.316 | 7.296 | (1.103) | 111097 | 60.2441 | 37.005 |
| 32 1,2-Dichloroethane | 62 | | | | | | |
| 33 Benzene | 78 | 7.457 | 7.437 | (0.975) | 3293 | 0.47830 | 0.2938 <i>alg</i> |
| * 34 1,4-Difluorobenzene | 114 | 7.648 | 7.628 | (1.000) | 209666 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | | |
| 36 1,2-Dichloropropane | 63 | | | | | | |
| 37 Bromodichloromethane | 83 | | | | | | |
| 39 Dibromomethane | 93 | | | | | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | | |
| \$ 43 d8-Toluene | 98 | 9.196 | 9.176 | (1.202) | 229938 | 49.9112 | 30.658 |
| 44 Toluene | 92 | | | | | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | | |
| 46 2-Hexanone | 43 | | | | | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | | |
| 48 1,3-Dichloropropane | 76 | | | | | | |
| 49 Tetrachloroethene | 166 | | | | | | |
| 50 Chlorodibromomethane | 129 | | | | | | |
| 51 1,2-Dibromoethane | 107 | | | | | | |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.774 | (1.000) | 174438 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | | |
| 54 Ethyl Benzene | 91 | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | | |
| 56 m,p-xylene | 106 | | | | | | |
| 57 o-Xylene | 106 | | | | | | |
| 58 Styrene | 104 | | | | | | |
| 59 Isopropyl Benzene | 105 | | | | | | |
| 60 Bromoform | 173 | | | | | | |
| 61 1,1,1,2,2-Tetrachloroethane | 83 | | | | | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.120 | 12.100 | (1.123) | 96481 | 47.2596 | 29.029 |
| 63 1,2,3-Trichloropropane | 110 | | | | | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.477 | 13.457 | (1.000) | 83991 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.909 | (1.033) | 79325 | 51.9231 | 31.894 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58B.d
 Lab Smp Id: RG58B
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18237

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB22-1.5-2-072910
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 141403 | 7.85 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 209666 | 9.45 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 174438 | 8.21 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 83991 | -4.86 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.65 | 0.26 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.48 | 0.15 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58B
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18237


Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-1.5-2-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 54.148 | 108.30 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 60.244 | 120.49 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 49.911 | 99.82 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 47.260 | 94.52 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.923 | 103.85 | 80-120 |

Data File: /chem1/finn5.i/09AUG10.b/RC588.d
Date : 09-AUG-2010 16:38
Client ID: PSB22-1,5-2-072910
Sample Info: RC588,5,8,14,0
Column phase: Rt:502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18

/chem1/finn5.i/09AUG10.b/RC588.d/RC588.LG



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58C.d
 Lab Smp Id: RG58C Client Smp ID: PSB22-2-4-072910
 Inj Date : 09-AUG-2010 17:04
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58C,5,9.26,0
 Misc Info : 10-18238
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 9.26000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.683 | 4.673 | (0.707) | 139115 | 202.014 | 109.08 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.797) | 7884 | 3.00380 | 1.622 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten mark

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |
| 15 Carbon Disulfide | 76 | | | | | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | | |
| 18 Vinyl Acetate | 43 | | | | | | |
| 19 1,1-Dichloroethane | 63 | | | | | | |
| 20 2-Butanone | 43 | 6.281 | 6.271 | (0.948) | 5926 | 7.64778 | 4.129 |
| 21 2,2-Dichloropropane | 77 | | | | | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 123053 | 50.0000 | |
| 24 Chloroform | 83 | | | | | | |
| 26 Bromochloromethane | 128 | | | | | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 78329 | 53.4081 | 28.838 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | | |
| 29 1,1-Dichloropropene | 75 | | | | | | |
| 30 Carbon Tetrachloride | 117 | | | | | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 97934 | 61.0257 | 32.951 |
| 32 1,2-Dichloroethane | 62 | | | | | | |
| 33 Benzene | 78 | | | | | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 179902 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | | |
| 36 1,2-Dichloropropane | 63 | | | | | | |
| 37 Bromodichloromethane | 83 | | | | | | |
| 39 Dibromomethane | 93 | | | | | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 200920 | 50.8279 | 27.445 |
| 44 Toluene | 92 | | | | | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | | |
| 46 2-Hexanone | 43 | | | | | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | | |
| 48 1,3-Dichloropropane | 76 | | | | | | |
| 49 Tetrachloroethene | 166 | | | | | | |
| 50 Chlorodibromomethane | 129 | | | | | | |
| 51 1,2-Dibromoethane | 107 | | | | | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 151011 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | | |
| 54 Ethyl Benzene | 91 | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | | |
| 56 m,p-xylene | 106 | | | | | | |
| 57 o-Xylene | 106 | | | | | | |
| 58 Styrene | 104 | | | | | | |
| 59 Isopropyl Benzene | 105 | | | | | | |
| 60 Bromoform | 173 | | | | | | |
| 61 1,1,1,2-Tetrachloroethane | 83 | | | | | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.123) | 85428 | 48.3371 | 26.100 |
| 63 1,2,3-Trichloropropane | 110 | | | | | | |

u6

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|----------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.457 | (1.000) | 75393 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 69826 | 50.9178 | 27.493 |
| 80 1,2-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58C.d
 Lab Smp Id: RG58C
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18238

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB22-2-4-072910
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 123053 | -6.15 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 179902 | -6.09 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 151011 | -6.32 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 75393 | -14.60 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58C
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18238

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-2-4-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 53.408 | 106.82 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 61.026 | 122.05 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 50.828 | 101.66 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 48.337 | 96.67 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.918 | 101.84 | 80-120 |

Data File: /chem1/finn5.1/09AUG10.b/R058C.d
Date : 09-AUG-2010 17:04
Client ID: PSB22-2-4-072910
Sample Info: R058C,5,9,26,0
Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58D.d
 Lab Smp Id: RG58D Client Smp ID: PSB22-4-6-072910
 Inj Date : 09-AUG-2010 17:31
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58D,5,9.04,0
 Misc Info : 10-18239
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 9.04000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 91270 | 143.006 | 79.096 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.797) | 11628 | 4.78023 | 2.644 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten mark

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | 6.281 | 6.271 | (0.948) | 3910 | 5.44465 | 3.011 |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 114044 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 75042 | 55.2088 | 30.536 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 94447 | 63.5019 | 35.123 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 169449 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 193120 | 51.8685 | 28.688 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 144305 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.123) | 79894 | 47.3066 | 26.165 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |

nlq

| Compounds | QUANT | SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------|-----|--------|--------|---------|------------------------|----------------|------------|
| | | | | | | | ON-COLUMN | FINAL |
| | MASS | | | | | | (ug/Kg) | (ug/Kg) |
| ===== | ===== | | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | | 13.467 | 13.457 | (1.000) | 70759 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | | 13.909 | 13.909 | (1.033) | 66069 | 51.3333 | 28.392 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58D.d
 Lab Smp Id: RG58D
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18239

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB22-4-6-072910
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 114044 | -13.02 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 169449 | -11.54 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 144305 | -10.48 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 70759 | -19.85 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.


Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58D
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18239

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-4-6-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 55.209 | 110.42 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 63.502 | 127.00 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 51.868 | 103.74 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 47.307 | 94.61 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.333 | 102.67 | 80-120 |



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58E.d
 Lab Smp Id: RG58E Client Smp ID: PSB22-17-19-072910
 Inj Date : 09-AUG-2010 17:57
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58E,5,9.32,0
 Misc Info : 10-18240
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 9.32000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.693 | 4.673 | (0.708) | 7073 | 11.4736 | 6.155 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.286 | 5.266 | (0.797) | 7694 | 3.27465 | 1.757 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten mark

| Compounds | QUANT | SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-------|-----|--------|--------|---------|------------------------|----------------|------------|
| | | | | | | | ON-COLUMN | FINAL |
| | MASS | | | | | | (ug/Kg) | (ug/Kg) |
| ===== | ==== | | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | | | | | Compound Not Detected. | | |
| 21 2,2-Dichloropropane | 77 | | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | | 6.633 | 6.613 | (1.000) | 110155 | 50.0000 | |
| 24 Chloroform | 83 | | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | | 6.854 | 6.834 | (1.033) | 76858 | 58.5412 | 31.406 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | | 7.316 | 7.296 | (1.103) | 97765 | 68.0535 | 36.509 |
| 32 1,2-Dichloroethane | 62 | | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | | 7.648 | 7.628 | (1.000) | 166411 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | | 9.196 | 9.176 | (1.202) | 196937 | 53.8593 | 28.894 |
| 44 Toluene | 92 | | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | | 10.794 | 10.774 | (1.000) | 149317 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | | 12.120 | 12.100 | (1.123) | 84998 | 48.6394 | 26.094 |
| 63 1,2,3-Trichloropropane | 110 | | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.477 | 13.457 | (1.000) | 78068 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.909 | (1.033) | 73236 | 51.5745 | 27.669 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: finn5.i
Lab File ID: RG58E.d
Lab Smp Id: RG58E
Analysis Type: VOA
Quant Type: ISTD
Operator: PB
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18240

Calibration Date: 09-AUG-2010
Calibration Time: 10:35
Client Smp ID: PSB22-17-19-072910
Level: LOW
Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 110155 | -15.99 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 166411 | -13.13 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 149317 | -7.37 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 78068 | -11.57 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.65 | 0.26 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.48 | 0.15 |

AREA UPPER LIMIT = +100% of internal standard area.
AREA LOWER LIMIT = - 50% of internal standard area.
RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58E
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18240

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-17-19-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 58.541 | 117.08 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 68.053 | 136.11 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 53.859 | 107.72 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 48.639 | 97.28 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.574 | 103.15 | 80-120 |

Data File: /chem1/finn5.1/09AUG10.b/RG58E.d
Date : 09-AUG-2010 17:57
Client ID: PSB22-17-19-072910
Sample Info: RG58E,5,9,32.0
Column phase: Rtx502.2

Instrument: finn5.1
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58F.d
 Lab Smp Id: RG58F Client Smp ID: PSB22-19-20-072910
 Inj Date : 09-AUG-2010 18:24
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58F,5,10.49,0
 Misc Info : 10-18241
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

f. st. l. b.

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|----------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 10.49000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|---|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.683 | 4.673 | (0.706) | 9368 | 16.1679 | 7.706 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.286 | 5.266 | (0.797) | 7483 | 3.38845 | 1.615 |
| 14 Acrylonitrile | 53 | | | | | | |

u/g

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|----------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | | | | Compound Not Detected. | | |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.633 | 6.613 | (1.000) | 103536 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.854 | 6.834 | (1.033) | 70717 | 57.3072 | 27.315 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.316 | 7.296 | (1.103) | 90369 | 66.9267 | 31.900 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.648 | 7.628 | (1.000) | 156457 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.196 | 9.176 | (1.202) | 179648 | 52.2568 | 24.908 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.774 | (1.000) | 137444 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.120 | 12.100 | (1.123) | 80300 | 49.9205 | 23.794 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------------------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | | |
| 66 N-Propyl Benzene | 91 | | | | | | |
| 67 Bromobenzene | 156 | | | | | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | | |
| 69 2-Chloro Toluene | 91 | | | | | | |
| 70 4-Chloro Toluene | 91 | | | | | | |
| 71 T-Butyl Benzene | 119 | | | | | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | | |
| 73 S-Butyl Benzene | 105 | | | | | | |
| 74 4-Isopropyl Toluene | 119 | | | | | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.477 | 13.457 | (1.000) | 73064 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | | |
| 78 N-Butyl Benzene | 91 | | | | | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.909 | (1.033) | 67895 | 51.0879 | 24.351 |
| 80 1,2-Dichlorobenzene | 146 | | | | | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | | |
| 84 Naphthalene | 128 | | | | | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: finn5.i
Lab File ID: RG58F.d
Lab Smp Id: RG58F
Analysis Type: VOA
Quant Type: ISTD
Operator: PB
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18241

Calibration Date: 09-AUG-2010
Calibration Time: 10:35
Client Smp ID: PSB22-19-20-072910
Level: LOW
Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 103536 | -21.03 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 156457 | -18.32 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 137444 | -14.74 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 73064 | -17.24 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.65 | 0.26 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.48 | 0.15 |

AREA UPPER LIMIT = +100% of internal standard area.
AREA LOWER LIMIT = - 50% of internal standard area.
RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58F
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18241

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-19-20-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 57.307 | 114.61 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 66.927 | 133.85 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.257 | 104.51 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 49.920 | 99.84 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.088 | 102.18 | 80-120 |

Data File: /chem1/finm5.1/09AUG10.b/RG58F.d

Date : 09-AUG-2010 18:24

Client ID: PS822-19-20-072910


Sample Info: RG58F.5,10,49,0

Column phase: Rtx502.2

Instrument: finm5.1

Operator: PB

Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58K.d
 Lab Smp Id: RG58K Client Smp ID: PSB23-14-16.5-07291
 Inj Date : 09-AUG-2010 18:50
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58K,5,12.35,0
 Misc Info : 10-18246
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|----------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 12.35000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|---|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 37824 | 64.6016 | 26.154 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.797) | 9637 | 4.31852 | 1.748 |
| 14 Acrylonitrile | 53 | | | | | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-------------------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |
| 15 Carbon Disulfide | 76 | 5.377 | 5.367 | (0.812) | 7873 | 1.28086 | 0.5186 |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | | |
| 18 Vinyl Acetate | 43 | | | | | | |
| 19 1,1-Dichloroethane | 63 | | | | | | |
| 20 2-Butanone | 43 | 6.281 | 6.271 | (0.948) | 2816 | 4.27440 | 1.730 |
| 21 2,2-Dichloropropane | 77 | | | | | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 104622 | 50.0000 | |
| 24 Chloroform | 83 | | | | | | |
| 26 Bromochloromethane | 128 | | | | | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 72264 | 57.9529 | 23.463 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | | |
| 29 1,1-Dichloropropene | 75 | | | | | | |
| 30 Carbon Tetrachloride | 117 | | | | | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 91309 | 66.9209 | 27.093 |
| 32 1,2-Dichloroethane | 62 | | | | | | |
| 33 Benzene | 78 | | | | | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 159024 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | | |
| 36 1,2-Dichloropropane | 63 | | | | | | |
| 37 Bromodichloromethane | 83 | | | | | | |
| 39 Dibromomethane | 93 | | | | | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 183616 | 52.5489 | 21.275 |
| 44 Toluene | 92 | | | | | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | | |
| 46 2-Hexanone | 43 | | | | | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | | |
| 48 1,3-Dichloropropane | 76 | | | | | | |
| 49 Tetrachloroethene | 166 | | | | | | |
| 50 Chlorodibromomethane | 129 | | | | | | |
| 51 1,2-Dibromoethane | 107 | | | | | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 137738 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | | |
| 54 Ethyl Benzene | 91 | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | | |
| 56 m,p-xylene | 106 | | | | | | |
| 57 o-Xylene | 106 | | | | | | |
| 58 Styrene | 104 | | | | | | |
| 59 Isopropyl Benzene | 105 | | | | | | |
| 60 Bromoform | 173 | | | | | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.123) | 78126 | 48.4653 | 19.622 |
| 63 1,2,3-Trichloropropane | 110 | | | | | | |

ng
↓

| Compounds | QUANT | SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------|-----|--------|--------|---------|------------------------|----------------|------------|
| | | | | | | | ON-COLUMN | FINAL |
| | MASS | | | | | | (ug/Kg) | (ug/Kg) |
| ===== | ==== | | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | | 13.467 | 13.457 | (1.000) | 67417 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | | 13.909 | 13.909 | (1.033) | 63469 | 51.7578 | 20.954 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58K.d
 Lab Smp Id: RG58K
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18246

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB23-14-16.5-07291
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 104622 | -20.21 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 159024 | -16.98 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 137738 | -14.55 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 67417 | -23.63 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58K
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18246

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB23-14-16.5-07291
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 57.953 | 115.91 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 66.921 | 133.84 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.549 | 105.10 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 48.465 | 96.93 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.758 | 103.52 | 80-120 |

Data File: /chem1/finn5.1/09AUG10.b/RG58K.d
Date : 09-AUG-2010 18:50
Client ID: PSB23-14-16.5-07291
Sample Info: RG58K.5.12.35.0
Column phase: Rt:502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58L.d
 Lab Smp Id: RG58L Client Smp ID: PSB23-16.5-19-07291
 Inj Date : 09-AUG-2010 19:16 ✓
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58L,5,9.92,0
 Misc Info : 10-18247
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 9.92000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 14127 | 25.0610 | 12.632 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.795) | 9026 | 4.20109 | 2.117 |
| 14 Acrylonitrile | 53 | | | | | | |

| Compounds | QUANT SIG MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-------------------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 16 Methyl tert-Butyl Ether | 73 | | | | Compound Not Detected. | | |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | | | | Compound Not Detected. | | |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 100728 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.032) | 71281 | 59.3745 | 29.927 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 91324 | 69.5194 | 35.040 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.628 | 7.628 | (1.000) | 154377 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.204) | 178253 | 52.5496 | 26.487 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 139039 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 81404 | 50.0263 | 25.215 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | | |
| 66 N-Propyl Benzene | 91 | | | | | | |
| 67 Bromobenzene | 156 | | | | | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | | |
| 69 2-Chloro Toluene | 91 | | | | | | |
| 70 4-Chloro Toluene | 91 | | | | | | |
| 71 T-Butyl Benzene | 119 | | | | | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | | |
| 73 S-Butyl Benzene | 105 | | | | | | |
| 74 4-Isopropyl Toluene | 119 | | | | | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 72259 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | | |
| 78 N-Butyl Benzene | 91 | | | | | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.034) | 69662 | 53.0014 | 26.714 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | | |
| 84 Naphthalene | 128 | | | | | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58L.d
 Lab Smp Id: RG58L
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18247

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB23-16.5-19-07291
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 100728 | -23.18 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 154377 | -19.41 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 139039 | -13.75 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 72259 | -18.15 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.46 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58L
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18247


Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB23-16.5-19-07291
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 59.374 | 118.75 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 69.519 | 139.04 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.550 | 105.10 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 50.026 | 100.05 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 53.001 | 106.00 | 80-120 |

Data File: /chem1/finn5.i/09AUG10.b/RGSBL.d
Date: 09-AUG-2010 19:16
Client ID: PSB23-16.5-19-07291
Sample Info: RGSBL,5,9,92,0

Column phase: Rt:502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58T.d
Lab Smp Id: RG58T Client Smp ID: PSB22-TB
Inj Date : 09-AUG-2010 19:43
Operator : PB Inst ID: finn5.i
Smp Info : RG58T,5,5,0
Misc Info : 10-18255
Comment :
Method : /chem1/finn5.i/09AUG10.b/s8260b.m
Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
Als bottle: 1
Dil Factor: 1.00000
Integrator: HP RTE Compound Sublist: voa.sub
Target Version: 3.50
Processing Host: cserv3



Concentration Formula: Amt * DF * Pv / Sa * CpndVariable

| Name | Value | Description |
|------|---------|-------------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | PurgeVolume (mL) |
| Sa | 0.00000 | SampleAmount (mL) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|--------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.663 | 4.673 | (0.705) | 2285 | 4.19136 | 4.191 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | | | | | | |
| 14 Acrylonitrile | 53 | | | | | | |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |



| Compounds | QUANT | SIG | | | | | CONCENTRATIONS | |
|--------------------------------|-------|-------|--------|--------|---------|----------|----------------------|------------------|
| | | | RT | EXP RT | REL RT | RESPONSE | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| ===== | ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 15 Carbon Disulfide | 76 | | | | | | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | | | |
| 18 Vinyl Acetate | 43 | | | | | | | |
| 19 1,1-Dichloroethane | 63 | | | | | | | |
| 20 2-Butanone | 43 | | | | | | | |
| 21 2,2-Dichloropropane | 77 | | | | | | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | | | |
| * 23 Pentafluorobenzene | 168 | | 6.613 | 6.613 | (1.000) | 97416 | 50.0000 | |
| 24 Chloroform | 83 | | | | | | | |
| 26 Bromochloromethane | 128 | | | | | | | |
| \$ 25 Dibromofluoromethane | 111 | | 6.834 | 6.834 | (1.033) | 66110 | 56.9395 | 56.939(Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | | | |
| 29 1,1-Dichloropropene | 75 | | | | | | | |
| 30 Carbon Tetrachloride | 117 | | | | | | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | | 7.296 | 7.296 | (1.103) | 77957 | 61.3615 | 61.362 |
| 32 1,2-Dichloroethane | 62 | | | | | | | |
| 33 Benzene | 78 | | | | | | | |
| * 34 1,4-Difluorobenzene | 114 | | 7.628 | 7.628 | (1.000) | 148990 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | | | |
| 36 1,2-Dichloropropane | 63 | | | | | | | |
| 37 Bromodichloromethane | 83 | | | | | | | |
| 39 Dibromomethane | 93 | | | | | | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | | | |
| \$ 43 d8-Toluene | 98 | | 9.176 | 9.176 | (1.203) | 171330 | 52.3349 | 52.335 |
| 44 Toluene | 92 | | | | | | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | | | |
| 46 2-Hexanone | 43 | | | | | | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | | | |
| 48 1,3-Dichloropropane | 76 | | | | | | | |
| 49 Tetrachloroethene | 166 | | | | | | | |
| 50 Chlorodibromomethane | 129 | | | | | | | |
| 51 1,2-Dibromoethane | 107 | | | | | | | |
| * 52 d5-Chlorobenzene | 117 | | 10.774 | 10.774 | (1.000) | 126813 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | | | |
| 54 Ethyl Benzene | 91 | | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | | | |
| 56 m,p-xylene | 106 | | | | | | | |
| 57 o-Xylene | 106 | | | | | | | |
| 58 Styrene | 104 | | | | | | | |
| 59 Isopropyl Benzene | 105 | | | | | | | |
| 60 Bromoform | 173 | | | | | | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | | | | |
| \$ 62 4-Bromofluorobenzene | 95 | | 12.100 | 12.100 | (1.123) | 70757 | 47.6754 | 47.675 |
| 63 1,2,3-Trichloropropane | 110 | | | | | | | |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 66 N-Propyl Benzene | 91 | | | | | | |
| 67 Bromobenzene | 156 | | | | | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | | |
| 69 2-Chloro Toluene | 91 | | | | | | |
| 70 4-Chloro Toluene | 91 | | | | | | |
| 71 T-Butyl Benzene | 119 | | | | | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | | |
| 73 S-Butyl Benzene | 105 | | | | | | |
| 74 4-Isopropyl Toluene | 119 | | | | | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 61537 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | | |
| 78 N-Butyl Benzene | 91 | | | | | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.899 | 13.909 | (1.033) | 58155 | 51.9558 | 51.956 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | | |
| 84 Naphthalene | 128 | | | | | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58T.d
 Lab Smp Id: RG58T
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18255

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB22-TB
 Level: LOW
 Sample Type: Water

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 97416 | -25.70 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 148990 | -22.22 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 126813 | -21.33 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 61537 | -30.29 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.61 | 0.00 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.63 | 0.00 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.77 | 0.00 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.46 | 0.00 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: LIQUID
Lab Smp Id: RG58T
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18255

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB22-TB
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 56.939 | 113.88 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 61.362 | 122.72 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.335 | 104.67 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 47.675 | 95.35 | 71-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.956 | 103.91 | 80-121 |

Data File: /chem1/firm5.i/09AUG10.b/RGS8T.d
Date : 09-AUG-2010 19:43
Client ID: PSB22-TB
Sample Info: RGS8T,5,5,0
Column phase: Rtx502.2

Instrument: firm5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58U.d
 Lab Smp Id: RG58U Client Smp ID: PSB23-TB
 Inj Date : 09-AUG-2010 20:09
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58U,5,5,0
 Misc Info : 10-18256
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

patrickb

Concentration Formula: Amt * DF * Pv / Sa * CpndVariable

| Name | Value | Description |
|------|---------|-------------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | PurgeVolume (mL) |
| Sa | 0.00000 | SampleAmount (mL) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|-----------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 1913 | 3.41740 | 3.417 <i>ug</i> |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | | | | | | |
| 14 Acrylonitrile | 53 | | | | | | |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | | | | Compound Not Detected. | | |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 100027 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 68816 | 57.7230 | 57.723 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 82613 | 63.3290 | 63.329 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 154248 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 179747 | 53.0344 | 53.034 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 136628 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.122) | 75887 | 47.4588 | 47.459 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 66 N-Propyl Benzene | 91 | | | | | | |
| 67 Bromobenzene | 156 | | | | | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | | |
| 69 2-Chloro Toluene | 91 | | | | | | |
| 70 4-Chloro Toluene | 91 | | | | | | |
| 71 T-Butyl Benzene | 119 | | | | | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | | |
| 73 S-Butyl Benzene | 105 | | | | | | |
| 74 4-Isopropyl Toluene | 119 | | | | | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.457 | (1.000) | 65693 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | | |
| 78 N-Butyl Benzene | 91 | | | | | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 61709 | 51.6432 | 51.643 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | | |
| 84 Naphthalene | 128 | | | | | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58U.d
 Lab Smp Id: RG58U
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18256

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB23-TB
 Level: LOW
 Sample Type: Water

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 100027 | -23.71 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 154248 | -19.48 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 136628 | -15.24 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 65693 | -25.58 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: LIQUID
Lab Smp Id: RG58U
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18256

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB23-TB
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 57.723 | 115.45 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 63.329 | 126.66 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 53.034 | 106.07 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 47.459 | 94.92 | 71-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 51.643 | 103.29 | 80-121 |

Data File: /chem1/finn5.i/09AUG10.b/RG58U.d
Date : 09-AUG-2010 20:09
Client ID: PSB23-TB
Sample Info: RG58U,5,5,0
Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58V.d
Lab Smp Id: RG58V Client Smp ID: PSB24-TB
Inj Date : 09-AUG-2010 20:35
Operator : PB Inst ID: finn5.i
Smp Info : RG58V,5,5,0
Misc Info : 10-18257
Comment :
Method : /chem1/finn5.i/09AUG10.b/s8260b.m
Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
Als bottle: 1
Dil Factor: 1.00000
Integrator: HP RTE Compound Sublist: voa.sub
Target Version: 3.50
Processing Host: cserv3

Concentration Formula: Amt * DF * Pv / Sa * CpndVariable

| Name | Value | Description |
|------|---------|-------------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | PurgeVolume (mL) |
| Sa | 0.00000 | SampleAmount (mL) |

Cpnd Variable Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.673 | 4.673 | (0.706) | 1912 | 3.38335 | 3.383 <i>nlq</i> |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | | | | | | |
| 14 Acrylonitrile | 53 | | | | | | |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|------------------------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| ===== | ===== | == | ===== | ===== | ===== | ===== | ===== |
| 15 Carbon Disulfide | 76 | | | | Compound Not Detected. | | |
| 17 Trans-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| 18 Vinyl Acetate | 43 | | | | Compound Not Detected. | | |
| 19 1,1-Dichloroethane | 63 | | | | Compound Not Detected. | | |
| 20 2-Butanone | 43 | | | | Compound Not Detected. | | |
| 21 2,2-Dichloropropane | 77 | | | | Compound Not Detected. | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | Compound Not Detected. | | |
| * 23 Pentafluorobenzene | 168 | 6.623 | 6.613 | (1.000) | 100981 | 50.0000 | |
| 24 Chloroform | 83 | | | | Compound Not Detected. | | |
| 26 Bromochloromethane | 128 | | | | Compound Not Detected. | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.033) | 68315 | 56.7614 | 56.761 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 29 1,1-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 30 Carbon Tetrachloride | 117 | | | | Compound Not Detected. | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.103) | 83269 | 63.2288 | 63.229 |
| 32 1,2-Dichloroethane | 62 | | | | Compound Not Detected. | | |
| 33 Benzene | 78 | | | | Compound Not Detected. | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 154524 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | Compound Not Detected. | | |
| 36 1,2-Dichloropropane | 63 | | | | Compound Not Detected. | | |
| 37 Bromodichloromethane | 83 | | | | Compound Not Detected. | | |
| 39 Dibromomethane | 93 | | | | Compound Not Detected. | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | Compound Not Detected. | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | Compound Not Detected. | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | Compound Not Detected. | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 176822 | 52.0782 | 52.078 |
| 44 Toluene | 92 | | | | Compound Not Detected. | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | Compound Not Detected. | | |
| 46 2-Hexanone | 43 | | | | Compound Not Detected. | | |
| 47 1,1,2-Trichloroethane | 97 | | | | Compound Not Detected. | | |
| 48 1,3-Dichloropropane | 76 | | | | Compound Not Detected. | | |
| 49 Tetrachloroethene | 166 | | | | Compound Not Detected. | | |
| 50 Chlorodibromomethane | 129 | | | | Compound Not Detected. | | |
| 51 1,2-Dibromoethane | 107 | | | | Compound Not Detected. | | |
| * 52 d5-Chlorobenzene | 117 | 10.784 | 10.774 | (1.000) | 131451 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | Compound Not Detected. | | |
| 54 Ethyl Benzene | 91 | | | | Compound Not Detected. | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | Compound Not Detected. | | |
| 56 m,p-xylene | 106 | | | | Compound Not Detected. | | |
| 57 o-Xylene | 106 | | | | Compound Not Detected. | | |
| 58 Styrene | 104 | | | | Compound Not Detected. | | |
| 59 Isopropyl Benzene | 105 | | | | Compound Not Detected. | | |
| 60 Bromoform | 173 | | | | Compound Not Detected. | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | Compound Not Detected. | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.123) | 74701 | 48.5570 | 48.557 |
| 63 1,2,3-Trichloropropane | 110 | | | | Compound Not Detected. | | |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | Compound Not Detected. | | |

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/L) |
| 66 N-Propyl Benzene | 91 | | | | | | |
| 67 Bromobenzene | 156 | | | | | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | | |
| 69 2-Chloro Toluene | 91 | | | | | | |
| 70 4-Chloro Toluene | 91 | | | | | | |
| 71 T-Butyl Benzene | 119 | | | | | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | | |
| 73 S-Butyl Benzene | 105 | | | | | | |
| 74 4-Isopropyl Toluene | 119 | | | | | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.467 | 13.457 | (1.000) | 64680 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | | |
| 78 N-Butyl Benzene | 91 | | | | | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.909 | 13.909 | (1.033) | 59920 | 50.9314 | 50.931 |
| 80 1,2-Dichlorobenzene | 146 | | | | | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | | |
| 84 Naphthalene | 128 | | | | | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58V.d
 Lab Smp Id: RG58V
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18257

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB24-TB
 Level: LOW
 Sample Type: Water

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 100981 | -22.98 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 154524 | -19.33 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 131451 | -18.45 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 64680 | -26.73 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.62 | 0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.78 | 0.09 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: LIQUID
Lab Smp Id: RG58V
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18257

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB24-TB
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 56.761 | 113.52 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 63.229 | 126.46 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.078 | 104.16 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 48.557 | 97.11 | 71-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.931 | 101.86 | 80-121 |

Data File: /chem1/firm5.i/09AUG10.b/RG58V.d
Date : 09-AUG-2010 20:35
Client ID: PSB24-TB
Sample Info: RG58V,5,5,0
Column phase: Rtx502.2

Instrument: firm5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/09AUG10.b/RG58R.d
 Lab Smp Id: RG58R Client Smp ID: PSB24-14-16-072910
 Inj Date : 09-AUG-2010 21:02
 Operator : PB Inst ID: finn5.i
 Smp Info : RG58R,5,10.91,0
 Misc Info : 10-18253
 Comment :
 Method : /chem1/finn5.i/09AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 12:17 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature: jslabo

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|----------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 10.91000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | | | | | | |
| 2 Chloromethane | 50 | | | | | | |
| 3 Vinyl Chloride | 62 | | | | | | |
| 4 Bromomethane | 94 | | | | | | |
| 5 Chloroethane | 64 | | | | | | |
| 6 Trichlorofluoromethane | 101 | | | | | | |
| 7 Acrolein | 56 | | | | | | |
| 8 112Trichloro122Trifluoroethane | 101 | | | | | | |
| 9 Acetone | 43 | 4.683 | 4.673 | (0.706) | 39053 | 68.5685 | 31.425 |
| 10 1,1-Dichloroethene | 96 | | | | | | |
| 11 Bromoethane | 108 | | | | | | |
| 12 Iodomethane | 142 | | | | | | |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.795) | 7568 | 3.48634 | 1.598 |
| 14 Acrylonitrile | 53 | | | | | | |

Handwritten signature: jslabo

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | | | | | | |
| 15 Carbon Disulfide | 76 | 5.387 | 5.367 | (0.812) | 4479 | 0.74910 | 0.3433 (Q) |
| 17 Trans-1,2-Dichloroethene | 96 | | | | | | |
| 18 Vinyl Acetate | 43 | | | | | | |
| 19 1,1-Dichloroethane | 63 | | | | | | |
| 20 2-Butanone | 43 | 6.291 | 6.271 | (0.948) | 2945 | 4.59540 | 2.106 |
| 21 2,2-Dichloropropane | 77 | | | | | | |
| 22 Cis-1,2-Dichloroethene | 96 | | | | | | |
| * 23 Pentafluorobenzene | 168 | 6.633 | 6.613 | (1.000) | 101772 | 50.0000 | |
| 24 Chloroform | 83 | | | | | | |
| 26 Bromochloromethane | 128 | | | | | | |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 | (1.032) | 72059 | 59.4068 | 27.226 (Q) |
| 27 1,1,1-Trichloroethane | 97 | | | | | | |
| 29 1,1-Dichloropropene | 75 | | | | | | |
| 30 Carbon Tetrachloride | 117 | | | | | | |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.306 | 7.296 | (1.101) | 92612 | 69.7766 | 31.978 |
| 32 1,2-Dichloroethane | 62 | | | | | | |
| 33 Benzene | 78 | | | | | | |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.628 | (1.000) | 157962 | 50.0000 | |
| 35 Trichloroethene | 95 | | | | | | |
| 36 1,2-Dichloropropane | 63 | | | | | | |
| 37 Bromodichloromethane | 83 | | | | | | |
| 39 Dibromomethane | 93 | | | | | | |
| 40 2-Chloroethyl Vinyl Ether | 63 | | | | | | |
| 41 4-Methyl-2-Pentanone | 58 | | | | | | |
| 42 Cis 1,3-dichloropropene | 75 | | | | | | |
| \$ 43 d8-Toluene | 98 | 9.186 | 9.176 | (1.203) | 181826 | 52.3864 | 24.008 |
| 44 Toluene | 92 | | | | | | |
| 45 Trans 1,3-Dichloropropene | 75 | | | | | | |
| 46 2-Hexanone | 43 | | | | | | |
| 47 1,1,2-Trichloroethane | 97 | | | | | | |
| 48 1,3-Dichloropropane | 76 | | | | | | |
| 49 Tetrachloroethene | 166 | | | | | | |
| 50 Chlorodibromomethane | 129 | | | | | | |
| 51 1,2-Dibromoethane | 107 | | | | | | |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.774 | (1.000) | 139242 | 50.0000 | |
| 53 Chlorobenzene | 112 | | | | | | |
| 54 Ethyl Benzene | 91 | | | | | | |
| 55 1,1,1,2-Tetrachloroethane | 131 | | | | | | |
| 56 m,p-xylene | 106 | | | | | | |
| 57 o-Xylene | 106 | | | | | | |
| 58 Styrene | 104 | | | | | | |
| 59 Isopropyl Benzene | 105 | | | | | | |
| 60 Bromoform | 173 | | | | | | |
| 61 1,1,2,2-Tetrachloroethane | 83 | | | | | | |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 | (1.122) | 80947 | 49.6729 | 22.765 |
| 63 1,2,3-Trichloropropane | 110 | | | | | | |

wg

| Compounds | QUANT | SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-------|-----|--------|--------|---------|------------------------|----------------|------------|
| | | | | | | | ON-COLUMN | FINAL |
| | MASS | | | | | | (ug/Kg) | (ug/Kg) |
| ===== | ===== | | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | | | | | Compound Not Detected. | | |
| 66 N-Propyl Benzene | 91 | | | | | Compound Not Detected. | | |
| 67 Bromobenzene | 156 | | | | | Compound Not Detected. | | |
| 68 1,3,5-Trimethyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 69 2-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 70 4-Chloro Toluene | 91 | | | | | Compound Not Detected. | | |
| 71 T-Butyl Benzene | 119 | | | | | Compound Not Detected. | | |
| 72 1,2,4-Trimethylbenzene | 105 | | | | | Compound Not Detected. | | |
| 73 S-Butyl Benzene | 105 | | | | | Compound Not Detected. | | |
| 74 4-Isopropyl Toluene | 119 | | | | | Compound Not Detected. | | |
| 75 1,3-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| * 76 d4-1,4-Dichlorobenzene | 152 | | 13.467 | 13.457 | (1.000) | 70424 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 78 N-Butyl Benzene | 91 | | | | | Compound Not Detected. | | |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | | 13.919 | 13.909 | (1.034) | 67591 | 52.7657 | 24.182 (Q) |
| 80 1,2-Dichlorobenzene | 146 | | | | | Compound Not Detected. | | |
| 81 1,2-Dibromo 3-Chloropropane | 75 | | | | | Compound Not Detected. | | |
| 82 1,2,4-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |
| 83 Hexachloro 1,3-Butadiene | 225 | | | | | Compound Not Detected. | | |
| 84 Naphthalene | 128 | | | | | Compound Not Detected. | | |
| 85 1,2,3-Trichlorobenzene | 180 | | | | | Compound Not Detected. | | |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: RG58R.d
 Lab Smp Id: RG58R
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
 Misc Info: 10-18253

Calibration Date: 09-AUG-2010
 Calibration Time: 10:35
 Client Smp ID: PSB24-14-16-072910
 Level: LOW
 Sample Type: Soil

Test Mode:

Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 101772 | -22.38 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 157962 | -17.54 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 139242 | -13.62 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 70424 | -20.23 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.64 | 0.13 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.47 | 0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT


Client Name: Floyd/Snider
Sample Matrix: SOLID
Lab Smp Id: RG58R
Level: LOW
Data Type: MS DATA
SpikeList File: all.spk
Sublist File: voa.sub
Method File: /chem1/finn5.i/09AUG10.b/s8260b.m
Misc Info: 10-18253

Client SDG: RG58
Fraction: VOA
Client Smp ID: PSB24-14-16-072910
Operator: PB
SampleType: SAMPLE
Quant Type: ISTD

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 59.407 | 118.81 | 30-160 |
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 69.777 | 139.55 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 52.386 | 104.77 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 49.673 | 99.35 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 52.766 | 105.53 | 80-120 |

Data File: /chem1/firm5.1/09AUG10.b/RG58R.d
Date : 09-AUG-2010 21:02
Client ID: PSB24-14-16-072910
Sample Info: RG58R,5,10,91,0
Column phase: Rtx502.2

Instrument: firm5.1
Operator: PB
Column diameter: 0.18





VOA Analyst Notes / Corrective Action Log

ARI Project ID: RG58 Client ID: Floyd Sander

ARI SOP: **404S**(Gas) **410S**(BTEX) **430S**(VPH) **700S**(8260C) **703S**(SIM) **706S**(524.2) **710S**(RSK-175)

Parameter(s): _____

Instrument: NT-3 NT-5 NT-7 NT-9 NT-10 PID-1 PID-2 PID-3 FID-6 **FINN-5**

Purge Volume (mL) 5 Curve Date: 7/23/10 Analysis Start Date: 8/10/10

| | | | |
|-----------------------------------|----------------------|----------------------------------|----------------------|
| pH ≤ 2.0 | YES / NO / NA | Method Blank In Control? | YES / NO |
| BFB Tune Meets Criteria? | YES / NO / NA | LCS / LCSD Recovery In Control? | YES / NO |
| Internal Standard Meets Criteria? | YES / NO / NA | Surrogate Recovery In Control? | YES / NO |
| ICal acceptable? | YES / NO | CCal acceptable? | YES / NO |
| Q flag applied? | YES / NO / NA | Q flag applied? | YES / NO / NA |
| Manual Integrations for ICal? | YES / NO | Manual Integrations for Samples? | Yes / NO |
| Special Analysis Criteria Met? | YES / NO / NA | | |

Bubbles/Headspace: None SM (≤ 2mm ●) PB (2-4mm) LG (> 4mm ●) Head Space

Detail problems, corrective actions and/or other pertinent information below (use reverse side when necessary):

sample 5 run

Additional Details on Reverse: Yes / **No**

Analyst: _____ Date: 8/10/10

Reviewer: _____ Date: 8/10/10

Analytical Resources Inc.: Organics Instrument Log

FINN5 Serial No.: 5500-000421A

Date: 8/10/06 Analysis: SMAC Analyst: JP
 GC Program: PS Column No: 821729 Column Type: WATER
 Instrument Tune (.U or .CT.): BFB010 EM Voltage: 1648
 Calibration File: 0500Y0A Curve Date: 7/25/06

| IS/SS | Ical/Ccal | LCS/ICV |
|----------------|----------------|----------------|
| <u>W 648-2</u> | <u>W 646-2</u> | <u>W 646-2</u> |
| | | |
| | | |
| | | |

INTERNAL STANDARD SUMMARY FOR DATABATCH - /chem1/finn5.i/10AUG10.b

| Time | Filename | LabID | ClientID | WT | |
|------|----------|------------|----------|---------------------|--|
| 1 | 0846 | BFB0810.d | BFB0810 | 0.00 | |
| 2 | 0914 | 0500810.d | CC0810 | VSTD050 | 5.00 6.62 115835 7.63 174069 10.78 145877 13.47 78708 |
| 3 | 1038 | 0500810A.d | CC0810 | VSTD050 | 5.00 6.61 117420 7.62 167913 10.77 137539 13.46 74652 |
| 4 | 1112 | LCS0810.d | LCS0810 | LCS0810 | 5.00 6.63 113963 7.65 170822 10.79 146772 13.48 80742 |
| 5 | 1137 | LCS0810A.d | LCS0810 | LCS0810 | 5.00 6.63 120686 7.64 178947 10.79 146633 13.47 78163 |
| 6 | 1206 | MB0810.d | MB0810 | MB0810 | 5.00 6.62 114844 7.64 162120 10.78 136524 13.47 66691 |
| 7 | 1235 | RG58S2.d | RG58S | PSB24-16-17-072910 | 5.00 6.62 109057 7.63 158794 10.78 136121 13.46 67577 |
| 8 | 1309 | RH20A2.d | RH20A | IT-ROB-CMP1-080410 | 5.00 6.62 100903 7.64 152273 10.78 123137 13.47 52183 |
| 9 | 1336 | RH20B2.d | RH20B | IT-ROB-CMP2-080410 | 5.00 6.63 106604 7.65 161402 10.79 120135 13.48 45383 |
| 10 | 1402 | RG52F2.d | RG52F | KSC-DP-3-S-7-8-1007 | 5.00 6.63 108297 7.64 157896 10.79 141897 13.48 84084 |
| 11 | 1431 | RG94A.d | RG94A | MW14-15-16.5-080210 | 5.00 6.62 136703 7.63 206520 10.77 170733 13.46 82102 |
| 12 | 1455 | RG94B.d | RG94B | MW14-22.5-24-080210 | 5.00 6.62 124371 7.64 184757 10.78 152814 13.47 73136 |
| 13 | 1522 | RG94C.d | RG94C | MW13-10-11.5-080210 | 5.00 6.63 128814 7.64 189147 10.79 162563 13.47 82845 |
| 14 | 1548 | RG94D.d | RG94D | MW13-14-14.5-080210 | 5.00 6.61 116703 7.63 175855 10.77 149298 13.46 74772 |
| 15 | 1615 | RG94E.d | RG94E | MW13-18.5-19.5-0802 | 5.00 6.63 121960 7.65 183448 10.79 157767 13.48 80744 |
| 16 | 1641 | RG94F.d | RG94F | MW13-18.5-19.5-0802 | 5.00 6.62 116169 7.64 173753 10.78 148950 13.47 72689 |
| 17 | 1708 | RG94G.d | RG94G | MW12-5.5-7.5-080210 | 5.00 6.62 119582 7.64 172971 10.78 131490 13.47 47111 |
| 18 | 1734 | RG94H.d | RG94H | MW12-8-9.5-080210 | 5.00 6.62 124485 7.63 187779 10.78 162157 13.46 80115 |
| 19 | 1800 | RG94I.d | RG94I | MW12-10-11.5-080210 | 5.00 6.63 121739 7.65 184223 10.79 160662 13.48 79097 |
| 20 | 1827 | RG94J.d | RG94J | MW12-17.5-19-080210 | 5.00 6.61 122631 7.63 185787 10.77 163042 13.46 81851 |
| 21 | 1853 | RG94HMS.d | RG94HMS | MW12-8-9.5-0802 MS | 5.00 6.63 141956 7.64 209660 10.79 170873 13.47 93777 |
| 22 | 1920 | RG94HMSD.d | RG94HMSD | MW12-8-9.5-0802 MSD | 5.00 6.62 141432 7.63 212955 10.78 171883 13.47 99347 |
| 23 | 1946 | RH57A.d | RH57A | 10080090 | 5.00 6.63 121001 7.65 182566 10.79 159819 13.48 79906 |
| 24 | 2012 | RH57B.d | RH57B | 10080099 | 5.00 6.62 129799 7.64 185561 10.78 173434 13.47 84041 |
| 25 | 2039 | RH57D0.d | RH57D | 10080110 | 5.00 6.61 120263 7.63 175914 10.78 263238 13.46 90055 |
| 26 | 2105 | RH57C0.d | RH57C | 10080108 | 5.00 6.63 117373 7.65 173509 10.80 333841 13.48 152401 |

Mail

Mail Every

period.

MANUAL INTEGRATION SUMMARY FOR DATABATCH - /chem1/finn5.i/10AUG10.b

ARI Job No.: BFB0 Method: bfb8260.m Instrument: finn5.i Date: 10-AUG-2010

Time Filename LabID ClientId DF Manually Integrated Compounds

0846 BFB0810.d BFB0810 BFB0810 1 NO MANUAL INTEGRATION

1038 0500810A.d CC0810 VSTD050 1 NO MANUAL INTEGRATION

1112 LCS0810.d LCS0810 LCS0810 1 NO MANUAL INTEGRATION

1137 LCS0810A.d LCS0810 LCS0810 1 NO MANUAL INTEGRATION

1206 MB0810.d MB0810 MB0810 1 NO MANUAL INTEGRATION

1235 RG58S2.d RG58S PSB24-16-1 1 NO MANUAL INTEGRATION

Q-FLAG SUMMARY FOR DATABATCH - /chem1/finn5.i/10AUG10.b

Instrument: finn5.i Date: 10-AUG-2010 Method: s8260b.m

INITIAL CAL: 23-JUL-2010

| Compound | %RSD or R ² |
|------------|------------------------|
| ----- | ----- |
| NO Q-FLAGS | |
| ----- | ----- |

CONTINUING CAL: 10-AUG-2010

| Compound | %D |
|---------------------|-------|
| ----- | ----- |
| Bromomethane | 39.0 |
| Iodomethane | -28.6 |
| 4-Chloro Toluene | 22.1 |
| 4-Isopropyl Toluene | 25.8 |
| N-Butyl Benzene | 30.4 |
| ----- | ----- |

Date : 10-AUG-2010 08:46

Client ID: BFB0810

Instrument: finn5.i

Sample Info: BFB0810,BFB0810,,1,10AUG10,,


Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

1 Bromofluorobenzene

118/106



| m/e | ION ABUNDANCE CRITERIA | % RELATIVE ABUNDANCE |
|-----|------------------------------------|----------------------|
| 95 | Base Peak, 100% relative abundance | 100.00 |
| 50 | 8.00 - 40.00% of mass 95 | 26.71 |
| 75 | 30.00 - 66.00% of mass 95 | 49.85 |
| 96 | 5.00 - 9.00% of mass 95 | 6.89 |
| 173 | Less than 2.00% of mass 174 | 0.17 < 0.24 |
| 174 | 50.00 - 101.00% of mass 95 | 70.44 |
| 175 | 4.00 - 9.00% of mass 174 | 5.11 < 7.25 |
| 176 | 93.00 - 101.00% of mass 174 | 68.29 < 96.96 |
| 177 | 5.00 - 9.00% of mass 176 | 4.54 < 6.65 |

Date : 10-AUG-2010 08:46

Client ID: BFB0810

Instrument: finn5.i

Sample Info: BFB0810,BFB0810,,1,10AUG10,,

Operator: PB

Column phase: RTX502.2

Column diameter: 0.18

Data File: BFB0810.d

Spectrum: Average Spectrum: 12.100 to 12.120 min. (SUB)

Location of Maximum: 95.00

Number of points: 50

| m/z | Y | m/z | Y | m/z | Y | m/z | Y |
|-------|------|-------|------|-------|-------|--------|------|
| 36.00 | 149 | 56.00 | 214 | 77.00 | 22 | 119.00 | 18 |
| 37.00 | 903 | 57.00 | 404 | 79.00 | 295 | 130.00 | 20 |
| 38.00 | 860 | 60.00 | 94 | 80.00 | 114 | 131.00 | 18 |
| 39.00 | 443 | 61.00 | 597 | 81.00 | 346 | 141.00 | 28 |
| 44.00 | 72 | 62.00 | 638 | 82.00 | 41 | 143.00 | 83 |
| 45.00 | 180 | 63.00 | 492 | 87.00 | 465 | 172.00 | 59 |
| 47.00 | 207 | 68.00 | 1423 | 88.00 | 427 | 173.00 | 21 |
| 48.00 | 64 | 69.00 | 1368 | 91.00 | 19 | 174.00 | 8672 |
| 49.00 | 687 | 70.00 | 69 | 92.00 | 252 | 175.00 | 629 |
| 50.00 | 3288 | 73.00 | 561 | 93.00 | 497 | 176.00 | 8408 |
| 51.00 | 985 | 74.00 | 1950 | 94.00 | 1400 | 177.00 | 559 |
| 52.00 | 18 | 75.00 | 6137 | 95.00 | 12312 | | |
| 55.00 | 36 | 76.00 | 563 | 96.00 | 848 | | |


Data File: /chem1/finns.i/10AUG10.b/BFB0810.d
Date: 10-AUG-2010 08:46
Client ID: BFB0810
Sample Info: BFB0810,BFB0810,,1,10AUG10,,

Instrument: finns.i

Column phase: RTX502.2

Operator: PB
Column diameter: 0.18

/chem1/finns.i/10AUG10.b/BFB0810.d/BFB0810.LG



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/10AUG10.b/0500810A.d
 Lab Smp Id: CC0810 Client Smp ID: VSTD050
 Inj Date : 10-AUG-2010 10:38
 Operator : PB Inst ID: finn5.i
 Smp Info : CC0810,5,5,0
 Misc Info : 10-
 Comment :
 Method : /chem1/finn5.i/10AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 11:38 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: voa.sub
 Target Version: 3.50
 Processing Host: cserv3

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | AMOUNTS | |
|---|-----------|-------|--------|---------|----------|-----------------|----------------|
| | | | | | | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 2.995 | 2.995 | (0.453) | 69539 | 50.0000 | 45.672 |
| 2 Chloromethane | 50 | 3.296 | 3.296 | (0.498) | 166930 | 50.0000 | 40.749 |
| 3 Vinyl Chloride | 62 | 3.407 | 3.407 | (0.515) | 157933 | 50.0000 | 48.753 |
| 4 Bromomethane | 94 | 3.899 | 3.899 | (0.590) | 122237 | 50.0000 | 69.481 |
| 5 Chloroethane | 64 | 3.970 | 3.970 | (0.600) | 105585 | 50.0000 | 49.909 |
| 6 Trichlorofluoromethane | 101 | 4.231 | 4.231 | (0.640) | 146352 | 50.0000 | 46.744 |
| 7 Acrolein | 56 | 4.613 | 4.613 | (0.698) | 92654 | 250.000 | 237.24 |
| 8 1,1,1-Trichloro-2,2,2-Trifluoroethane | 101 | 4.623 | 4.623 | (0.699) | 121656 | 50.0000 | 49.632 |
| 9 Acetone | 43 | 4.663 | 4.663 | (0.705) | 155626 | 250.000 | 236.83 |
| 10 1,1-Dichloroethene | 96 | 4.824 | 4.824 | (0.729) | 100144 | 50.0000 | 45.023 |
| 11 Bromoethane | 108 | 5.045 | 5.045 | (0.763) | 66725 | 50.0000 | 40.509 |
| 12 Iodomethane | 142 | 5.146 | 5.146 | (0.778) | 93936 | 50.0000 | 35.719 |
| 13 Methylene Chloride | 84 | 5.266 | 5.266 | (0.796) | 108037 | 50.0000 | 43.137 |
| 14 Acrylonitrile | 53 | 5.347 | 5.347 | (0.808) | 29916 | 50.0000 | 51.564 (Q) |

| Compounds | QUANT SIG | | AMOUNTS | | | | |
|------------------------------|-----------|--------|---------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | 5.387 | 5.387 | (0.815) | 148921 | 50.0000 | 43.538 (Q) |
| 15 Carbon Disulfide | 76 | 5.367 | 5.367 | (0.812) | 281605 | 50.0000 | 40.821 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.548 | 5.548 | (0.839) | 91632 | 50.0000 | 48.340 |
| 18 Vinyl Acetate | 43 | 5.869 | 5.869 | (0.888) | 176952 | 50.0000 | 53.299 |
| 19 1,1-Dichloroethane | 63 | 5.919 | 5.919 | (0.895) | 173721 | 50.0000 | 49.817 |
| 20 2-Butanone | 43 | 6.271 | 6.271 | (0.948) | 193802 | 250.000 | 262.11 |
| 21 2,2-Dichloropropane | 77 | 6.442 | 6.442 | (0.974) | 95006 | 50.0000 | 44.524 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.482 | 6.482 | (0.980) | 81737 | 50.0000 | 48.924 |
| * 23 Pentafluorobenzene | 168 | 6.613 | 6.613 | (1.000) | 117420 | 50.0000 | |
| 24 Chloroform | 83 | 6.633 | 6.633 | (1.003) | 137383 | 50.0000 | 48.501 |
| 26 Bromochloromethane | 128 | 6.794 | 6.794 | (1.027) | 36260 | 50.0000 | 45.713 |
| \$ 25 Dibromofluoromethane | 111 | 6.834 | 6.834 | (1.033) | 64083 | 50.0000 | 45.791 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.025 | 7.025 | (1.062) | 98355 | 50.0000 | 44.644 |
| 29 1,1-Dichloropropene | 75 | 7.166 | 7.166 | (0.941) | 112667 | 50.0000 | 49.411 |
| 30 Carbon Tetrachloride | 117 | 7.276 | 7.276 | (0.955) | 90144 | 50.0000 | 45.462 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.296 | 7.296 | (1.103) | 69688 | 50.0000 | 45.508 |
| 32 1,2-Dichloroethane | 62 | 7.377 | 7.377 | (0.968) | 98291 | 50.0000 | 49.103 |
| 33 Benzene | 78 | 7.427 | 7.427 | (0.975) | 277370 | 50.0000 | 50.305 |
| * 34 1,4-Difluorobenzene | 114 | 7.618 | 7.618 | (1.000) | 167913 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.000 | 8.000 | (1.050) | 79016 | 50.0000 | 48.912 |
| 36 1,2-Dichloropropane | 63 | 8.161 | 8.161 | (1.071) | 82411 | 50.0000 | 47.414 |
| 37 Bromodichloromethane | 83 | 8.392 | 8.392 | (1.102) | 90281 | 50.0000 | 48.582 |
| 39 Dibromomethane | 93 | 8.462 | 8.462 | (1.111) | 42927 | 50.0000 | 49.753 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.613 | 8.613 | (1.131) | 33941 | 50.0000 | 55.760 |
| 41 4-Methyl-2-Pentanone | 58 | 8.643 | 8.643 | (1.135) | 107881 | 250.000 | 243.04 |
| 42 Cis 1,3-dichloropropene | 75 | 8.894 | 8.894 | (1.168) | 104648 | 50.0000 | 51.579 |
| \$ 43 d8-Toluene | 98 | 9.176 | 9.176 | (1.204) | 188908 | 50.0000 | 51.201 |
| 44 Toluene | 92 | 9.256 | 9.256 | (1.215) | 156489 | 50.0000 | 47.835 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.387 | 9.387 | (1.232) | 83465 | 50.0000 | 48.942 |
| 46 2-Hexanone | 43 | 9.517 | 9.517 | (0.883) | 264492 | 250.000 | 235.25 |
| 47 1,1,2-Trichloroethane | 97 | 9.568 | 9.568 | (1.256) | 50813 | 50.0000 | 49.892 |
| 48 1,3-Dichloropropane | 76 | 9.829 | 9.829 | (0.912) | 97684 | 50.0000 | 50.462 |
| 49 Tetrachloroethene | 166 | 9.949 | 9.949 | (0.924) | 72963 | 50.0000 | 47.748 |
| 50 Chlorodibromomethane | 129 | 10.150 | 10.150 | (0.942) | 62942 | 50.0000 | 48.333 |
| 51 1,2-Dibromoethane | 107 | 10.382 | 10.382 | (1.363) | 53668 | 50.0000 | 49.196 |
| * 52 d5-Chlorobenzene | 117 | 10.774 | 10.774 | (1.000) | 137539 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.814 | 10.814 | (1.004) | 157888 | 50.0000 | 48.943 |
| 54 Ethyl Benzene | 91 | 10.854 | 10.854 | (1.007) | 291716 | 50.0000 | 53.474 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.844 | 10.844 | (1.007) | 52454 | 50.0000 | 42.484 |
| 56 m,p-xylene | 106 | 10.934 | 10.934 | (1.015) | 224544 | 100.000 | 112.61 |
| 57 o-Xylene | 106 | 11.417 | 11.417 | (1.060) | 107750 | 50.0000 | 51.995 |
| 58 Styrene | 104 | 11.447 | 11.447 | (1.062) | 179504 | 50.0000 | 56.022 |
| 59 Isopropyl Benzene | 105 | 11.799 | 11.799 | (0.877) | 284060 | 50.0000 | 56.527 |
| 60 Bromoform | 173 | 11.859 | 11.859 | (0.881) | 38440 | 50.0000 | 47.576 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.980 | 11.980 | (0.890) | 69489 | 50.0000 | 47.864 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.100 | 12.100 | (1.123) | 79821 | 50.0000 | 49.588 |
| 63 1,2,3-Trichloropropane | 110 | 12.150 | 12.150 | (0.903) | 13852 | 50.0000 | 48.162 |

| Compounds | QUANT SIG | | | AMOUNTS | | | |
|--------------------------------|-----------|--------|--------|---------|----------|--------------------|-------------------|
| | MASS | RT | EXP RT | REL RT | RESPONSE | CAL-AMT (ug/Kg) | ON-COL (ug/Kg) |
| ===== | ==== | == | ===== | ===== | ===== | ===== | ===== |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.201 | 12.201 | (0.907) | 25643 | 50.0000 | 57.468 |
| 66 N-Propyl Benzene | 91 | 12.251 | 12.251 | (0.910) | 357990 | 50.0000 | 55.185 |
| 67 Bromobenzene | 156 | 12.341 | 12.341 | (0.917) | 70424 | 50.0000 | 50.271 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.422 | 12.422 | (0.923) | 241420 | 50.0000 | 59.183 |
| 69 2-Chloro Toluene | 91 | 12.482 | 12.482 | (0.928) | 223508 | 50.0000 | 52.436 |
| 70 4-Chloro Toluene | 91 | 12.532 | 12.532 | (0.931) | 249450 | 50.0000 | 61.052 |
| 71 T-Butyl Benzene | 119 | 12.834 | 12.834 | (0.954) | 205471 | 50.0000 | 58.878 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.884 | 12.884 | (0.957) | 240259 | 50.0000 | 59.830 |
| 73 S-Butyl Benzene | 105 | 13.085 | 13.085 | (0.972) | 327972 | 50.0000 | 57.125 |
| 74 4-Isopropyl Toluene | 119 | 13.226 | 13.226 | (0.983) | 247784 | 50.0000 | 62.898 |
| 75 1,3-Dichlorobenzene | 146 | 13.377 | 13.377 | (0.994) | 138038 | 50.0000 | 57.675 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.457 | 13.457 | (1.000) | 74652 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.497 | 13.497 | (1.003) | 136656 | 50.0000 | 57.060 |
| 78 N-Butyl Benzene | 91 | 13.708 | 13.708 | (1.019) | 277283 | 50.0000 | 65.182 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.899 | 13.899 | (1.033) | 67527 | 50.0000 | 49.730 |
| 80 1,2-Dichlorobenzene | 146 | 13.929 | 13.929 | (1.035) | 123289 | 50.0000 | 54.202 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.834 | 14.834 | (1.102) | 12090 | 50.0000 | 48.126 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.879 | 15.879 | (1.180) | 80300 | 50.0000 | 58.012 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.040 | 16.040 | (1.192) | 49970 | 50.0000 | 53.600 |
| 84 Naphthalene | 128 | 16.211 | 16.211 | (1.205) | 130926 | 50.0000 | 52.148 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.502 | 16.502 | (1.226) | 69204 | 50.0000 | 52.294 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.
INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: finn5.i
Lab File ID: 0500810A.d
Lab Smp Id: CC0810
Analysis Type: VOA
Quant Type: ISTD
Operator: PB
Method File: /chem1/finn5.i/10AUG10.b/s8260b.m
Misc Info: 10-

Calibration Date: 10-AUG-2010
Calibration Time: 10:38
Client Smp ID: VSTD050
Level: LOW
Sample Type: SOIL

Test Mode:

Use Initial Calibration Level 5.
If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzon | 131115 | 65558 | 262230 | 117420 | -10.45 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 167913 | -12.34 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 137539 | -14.68 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 74652 | -15.44 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzon | 6.62 | 6.12 | 7.12 | 6.61 | -0.15 |
| 34 1,4-Difluorobenze | 7.63 | 7.13 | 8.13 | 7.62 | -0.13 |
| 52 d5-Chlorobenzene | 10.78 | 10.28 | 11.28 | 10.77 | -0.09 |
| 76 d4-1,4-Dichlorobe | 13.47 | 12.97 | 13.97 | 13.46 | -0.07 |

AREA UPPER LIMIT = +100% of internal standard area.
AREA LOWER LIMIT = - 50% of internal standard area.
RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: finn5.i Injection Date: 10-AUG-2010 10:38
 Lab File ID: 0500810A.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
 Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
 Lab Sample ID: CC0810 Quant Type: ISTD
 Method: /chem1/finn5.i/10AUG10.b/s8260b.m

| COMPOUND | RRF / AMOUNT | RF50 | MIN | | MAX | | CURVE TYPE |
|-------------------------------|--------------|---------|-------|-------------|-------------|----------|------------|
| | | | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 1 Dichlorodifluoromethane | 0.64835 | 0.59222 | 0.010 | -8.65651 | 20.00000 | Averaged | |
| 2 Chloromethane | 1.74440 | 1.42165 | 0.100 | -18.50218 | 20.00000 | Averaged | |
| 3 Vinyl Chloride | 1.37944 | 1.34503 | 0.010 | -2.49476 | 20.00000 | Averaged | |
| 4 Bromomethane | 0.74914 | 1.04102 | 0.010 | 38.96278 | 20.00000 | Averaged | <- |
| 5 Chloroethane | 0.90084 | 0.89921 | 0.010 | -0.18161 | 20.00000 | Averaged | |
| 6 Trichlorofluoromethane | 1.33321 | 1.24640 | 0.010 | -6.51158 | 20.00000 | Averaged | |
| 7 Acrolein | 0.16631 | 0.15782 | 0.010 | -5.10476 | 20.00000 | Averaged | |
| 8 112Trichloro122Trifluoroeth | 1.04376 | 1.03608 | 0.010 | -0.73609 | 20.00000 | Averaged | |
| 9 Acetone | 0.27982 | 0.26508 | 0.010 | -5.26756 | 20.00000 | Averaged | |
| 10 1,1-Dichloroethene | 0.94715 | 0.85287 | 0.010 | -9.95388 | 20.00000 | Averaged | |
| 11 Bromoethane | 0.70140 | 0.56826 | 0.010 | -18.98272 | 20.00000 | Averaged | |
| 12 Iodomethane | 1.11986 | 0.80000 | 0.010 | -28.56224 | 20.00000 | Averaged | <- |
| 13 Methylene Chloride | 1.06648 | 0.92009 | 0.010 | -13.72662 | 20.00000 | Averaged | |
| 14 Acrylonitrile | 0.24705 | 0.25478 | 0.010 | 3.12737 | 20.00000 | Averaged | |
| 16 Methyl tert-Butyl Ether | 1.45653 | 1.26828 | 0.010 | -12.92468 | 20.00000 | Averaged | |
| 15 Carbon Disulfide | 2.93755 | 2.39827 | 0.010 | -18.35806 | 20.00000 | Averaged | |
| 17 Trans-1,2-Dichloroethene | 0.80717 | 0.78038 | 0.010 | -3.31967 | 20.00000 | Averaged | |
| 18 Vinyl Acetate | 1.41371 | 1.50700 | 0.010 | 6.59872 | 20.00000 | Averaged | |
| 19 1,1-Dichloroethane | 1.48492 | 1.47948 | 0.100 | -0.36626 | 20.00000 | Averaged | |
| 20 2-Butanone | 0.31485 | 0.33010 | 0.010 | 4.84363 | 20.00000 | Averaged | |
| 21 2,2-Dichloropropane | 0.90863 | 0.80911 | 0.010 | -10.95265 | 20.00000 | Averaged | |
| 22 Cis-1,2-Dichloroethene | 0.71142 | 0.69611 | 0.010 | -2.15227 | 20.00000 | Averaged | |
| 24 Chloroform | 1.20617 | 1.17001 | 0.010 | -2.99745 | 20.00000 | Averaged | |
| 26 Bromochloromethane | 0.33777 | 0.30881 | 0.010 | -8.57447 | 20.00000 | Averaged | |
| \$ 25 Dibromofluoromethane | 0.59593 | 0.54576 | 0.010 | -8.41860 | 20.00000 | Averaged | |
| 27 1,1,1-Trichloroethane | 0.93813 | 0.83763 | 0.010 | -10.71248 | 20.00000 | Averaged | |
| 29 1,1-Dichloropropene | 0.67899 | 0.67098 | 0.010 | -1.17837 | 20.00000 | Averaged | |
| 30 Carbon Tetrachloride | 0.59044 | 0.53685 | 0.010 | -9.07603 | 20.00000 | Averaged | |
| \$ 31 d4-1,2-Dichloroethane | 0.65208 | 0.59349 | 0.010 | -8.98414 | 20.00000 | Averaged | |
| 32 1,2-Dichloroethane | 0.59607 | 0.58537 | 0.010 | -1.79458 | 20.00000 | Averaged | |
| 33 Benzene | 1.64186 | 1.65187 | 0.010 | 0.60939 | 20.00000 | Averaged | |
| 35 Trichloroethene | 0.48104 | 0.47058 | 0.010 | -2.17569 | 20.00000 | Averaged | |
| 36 1,2-Dichloropropane | 0.51756 | 0.49080 | 0.010 | -5.17133 | 20.00000 | Averaged | |
| 37 Bromodichloromethane | 0.55335 | 0.53767 | 0.010 | -2.83530 | 20.00000 | Averaged | |
| 39 Dibromomethane | 0.25692 | 0.25565 | 0.010 | -0.49363 | 20.00000 | Averaged | |

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: finn5.i Injection Date: 10-AUG-2010 10:38
 Lab File ID: 0500810A.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
 Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
 Lab Sample ID: CC0810 Quant Type: ISTD
 Method: /chem1/finn5.i/10AUG10.b/s8260b.m

| COMPOUND | RF50 | | MIN | | MAX | | CURVE TYPE |
|--------------------------------|--------------|---------|-------|-------------|-------------|-------------|------------|
| | RRF / AMOUNT | RF50 | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 40 2-Chloroethyl Vinyl Ether | 0.18125 | 0.20213 | 0.001 | 11.52071 | 20.00000 | Averaged | |
| 41 4-Methyl-2-Pentanone | 0.13218 | 0.12850 | 0.010 | -2.78338 | 20.00000 | Averaged | |
| 42 Cis 1,3-dichloropropene | 0.60415 | 0.62323 | 0.010 | 3.15779 | 20.00000 | Averaged | |
| 43 d8-Toluene | 1.09864 | 1.12503 | 0.010 | 2.40270 | 20.00000 | Averaged | |
| 44 Toluene | 0.97414 | 0.93196 | 0.010 | -4.32961 | 20.00000 | Averaged | |
| 45 Trans 1,3-Dichloropropene | 0.50782 | 0.49707 | 0.010 | -2.11624 | 20.00000 | Averaged | |
| 46 2-Hexanone | 0.40872 | 0.38461 | 0.010 | -5.90037 | 20.00000 | Averaged | |
| 47 1,1,2-Trichloroethane | 0.30327 | 0.30262 | 0.010 | -0.21518 | 20.00000 | Averaged | |
| 48 1,3-Dichloropropane | 0.70372 | 0.71023 | 0.010 | 0.92406 | 20.00000 | Averaged | |
| 49 Tetrachloroethene | 0.55550 | 0.53049 | 0.010 | -4.50280 | 20.00000 | Averaged | |
| 50 Chlorodibromomethane | 0.47341 | 0.45763 | 0.010 | -3.33311 | 20.00000 | Averaged | |
| 51 1,2-Dibromoethane | 0.32484 | 0.31962 | 0.010 | -1.60709 | 20.00000 | Averaged | |
| 53 Chlorobenzene | 1.17275 | 1.14795 | 0.300 | -2.11431 | 20.00000 | Averaged | |
| 54 Ethyl Benzene | 1.98319 | 2.12097 | 0.010 | 6.94713 | 20.00000 | Averaged | |
| 55 1,1,1,2-Tetrachloroethane | 0.44884 | 0.38138 | 0.010 | -15.03091 | 20.00000 | Averaged | |
| 56 m,p-xylene | 0.72486 | 0.81629 | 0.010 | 12.61410 | 20.00000 | Averaged | |
| 57 o-Xylene | 0.75335 | 0.78341 | 0.010 | 3.99055 | 20.00000 | Averaged | |
| 58 Styrene | 1.16482 | 1.30511 | 0.010 | 12.04394 | 20.00000 | Averaged | |
| 59 Isopropyl Benzene | 3.36576 | 3.80512 | 0.010 | 13.05404 | 20.00000 | Averaged | |
| 60 Bromoform | 0.54116 | 0.51492 | 0.100 | -4.84755 | 20.00000 | Averaged | |
| 61 1,1,1,2,2-Tetrachloroethane | 0.97237 | 0.93084 | 0.300 | -4.27157 | 20.00000 | Averaged | |
| 62 4-Bromofluorobenzene | 0.58517 | 0.58035 | 0.010 | -0.82316 | 20.00000 | Averaged | |
| 63 1,2,3-Trichloropropane | 0.19264 | 0.18555 | 0.010 | -3.67662 | 20.00000 | Averaged | |
| 65 Trans-1,4-Dichloro 2-Butene | 0.29886 | 0.34350 | 0.010 | 14.93704 | 20.00000 | Averaged | |
| 66 N-Propyl Benzene | 4.34491 | 4.79545 | 0.010 | 10.36933 | 20.00000 | Averaged | |
| 67 Bromobenzene | 0.93828 | 0.94336 | 0.010 | 0.54188 | 20.00000 | Averaged | |
| 68 1,3,5-Trimethyl Benzene | 2.73214 | 3.23394 | 0.010 | 18.36656 | 20.00000 | Averaged | |
| 69 2-Chloro Toluene | 2.85492 | 2.99400 | 0.010 | 4.87157 | 20.00000 | Averaged | |
| 70 4-Chloro Toluene | 2.73658 | 3.34150 | 0.010 | 22.10498 | 20.00000 | Averaged <- | |
| 71 T-Butyl Benzene | 2.33736 | 2.75238 | 0.010 | 17.75592 | 20.00000 | Averaged | |
| 72 1,2,4-Trimethylbenzene | 2.68961 | 3.21839 | 0.010 | 19.65987 | 20.00000 | Averaged | |
| 73 S-Butyl Benzene | 3.84536 | 4.39335 | 0.010 | 14.25055 | 20.00000 | Averaged | |
| 74 4-Isopropyl Toluene | 2.63853 | 3.31919 | 0.010 | 25.79668 | 20.00000 | Averaged <- | |
| 75 1,3-Dichlorobenzene | 1.60301 | 1.84909 | 0.010 | 15.35072 | 20.00000 | Averaged | |
| 77 1,4-Dichlorobenzene | 1.60408 | 1.83057 | 0.010 | 14.11969 | 20.00000 | Averaged | |

Analytical Resources, Inc.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: finn5.i Injection Date: 10-AUG-2010 10:38
Lab File ID: 0500810A.d Init. Cal. Date(s): 23-JUL-2010 23-JUL-2010
Analysis Type: SOIL Init. Cal. Times: 17:18 20:28
Lab Sample ID: CC0810 Quant Type: ISTD
Method: /chem1/finn5.i/10AUG10.b/s8260b.m


| COMPOUND | ___ | | MIN | | MAX | | CURVE TYPE |
|--------------------------------|--------------|---------|-------|-------------|-------------|----------|------------|
| | RRF / AMOUNT | RF50 | RRF | %D / %DRIFT | %D / %DRIFT | | |
| 78 N-Butyl Benzene | 2.84923 | 3.71434 | 0.010 | 30.36306 | 20.00000 | Averaged | |
| \$ 79 d4-1,2-Dichlorobenzene | 0.90947 | 0.90456 | 0.010 | -0.53977 | 20.00000 | Averaged | |
| 80 1,2-Dichlorobenzene | 1.52349 | 1.65152 | 0.010 | 8.40341 | 20.00000 | Averaged | |
| 81 1,2-Dibromo 3-Chloropropane | 0.16826 | 0.16195 | 0.010 | -3.74745 | 20.00000 | Averaged | |
| 82 1,2,4-Trichlorobenzene | 0.92710 | 1.07566 | 0.010 | 16.02393 | 20.00000 | Averaged | |
| 83 Hexachloro 1,3-Butadiene | 0.62441 | 0.66937 | 0.010 | 7.20047 | 20.00000 | Averaged | |
| 84 Naphthalene | 1.68157 | 1.75382 | 0.010 | 4.29669 | 20.00000 | Averaged | |
| 85 1,2,3-Trichlorobenzene | 0.88636 | 0.92702 | 0.010 | 4.58772 | 20.00000 | Averaged | |

Data File: /chem1/finn5.i/10AUG10.b/0500810A.d
Date : 10-AUG-2010 10:38
Client ID: VSTD050
Sample Info: CC0810,5,5,0

Column phase: Rtx502.2

Instrument: finn5.i
Operator: PB
Column diameter: 0.18

/chem1/finn5.i/10AUG10.b/0500810A.d/0500810A.LC



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/10AUG10.b/LCS0810.d
 Lab Smp Id: LCS0810 Client Smp ID: LCS0810
 Inj Date : 10-AUG-2010 11:12
 Operator : PB Inst ID: finn5.i
 Smp Info : LCS0810,5,5,0
 Misc Info : 10-18196
 Comment :
 Method : /chem1/finn5.i/10AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 15:05 patrickb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000 Compound Sublist: voa.sub
 Integrator: HP RTE
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature/initials: J 8/10/10

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.015 | 2.995 | (0.455) | 64342 | 43.5404 | 43.540 |
| 2 Chloromethane | 50 | 3.316 | 3.296 | (0.500) | 168769 | 42.4475 | 42.448 |
| 3 Vinyl Chloride | 62 | 3.427 | 3.407 | (0.517) | 150417 | 47.8410 | 47.841 |
| 4 Bromomethane | 94 | 3.919 | 3.899 | (0.591) | 110128 | 64.4973 | 64.497 |
| 5 Chloroethane | 64 | 3.990 | 3.970 | (0.602) | 101040 | 49.2096 | 49.210 |
| 6 Trichlorofluoromethane | 101 | 4.251 | 4.231 | (0.641) | 153087 | 50.3786 | 50.378 |
| 7 Acrolein | 56 | 4.633 | 4.613 | (0.698) | 97944 | 258.390 | 258.39 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.653 | 4.623 | (0.702) | 117468 | 49.3771 | 49.377 |
| 9 Acetone | 43 | 4.683 | 4.663 | (0.706) | 171039 | 268.182 | 268.18 |
| 10 1,1-Dichloroethene | 96 | 4.844 | 4.824 | (0.730) | 109289 | 50.6250 | 50.625 |
| 11 Bromoethane | 108 | 5.065 | 5.045 | (0.764) | 80282 | 50.2175 | 50.218 |
| 12 Iodomethane | 142 | 5.166 | 5.146 | (0.779) | 142800 | 55.9464 | 55.946 |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.795) | 107768 | 44.3346 | 44.334 |
| 14 Acrylonitrile | 53 | 5.367 | 5.347 | (0.809) | 32991 | 58.5887 | 58.589 (Q) |

| Compounds | QUANT SIG | MASS | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|------|--------|--------|---------|----------|-------------------|---------------|
| | | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | | 73 | 5.407 | 5.387 | (0.815) | 155096 | 46.7184 | 46.718 (Q) |
| 15 Carbon Disulfide | | 76 | 5.387 | 5.367 | (0.812) | 363482 | 54.2880 | 54.288 |
| 17 Trans-1,2-Dichloroethene | | 96 | 5.568 | 5.548 | (0.839) | 94021 | 51.1051 | 51.105 |
| 18 Vinyl Acetate | | 43 | 5.889 | 5.869 | (0.888) | 183716 | 57.0153 | 57.015 |
| 19 1,1-Dichloroethane | | 63 | 5.950 | 5.919 | (0.897) | 176001 | 52.0017 | 52.002 |
| 20 2-Butanone | | 43 | 6.291 | 6.271 | (0.948) | 204819 | 285.412 | 285.41 |
| 21 2,2-Dichloropropane | | 77 | 6.462 | 6.442 | (0.974) | 94841 | 45.7946 | 45.795 |
| 22 Cis-1,2-Dichloroethene | | 96 | 6.502 | 6.482 | (0.980) | 85027 | 52.4369 | 52.437 |
| * 23 Pentafluorobenzene | | 168 | 6.633 | 6.613 | (1.000) | 113963 | 50.0000 | |
| 24 Chloroform | | 83 | 6.653 | 6.633 | (1.003) | 136615 | 49.6932 | 49.693 |
| 26 Bromochloromethane | | 128 | 6.814 | 6.794 | (1.027) | 39559 | 51.3846 | 51.385 |
| \$ 25 Dibromofluoromethane | | 111 | 6.854 | 6.834 | (1.033) | 69725 | 51.3335 | 51.334 (Q) |
| 27 1,1,1-Trichloroethane | | 97 | 7.045 | 7.025 | (1.062) | 98466 | 46.0499 | 46.050 |
| 29 1,1-Dichloropropene | | 75 | 7.186 | 7.166 | (0.940) | 114851 | 49.5109 | 49.511 |
| 30 Carbon Tetrachloride | | 117 | 7.296 | 7.276 | (0.954) | 91523 | 45.3714 | 45.371 |
| \$ 31 d4-1,2-Dichloroethane | | 65 | 7.316 | 7.296 | (1.103) | 79635 | 53.5811 | 53.581 |
| 32 1,2-Dichloroethane | | 62 | 7.407 | 7.377 | (0.968) | 100418 | 49.3110 | 49.311 |
| 33 Benzene | | 78 | 7.447 | 7.427 | (0.974) | 280556 | 50.0160 | 50.016 |
| * 34 1,4-Difluorobenzene | | 114 | 7.648 | 7.618 | (1.000) | 170822 | 50.0000 | |
| 35 Trichloroethene | | 95 | 8.020 | 8.000 | (1.049) | 79578 | 48.4212 | 48.421 |
| 36 1,2-Dichloropropane | | 63 | 8.181 | 8.161 | (1.070) | 83113 | 47.0039 | 47.004 |
| 37 Bromodichloromethane | | 83 | 8.412 | 8.392 | (1.100) | 91360 | 48.3258 | 48.326 |
| 39 Dibromomethane | | 93 | 8.482 | 8.462 | (1.109) | 43774 | 49.8709 | 49.871 |
| 40 2-Chloroethyl Vinyl Ether | | 63 | 8.633 | 8.613 | (1.129) | 34860 | 56.2949 | 56.295 (Q) |
| 41 4-Methyl-2-Pentanone | | 58 | 8.663 | 8.643 | (1.133) | 117093 | 259.303 | 259.30 |
| 42 Cis 1,3-dichloropropene | | 75 | 8.914 | 8.894 | (1.166) | 105152 | 50.9447 | 50.945 |
| \$ 43 d8-Toluene | | 98 | 9.196 | 9.176 | (1.202) | 192194 | 51.2049 | 51.205 |
| 44 Toluene | | 92 | 9.276 | 9.256 | (1.213) | 157738 | 47.3959 | 47.396 |
| 45 Trans 1,3-Dichloropropene | | 75 | 9.407 | 9.387 | (1.230) | 86370 | 49.7828 | 49.783 |
| 46 2-Hexanone | | 43 | 9.537 | 9.517 | (0.884) | 284412 | 237.053 | 237.05 |
| 47 1,1,2-Trichloroethane | | 97 | 9.588 | 9.568 | (1.254) | 52263 | 50.4423 | 50.442 |
| 48 1,3-Dichloropropane | | 76 | 9.849 | 9.829 | (0.912) | 100608 | 48.7031 | 48.703 |
| 49 Tetrachloroethene | | 166 | 9.970 | 9.949 | (0.924) | 70655 | 43.3295 | 43.329 |
| 50 Chlorodibromomethane | | 129 | 10.171 | 10.150 | (0.942) | 63658 | 45.8082 | 45.808 |
| 51 1,2-Dibromoethane | | 107 | 10.402 | 10.382 | (1.360) | 55317 | 49.8445 | 49.844 |
| * 52 d5-Chlorobenzene | | 117 | 10.794 | 10.774 | (1.000) | 146772 | 50.0000 | |
| 53 Chlorobenzene | | 112 | 10.834 | 10.814 | (1.004) | 159696 | 46.3892 | 46.389 |
| 54 Ethyl Benzene | | 91 | 10.864 | 10.854 | (1.007) | 289400 | 49.7119 | 49.712 |
| 55 1,1,1,2-Tetrachloroethane | | 131 | 10.864 | 10.844 | (1.007) | 53746 | 40.7926 | 40.792 |
| 56 m,p-xylene | | 106 | 10.944 | 10.934 | (1.014) | 223430 | 105.006 | 105.01 |
| 57 o-Xylene | | 106 | 11.437 | 11.417 | (1.060) | 110179 | 49.8228 | 49.823 |
| 58 Styrene | | 104 | 11.467 | 11.447 | (1.062) | 182034 | 53.2377 | 53.238 |
| 59 Isopropyl Benzene | | 105 | 11.819 | 11.799 | (0.877) | 288073 | 53.0018 | 53.002 |
| 60 Bromoform | | 173 | 11.879 | 11.859 | (0.881) | 40208 | 46.0109 | 46.011 |
| 61 1,1,2,2-Tetrachloroethane | | 83 | 12.000 | 11.980 | (0.890) | 74485 | 47.4357 | 47.436 |
| \$ 62 4-Bromofluorobenzene | | 95 | 12.120 | 12.100 | (1.123) | 84603 | 49.2529 | 49.253 |
| 63 1,2,3-Trichloropropane | | 110 | 12.171 | 12.150 | (0.903) | 15140 | 48.6695 | 48.670 (Q) |

| Compounds | QUANT SIG | | | | RESPONSE | CONCENTRATIONS | |
|--------------------------------|-----------|--------|--------|---------|----------|----------------------|------------------|
| | MASS | RT | EXP RT | REL RT | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 65 Trans-1,4-Dichloro 2-Butene | 53 | 12.221 | 12.201 | (0.907) | 27118 | 56.1902 | 56.190 |
| 66 N-Propyl Benzene | 91 | 12.271 | 12.251 | (0.910) | 360053 | 51.3164 | 51.316 |
| 67 Bromobenzene | 156 | 12.361 | 12.341 | (0.917) | 71681 | 47.3088 | 47.309 |
| 68 1,3,5-Trimethyl Benzene | 105 | 12.442 | 12.422 | (0.923) | 245019 | 55.5351 | 55.535 |
| 69 2-Chloro Toluene | 91 | 12.502 | 12.482 | (0.928) | 226268 | 49.0795 | 49.079 |
| 70 4-Chloro Toluene | 91 | 12.552 | 12.532 | (0.931) | 248079 | 56.1373 | 56.137 |
| 71 T-Butyl Benzene | 119 | 12.854 | 12.834 | (0.954) | 208379 | 55.2075 | 55.208 |
| 72 1,2,4-Trimethylbenzene | 105 | 12.904 | 12.884 | (0.957) | 244388 | 56.2679 | 56.268 |
| 73 S-Butyl Benzene | 105 | 13.105 | 13.085 | (0.972) | 330803 | 53.2725 | 53.272 |
| 74 4-Isopropyl Toluene | 119 | 13.246 | 13.226 | (0.983) | 249945 | 58.6614 | 58.661 |
| 75 1,3-Dichlorobenzene | 146 | 13.397 | 13.377 | (0.994) | 139293 | 53.8100 | 53.810 |
| * 76 d4-1,4-Dichlorobenzene | 152 | 13.477 | 13.457 | (1.000) | 80742 | 50.0000 | |
| 77 1,4-Dichlorobenzene | 146 | 13.517 | 13.497 | (1.003) | 137054 | 52.9097 | 52.910 |
| 78 N-Butyl Benzene | 91 | 13.728 | 13.708 | (1.019) | 278627 | 60.5573 | 60.557 |
| \$ 79 d4-1,2-Dichlorobenzene | 152 | 13.919 | 13.899 | (1.033) | 73916 | 50.3295 | 50.329 |
| 80 1,2-Dichlorobenzene | 146 | 13.949 | 13.929 | (1.035) | 125037 | 50.8240 | 50.824 |
| 81 1,2-Dibromo 3-Chloropropane | 75 | 14.854 | 14.834 | (1.102) | 12933 | 47.5989 | 47.599 |
| 82 1,2,4-Trichlorobenzene | 180 | 15.899 | 15.879 | (1.180) | 80090 | 53.4961 | 53.496 |
| 83 Hexachloro 1,3-Butadiene | 225 | 16.060 | 16.040 | (1.192) | 51907 | 51.4784 | 51.478 |
| 84 Naphthalene | 128 | 16.231 | 16.211 | (1.204) | 139384 | 51.3298 | 51.330 |
| 85 1,2,3-Trichlorobenzene | 180 | 16.522 | 16.502 | (1.226) | 71247 | 49.7769 | 49.777 |

QC Flag Legend

Q - Qualifier signal failed the ratio test.

Analytical Resources, Inc.

INTERNAL STANDARD COMPOUNDS
 AREA AND RT SUMMARY

Instrument ID: finn5.i
 Lab File ID: LCS0810.d
 Lab Smp Id: LCS0810
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: PB
 Method File: /chem1/finn5.i/10AUG10.b/s8260b.m
 Misc Info: 10-18196

Calibration Date: 10-AUG-2010
 Calibration Time: 10:38
 Client Smp ID: LCS0810
 Level: LOW
 Sample Type: SOIL

Test Mode: Use Initial Calibration Level 5.
 If Continuing Cal. use Initial Cal. Level 5

| COMPOUND | STANDARD | AREA LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|------------|--------|--------|--------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 131115 | 65558 | 262230 | 113963 | -13.08 |
| 34 1,4-Difluorobenze | 191559 | 95780 | 383118 | 170822 | -10.83 |
| 52 d5-Chlorobenzene | 161199 | 80600 | 322398 | 146772 | -8.95 |
| 76 d4-1,4-Dichlorobe | 88279 | 44140 | 176558 | 80742 | -8.54 |

| COMPOUND | STANDARD | RT LIMIT | | SAMPLE | %DIFF |
|----------------------|----------|----------|-------|--------|-------|
| | | LOWER | UPPER | | |
| 23 Pentafluorobenzen | 6.61 | 6.11 | 7.11 | 6.63 | 0.30 |
| 34 1,4-Difluorobenze | 7.62 | 7.12 | 8.12 | 7.65 | 0.40 |
| 52 d5-Chlorobenzene | 10.77 | 10.27 | 11.27 | 10.79 | 0.19 |
| 76 d4-1,4-Dichlorobe | 13.46 | 12.96 | 13.96 | 13.48 | 0.15 |

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = - 50% of internal standard area.
 RT UPPER LIMIT = + 0.50 minutes of internal standard RT.
 RT LOWER LIMIT = - 0.50 minutes of internal standard RT.

Analytical Resources, Inc.

RECOVERY REPORT

Client Name:
 Sample Matrix: SOLID
 Lab Smp Id: LCS0810
 Level: LOW
 Data Type: MS DATA
 SpikeList File: all.spk
 Sublist File: voa.sub
 Method File: /chem1/finn5.i/10AUG10.b/s8260b.m
 Misc Info: 10-18196

Client SDG: 10AUG10
 Fraction: VOA
 Client Smp ID: LCS0810
 Operator: PB
 SampleType: LCS
 Quant Type: ISTD

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|-----------------------|------------------------|----------------------------|----------------|--------|
| 1 Dichlorodifluorome | 50.000 | 43.540 | 87.08 | 53-148 |
| 2 Chloromethane | 50.000 | 42.448 | 84.90 | 64-125 |
| 3 Vinyl Chloride | 50.000 | 47.841 | 95.68 | 63-137 |
| 4 Bromomethane | 50.000 | 64.497 | 128.99 | 57-136 |
| 5 Chloroethane | 50.000 | 49.210 | 98.42 | 64-131 |
| 6 Trichlorofluoromet | 50.000 | 50.378 | 100.76 | 69-132 |
| 7 Acrolein | 250.00 | 258.39 | 103.36 | 54-137 |
| 8 112Trichloro122Tri | 50.000 | 49.377 | 98.75 | 74-130 |
| 9 Acetone | 250.00 | 268.18 | 107.27 | 60-131 |
| 10 1,1-Dichloroethene | 50.000 | 50.625 | 101.25 | 75-126 |
| 11 Bromoethane | 50.000 | 50.218 | 100.44 | 76-126 |
| 12 Iodomethane | 50.000 | 55.946 | 111.89 | 65-139 |
| 13 Methylene Chloride | 50.000 | 44.334 | 88.67 | 70-123 |
| 15 Carbon Disulfide | 50.000 | 54.288 | 108.58 | 71-129 |
| 14 Acrylonitrile | 50.000 | 58.589 | 117.18 | 67-125 |
| 16 Methyl tert-Butyl | 50.000 | 46.718 | 93.44 | 70-120 |
| 17 Trans-1,2-Dichloro | 50.000 | 51.105 | 102.21 | 80-120 |
| 18 Vinyl Acetate | 50.000 | 57.015 | 114.03 | 60-136 |
| 19 1,1-Dichloroethane | 50.000 | 52.002 | 104.00 | 80-120 |
| 20 2-Butanone | 250.00 | 285.41 | 114.16 | 70-120 |
| 21 2,2-Dichloropropan | 50.000 | 45.795 | 91.59 | 74-123 |
| 22 Cis-1,2-Dichloroet | 50.000 | 52.437 | 104.87 | 80-120 |
| 24 Chloroform | 50.000 | 49.693 | 99.39 | 80-120 |
| 26 Bromochloromethane | 50.000 | 51.385 | 102.77 | 80-120 |
| 27 1,1,1-Trichloroeth | 50.000 | 46.050 | 92.10 | 77-121 |
| 29 1,1-Dichloropropen | 50.000 | 49.511 | 99.02 | 80-120 |
| 30 Carbon Tetrachlori | 50.000 | 45.371 | 90.74 | 77-122 |
| 32 1,2-Dichloroethane | 50.000 | 49.311 | 98.62 | 76-120 |
| 33 Benzene | 50.000 | 50.016 | 100.03 | 80-120 |
| 35 Trichloroethene | 50.000 | 48.421 | 96.84 | 80-120 |
| 36 1,2-Dichloropropan | 50.000 | 47.004 | 94.01 | 80-120 |
| 37 Bromodichlorometha | 50.000 | 48.326 | 96.65 | 77-121 |
| 39 Dibromomethane | 50.000 | 49.871 | 99.74 | 80-120 |

| SPIKE COMPOUND | CONC ADDED ug/Kg | CONC RECOVERED ug/Kg | % RECOVERED | LIMITS |
|------------------------|------------------------|----------------------------|----------------|--------|
| 40 2-Chloroethyl Vinyl | 50.000 | 56.295 | 112.59 | 10-191 |
| 41 4-Methyl-2-Pentano | 250.00 | 259.30 | 103.72 | 67-120 |
| 42 Cis 1,3-dichloropr | 50.000 | 50.945 | 101.89 | 74-120 |
| 44 Toluene | 50.000 | 47.396 | 94.79 | 80-120 |
| 45 Trans 1,3-Dichloro | 50.000 | 49.783 | 99.57 | 65-120 |
| 46 2-Hexanone | 250.00 | 237.05 | 94.82 | 65-130 |
| 47 1,1,2-Trichloroeth | 50.000 | 50.442 | 100.88 | 80-120 |
| 48 1,3-Dichloropropan | 50.000 | 48.703 | 97.41 | 80-120 |
| 49 Tetrachloroethene | 50.000 | 43.329 | 86.66 | 80-121 |
| 50 Chlorodibromometha | 50.000 | 45.808 | 91.62 | 64-120 |
| 51 1,2-Dibromoethane | 50.000 | 49.844 | 99.69 | 75-120 |
| 53 Chlorobenzene | 50.000 | 46.389 | 92.78 | 80-120 |
| 55 1,1,1,2-Tetrachlor | 50.000 | 40.792 | 81.59 | 69-121 |
| 54 Ethyl Benzene | 50.000 | 49.712 | 99.42 | 80-127 |
| 56 m,p-xylene | 100.00 | 105.01 | 105.01 | 80-125 |
| 57 o-Xylene | 50.000 | 49.823 | 99.65 | 78-120 |
| 58 Styrene | 50.000 | 53.238 | 106.48 | 80-123 |
| 59 Isopropyl Benzene | 50.000 | 53.002 | 106.00 | 80-127 |
| 60 Bromoform | 50.000 | 46.011 | 92.02 | 60-120 |
| 61 1,1,2,2-Tetrachlor | 50.000 | 47.436 | 94.87 | 74-120 |
| 63 1,2,3-Trichloropro | 50.000 | 48.670 | 97.34 | 72-121 |
| 65 Trans-1,4-Dichloro | 50.000 | 56.190 | 112.38 | 65-126 |
| 66 N-Propyl Benzene | 50.000 | 51.316 | 102.63 | 80-132 |
| 67 Bromobenzene | 50.000 | 47.309 | 94.62 | 80-120 |
| 68 1,3,5-Trimethyl Be | 50.000 | 55.535 | 111.07 | 80-125 |
| 69 2-Chloro Toluene | 50.000 | 49.079 | 98.16 | 80-125 |
| 70 4-Chloro Toluene | 50.000 | 56.137 | 112.27 | 80-127 |
| 71 T-Butyl Benzene | 50.000 | 55.208 | 110.42 | 87-122 |
| 72 1,2,4-Trimethylben | 50.000 | 56.268 | 112.54 | 80-126 |
| 73 S-Butyl Benzene | 50.000 | 53.272 | 106.54 | 80-134 |
| 74 4-Isopropyl Toluen | 50.000 | 58.661 | 117.32 | 80-131 |
| 75 1,3-Dichlorobenzen | 50.000 | 53.810 | 107.62 | 80-120 |
| 77 1,4-Dichlorobenzen | 50.000 | 52.910 | 105.82 | 80-120 |
| 78 N-Butyl Benzene | 50.000 | 60.557 | 121.11 | 80-138 |
| 80 1,2-Dichlorobenzen | 50.000 | 50.824 | 101.65 | 80-120 |
| 81 1,2-Dibromo 3-Chlo | 50.000 | 47.599 | 95.20 | 59-120 |
| 82 1,2,4-Trichloroben | 50.000 | 53.496 | 106.99 | 78-130 |
| 83 Hexachloro 1,3-But | 50.000 | 51.478 | 102.96 | 76-129 |
| 84 Naphthalene | 50.000 | 51.330 | 102.66 | 66-120 |
| 85 1,2,3-Trichloroben | 50.000 | 49.777 | 99.55 | 73-123 |

| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 25 Dibromofluorometha | 50.000 | 51.334 | 102.67 | 30-160 |


| SURROGATE COMPOUND | AMOUNT ADDED ug/Kg | AMOUNT RECOVERED ug/Kg | % RECOVERED | LIMITS |
|--------------------------|--------------------------|------------------------------|----------------|--------|
| \$ 31 d4-1,2-Dichloroeth | 50.000 | 53.581 | 107.16 | 75-152 |
| \$ 43 d8-Toluene | 50.000 | 51.205 | 102.41 | 82-115 |
| \$ 62 4-Bromofluorobenze | 50.000 | 49.253 | 98.51 | 64-120 |
| \$ 79 d4-1,2-Dichloroben | 50.000 | 50.329 | 100.66 | 80-120 |

Data File: /chem1/finn5.i/10AUG10.b/LCS0810.d
Date: 10-AUG-2010 11:12
Client ID: LCS0810
Sample Info: LCS0810,5,5,0

Column phase: Rt:502.2

/chem1/finn5.i/10AUG10.b/LCS0810.d/LCS0810.LG

Instrument: finn5.i
Operator: PB
Column diameter: 0.18



Analytical Resources, Inc.

8260C

Data file : /chem1/finn5.i/10AUG10.b/LCS0810A.d
 Lab Smp Id: LCS0810 Client Smp ID: LCS0810
 Inj Date : 10-AUG-2010 11:37
 Operator : PB Inst ID: finn5.i
 Smp Info : LCS0810,5,5,0
 Misc Info : 10-18196
 Comment :
 Method : /chem1/finn5.i/10AUG10.b/s8260b.m
 Meth Date : 10-Aug-2010 15:05 patrickkb Quant Type: ISTD
 Cal Date : 23-JUL-2010 17:18 Cal File: 2000723.d
 Als bottle: 1 QC Sample: LCSD
 Dil Factor: 1.00000 Compound Sublist: voa.sub
 Integrator: HP RTE
 Target Version: 3.50
 Processing Host: cserv3

Handwritten signature/initials

Concentration Formula: $Amt * DF * Pv * 1 / (Sa * ((100 - M) / 100)) * CpndVaria$

| Name | Value | Description |
|------|---------|-----------------|
| DF | 1.00000 | Dilution Factor |
| Pv | 5.00000 | Purge Volume |
| Sa | 5.00000 | Sample Amount |
| M | 0.00000 | Moisture (%) |

Cpnd Variable

Local Compound Variable

| Compounds | QUANT SIG | RT | EXP RT | REL RT | RESPONSE | CONCENTRATIONS | |
|----------------------------------|-----------|-------|--------|---------|----------|-------------------|---------------|
| | | | | | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 1 Dichlorodifluoromethane | 85 | 3.015 | 2.995 | (0.455) | 59457 | 37.9933 | 37.993 |
| 2 Chloromethane | 50 | 3.316 | 3.296 | (0.500) | 162883 | 38.6850 | 38.685 |
| 3 Vinyl Chloride | 62 | 3.427 | 3.407 | (0.517) | 139237 | 41.8182 | 41.818 |
| 4 Bromomethane | 94 | 3.919 | 3.899 | (0.591) | 103166 | 57.0542 | 57.054 |
| 5 Chloroethane | 64 | 3.980 | 3.970 | (0.600) | 94412 | 43.4201 | 43.420 |
| 6 Trichlorofluoromethane | 101 | 4.251 | 4.231 | (0.641) | 145948 | 45.3537 | 45.354 |
| 7 Acrolein | 56 | 4.633 | 4.613 | (0.698) | 102873 | 256.275 | 256.28 |
| 8 112Trichloro122Trifluoroethane | 101 | 4.643 | 4.623 | (0.700) | 110528 | 43.8718 | 43.872 |
| 9 Acetone | 43 | 4.683 | 4.663 | (0.706) | 185274 | 274.319 | 274.32 |
| 10 1,1-Dichloroethene | 96 | 4.844 | 4.824 | (0.730) | 104667 | 45.7831 | 45.783 |
| 11 Bromoethane | 108 | 5.065 | 5.045 | (0.764) | 79532 | 46.9771 | 46.977 |
| 12 Iodomethane | 142 | 5.166 | 5.146 | (0.779) | 144377 | 53.4132 | 53.413 |
| 13 Methylene Chloride | 84 | 5.276 | 5.266 | (0.795) | 107119 | 41.6127 | 41.613 |
| 14 Acrylonitrile | 53 | 5.367 | 5.347 | (0.809) | 35437 | 59.4268 | 59.427 (Q) |

| Compounds | QUANT SIG | | | RESPONSE | CONCENTRATIONS | |
|------------------------------|-----------|--------|----------------|----------|----------------------|------------------|
| | MASS | RT | EXP RT REL RT | | ON-COLUMN (ug/Kg) | FINAL (ug/Kg) |
| 16 Methyl tert-Butyl Ether | 73 | 5.407 | 5.387 (0.815) | 160779 | 45.7324 | 45.732 (Q) |
| 15 Carbon Disulfide | 76 | 5.377 | 5.367 (0.811) | 348805 | 49.1939 | 49.194 |
| 17 Trans-1,2-Dichloroethene | 96 | 5.558 | 5.548 (0.838) | 89450 | 45.9120 | 45.912 |
| 18 Vinyl Acetate | 43 | 5.889 | 5.869 (0.888) | 192137 | 56.3070 | 56.307 |
| 19 1,1-Dichloroethane | 63 | 5.940 | 5.919 (0.895) | 172532 | 48.1370 | 48.137 |
| 20 2-Butanone | 43 | 6.281 | 6.271 (0.947) | 218894 | 288.033 | 288.03 |
| 21 2,2-Dichloropropane | 77 | 6.462 | 6.442 (0.974) | 90369 | 41.2045 | 41.204 |
| 22 Cis-1,2-Dichloroethene | 96 | 6.502 | 6.482 (0.980) | 81945 | 47.7210 | 47.721 |
| * 23 Pentafluorobenzene | 168 | 6.633 | 6.613 (1.000) | 120686 | 50.0000 | |
| 24 Chloroform | 83 | 6.643 | 6.633 (1.002) | 134577 | 46.2249 | 46.225 |
| 26 Bromochloromethane | 128 | 6.814 | 6.794 (1.027) | 39494 | 48.4424 | 48.442 |
| \$ 25 Dibromofluoromethane | 111 | 6.844 | 6.834 (1.032) | 74025 | 51.4633 | 51.463 (Q) |
| 27 1,1,1-Trichloroethane | 97 | 7.035 | 7.025 (1.061) | 95264 | 42.0706 | 42.070 |
| 29 1,1-Dichloropropene | 75 | 7.186 | 7.166 (0.941) | 107756 | 44.3432 | 44.343 |
| 30 Carbon Tetrachloride | 117 | 7.296 | 7.276 (0.955) | 87122 | 41.2287 | 41.229 |
| \$ 31 d4-1,2-Dichloroethane | 65 | 7.316 | 7.296 (1.103) | 84469 | 53.6675 | 53.668 |
| 32 1,2-Dichloroethane | 62 | 7.397 | 7.377 (0.968) | 102874 | 48.2233 | 48.223 |
| 33 Benzene | 78 | 7.447 | 7.427 (0.975) | 277311 | 47.1928 | 47.193 |
| * 34 1,4-Difluorobenzene | 114 | 7.638 | 7.618 (1.000) | 178947 | 50.0000 | |
| 35 Trichloroethene | 95 | 8.010 | 8.000 (1.049) | 74898 | 43.5043 | 43.504 |
| 36 1,2-Dichloropropane | 63 | 8.171 | 8.161 (1.070) | 83947 | 45.3200 | 45.320 |
| 37 Bromodichloromethane | 83 | 8.412 | 8.392 (1.101) | 90085 | 45.4878 | 45.488 |
| 39 Dibromomethane | 93 | 8.482 | 8.462 (1.111) | 44145 | 48.0100 | 48.010 |
| 40 2-Chloroethyl Vinyl Ether | 63 | 8.623 | 8.613 (1.129) | 36062 | 55.5918 | 55.592 (Q) |
| 41 4-Methyl-2-Pentanone | 58 | 8.663 | 8.643 (1.134) | 122162 | 258.245 | 258.24 |
| 42 Cis 1,3-dichloropropene | 75 | 8.914 | 8.894 (1.167) | 104981 | 48.5525 | 48.552 |
| \$ 43 d8-Toluene | 98 | 9.196 | 9.176 (1.204) | 201110 | 51.1475 | 51.148 |
| 44 Toluene | 92 | 9.276 | 9.256 (1.214) | 151283 | 43.3924 | 43.392 |
| 45 Trans 1,3-Dichloropropene | 75 | 9.407 | 9.387 (1.232) | 86740 | 47.7261 | 47.726 |
| 46 2-Hexanone | 43 | 9.537 | 9.517 (0.884) | 297529 | 248.221 | 248.22 |
| 47 1,1,2-Trichloroethane | 97 | 9.588 | 9.568 (1.255) | 53729 | 49.5026 | 49.503 |
| 48 1,3-Dichloropropane | 76 | 9.849 | 9.829 (0.912) | 101540 | 49.2008 | 49.201 |
| 49 Tetrachloroethene | 166 | 9.960 | 9.949 (0.923) | 67148 | 41.2178 | 41.218 |
| 50 Chlorodibromomethane | 129 | 10.171 | 10.150 (0.942) | 64117 | 46.1822 | 46.182 |
| 51 1,2-Dibromoethane | 107 | 10.392 | 10.382 (1.361) | 55459 | 47.7035 | 47.704 |
| * 52 d5-Chlorobenzene | 117 | 10.794 | 10.774 (1.000) | 146633 | 50.0000 | |
| 53 Chlorobenzene | 112 | 10.834 | 10.814 (1.004) | 152771 | 44.4197 | 44.420 |
| 54 Ethyl Benzene | 91 | 10.864 | 10.854 (1.007) | 274940 | 47.2728 | 47.273 |
| 55 1,1,1,2-Tetrachloroethane | 131 | 10.864 | 10.844 (1.007) | 51991 | 39.4980 | 39.498 |
| 56 m,p-xylene | 106 | 10.944 | 10.934 (1.014) | 212357 | 99.8969 | 99.897 |
| 57 o-Xylene | 106 | 11.437 | 11.417 (1.060) | 104428 | 47.2670 | 47.267 |
| 58 Styrene | 104 | 11.467 | 11.447 (1.062) | 173270 | 50.7226 | 50.723 |
| 59 Isopropyl Benzene | 105 | 11.819 | 11.799 (0.878) | 269609 | 51.2414 | 51.241 |
| 60 Bromoform | 173 | 11.879 | 11.859 (0.882) | 40536 | 47.9168 | 47.917 |
| 61 1,1,2,2-Tetrachloroethane | 83 | 11.990 | 11.980 (0.890) | 74536 | 49.0344 | 49.034 |
| \$ 62 4-Bromofluorobenzene | 95 | 12.110 | 12.100 (1.122) | 85132 | 49.6078 | 49.608 |
| 63 1,2,3-Trichloropropane | 110 | 12.160 | 12.150 (0.903) | 15057 | 49.9998 | 50.000 (Q) |